


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081518\
Data File : VN050638.D
Acq On : 15 Aug 2018 7:55
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
Title : SW846 8260
Last Update : Tue Aug 14 08:07:08 2018

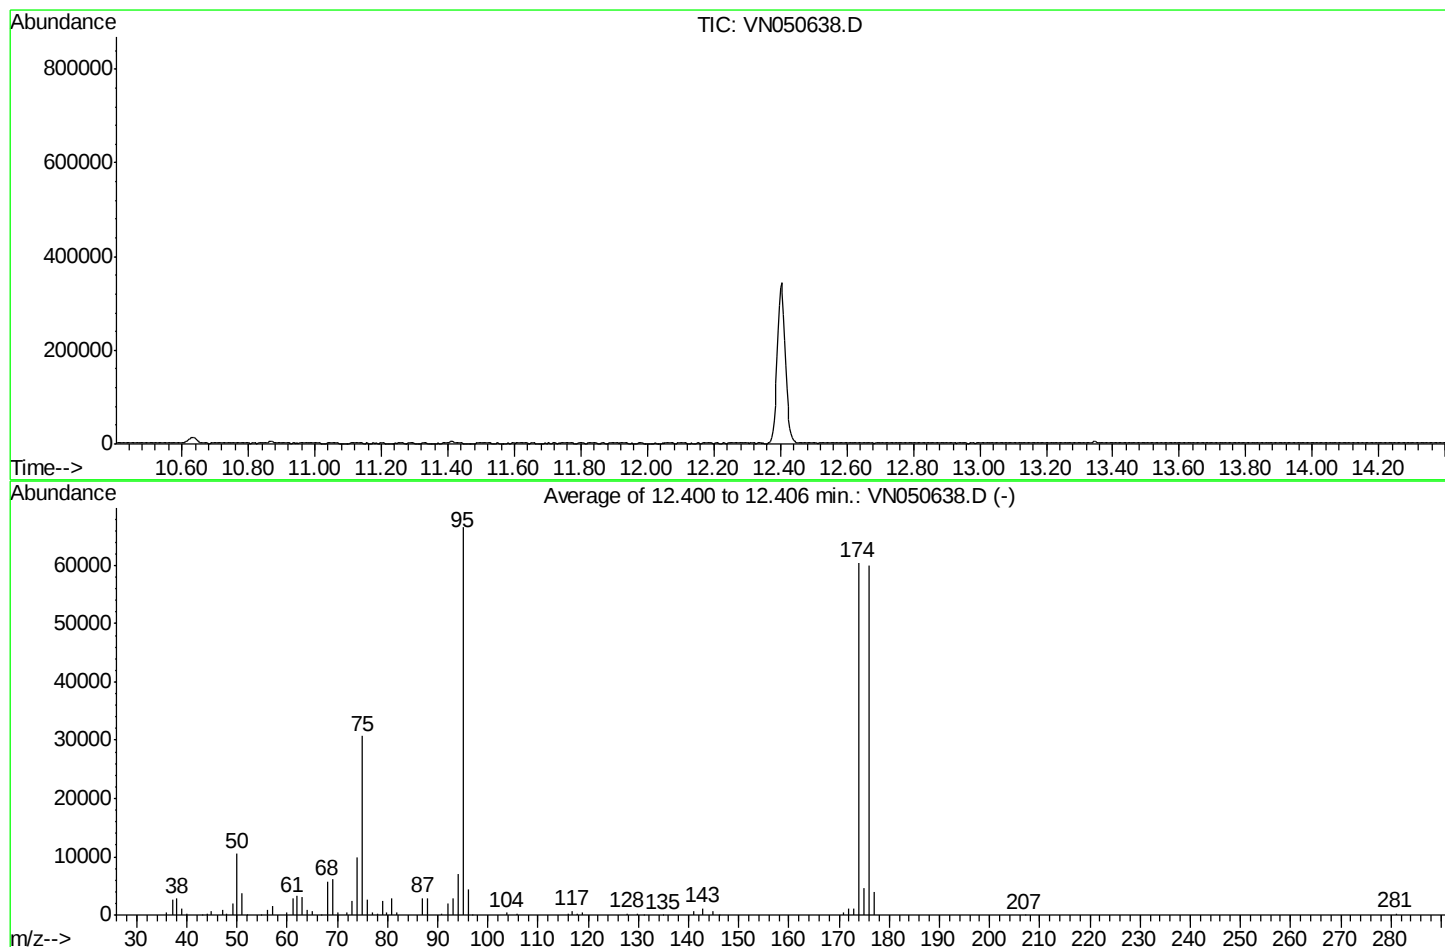

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	10541	PASS
75	95	30	60	46.2	30752	PASS
95	95	100	100	100.0	66544	PASS
96	95	5	9	6.6	4366	PASS
173	174	0.00	2	1.8	1080	PASS
174	95	50	100	90.8	60437	PASS
175	174	5	9	7.8	4708	PASS
176	174	95	101	99.1	59909	PASS
177	176	5	9	6.6	3952	PASS