


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081518\
Data File : VN050666.D
Acq On : 15 Aug 2018 20:11
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N072518W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Jul 26 15:21:50 2018

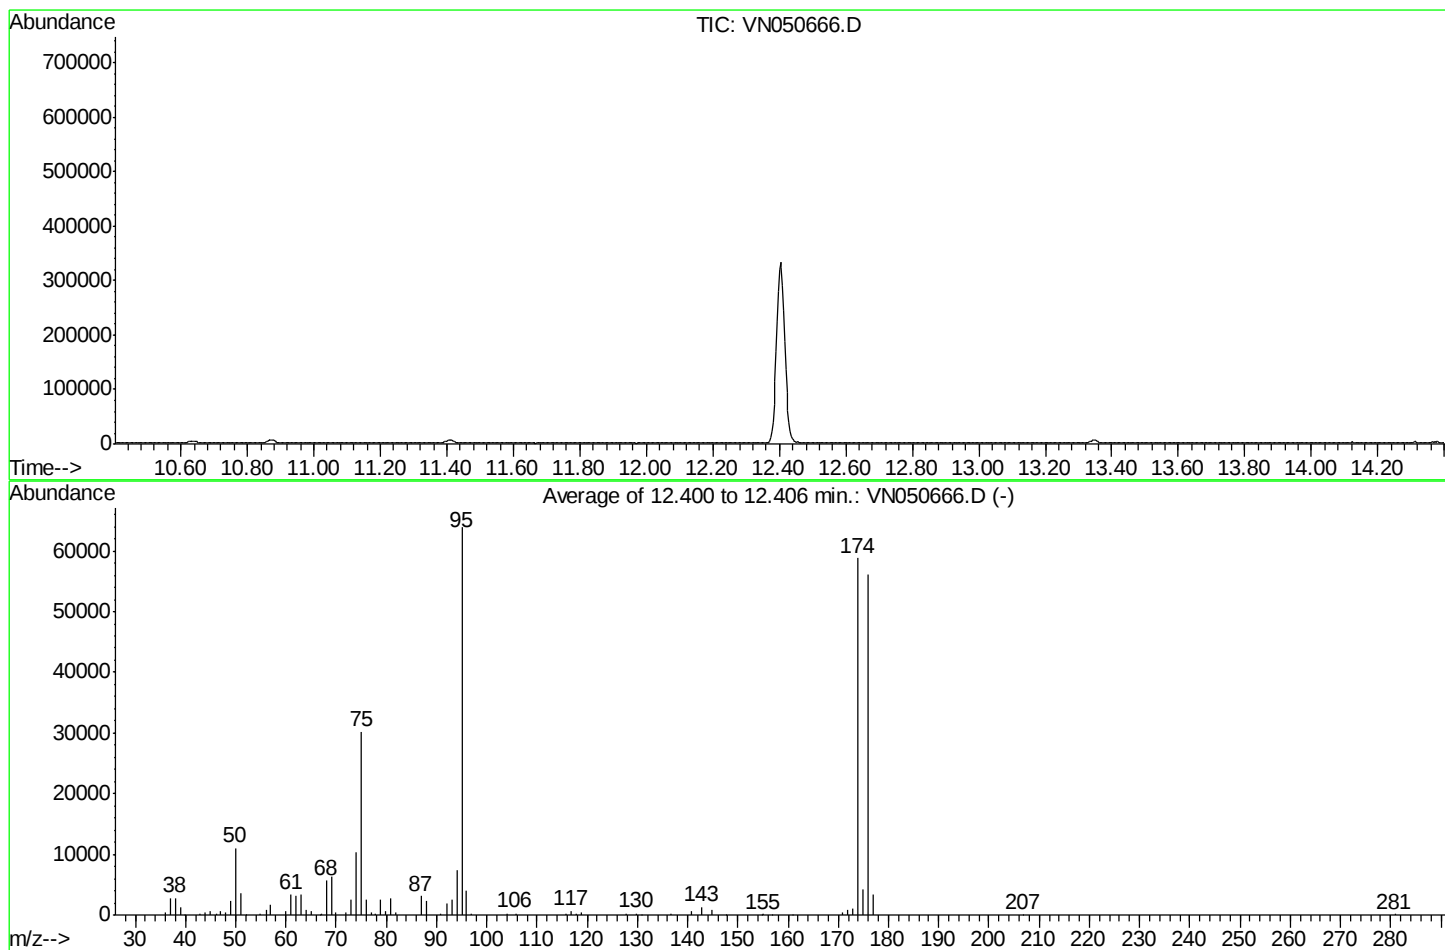

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3350

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	11041	PASS
75	95	30	60	47.4	30280	PASS
95	95	100	100	100.0	63898	PASS
96	95	5	9	6.4	4117	PASS
173	174	0.00	2	1.8	1051	PASS
174	95	50	100	92.1	58834	PASS
175	174	5	9	7.2	4249	PASS
176	174	95	101	95.3	56069	PASS
177	176	5	9	6.2	3462	PASS