



sec-Butylbenzene

Response Ratio

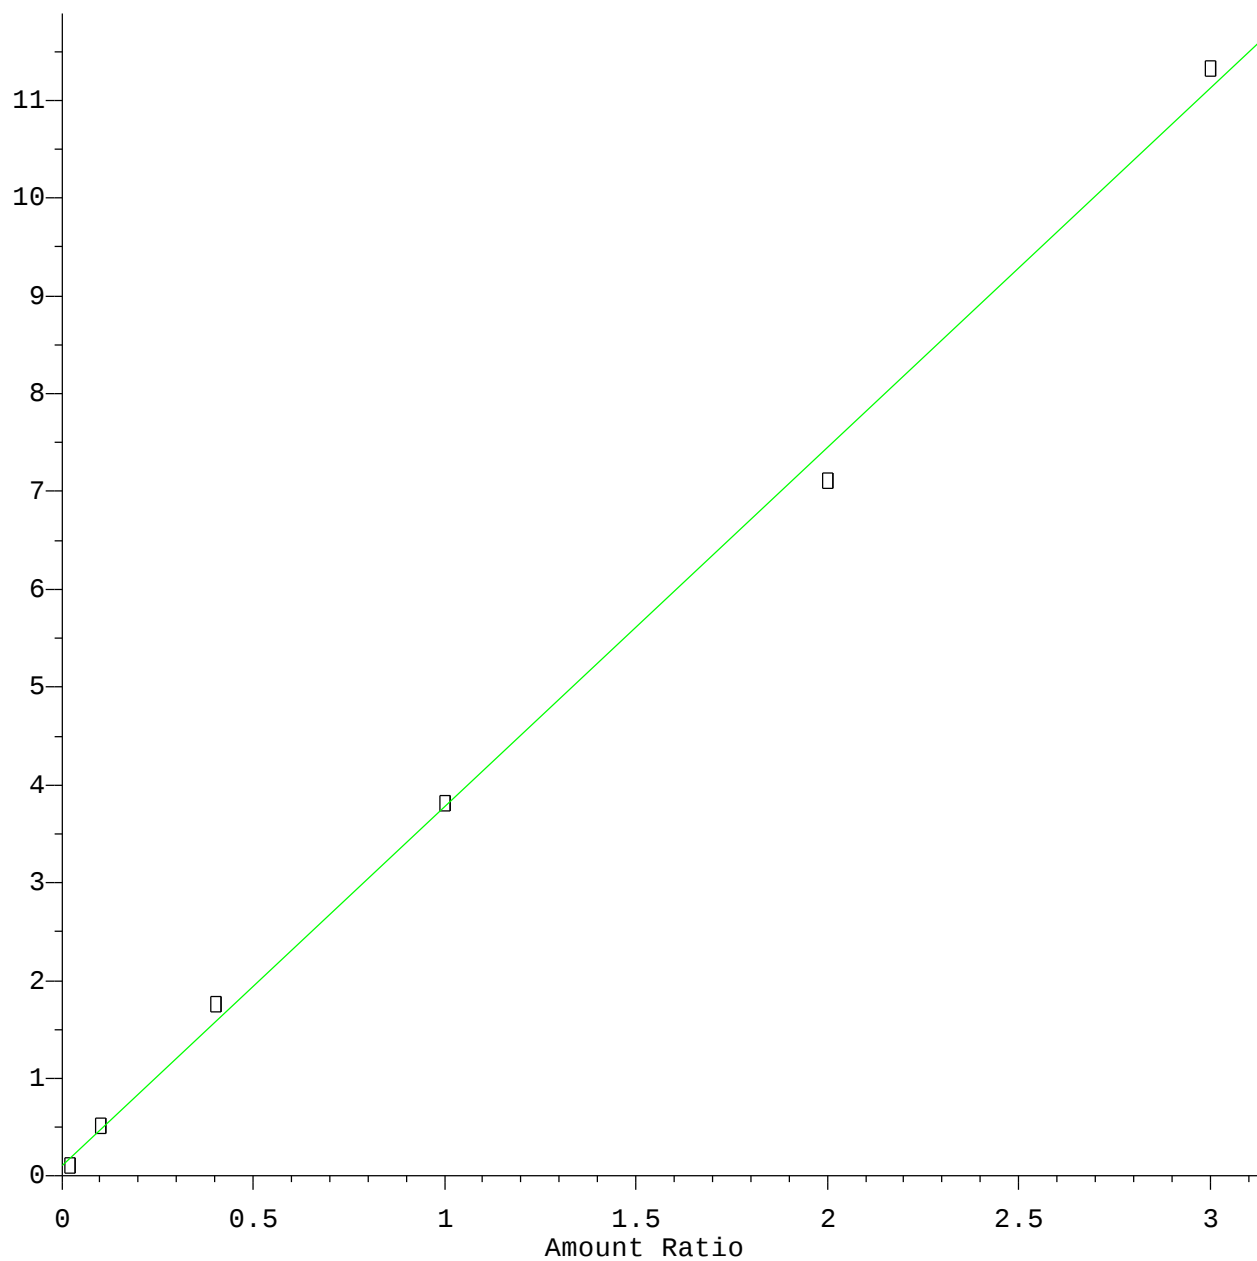

Resp Ratio = 3.67e+000 * Amt + 1.14e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019

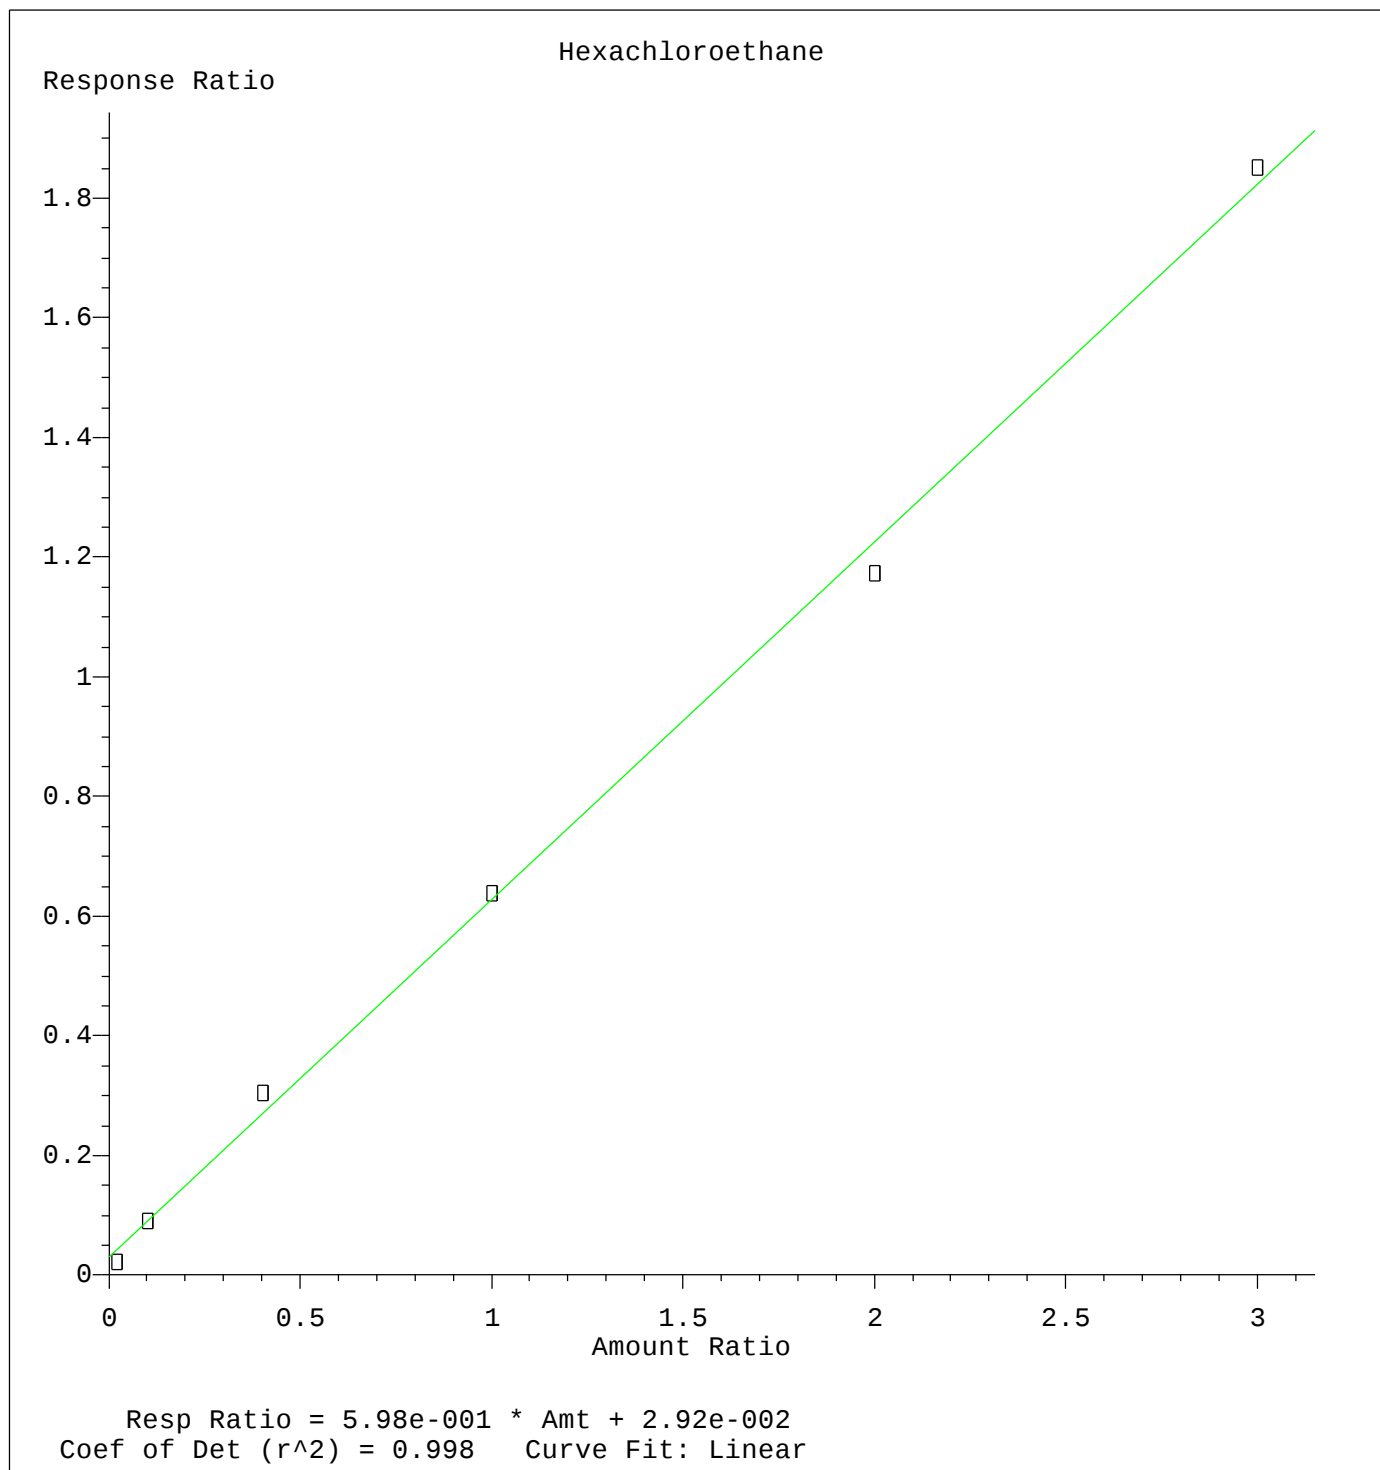

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019


1,2,4-Trichlorobenzene

Response Ratio

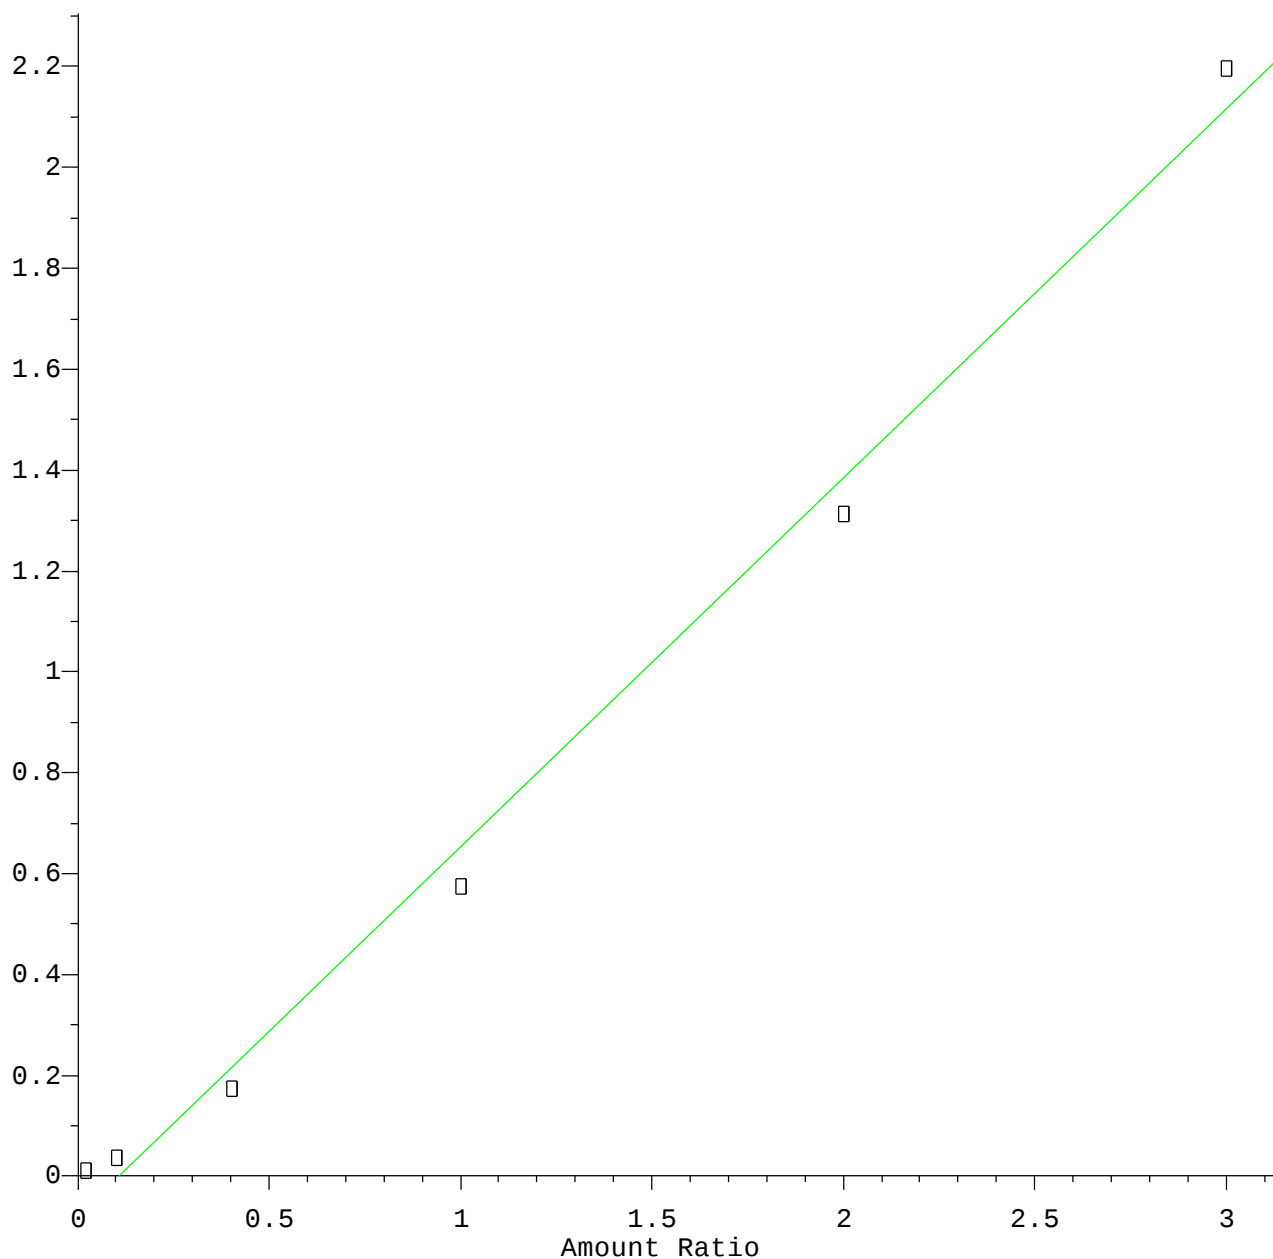


Resp Ratio = 7.31×10^{-1} * Amt - 7.83×10^{-2}
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019

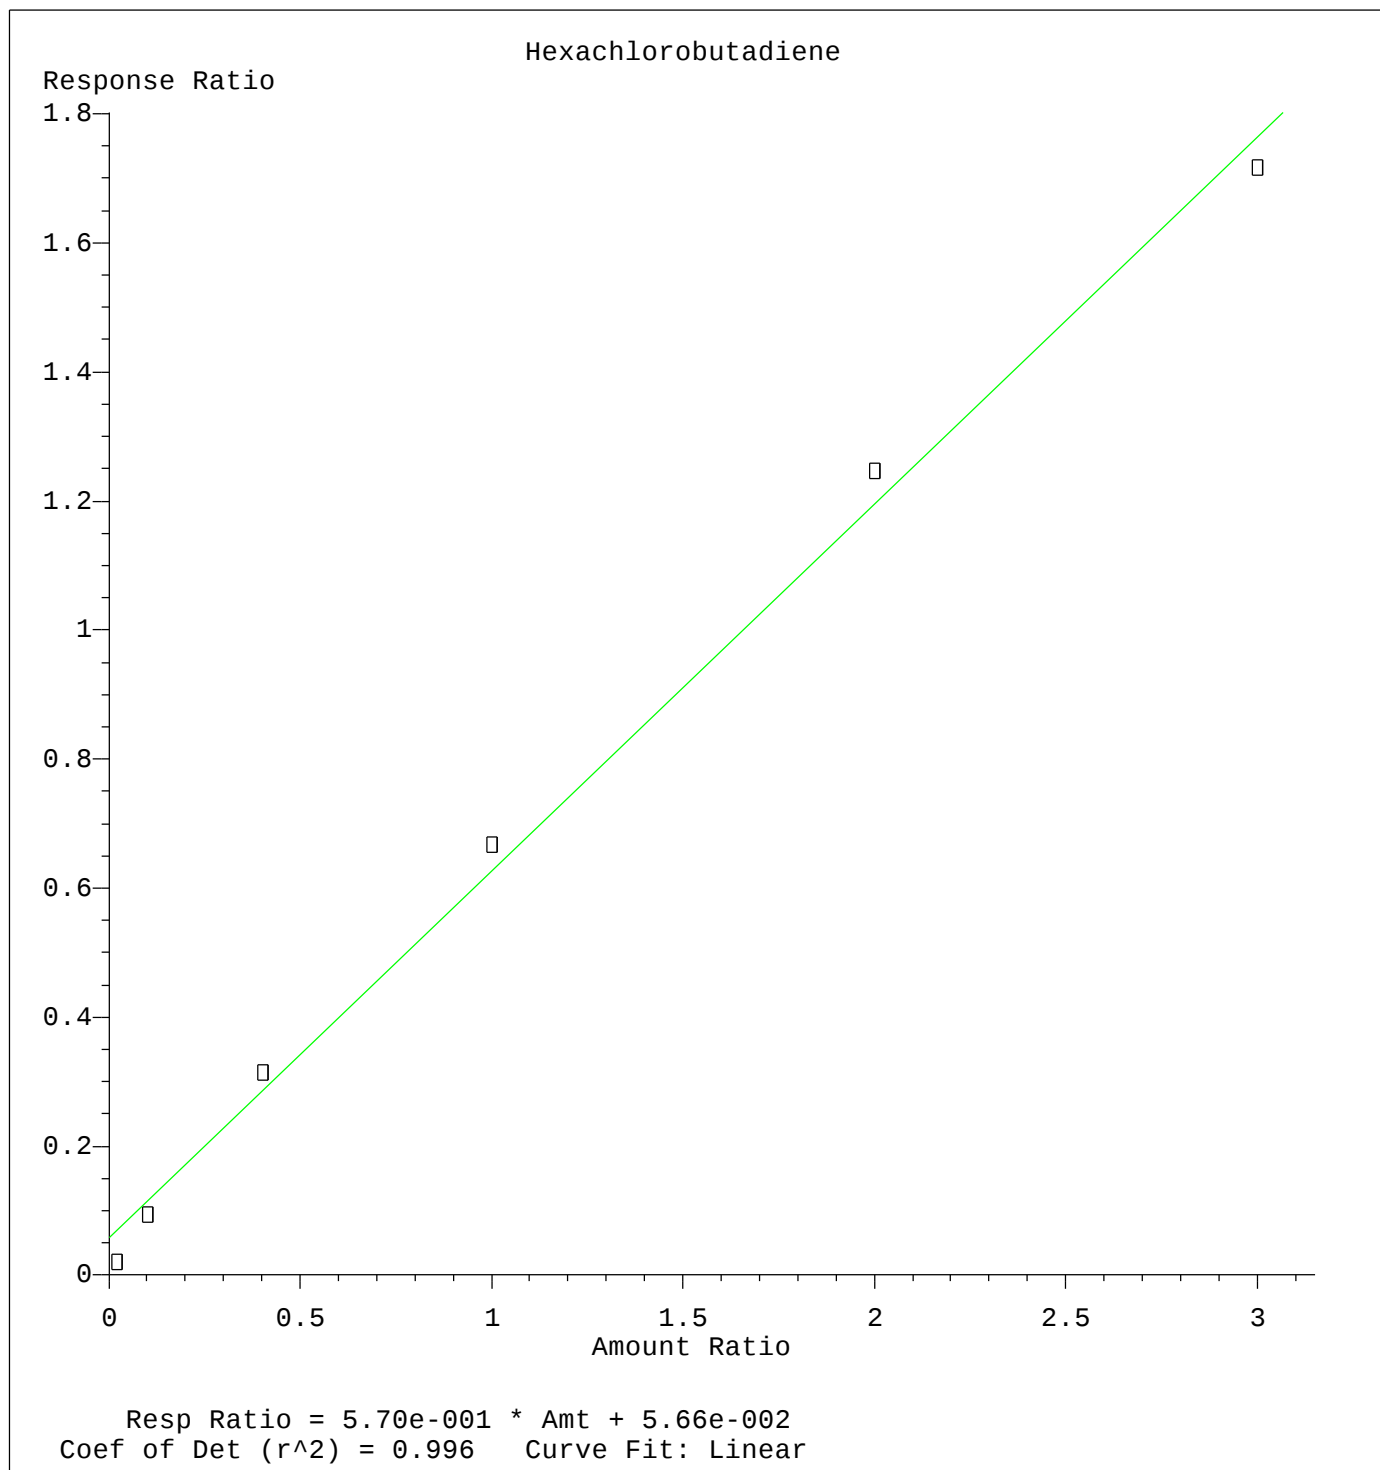


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019

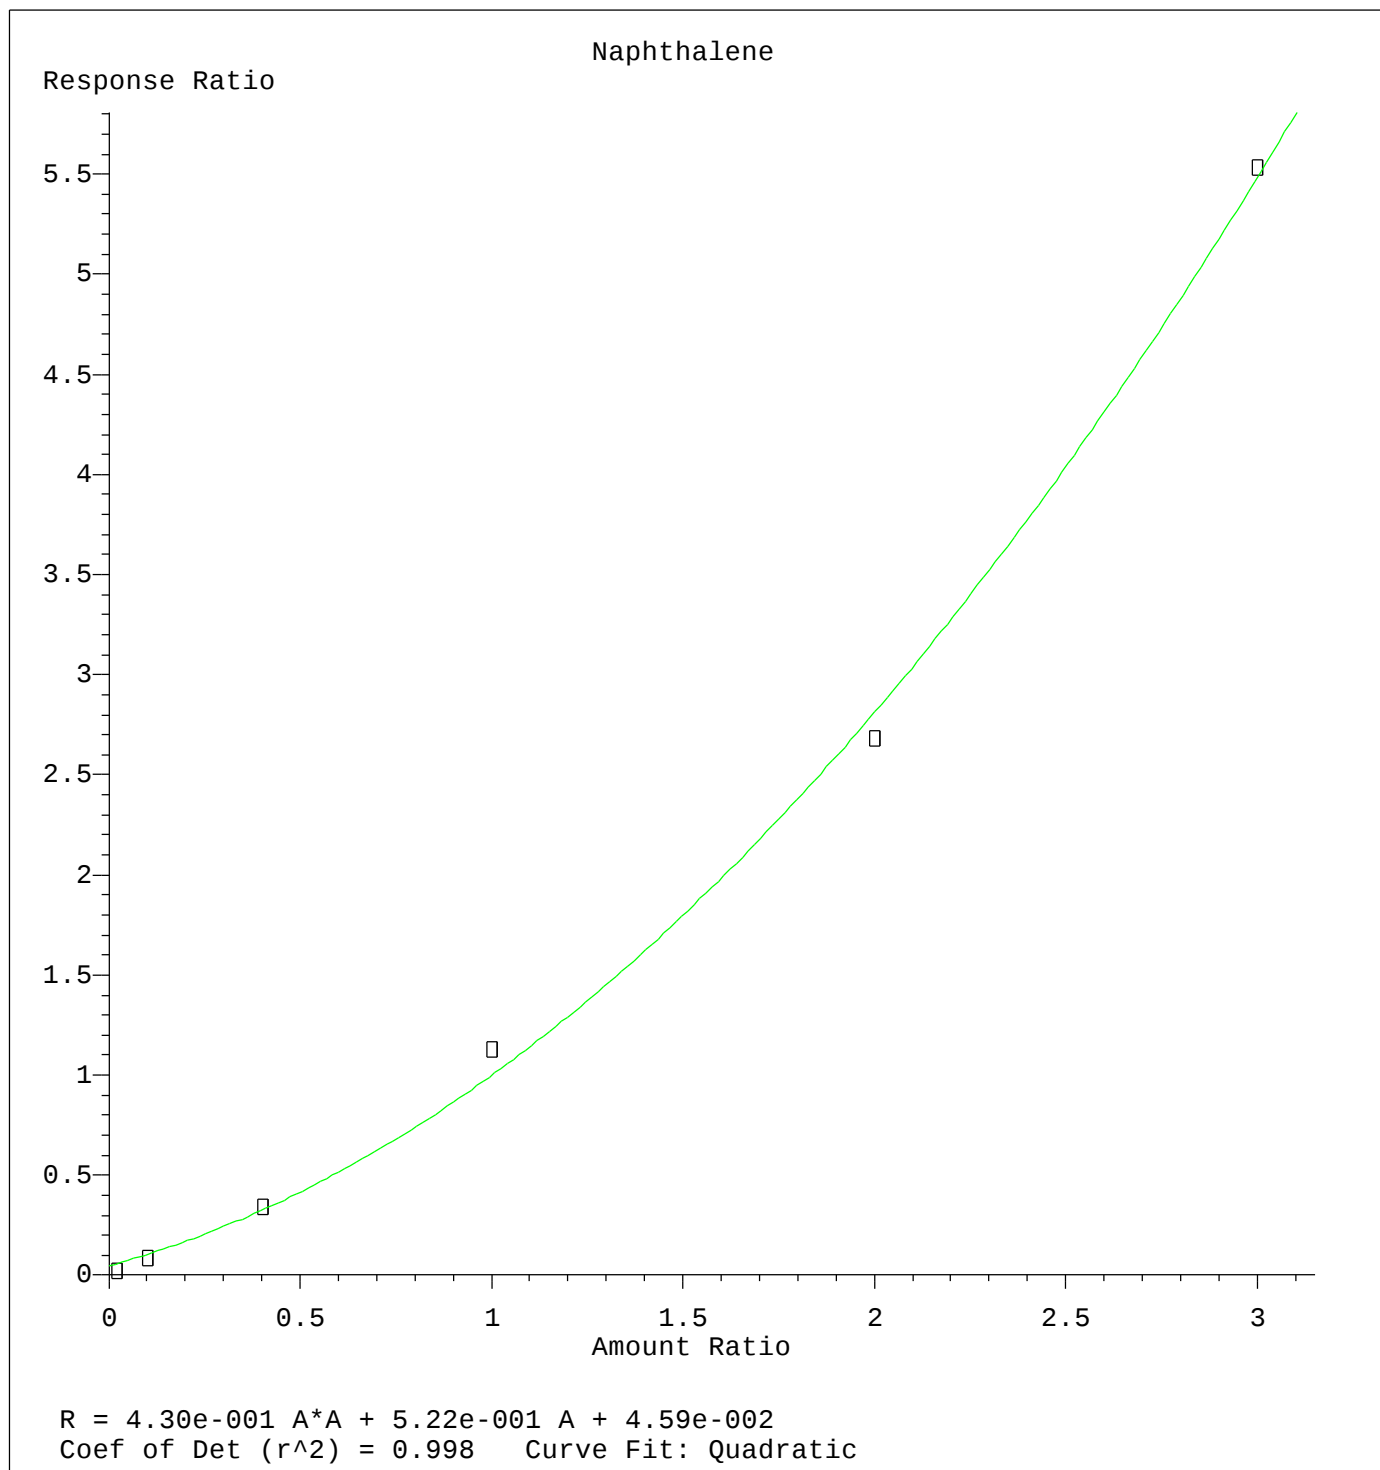

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019


1,2,3-Trichlorobenzene

Response Ratio

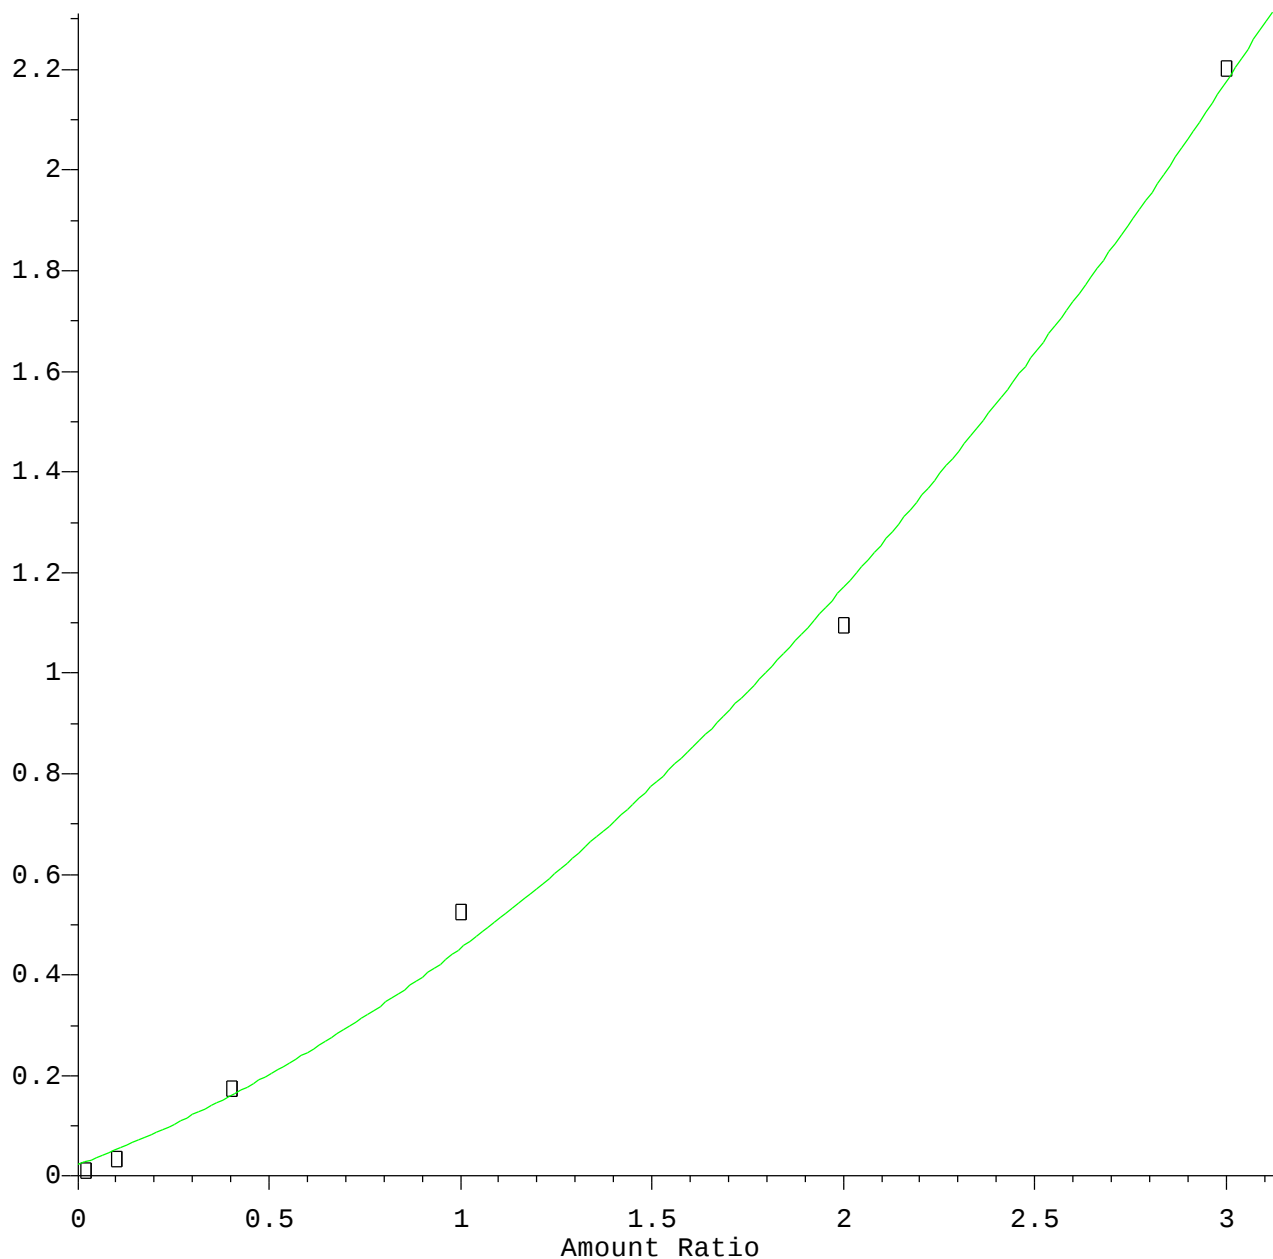

$R = 1.44e-001 A^2 + 2.87e-001 A + 2.20e-002$
Coef of Det (r^2) = 0.997 Curve Fit: Quadratic


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019

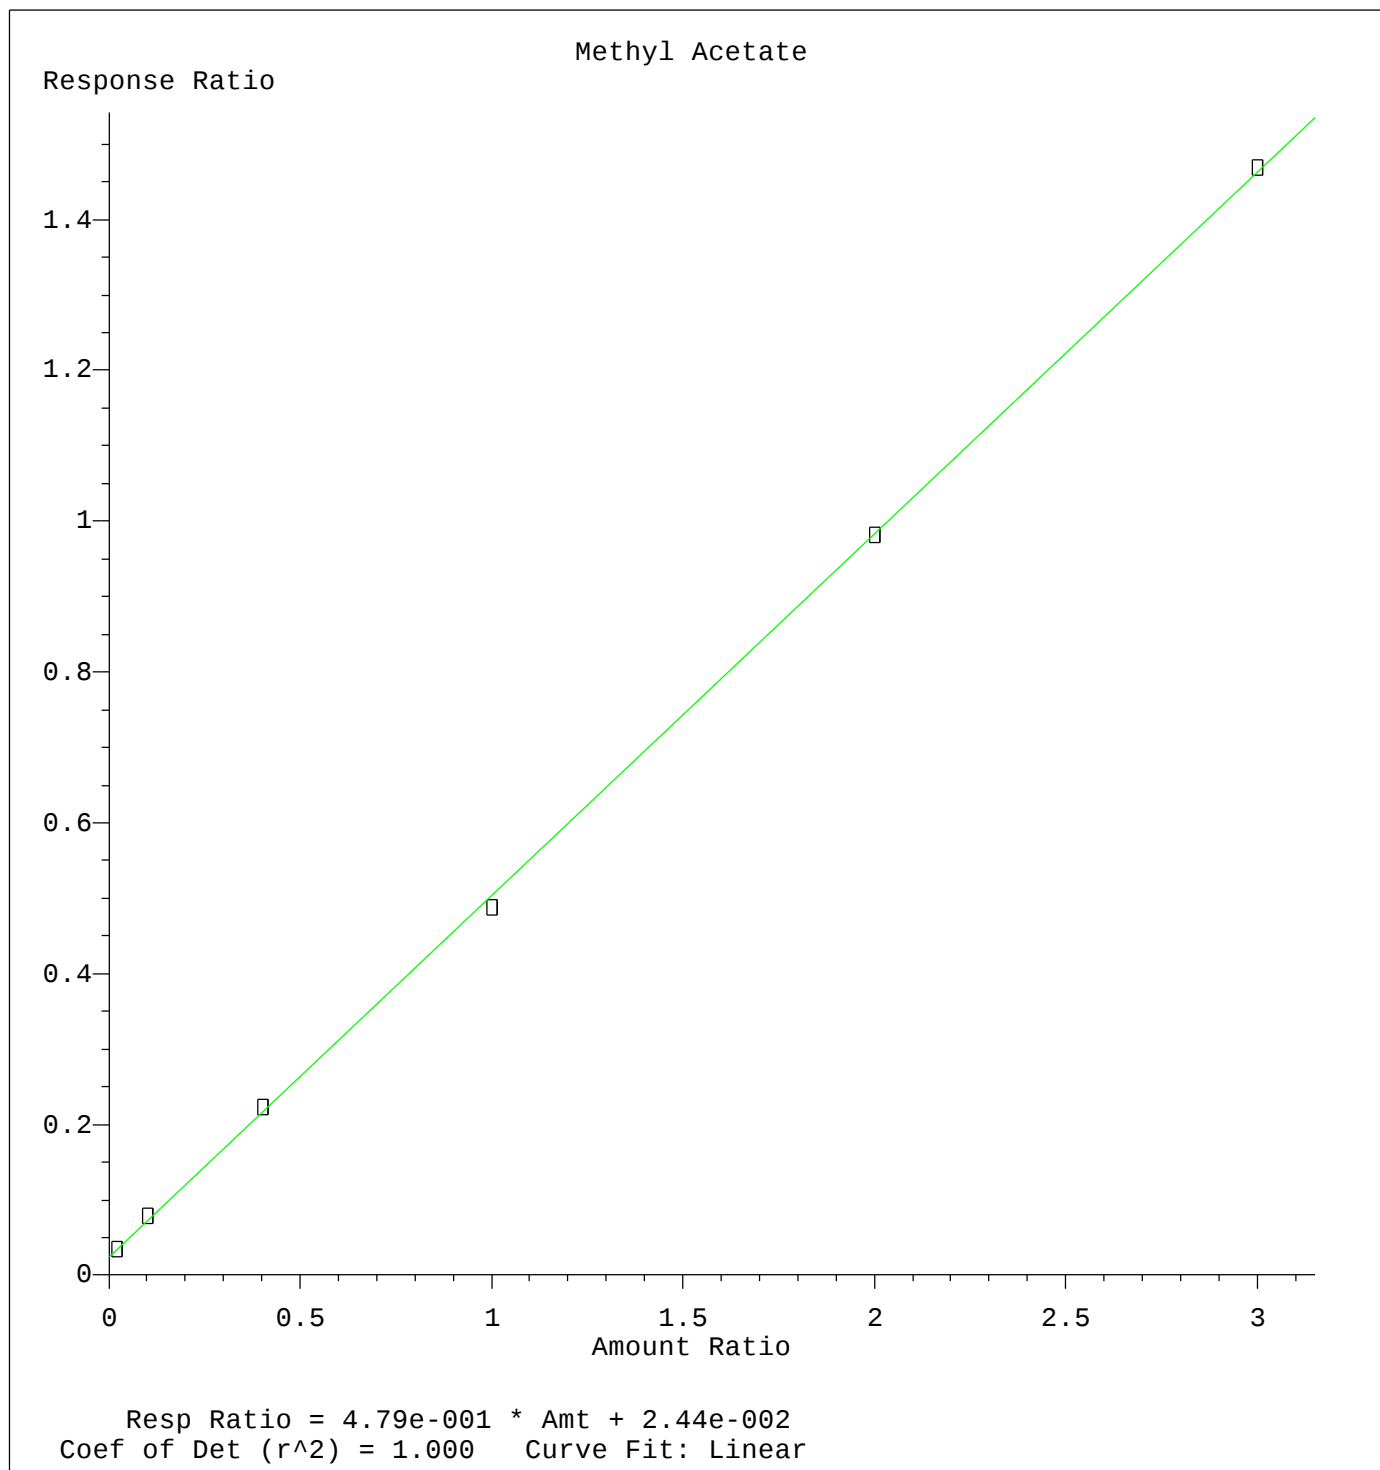

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019

Isopropyl Acetate

Response Ratio

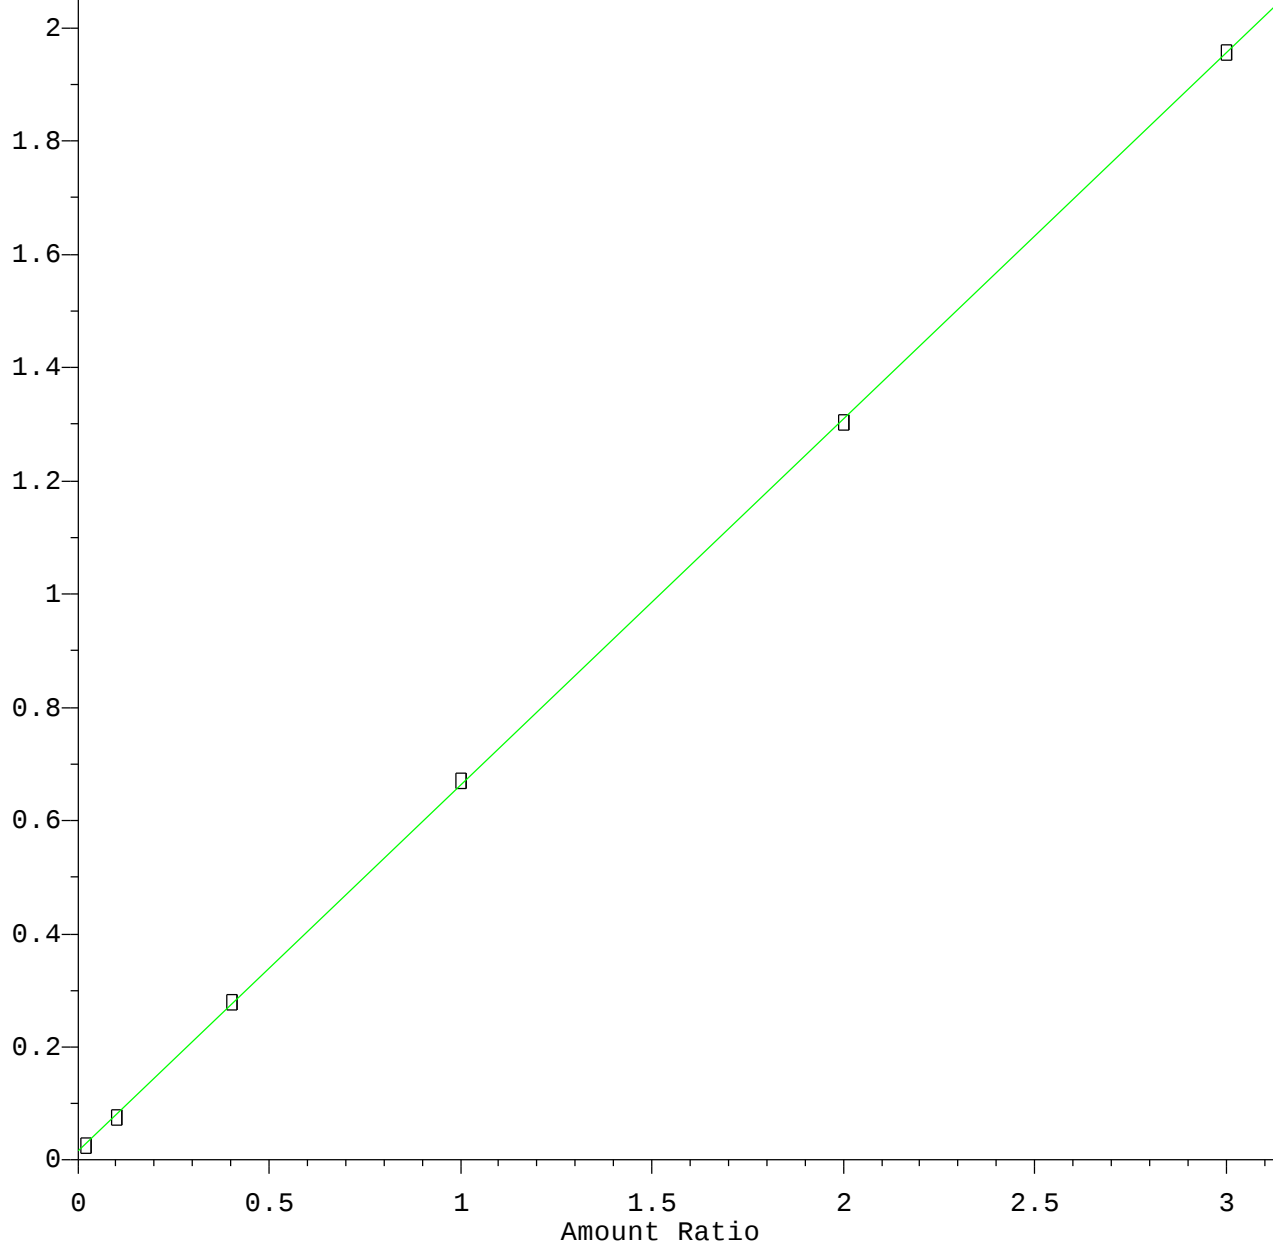


Resp Ratio = $6.46 \times 10^{-1} \times \text{Amt} + 1.49 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019

2-Chloroethyl Vinyl ether

Response Ratio

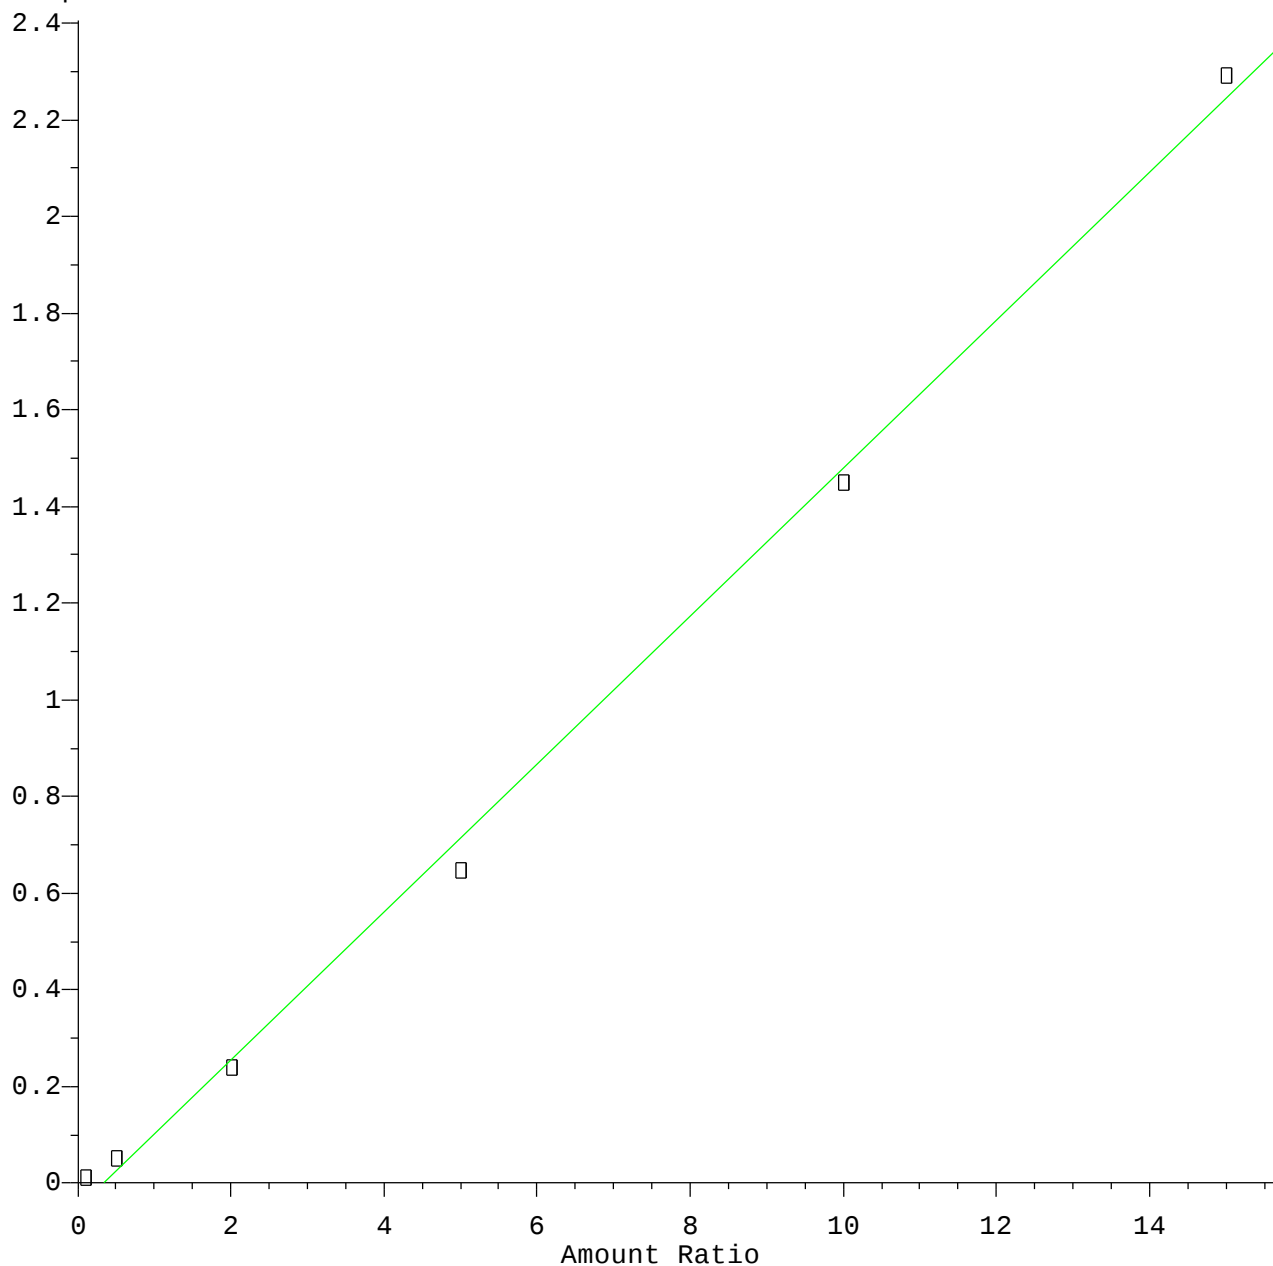


Resp Ratio = $1.53 \times 10^{-1} \times \text{Amt} - 5.07 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019

Isopropylbenzene

Response Ratio

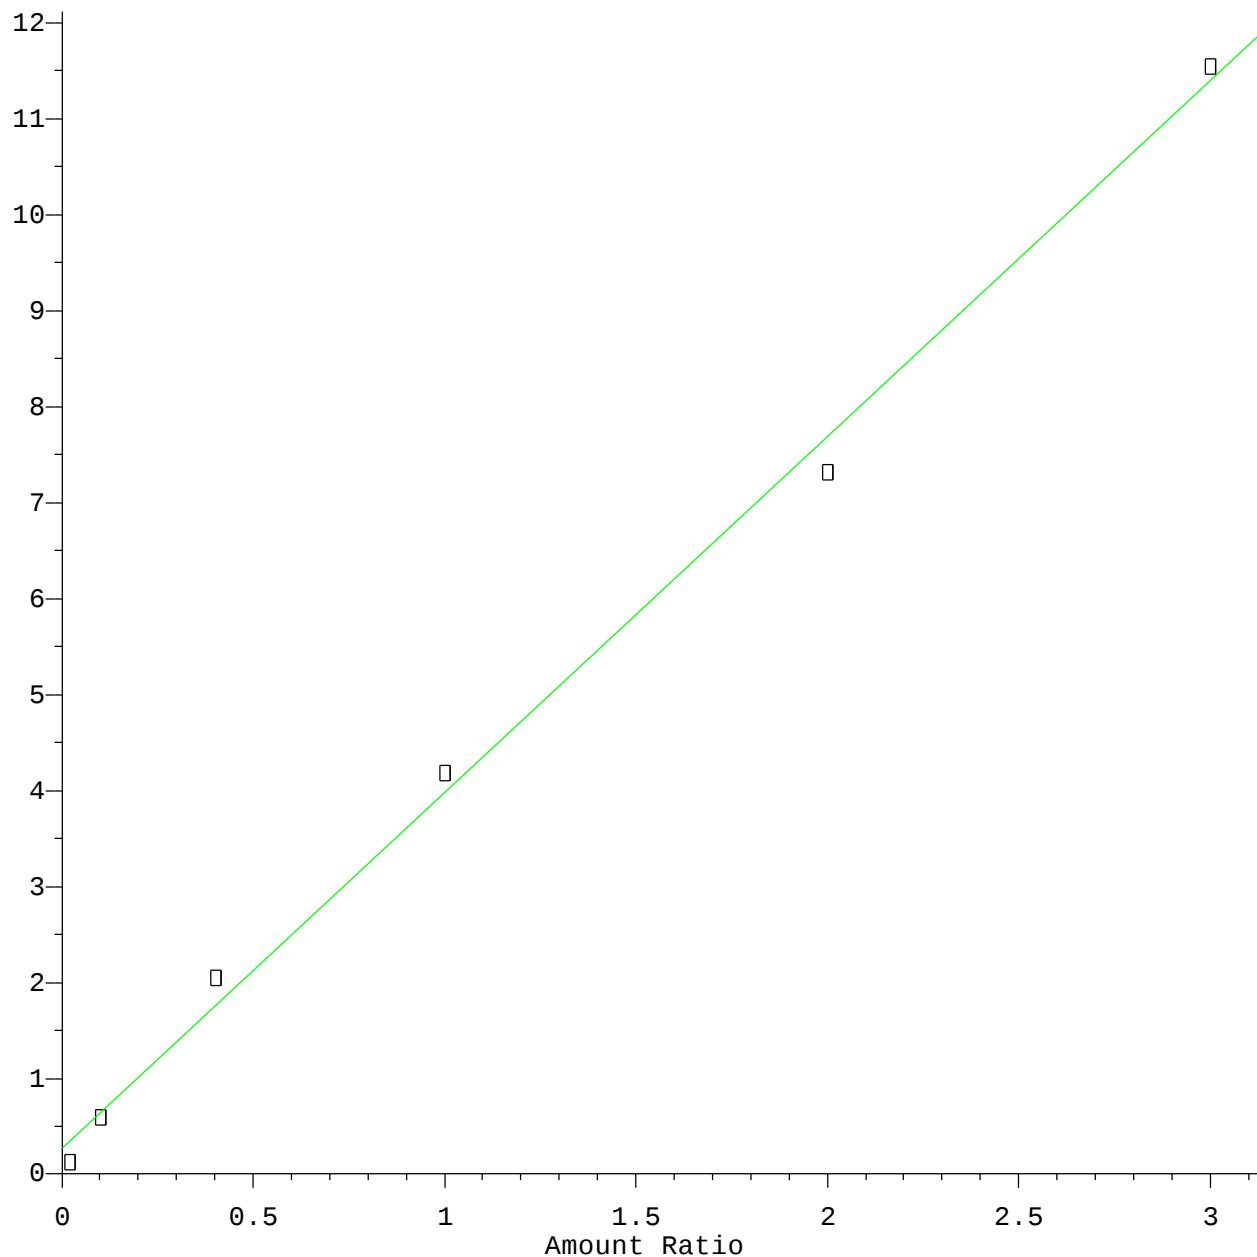


Resp Ratio = 3.71×10^0 * Amt + 2.69×10^{-1}
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019

1,1,2,2-Tetrachloroethane

Response Ratio

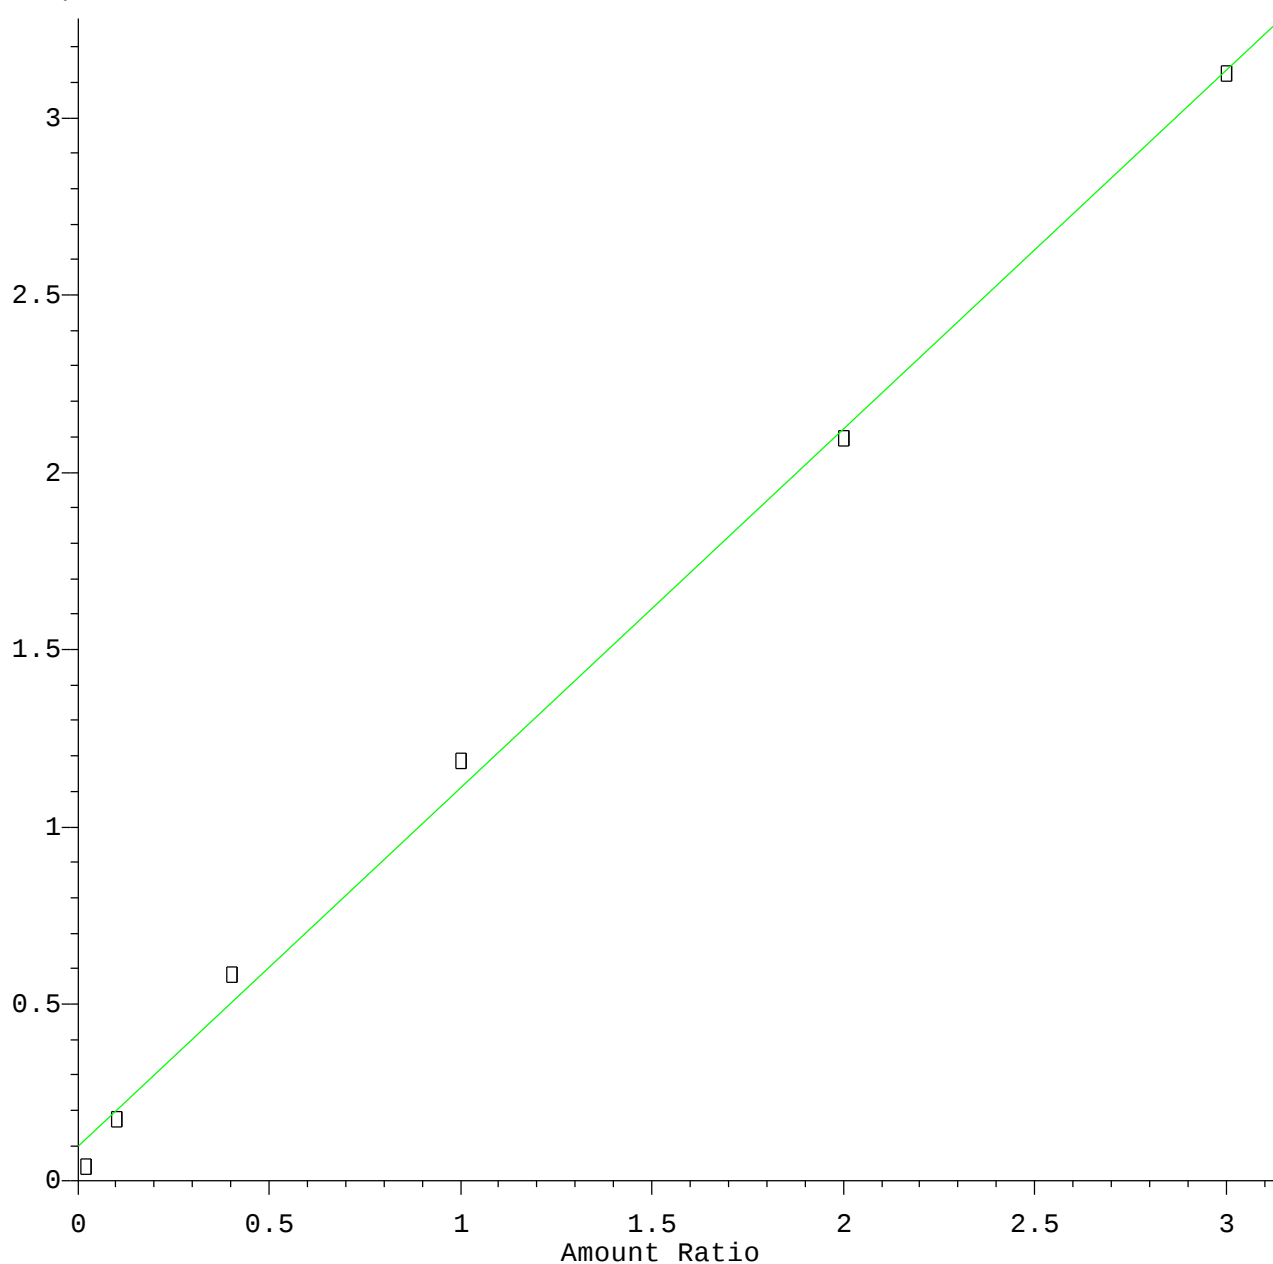


Resp Ratio = 1.01e+000 * Amt + 9.95e-002
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019


1,2,3-Trichloropropane

Response Ratio

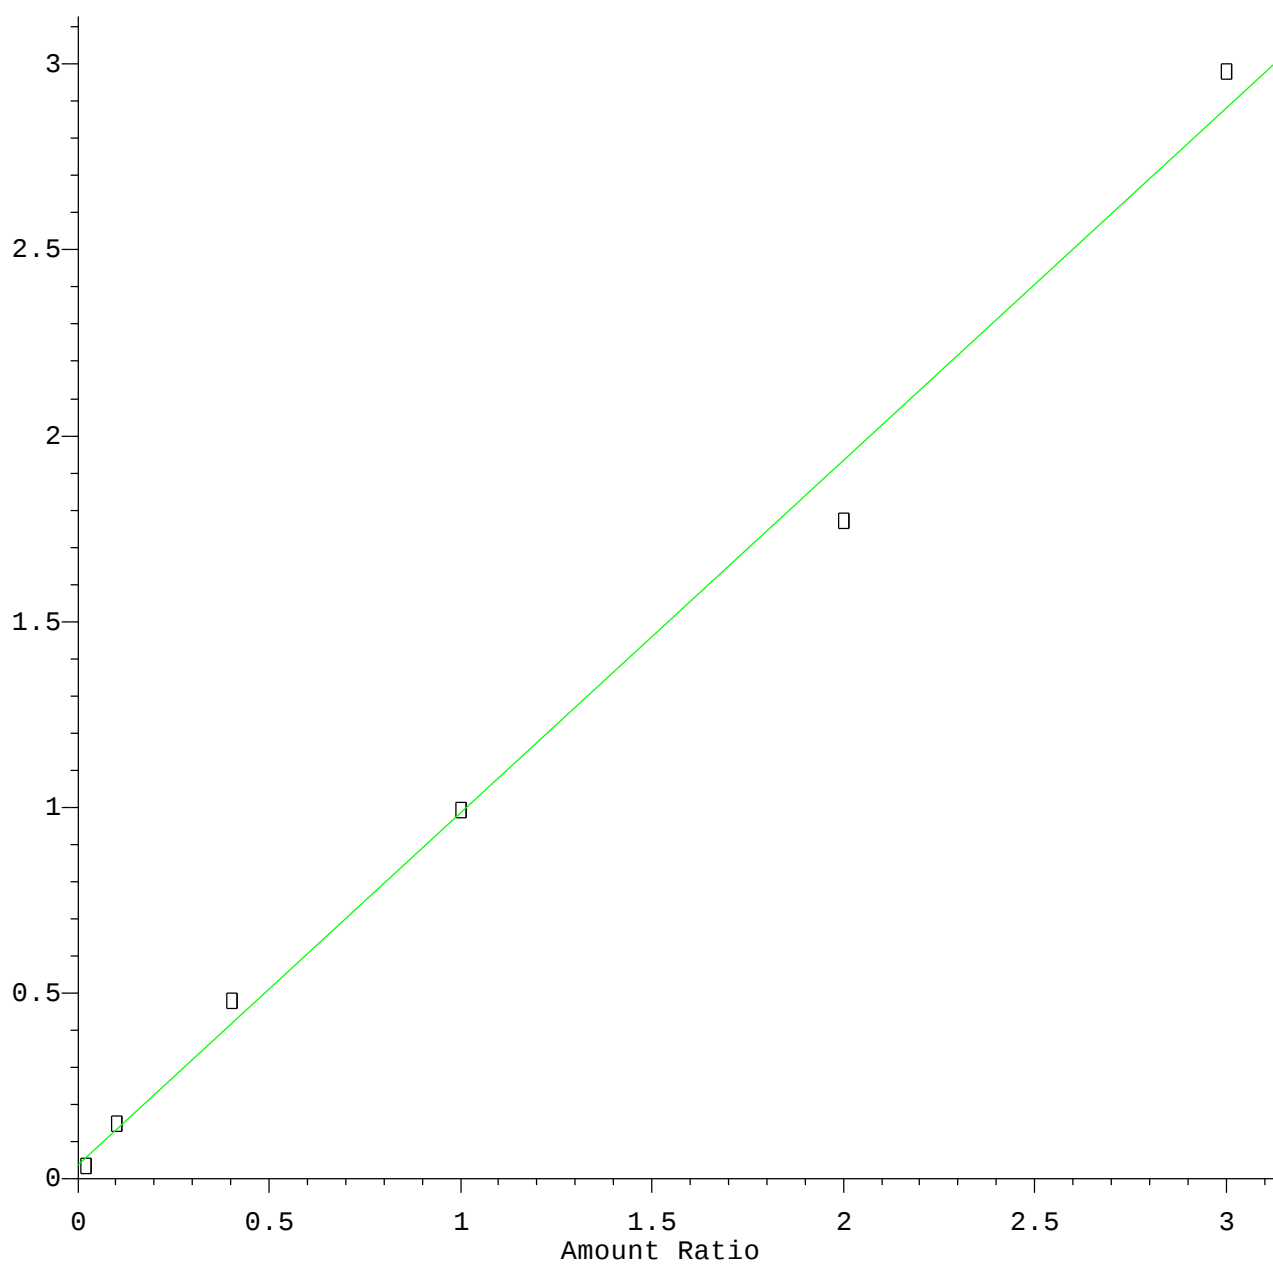

Resp Ratio = $9.48 \times 10^{-1} \times \text{Amt} + 3.66 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019

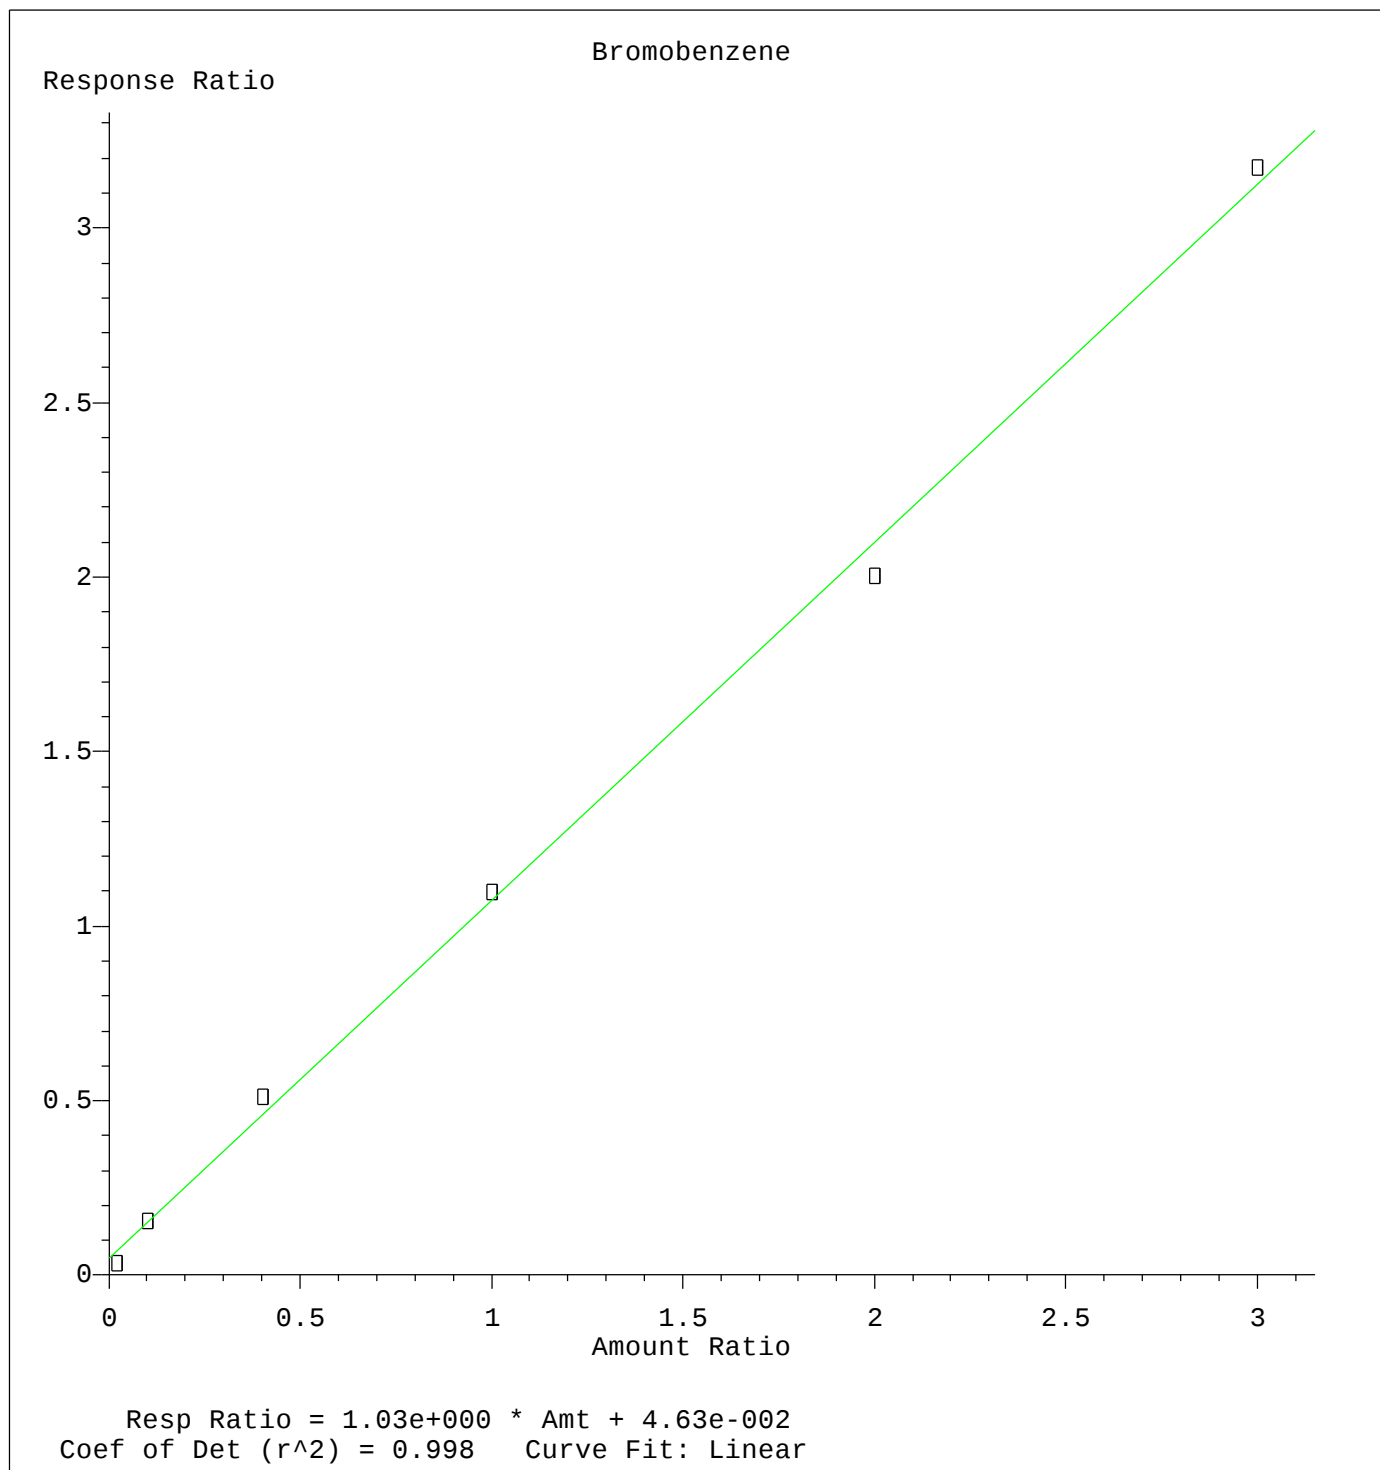

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019

2-Chlorotoluene

Response Ratio

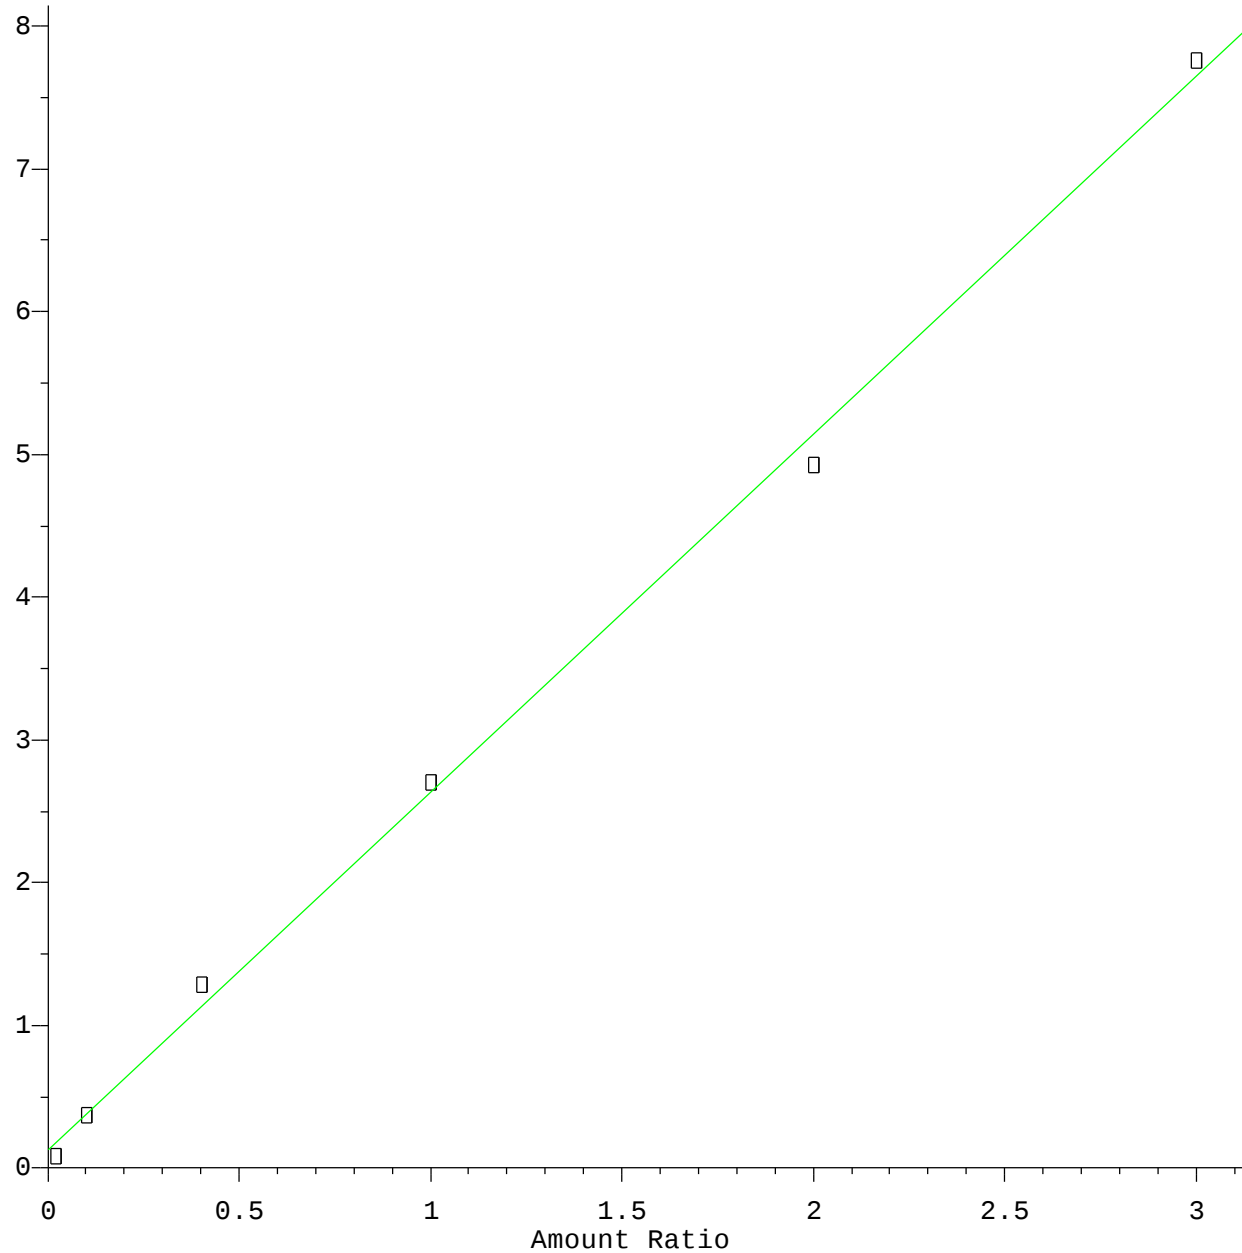


Resp Ratio = 2.51×10^0 * Amt + 1.24×10^{-1}
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019

1,3,5-Trimethylbenzene

Response Ratio

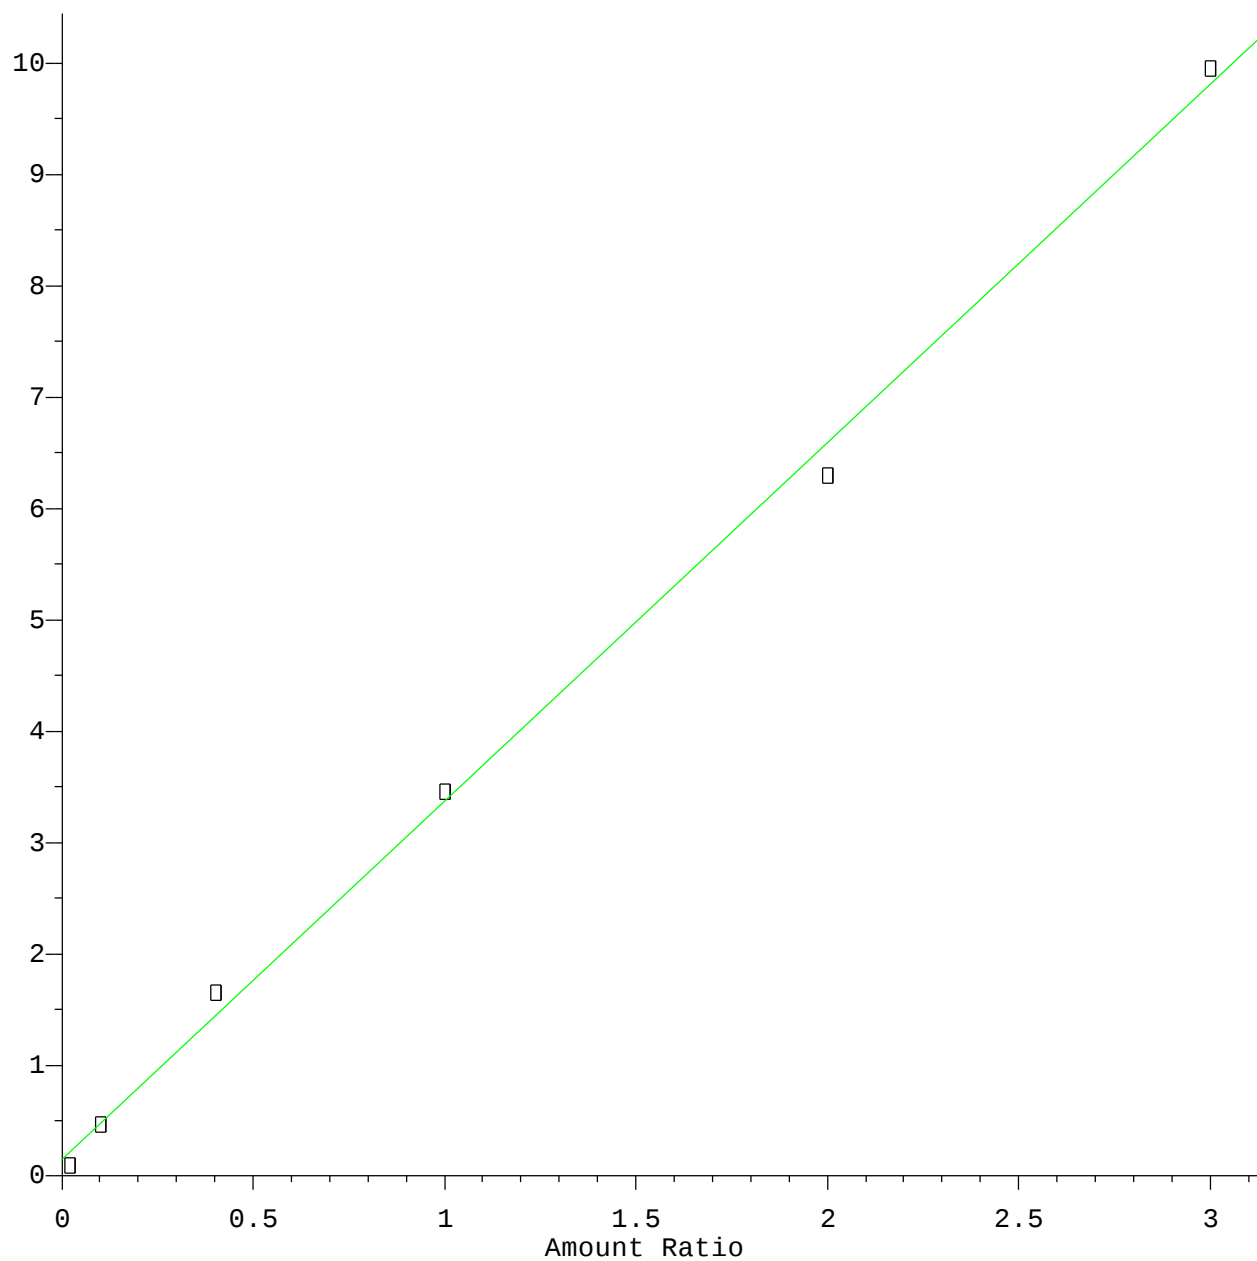


Resp Ratio = 3.22e+000 * Amt + 1.52e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019

tert-Butylbenzene

Response Ratio

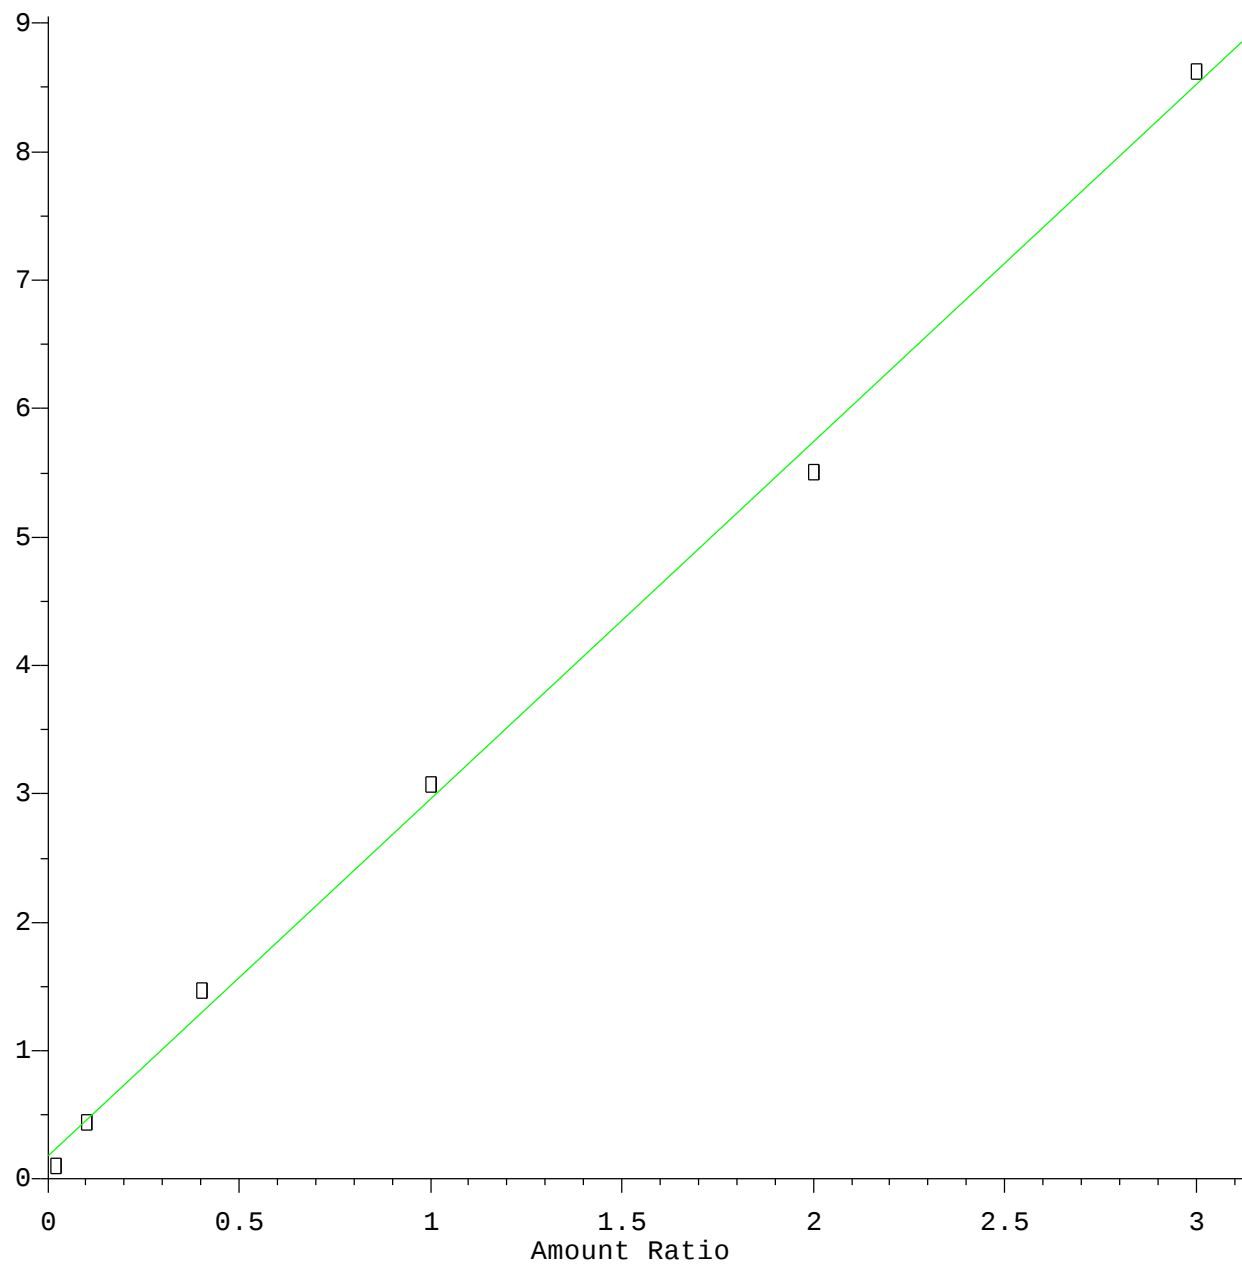

Resp Ratio = 2.78e+000 * Amt + 1.78e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Calibration Table Last Updated: Thu Aug 15 11:33:14 2019