
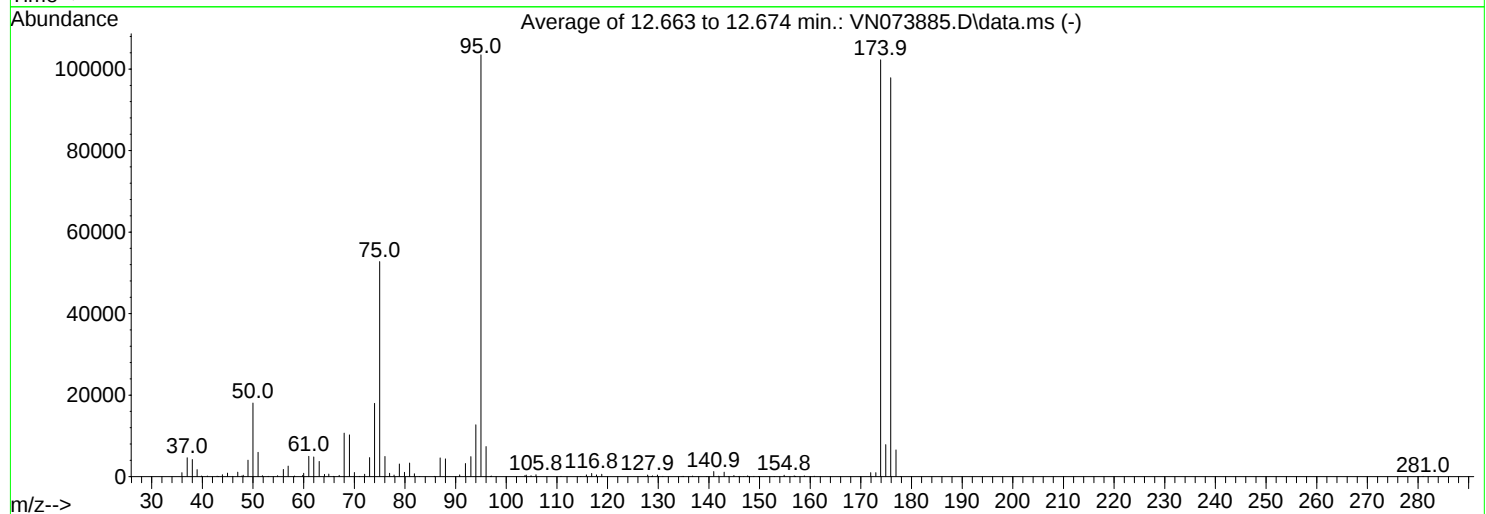


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081522\
Data File : VN073885.D
Acq On : 15 Aug 2022 09:19
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081522W.M
Title : SW846 8260
Last Update : Tue Aug 16 00:45:21 2022

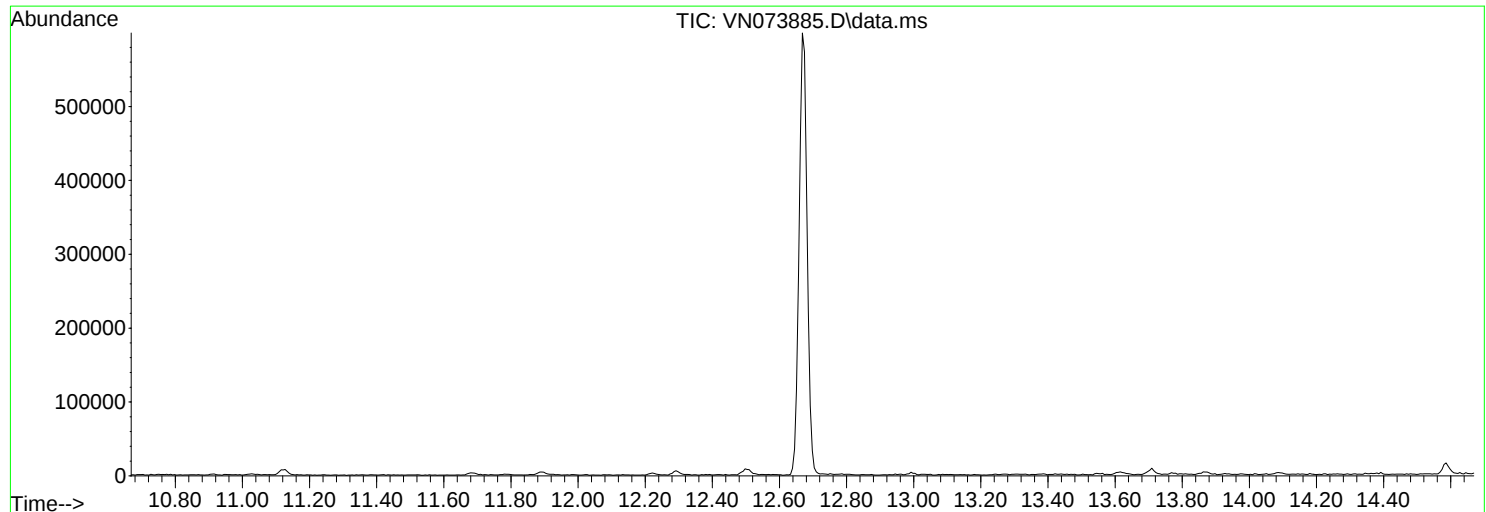

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	18055	PASS
75	95	30	60	51.0	52776	PASS
95	95	100	100	100.0	103488	PASS
96	95	5	9	7.1	7383	PASS
173	174	0.00	2	1.0	1000	PASS
174	95	50	100	98.8	102251	PASS
175	174	5	9	7.7	7845	PASS
176	174	95	101	95.7	97864	PASS
177	176	5	9	6.7	6541	PASS