
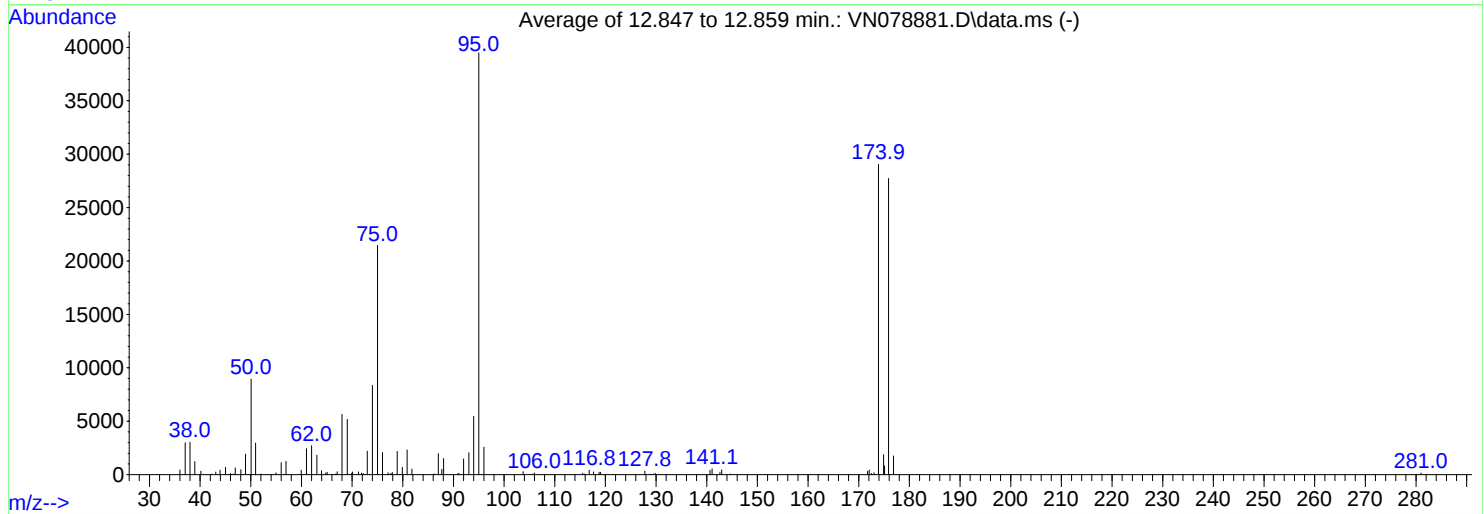


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081523\
 Data File : VN078881.D
 Acq On : 15 Aug 2023 10:12
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
 Title : SW846 8260
 Last Update : Wed Aug 16 02:42:02 2023

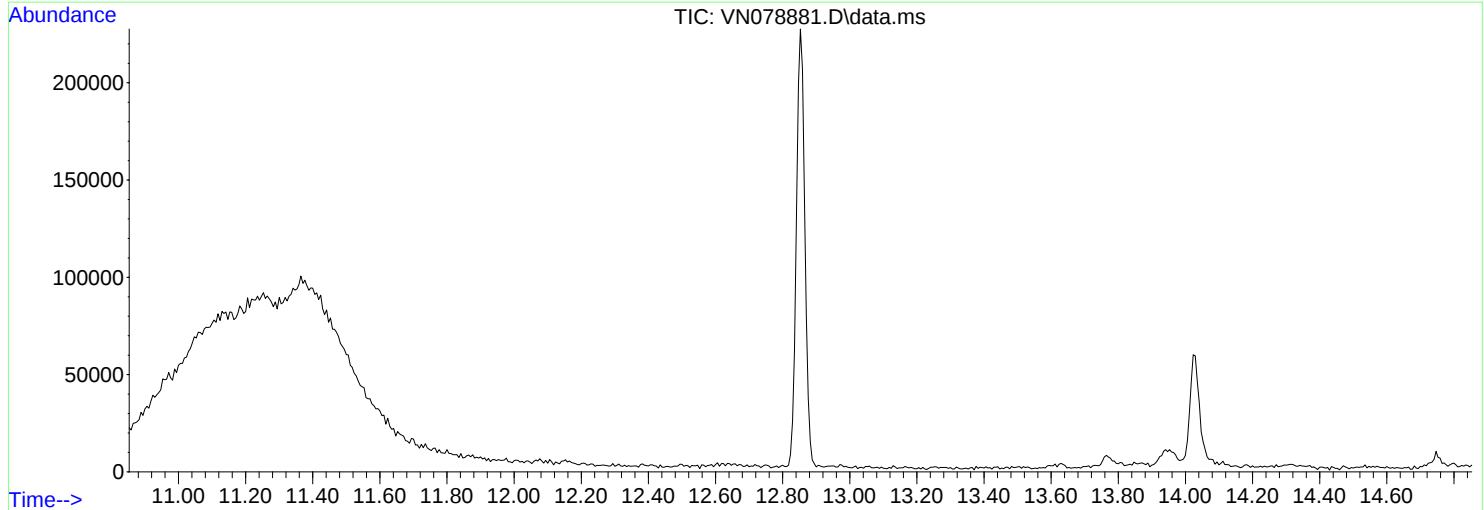

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	8942	PASS
75	95	30	60	54.3	21459	PASS
95	95	100	100	100.0	39488	PASS
96	95	5	9	6.5	2572	PASS
173	174	0.00	2	0.6	181	PASS
174	95	50	100	73.6	29051	PASS
175	174	5	9	6.5	1878	PASS
176	174	95	101	95.4	27723	PASS
177	176	5	9	6.3	1753	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	440	46.95	637	62.00	2711	71.25	261
37.05	2977	48.05	460	63.05	1826	71.85	151
38.00	3044	48.95	1913	63.95	383	72.20	101
38.95	1234	50.05	8942	64.80	161	73.00	220
40.15	337	50.95	2951	65.05	220	74.00	8364
42.30	63	52.00	61	66.80	70	75.00	21459
43.10	241	55.00	163	67.05	271	76.00	2071
43.95	419	56.00	1118	68.00	5642	77.10	186
45.00	671	56.95	1242	69.05	5175	77.70	143
46.00	110	59.95	417	69.90	130	77.95	196
46.70	79	61.00	2420	70.10	248	78.90	2176

Average of 12.847 to 12.859 min.: VN078881.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.90	695	94.00	5450	119.05	211	172.05	443
80.85	2306	95.00	39488	127.80	342	172.50	113
81.80	518	96.00	2572	128.80	51	173.00	181
86.20	68	103.75	292	129.60	68	173.90	29051
87.00	1982	105.70	75	129.90	103	174.90	1878
87.70	490	106.00	149	140.65	413	175.10	814
88.05	1511	115.50	138	141.05	554	175.90	27723
90.80	82	115.90	64	142.60	212	176.85	1753
91.10	128	116.80	419	142.95	446	281.00	152
92.00	1467	117.65	262	144.70	60		
93.05	2060	118.75	232	171.75	320		

Instrument :

MSVOA_N

ClientSampleId :

BFB