
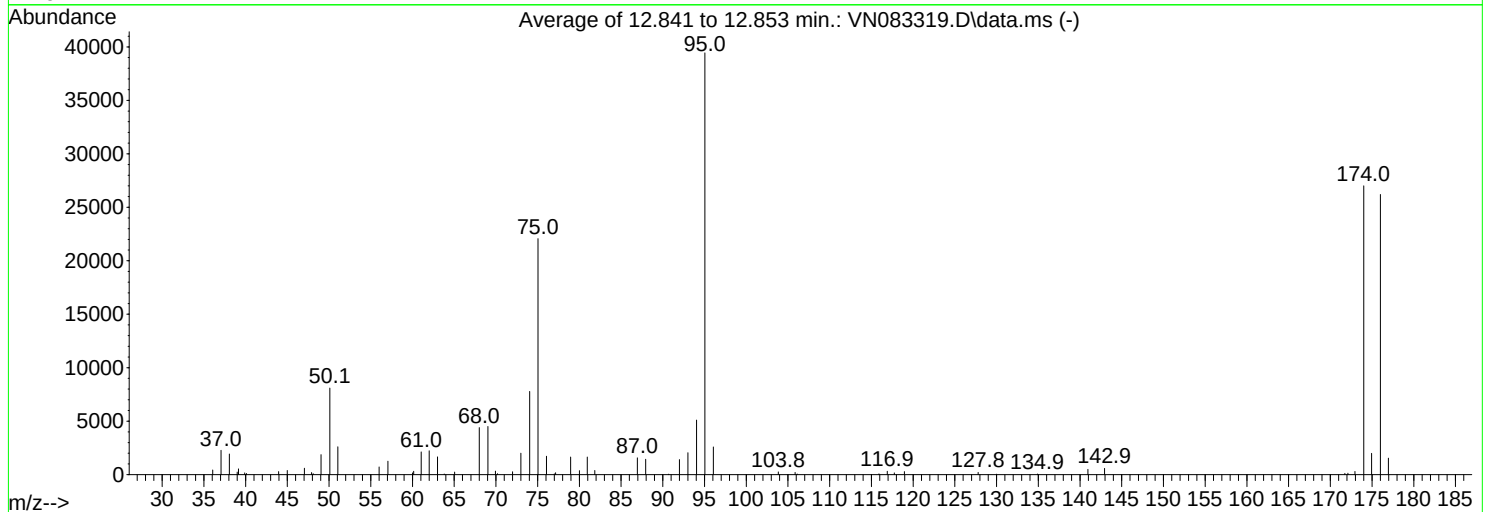


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081524\
Data File : VN083319.D
Acq On : 15 Aug 2024 09:38
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

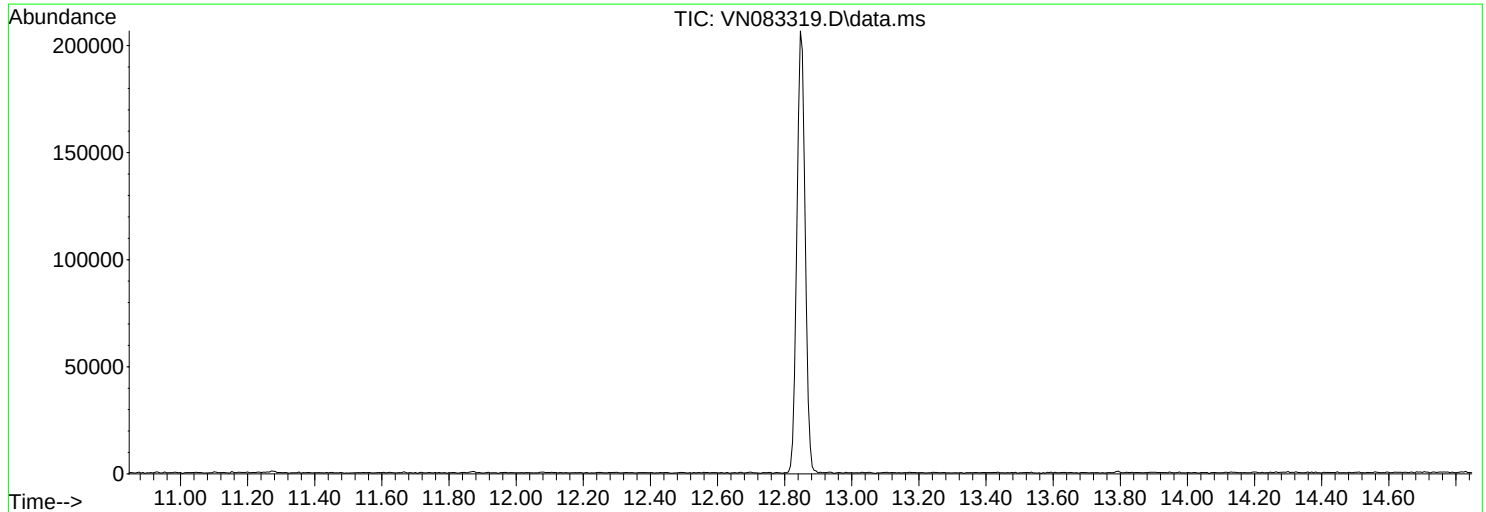

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	8100	PASS
75	95	30	60	56.0	22072	PASS
95	95	100	100	100.0	39443	PASS
96	95	5	9	6.6	2588	PASS
173	174	0.00	2	1.1	296	PASS
174	95	50	100	68.5	27013	PASS
175	174	5	9	7.4	1992	PASS
176	174	95	101	97.0	26195	PASS
177	176	5	9	5.9	1548	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	441	48.10	86	63.80	58	77.00	7
37.05	2270	49.05	1877	65.05	235	77.15	18
38.05	1937	50.10	8100	68.00	4393	78.95	164
39.00	241	51.05	2606	69.05	4511	80.00	37
39.15	540	56.00	724	69.95	326	80.95	1641
39.90	173	57.05	1253	70.20	85	81.85	386
40.10	109	60.00	172	72.00	276	86.95	1574
43.95	290	60.15	308	73.00	2010	87.95	1430
45.00	384	61.05	2133	74.05	7783	90.70	52
47.05	605	62.00	2233	75.05	22072	92.00	1415
47.90	200	63.00	1668	76.05	1726	93.00	2048

Average of 12.841 to 12.853 min.: VN083319.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	5109	130.00	50				
95.05	39443	134.90	54				
96.05	2588	140.95	496				
103.85	251	142.95	586				
105.85	217	171.75	125				
106.10	59	172.10	136				
115.90	73	172.95	296				
116.90	314	174.00	27013				
117.75	163	174.95	1992				
118.95	279	176.00	26195				
127.80	213	176.95	1548				

Instrument :

MSVOA_N

ClientSampleId :

BFB