


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081525\
Data File : VN087572.D
Acq On : 15 Aug 2025 09:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Title : SW846 8260
Last Update : Thu Jul 17 02:56:13 2025

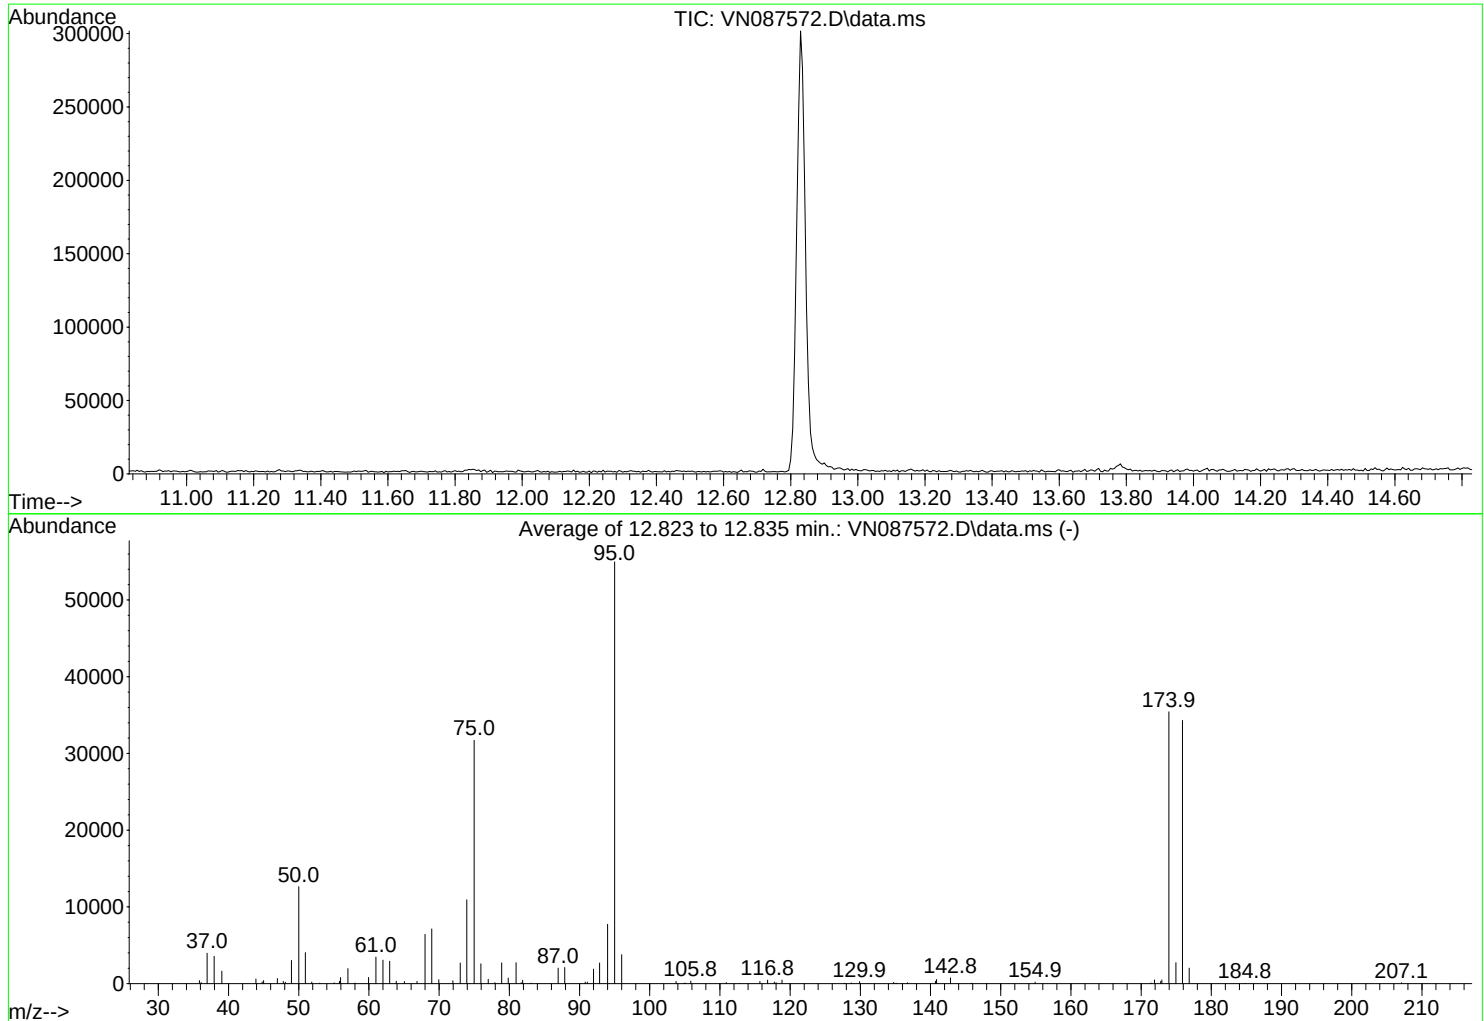

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	12636	PASS
75	95	30	60	57.7	31723	PASS
95	95	100	100	100.0	54971	PASS
96	95	5	9	6.9	3773	PASS
173	174	0.00	2	1.4	484	PASS
174	95	50	100	64.5	35435	PASS
175	174	5	9	7.7	2723	PASS
176	174	95	101	96.8	34307	PASS
177	176	5	9	5.9	2032	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	392	48.95	3030	61.00	3458	73.95	1092
36.10	154	50.00	12636	62.00	3058	75.00	3172
36.95	3959	50.95	4057	62.95	2924	75.95	258
37.95	3561	51.85	207	63.90	312	77.00	55
39.05	1625	53.00	54	65.05	264	77.95	129
43.90	598	55.05	109	66.85	295	78.90	2718
44.80	227	55.80	309	68.00	6415	79.85	740
45.00	395	55.95	791	68.95	7142	80.95	2738
46.95	669	57.00	1958	69.95	519	81.70	132
47.80	290	58.00	92	71.95	377	81.90	438
48.10	193	59.95	814	73.00	2698	83.10	63

Average of 12.823 to 12.835 min.: VN087572.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	2018	105.10	67	129.90	273	171.90	487
87.90	2098	105.85	333	134.75	166	172.80	299
90.80	213	110.90	143	135.10	56	172.95	484
91.10	216	112.80	52	136.70	130	173.95	35435
92.00	1897	115.70	287	140.70	309	174.95	2723
92.85	2686	116.80	456	140.85	536	175.90	34307
94.00	7730	117.75	209	142.85	746	176.85	2032
95.00	54971	118.00	131	145.80	55	184.80	52
96.00	3773	118.85	454	148.00	51	207.10	121
103.75	287	127.80	69	154.90	212		
104.90	73	128.70	90	171.40	76		

Instrument :

MSVOA_N

ClientSampleId :

BFB