

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN081618\
 Data File : VN050691.D
 Acq On : 16 Aug 2018 10:05
 Operator : MD\SY
 Sample : VN0816MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0816MBL01

Quant Time: Aug 17 03:47:33 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 14 08:07:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	632733	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1006228	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	853662	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	284143	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	422176	52.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.86%	
35) Dibromofluoromethane	7.59	113	398324	49.58	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.16%	
50) Toluene-d8	10.09	98	1417750	46.89	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.78%	
62) 4-Bromofluorobenzene	12.40	95	364874	36.53	ug/l	0.00
Spiked Amount	50.000		Recovery	=	73.06%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN081618\
Data File : VN050691.D
Acq On : 16 Aug 2018 10:05
Operator : MD\SY
Sample : VN0816MBL01
Misc : 5.00µ/10mL/100µL/5.00mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0816MBL01

Quant Time: Aug 17 03:47:33 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 14 08:07:08 2018
Response via : Initial Calibration

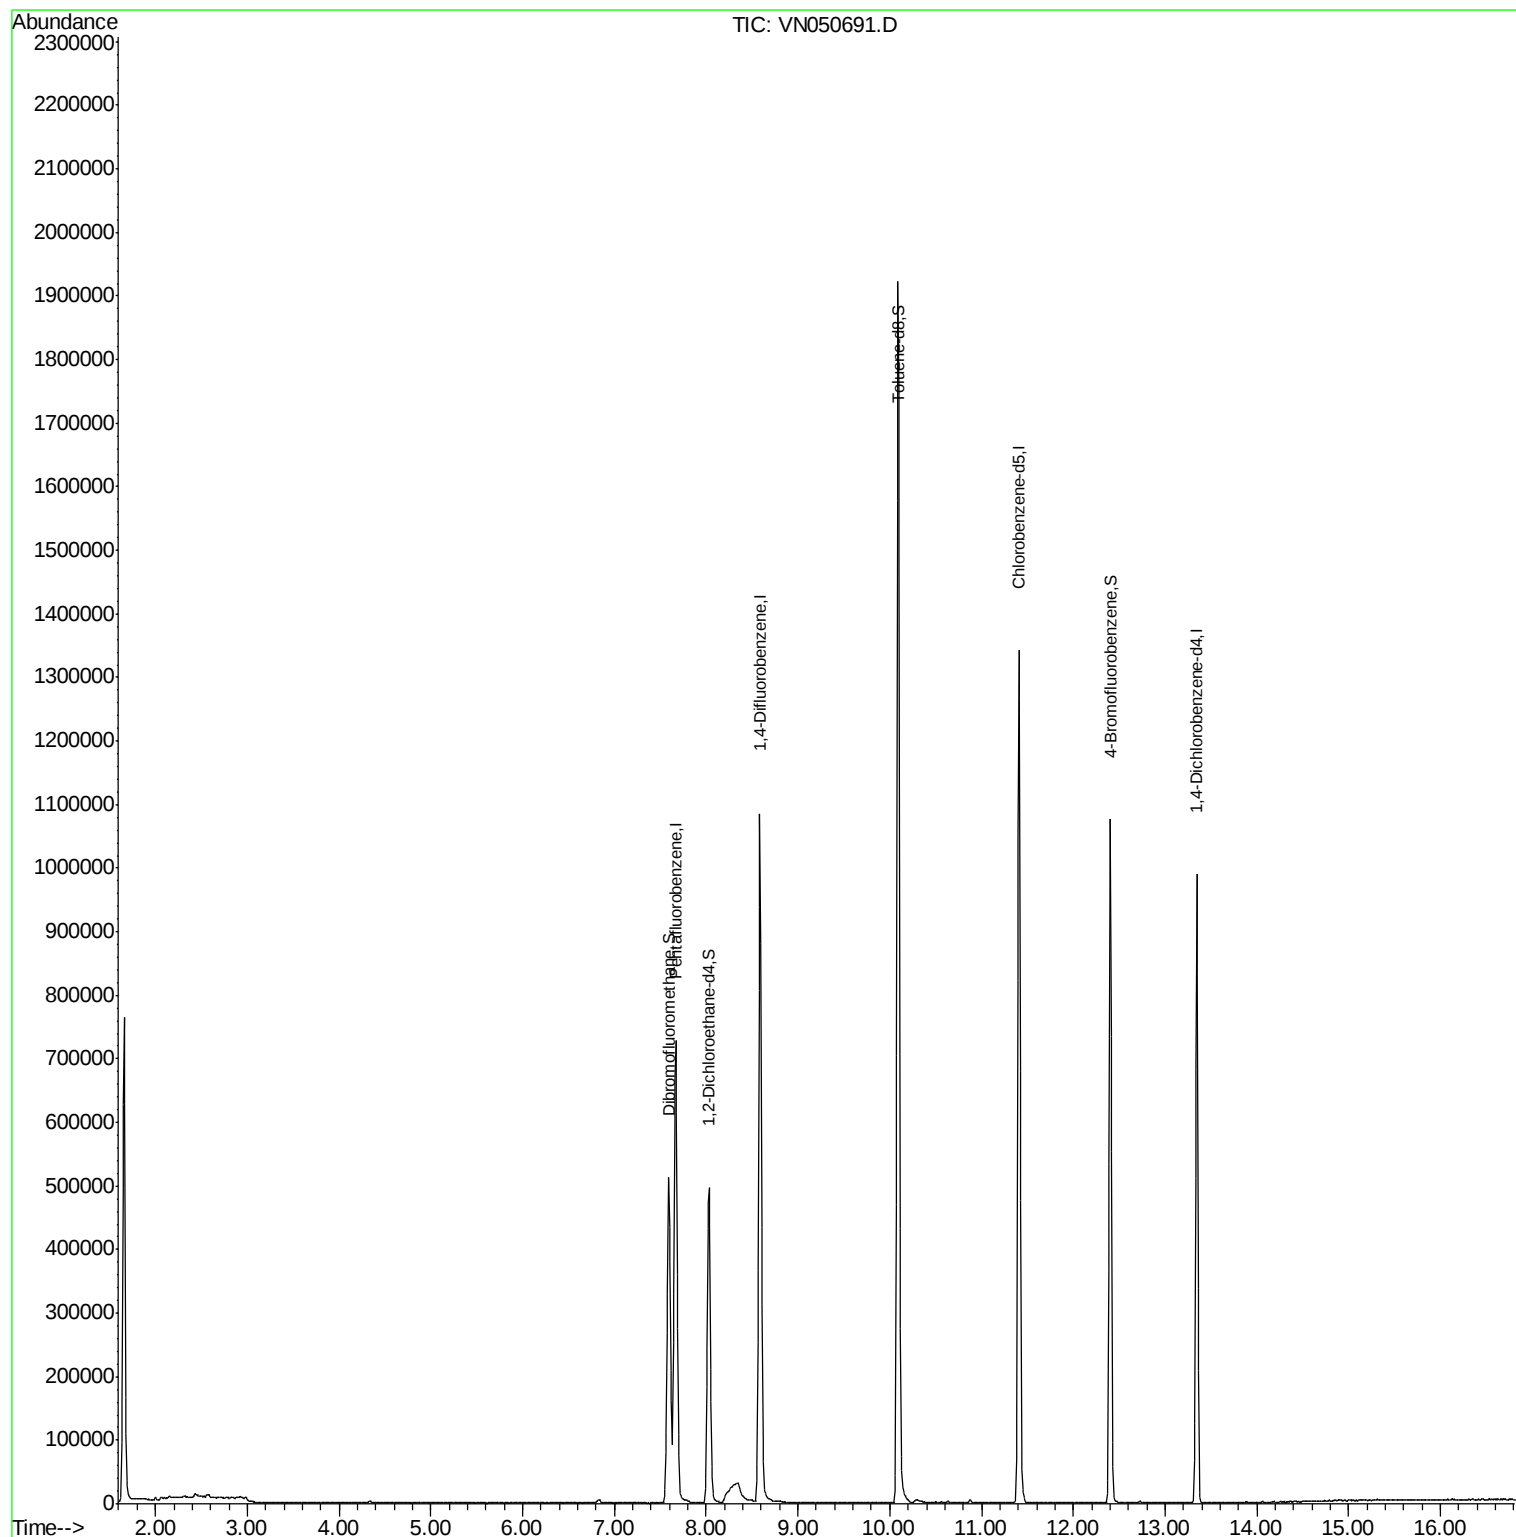

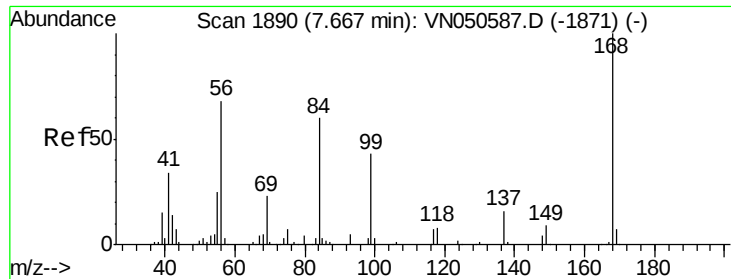

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1890

Delta R.T. -0.00 min

Lab File: VN050691.D

Acq: 16 Aug 2018 10:05

Instrument :

MSVOA_N

ClientSampled :


VN0816MBL01

Tot Ion:168 Resp: 632733

Ion Ratio Lower Upper

168 100

99 51.1 40.8 61.2

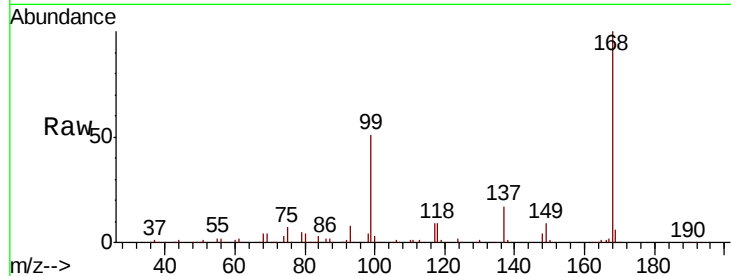

Abundance Ion 167.90 (167.60 to 168.60): VN050587.D (-1871) (-)

Ion 98.90 (98.60 to 99.60): VN050587.D (-1871) (-)

7.67

250000

200000



150000

100000

50000

0

Time-->

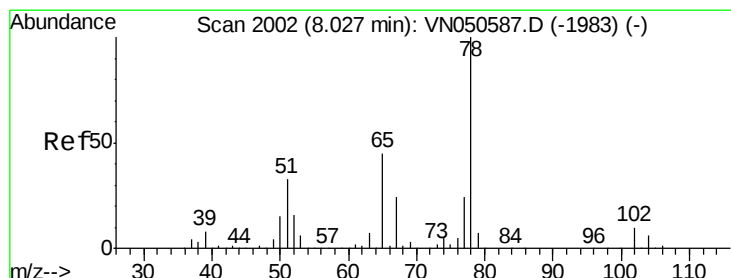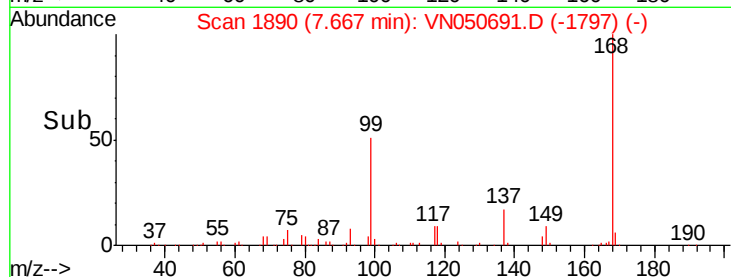

#33

1,2-Dichloroethane-d4

Concen: 52.93 ug/l

RT: 8.03 min Scan# 2003

Delta R.T. 0.00 min

Lab File: VN050691.D


Acq: 16 Aug 2018 10:05

Tgt Ion: 65 Resp: 422176

Ion Ratio Lower Upper

65 100

67 54.9 0.0 109.8

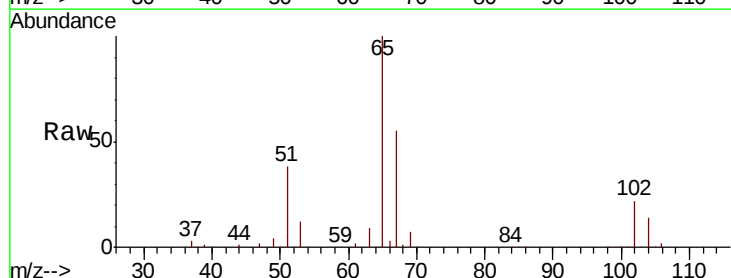

Abundance Ion 64.90 (64.60 to 65.60): VN050587.D (-1983) (-)

Ion 66.90 (66.60 to 67.60): VN050587.D (-1983) (-)

8.03

200000


150000


100000

50000

0

Time-->

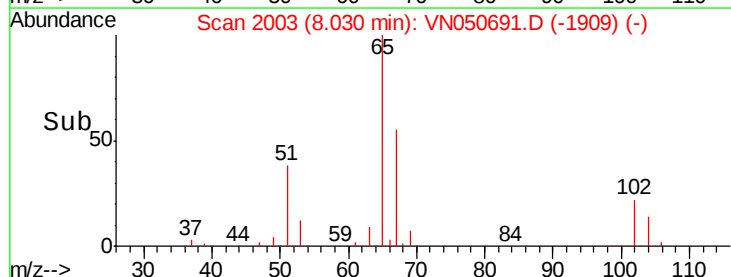


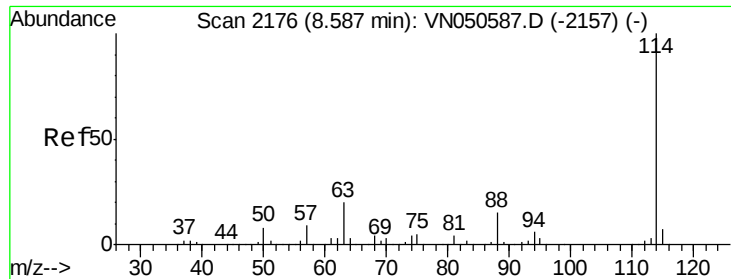




#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2176
 Delta R.T. -0.00 min
 Lab File: VN050691.D
 Acq: 16 Aug 2018 10:05

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0816MBL01

Tot Ion:114 Resp: 1006228
 Ion Ratio Lower Upper
 114 100
 63 19.5 0.0 40.0
 88 15.2 0.0 30.8

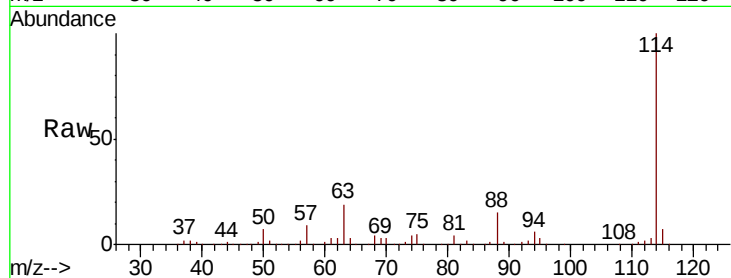


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

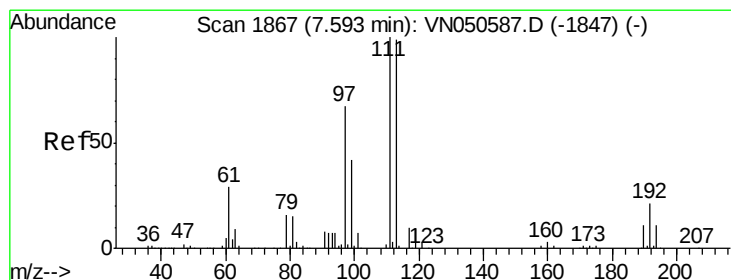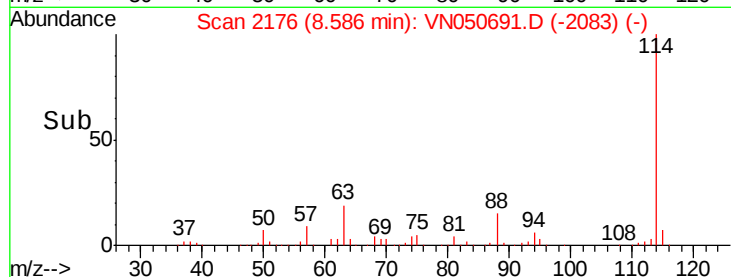
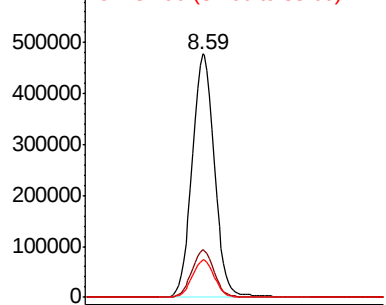



#35
 Dibromofluoromethane
 Concen: 49.58 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. -0.00 min
 Lab File: VN050691.D
 Acq: 16 Aug 2018 10:05

Tgt Ion:113 Resp: 398324
 Ion Ratio Lower Upper
 113 100
 111 102.2 81.0 121.6
 192 22.5 17.6 26.4

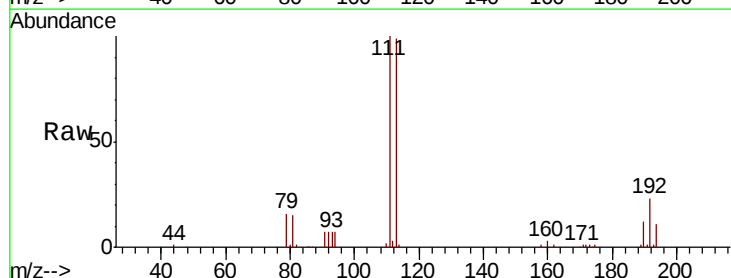

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



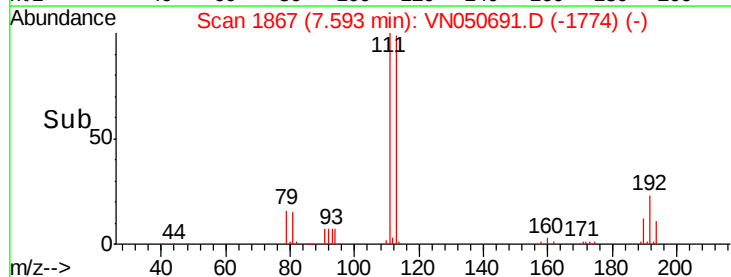
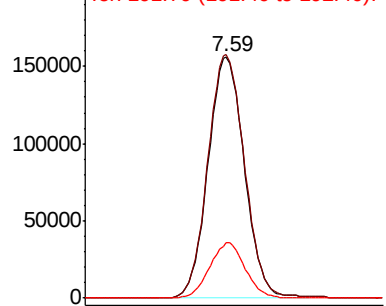


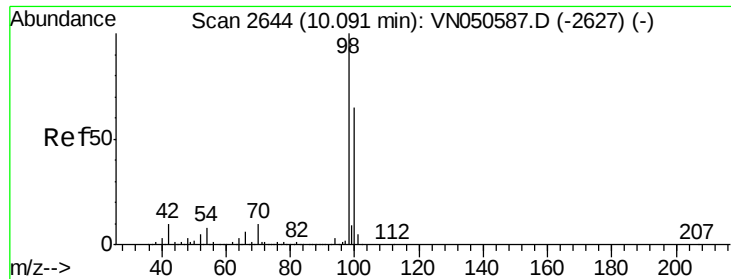

#50
Toluene-d8
Concen: 46.89 ug/l
RT: 10.09 min Scan# 2644
Delta R.T. -0.00 min
Lab File: VN050691.D
Acq: 16 Aug 2018 10:05




Instrument :
MSVOA_N
ClientSampleId :
VN0816MBL01


Tot Ion: 98 Resp: 1417750
Ion Ratio Lower Upper
98 100
100 63.1 51.8 77.8

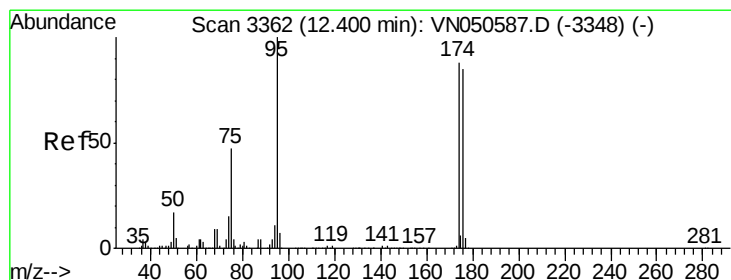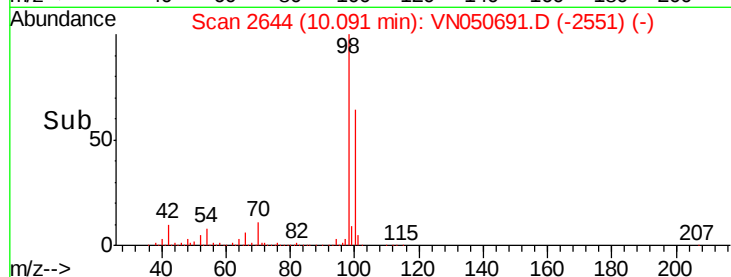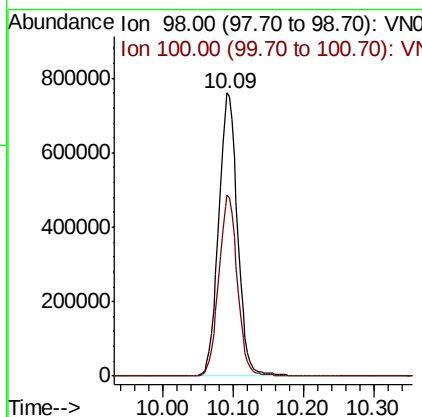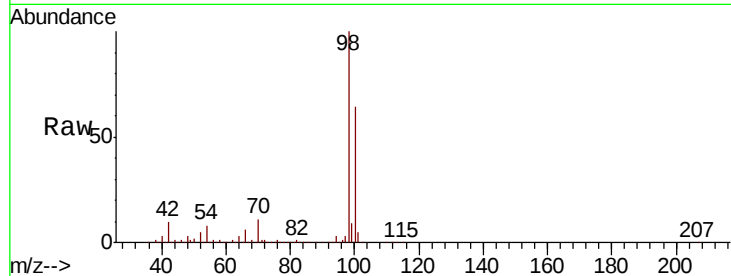

#62
4-Bromofluorobenzene
Concen: 36.53 ug/l
RT: 12.40 min Scan# 3363
Delta R.T. 0.00 min
Lab File: VN050691.D
Acq: 16 Aug 2018 10:05

Tgt Ion: 95 Resp: 364874
Ion Ratio Lower Upper
95 100
174 91.4 0.0 177.8
176 88.6 0.0 175.0

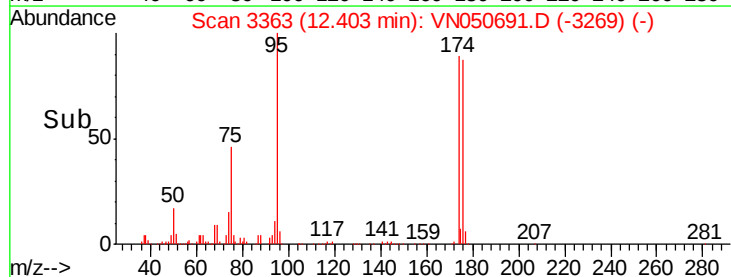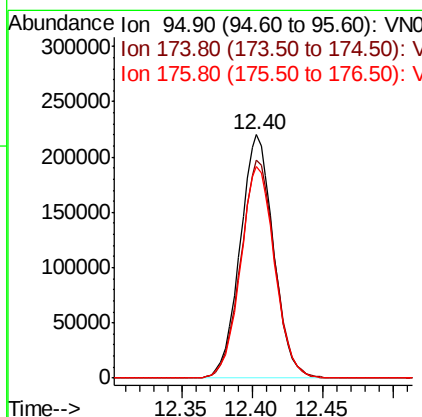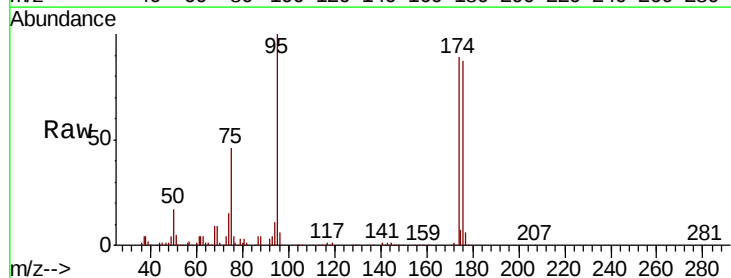


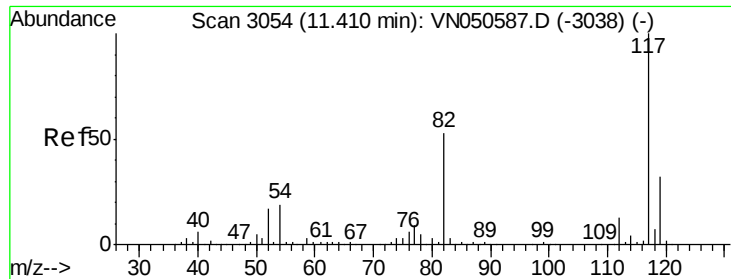




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.41 min Scan# 3054
Delta R.T. -0.00 min
Lab File: VN050691.D
Acq: 16 Aug 2018 10:05

Instrument :
MSVOA_N
ClientSampleId :
VN0816MBL01

Tot Ion:117 Resp: 853662
Ion Ratio Lower Upper
117 100
82 52.0 42.4 63.6
119 32.2 25.8 38.8

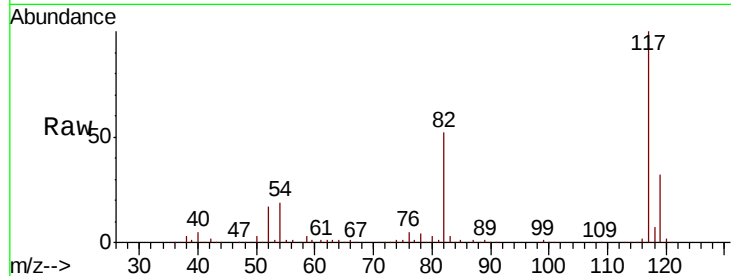


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

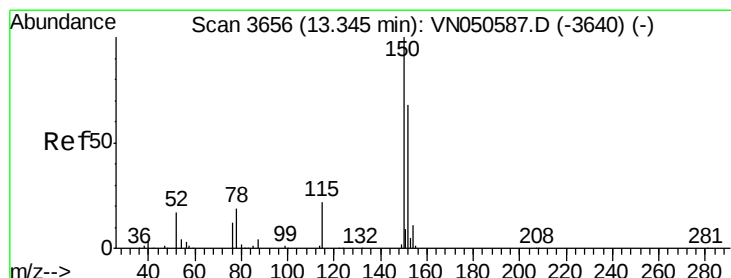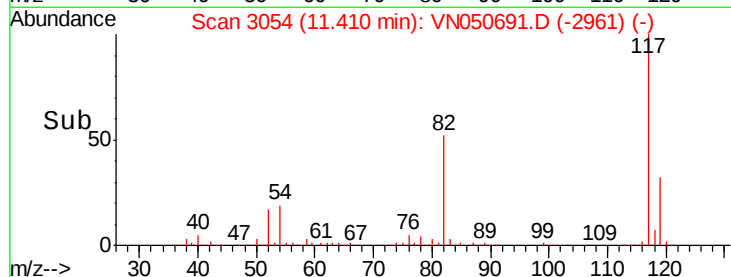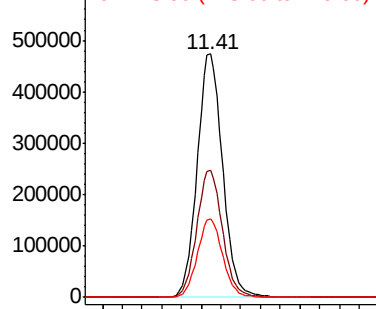

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.35 min Scan# 3656
Delta R.T. -0.00 min
Lab File: VN050691.D
Acq: 16 Aug 2018 10:05

Tgt Ion:152 Resp: 284143
Ion Ratio Lower Upper
152 100
115 56.7 28.1 84.2
150 156.7 0.0 347.8

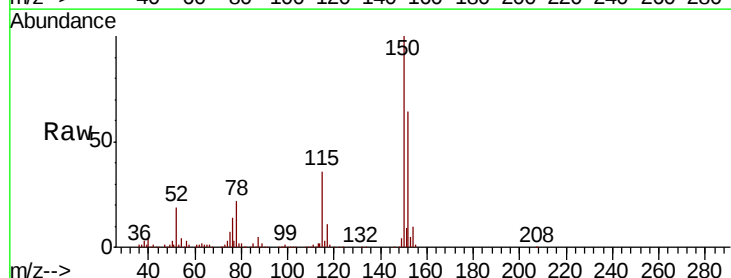

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

