


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081618\
Data File : VN050688.D
Acq On : 16 Aug 2018 8:31
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
Title : SW846 8260
Last Update : Tue Aug 14 08:07:08 2018

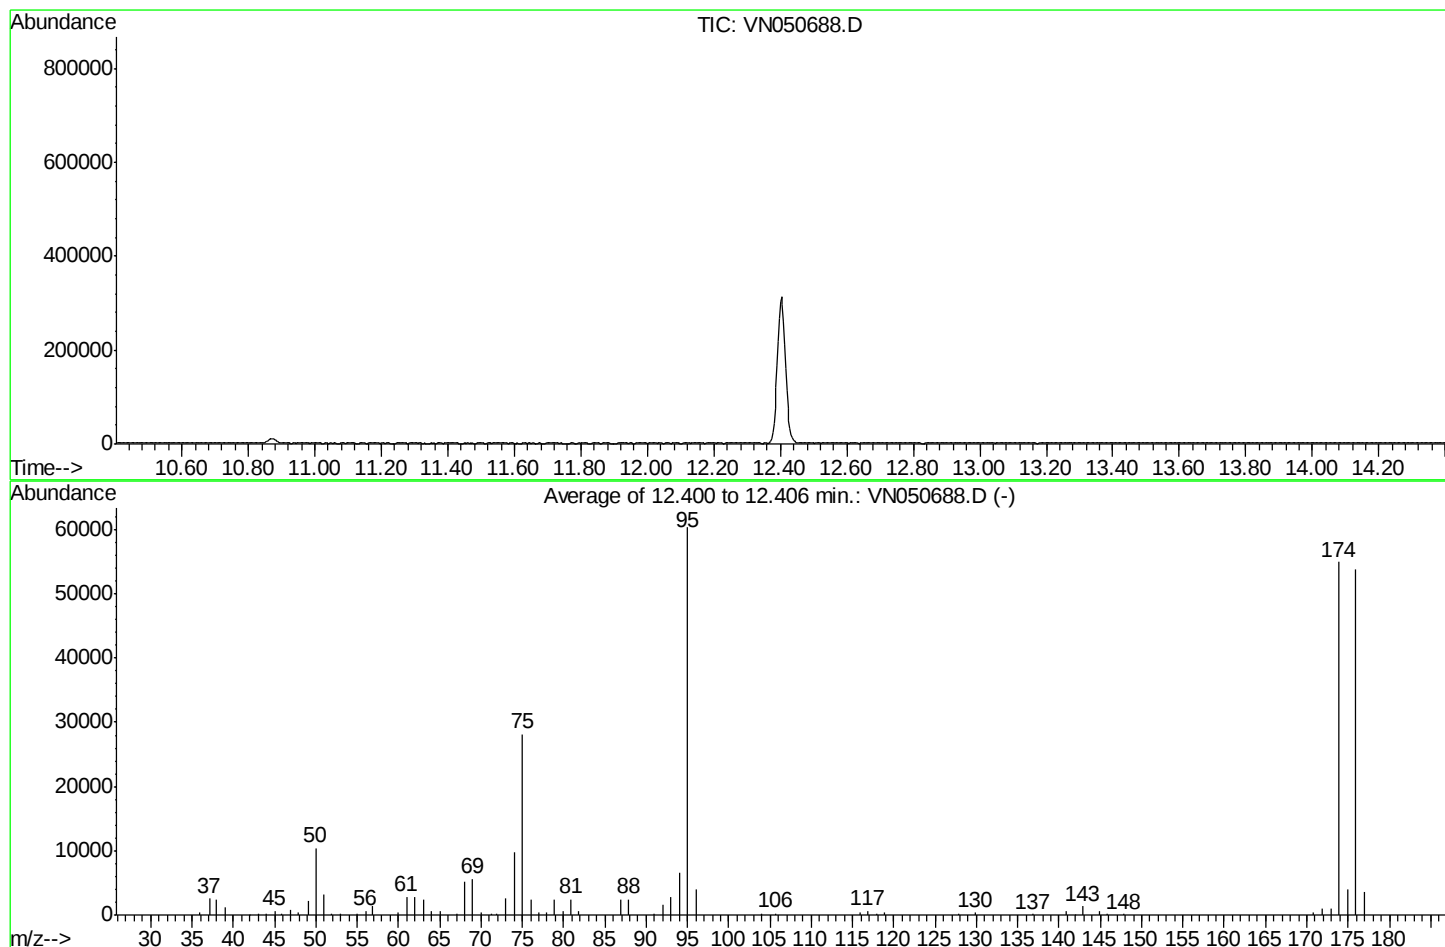

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	10394	PASS
75	95	30	60	46.7	28157	PASS
95	95	100	100	100.0	60352	PASS
96	95	5	9	6.6	3996	PASS
173	174	0.00	2	1.9	1025	PASS
174	95	50	100	91.0	54949	PASS
175	174	5	9	7.4	4056	PASS
176	174	95	101	98.1	53904	PASS
177	176	5	9	6.7	3629	PASS