


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081619\
Data File : VN057316.D
Acq On : 15 Aug 2019 8:19
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Title : SW846 8260
Last Update : Thu Aug 15 11:33:14 2019

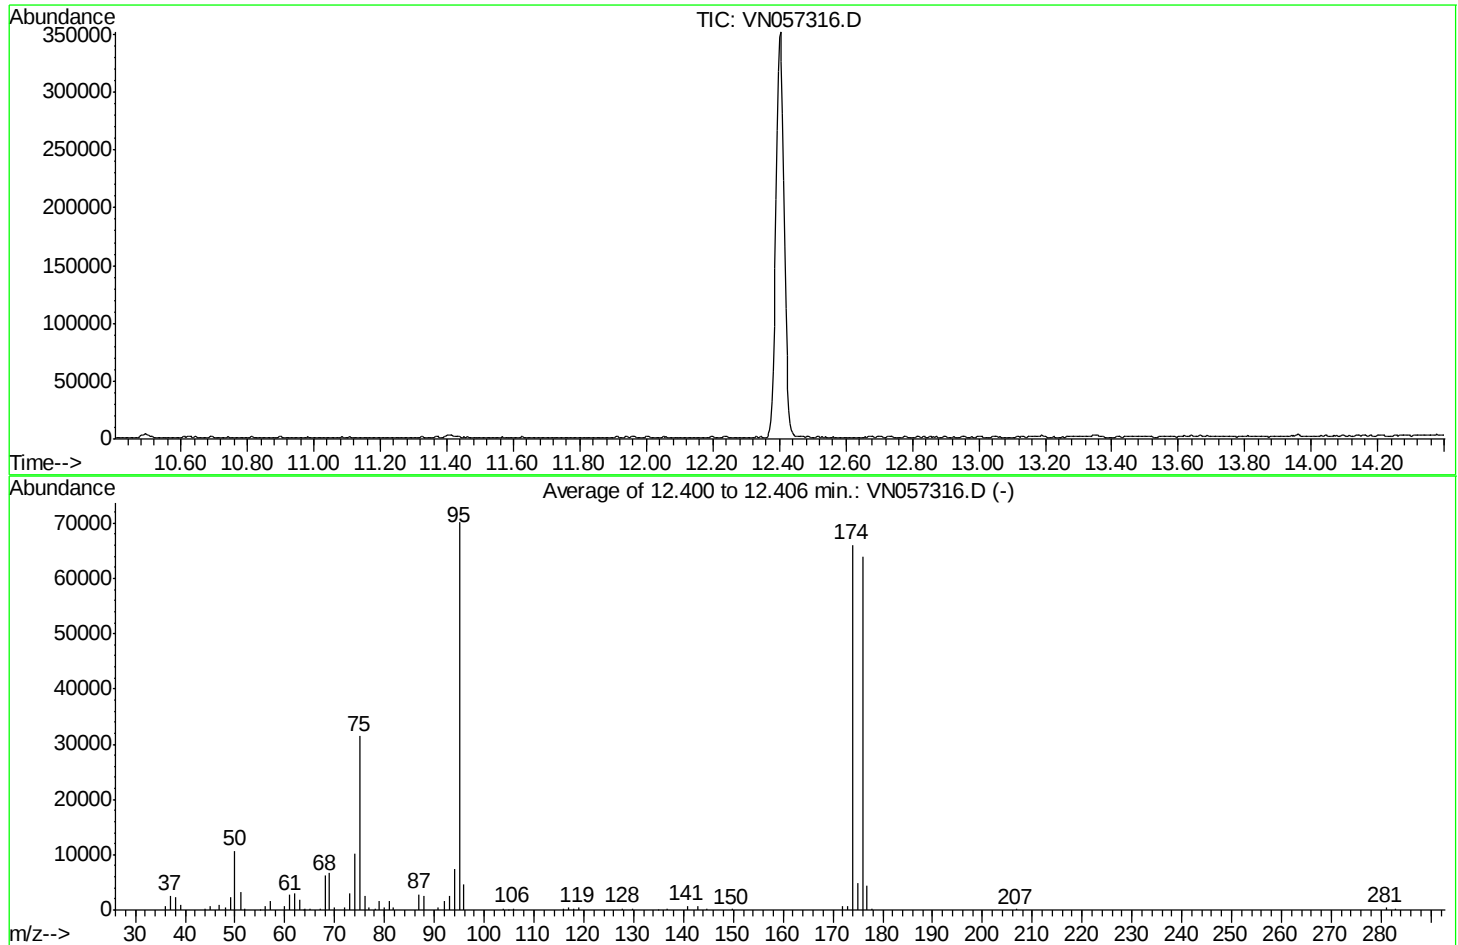

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.2	10674	PASS
75	95	30	60	44.9	31472	PASS
95	95	100	100	100.0	70157	PASS
96	95	5	9	6.5	4561	PASS
173	174	0.00	2	1.1	728	PASS
174	95	50	100	94.2	66064	PASS
175	174	5	9	7.5	4961	PASS
176	174	95	101	96.7	63856	PASS
177	176	5	9	7.1	4526	PASS