

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081621\
 Data File : VN068119.D
 Acq On : 16 Aug 2021 16:36
 Operator : JC/MD
 Sample : PB138399ZHE#08
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB138399ZHE#08

Quant Time: Aug 17 07:14:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 29 15:02:35 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	232187	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	470530	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	517500	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.677	152	177412	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	197844	60.190	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 120.380%			
35) Dibromofluoromethane	8.024	113	146476	53.416	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 106.840%			
50) Toluene-d8	10.443	98	650187	51.270	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 102.540%			
62) 4-Bromofluorobenzene	12.733	95	225347	48.782	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 97.560%			
Target Compounds						Qvalue
11) Tert butyl alcohol	5.382	59	211	0.479	ug/l #	71
13) Acrolein	4.049	56	167	0.559	ug/l #	53
16) Acetone	4.293	43	40470	33.743	ug/l #	87
18) Methyl Acetate	4.862	43	6596	2.190	ug/l #	90
20) Methylene Chloride	5.095	84	26407	9.304	ug/l	91
23) Vinyl Acetate	6.315	43	25	8.803	ug/l #	75
25) 2-Butanone	7.343	43	7120	4.092	ug/l	99
29) Tetrahydrofuran	7.694	42	1018	0.914	ug/l #	68
31) Cyclohexane	8.088	56	6283	1.296	ug/l #	1
36) 1,1-Dichloropropene	8.088	75	21931	5.039	ug/l #	50
38) Carbon Tetrachloride	8.088	117	26063	6.089	ug/l #	19
43) Isopropyl Acetate	8.563	43	38614	5.657	ug/l #	90
45) 1,2-Dichloropropane	9.628	63	2350	0.732	ug/l #	44
48) Methyl methacrylate	9.544	41	7722	4.469	ug/l #	12
49) 1,4-Dioxane	9.633	88	132	2.431	ug/l #	1
51) 4-Methyl-2-Pentanone	10.336	43	8220	14.136	ug/l #	86
53) t-1,3-Dichloropropene	10.443	75	51	2.842	ug/l #	82
54) cis-1,3-Dichloropropene	10.247	75	56597	11.617	ug/l #	62
56) Ethyl methacrylate	10.872	69	560	3.189	ug/l #	1
57) 1,3-Dichloropropane	11.095	76	36916	6.975	ug/l #	43
59) 2-Hexanone	11.095	43	550843	160.408	ug/l #	54
60) Dibromochloromethane	11.492	129	263	3.363	ug/l #	11
68) m/p-Xylenes	11.950	106	103	4.074	ug/l #	32
70) Styrene	12.296	104	195	2.645	ug/l #	22
71) Bromoform	12.731	173	473	4.162	ug/l #	1
76) 1,2,3-Trichloropropane	12.733	75	122303	34.326	ug/l #	100
80) 1,3,5-Trimethylbenzene	13.063	105	6830	0.582	ug/l	95
81) trans-1,4-Dichloro-2-b...	12.733	75	122303	91.980	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.262	180	100	2.503	ug/l #	12
95) Naphthalene	15.512	128	855	3.228	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.710	180	163	2.430	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081621\
Data File : VN068119.D
Acq On : 16 Aug 2021 16:36
Operator : JC/MD
Sample : PB138399ZHE#08
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08

Quant Time: Aug 17 07:14:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 29 15:02:35 2021
Response via : Initial Calibration




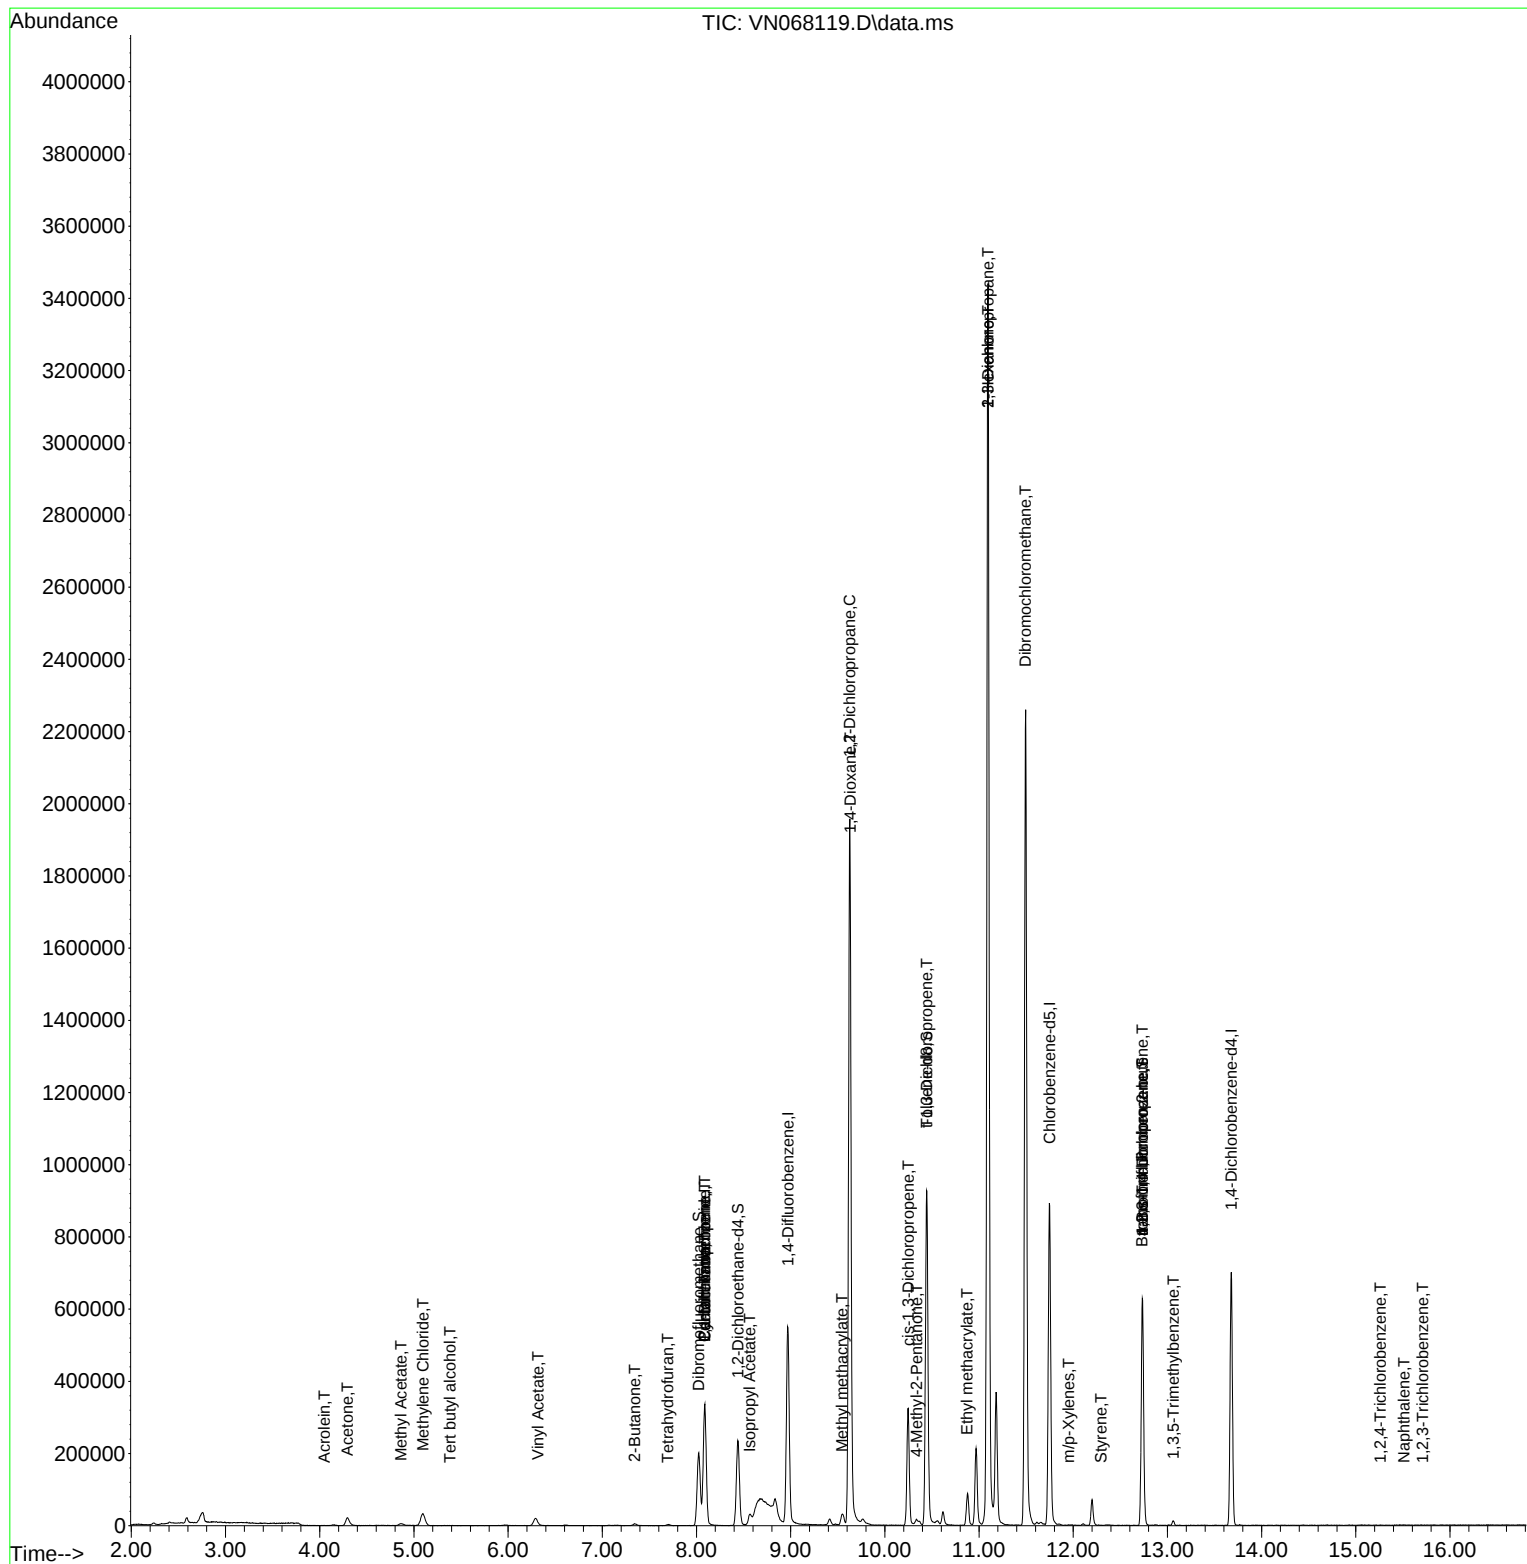


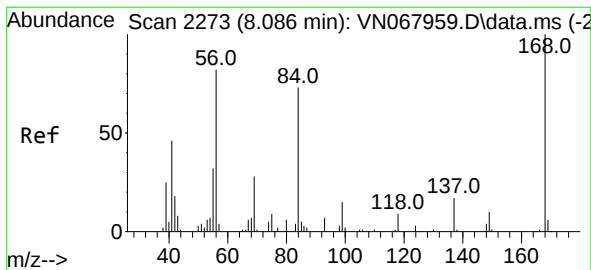

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08


Tgt Ion:168 Resp: 232187
Ion Ratio Lower Upper
168 100
99 65.1 62.9 94.3

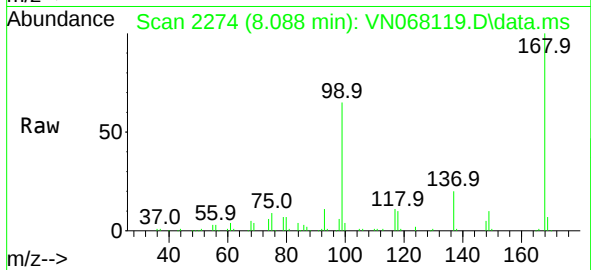

#11
Tert butyl alcohol
Concen: 0.479 ug/l
RT: 5.382 min Scan# 1265
Delta R.T. -0.008 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Tgt Ion: 59 Resp: 211
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


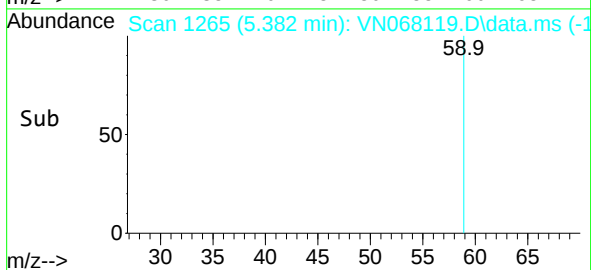

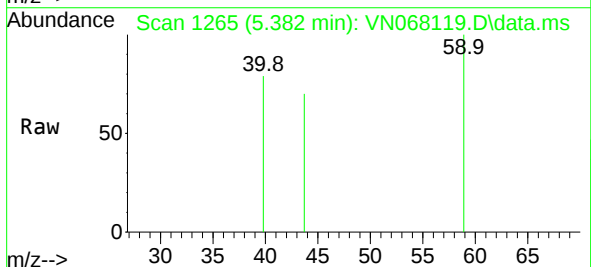


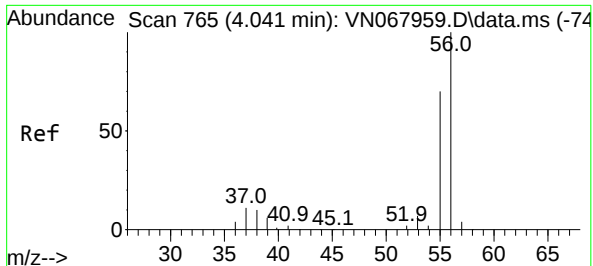

#13
Acrolein
Concen: 0.559 ug/l
RT: 4.049 min Scan# 768
Delta R.T. 0.008 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08


Tgt Ion: 56 Resp: 167
Ion Ratio Lower Upper
56 100
55 32.3 57.4 86.0#

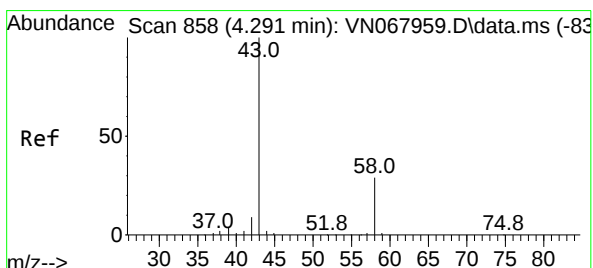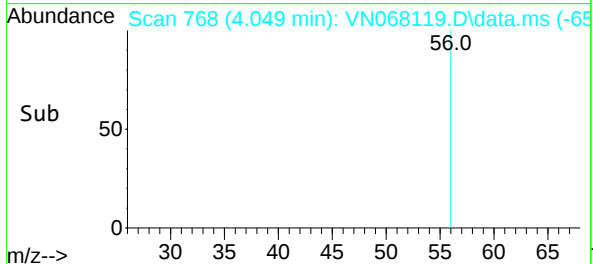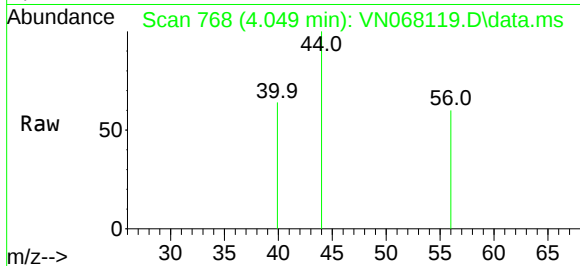

#16
Acetone
Concen: 33.743 ug/l
RT: 4.293 min Scan# 859
Delta R.T. 0.002 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Tgt Ion: 43 Resp: 40470
Ion Ratio Lower Upper
43 100
58 33.2 21.2 31.8#

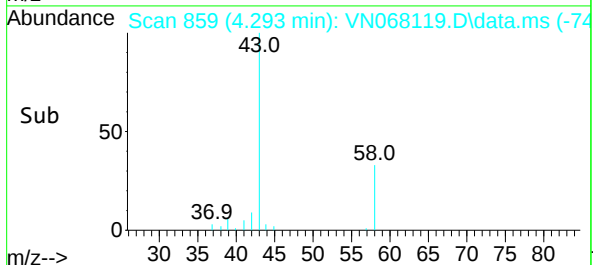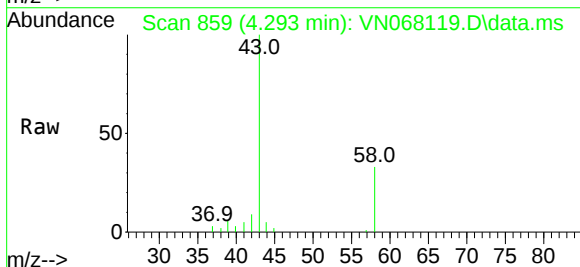

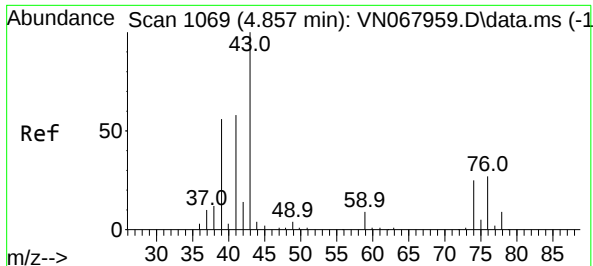

#18

Methyl Acetate

Concen: 2.190 ug/l

RT: 4.862 min Scan# 1071

Delta R.T. 0.005 min

Lab File: VN068119.D

Acq: 16 Aug 2021 16:36

Tgt Ion: 43 Resp: 6596

Ion Ratio Lower Upper

43 100





74 26.5 17.4 26.0#

Instrument :

MSVOA_N

ClientSampleId :

PB138399ZHE#08

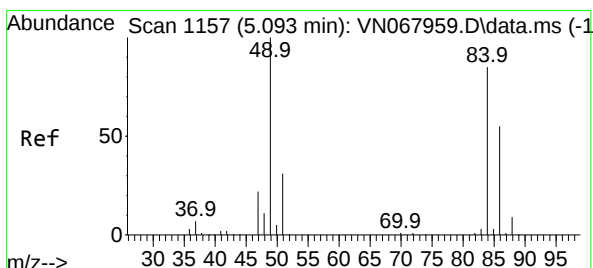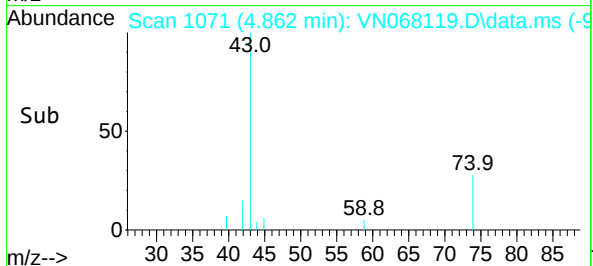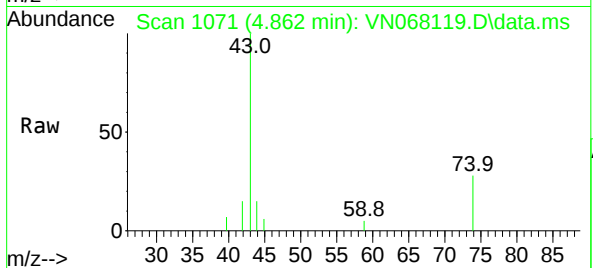

#20

Methylene Chloride

Concen: 9.304 ug/l

RT: 5.095 min Scan# 1158

Delta R.T. 0.002 min

Lab File: VN068119.D

Acq: 16 Aug 2021 16:36

Tgt Ion: 84 Resp: 26407




Ion Ratio Lower Upper


84 100

49 124.3 110.9 166.3

51 39.6 32.6 49.0

86 71.7 51.6 77.4

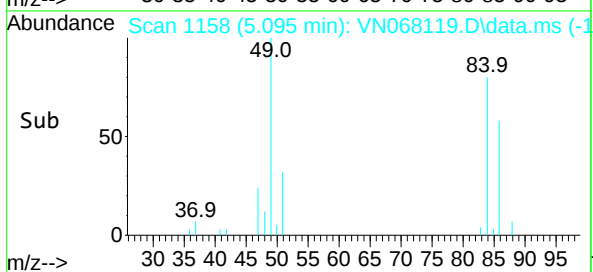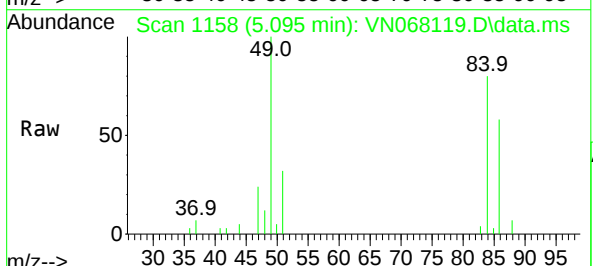

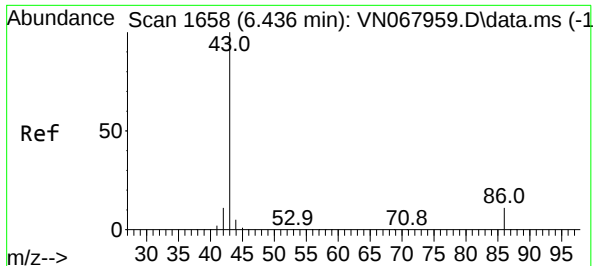

#23

Vinyl Acetate

Concen: 8.803 ug/l

RT: 6.315 min Scan# 1613

Delta R.T. -0.121 min

Lab File: VN068119.D

Acq: 16 Aug 2021 16:36

Instrument :

MSVOA_N

ClientSampleId :





PB138399ZHE#08

Tgt Ion: 43 Resp: 25

Ion Ratio Lower Upper

43 100

86 0.0 7.3 10.9#

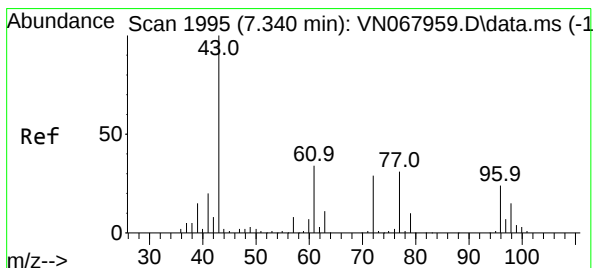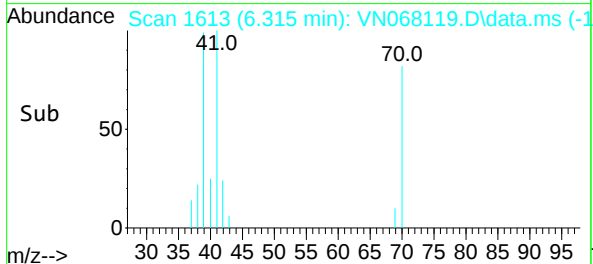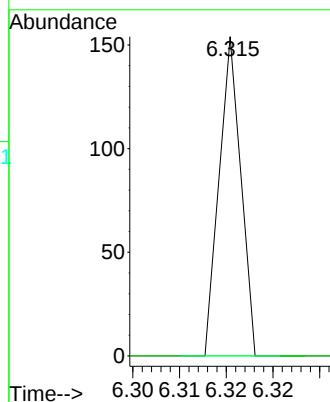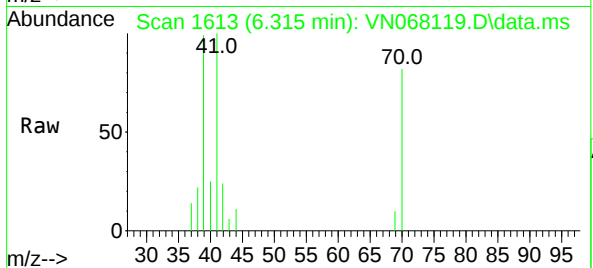

#25

2-Butanone

Concen: 4.092 ug/l

RT: 7.343 min Scan# 1996

Delta R.T. 0.003 min

Lab File: VN068119.D




Acq: 16 Aug 2021 16:36


Tgt Ion: 43 Resp: 7120

Ion Ratio Lower Upper

43 100

72 25.1 19.7 29.5

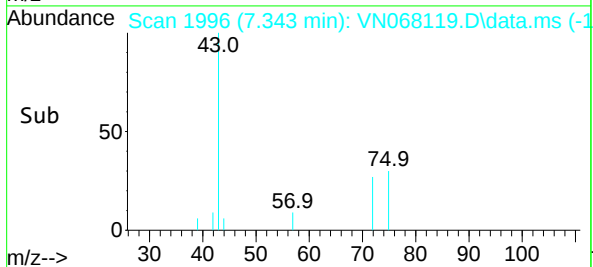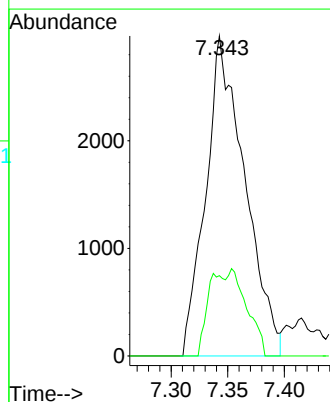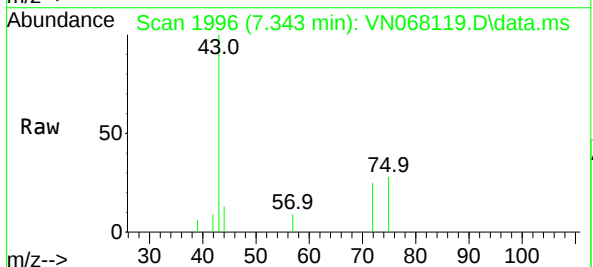



#29

Tetrahydrofuran

Concen: 0.914 ug/l

RT: 7.694 min Scan# 2127





Delta R.T. 0.005 min

Lab File: VN068119.D

Acq: 16 Aug 2021 16:36

Tgt Ion:	42	Resp:	1018
Ion	Ratio	Lower	Upper
42	100		
72	11.6	32.8	49.2#
71	29.7	31.2	46.8#

Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08



#31

Cyclohexane

Concen: 1.296 ug/l




RT: 8.088 min Scan# 2274


Delta R.T. -0.008 min

Lab File: VN068119.D

Acq: 16 Aug 2021 16:36

Tgt Ion:	56	Resp:	6283
Ion	Ratio	Lower	Upper
56	100		
69	150.9	27.3	40.9#
84	142.5	64.9	97.3#

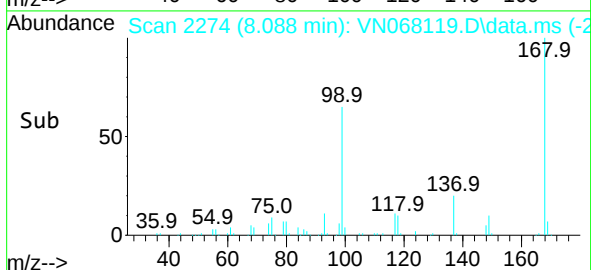







#33

1,2-Dichloroethane-d4
Concen: 60.190 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. 0.003 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08




Tgt Ion: 65 Resp: 197844
Ion Ratio Lower Upper
65 100
67 52.1 0.0 98.6




#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Tgt Ion: 114 Resp: 470530
Ion Ratio Lower Upper
114 100
63 22.1 0.0 49.0
88 15.4 0.0 36.6


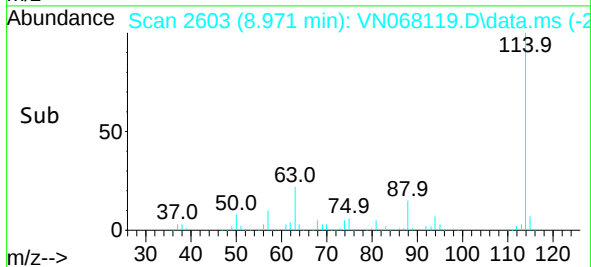

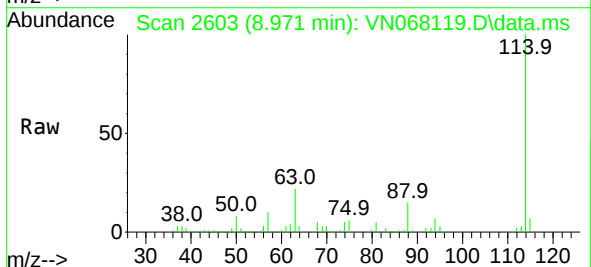




#35
Dibromofluoromethane
Concen: 53.416 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. -0.000 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08


Tgt Ion:113 Resp: 146476
Ion Ratio Lower Upper
113 100
111 103.7 83.8 125.8
192 16.1 13.4 20.0

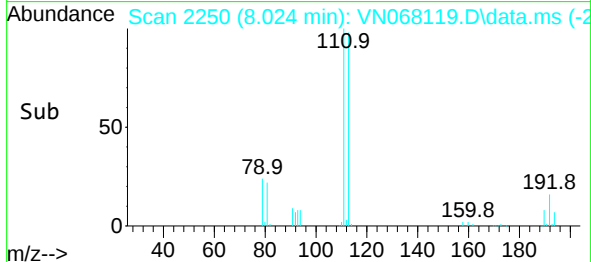

#36
1,1-Dichloropropene
Concen: 5.039 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36


Tgt Ion: 75 Resp: 21931
Ion Ratio Lower Upper
75 100
110 6.9 15.7 47.0#
77 0.0 24.6 37.0#

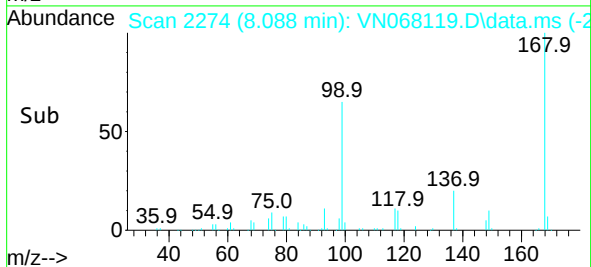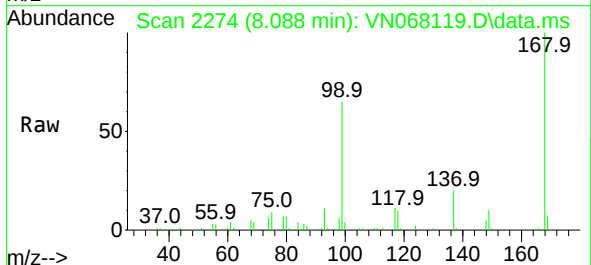






#38
Carbon Tetrachloride
Concen: 6.089 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.116 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08







Tgt Ion:117 Resp: 26063
Ion Ratio Lower Upper
117 100
119 7.6 75.4 113.2#
121 0.0 23.5 35.3#



#43
Isopropyl Acetate
Concen: 5.657 ug/l
RT: 8.563 min Scan# 2451
Delta R.T. -0.000 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Tgt Ion: 43 Resp: 38614
Ion Ratio Lower Upper
43 100
61 16.5 19.0 28.4#
87 11.9 9.5 14.3

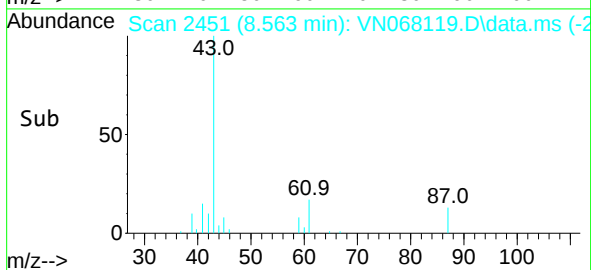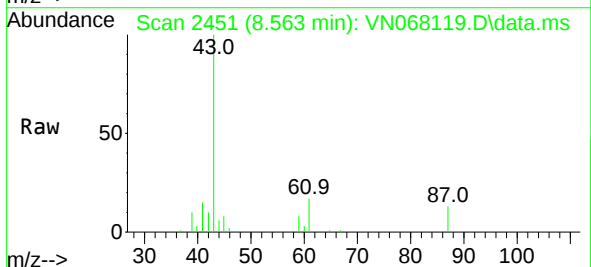







#45

1,2-Dichloropropane
Concen: 0.732 ug/l
RT: 9.628 min Scan# 2848
Delta R.T. 0.137 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08




Tgt Ion: 63 Resp: 2350
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#




#48

Methyl methacrylate
Concen: 4.469 ug/l
RT: 9.544 min Scan# 2817
Delta R.T. -0.019 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Tgt Ion: 41 Resp: 7722
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#


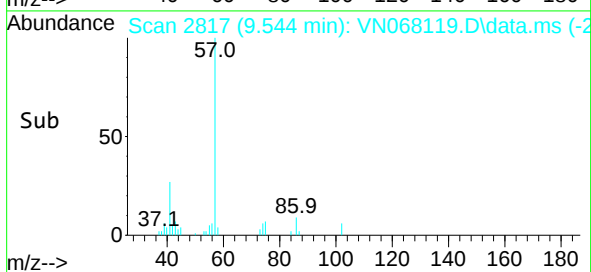






#49
1,4-Dioxane
Concen: 2.431 ug/l
RT: 9.633 min Scan# 2850
Delta R.T. 0.061 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08


Tgt Ion: 88 Resp: 132
Ion Ratio Lower Upper
88 100
43 1474887.1 28.8 43.2#
58 6950.0 60.4 90.6#

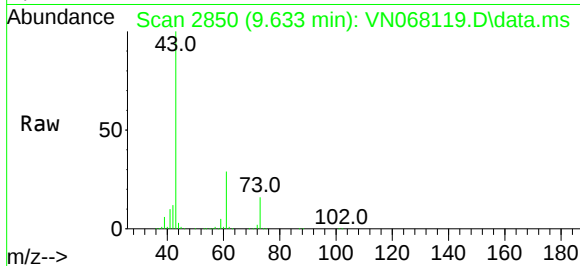

#50
Toluene-d8
Concen: 51.270 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.000 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Tgt Ion: 98 Resp: 650187
Ion Ratio Lower Upper
98 100
100 62.8 51.7 77.5


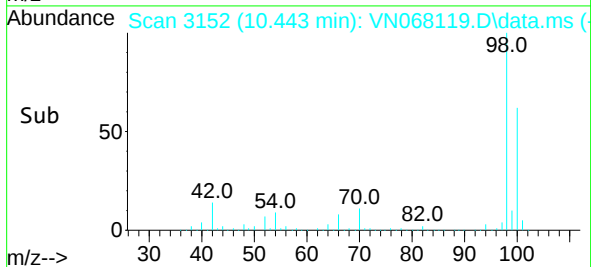

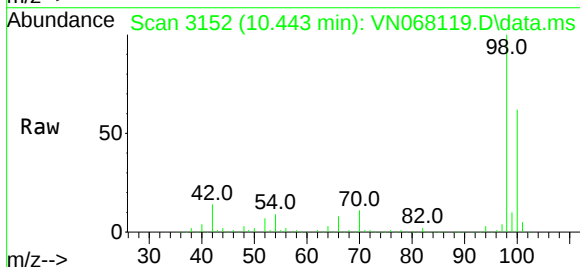




#51
4-Methyl-2-Pentanone
Concen: 14.136 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08


Tgt Ion: 43 Resp: 8220
Ion Ratio Lower Upper
43 100
58 43.9 28.6 43.0#



#53
t-1,3-Dichloropropene
Concen: 2.842 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. -0.279 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Tgt Ion: 75 Resp: 51
Ion Ratio Lower Upper
75 100
77 41.6 25.1 37.7#


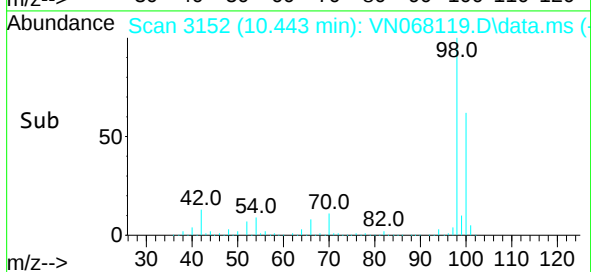






#54
cis-1,3-Dichloropropene
Concen: 11.617 ug/l
RT: 10.247 min Scan# 3079
Delta R.T. 0.056 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08


Tgt Ion: 75 Resp: 56597
Ion Ratio Lower Upper
75 100
77 0.7 24.6 37.0#
39 40.2 50.7 76.1#

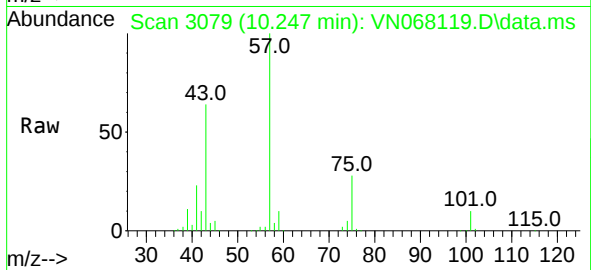

#56
Ethyl methacrylate
Concen: 3.189 ug/l
RT: 10.872 min Scan# 3312
Delta R.T. 0.107 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Tgt Ion: 69 Resp: 560
Ion Ratio Lower Upper
69 100
41 3597.5 58.6 88.0#
39 1743.9 38.3 57.5#


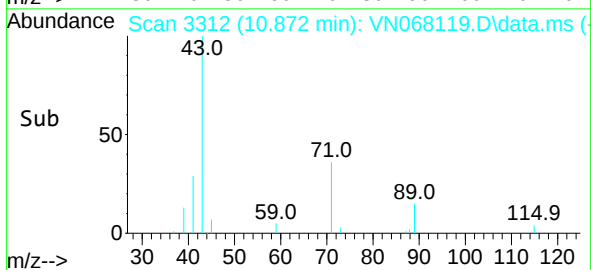

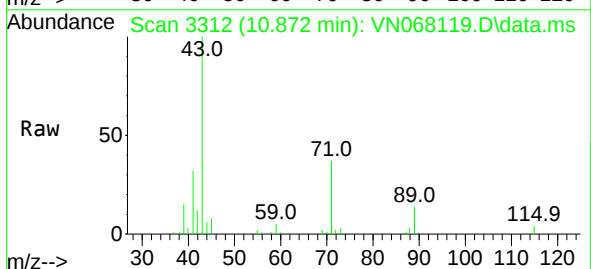




#57
1,3-Dichloropropane
Concen: 6.975 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.048 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08


Tgt Ion: 76 Resp: 36916
Ion Ratio Lower Upper
76 100
78 0.1 25.7 38.5#



#59
2-Hexanone
Concen: 160.408 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Tgt Ion: 43 Resp: 550843
Ion Ratio Lower Upper
43 100
58 17.9 24.7 74.1#









#60
Dibromochloromethane
Concen: 3.363 ug/l
RT: 11.492 min Scan# 3543
Delta R.T. 0.252 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08


Tgt Ion:129 Resp: 263
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

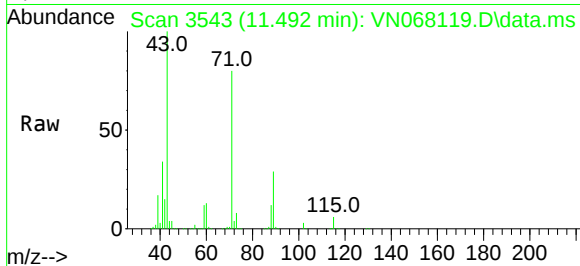

#62
4-Bromofluorobenzene
Concen: 48.782 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.001 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Tgt Ion: 95 Resp: 225347
Ion Ratio Lower Upper
95 100
174 69.0 0.0 122.0
176 66.1 0.0 117.6


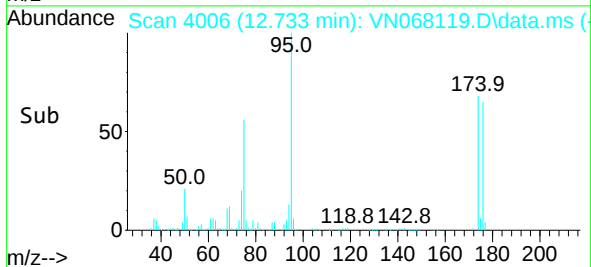

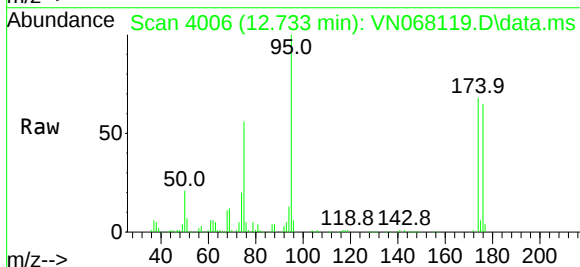




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.002 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08


Tgt Ion:117 Resp: 517500
Ion Ratio Lower Upper
117 100
82 57.2 53.1 79.7
119 31.5 25.5 38.3

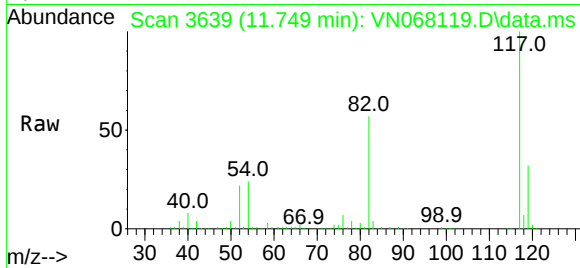

#68
m/p-Xylenes
Concen: 4.074 ug/l
RT: 11.950 min Scan# 3714
Delta R.T. -0.006 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Tgt Ion:106 Resp: 103
Ion Ratio Lower Upper
106 100
91 336.9 180.6 270.8#

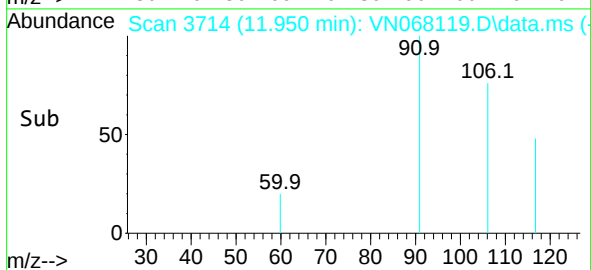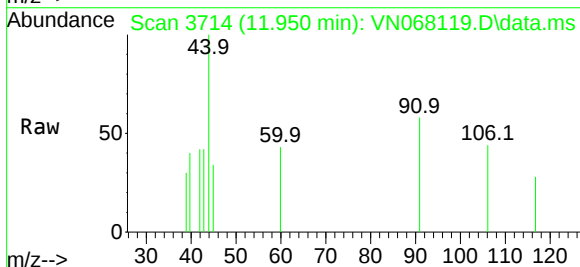

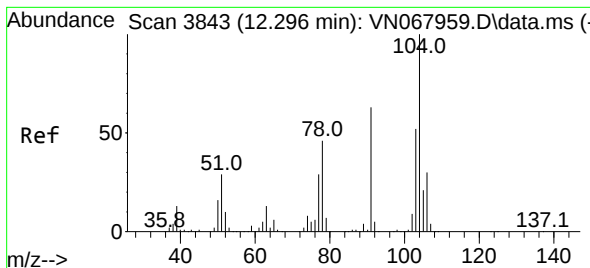

#70

Styrene

Concen: 2.645 ug/l

RT: 12.296 min Scan# 3843

Delta R.T. 0.000 min

Lab File: VN068119.D

Acq: 16 Aug 2021 16:36





Instrument :

MSVOA_N

ClientSampleId :

PB138399ZHE#08

Tgt Ion:104	Resp:	195
Ion Ratio	Lower	Upper
104	100	
78	0.0	48.2 72.2#
103	0.0	44.5 66.7#

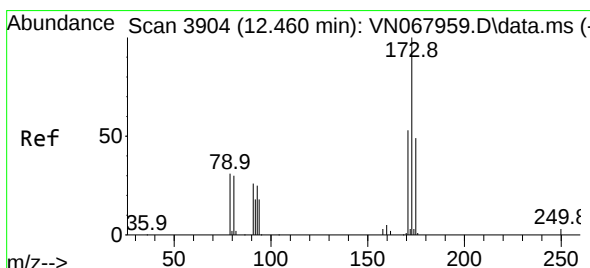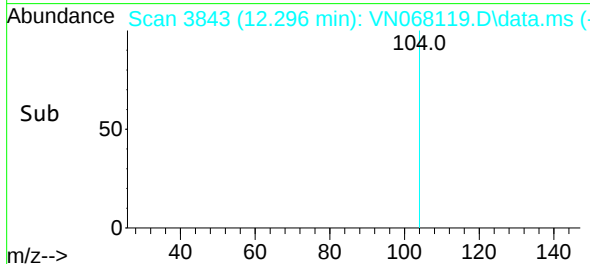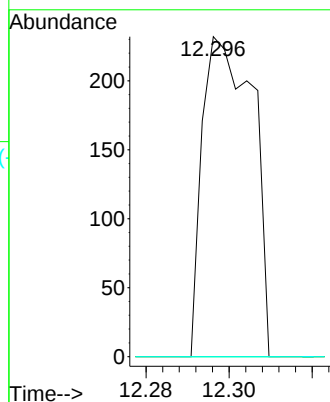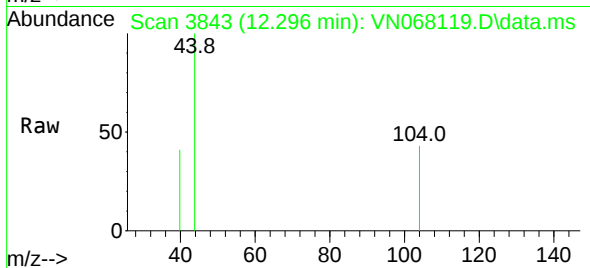

#71

Bromoform

Concen: 4.162 ug/l




RT: 12.731 min Scan# 4005


Delta R.T. 0.271 min

Lab File: VN068119.D

Acq: 16 Aug 2021 16:36

Tgt Ion:173	Resp:	473
Ion Ratio	Lower	Upper
173	100	
175	2449.5	23.9 71.8#
254	0.0	0.0 0.0


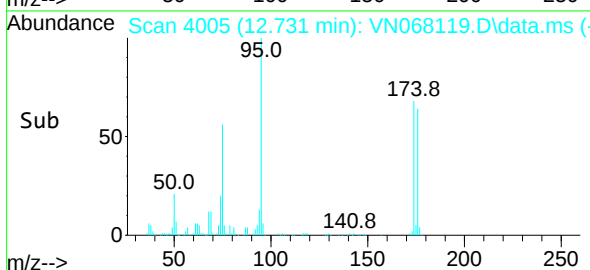
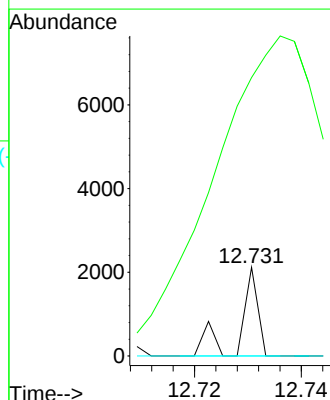
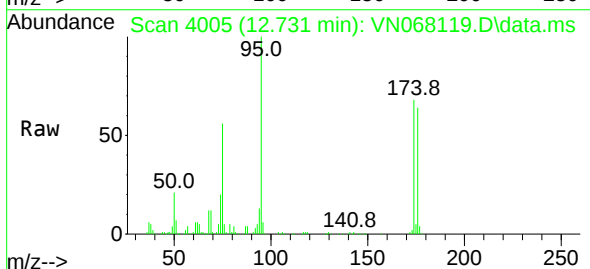


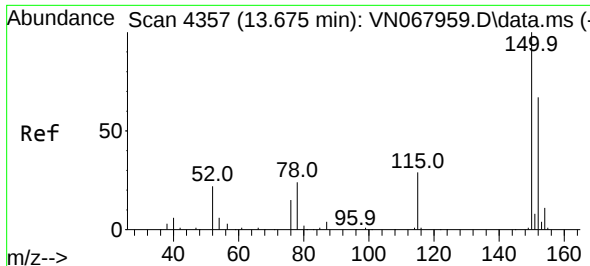

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.677 min Scan# 4358
 Delta R.T. 0.002 min
 Lab File: VN068119.D
 Acq: 16 Aug 2021 16:36




Instrument :
 MSVOA_N
 ClientSampleId :
 PB138399ZHE#08


Tgt Ion:152 Resp: 177412
 Ion Ratio Lower Upper
 152 100
 115 63.7 36.1 108.5
 150 159.7 0.0 351.8

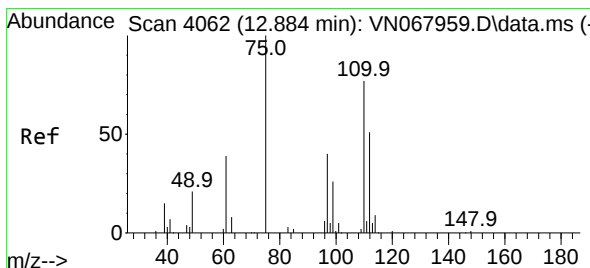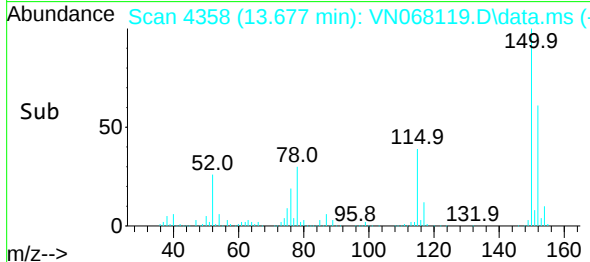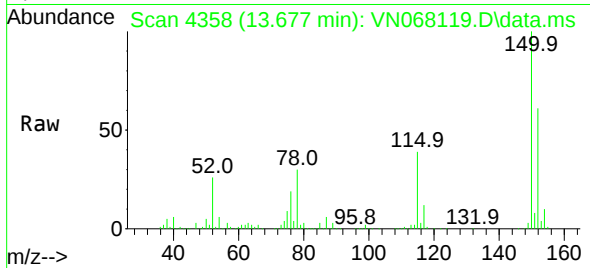

#76
 1,2,3-Trichloropropane
 Concen: 34.326 ug/l
 RT: 12.733 min Scan# 4006
 Delta R.T. -0.151 min
 Lab File: VN068119.D
 Acq: 16 Aug 2021 16:36

Tgt Ion: 75 Resp: 122303
 Ion Ratio Lower Upper
 75 100
 77 1.2 0.0 0.0#


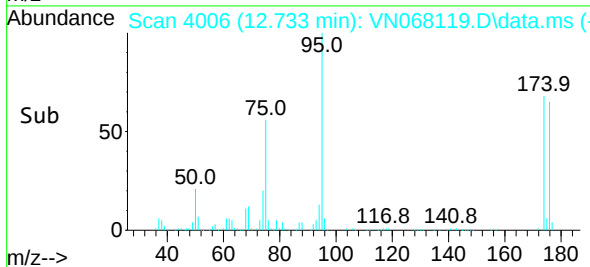

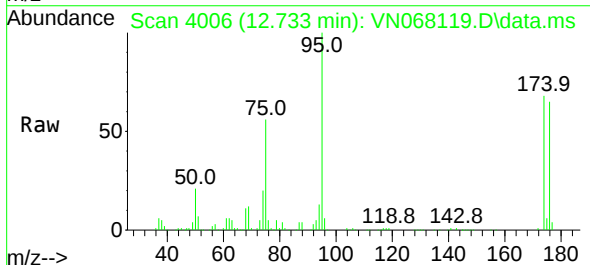




#80
1,3,5-Trimethylbenzene
Concen: 0.582 ug/l
RT: 13.063 min Scan# 4129
Delta R.T. 0.000 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08


Tgt Ion:105 Resp: 6830
Ion Ratio Lower Upper
105 100
120 47.5 22.2 66.6

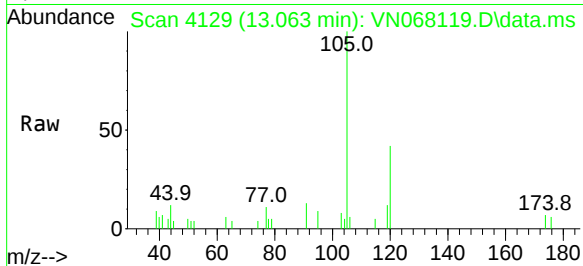

#81
trans-1,4-Dichloro-2-butene
Concen: 91.980 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36

Tgt Ion: 75 Resp: 122303
Ion Ratio Lower Upper
75 100
53 0.1 87.6 131.4#
89 0.0 37.8 56.8#


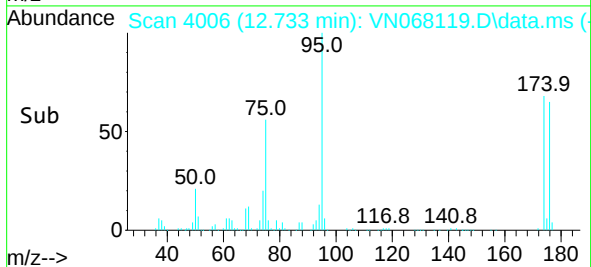

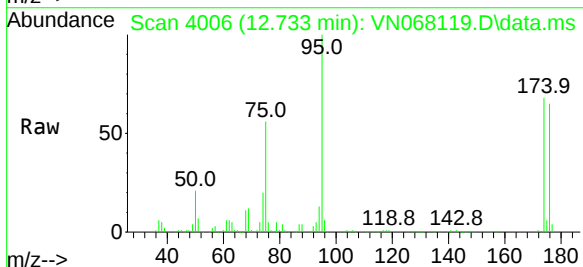




#93
1,2,4-Trichlorobenzene
Concen: 2.503 ug/l
RT: 15.262 min Scan# 4949
Delta R.T. -0.003 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#08


Tgt Ion:180 Resp: 100
Ion Ratio Lower Upper
180 100
182 0.0 47.5 142.5#
145 0.0 17.2 51.6#

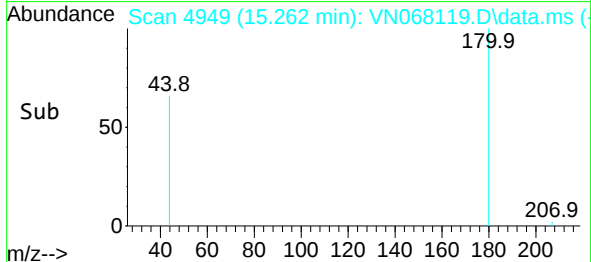

#95
Naphthalene
Concen: 3.228 ug/l
RT: 15.512 min Scan# 5042
Delta R.T. 0.003 min
Lab File: VN068119.D
Acq: 16 Aug 2021 16:36


Tgt Ion:128 Resp: 855
Ion Ratio Lower Upper
128 100
127 0.0 10.6 15.8#
129 0.0 8.6 12.8#

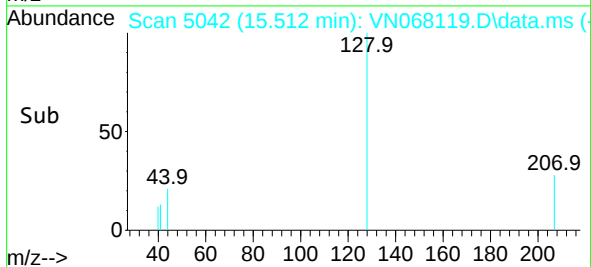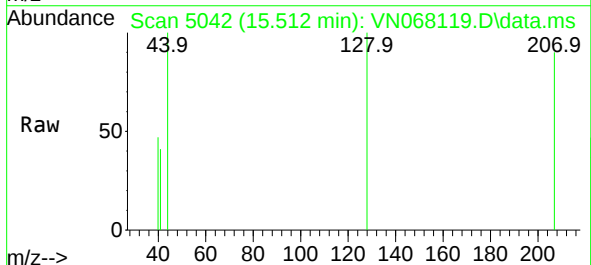



#96
 1,2,3-Trichlorobenzene
 Concen: 2.430 ug/l
 RT: 15.710 min Scan# 5116
 Delta R.T. 0.008 min
 Lab File: VN068119.D
 Acq: 16 Aug 2021 16:36

Instrument :
 MSVOA_N
 ClientSampleId :
 PB138399ZHE#08

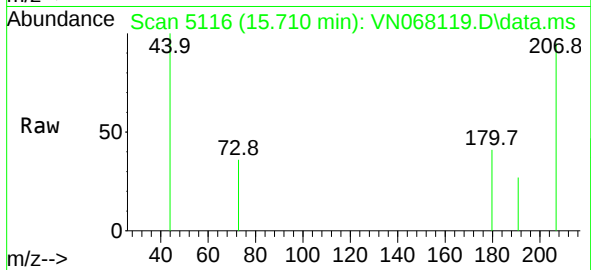

Tgt Ion	Ratio	Lower	Upper
180	100		
182	0.0	47.8	143.3#
145	0.0	18.2	54.6#

