

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081621\
 Data File : VN068128.D
 Acq On : 16 Aug 2021 20:17
 Operator : JC/MD
 Sample : PB138399ZHE#17
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB138399ZHE#17

Quant Time: Aug 17 07:17:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
 Quant Title : SW846 8260
 QLast Update : Thu Jul 29 15:02:35 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	225792	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	462781	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	491541	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	168984	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	193466	60.525	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 121.040%			
35) Dibromofluoromethane	8.024	113	142815	52.953	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 105.900%			
50) Toluene-d8	10.443	98	628232	50.436	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 100.880%			
62) 4-Bromofluorobenzene	12.734	95	215663	47.602	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 95.200%			
Target Compounds						Qvalue
11) Tert butyl alcohol	5.388	59	417	0.974	ug/l #	71
13) Acrolein	4.052	56	124	0.427	ug/l #	76
16) Acetone	4.296	43	37589	32.229	ug/l	92
18) Methyl Acetate	4.873	43	12357	4.313	ug/l #	68
20) Methylene Chloride	5.095	84	27358	9.931	ug/l	94
23) Vinyl Acetate	6.337	43	25	8.804	ug/l #	75
25) 2-Butanone	7.346	43	7700	4.551	ug/l	100
29) Tetrahydrofuran	7.691	42	876	0.808	ug/l	98
31) Cyclohexane	8.083	56	6111	1.296	ug/l #	30
36) 1,1-Dichloropropene	8.086	75	21286	4.973	ug/l #	53
37) Ethyl Acetate	7.346	43	7700	1.911	ug/l #	69
38) Carbon Tetrachloride	8.088	117	25500	6.057	ug/l #	17
41) Methacrylonitrile	7.694	41	1301	0.678	ug/l #	44
43) Isopropyl Acetate	8.568	43	35062	5.223	ug/l	94
45) 1,2-Dichloropropane	9.623	63	2336	0.740	ug/l #	44
48) Methyl methacrylate	9.545	41	9096	4.897	ug/l #	12
49) 1,4-Dioxane	9.620	88	89	1.667	ug/l #	1
51) 4-Methyl-2-Pentanone	10.336	43	8001	14.120	ug/l #	82
53) t-1,3-Dichloropropene	10.446	75	82	2.847	ug/l	99
54) cis-1,3-Dichloropropene	10.247	75	54836	11.479	ug/l #	60
56) Ethyl methacrylate	10.872	69	707	3.214	ug/l #	1
57) 1,3-Dichloropropane	11.092	76	34513	6.630	ug/l #	43
59) 2-Hexanone	11.095	43	519125	154.258	ug/l #	55
60) Dibromochloromethane	11.492	129	184	3.346	ug/l #	11
74) N-amyl acetate	12.200	43	21127	4.409	ug/l #	57
76) 1,2,3-Trichloropropane	12.736	75	117385	34.589	ug/l #	100
80) 1,3,5-Trimethylbenzene	13.061	105	6336	0.567	ug/l	92
81) trans-1,4-Dichloro-2-b...	12.736	75	117385	92.657	ug/l #	6
95) Naphthalene	15.507	128	153	3.140	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081621\
Data File : VN068128.D
Acq On : 16 Aug 2021 20:17
Operator : JC/MD
Sample : PB138399ZHE#17
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17


Quant Time: Aug 17 07:17:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N072921W.M
Quant Title : SW846 8260
QLast Update : Thu Jul 29 15:02:35 2021
Response via : Initial Calibration

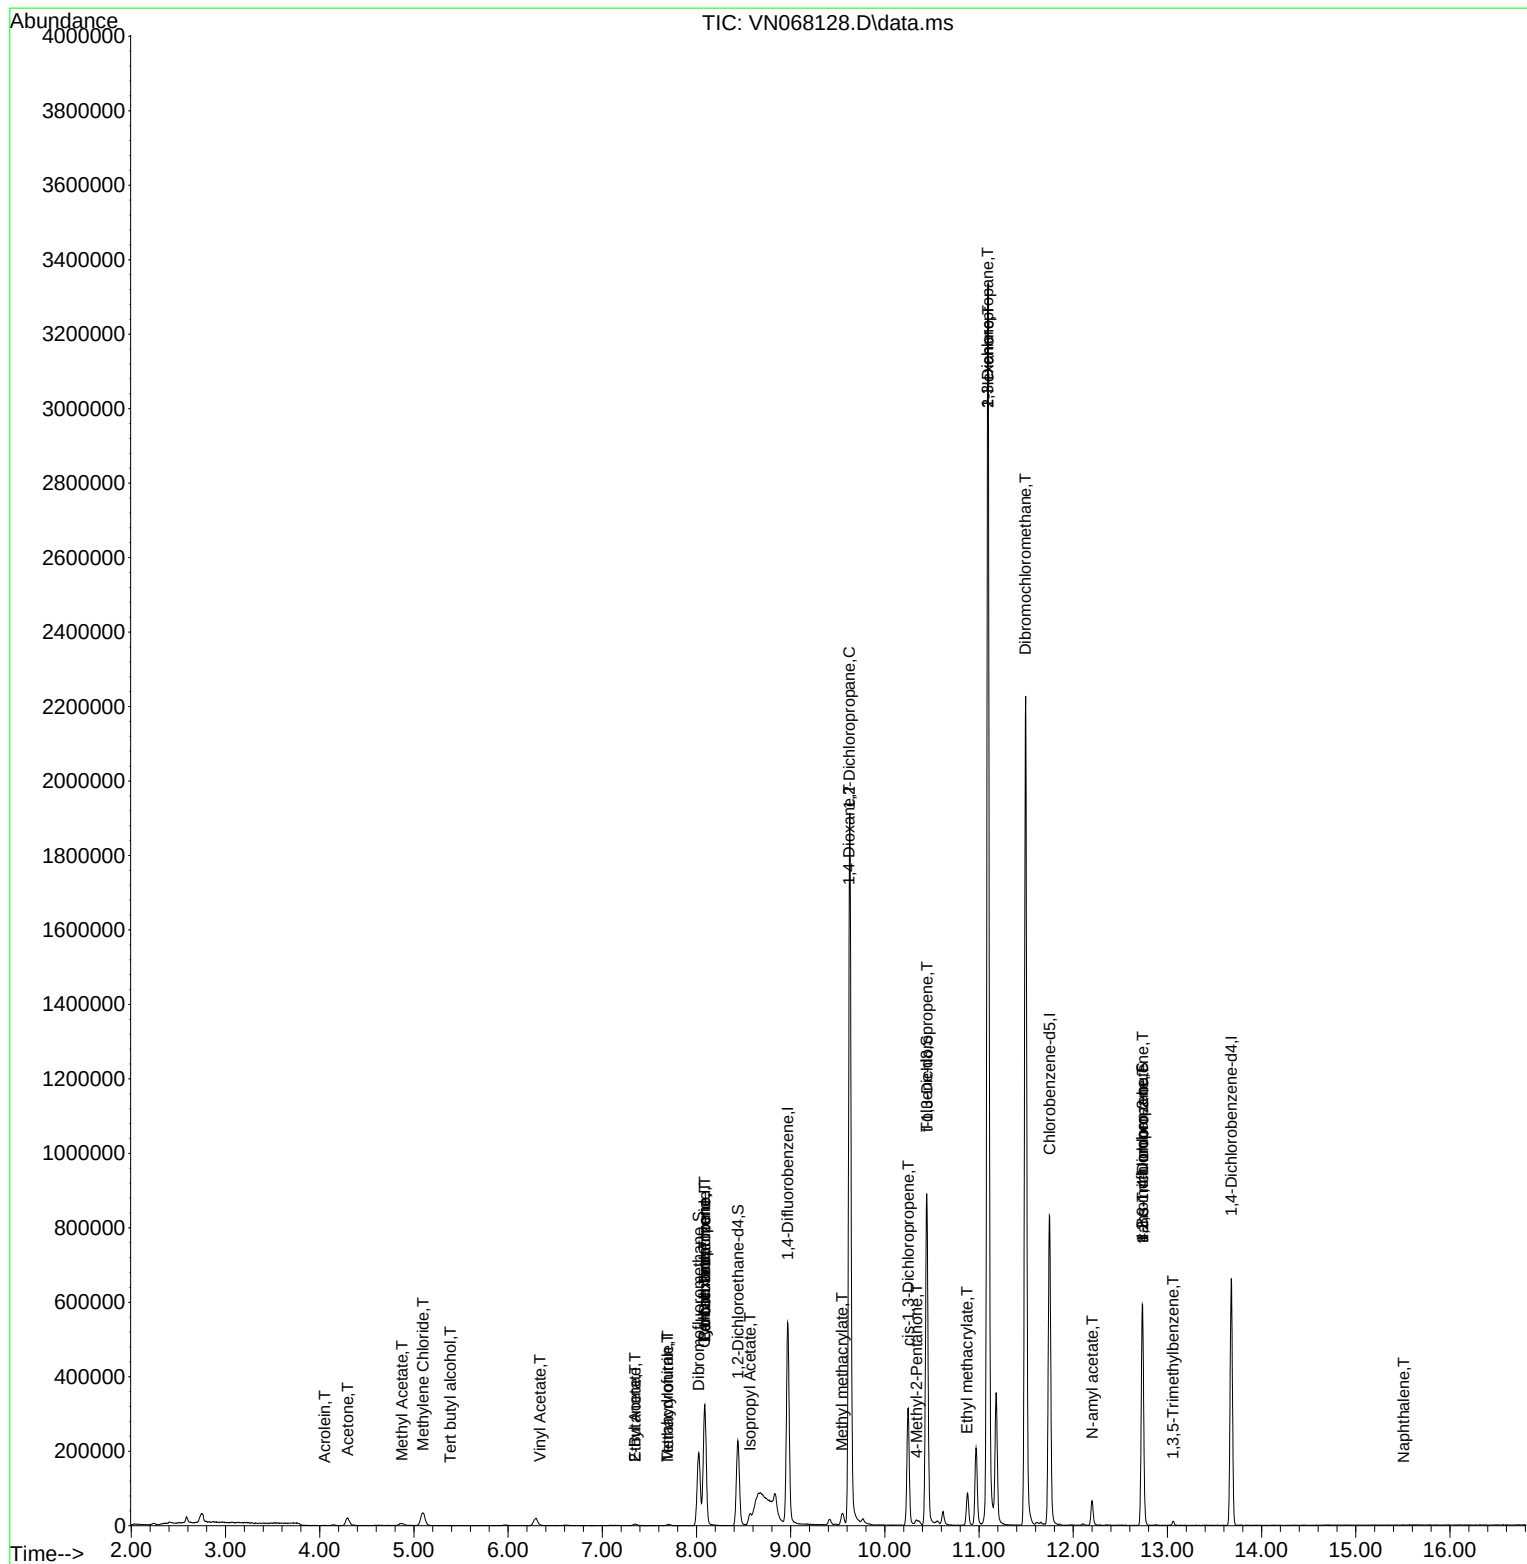






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17



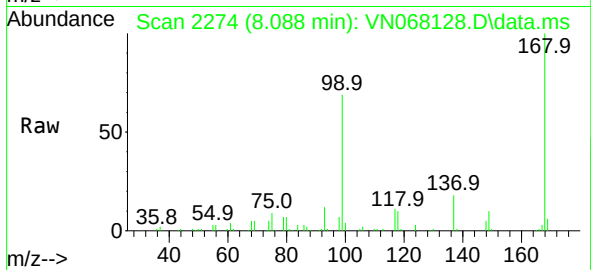



Tgt Ion:168 Resp: 225792
Ion Ratio Lower Upper
168 100
99 69.3 62.9 94.3

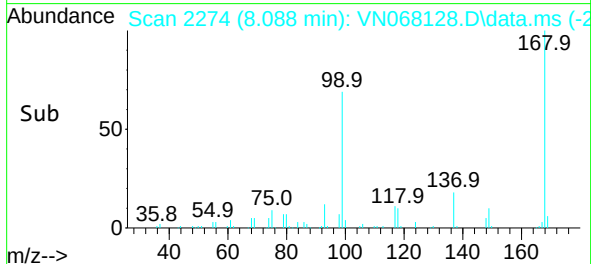

#11
Tert butyl alcohol
Concen: 0.974 ug/l
RT: 5.388 min Scan# 1267
Delta R.T. -0.002 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Tgt Ion: 59 Resp: 417
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


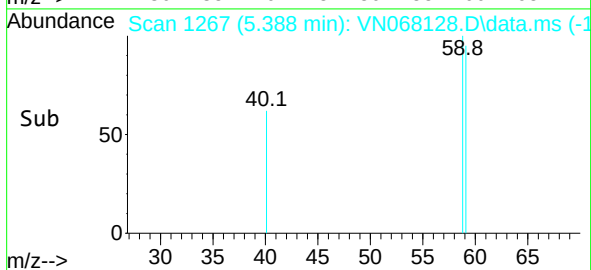

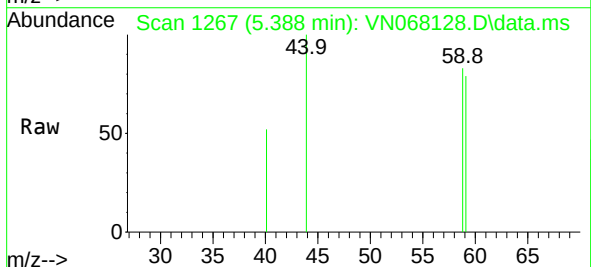


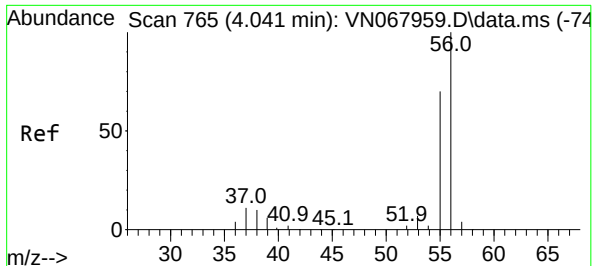

#13
Acrolein
Concen: 0.427 ug/l
RT: 4.052 min Scan# 769
Delta R.T. 0.011 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17


Tgt Ion: 56 Resp: 124
Ion Ratio Lower Upper
56 100
55 51.6 57.4 86.0#

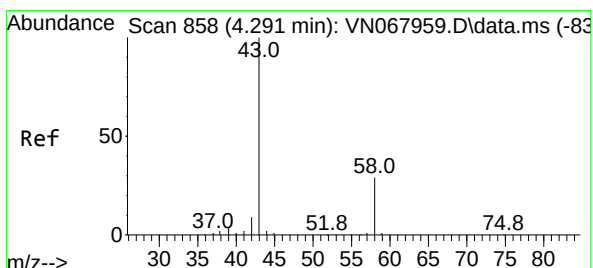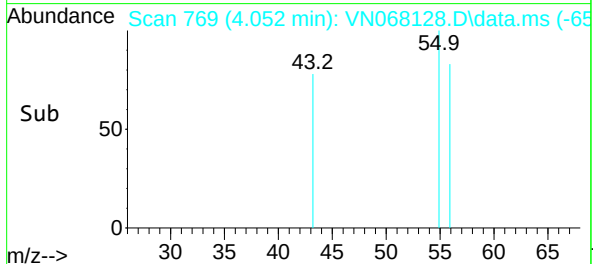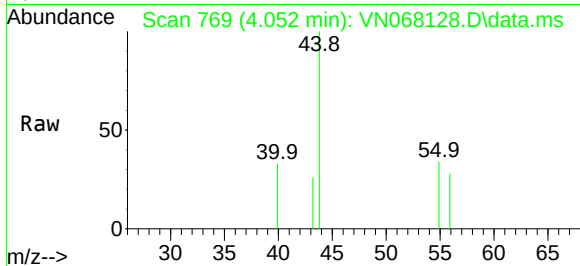

#16
Acetone
Concen: 32.229 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.005 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Tgt Ion: 43 Resp: 37589
Ion Ratio Lower Upper
43 100
58 30.5 21.2 31.8

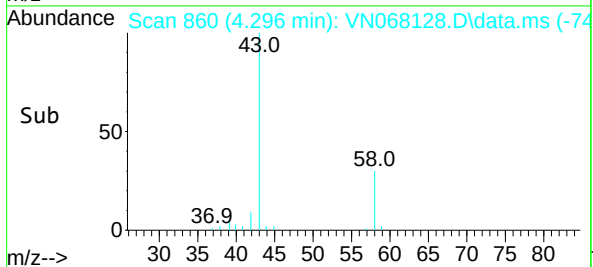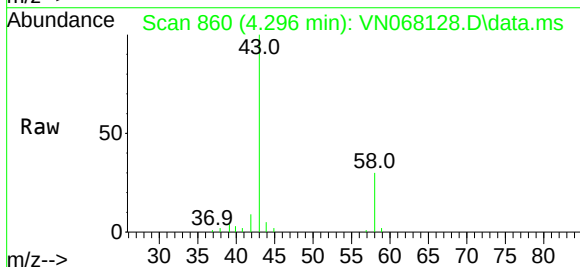

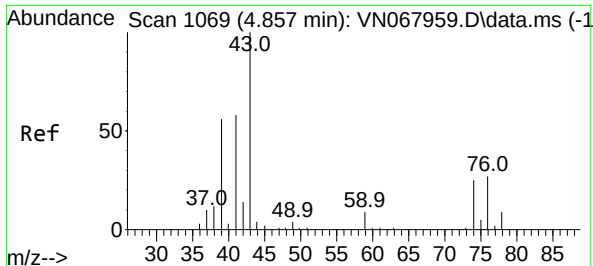

#18

Methyl Acetate

Concen: 4.313 ug/l

RT: 4.873 min Scan# 1075

Delta R.T. 0.016 min

Lab File: VN068128.D





Acq: 16 Aug 2021 20:17

Tgt Ion: 43 Resp: 12357

Ion Ratio Lower Upper

43 100

74 6.5 17.4 26.0#

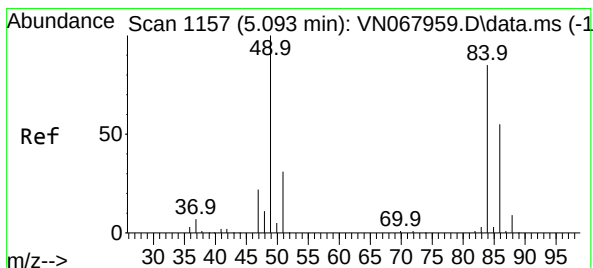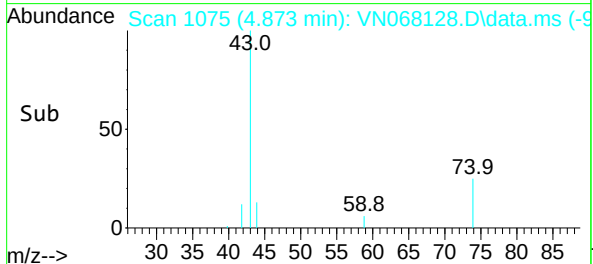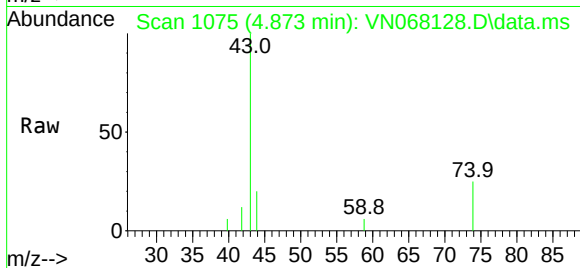

#20

Methylene Chloride

Concen: 9.931 ug/l

RT: 5.095 min Scan# 1158

Delta R.T. 0.002 min

Lab File: VN068128.D

Acq: 16 Aug 2021 20:17

Tgt Ion: 84 Resp: 27358




Ion Ratio Lower Upper


84 100

49 126.4 110.9 166.3

51 39.3 32.6 49.0

86 64.1 51.6 77.4


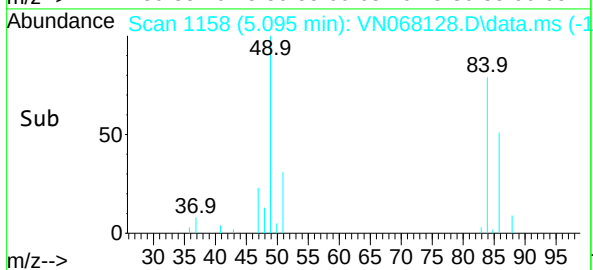

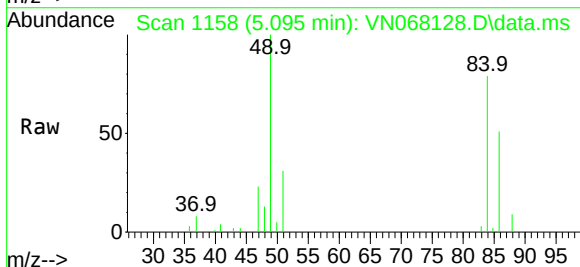


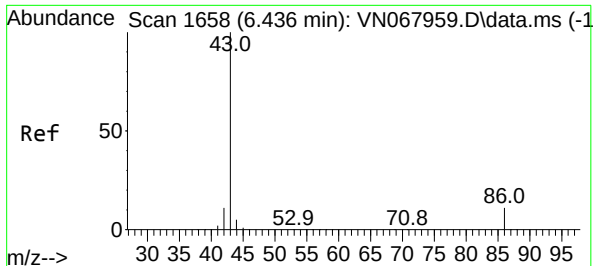

#23
 Vinyl Acetate
 Concen: 8.804 ug/l
 RT: 6.337 min Scan# 1621
 Delta R.T. -0.099 min
 Lab File: VN068128.D
 Acq: 16 Aug 2021 20:17




Instrument :
 MSVOA_N
 ClientSampleId :
 PB138399ZHE#17


Tgt Ion: 43 Resp: 25
 Ion Ratio Lower Upper
 43 100
 86 0.0 7.3 10.9#

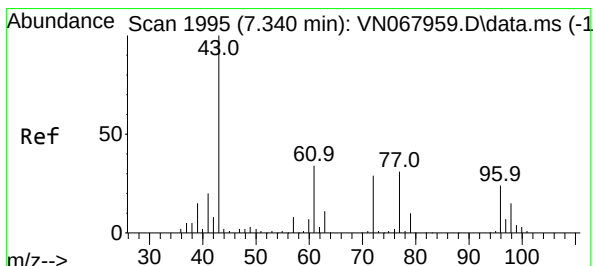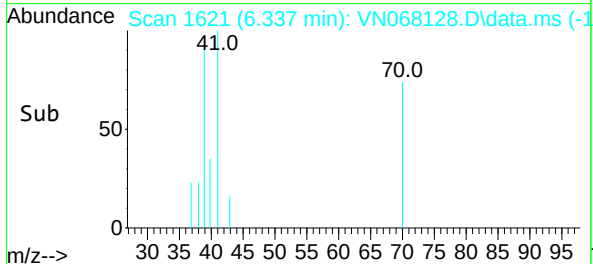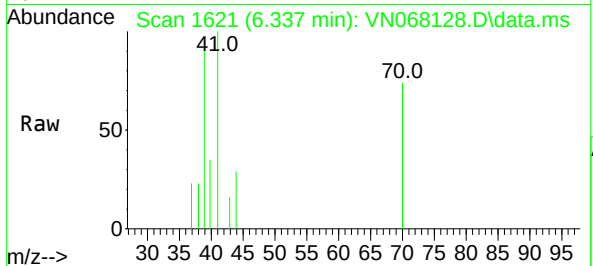

#25
 2-Butanone
 Concen: 4.551 ug/l
 RT: 7.346 min Scan# 1997
 Delta R.T. 0.006 min
 Lab File: VN068128.D
 Acq: 16 Aug 2021 20:17

Tgt Ion: 43 Resp: 7700
 Ion Ratio Lower Upper
 43 100
 72 24.7 19.7 29.5

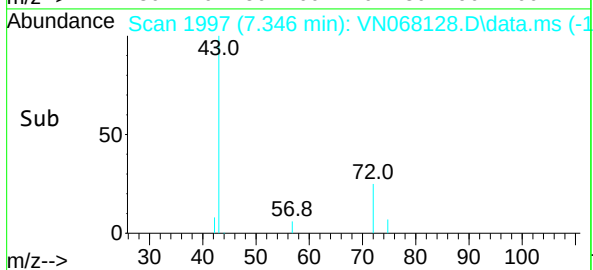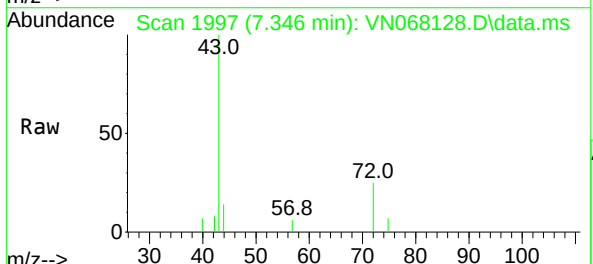



#29

Tetrahydrofuran

Concen: 0.808 ug/l

RT: 7.691 min Scan# 2126

Delta R.T. 0.002 min





Lab File: VN068128.D

Acq: 16 Aug 2021 20:17

Tgt Ion: 42 Resp: 876

Ion	Ratio	Lower	Upper
42	100		
72	41.0	32.8	49.2
71	36.2	31.2	46.8

Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17

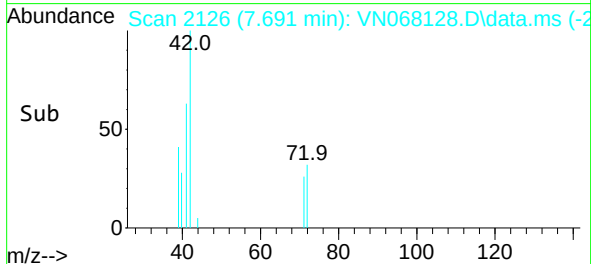

#31

Cyclohexane

Concen: 1.296 ug/l

RT: 8.083 min Scan# 2272




Delta R.T. -0.013 min


Lab File: VN068128.D

Acq: 16 Aug 2021 20:17

Tgt Ion: 56 Resp: 6111

Ion	Ratio	Lower	Upper
56	100		
69	148.0	27.3	40.9#
84	94.7	64.9	97.3









#33
 1,2-Dichloroethane-d4
 Concen: 60.525 ug/l
 RT: 8.440 min Scan# 2405
 Delta R.T. 0.003 min
 Lab File: VN068128.D
 Acq: 16 Aug 2021 20:17




Instrument :
 MSVOA_N
 ClientSampleId :
 PB138399ZHE#17


Tgt Ion: 65 Resp: 193466
 Ion Ratio Lower Upper
 65 100
 67 51.6 0.0 98.6

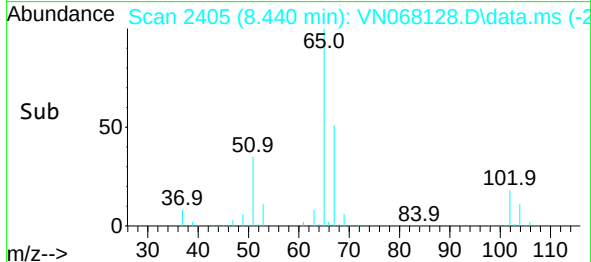

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.968 min Scan# 2602
 Delta R.T. 0.000 min
 Lab File: VN068128.D
 Acq: 16 Aug 2021 20:17

Tgt Ion: 114 Resp: 462781
 Ion Ratio Lower Upper
 114 100
 63 21.2 0.0 49.0
 88 15.0 0.0 36.6


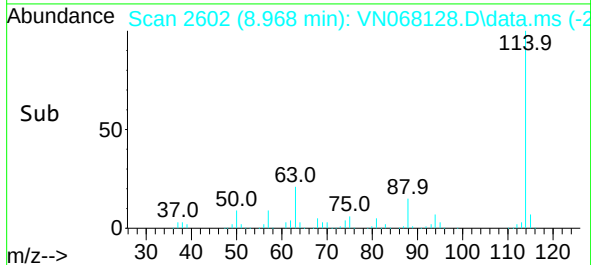

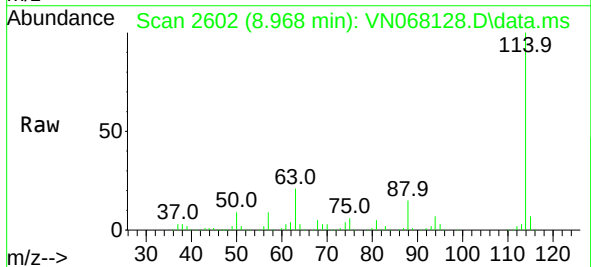




#35
Dibromofluoromethane
Concen: 52.953 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.000 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17


Tgt Ion:	113	Resp:	142815
Ion	Ratio	Lower	Upper
113	100		
111	103.2	83.8	125.8
192	15.8	13.4	20.0

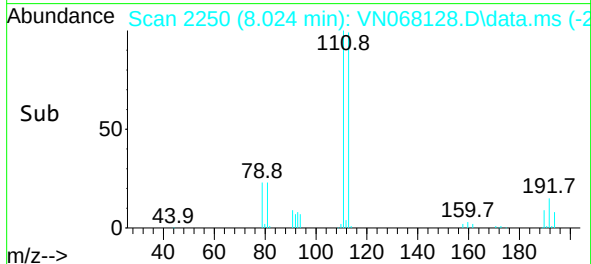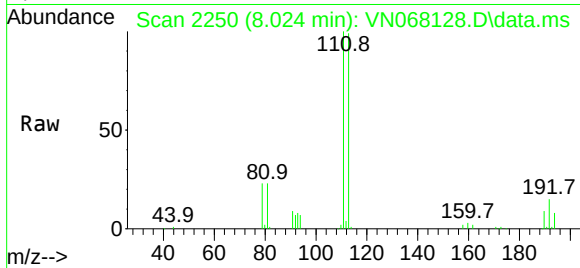

#36
1,1-Dichloropropene
Concen: 4.973 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.136 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Tgt Ion:	75	Resp:	21286
Ion	Ratio	Lower	Upper
75	100		
110	9.9	15.7	47.0#
77	0.0	24.6	37.0#

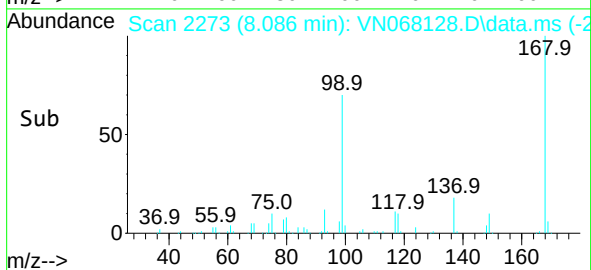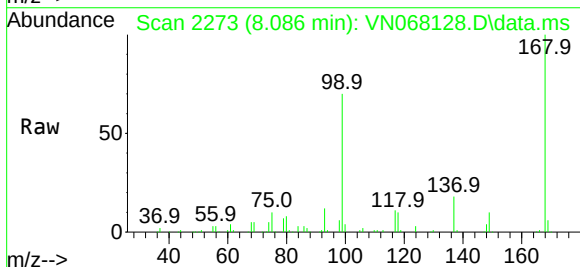



#37

Ethyl Acetate

Concen: 1.911 ug/l

RT: 7.346 min Scan# 1997

Delta R.T. -0.072 min

Lab File: VN068128.D


Acq: 16 Aug 2021 20:17

Instrument :




MSVOA_N

ClientSampleId :

PB138399ZHE#17

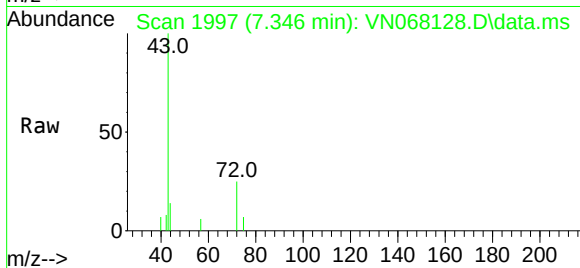

Tgt Ion:	43	Resp:	7700
Ion	Ratio	Lower	Upper
43	100		
61	0.0	10.6	16.0#
70	0.0	8.1	12.1#

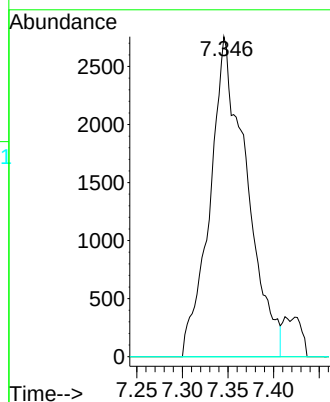

#38

Carbon Tetrachloride

Concen: 6.057 ug/l




RT: 8.088 min Scan# 2274


Delta R.T. -0.116 min

Lab File: VN068128.D

Acq: 16 Aug 2021 20:17

Tgt Ion:	117	Resp:	25500
Ion	Ratio	Lower	Upper
117	100		
119	5.0	75.4	113.2#
121	0.0	23.5	35.3#


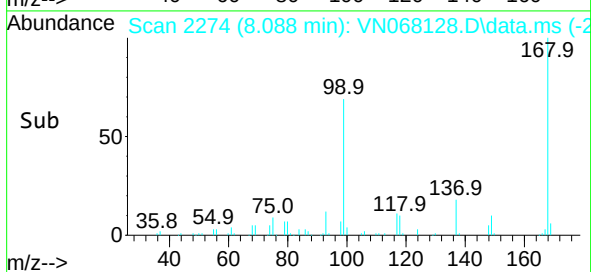
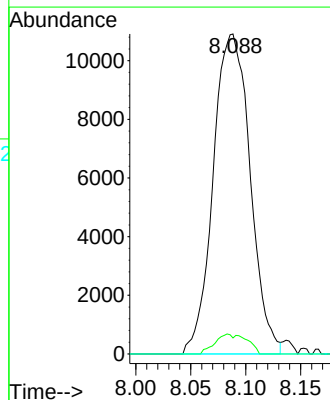
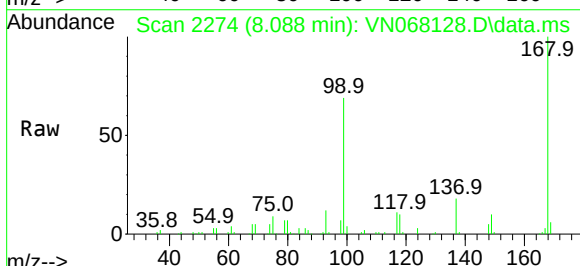


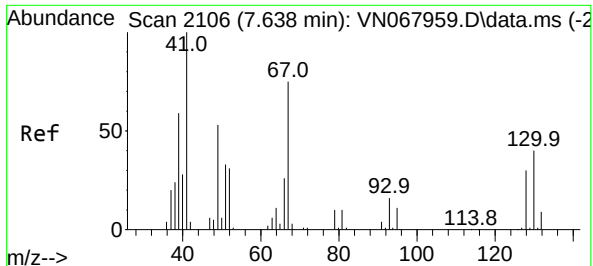

#41
Methacrylonitrile
Concen: 0.678 ug/l
RT: 7.694 min Scan# 2127
Delta R.T. 0.056 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17


Tgt Ion:	41	Resp:	1301
Ion	Ratio	Lower	Upper
41	100		
39	72.6	47.6	71.4#
67	0.0	57.7	86.5#
52	0.0	26.2	39.4#

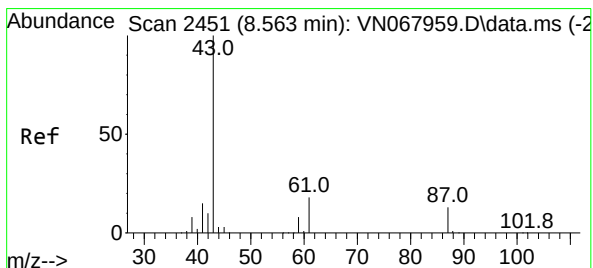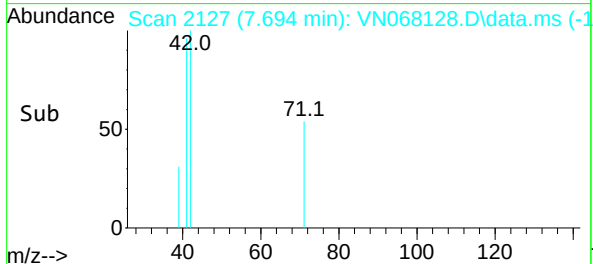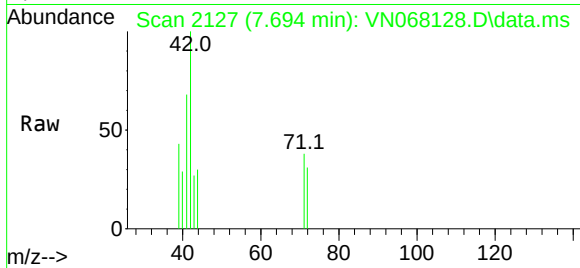

#43
Isopropyl Acetate
Concen: 5.223 ug/l
RT: 8.568 min Scan# 2453
Delta R.T. 0.005 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Tgt Ion:	43	Resp:	35062
Ion	Ratio	Lower	Upper
43	100		
61	19.4	19.0	28.4
87	11.7	9.5	14.3

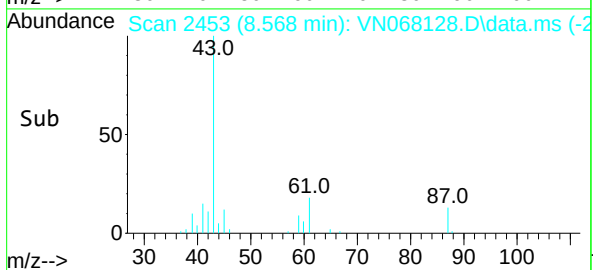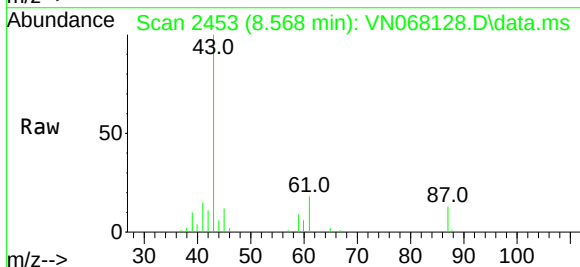







#45

1,2-Dichloropropane
Concen: 0.740 ug/l
RT: 9.623 min Scan# 2846
Delta R.T. 0.132 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17




Tgt Ion: 63 Resp: 2336
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#




#48

Methyl methacrylate
Concen: 4.897 ug/l
RT: 9.545 min Scan# 2817
Delta R.T. -0.018 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Tgt Ion: 41 Resp: 9096
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#

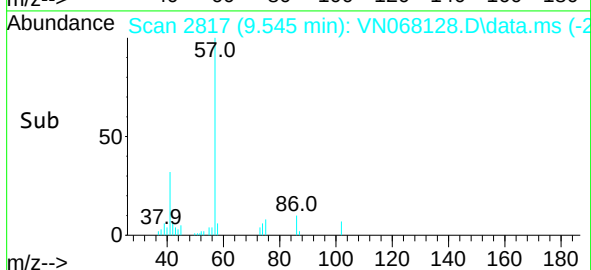



#49

1,4-Dioxane

Concen: 1.667 ug/l

RT: 9.620 min Scan# 2845

Delta R.T. 0.048 min

Lab File: VN068128.D

Acq: 16 Aug 2021 20:17





Tgt Ion: 88 Resp: 89

Ion Ratio Lower Upper

88 100

43 2137165.2 28.8 43.2#

58 10642.7 60.4 90.6#

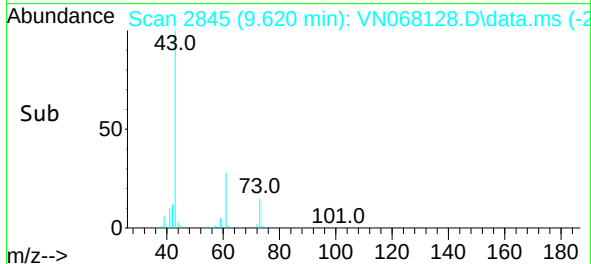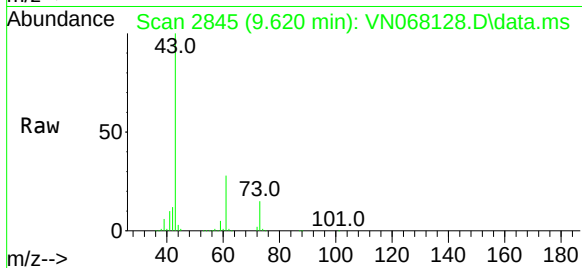

#50

Toluene-d8

Concen: 50.436 ug/l

RT: 10.443 min Scan# 3152

Delta R.T. 0.000 min

Lab File: VN068128.D




Acq: 16 Aug 2021 20:17


Tgt Ion: 98 Resp: 628232

Ion Ratio Lower Upper

98 100

100 63.1 51.7 77.5


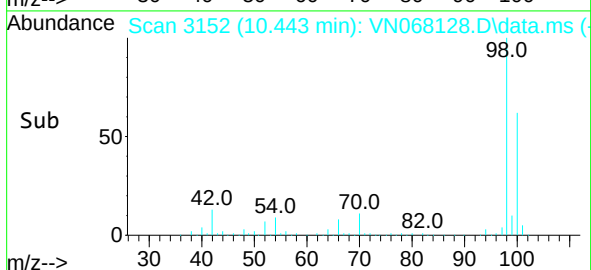

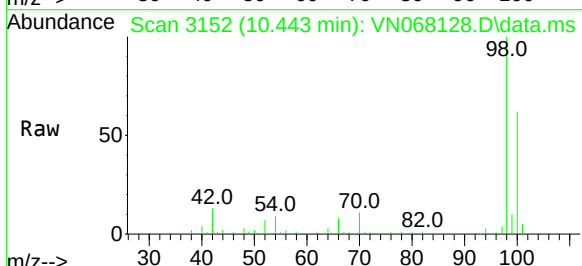




#51
4-Methyl-2-Pentanone
Concen: 14.120 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17


Tgt Ion: 43 Resp: 8001
Ion Ratio Lower Upper
43 100
58 46.2 28.6 43.0#

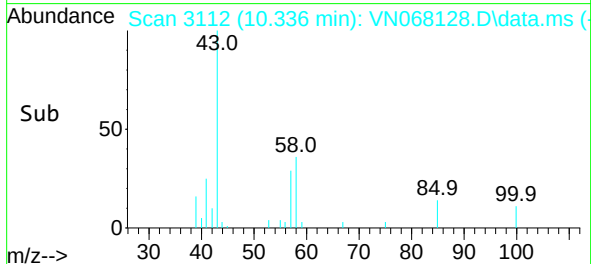

#53
t-1,3-Dichloropropene
Concen: 2.847 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. -0.276 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Tgt Ion: 75 Resp: 82
Ion Ratio Lower Upper
75 100
77 31.8 25.1 37.7


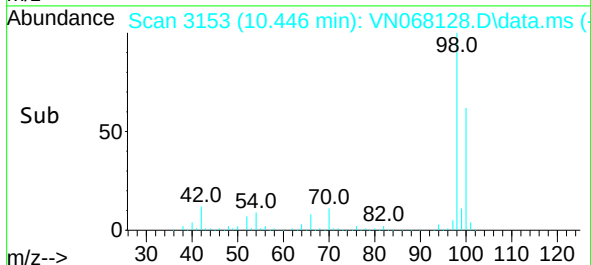

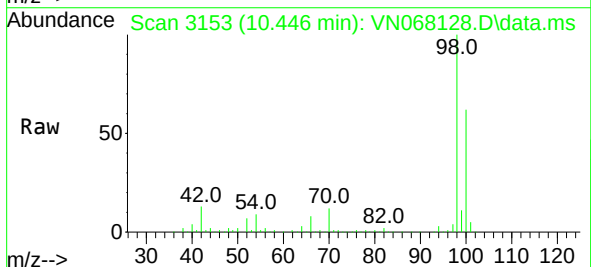




#54
 cis-1,3-Dichloropropene
 Concen: 11.479 ug/l
 RT: 10.247 min Scan# 3079
 Delta R.T. 0.056 min
 Lab File: VN068128.D
 Acq: 16 Aug 2021 20:17




Instrument :
 MSVOA_N
 ClientSampleId :
 PB138399ZHE#17


Tgt Ion: 75 Resp: 54836
 Ion Ratio Lower Upper
 75 100
 77 0.8 24.6 37.0#
 39 37.4 50.7 76.1#

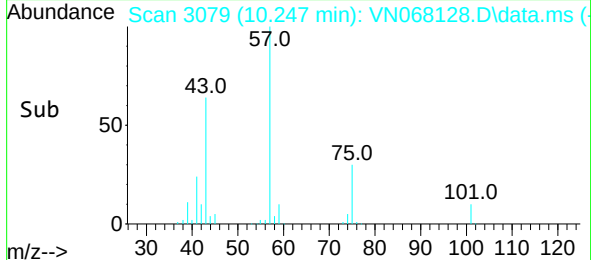

#56
 Ethyl methacrylate
 Concen: 3.214 ug/l
 RT: 10.872 min Scan# 3312
 Delta R.T. 0.107 min
 Lab File: VN068128.D
 Acq: 16 Aug 2021 20:17

Tgt Ion: 69 Resp: 707
 Ion Ratio Lower Upper
 69 100
 41 2708.2 58.6 88.0#
 39 1397.6 38.3 57.5#


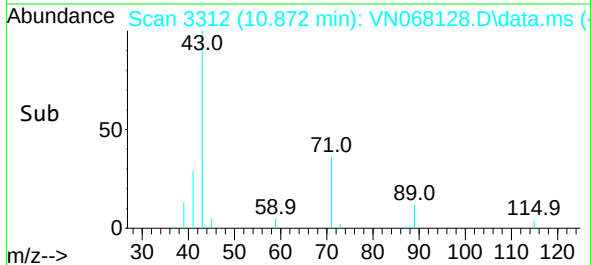

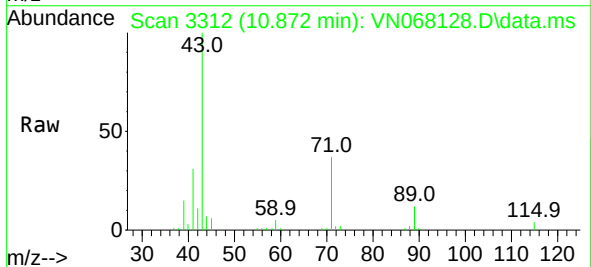




#57
1,3-Dichloropropane
Concen: 6.630 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.045 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17


Tgt Ion: 76 Resp: 34513
Ion Ratio Lower Upper
76 100
78 0.0 25.7 38.5#

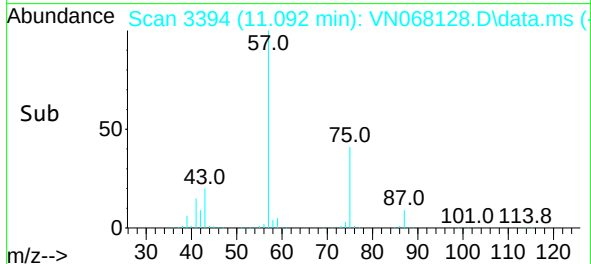

#59
2-Hexanone
Concen: 154.258 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Tgt Ion: 43 Resp: 519125
Ion Ratio Lower Upper
43 100
58 18.6 24.7 74.1#


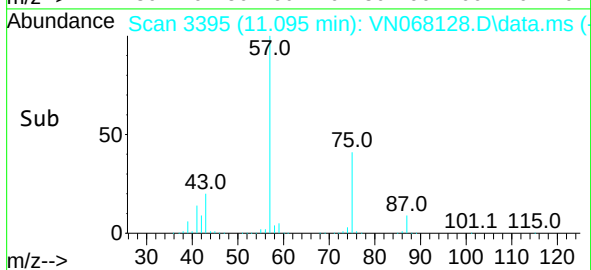

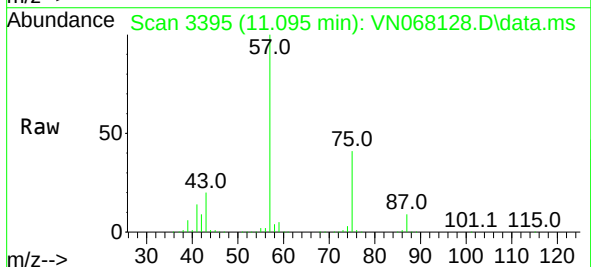




#60
Dibromochloromethane
Concen: 3.346 ug/l
RT: 11.492 min Scan# 3543
Delta R.T. 0.252 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17


Tgt Ion:129 Resp: 184
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

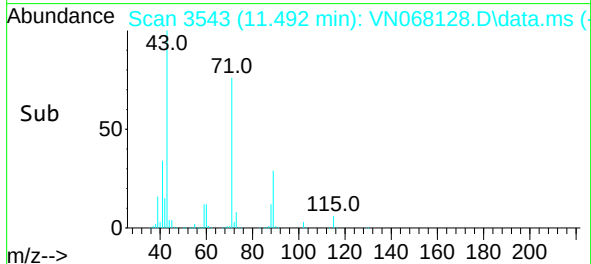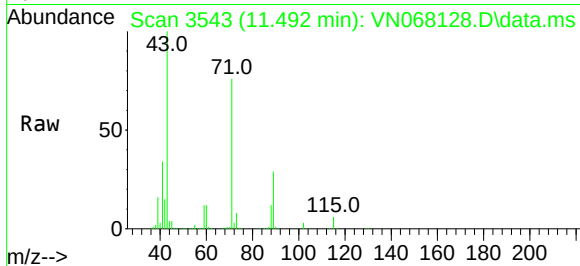

#62
4-Bromofluorobenzene
Concen: 47.602 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.000 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Tgt Ion: 95 Resp: 215663
Ion Ratio Lower Upper
95 100
174 68.8 0.0 122.0
176 65.1 0.0 117.6


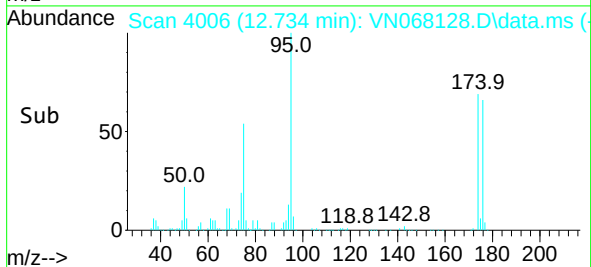

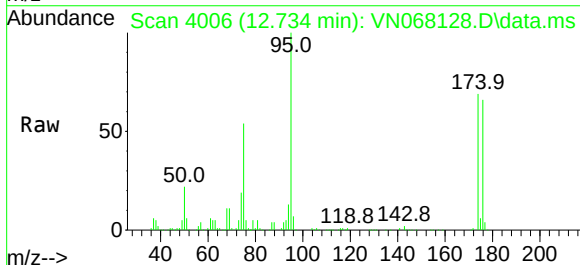


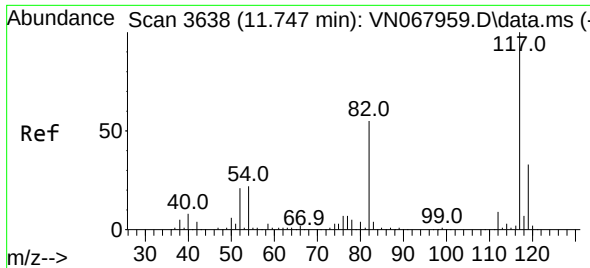

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.002 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17


Tgt Ion:117 Resp: 491541
Ion Ratio Lower Upper
117 100
82 57.7 53.1 79.7
119 32.9 25.5 38.3

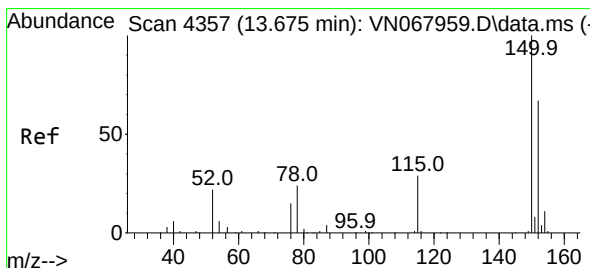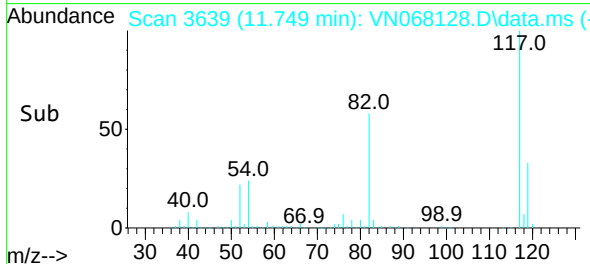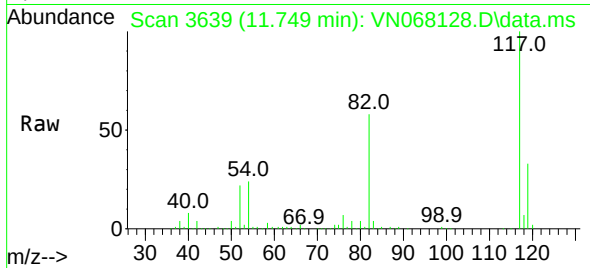

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.003 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Tgt Ion:152 Resp: 168984
Ion Ratio Lower Upper
152 100
115 63.2 36.1 108.5
150 158.5 0.0 351.8


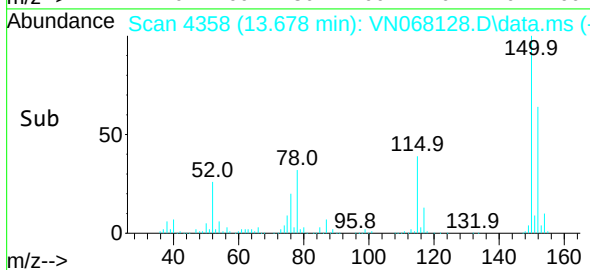

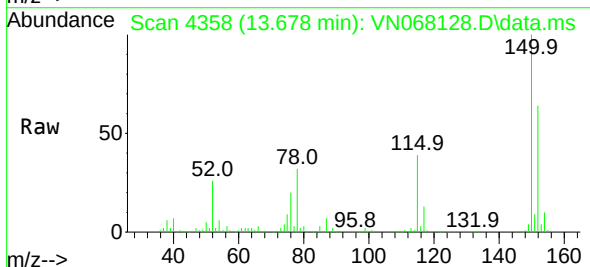


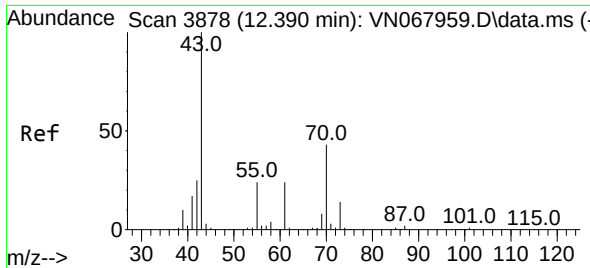

#74
N-amy1 acetate
Concen: 4.409 ug/l
RT: 12.200 min Scan# 3807
Delta R.T. -0.190 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17


Tgt Ion	Ratio	Lower	Upper
43	100		
70	2.6	29.4	44.2#
55	6.1	17.0	25.4#
61	8.7	17.6	26.4#

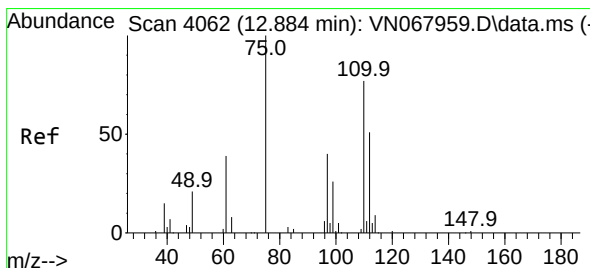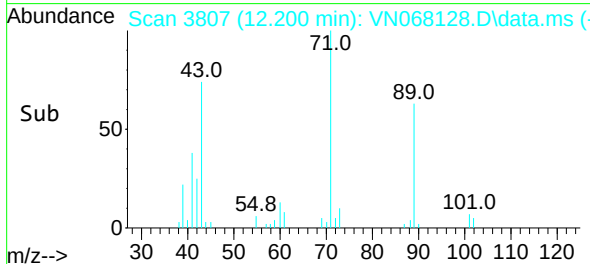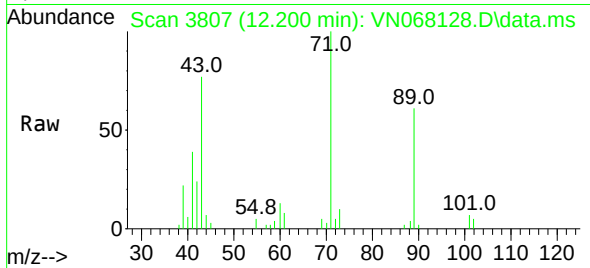

#76
1,2,3-Trichloropropane
Concen: 34.589 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. -0.148 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Tgt Ion	Ratio	Lower	Upper
75	100		
77	1.1	0.0	0.0#


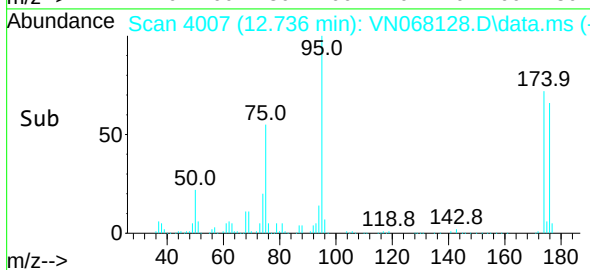

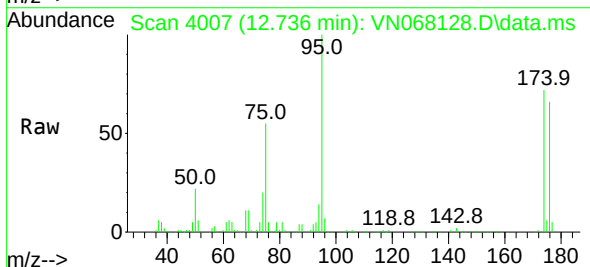


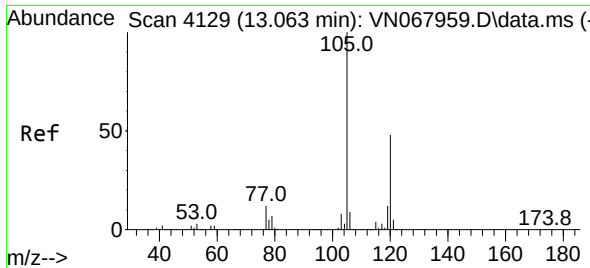

#80
1,3,5-Trimethylbenzene
Concen: 0.567 ug/l
RT: 13.061 min Scan# 4128
Delta R.T. -0.002 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17




Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17


Tgt Ion:105 Resp: 6336
Ion Ratio Lower Upper
105 100
120 39.3 22.2 66.6

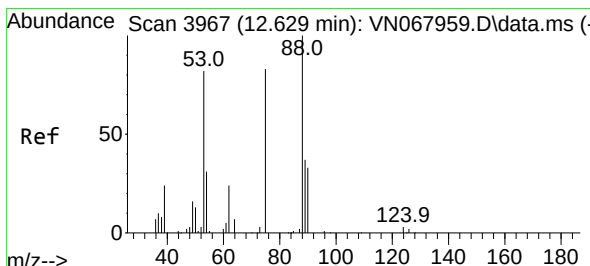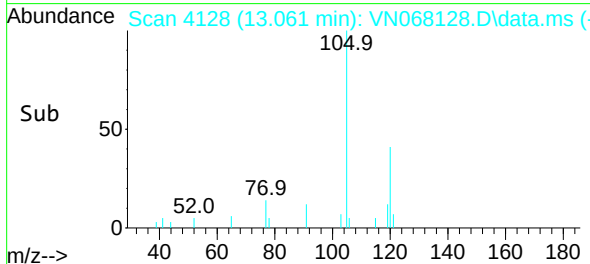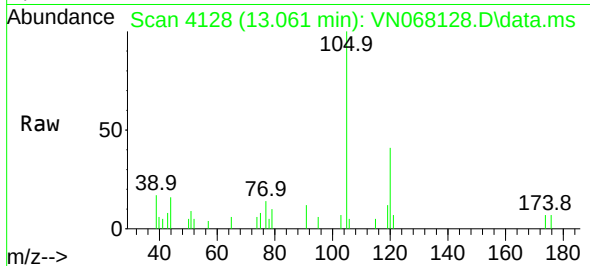

#81
trans-1,4-Dichloro-2-butene
Concen: 92.657 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.107 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17


Tgt Ion: 75 Resp: 117385
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

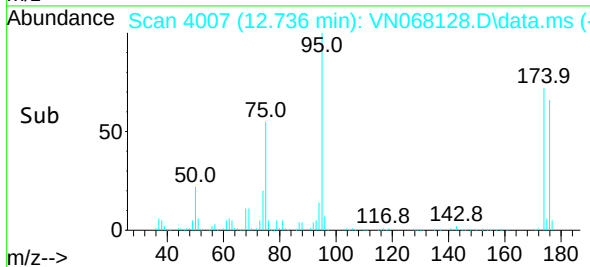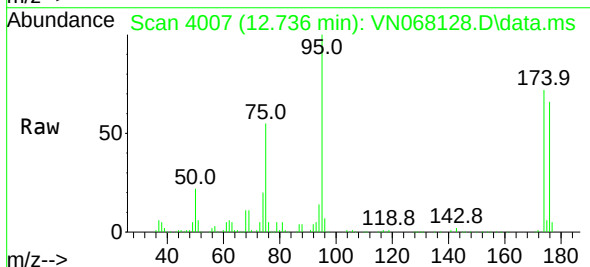

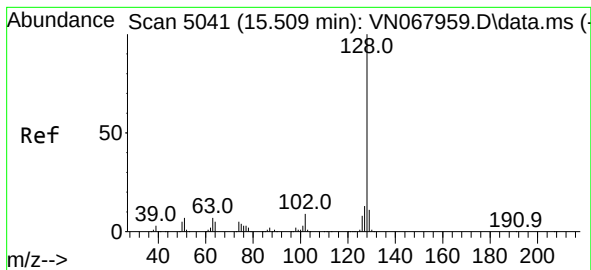

#95
Naphthalene
Concen: 3.140 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.002 min
Lab File: VN068128.D
Acq: 16 Aug 2021 20:17

Instrument :
MSVOA_N
ClientSampleId :
PB138399ZHE#17

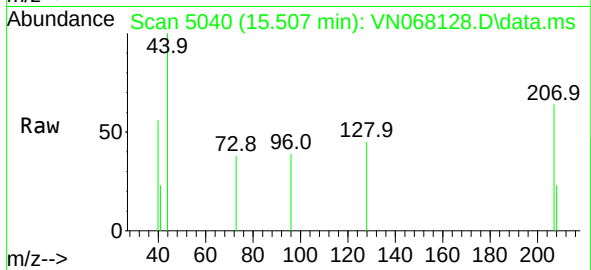

Tgt Ion:	128	Resp:	153
Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.6	15.8#
129	0.0	8.6	12.8#

