

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN081623\  
 Data File : VN078902.D  
 Acq On : 16 Aug 2023 14:52  
 Operator : JC\MD  
 Sample : PB154855ZHE#05  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 PB154855ZHE#05

Quant Time: Aug 17 01:16:57 2023  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N081523W.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Aug 16 02:42:02 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc      | Units      | Dev(Min) |
|-------------------------------|--------|-------|----------|-----------|------------|----------|
| -----                         |        |       |          |           |            |          |
| Internal Standards            |        |       |          |           |            |          |
| 1) Pentafluorobenzene         | 8.230  | 168   | 149112   | 50.000    | ug/l       | 0.00     |
| 34) 1,4-Difluorobenzene       | 9.112  | 114   | 298798   | 50.000    | ug/l       | 0.00     |
| 63) Chlorobenzene-d5          | 11.870 | 117   | 291987   | 50.000    | ug/l       | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.800 | 152   | 94343    | 50.000    | ug/l       | 0.00     |
| System Monitoring Compounds   |        |       |          |           |            |          |
| 33) 1,2-Dichloroethane-d4     | 8.588  | 65    | 125320   | 54.010    | ug/l       | 0.00     |
| Spiked Amount                 | 50.000 | Range | 74 - 125 | Recovery  | = 108.020% |          |
| 35) Dibromofluoromethane      | 8.171  | 113   | 102241   | 50.832    | ug/l       | 0.00     |
| Spiked Amount                 | 50.000 | Range | 75 - 124 | Recovery  | = 101.660% |          |
| 50) Toluene-d8                | 10.571 | 98    | 386795   | 51.791    | ug/l       | 0.00     |
| Spiked Amount                 | 50.000 | Range | 86 - 113 | Recovery  | = 103.580% |          |
| 62) 4-Bromofluorobenzene      | 12.853 | 95    | 116888   | 47.883    | ug/l       | 0.00     |
| Spiked Amount                 | 50.000 | Range | 83 - 123 | Recovery  | = 95.760%  |          |
| Target Compounds              |        |       |          |           |            |          |
|                               |        |       |          |           | Qvalue     |          |
| 3) Chloromethane              | 2.365  | 50    | 1367     | 0.473     | ug/l       | 96       |
| 5) Bromomethane               | 2.959  | 94    | 384      | 0.264     | ug/l #     | 55       |
| 6) Chloroethane               | 3.118  | 64    | 514      | 0.290     | ug/l #     | 43       |
| 11) Tert butyl alcohol        | 5.541  | 59    | 163      | 0.419     | ug/l #     | 72       |
| 16) Acetone                   | 4.442  | 43    | 27732    | 28.966    | ug/l       | 89       |
| 18) Methyl Acetate            | 5.042  | 43    | 4830     | 1.194     | ug/l #     | 74       |
| 20) Methylene Chloride        | 5.283  | 84    | 14530    | 7.122     | ug/l #     | 67       |
| 25) 2-Butanone                | 7.494  | 43    | 9119     | 5.941     | ug/l #     | 69       |
| 31) Cyclohexane               | 8.224  | 56    | 4310     | Below Cal | #          | 53       |
| 36) 1,1-Dichloropropene       | 8.230  | 75    | 13339    | 4.409     | ug/l #     | 42       |
| 37) Ethyl Acetate             | 7.582  | 43    | 4267     | 1.260     | ug/l #     | 79       |
| 38) Carbon Tetrachloride      | 8.230  | 117   | 17052    | 5.625     | ug/l #     | 16       |
| 42) 1,2-Dichloroethane        | 8.694  | 62    | 1093     | 0.327     | ug/l #     | 73       |
| 43) Isopropyl Acetate         | 8.694  | 43    | 236815   | 39.579    | ug/l #     | 70       |
| 48) Methyl methacrylate       | 9.676  | 41    | 5067     | 1.869     | ug/l #     | 29       |
| 49) 1,4-Dioxane               | 9.747  | 88    | 175      | 3.789     | ug/l #     | 1        |
| 51) 4-Methyl-2-Pentanone      | 10.453 | 43    | 39443    | 11.115    | ug/l #     | 78       |
| 54) cis-1,3-Dichloropropene   | 10.365 | 75    | 50367    | 13.372    | ug/l #     | 71       |
| 57) 1,3-Dichloropropane       | 11.206 | 76    | 6757     | 1.716     | ug/l #     | 42       |
| 59) 2-Hexanone                | 11.176 | 43    | 143660   | 55.892    | ug/l #     | 19       |
| 71) Bromoform                 | 12.847 | 173   | 720      | 0.422     | ug/l #     | 28       |
| 74) N-amyl acetate            | 12.494 | 43    | 2138     | 0.538     | ug/l #     | 36       |
| 76) 1,2,3-Trichloropropane    | 12.853 | 75    | 67397    | 29.648    | ug/l #     | 1        |
| 81) trans-1,4-Dichloro-2-b... | 12.853 | 75    | 67397    | 75.739    | ug/l #     | 15       |
| 92) 1,2-Dibromo-3-Chloropr... | 14.694 | 75    | 54       | Below Cal | #          | 4        |
| 95) Naphthalene               | 15.641 | 128   | 64       | 2.589     | ug/l #     | 70       |
| -----                         |        |       |          |           |            |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN081623\  
Data File : VN078902.D  
Acq On : 16 Aug 2023 14:52  
Operator : JC\MD  
Sample : PB154855ZHE#05  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
PB154855ZHE#05

Quant Time: Aug 17 01:16:57 2023  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N081523W.M  
Quant Title : SW846 8260  
QLast Update : Wed Aug 16 02:42:02 2023  
Response via : Initial Calibration

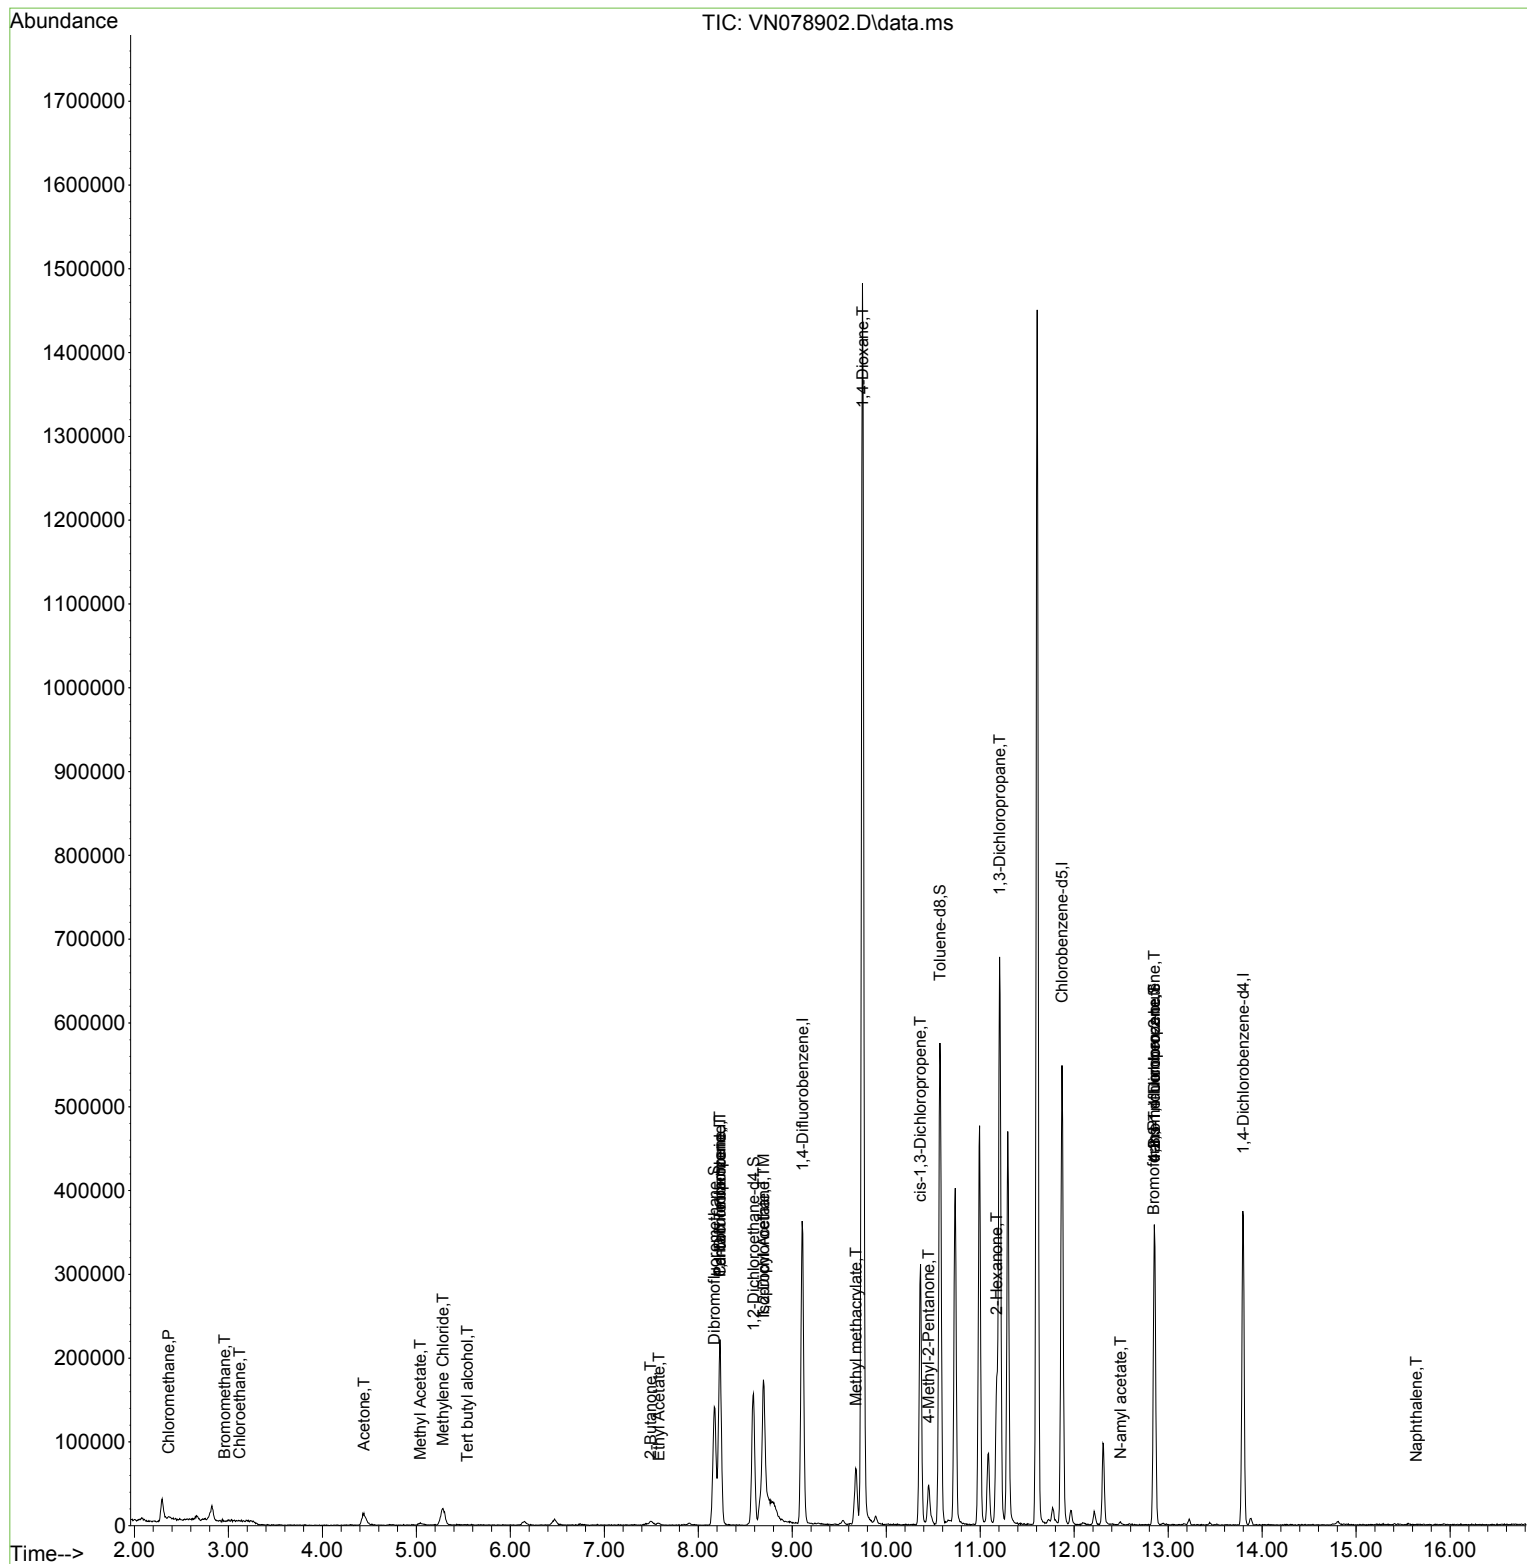



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.230 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52

Instrument :

MSVOA\_N

ClientSampleId :





PB154855ZHE#05

Tgt Ion:168 Resp: 149112

Ion Ratio Lower Upper

168 100

99 61.7 53.0 79.6

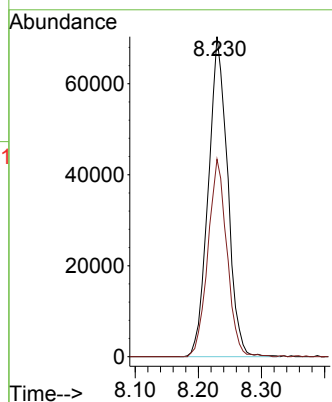

#3

Chloromethane

Concen: 0.473 ug/l

RT: 2.365 min Scan# 70

Delta R.T. -0.006 min

Lab File: VN078902.D




Acq: 16 Aug 2023 14:52


Tgt Ion: 50 Resp: 1367

Ion Ratio Lower Upper

50 100

52 35.2 26.5 39.7

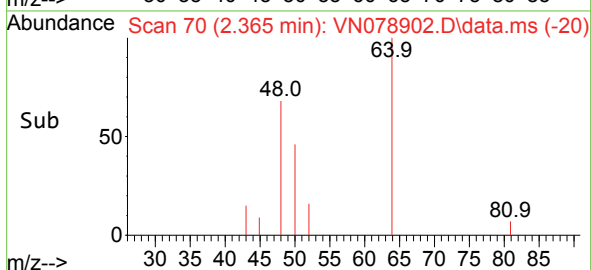



#5

Bromomethane

Concen: 0.264 ug/l

RT: 2.959 min Scan# 11

Delta R.T. 0.011 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52

Instrument :

MSVOA\_N

ClientSampleId :





PB154855ZHE#05

Tgt Ion: 94 Resp: 384

Ion Ratio Lower Upper

94 100

96 48.4 73.1 109.7#

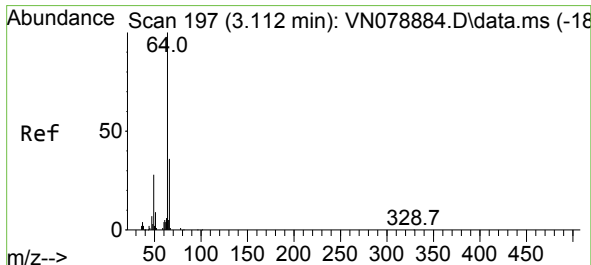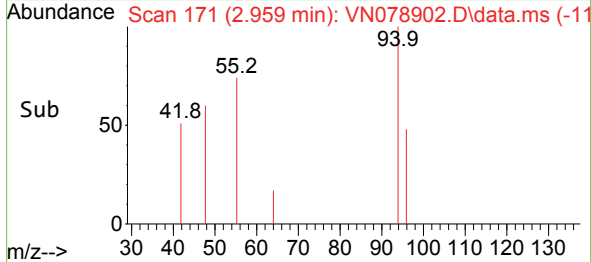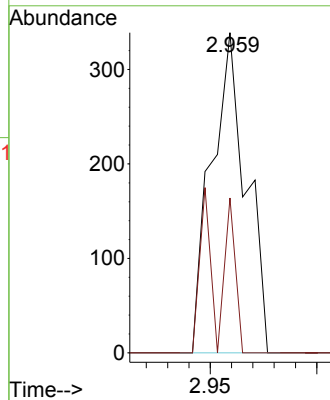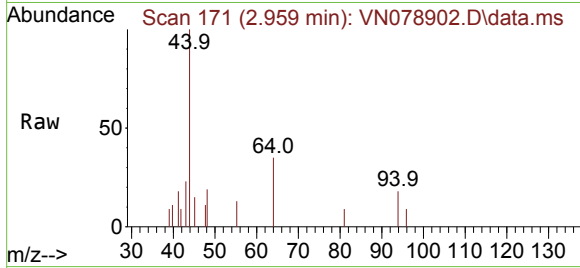

#6

Chloroethane

Concen: 0.290 ug/l

RT: 3.118 min Scan# 198

Delta R.T. 0.000 min

Lab File: VN078902.D




Acq: 16 Aug 2023 14:52


Tgt Ion: 64 Resp: 514

Ion Ratio Lower Upper

64 100

66 0.0 25.4 38.2#


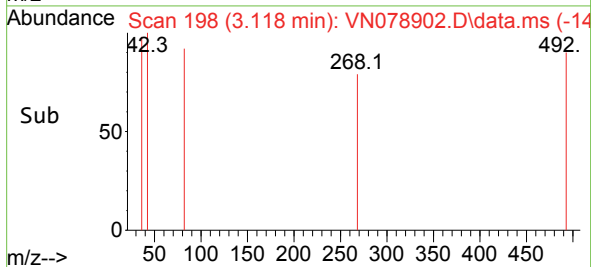
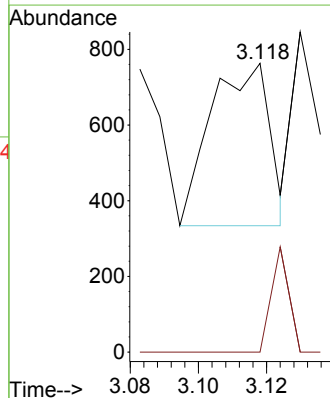
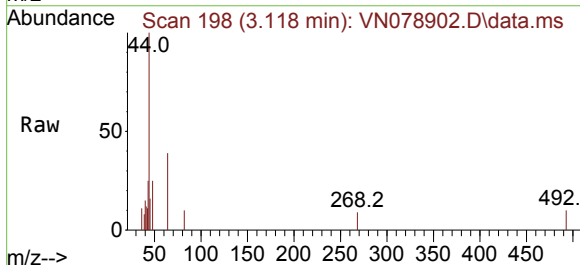




#11  
Tert butyl alcohol  
Concen: 0.419 ug/l  
RT: 5.541 min Scan# 610  
Delta R.T. -0.001 min  
Lab File: VN078902.D  
Acq: 16 Aug 2023 14:52




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB154855ZHE#05


Tgt Ion: 59 Resp: 163  
Ion Ratio Lower Upper  
59 100  
57 0.0 8.2 12.4#



#16  
Acetone  
Concen: 28.966 ug/l  
RT: 4.442 min Scan# 423  
Delta R.T. -0.000 min  
Lab File: VN078902.D  
Acq: 16 Aug 2023 14:52

Tgt Ion: 43 Resp: 27732  
Ion Ratio Lower Upper  
43 100  
58 28.8 28.0 42.0


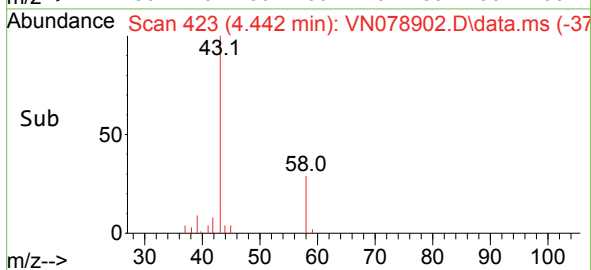






#18  
Methyl Acetate  
Concen: 1.194 ug/l  
RT: 5.042 min Scan# 51  
Delta R.T. -0.000 min  
Lab File: VN078902.D  
Acq: 16 Aug 2023 14:52




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB154855ZHE#05


Tgt Ion: 43 Resp: 4830  
Ion Ratio Lower Upper  
43 100  
74 18.0 26.2 39.4#

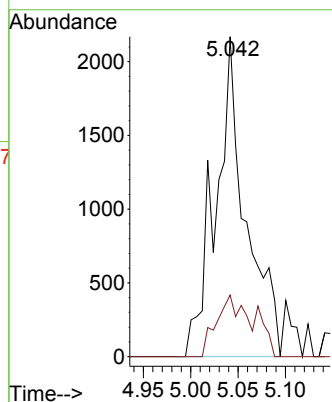

#20  
Methylene Chloride  
Concen: 7.122 ug/l  
RT: 5.283 min Scan# 566  
Delta R.T. -0.000 min  
Lab File: VN078902.D  
Acq: 16 Aug 2023 14:52

Tgt Ion: 84 Resp: 14530  
Ion Ratio Lower Upper  
84 100  
49 150.6 79.7 119.5#  
51 46.9 25.2 37.8#  
86 60.0 53.3 79.9


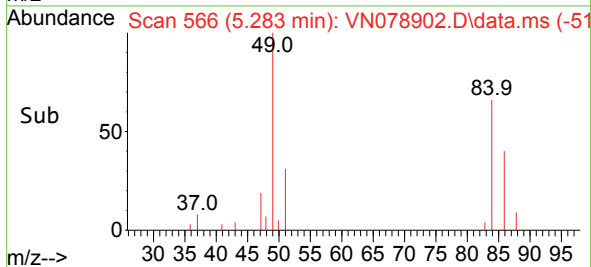

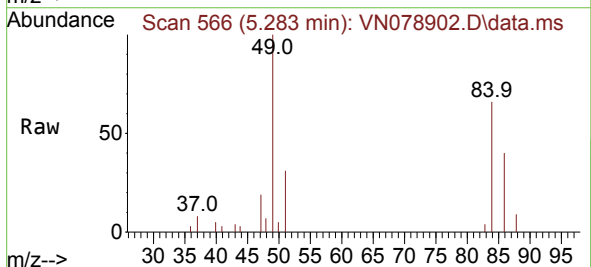




#25  
2-Butanone  
Concen: 5.941 ug/l  
RT: 7.494 min Scan# 941  
Delta R.T. 0.000 min  
Lab File: VN078902.D  
Acq: 16 Aug 2023 14:52




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB154855ZHE#05


Tgt Ion: 43 Resp: 9119  
Ion Ratio Lower Upper  
43 100  
72 18.9 30.2 45.2#

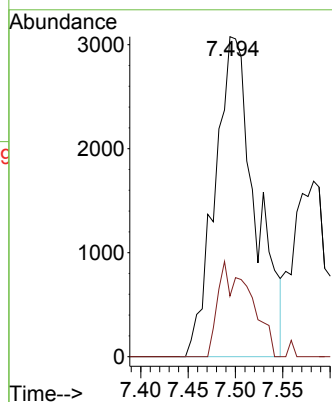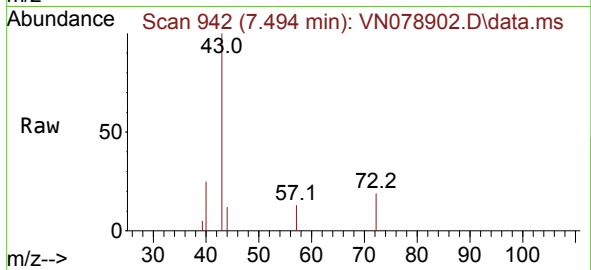

#31  
Cyclohexane  
Concen: Below Cal  
RT: 8.224 min Scan# 1066  
Delta R.T. -0.041 min  
Lab File: VN078902.D  
Acq: 16 Aug 2023 14:52

Tgt Ion: 56 Resp: 4310  
Ion Ratio Lower Upper  
56 100  
69 120.1 26.8 40.2#  
84 89.3 81.8 122.6

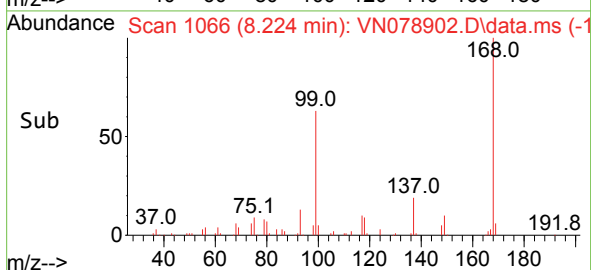



#33

1,2-Dichloroethane-d4

Concen: 54.010 ug/l

RT: 8.588 min Scan# 1127

Delta R.T. 0.005 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52

Instrument :

MSVOA\_N

ClientSampleId :





PB154855ZHE#05

Tgt Ion: 65 Resp: 125320

Ion Ratio Lower Upper

65 100

67 52.0 0.0 106.6

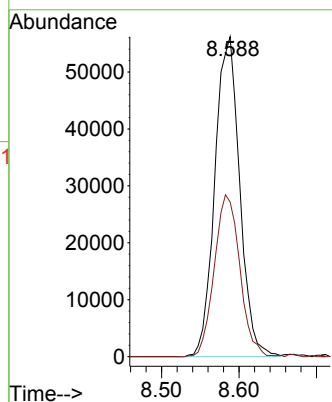

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1217

Delta R.T. -0.000 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52




Tgt Ion: 114 Resp: 298798

Ion Ratio Lower Upper


114 100

63 21.1 0.0 36.4

88 15.0 0.0 30.6

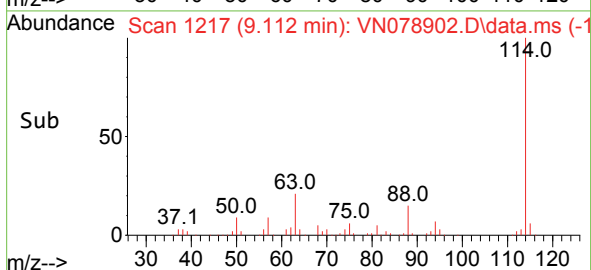





#35

Dibromofluoromethane

Concen: 50.832 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52

Instrument :

MSVOA\_N

ClientSampleId :

PB154855ZHE#05





Tgt Ion:113 Resp: 102241

Ion Ratio Lower Upper

113 100

111 101.0 82.6 123.8

192 17.4 12.7 19.1



#36

1,1-Dichloropropene

Concen: 4.409 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.147 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52




Tgt Ion: 75 Resp: 13339


Ion Ratio Lower Upper

75 100

110 2.3 19.1 57.3#

77 0.0 25.0 37.4#

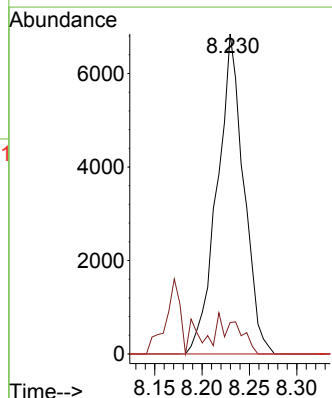



#37

Ethyl Acetate

Concen: 1.260 ug/l

RT: 7.582 min Scan# 91

Delta R.T. 0.011 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52

Instrument :

MSVOA\_N

ClientSampleId :

PB154855ZHE#05





Tgt Ion: 43 Resp: 4267

Ion Ratio Lower Upper

43 100

61 11.5 13.2 19.8#

70 1.5 11.3 16.9#

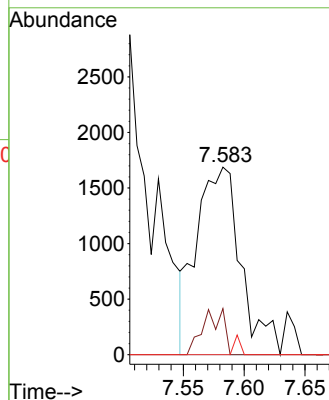

#38

Carbon Tetrachloride

Concen: 5.625 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.141 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52




Tgt Ion: 117 Resp: 17052


Ion Ratio Lower Upper

117 100

119 6.1 77.3 115.9#

121 0.0 23.3 34.9#

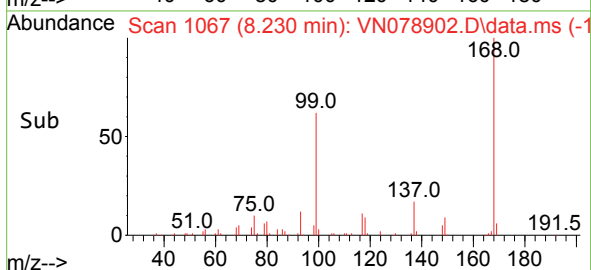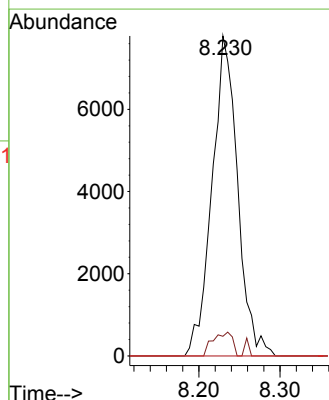



#42

1,2-Dichloroethane

Concen: 0.327 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. 0.017 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52

Instrument :

MSVOA\_N

ClientSampleId :





PB154855ZHE#05

Tgt Ion: 62 Resp: 1093

Ion Ratio Lower Upper

62 100

98 0.0 0.0 19.8

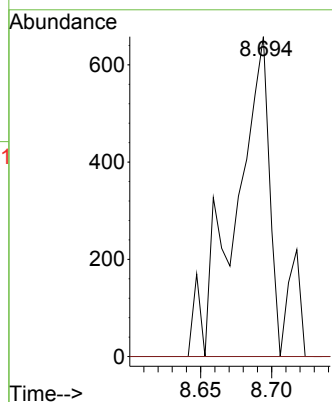

#43

Isopropyl Acetate

Concen: 39.579 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. 0.000 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52




Tgt Ion: 43 Resp: 236815


Ion Ratio Lower Upper

43 100

61 12.3 24.7 37.1#

87 7.6 14.6 21.8#

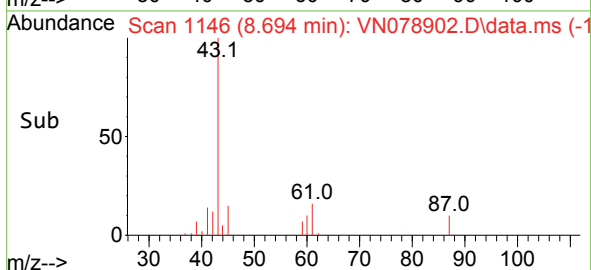



#48

Methyl methacrylate

Concen: 1.869 ug/l

RT: 9.676 min Scan# 11

Delta R.T. -0.012 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52

Instrument :

MSVOA\_N

ClientSampleId :

PB154855ZHE#05





Tgt Ion: 41 Resp: 5067

Ion Ratio Lower Upper

41 100

69 0.0 90.4 135.6#

39 56.7 54.6 81.8

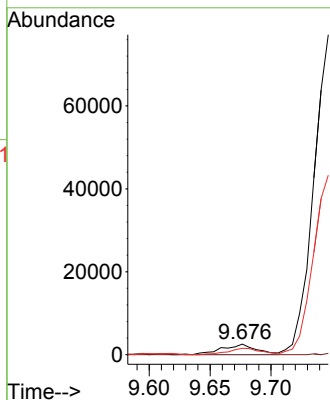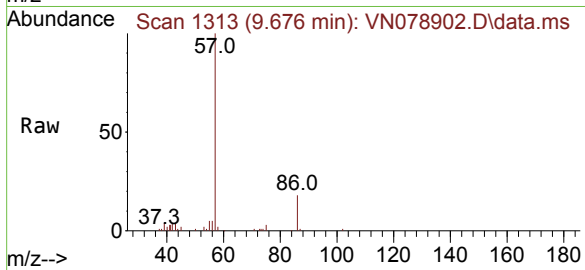

#49

1,4-Dioxane

Concen: 3.789 ug/l

RT: 9.747 min Scan# 1325

Delta R.T. 0.047 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52




Tgt Ion: 88 Resp: 175


Ion Ratio Lower Upper

88 100

43 824688.0 17.0 25.6#

58 4016.0 47.0 70.4#


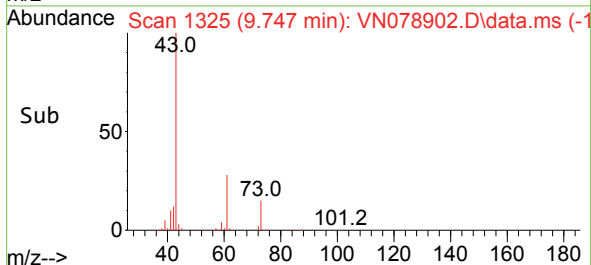
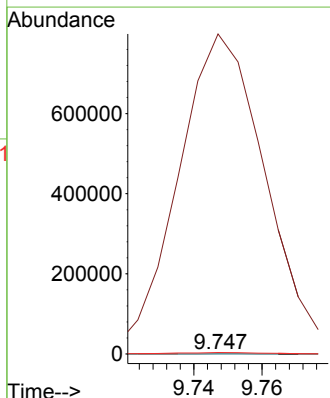
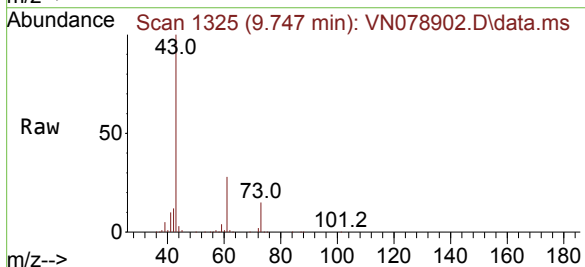




#50  
Toluene-d8  
Concen: 51.791 ug/l  
RT: 10.571 min Scan# 1465  
Delta R.T. -0.000 min  
Lab File: VN078902.D  
Acq: 16 Aug 2023 14:52




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB154855ZHE#05


Tgt Ion: 98 Resp: 386795  
Ion Ratio Lower Upper  
98 100  
100 63.4 52.0 78.0

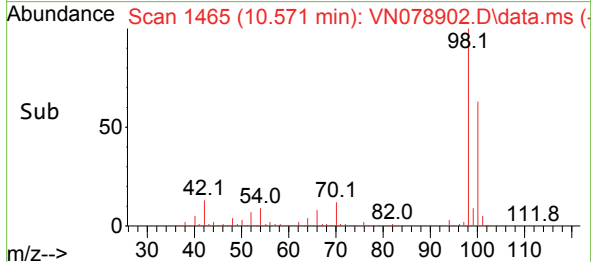

#51  
4-Methyl-2-Pentanone  
Concen: 11.115 ug/l  
RT: 10.453 min Scan# 1445  
Delta R.T. -0.000 min  
Lab File: VN078902.D  
Acq: 16 Aug 2023 14:52

Tgt Ion: 43 Resp: 39443  
Ion Ratio Lower Upper  
43 100  
58 31.2 36.6 54.8#


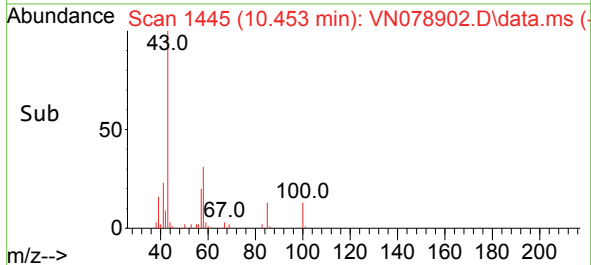

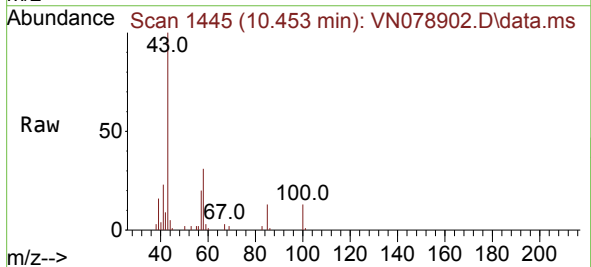


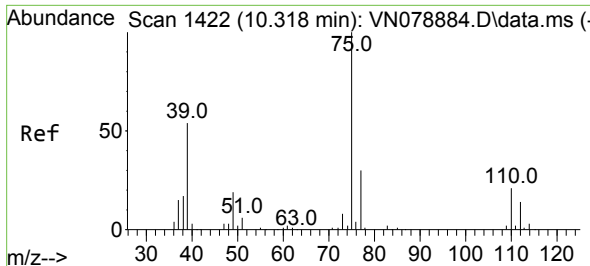

#54  
 cis-1,3-Dichloropropene  
 Concen: 13.372 ug/l  
 RT: 10.365 min Scan# 14  
 Delta R.T. 0.047 min  
 Lab File: VN078902.D  
 Acq: 16 Aug 2023 14:52




Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 PB154855ZHE#05


Tgt Ion: 75 Resp: 50367  
 Ion Ratio Lower Upper  
 75 100  
 77 0.0 26.1 39.1#  
 39 42.3 31.6 47.4

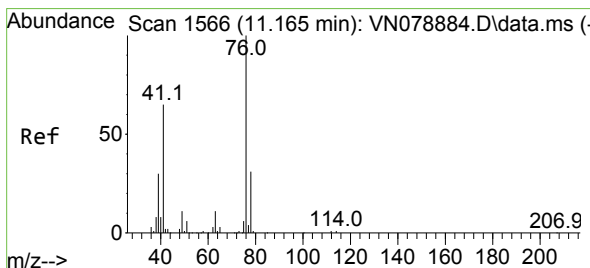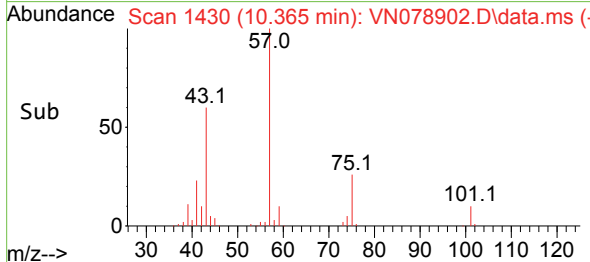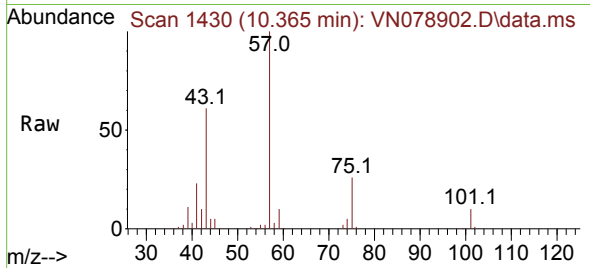

#57  
 1,3-Dichloropropane  
 Concen: 1.716 ug/l  
 RT: 11.206 min Scan# 1573  
 Delta R.T. 0.041 min  
 Lab File: VN078902.D  
 Acq: 16 Aug 2023 14:52

Tgt Ion: 76 Resp: 6757  
 Ion Ratio Lower Upper  
 76 100  
 78 0.0 26.1 39.1#


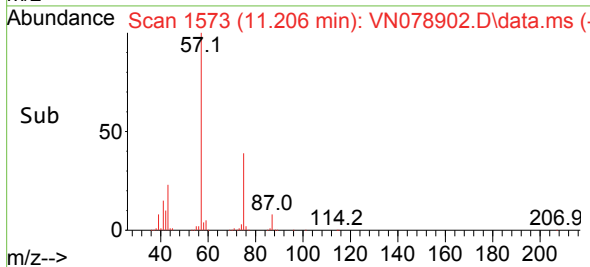

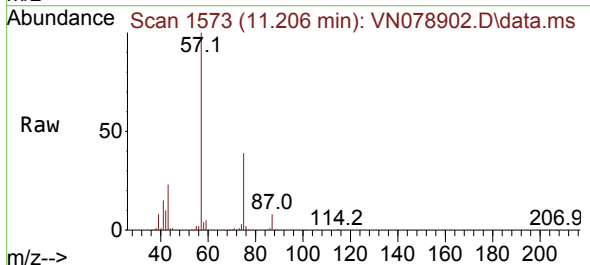


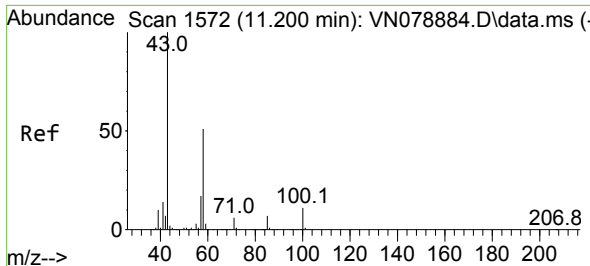

#59  
2-Hexanone  
Concen: 55.892 ug/l  
RT: 11.176 min Scan# 11176  
Delta R.T. -0.024 min  
Lab File: VN078902.D  
Acq: 16 Aug 2023 14:52




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB154855ZHE#05


Tgt Ion: 43 Resp: 143660  
Ion Ratio Lower Upper  
43 100  
58 0.0 31.7 95.1#

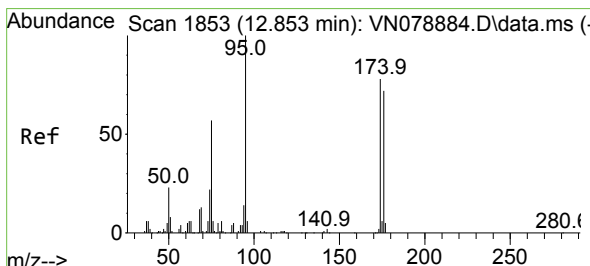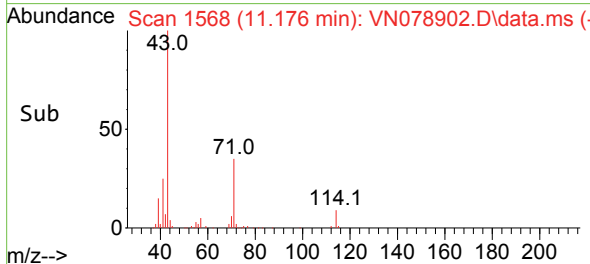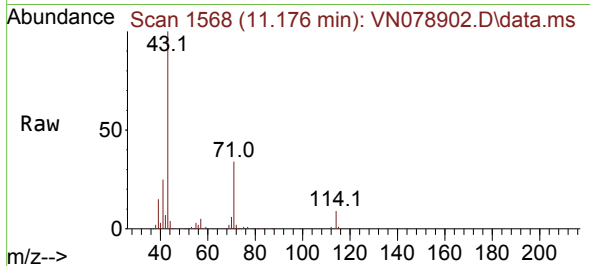

#62  
4-Bromofluorobenzene  
Concen: 47.883 ug/l  
RT: 12.853 min Scan# 1853  
Delta R.T. -0.000 min  
Lab File: VN078902.D  
Acq: 16 Aug 2023 14:52

Tgt Ion: 95 Resp: 116888  
Ion Ratio Lower Upper  
95 100  
174 75.3 0.0 143.8  
176 73.2 0.0 135.8

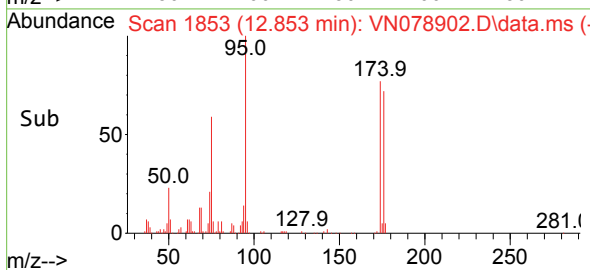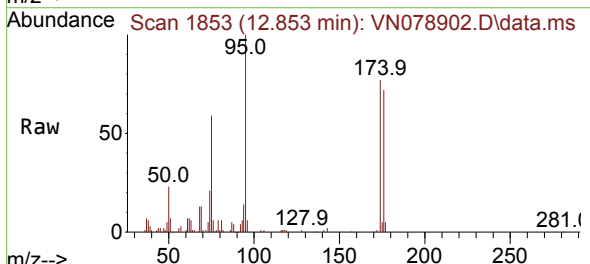



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.870 min Scan# 1

Delta R.T. -0.001 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52

Instrument :

MSVOA\_N

ClientSampleId :

PB154855ZHE#05





Tgt Ion:117 Resp: 291987

Ion Ratio Lower Upper

117 100

82 55.8 44.0 66.0

119 32.3 25.6 38.4



#71

Bromoform

Concen: 0.422 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.265 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52




Tgt Ion:173 Resp: 720

Ion Ratio Lower Upper


173 100

175 0.0 24.3 73.0#

254 0.0 0.0 0.0

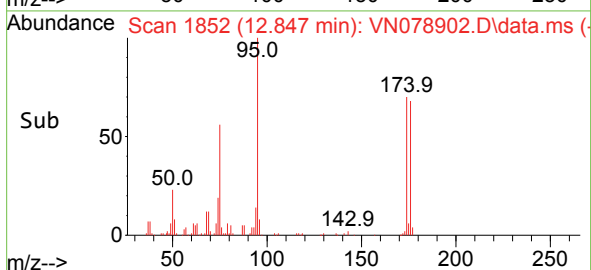



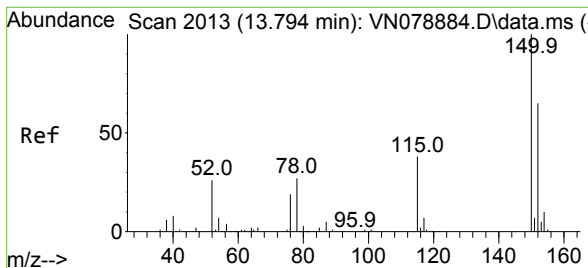

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.800 min Scan# 20

Delta R.T. 0.006 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52

Instrument :

MSVOA\_N

ClientSampleId :

PB154855ZHE#05





Tgt Ion:152 Resp: 94343

Ion Ratio Lower Upper

152 100

115 60.2 32.3 96.8

150 157.6 0.0 355.8

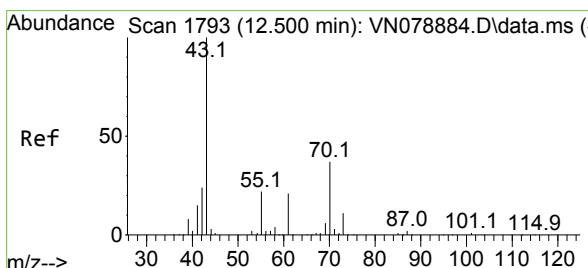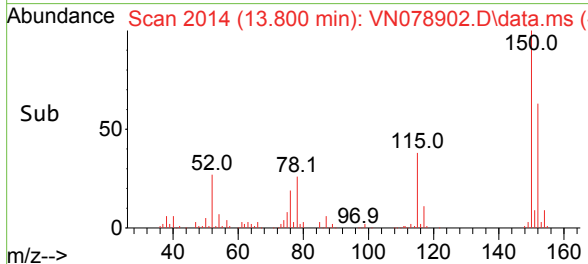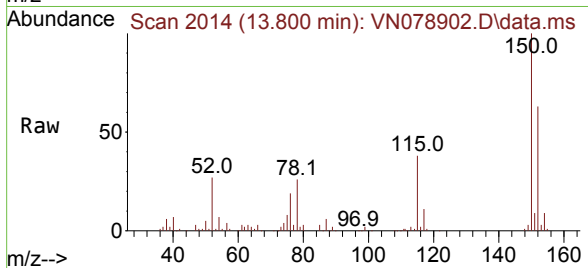

#74

N-ethyl acetate

Concen: 0.538 ug/l

RT: 12.494 min Scan# 1792

Delta R.T. -0.006 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52

Tgt Ion: 43 Resp: 2138




Ion Ratio Lower Upper


43 100

70 0.0 43.4 65.2#

55 0.0 21.4 32.0#

61 0.0 22.8 34.2#

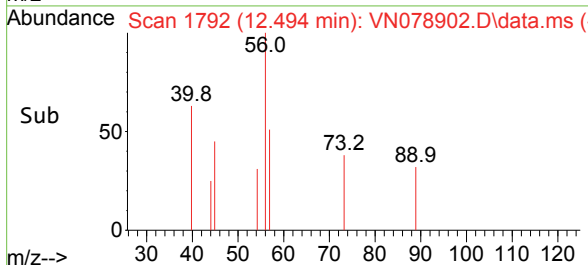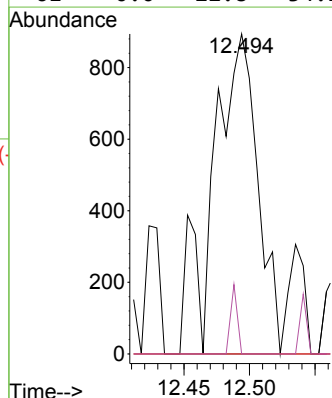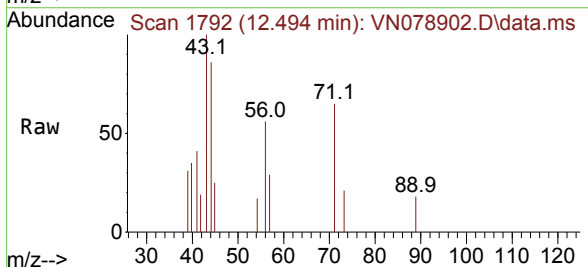

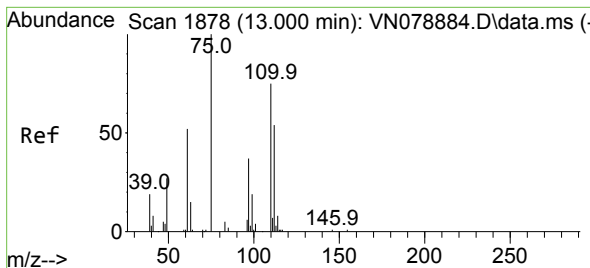

#76

1,2,3-Trichloropropane

Concen: 29.648 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.147 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52

Instrument :

MSVOA\_N

ClientSampleId :





PB154855ZHE#05

Tgt Ion: 75 Resp: 67397

Ion Ratio Lower Upper

75 100

77 1.5 84.5 253.5#

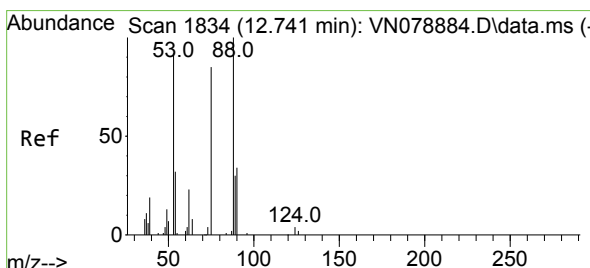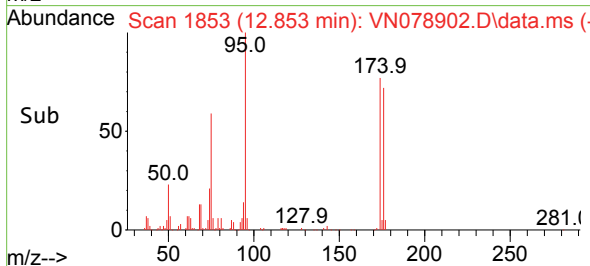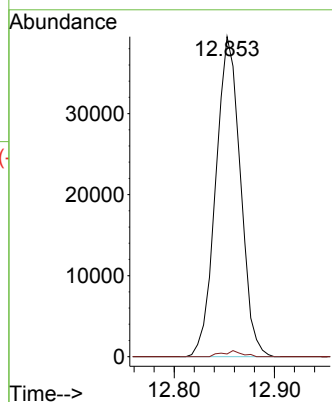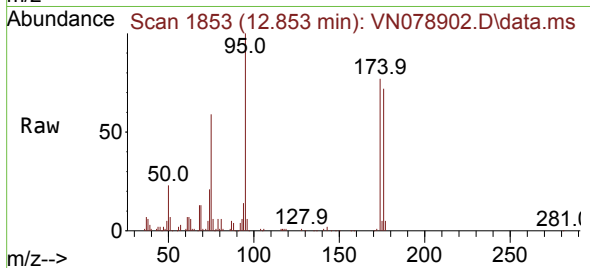

#81

trans-1,4-Dichloro-2-butene

Concen: 75.739 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.112 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52




Tgt Ion: 75 Resp: 67397


Ion Ratio Lower Upper

75 100

53 0.0 67.4 101.2#

89 0.1 38.8 58.2#

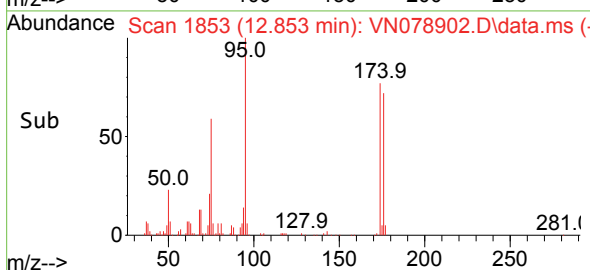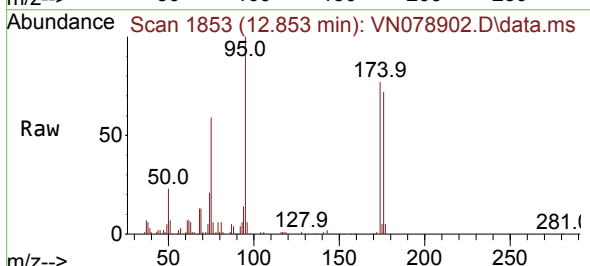



#92

1,2-Dibromo-3-Chloropropane

Concen: Below Cal

RT: 14.694 min Scan# 2171

Delta R.T. -0.029 min

Lab File: VN078902.D


Acq: 16 Aug 2023 14:52

Instrument :

MSVOA\_N

ClientSampleId :

PB154855ZHE#05






Tgt Ion: 75 Resp: 54

Ion Ratio Lower Upper

75 100

155 0.0 39.1 117.2#

157 0.0 50.3 150.9#

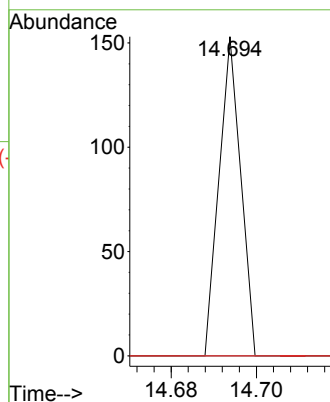

#95

Naphthalene

Concen: 2.589 ug/l

RT: 15.641 min Scan# 2327

Delta R.T. -0.006 min

Lab File: VN078902.D

Acq: 16 Aug 2023 14:52

Tgt Ion:128 Resp: 64

Ion Ratio Lower Upper

128 100

127 0.0 10.0 15.0#

129 0.0 8.7 13.1#

