
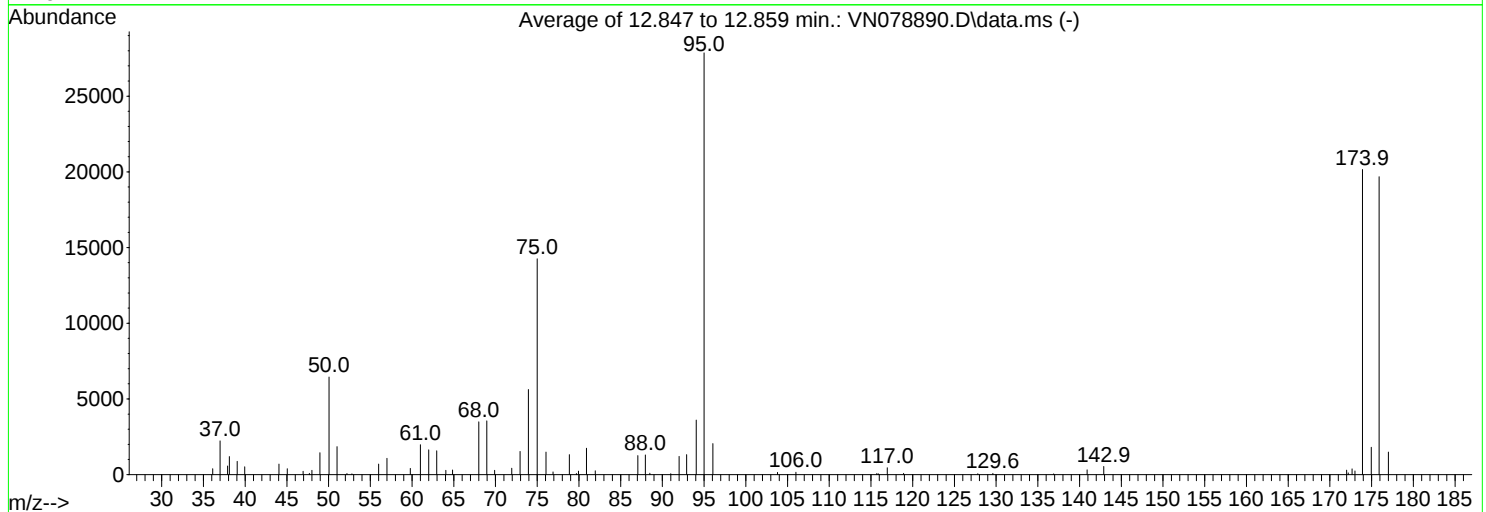


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081623\
Data File : VN078890.D
Acq On : 16 Aug 2023 09:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
Title : SW846 8260
Last Update : Wed Aug 16 02:42:02 2023

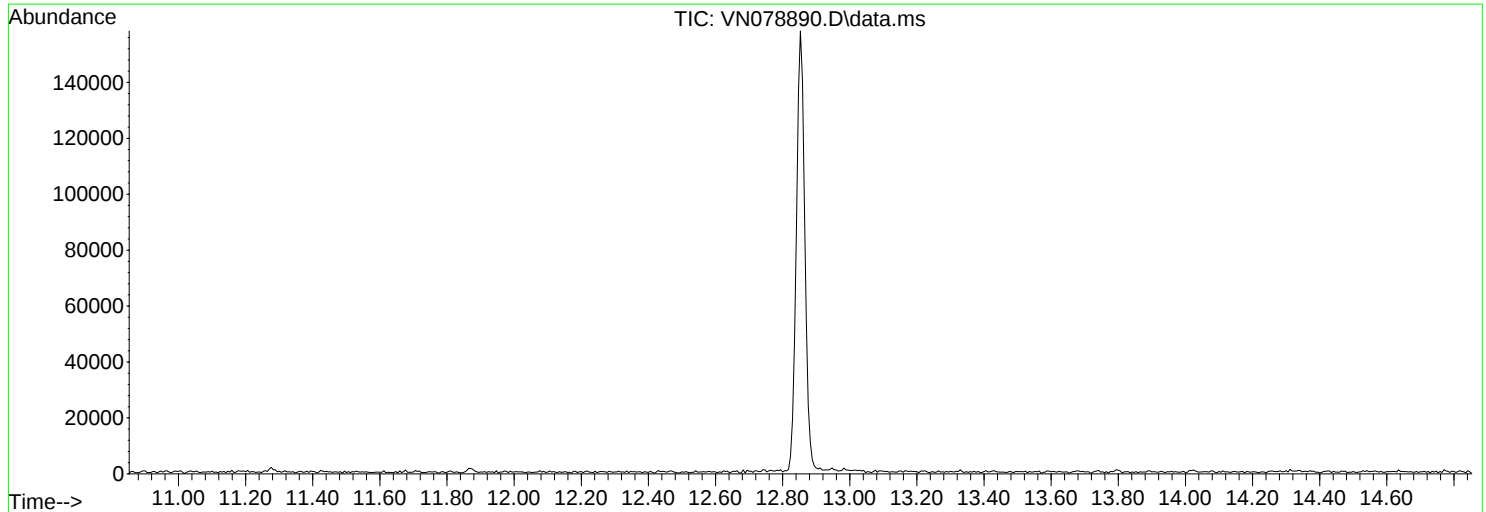

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	6451	PASS
75	95	30	60	51.2	14260	PASS
95	95	100	100	100.0	27861	PASS
96	95	5	9	7.4	2055	PASS
173	174	0.00	2	1.2	241	PASS
174	95	50	100	72.3	20155	PASS
175	174	5	9	9.0	1806	PASS
176	174	95	101	97.6	19677	PASS
177	176	5	9	7.6	1489	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	395	48.95	1448	64.05	281	78.85	1321
37.00	2227	50.05	6451	64.85	309	79.70	79
37.90	570	51.00	1847	68.00	3487	79.95	23
38.10	1198	52.20	70	68.95	3553	80.90	174
39.05	879	52.80	55	69.90	288	81.95	253
39.95	516	56.00	697	71.95	423	87.05	1255
44.05	695	57.00	1076	72.95	1533	87.95	1295
45.05	390	59.80	409	73.95	5626	88.50	100
46.95	221	61.00	1981	75.00	14260	91.00	62
47.70	90	62.00	1634	76.05	1494	92.00	1206
48.00	289	62.95	1578	76.90	185	92.90	1324

Average of 12.847 to 12.859 min.: VN078890.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	3607	136.90	50				
95.00	27861	140.90	321				
96.05	2055	142.90	535				
103.80	153	172.00	293				
106.00	164	172.20	118				
115.70	89	172.65	385				
115.90	51	173.00	241				
116.95	454	173.90	20155				
118.90	86	174.95	1806				
127.80	63	175.90	19677				
129.60	85	177.00	1489				

Instrument :

MSVOA_N

ClientSampleId :

BFB