
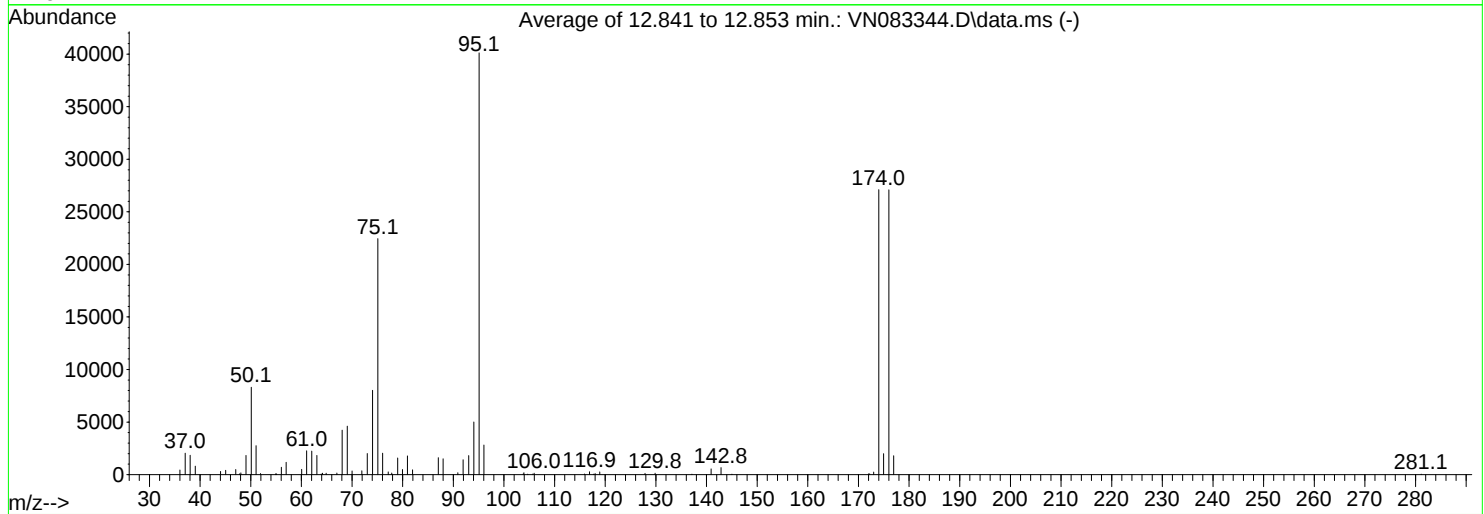


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081624\
Data File : VN083344.D
Acq On : 16 Aug 2024 07:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

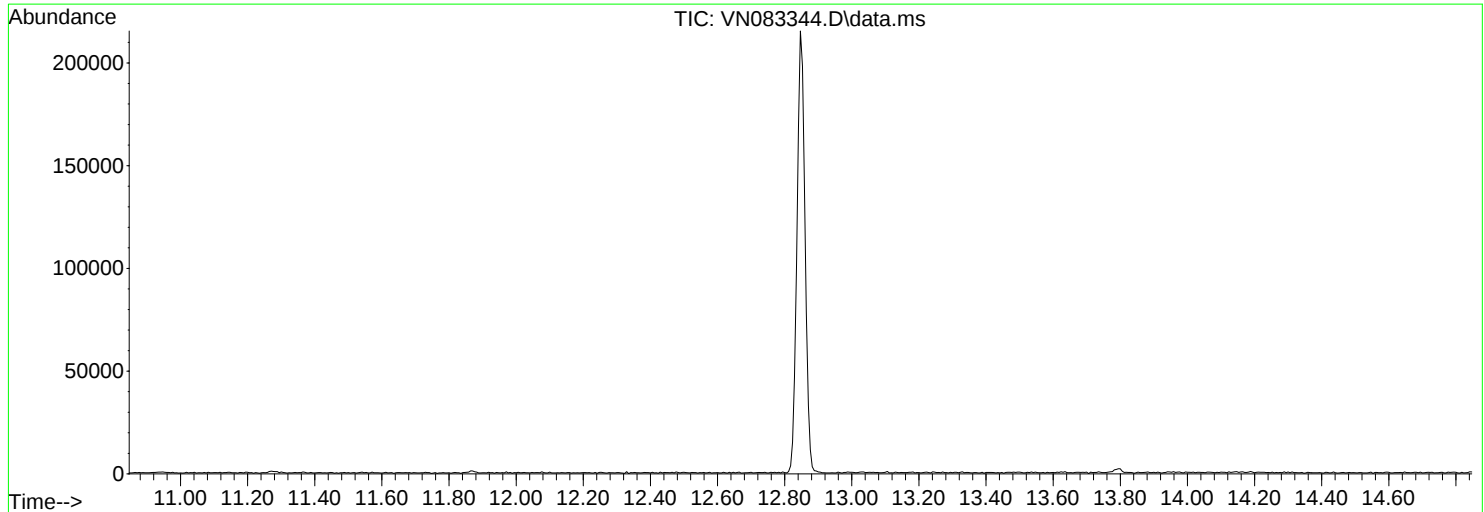

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	8306	PASS
75	95	30	60	56.0	22451	PASS
95	95	100	100	100.0	40123	PASS
96	95	5	9	7.0	2823	PASS
173	174	0.00	2	0.9	251	PASS
174	95	50	100	67.6	27115	PASS
175	174	5	9	7.4	1994	PASS
176	174	95	101	99.9	27099	PASS
177	176	5	9	6.7	1805	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	439	51.05	2749	64.15	144	77.15	25
37.05	2040	51.95	110	64.90	132	77.85	14
38.05	1839	54.90	75	67.00	146	79.00	157
39.05	804	55.10	74	68.05	4224	79.95	48
44.05	310	56.05	709	69.05	4616	80.95	1776
45.05	415	57.00	1179	70.00	352	81.95	453
47.05	492	60.05	510	71.95	366	87.05	1609
47.80	71	61.05	2271	73.00	2012	88.00	1511
48.05	171	62.05	2239	74.05	8020	90.90	179
49.05	1828	63.05	1829	75.10	22451	91.95	1416
50.10	8306	63.90	69	76.05	2046	93.05	1818

Average of 12.841 to 12.853 min.: VN083344.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	5012	118.00	101	174.00	27115		
95.10	40123	118.90	261	174.95	1994		
96.05	2823	127.85	116	176.00	27099		
103.80	72	129.85	144	176.95	1805		
103.95	177	137.10	50	281.10	50		
104.70	53	140.90	550				
105.70	54	142.85	676				
105.95	131	145.00	53				
115.90	60	172.00	78				
116.90	273	172.20	82				
117.70	51	173.00	251				

Instrument :

MSVOA_N

ClientSampleId :

BFB