

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN081718\
 Data File : VN050756.D
 Acq On : 18 Aug 2018 7:02
 Operator : MD\SY
 Sample : J4521-18
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 72-11990

Quant Time: Aug 20 00:49:13 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 14 08:07:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	620464	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1012162	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	894334	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	313052	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	420466	53.76	ug/l	0.00
Spiked Amount			Recovery	=	107.52%	
35) Dibromofluoromethane	7.59	113	389307	48.18	ug/l	0.00
Spiked Amount			Recovery	=	96.36%	
50) Toluene-d8	10.09	98	1413671	46.48	ug/l	0.00
Spiked Amount			Recovery	=	92.96%	
62) 4-Bromofluorobenzene	12.40	95	386908	38.51	ug/l	0.00
Spiked Amount			Recovery	=	77.02%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Chloromethane	2.06	50	3085	Below Cal	#	88
5) Bromomethane	2.57	94	2526	Below Cal		97
6) Chloroethane	2.71	64	108	Below Cal	#	43
10) Methyl Iodide	3.96	142	222	6.99	ug/l	# 42
14) Allyl chloride	4.56	41	4364	0.42	ug/l	# 25
16) Acetone	3.82	43	13152	5.32	ug/l	96
18) Methyl Acetate	4.34	43	14431	1.67	ug/l	95
20) Methylene Chloride	4.56	84	118045	14.99	ug/l	98
25) 2-Butanone	6.84	43	1231	0.38	ug/l	# 88
29) Tetrahydrofuran	7.22	42	929	0.55	ug/l	# 60
30) Chloroform	7.37	83	9861	0.70	ug/l	99
31) Cyclohexane	7.66	56	11069	0.59	ug/l	# 1
36) 1,1-Dichloropropene	7.67	75	42417	3.76	ug/l	# 49
38) Carbon Tetrachloride	7.67	117	54339	4.65	ug/l	# 17
43) Isopropyl Acetate	8.17	43	226647	19.53	ug/l	98
47) Bromodichloromethane	9.41	83	2366	0.21	ug/l	# 93
48) Methyl methacrylate	9.19	41	7021	1.20	ug/l	# 19
51) 4-Methyl-2-Pentanone	9.99	43	2362	0.30	ug/l	# 78
56) Ethyl methacrylate	10.22	69	944	2.00	ug/l	# 25
59) 2-Hexanone	10.76	43	15161	2.99	ug/l	# 58
70) Styrene	11.97	104	151	0.95	ug/l	# 26
75) 1,1,2,2-Tetrachloroethane	12.40	83	117	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.40	75	186490	36.60	ug/l	# 100
81) trans-1,4-Dichloro-2-buten	12.40	75	186490	132.44	ug/l	# 13
95) Naphthalene	15.14	128	30517	6.20	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN081718\
Data File : VN050756.D
Acq On : 18 Aug 2018 7:02
Operator : MD\SY
Sample : J4521-18
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
72-11990

Quant Time: Aug 20 00:49:13 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 14 08:07:08 2018
Response via : Initial Calibration

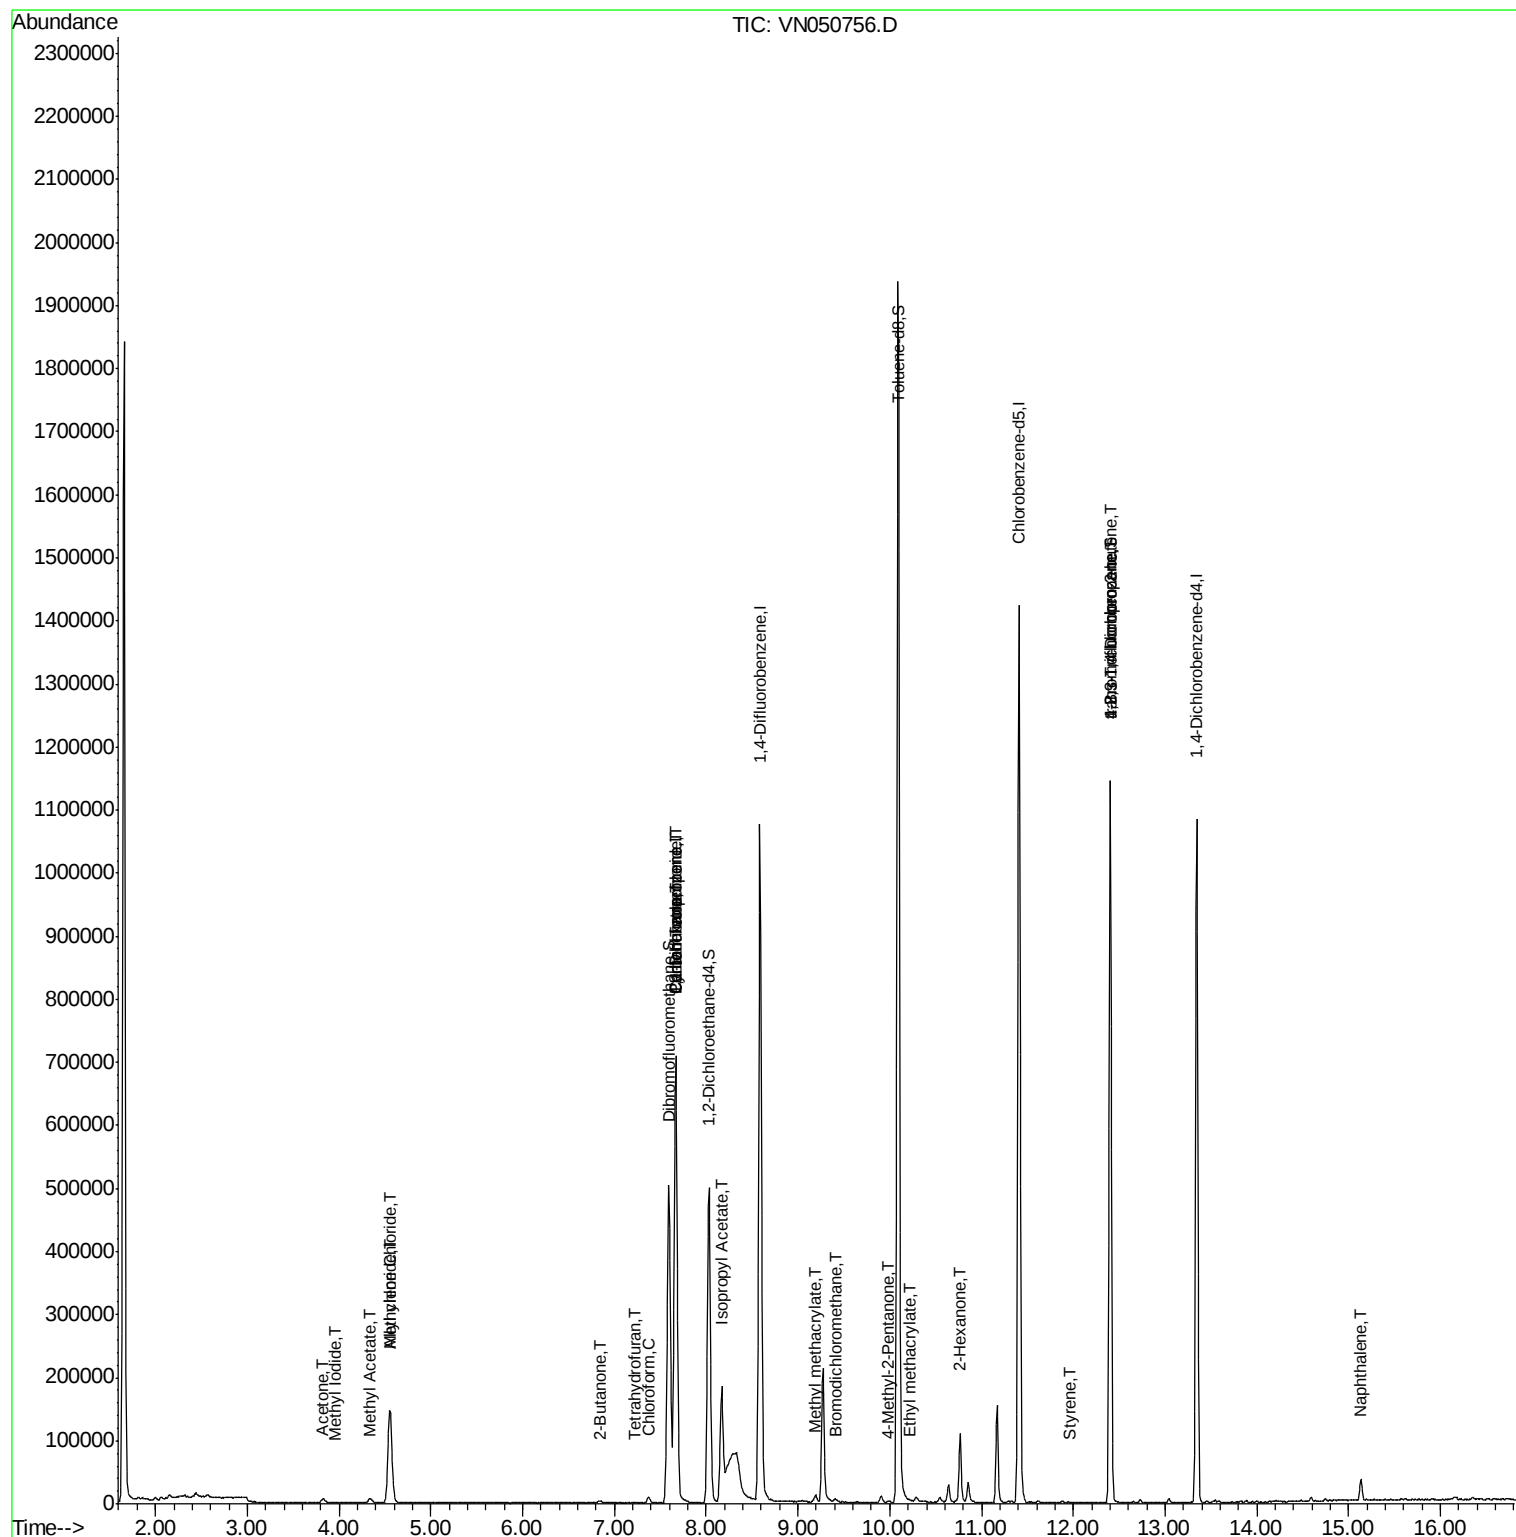

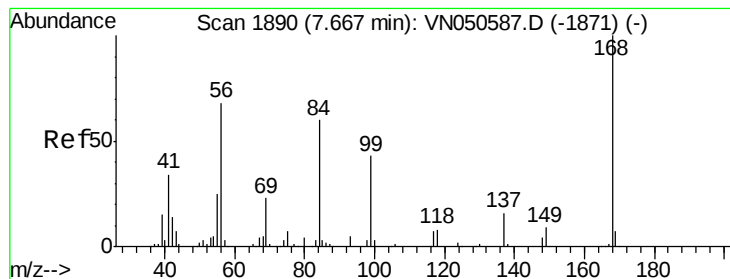

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1891

Delta R.T. 0.00 min

Lab File: VN050756.D

Acq: 18 Aug 2018 7:02

Instrument :

MSVOA_N

ClientSampled :


72-11990

Tot Ion:168 Resp: 620464

Ion Ratio Lower Upper

168 100

99 49.6 40.8 61.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.67

250000

200000



150000

100000

50000

0

Time-->



#5

Bromomethane

Concen: Below Cal

RT: 2.57 min Scan# 305

Delta R.T. 0.01 min

Lab File: VN050756.D


Acq: 18 Aug 2018 7:02

Tgt Ion: 94 Resp: 2526

Ion Ratio Lower Upper

94 100

96 89.8 74.0 111.0



Abundance Ion 93.90 (93.60 to 94.60): VNO

Ion 95.90 (95.60 to 96.60): VNO

2.57


1500


1000

500

0

Time-->





#6

Chloroethane

Concen: Below Cal

RT: 2.71 min Scan# 349

Delta R.T. 0.01 min

Lab File: VN050756.D

Acq: 18 Aug 2018 7:02

Instrument :

MSVOA_N

ClientSampleId :


72-11990

Tot Ion: 64 Resp: 108

Ion Ratio Lower Upper

64 100

66 0.0 25.7 38.5#

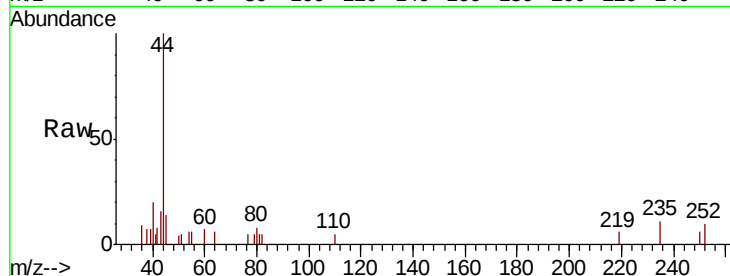

Abundance Ion 63.90 (63.60 to 64.60): VN050756.D (-252) (-)

Ion 65.90 (65.60 to 66.60): VN050756.D (-252) (-)

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71

2.71


2.71

2.71


2.71

2.71

2.71



Time-->



#10

Methyl Iodide

Concen: 6.99 ug/l

RT: 3.96 min Scan# 737

Delta R.T. 0.01 min

Lab File: VN050756.D

Acq: 18 Aug 2018 7:02


Tgt Ion: 142 Resp: 222

Ion Ratio Lower Upper

142 100

127 0.0 32.6 49.0#

141 0.0 11.5 17.3#



Abundance Ion 141.80 (141.50 to 142.50): VN050756.D (-642) (-)

Ion 126.80 (126.50 to 127.50): VN050756.D (-642) (-)

Ion 140.80 (140.50 to 141.50): VN050756.D (-642) (-)

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96

3.96


3.96

3.96


3.96

3.96

3.96







Time-->

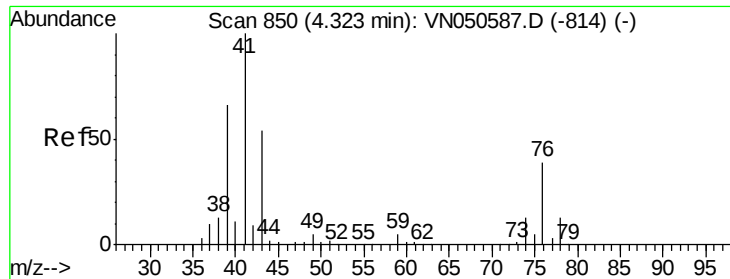

#14
Allvl chloride
Concen: 0.42 ug/l
RT: 4.56 min Scan# 923
Delta R.T. 0.23 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02




Instrument :
MSVOA_N
ClientSampleId :
72-11990


Tot Ion: 41 Resp: 4364
Ion Ratio Lower Upper
41 100
39 0.0 51.4 77.0#
76 0.0 29.4 44.0#

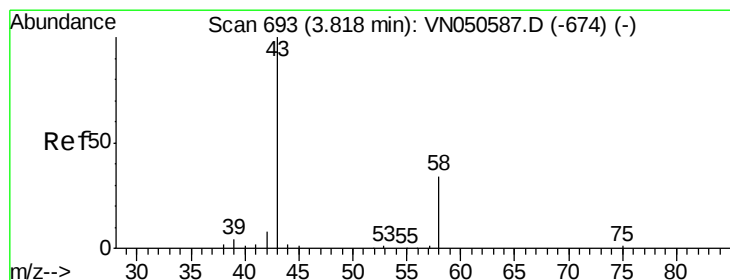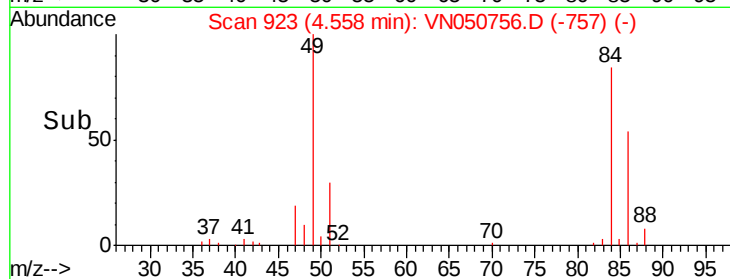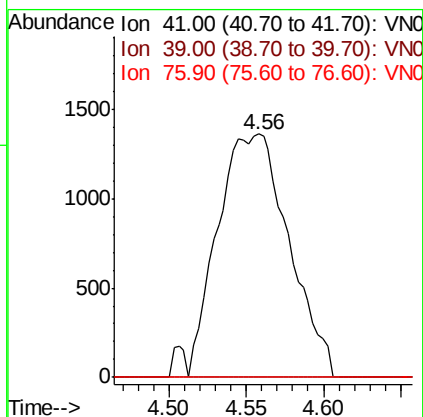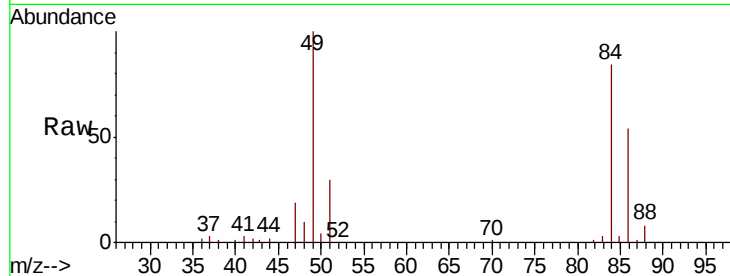

#16
Acetone
Concen: 5.32 ug/l
RT: 3.82 min Scan# 695
Delta R.T. 0.01 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02

Tgt Ion: 43 Resp: 13152
Ion Ratio Lower Upper
43 100
58 31.8 27.1 40.7


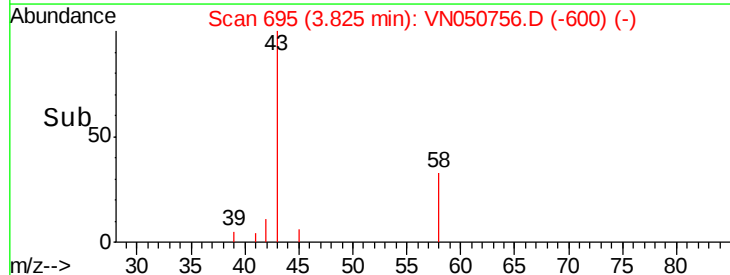
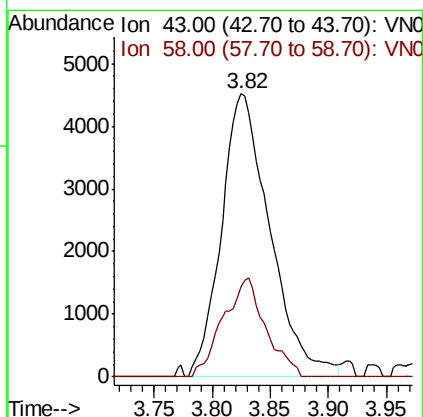



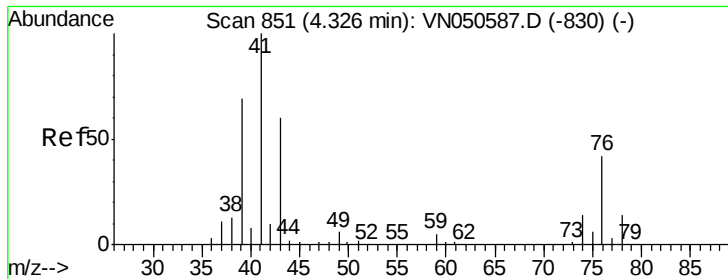

#18
Methyl Acetate
Concen: 1.67 ug/l
RT: 4.34 min Scan# 854
Delta R.T. 0.01 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02




Instrument :
MSVOA_N
ClientSampled :
72-11990


Tot Ion: 43 Resp: 14431
Ion Ratio Lower Upper
43 100
74 21.9 19.7 29.5

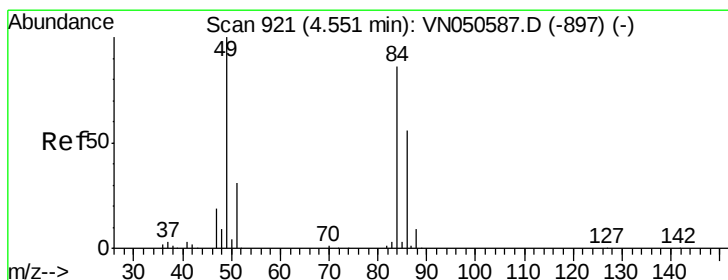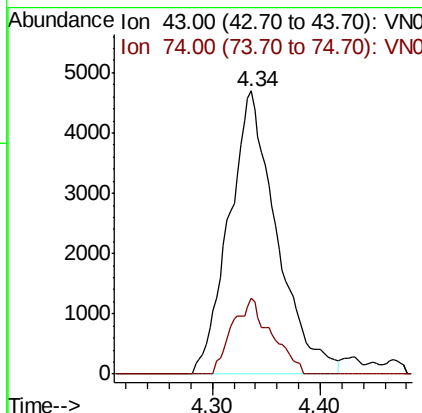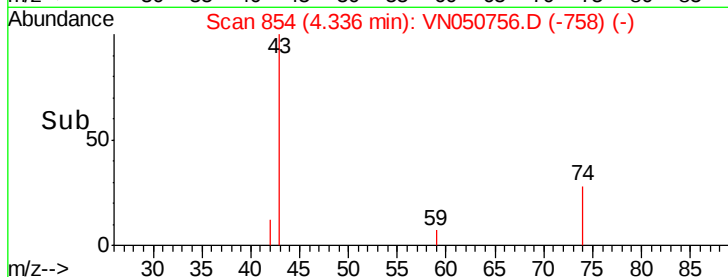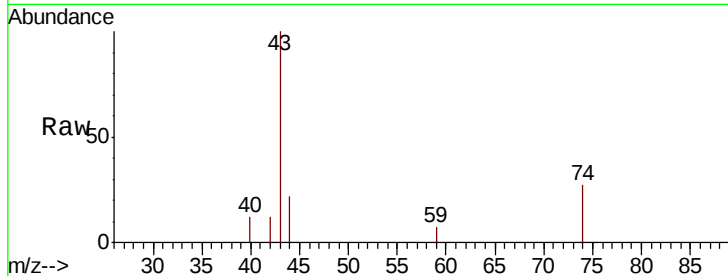

#20
Methylene Chloride
Concen: 14.99 ug/l
RT: 4.56 min Scan# 923
Delta R.T. 0.01 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02

Tgt Ion: 84 Resp: 118045
Ion Ratio Lower Upper
84 100
49 119.3 92.6 138.8
51 36.3 28.6 43.0
86 64.9 52.2 78.2


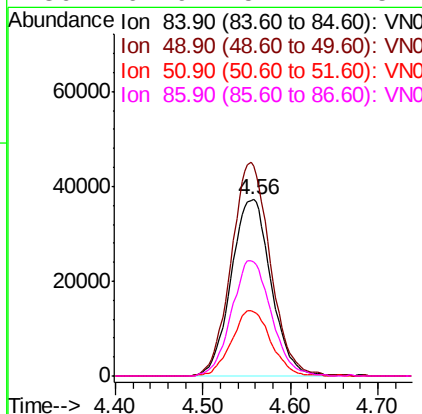
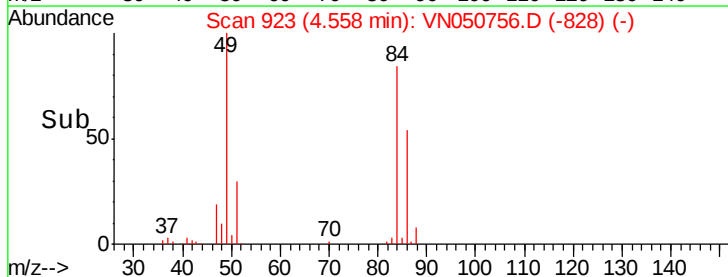
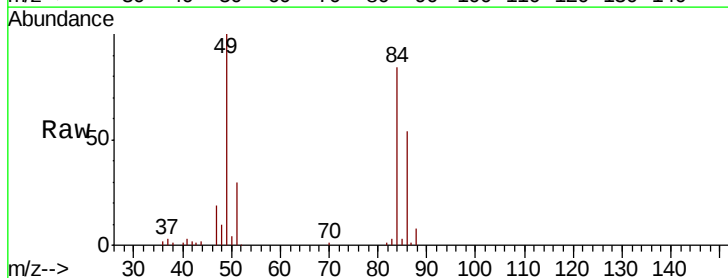


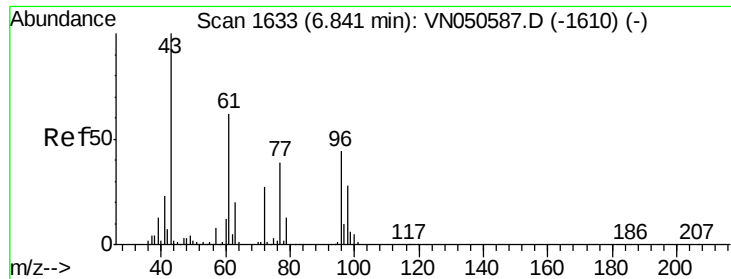

#25
2-Butanone
Concen: 0.38 ug/l
RT: 6.84 min Scan# 1634
Delta R.T. 0.00 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02




Instrument :
MSVOA_N
ClientSampled :
72-11990


Tot Ion: 43 Resp: 1231
Ion Ratio Lower Upper
43 100
72 21.1 21.8 32.6#

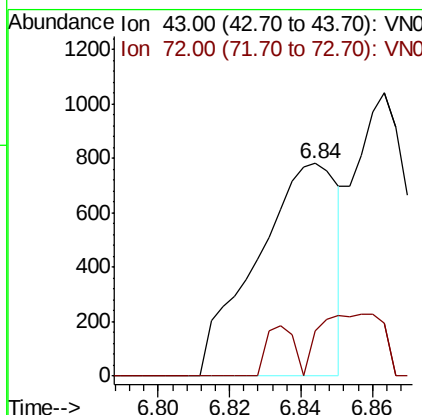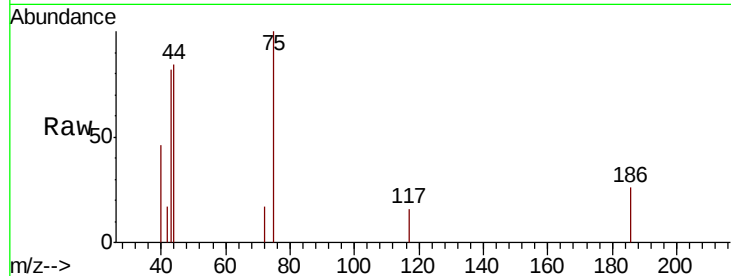

#29
Tetrahydrofuran
Concen: 0.55 ug/l
RT: 7.22 min Scan# 1750
Delta R.T. 0.00 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02

Tgt Ion: 42 Resp: 929
Ion Ratio Lower Upper
42 100
72 28.3 35.8 53.6#
71 6.8 33.4 50.0#


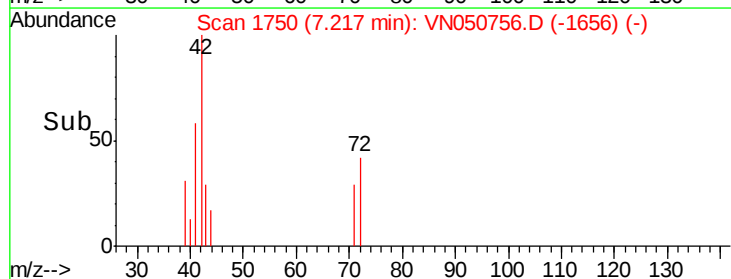
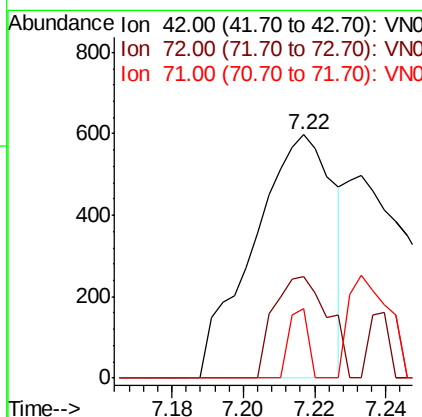





#30
Chloroform
Concen: 0.70 ug/l
RT: 7.37 min Scan# 1799
Delta R.T. 0.00 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02




Instrument :
MSVOA_N
ClientSampleId :
72-11990


Tot Ion: 83 Resp: 9861
Ion Ratio Lower Upper
83 100
85 66.1 52.5 78.7

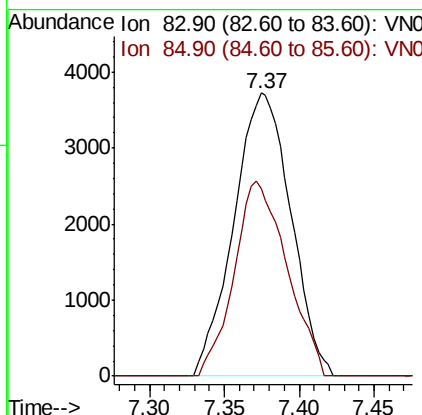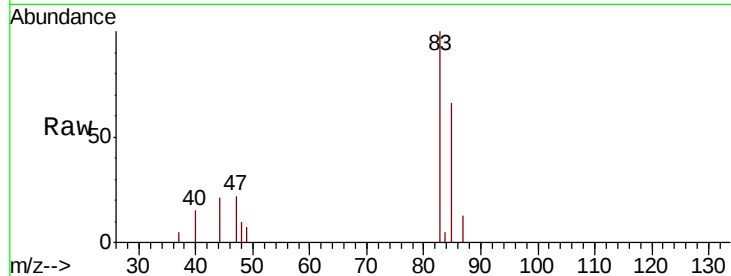

#31
Cyclohexane
Concen: 0.59 ug/l
RT: 7.66 min Scan# 1889
Delta R.T. 0.01 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02

Tgt Ion: 56 Resp: 11069
Ion Ratio Lower Upper
56 100
69 198.0 25.8 38.6#
84 150.8 67.8 101.6#


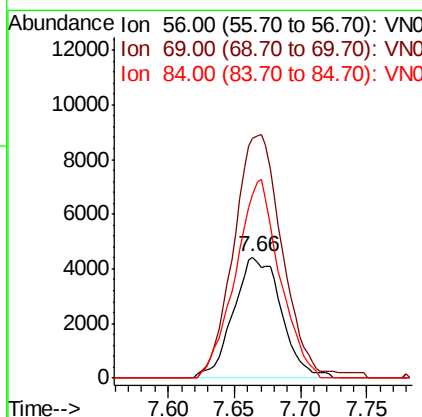

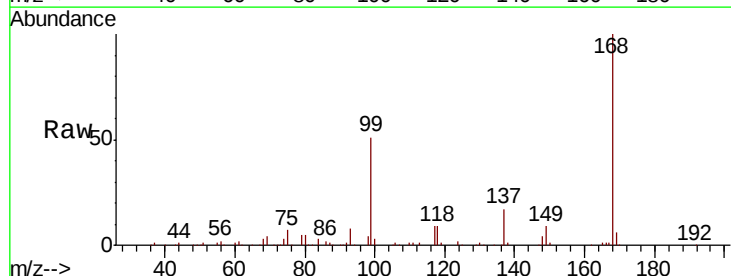


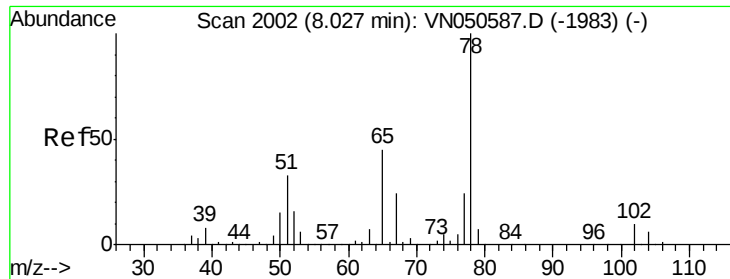

#33
 1,2-Dichloroethane-d4
 Concen: 53.76 ug/l
 RT: 8.03 min Scan# 2003
 Delta R.T. 0.00 min
 Lab File: VN050756.D
 Acq: 18 Aug 2018 7:02




Instrument :
 MSVOA_N
 ClientSampleId :
 72-11990


Tot Ion: 65 Resp: 420466
 Ion Ratio Lower Upper
 65 100
 67 54.6 0.0 109.8

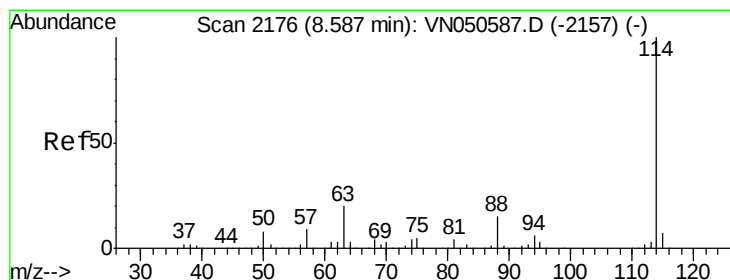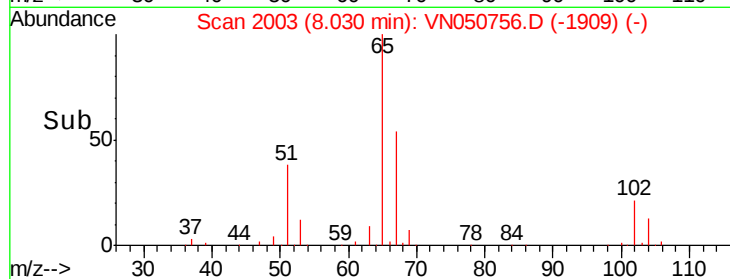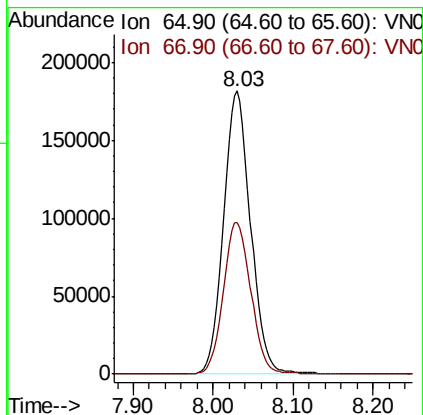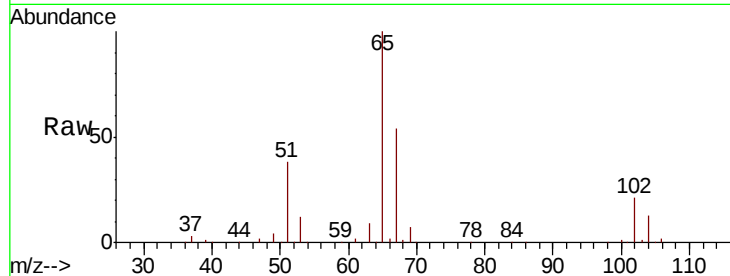

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2177
 Delta R.T. 0.00 min
 Lab File: VN050756.D
 Acq: 18 Aug 2018 7:02

Tgt Ion: 114 Resp: 1012162
 Ion Ratio Lower Upper
 114 100
 63 19.7 0.0 40.0
 88 15.1 0.0 30.8


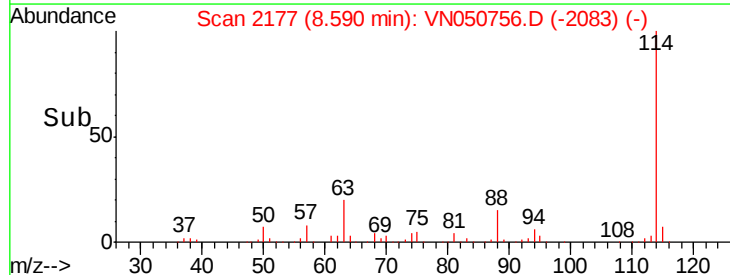
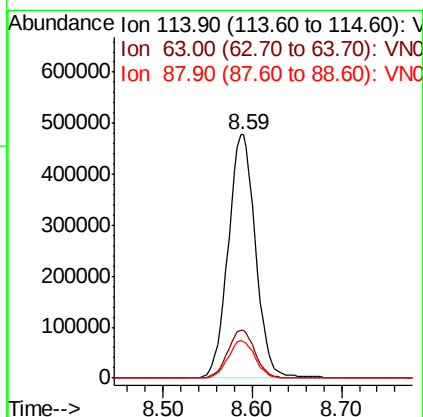





#35
 Dibromofluoromethane
 Concen: 48.18 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. 0.00 min
 Lab File: VN050756.D
 Acq: 18 Aug 2018 7:02




Instrument :
 MSVOA_N
 ClientSampleId :
 72-11990


Tot Ion	Ratio	Lower	Upper
113	100		
111	103.5	81.0	121.6
192	22.5	17.6	26.4

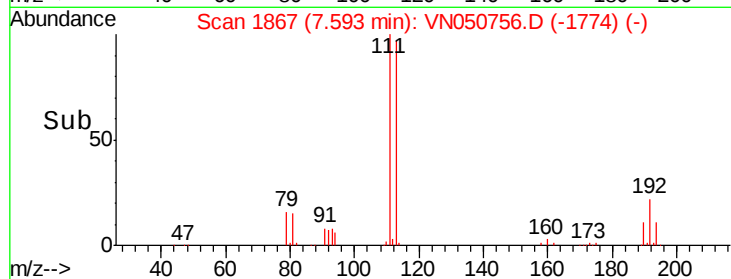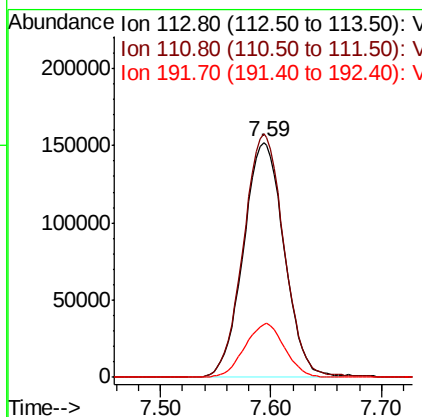

#36
 1,1-Dichloropropene
 Concen: 3.76 ug/l
 RT: 7.67 min Scan# 1890
 Delta R.T. -0.13 min
 Lab File: VN050756.D
 Acq: 18 Aug 2018 7:02

Tgt Ion	Ratio	Lower	Upper
75	100		
110	9.3	18.3	54.9#
77	0.0	25.0	37.4#



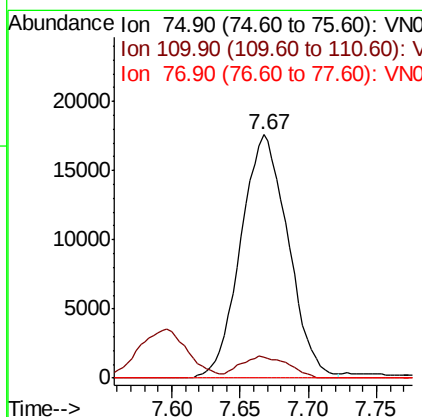





#38
Carbon Tetrachloride
Concen: 4.65 ug/l
RT: 7.67 min Scan# 1890
Delta R.T. -0.11 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02




Instrument :
MSVOA_N
ClientSampleId :
72-11990


Tot Ion:117 Resp: 54339
Ion Ratio Lower Upper
117 100
119 6.3 76.6 115.0#
121 0.0 25.0 37.6#

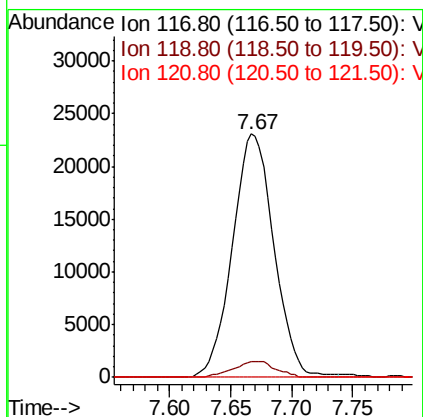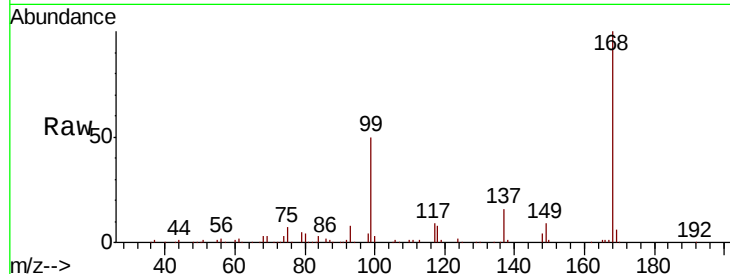

#43
Isopropyl Acetate
Concen: 19.53 ug/l
RT: 8.17 min Scan# 2046
Delta R.T. 0.00 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02

Tgt Ion: 43 Resp: 226647
Ion Ratio Lower Upper
43 100
61 19.1 16.2 24.2
87 12.8 10.9 16.3

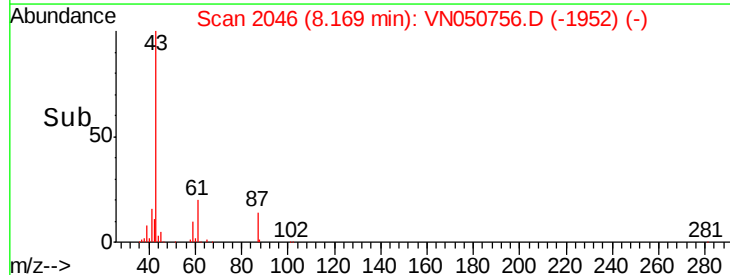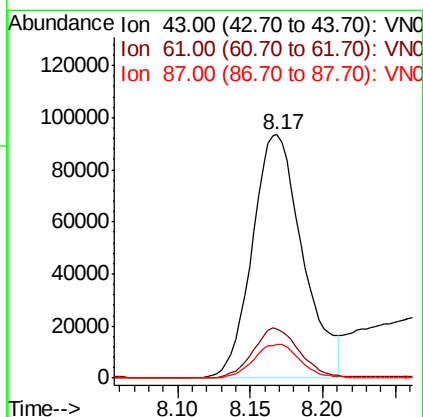

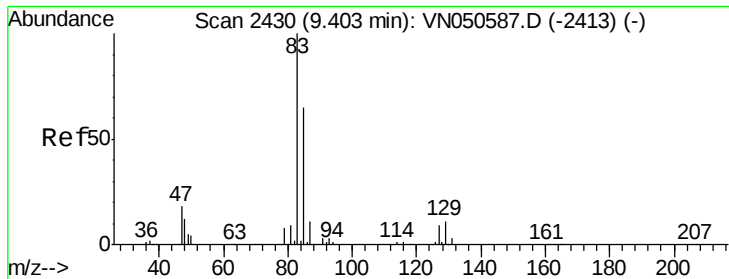

#47

Bromodichloromethane

Concen: 0.21 ug/l

RT: 9.41 min Scan# 2431

Delta R.T. 0.00 min

Lab File: VN050756.D

Acq: 18 Aug 2018 7:02

Instrument :

MSVOA_N

ClientSampleId :

72-11990


Tot Ion: 83 Resp: 2366

Ion Ratio Lower Upper

83 100

85 69.2 51.8 77.6

127 13.4 7.2 10.8#

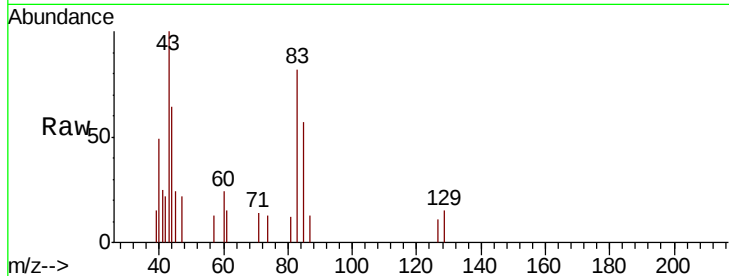


Abundance Ion 82.90 (82.60 to 83.60): VN050587.D (-2413) (-)

Ion 84.90 (84.60 to 85.60): VN050587.D (-2413) (-)

Ion 126.80 (126.50 to 127.50): VN050587.D (-2413) (-)

Time-->

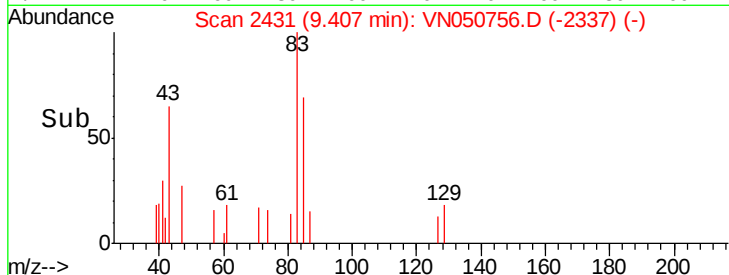


Abundance Ion 82.90 (82.60 to 83.60): VN050756.D (-2337) (-)

Ion 84.90 (84.60 to 85.60): VN050756.D (-2337) (-)

Ion 126.80 (126.50 to 127.50): VN050756.D (-2337) (-)

Time-->

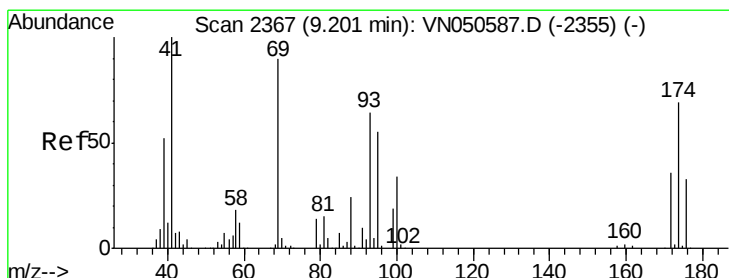

#48

Methyl methacrylate

Concen: 1.20 ug/l

RT: 9.19 min Scan# 2363

Delta R.T. -0.01 min

Lab File: VN050756.D

Acq: 18 Aug 2018 7:02


Tgt Ion: 41 Resp: 7021

Ion Ratio Lower Upper

41 100

69 0.0 73.4 110.0#

39 13.8 43.0 64.6#

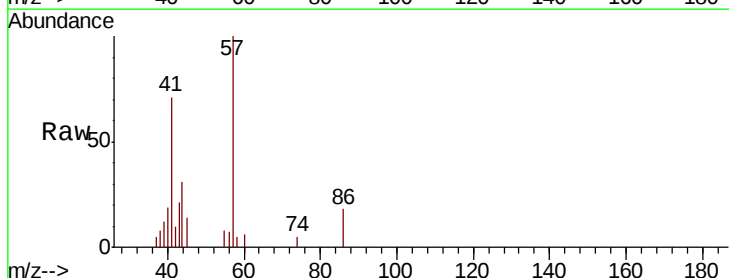


Abundance Ion 41.00 (40.70 to 41.70): VN050587.D (-2355) (-)

Ion 69.00 (68.70 to 69.70): VN050587.D (-2355) (-)

Ion 39.00 (38.70 to 39.70): VN050587.D (-2355) (-)

Time-->

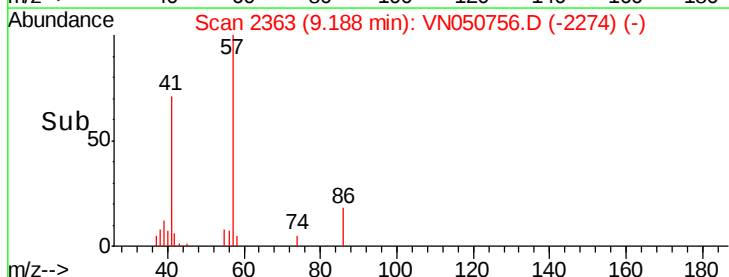


Abundance Ion 41.00 (40.70 to 41.70): VN050756.D (-2274) (-)

Ion 69.00 (68.70 to 69.70): VN050756.D (-2274) (-)

Ion 39.00 (38.70 to 39.70): VN050756.D (-2274) (-)

Time-->



#50

Toluene-d8

Concen: 46.48 ug/l

RT: 10.09 min Scan# 2644

Delta R.T. 0.00 min

Lab File: VN050756.D

Acq: 18 Aug 2018 7:02

Instrument :

MSVOA_N

ClientSampleId :


72-11990

Tot Ion: 98 Resp: 1413671

Ion Ratio Lower Upper

98 100

100 63.3 51.8 77.8

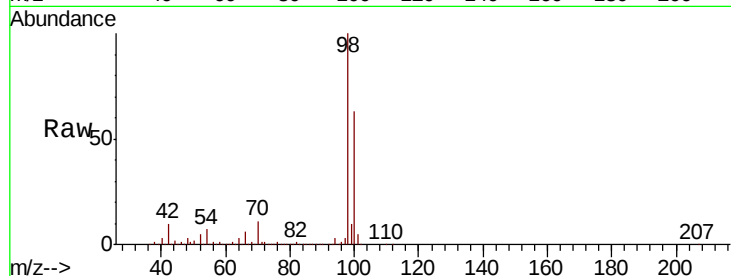

Abundance Ion 98.00 (97.70 to 98.70): VN050587.D (-2627) (-)

Ion 100.00 (99.70 to 100.70): VN050587.D (-2627) (-)

10.09

800000



600000

400000

200000

0

Time-->



#51

4-Methyl-2-Pentanone

Concen: 0.30 ug/l

RT: 9.99 min Scan# 2611

Delta R.T. 0.00 min

Lab File: VN050756.D


Acq: 18 Aug 2018 7:02

Tgt Ion: 43 Resp: 2362

Ion Ratio Lower Upper

43 100

58 26.7 32.5 48.7#



Abundance Ion 43.00 (42.70 to 43.70): VN050587.D (-2591) (-)

Ion 58.00 (57.70 to 58.70): VN050587.D (-2591) (-)

9.99

2500

2000


1500


1000

500

0

Time-->





#56

Ethyl methacrylate

Concen: 2.00 ug/l

RT: 10.22 min Scan# 2685

Delta R.T. -0.20 min

Lab File: VN050756.D

Acq: 18 Aug 2018 7:02

Instrument :

MSVOA_N

ClientSampled :

72-11990


Tot Ion: 69 Resp: 944

Ion Ratio Lower Upper

69 100

41 111.8 49.7 74.5#




39 82.6 24.2 36.2#

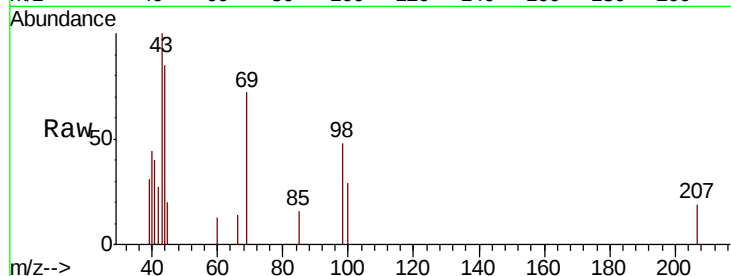

Abundance Ion 69.00 (68.70 to 69.70): VN0

Ion 41.00 (40.70 to 41.70): VN0

Ion 39.00 (38.70 to 39.70): VN0

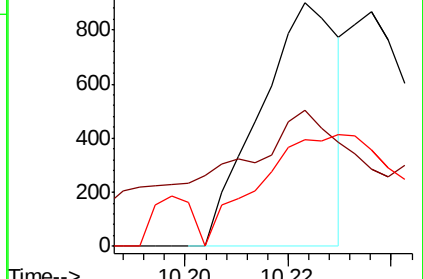

#59

2-Hexanone

Concen: 2.99 ug/l

RT: 10.76 min Scan# 2853

Delta R.T. 0.01 min

Lab File: VN050756.D


Acq: 18 Aug 2018 7:02

Tgt Ion: 43 Resp: 15161

Ion Ratio Lower Upper



43 100


58 25.5 28.0 84.0#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

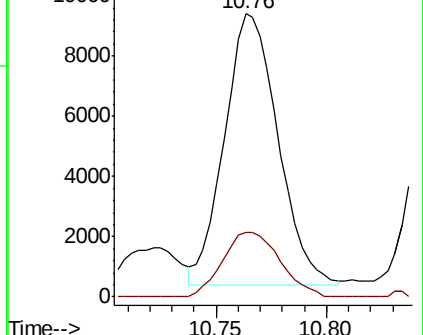

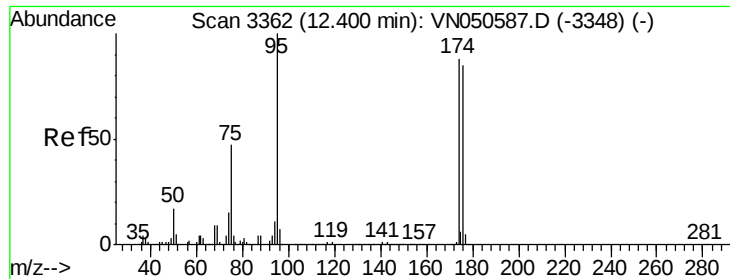

#62

4-Bromofluorobenzene

Concen: 38.51 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.00 min

Lab File: VN050756.D

Acq: 18 Aug 2018 7:02

Instrument :

MSVOA_N

ClientSampleId :

72-11990


Tot Ion: 95 Resp: 386908

Ion Ratio Lower Upper

95 100

174 91.2 0.0 177.8

176 87.7 0.0 175.0




Abundance Ion 94.90 (94.60 to 95.60): VN050587.D (-3348) (-)

Ion 173.80 (173.50 to 174.50): VN050587.D (-3348) (-)

Ion 175.80 (175.50 to 176.50): VN050587.D (-3348) (-)

12.40

Time-->




Abundance Ion 94.90 (94.60 to 95.60): VN050756.D (-3269) (-)

Ion 173.80 (173.50 to 174.50): VN050756.D (-3269) (-)

Ion 175.80 (175.50 to 176.50): VN050756.D (-3269) (-)

12.40

Time-->



#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 11.41 min Scan# 3054

Delta R.T. 0.00 min

Lab File: VN050756.D

Acq: 18 Aug 2018 7:02


Tgt Ion: 117 Resp: 894334

Ion Ratio Lower Upper

117 100

82 52.9 42.4 63.6

119 32.1 25.8 38.8




Abundance Ion 116.90 (116.60 to 117.60): VN050587.D (-3038) (-)

Ion 82.00 (81.70 to 82.70): VN050587.D (-3038) (-)

Ion 118.90 (118.60 to 119.60): VN050587.D (-3038) (-)

11.41

Time-->




Abundance Ion 116.90 (116.60 to 117.60): VN050756.D (-2961) (-)

Ion 82.00 (81.70 to 82.70): VN050756.D (-2961) (-)

Ion 118.90 (118.60 to 119.60): VN050756.D (-2961) (-)

11.41


Time-->

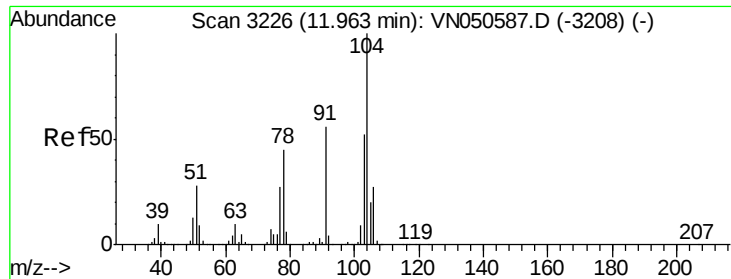




#70
Stvrene
Concen: 0.95 ug/l
RT: 11.97 min Scan# 3227
Delta R.T. 0.00 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02

Instrument :
MSVOA_N
ClientSampled :
72-11990

Tot Ion	Ratio	Lower	Upper
104	100		
78	0.0	39.1	58.7#
103	0.0	44.9	67.3#




Abundance Ion 104.00 (103.70 to 104.70): V
Ion 78.00 (77.70 to 78.70): V
Ion 103.00 (102.70 to 103.70): V


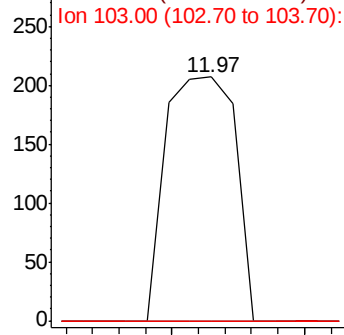



#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.35 min Scan# 3656
Delta R.T. 0.00 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02

Tgt Ion	Ratio	Lower	Upper
152	100		
115	56.8	28.1	84.2
150	157.8	0.0	347.8



Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

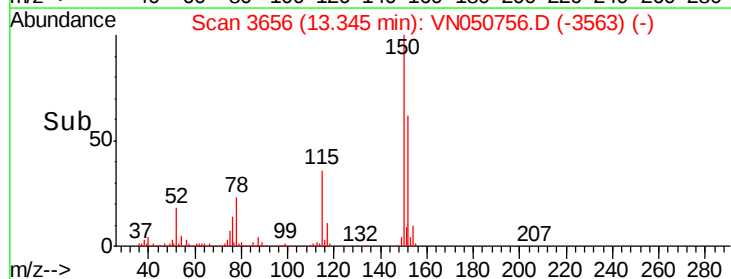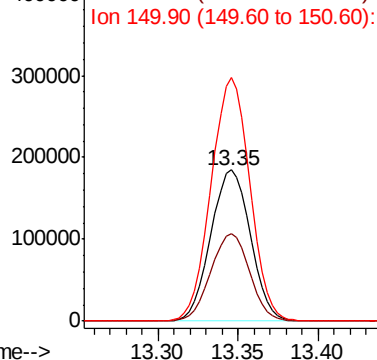



#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.40 min Scan# 3362

Delta R.T. -0.10 min

Lab File: VN050756.D

Acq: 18 Aug 2018 7:02

Instrument :

MSVOA_N

ClientSampleId :

72-11990


Tot Ion: 83 Resp: 117

Ion Ratio Lower Upper

83 100

131 368.4 5.3 15.9#




85 0.0 32.1 96.5#



Abundance Ion 82.90 (82.60 to 83.60): VNO

Ion 130.80 (130.50 to 131.50): VNO

Ion 84.90 (84.60 to 85.60): VNO

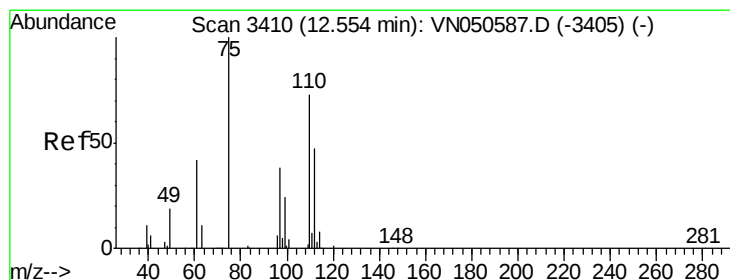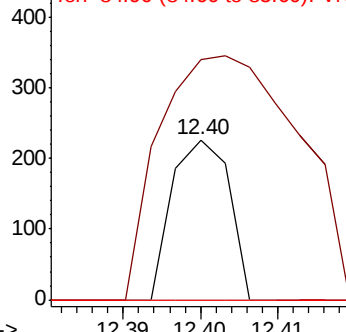

#76

1,2,3-Trichloropropane

Concen: 36.60 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. -0.15 min

Lab File: VN050756.D


Acq: 18 Aug 2018 7:02

Tgt Ion: 75 Resp: 186490

Ion Ratio Lower Upper



75 100


77 1.2 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VNO

Ion 77.00 (76.70 to 77.70): VNO




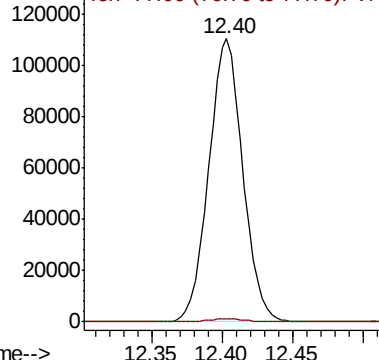




#81
trans-1,4-Dichloro-2-butene
Concen: 132.44 ug/l
RT: 12.40 min Scan# 3363
Delta R.T. 0.10 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02

Instrument :
MSVOA_N
ClientSampled :
72-11990

Tot Ion: 75 Resp: 186490
Ion Ratio Lower Upper
75 100
53 0.2 72.2 108.2#
89 0.0 36.3 54.5#

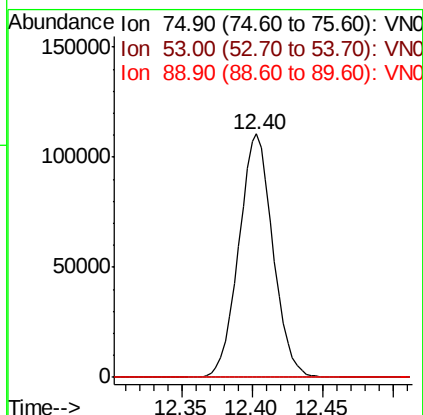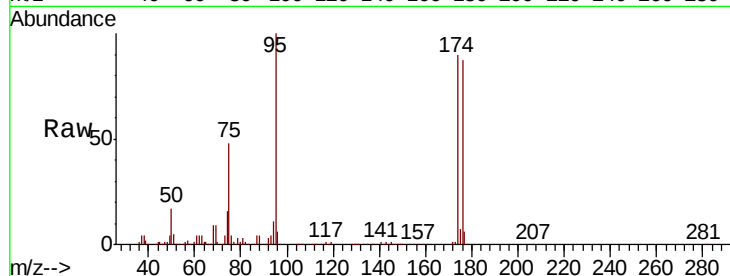

#95
Naphthalene
Concen: 6.20 ug/l
RT: 15.14 min Scan# 4213
Delta R.T. 0.00 min
Lab File: VN050756.D
Acq: 18 Aug 2018 7:02

Tgt Ion:128 Resp: 30517
Ion Ratio Lower Upper
128 100
127 12.8 10.3 15.5
129 11.2 8.5 12.7

