

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN081718\
 Data File : VN050727.D
 Acq On : 17 Aug 2018 13:58
 Operator : MD\SY
 Sample : PB112140ZHE#01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB112140ZHE#01

Quant Time: Aug 18 00:19:19 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 14 08:07:08 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	619885	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1012799	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	870750	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	310406	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	420996	53.88	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.76%	
35) Dibromofluoromethane	7.59	113	393095	48.62	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.24%	
50) Toluene-d8	10.09	98	1390814	45.70	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.40%	
62) 4-Bromofluorobenzene	12.40	95	381571	37.95	ug/l	0.00
Spiked Amount 50.000			Recovery	=	75.90%	
Target Compounds						
16) Acetone	3.83	43	24614	11.23	ug/l	94
18) Methyl Acetate	4.33	43	12190	1.25	ug/l	93
20) Methylene Chloride	4.55	84	21498	1.67	ug/l	88
43) Isopropyl Acetate	8.17	43	241051	20.76	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN081718\
Data File : VN050727.D
Acq On : 17 Aug 2018 13:58
Operator : MD\SY
Sample : PB112140ZHE#01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB112140ZHE#01

Quant Time: Aug 18 00:19:19 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 14 08:07:08 2018
Response via : Initial Calibration

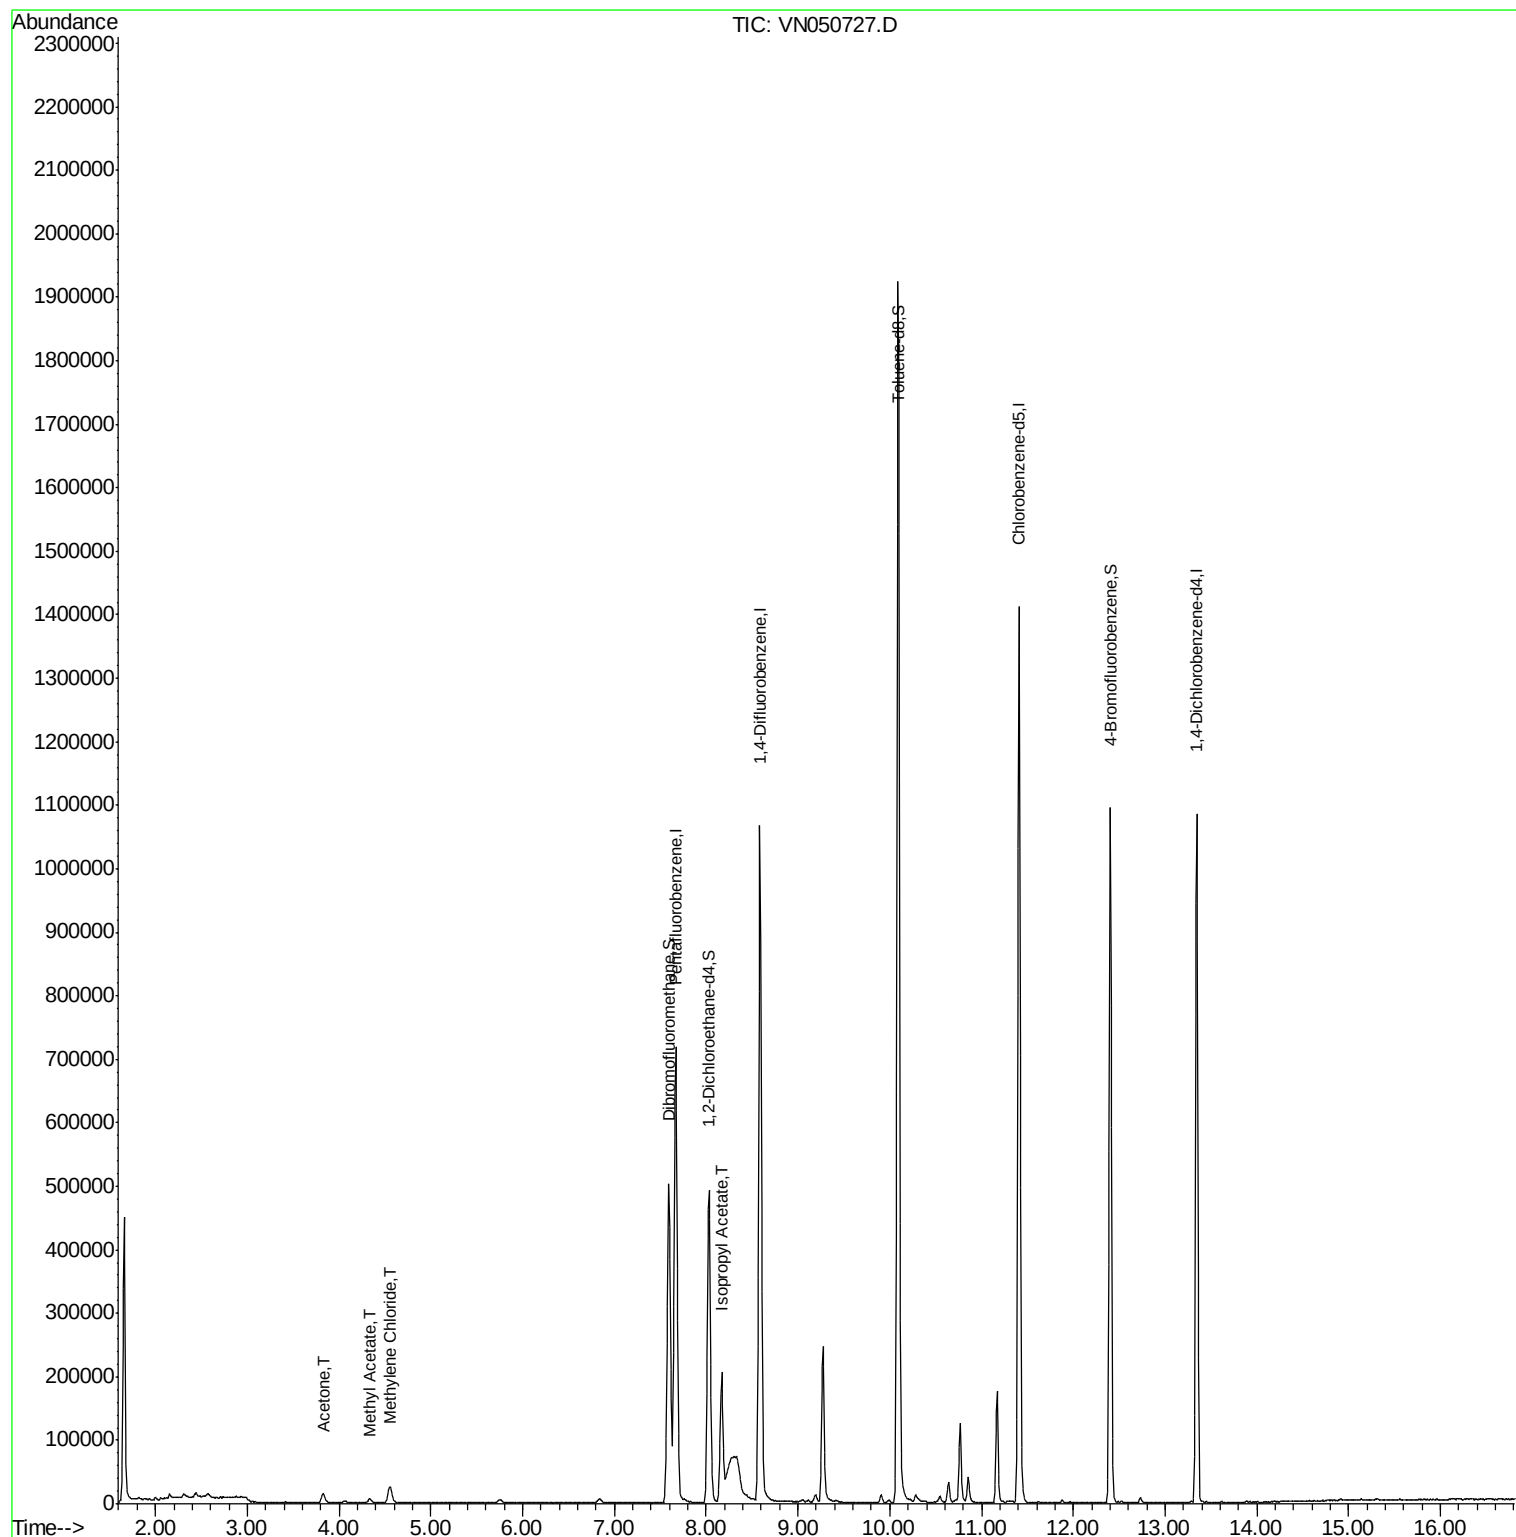

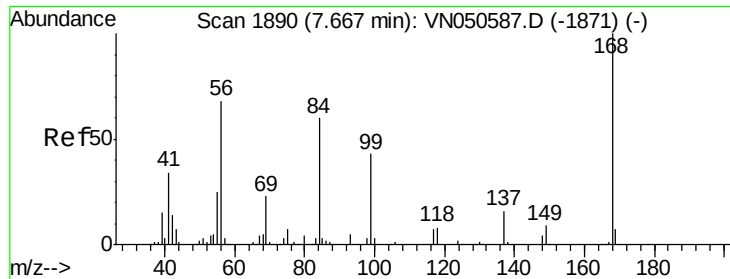

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1891

Delta R.T. 0.00 min

Lab File: VN050727.D

Acq: 17 Aug 2018 13:58

Instrument :

MSVOA_N

ClientSampleId :


PB112140ZHE#01

Tot Ion:168 Resp: 619885

Ion Ratio Lower Upper

168 100

99 49.8 40.8 61.2

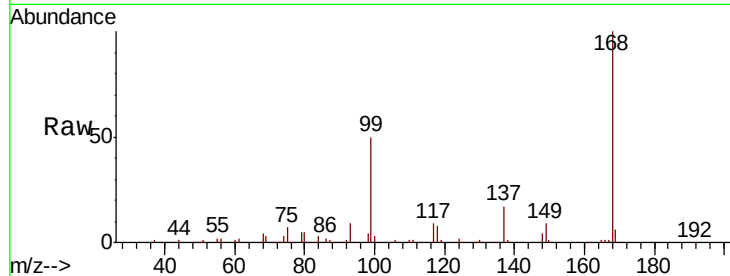

Abundance Ion 167.90 (167.60 to 168.60): VN050727.D (-1797) (-)

Ion 98.90 (98.60 to 99.60): VN050727.D (-1797) (-)

7.67

250000

200000



150000

100000

50000

0

Time-->

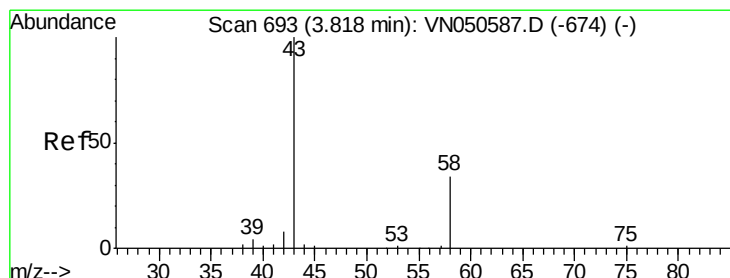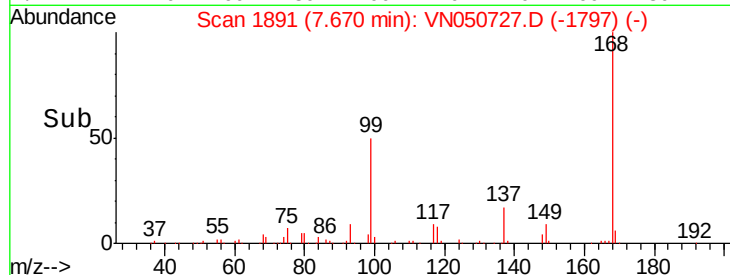

#16

Acetone

Concen: 11.23 ug/l

RT: 3.83 min Scan# 697

Delta R.T. 0.01 min

Lab File: VN050727.D


Acq: 17 Aug 2018 13:58

Tgt Ion: 43 Resp: 24614

Ion Ratio Lower Upper

43 100

58 37.3 27.1 40.7

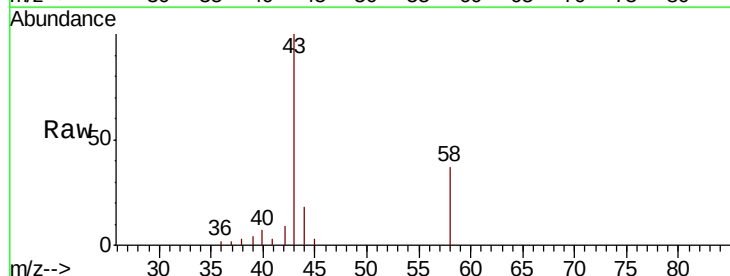

Abundance Ion 43.00 (42.70 to 43.70): VN050727.D (-600) (-)

Ion 58.00 (57.70 to 58.70): VN050727.D (-600) (-)

3.83

10000

8000


6000


4000

2000

0

Time-->




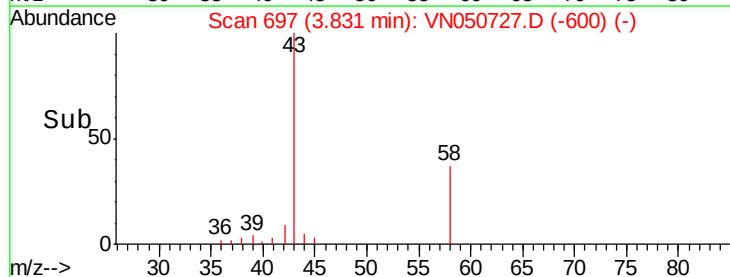


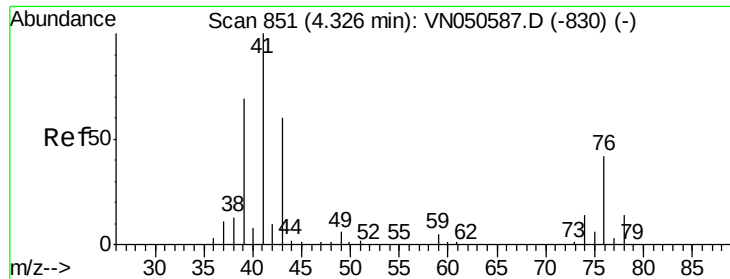

#18
Methvl Acetate
Concen: 1.25 ug/l
RT: 4.33 min Scan# 853
Delta R.T. 0.01 min
Lab File: VN050727.D
Acq: 17 Aug 2018 13:58




Instrument :
MSVOA_N
ClientSampleId :
PB112140ZHE#01


Tot Ion: 43 Resp: 12190
Ion Ratio Lower Upper
43 100
74 21.1 19.7 29.5

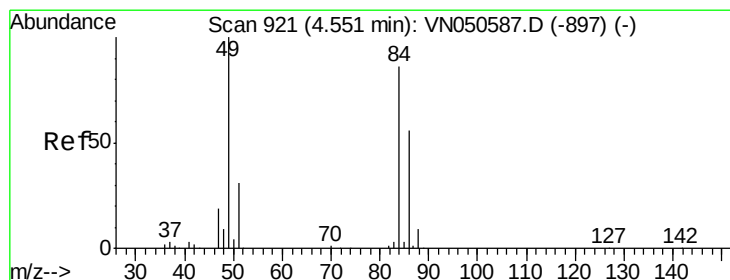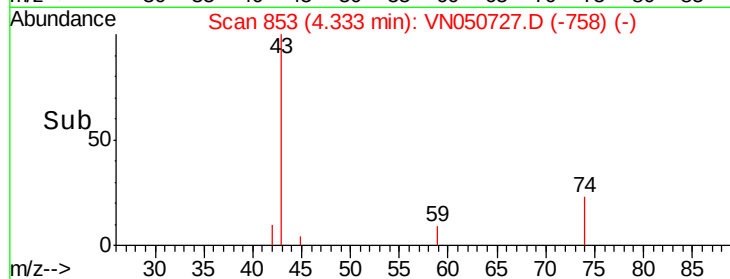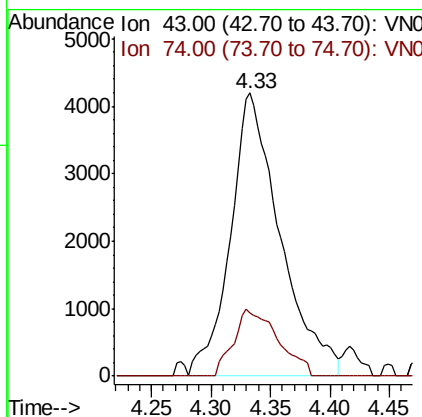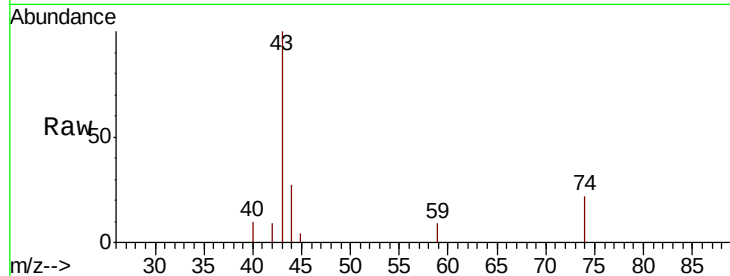

#20
Methylene Chloride
Concen: 1.67 ug/l
RT: 4.55 min Scan# 921
Delta R.T. 0.00 min
Lab File: VN050727.D
Acq: 17 Aug 2018 13:58

Tgt Ion: 84 Resp: 21498
Ion Ratio Lower Upper
84 100
49 100.2 92.6 138.8
51 31.6 28.6 43.0
86 58.1 52.2 78.2


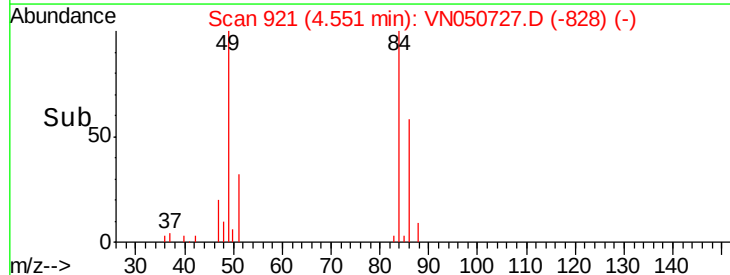
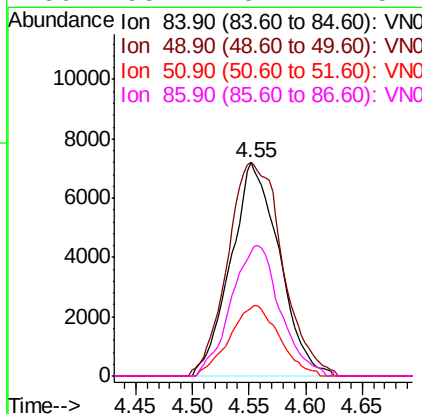
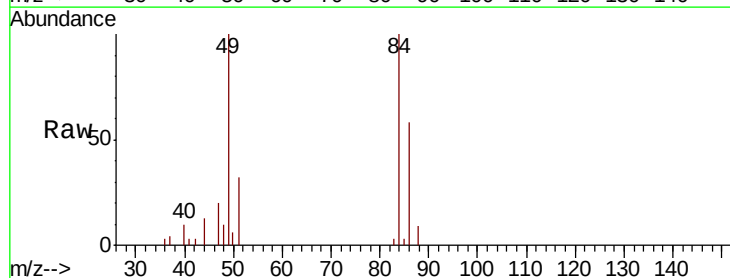


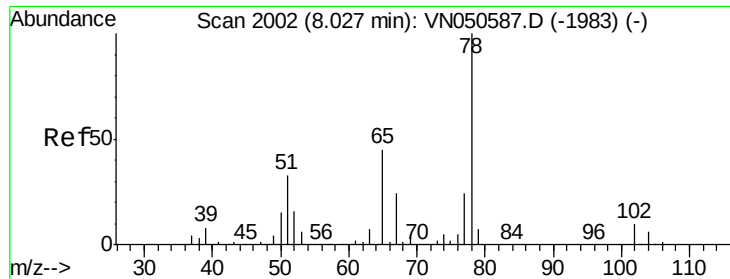

#33
 1,2-Dichloroethane-d4
 Concen: 53.88 ug/l
 RT: 8.03 min Scan# 2003
 Delta R.T. 0.00 min
 Lab File: VN050727.D
 Acq: 17 Aug 2018 13:58




Instrument :
 MSVOA_N
 ClientSampleId :
 PB112140ZHE#01


Tot Ion: 65 Resp: 420996
 Ion Ratio Lower Upper
 65 100
 67 54.4 0.0 109.8

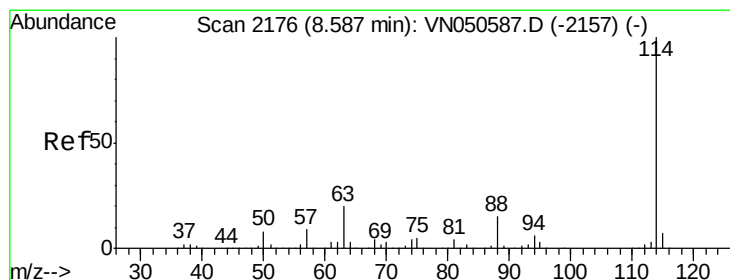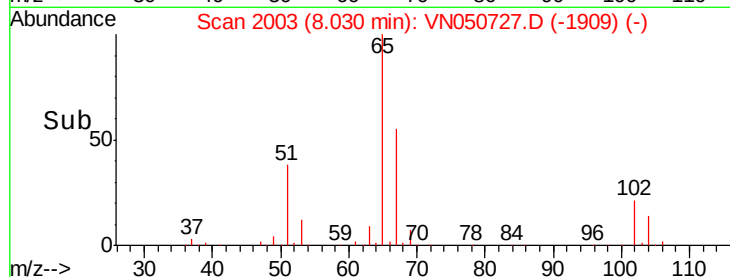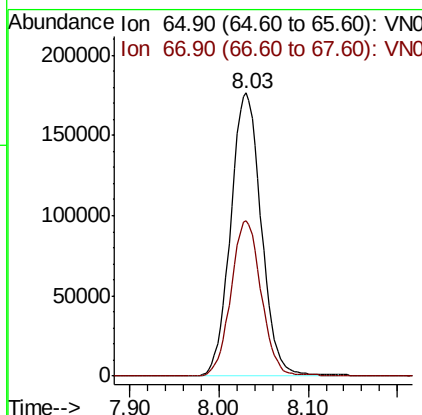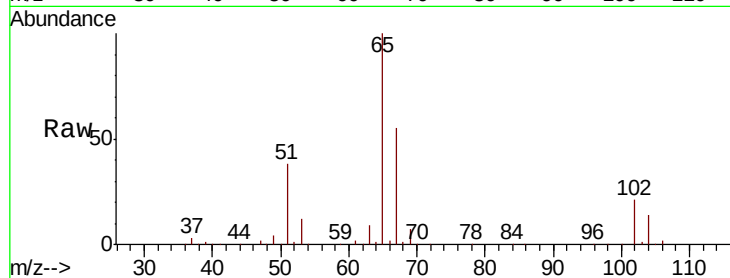

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2176
 Delta R.T. 0.00 min
 Lab File: VN050727.D
 Acq: 17 Aug 2018 13:58

Tgt Ion: 114 Resp: 1012799
 Ion Ratio Lower Upper
 114 100
 63 19.9 0.0 40.0
 88 15.8 0.0 30.8


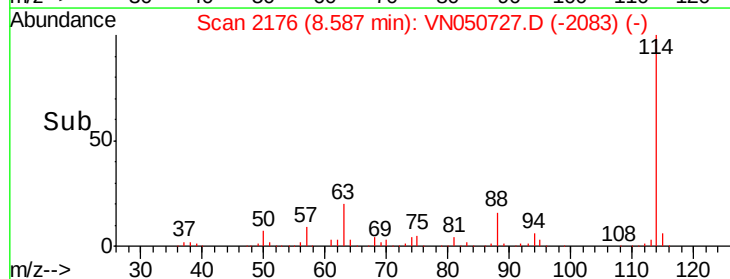
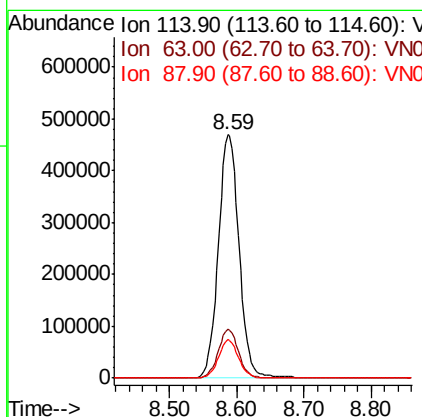
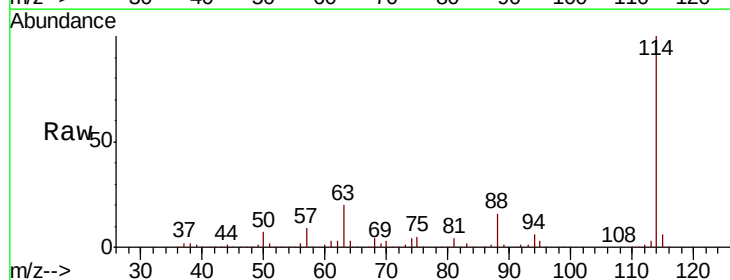


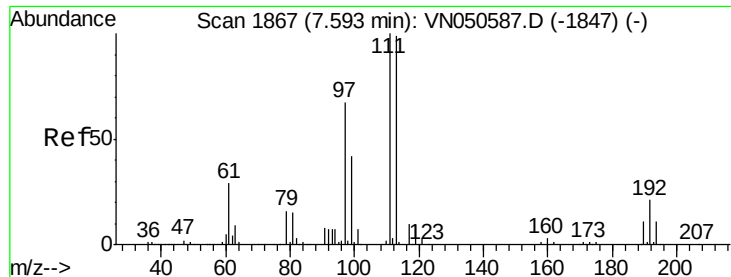

#35
 Dibromofluoromethane
 Concen: 48.62 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. 0.00 min
 Lab File: VN050727.D
 Acq: 17 Aug 2018 13:58




Instrument :
 MSVOA_N
 ClientSampleId :
 PB112140ZHE#01


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.3	81.0	121.6
192	21.9	17.6	26.4

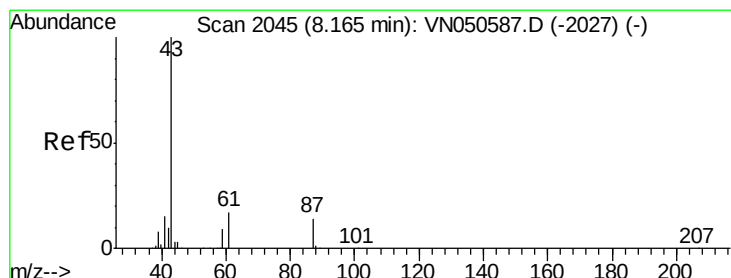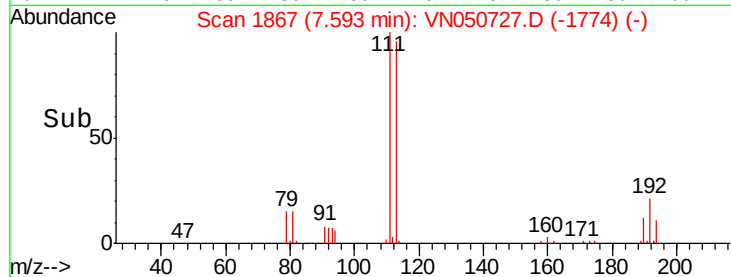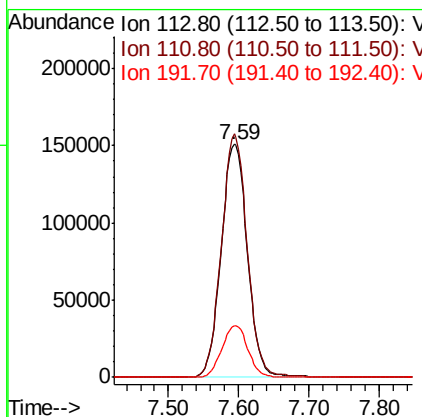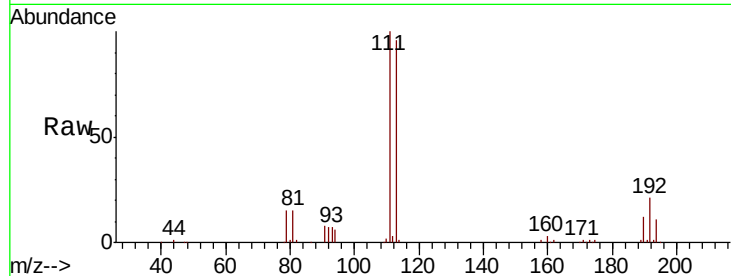

#43
 Isopropyl Acetate
 Concen: 20.76 ug/l
 RT: 8.17 min Scan# 2046
 Delta R.T. 0.00 min
 Lab File: VN050727.D
 Acq: 17 Aug 2018 13:58

Tgt Ion	Ratio	Lower	Upper
43	100		
61	20.2	16.2	24.2
87	13.2	10.9	16.3

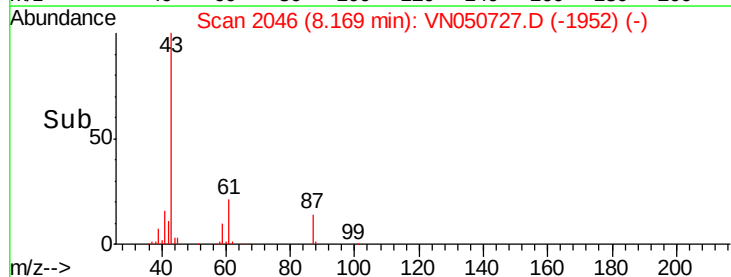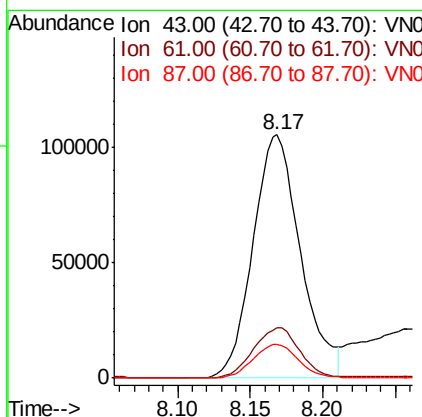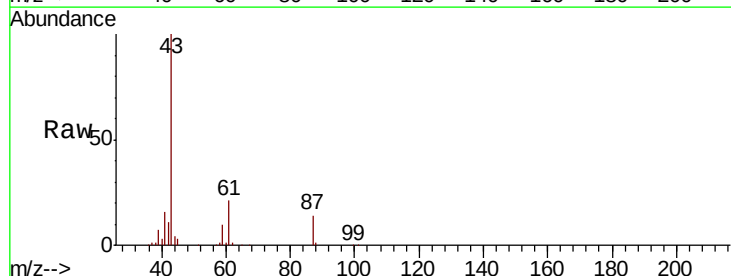

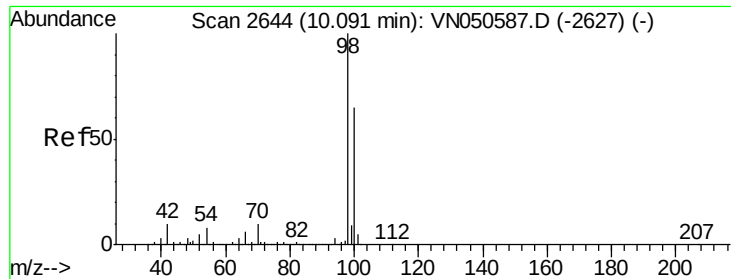

#50

Toluene-d8

Concen: 45.70 ug/l

RT: 10.09 min Scan# 2644

Delta R.T. 0.00 min

Lab File: VN050727.D

Acq: 17 Aug 2018 13:58

Instrument :

MSVOA_N

ClientSampleId :





PB112140ZHE#01

Tot Ion: 98 Resp: 1390814

Ion Ratio Lower Upper

98 100

100 64.1 51.8 77.8

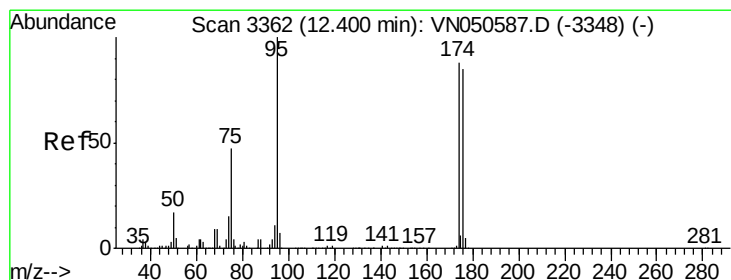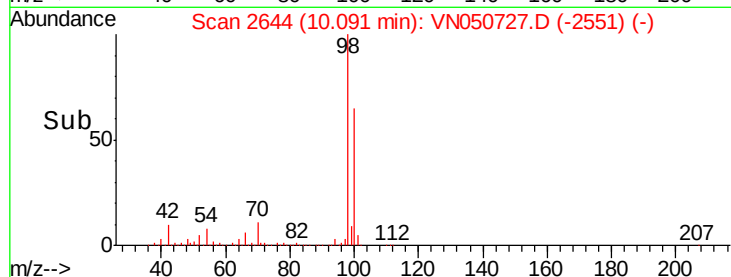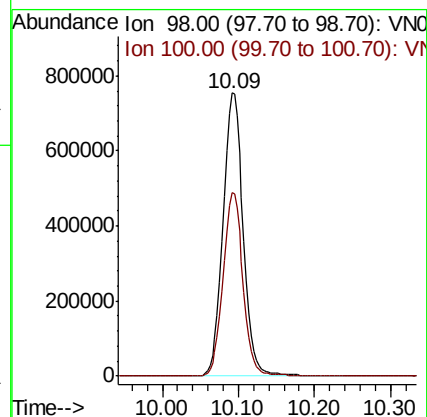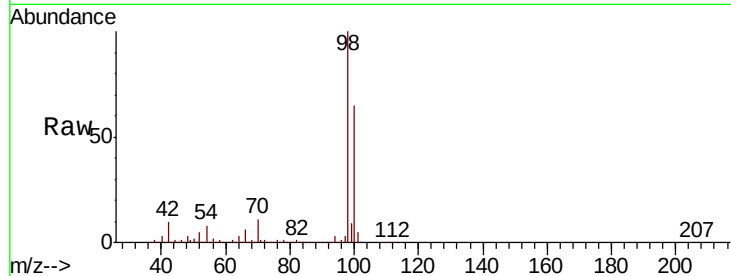

#62

4-Bromofluorobenzene

Concen: 37.95 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.00 min

Lab File: VN050727.D

Acq: 17 Aug 2018 13:58




Tgt Ion: 95 Resp: 381571


Ion Ratio Lower Upper

95 100

174 90.5 0.0 177.8

176 87.1 0.0 175.0

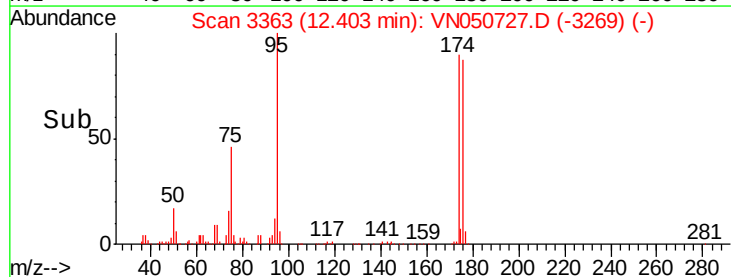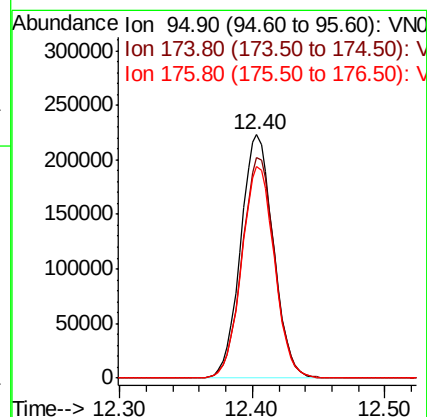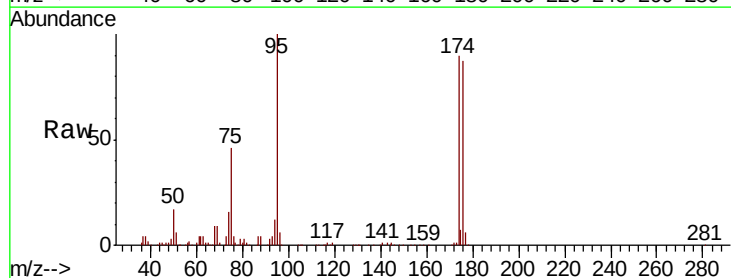

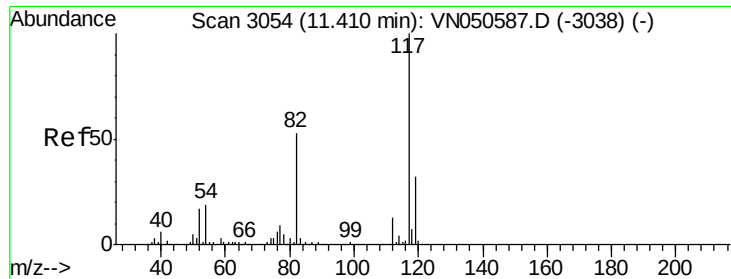

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 11.41 min Scan# 3054

Delta R.T. 0.00 min

Lab File: VN050727.D

Acq: 17 Aug 2018 13:58

Instrument :

MSVOA_N

ClientSampleId :

PB112140ZHE#01


Tot Ion:117 Resp: 870750

Ion Ratio Lower Upper

117 100

82 53.7 42.4 63.6




119 32.4 25.8 38.8

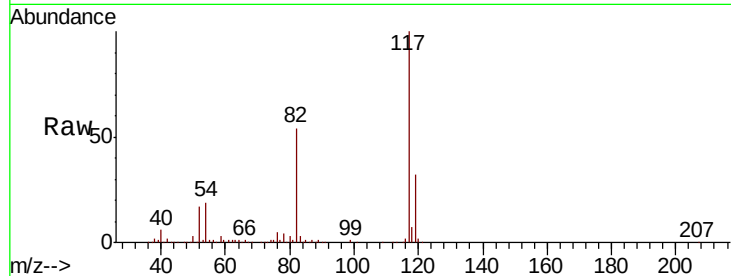

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): V

Ion 118.90 (118.60 to 119.60): V

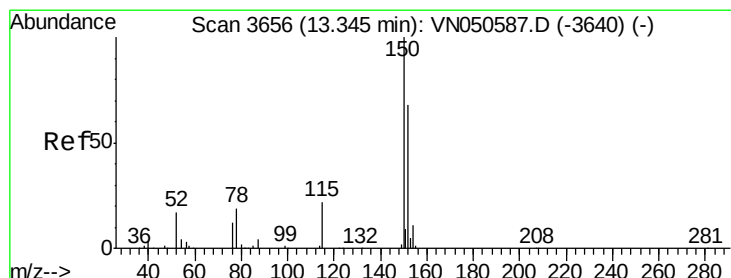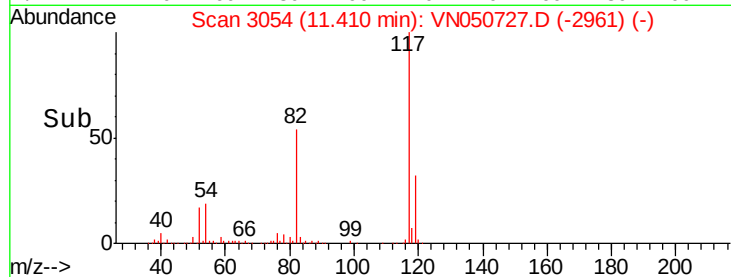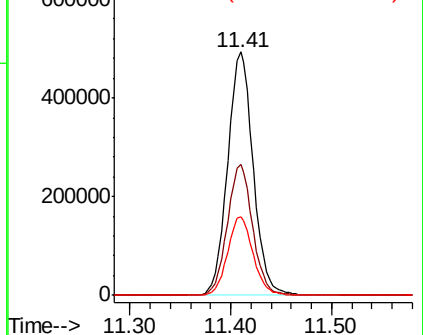

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.35 min Scan# 3656

Delta R.T. 0.00 min

Lab File: VN050727.D

Acq: 17 Aug 2018 13:58


Tgt Ion:152 Resp: 310406

Ion Ratio Lower Upper

152 100

115 56.3 28.1 84.2

150 155.8 0.0 347.8

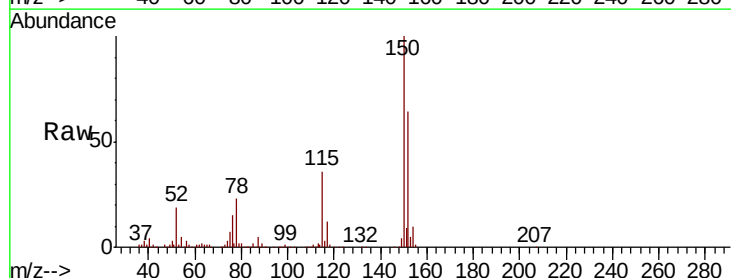

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

