


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081718\
 Data File : VN050714.D
 Acq On : 17 Aug 2018 7:25
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N072518W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Jul 26 15:21:50 2018

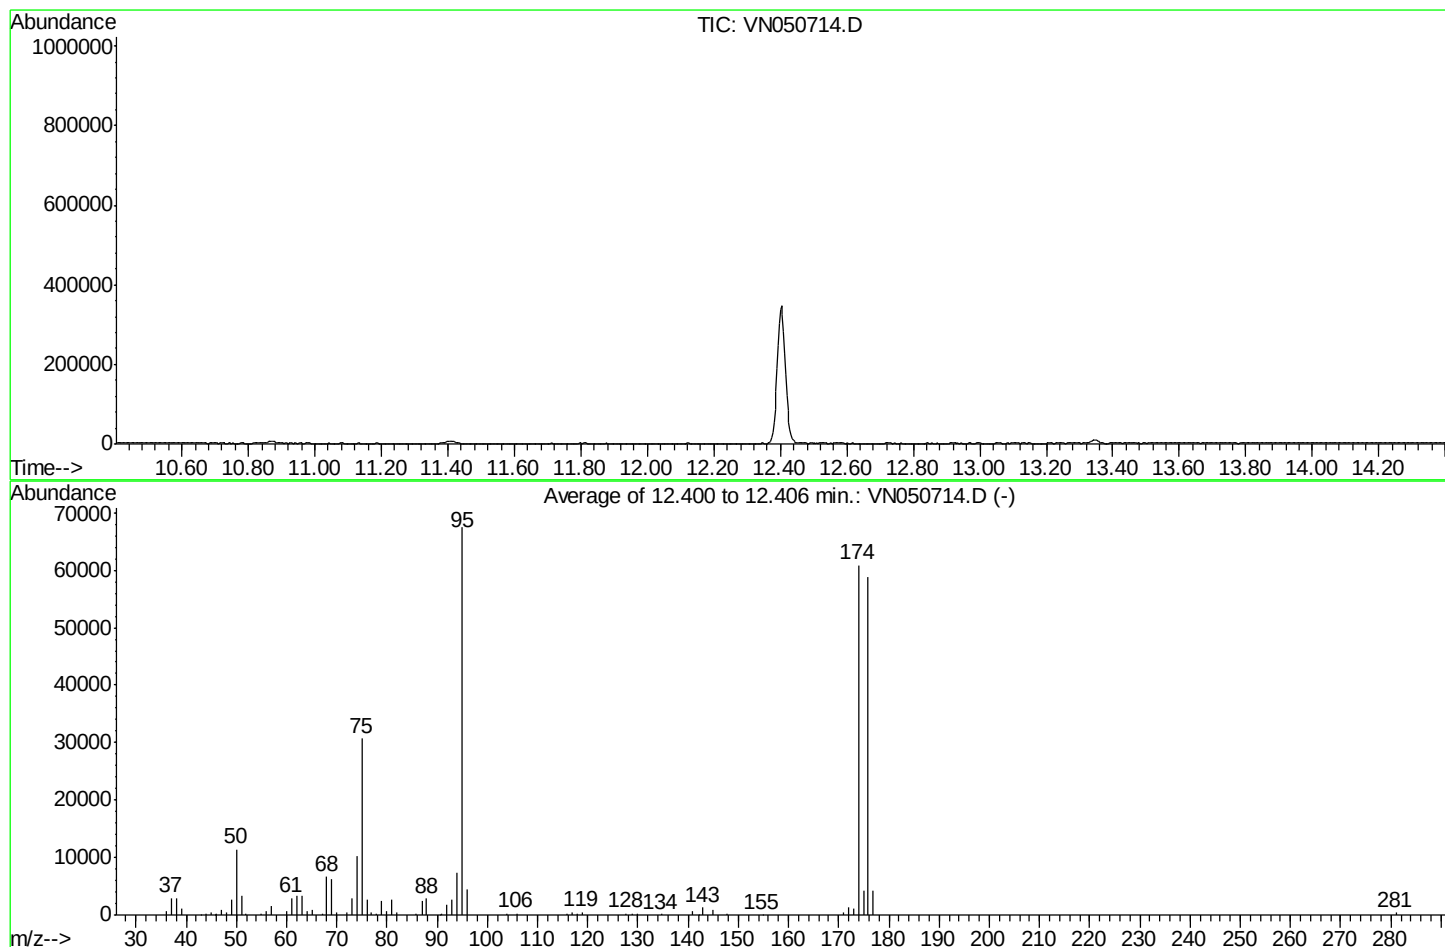

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	11414	PASS
75	95	30	60	45.6	30736	PASS
95	95	100	100	100.0	67461	PASS
96	95	5	9	6.7	4491	PASS
173	174	0.00	2	1.8	1091	PASS
174	95	50	100	90.2	60834	PASS
175	174	5	9	7.1	4328	PASS
176	174	95	101	96.6	58776	PASS
177	176	5	9	7.3	4298	PASS