


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081719\
Data File : VN057345.D
Acq On : 16 Aug 2019 9:21
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N081719W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Aug 16 15:42:00 2019

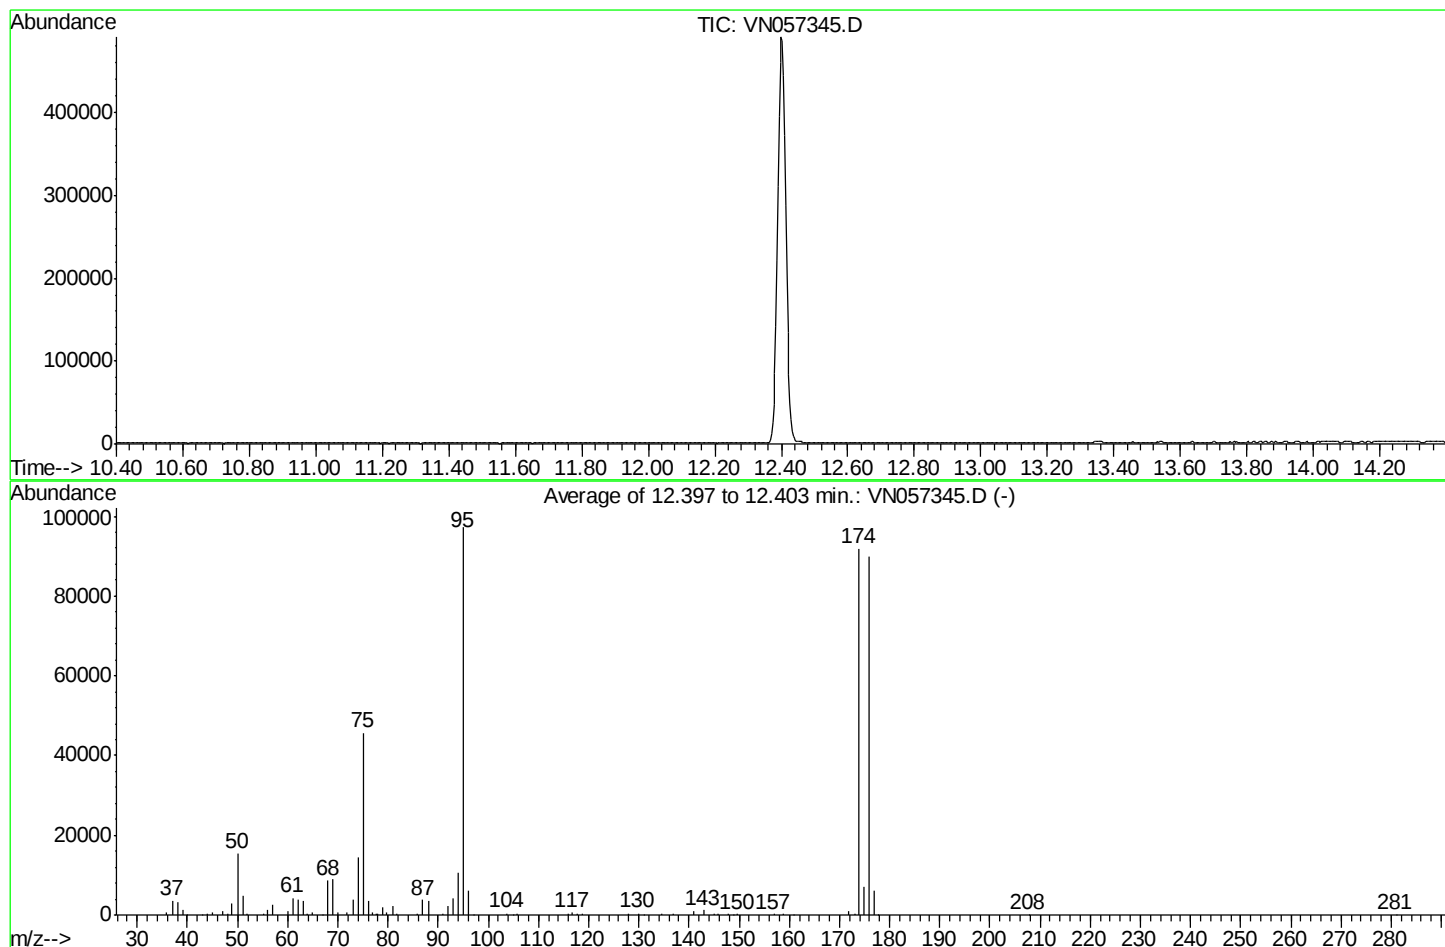

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	15280	PASS
75	95	30	60	46.9	45594	PASS
95	95	100	100	100.0	97237	PASS
96	95	5	9	6.3	6082	PASS
173	174	0.00	2	0.4	349	PASS
174	95	50	100	94.5	91930	PASS
175	174	5	9	7.8	7167	PASS
176	174	95	101	97.8	89941	PASS
177	176	5	9	6.6	5978	PASS