



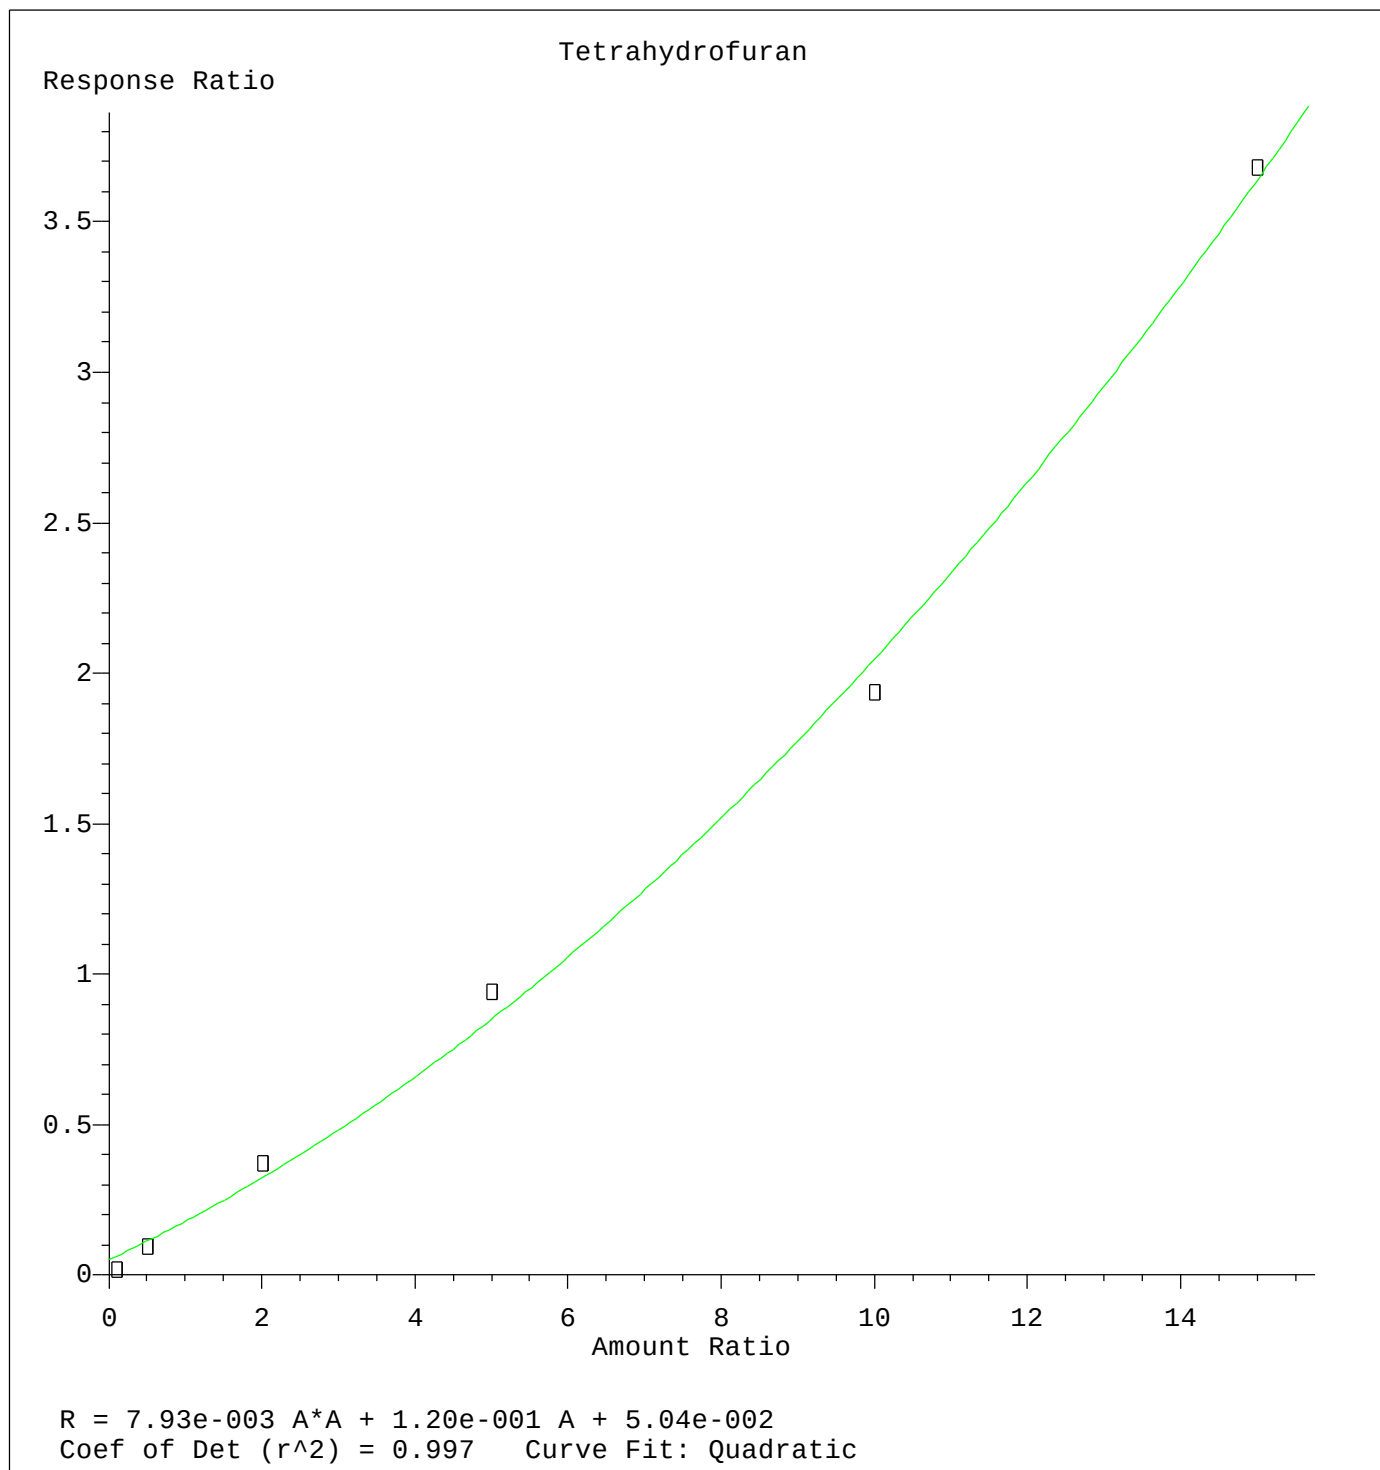


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081720W.M
Calibration Table Last Updated: Mon Aug 17 17:31:03 2020

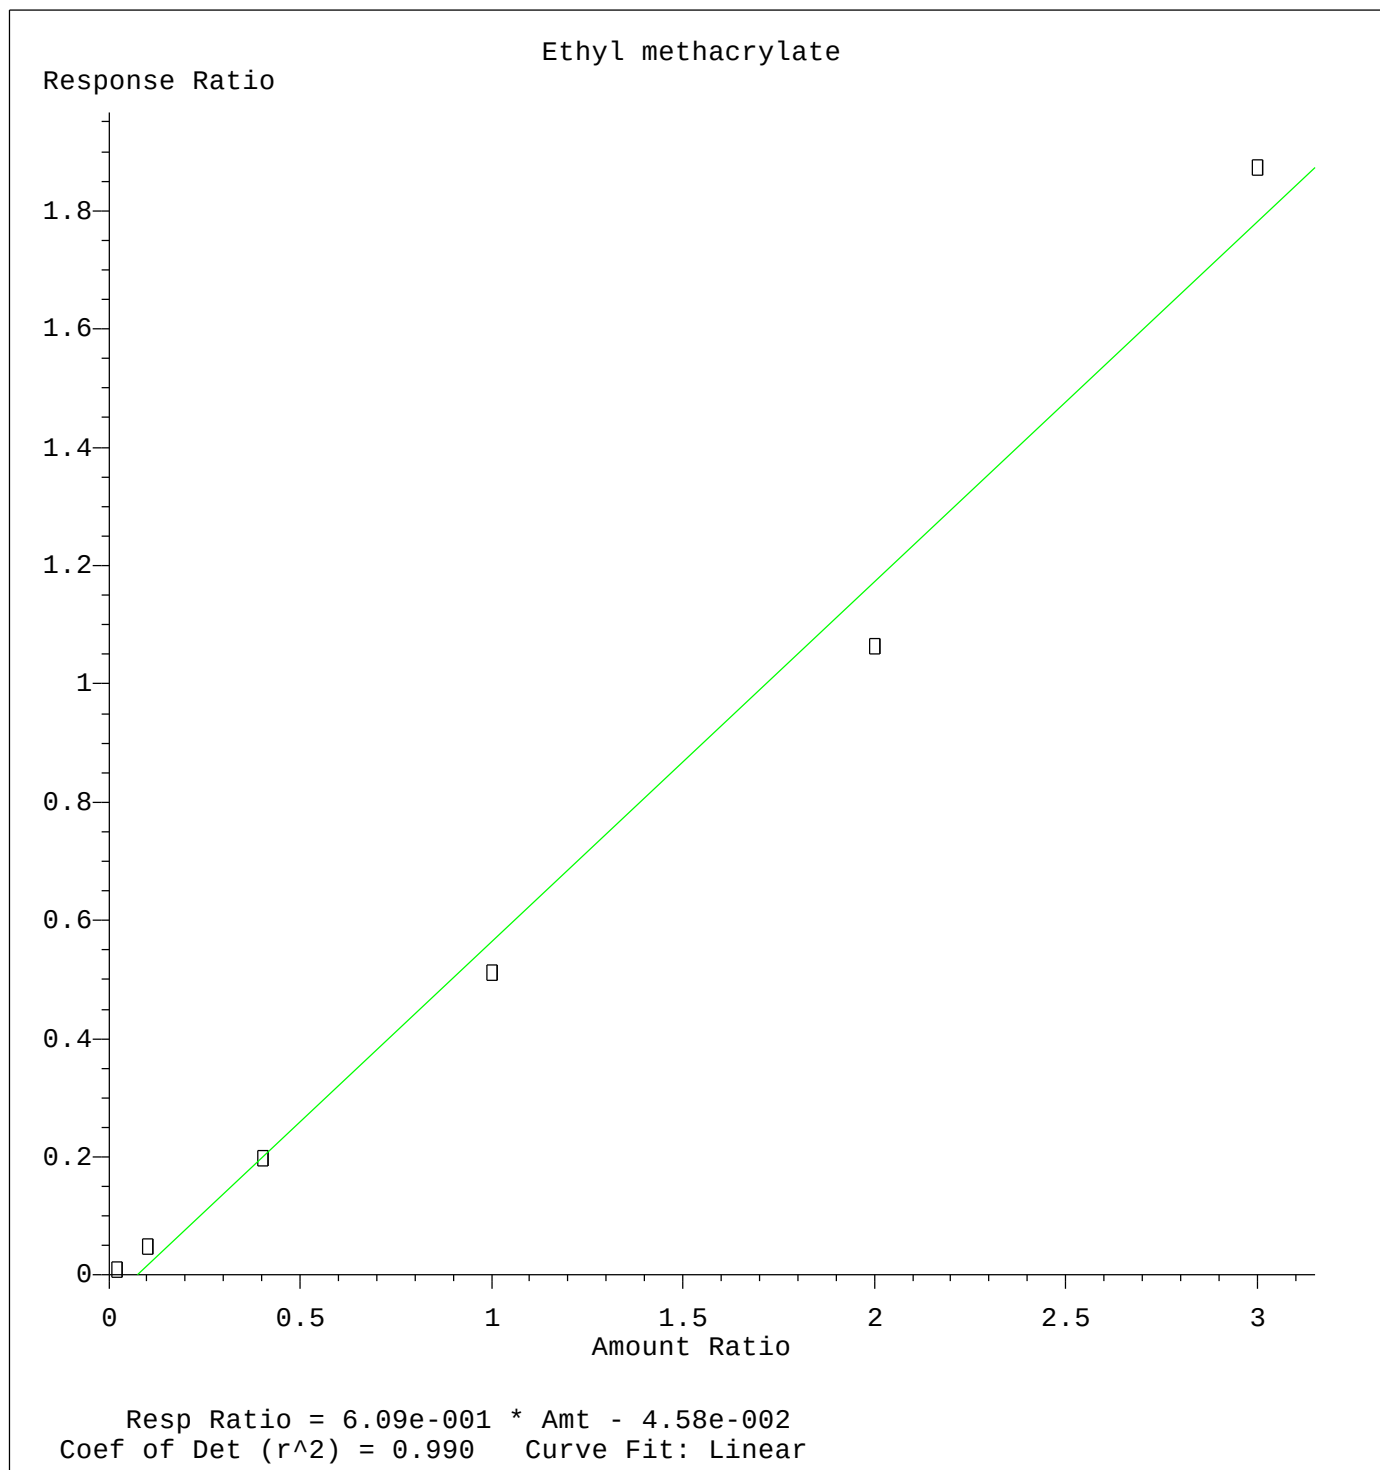

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081720W.M
Calibration Table Last Updated: Mon Aug 17 17:31:03 2020

2-Chloroethyl Vinyl ether

Response Ratio

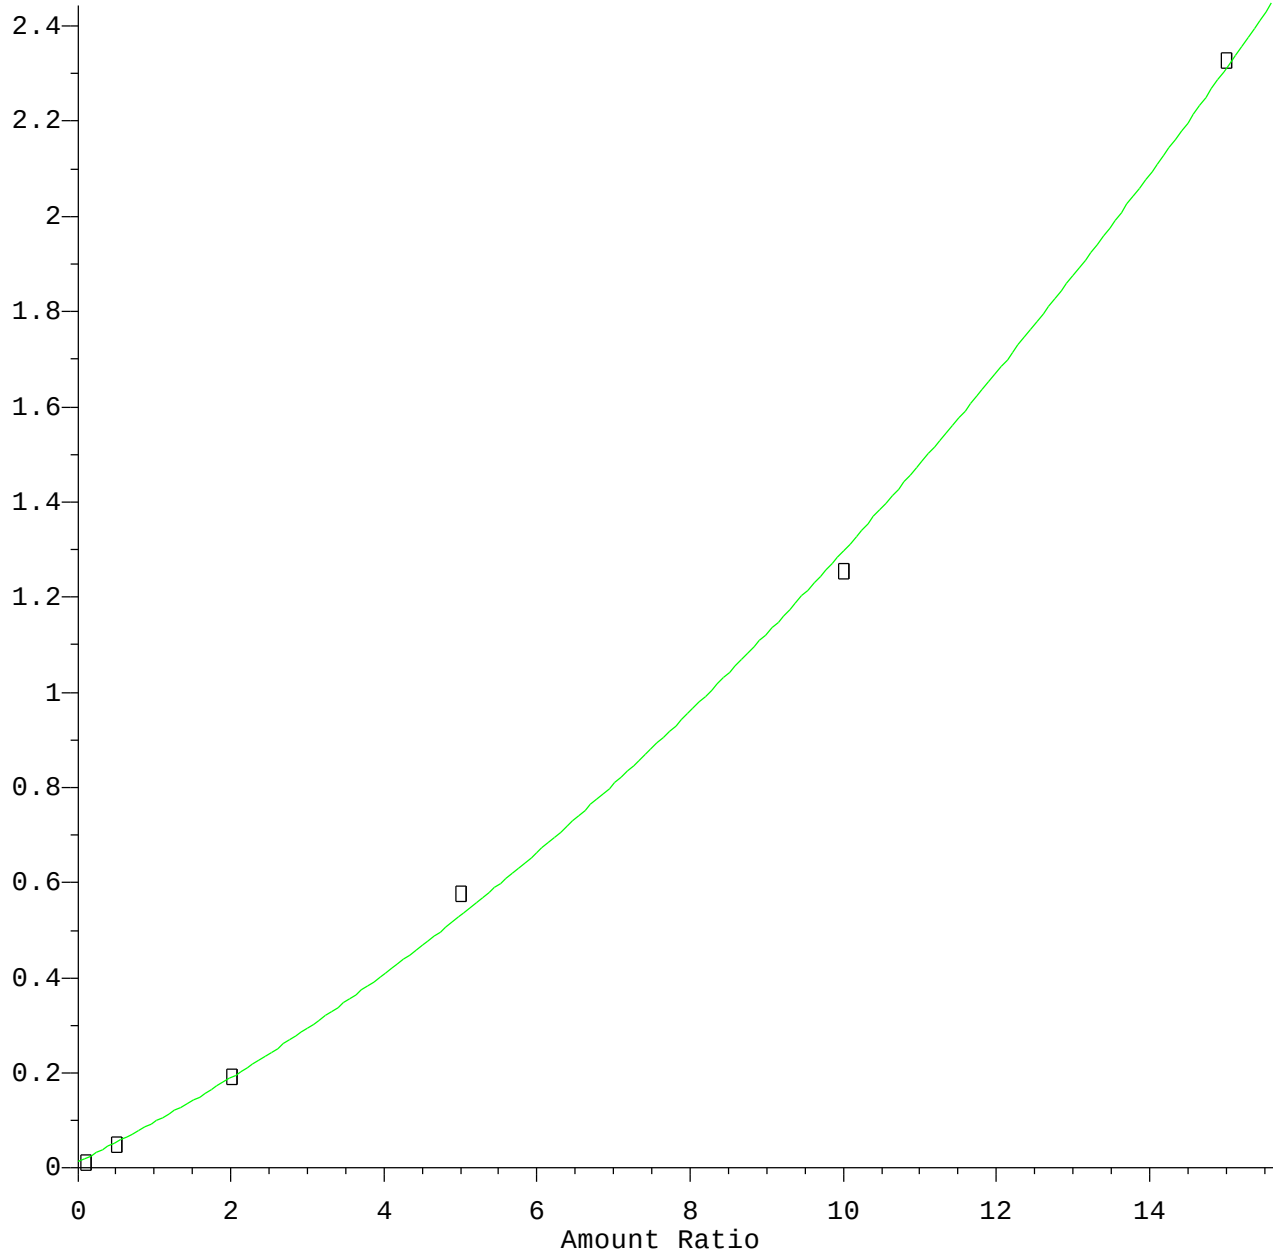


$R = 4.96e-003 A^2 + 7.88e-002 A + 1.29e-002$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081720W.M
Calibration Table Last Updated: Mon Aug 17 17:31:03 2020

2-Hexanone

Response Ratio

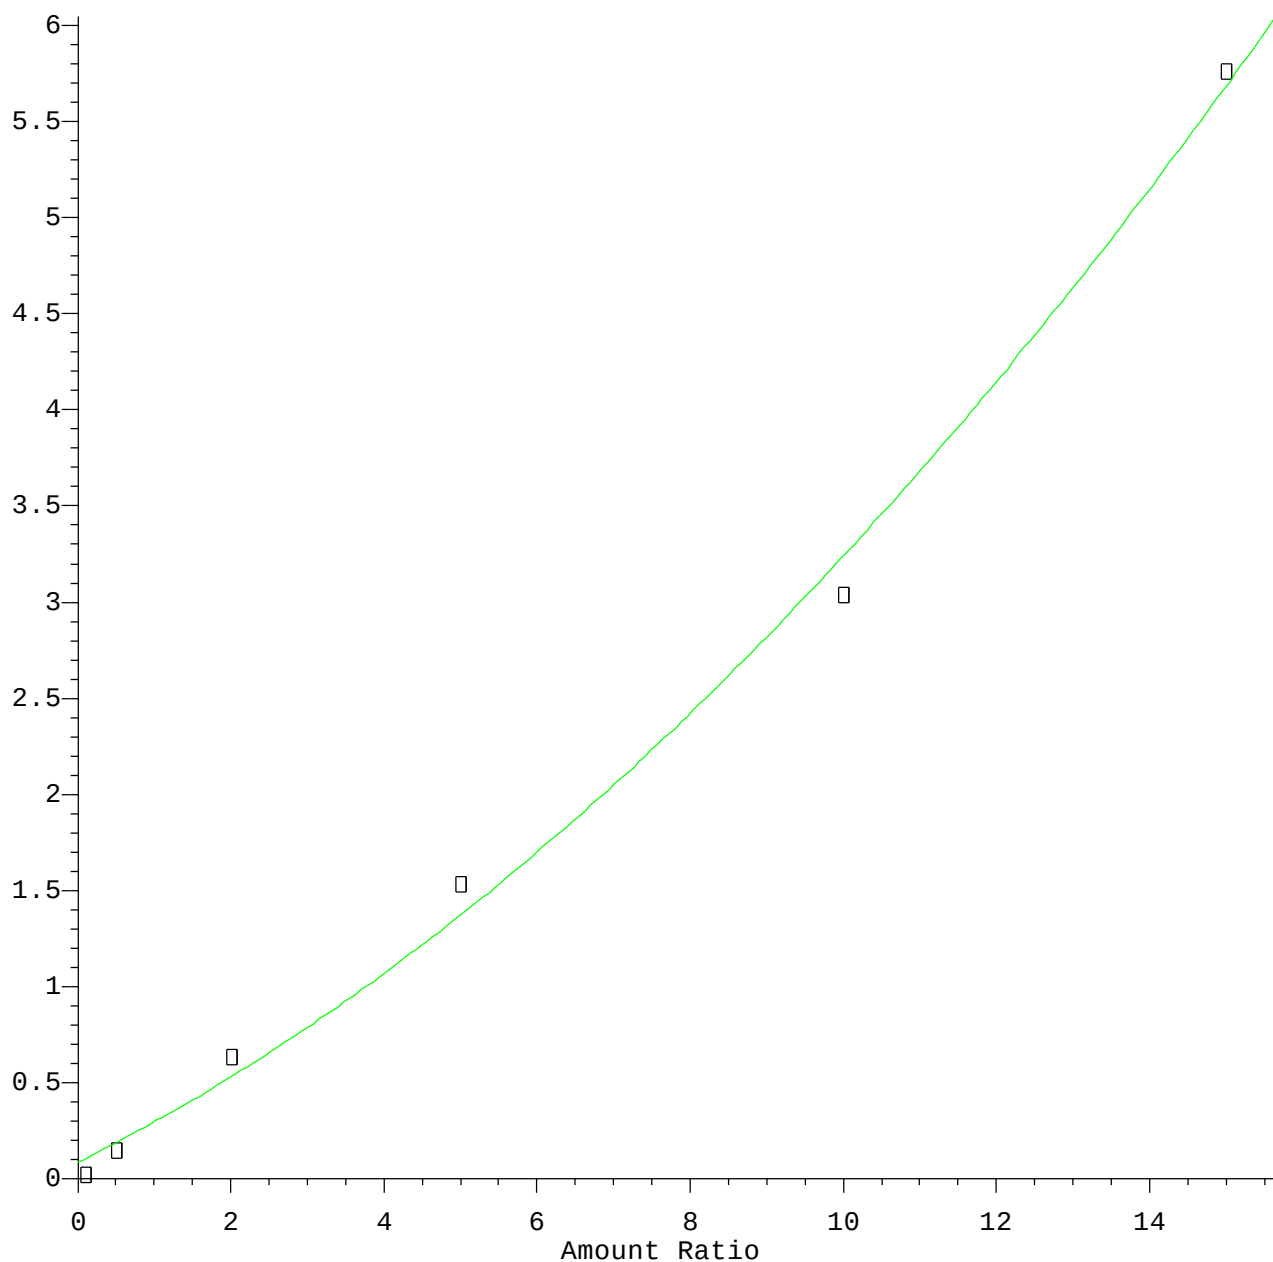


$R = 1.16e-002 A^2 + 1.99e-001 A + 8.63e-002$
Coef of Det (r^2) = 0.996 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081720W.M
Calibration Table Last Updated: Mon Aug 17 17:31:03 2020

1,1,2,2-Tetrachloroethane

Response Ratio

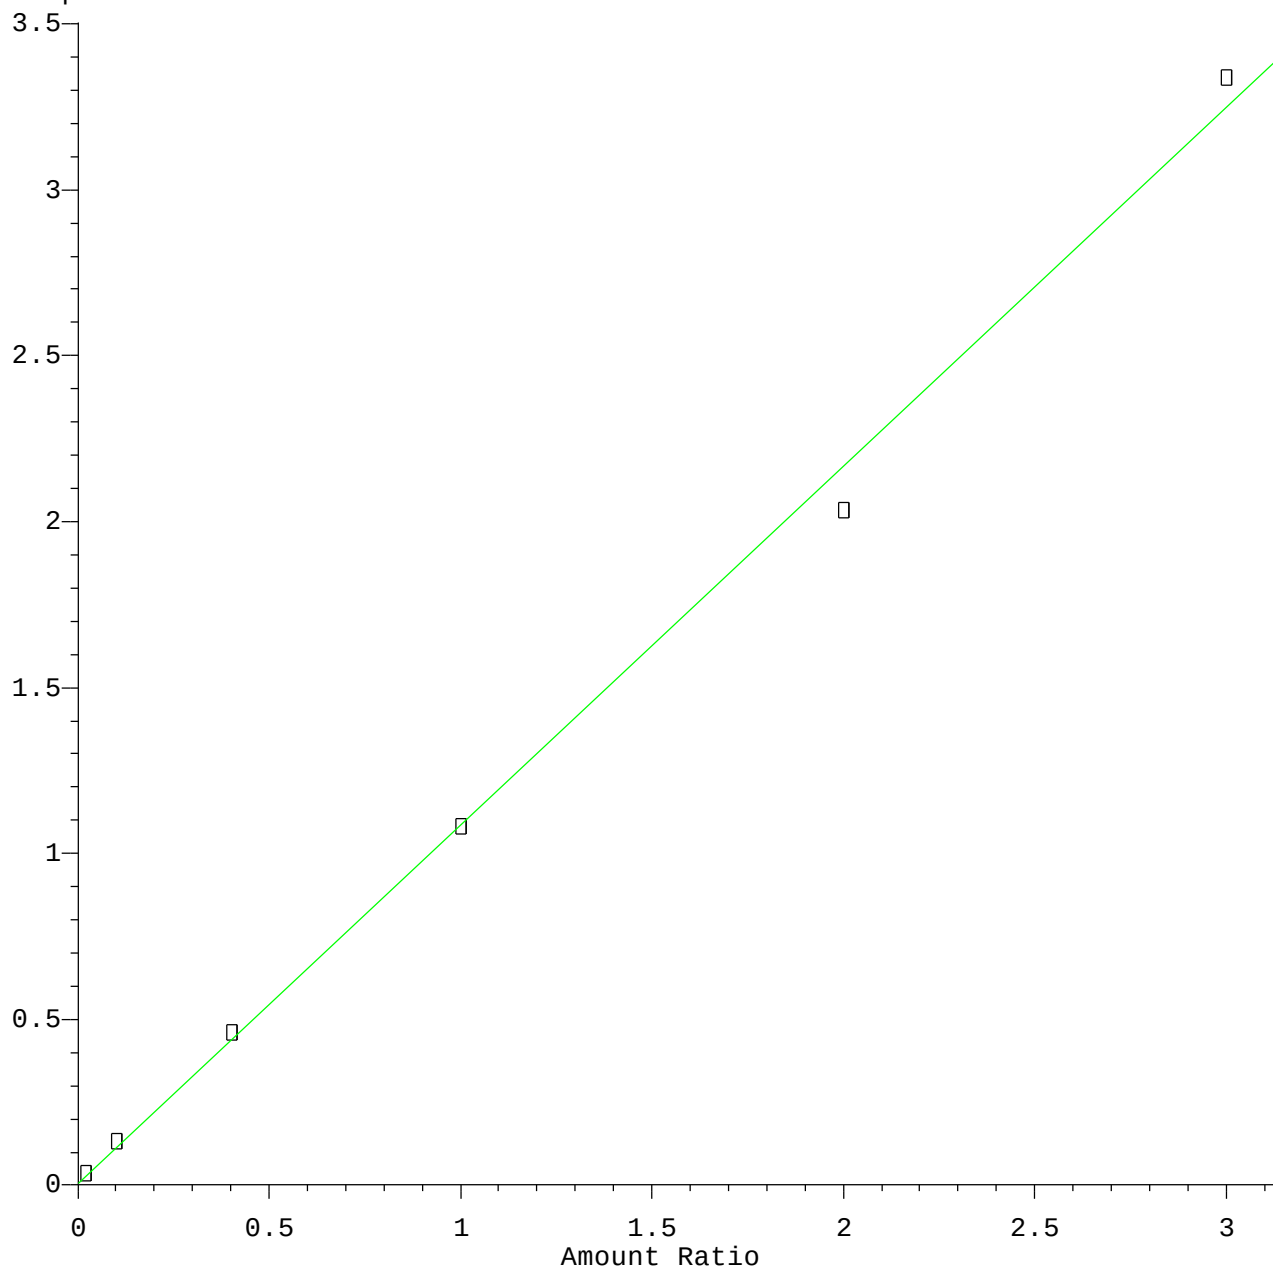


Resp Ratio = 1.08×10^0 * Amt + 4.15×10^{-3}
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081720W.M
Calibration Table Last Updated: Mon Aug 17 17:31:03 2020

1,2,3-Trichloropropane

Response Ratio

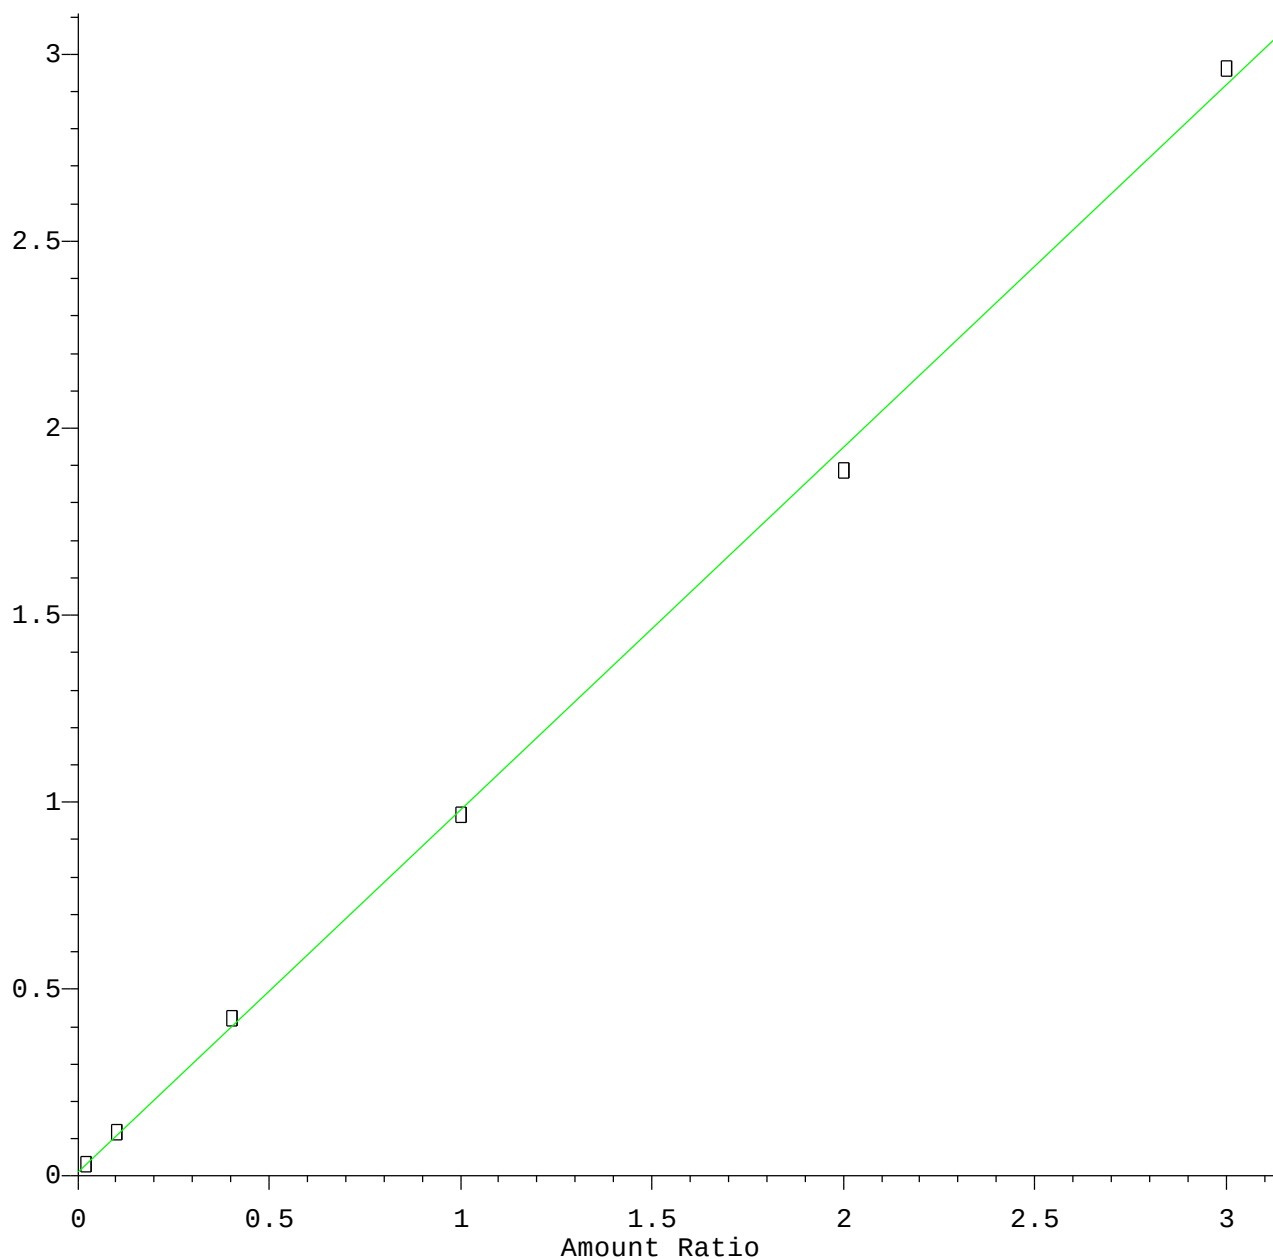


Resp Ratio = $9.69 \times 10^{-1} \times \text{Amt} + 1.05 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081720W.M
Calibration Table Last Updated: Mon Aug 17 17:31:03 2020

1,2,4-Trichlorobenzene

Response Ratio

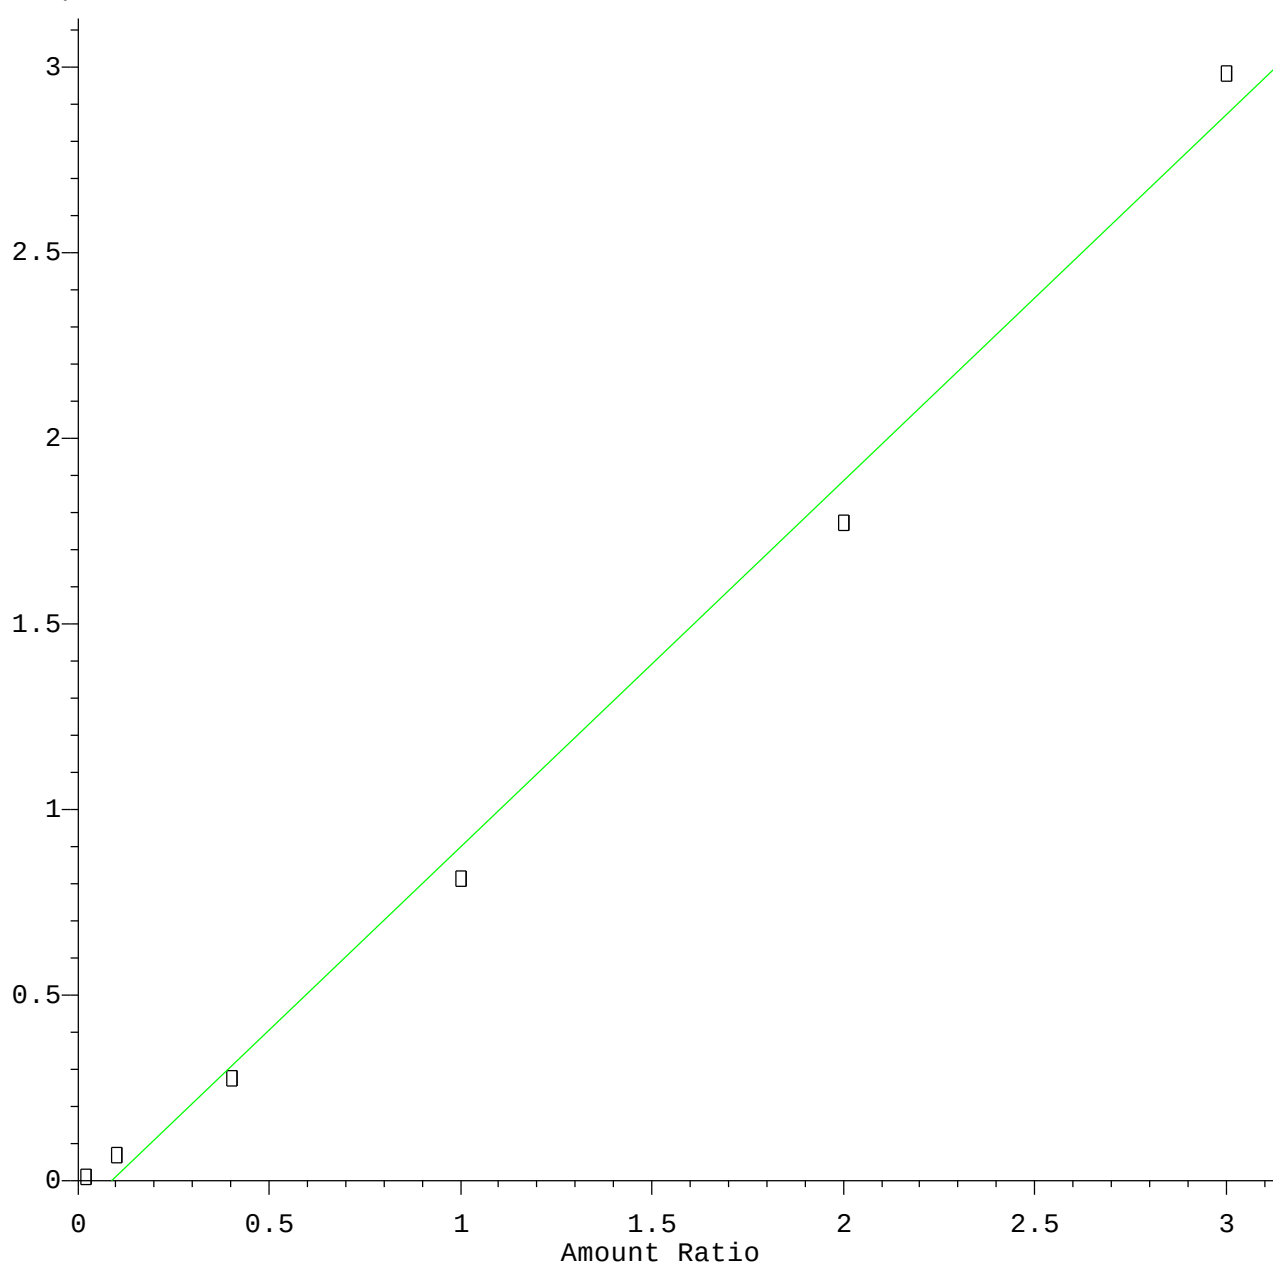


Resp Ratio = $9.85 \times 10^{-1} \times \text{Amt} - 8.44 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081720W.M
Calibration Table Last Updated: Mon Aug 17 17:31:03 2020

Naphthalene

Response Ratio

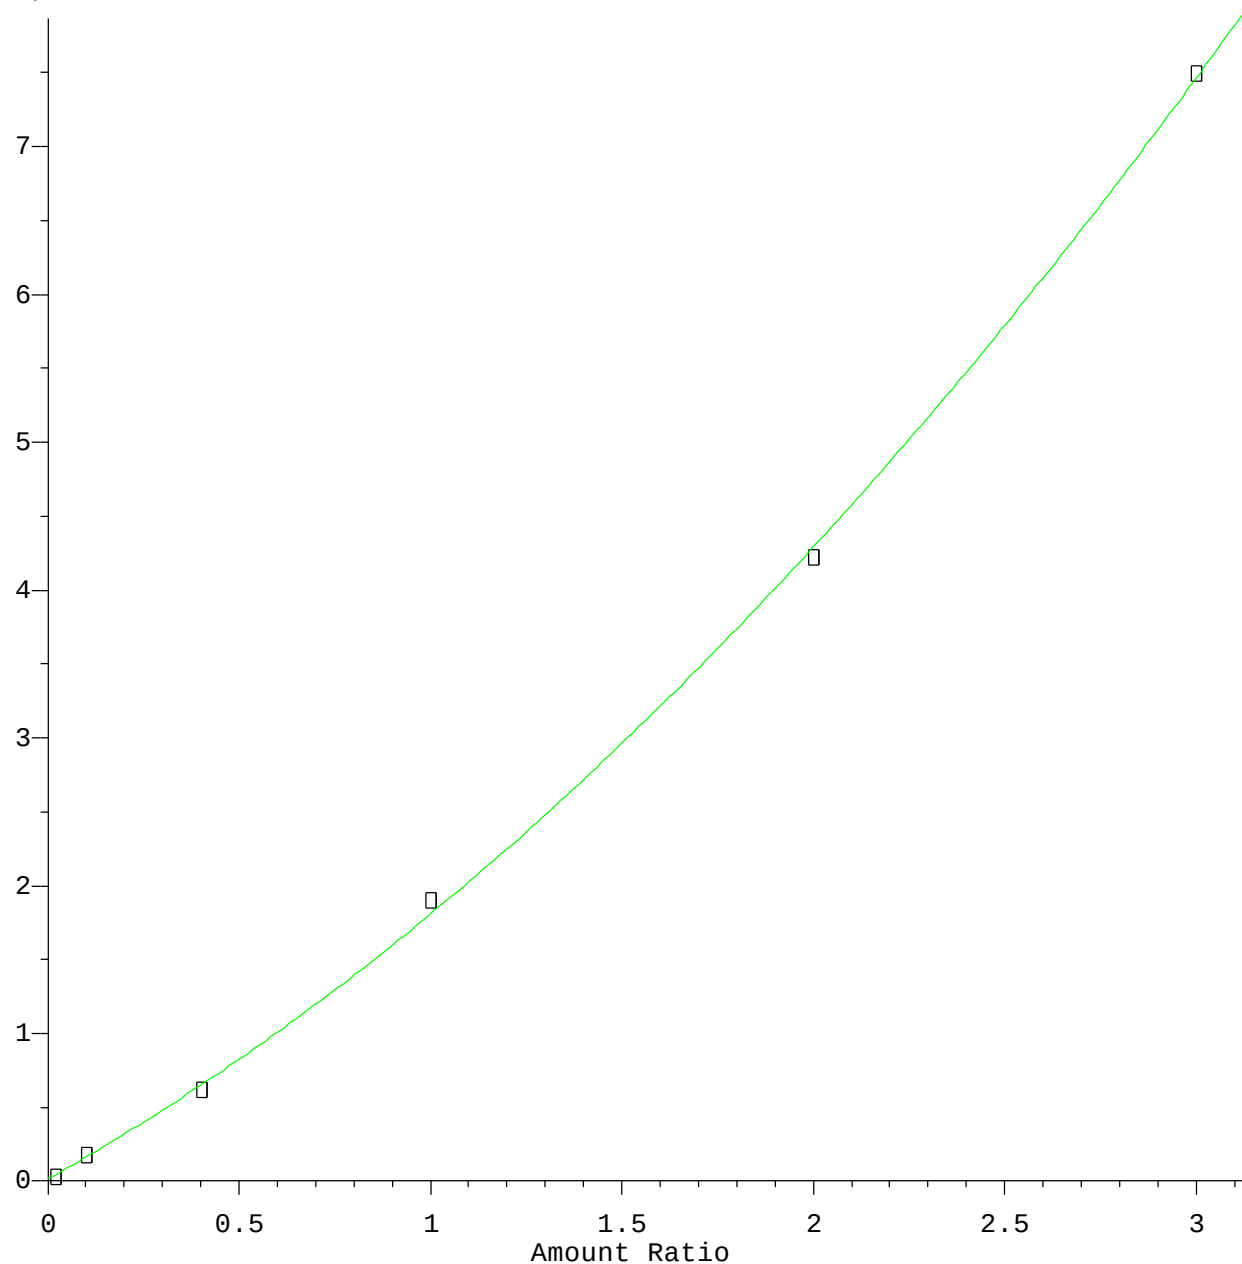


$R = 3.45e-001 A^2 + 1.45e+000 A + 1.50e-002$
Coef of Det (r^2) = 1.000 Curve Fit: Quadratic

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081720W.M
Calibration Table Last Updated: Mon Aug 17 17:31:03 2020

1,2,3-Trichlorobenzene

Response Ratio

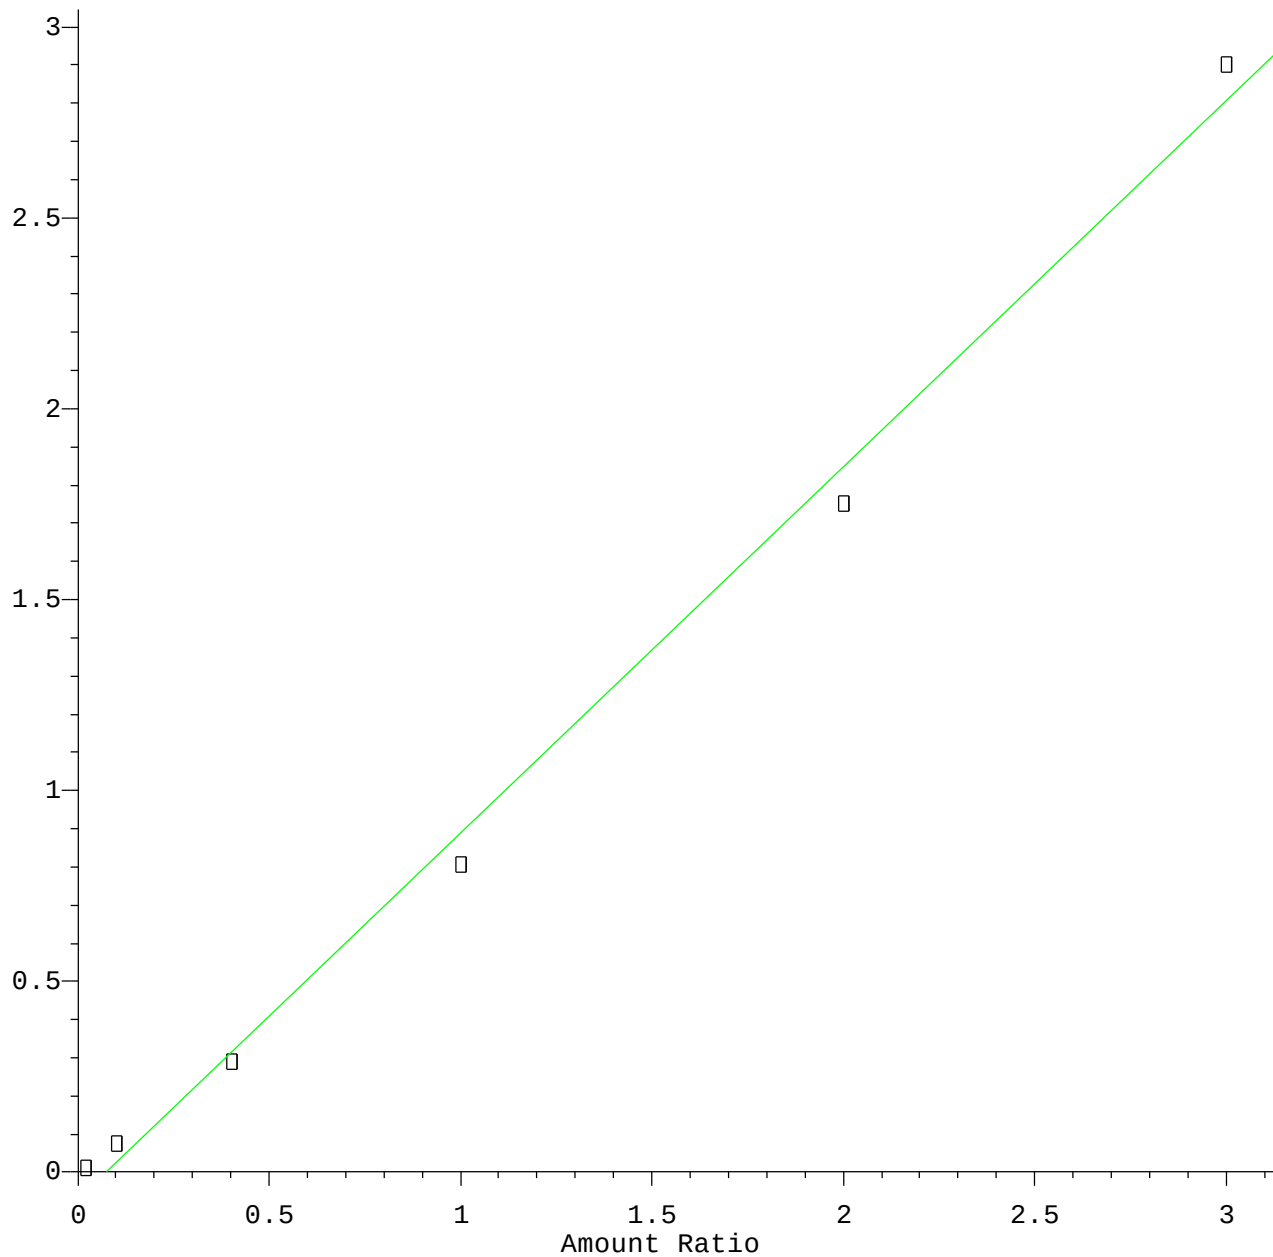


Resp Ratio = $9.59 \times 10^{-1} \times \text{Amt} - 7.14 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081720W.M
Calibration Table Last Updated: Mon Aug 17 17:31:03 2020


Dichlorodifluoromethane

Response Ratio

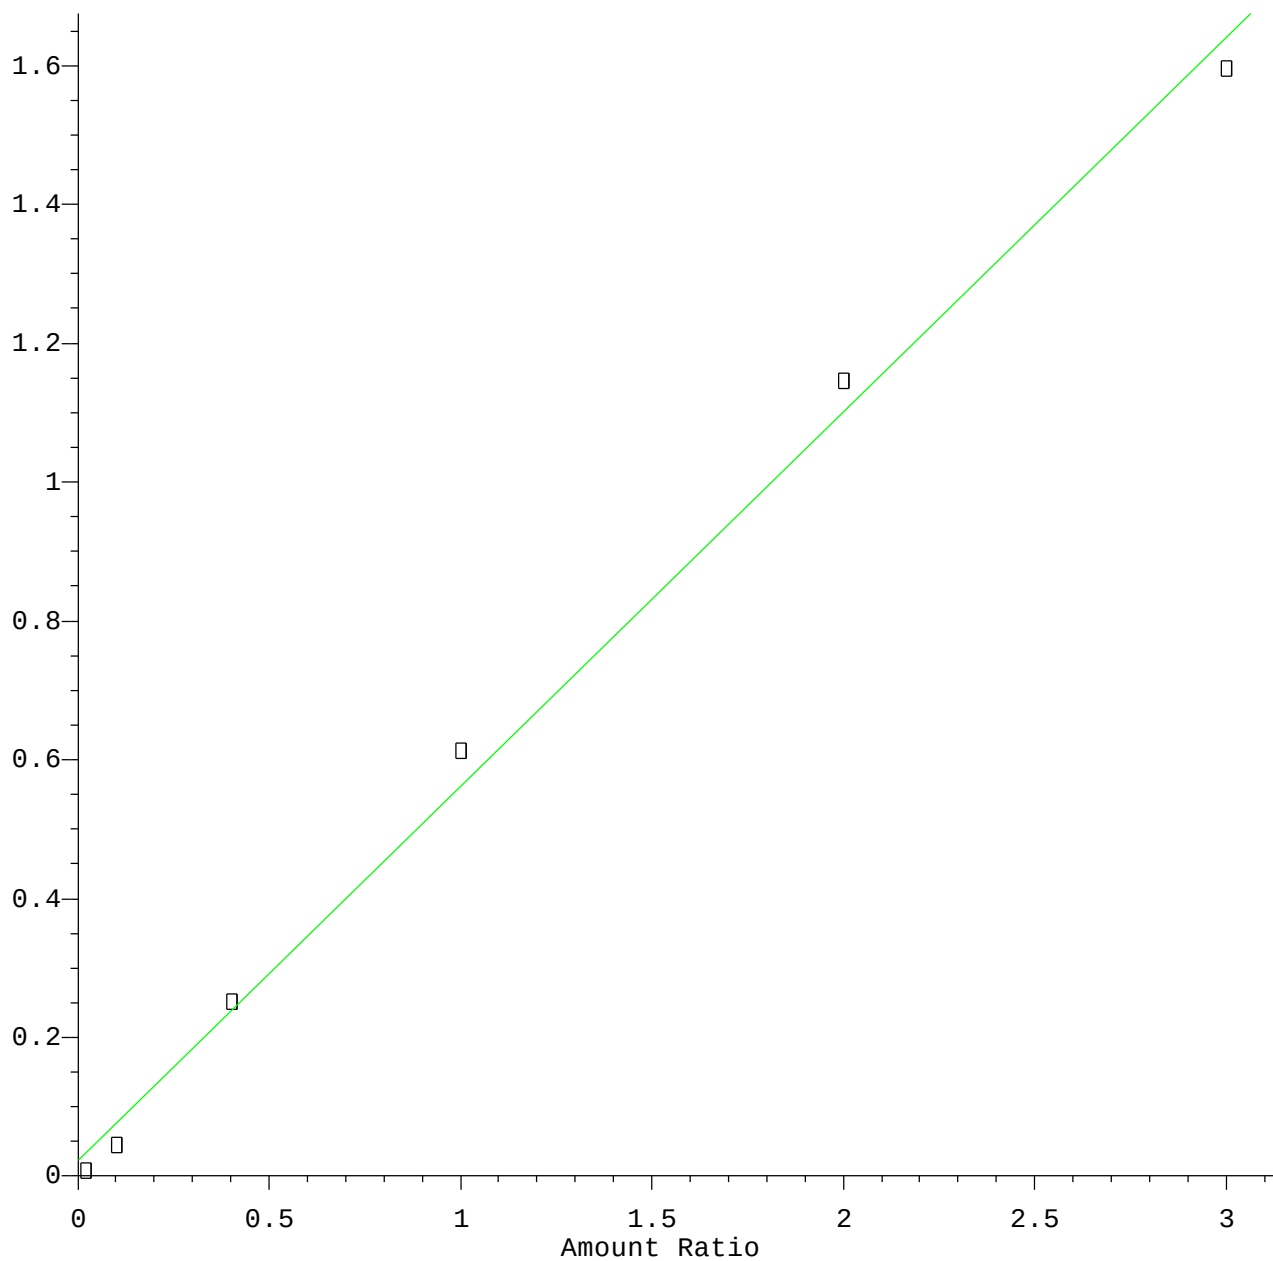

Resp Ratio = $5.39 \times 10^{-1} \times \text{Amt} + 2.27 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081720W.M
Calibration Table Last Updated: Mon Aug 17 17:31:03 2020

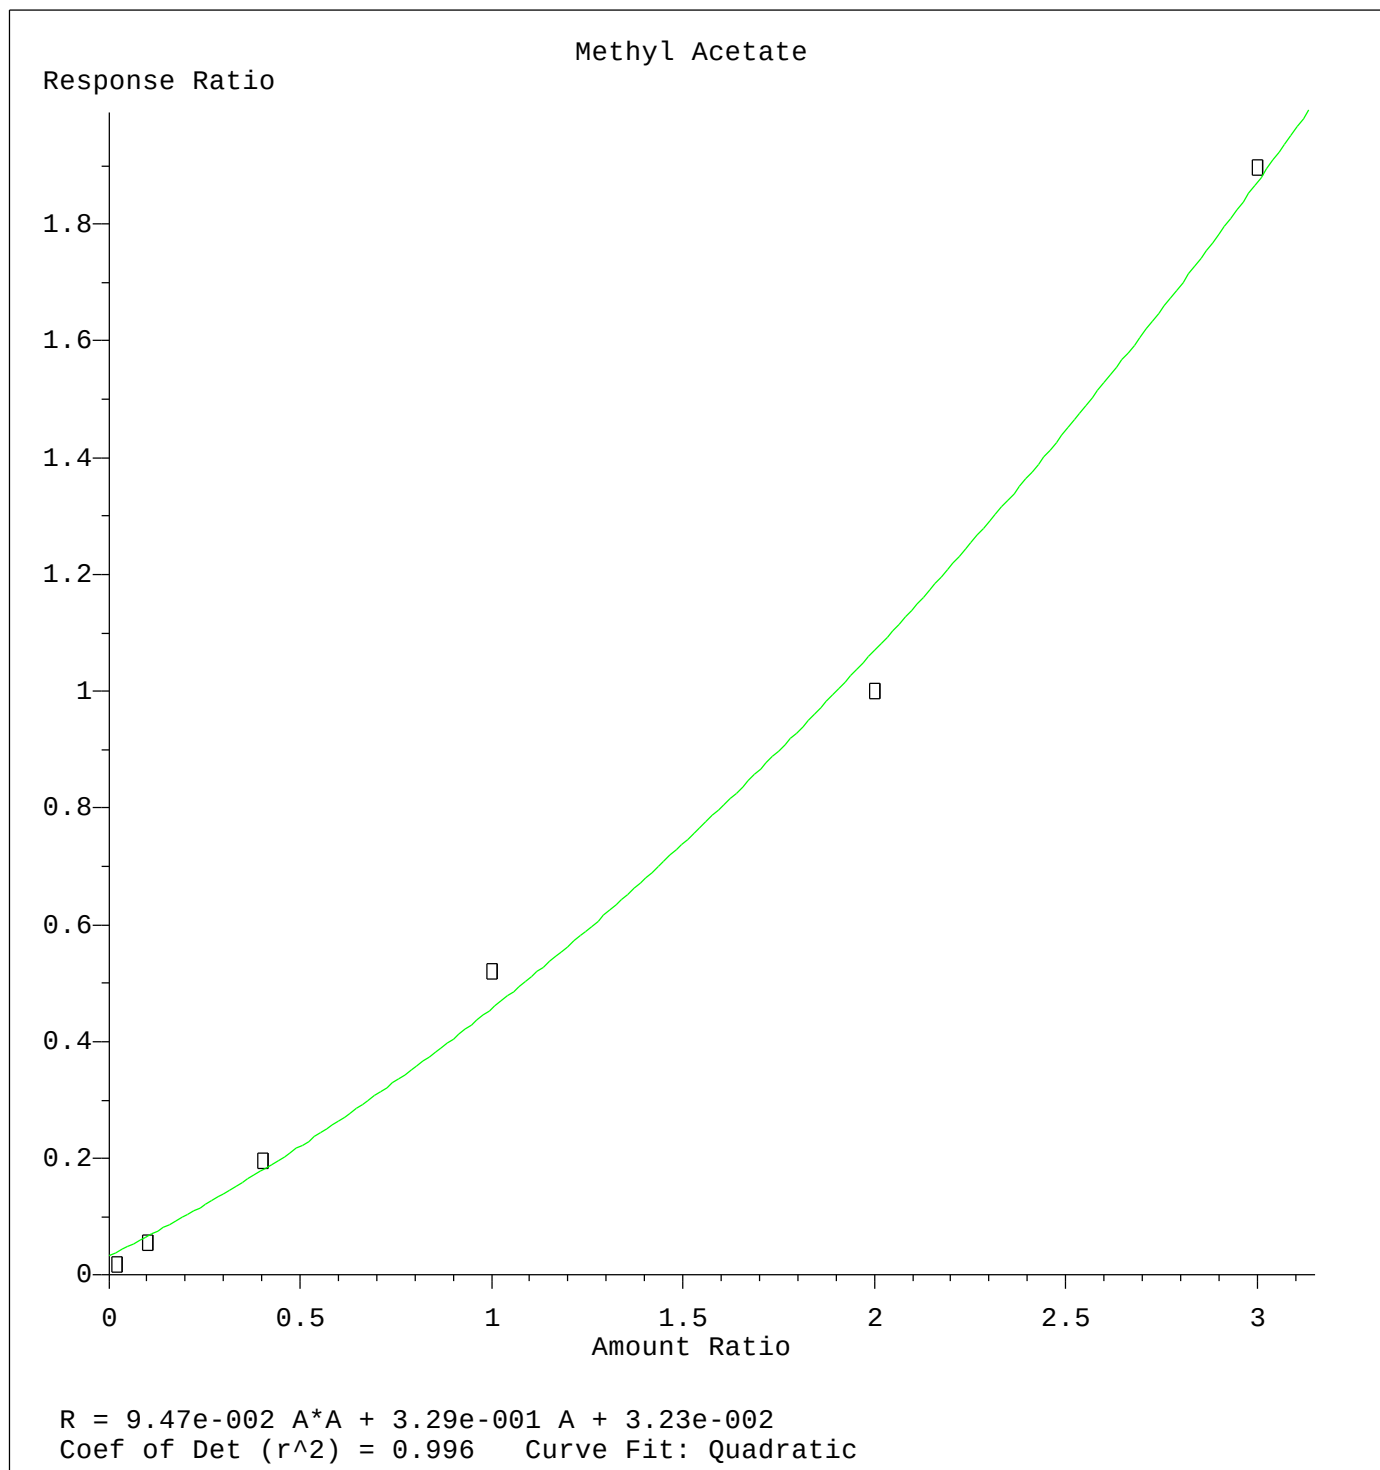

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081720W.M
Calibration Table Last Updated: Mon Aug 17 17:31:03 2020

Methylene Chloride

Response Ratio

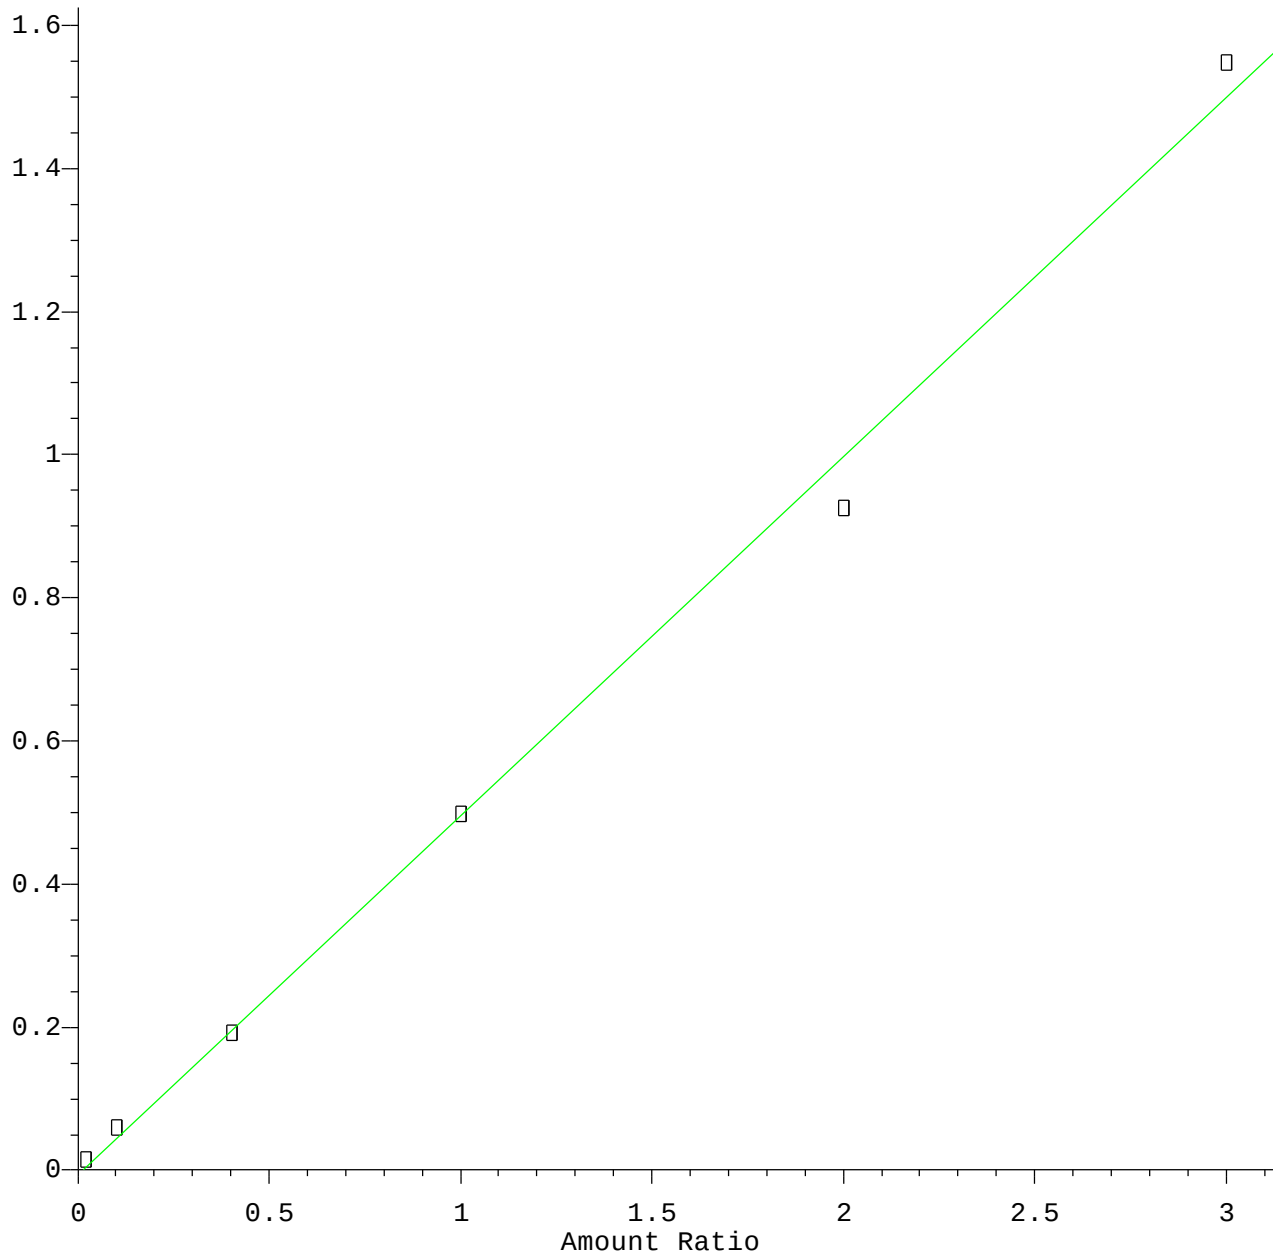

Resp Ratio = $5.02 \times 10^{-1} \times \text{Amt} - 6.14 \times 10^{-3}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081720W.M
Calibration Table Last Updated: Mon Aug 17 17:31:03 2020