

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081721\
 Data File : VN068170.D
 Acq On : 18 Aug 2021 3:30
 Operator : JC/MD
 Sample : M3446-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RW6B-GW-20210816

Quant Time: Aug 18 08:41:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 13:09:49 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	415890	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.971	114	694776	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	690793	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	260250	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	237416	53.465	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 106.940%	
35) Dibromofluoromethane	8.024	113	214494	49.173	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 98.340%	
50) Toluene-d8	10.443	98	846952	50.958	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 101.920%	
62) 4-Bromofluorobenzene	12.736	95	273574	49.444	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 98.880%	
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	2.073	85	2688	0.816	ug/l	99
3) Chloromethane	2.303	50	4015	1.078	ug/l	99
5) Bromomethane	2.834	94	202	Below Cal		88
6) Chloroethane	2.982	64	83	Below Cal	#	44
9) 1,1,2-Trichlorotrifluo...	4.208	101	28309	8.073	ug/l	# 69
12) 1,1-Dichloroethene	4.181	96	7948	2.357	ug/l	# 71
13) Acrolein	4.049	56	49	Below Cal	#	14
16) Acetone	4.304	43	2514	1.939	ug/l	99
18) Methyl Acetate	4.843	43	733	Below Cal	#	54
20) Methylene Chloride	5.098	84	144	Below Cal	#	40
24) 1,1-Dichloroethane	6.377	63	1260	0.200	ug/l	# 85
27) cis-1,2-Dichloroethene	7.329	96	4970	1.100	ug/l	59
28) Bromochloromethane	7.823	49	719	0.260	ug/l	# 22
30) Chloroform	7.817	83	10429	1.392	ug/l	99
31) Cyclohexane	8.091	56	7170	1.226	ug/l	# 16
36) 1,1-Dichloropropene	8.086	75	27070	4.766	ug/l	# 47
38) Carbon Tetrachloride	8.209	117	20245	3.091	ug/l	97
39) Methylcyclohexane	9.215	83	12520	1.952	ug/l	# 1
43) Isopropyl Acetate	8.643	43	4080	0.526	ug/l	# 58
44) Trichloroethene	9.217	130	1101764	211.353	ug/l	78
45) 1,2-Dichloropropane	9.217	63	2996	0.735	ug/l	# 1
49) 1,4-Dioxane	9.571	88	275	3.523	ug/l	# 77
55) 1,1,2-Trichloroethane	10.904	97	1281	0.271	ug/l	89
60) Dibromochloromethane	10.982	129	1428	0.268	ug/l	# 11
64) Tetrachloroethene	10.977	164	1432	0.268	ug/l	# 75
76) 1,2,3-Trichloropropane	12.736	75	139050	32.146	ug/l	# 100
81) trans-1,4-Dichloro-2-b...	12.736	75	139050	105.315	ug/l	# 6
93) 1,2,4-Trichlorobenzene	15.265	180	300	2.750	ug/l	# 74
95) Naphthalene	15.515	128	1553	3.486	ug/l	# 69
96) 1,2,3-Trichlorobenzene	15.702	180	298	2.900	ug/l	# 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081721\
Data File : VN068170.D
Acq On : 18 Aug 2021 3:30
Operator : JC/MD
Sample : M3446-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816

Quant Time: Aug 18 08:41:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 13:09:49 2021
Response via : Initial Calibration




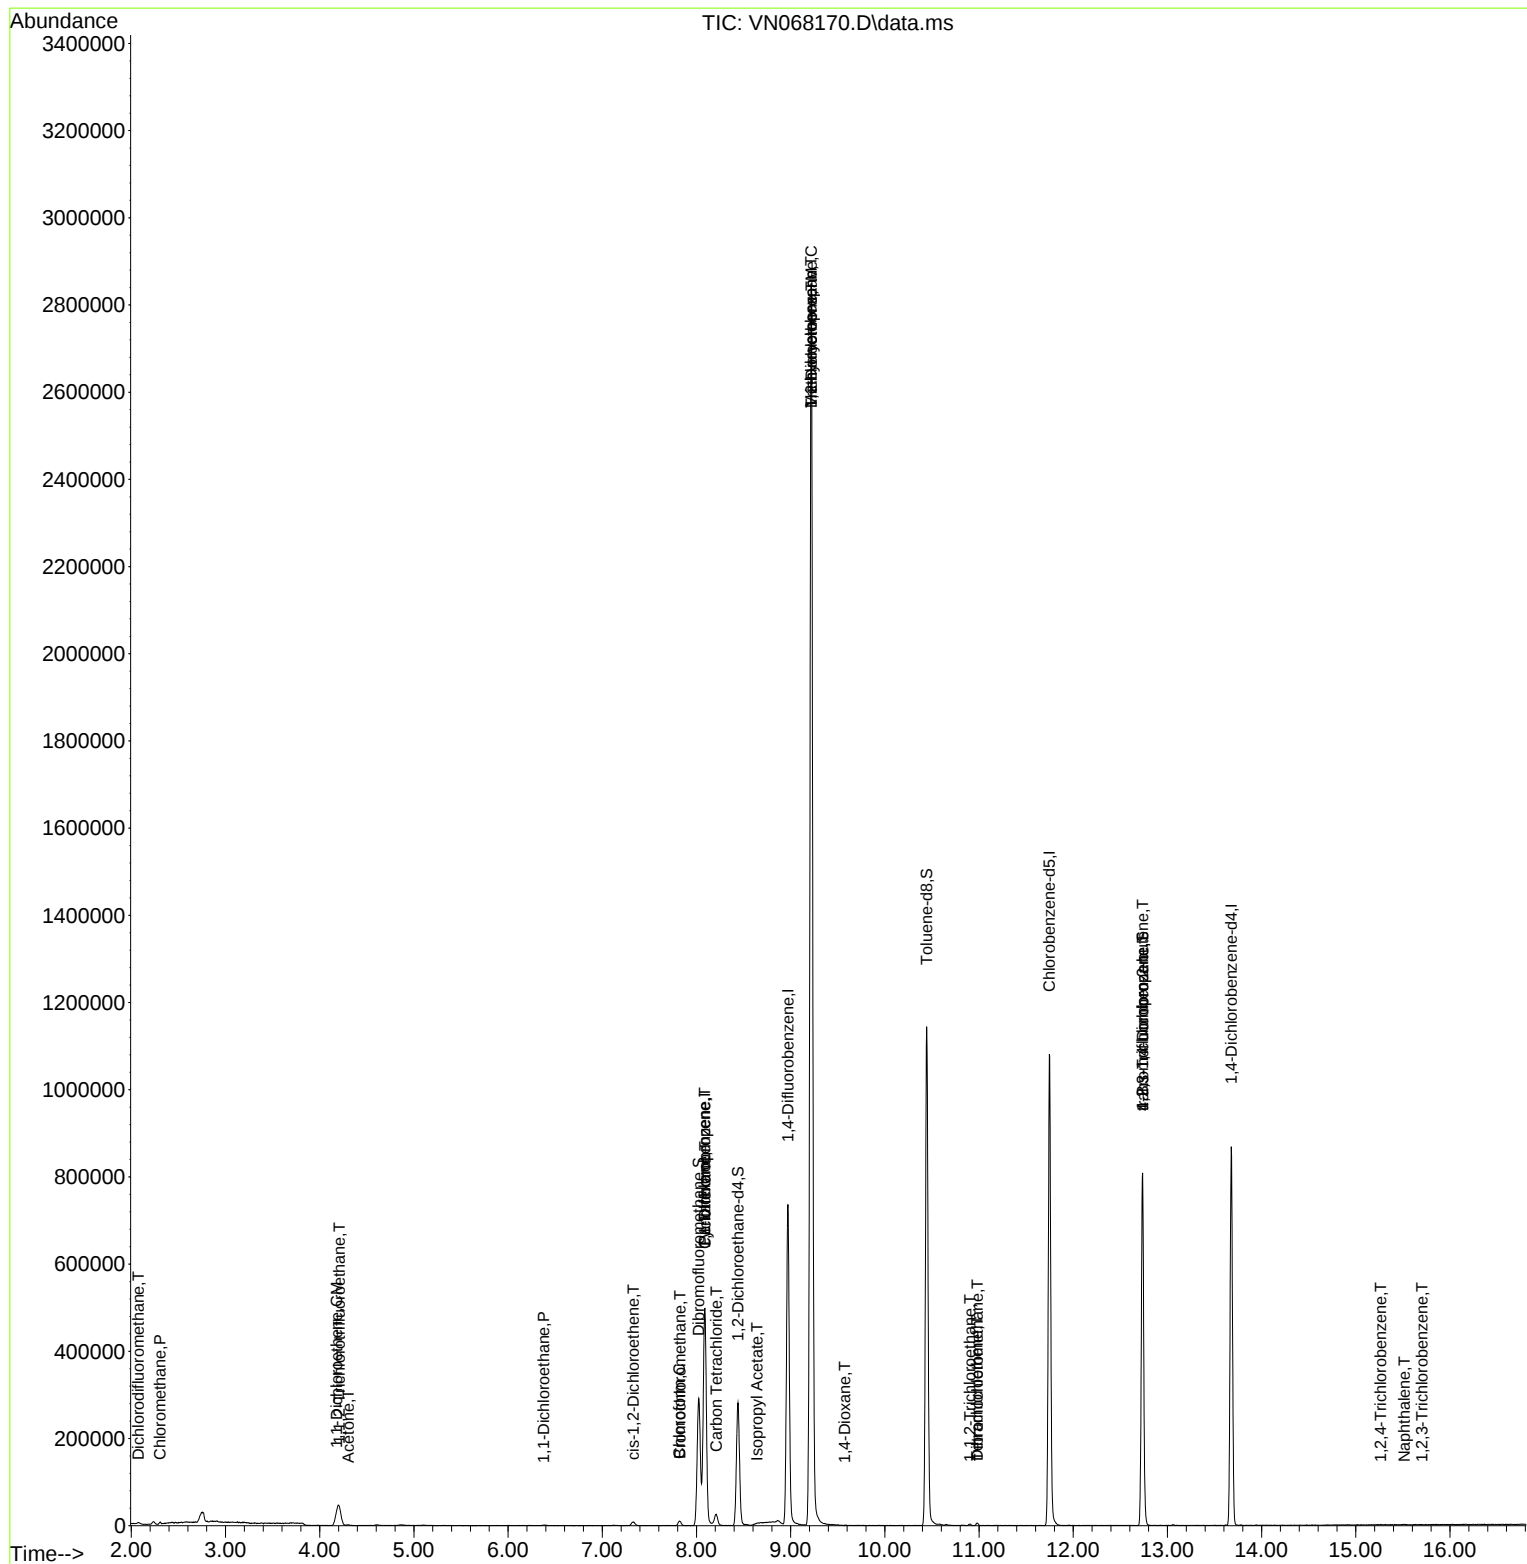




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.000 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion:168 Resp: 415890
Ion Ratio Lower Upper
168 100
99 51.0 62.9 94.3#

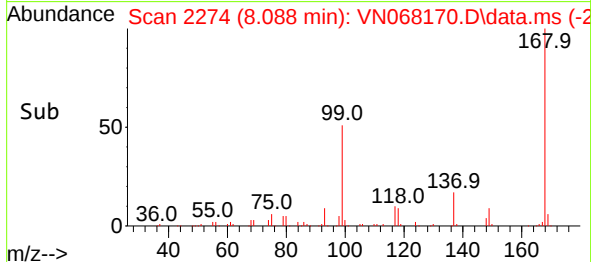

#2
Dichlorodifluoromethane
Concen: 0.816 ug/l
RT: 2.073 min Scan# 31
Delta R.T. 0.003 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion: 85 Resp: 2688
Ion Ratio Lower Upper
85 100
87 31.5 16.1 48.2


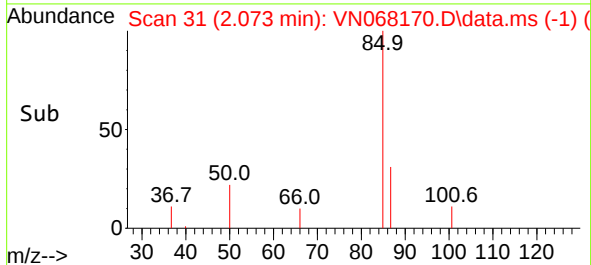






#3
Chloromethane
Concen: 1.078 ug/l
RT: 2.303 min Scan# 117
Delta R.T. 0.002 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion: 50 Resp: 4015
Ion Ratio Lower Upper
50 100
52 31.2 25.6 38.4

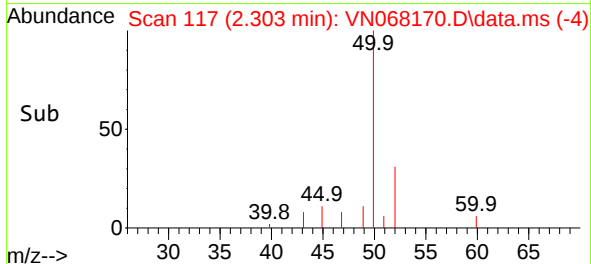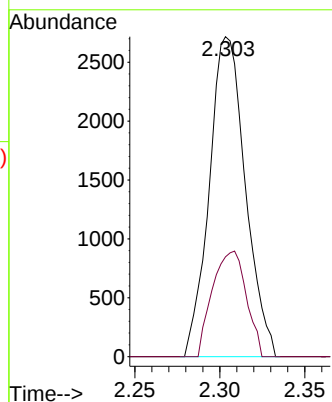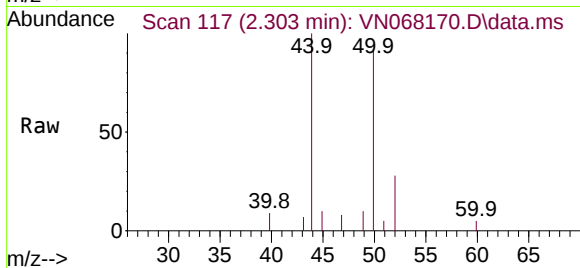

#5
Bromomethane
Concen: Below Cal
RT: 2.834 min Scan# 315
Delta R.T. -0.003 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion: 94 Resp: 202
Ion Ratio Lower Upper
94 100
96 80.9 73.7 110.5



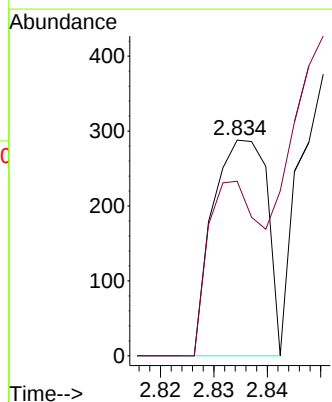
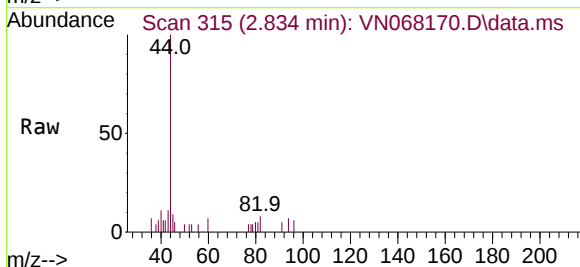




#6
Chloroethane
Concen: Below Cal
RT: 2.982 min Scan# 370
Delta R.T. -0.024 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion: 64 Resp: 83
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#

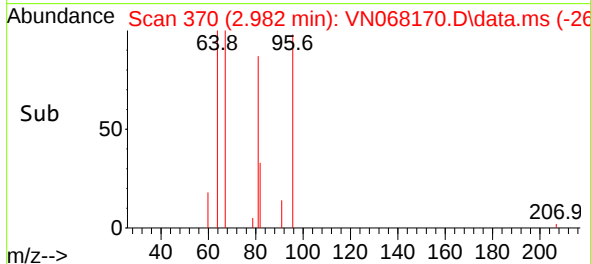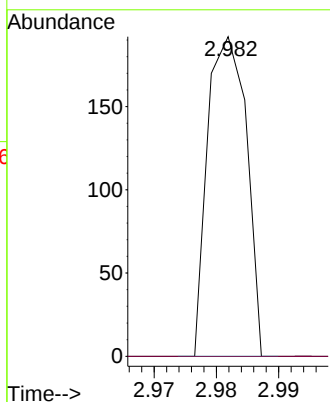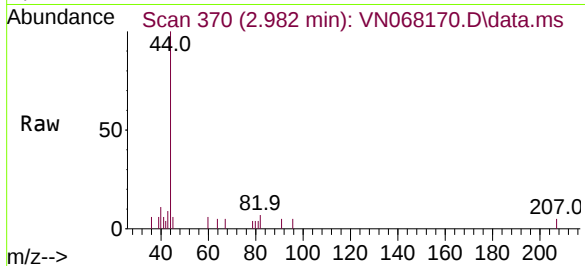

#9
1,1,2-Trichlorotrifluoroethane
Concen: 8.073 ug/l
RT: 4.208 min Scan# 827
Delta R.T. 0.008 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion: 101 Resp: 28309
Ion Ratio Lower Upper
101 100
85 18.7 39.6 59.4#
151 84.3 54.1 81.1#




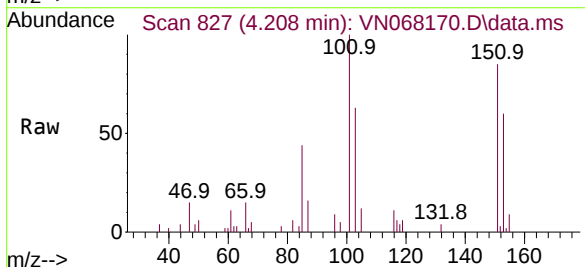




#12
1,1-Dichloroethene
Concen: 2.357 ug/l
RT: 4.181 min Scan# 817
Delta R.T. 0.011 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion: 96 Resp: 7948
Ion Ratio Lower Upper
96 100
61 135.7 152.6 229.0#
98 66.4 50.9 76.3

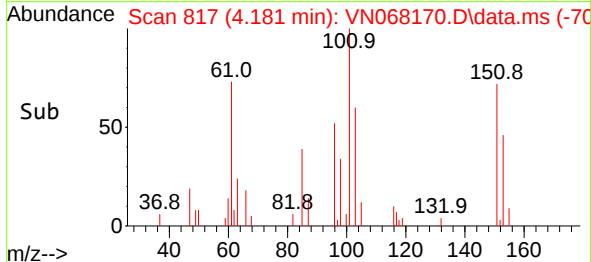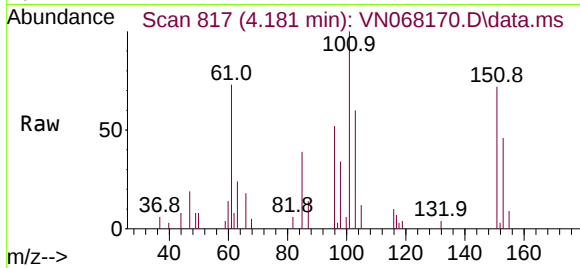

#13
Acrolein
Concen: Below Cal
RT: 4.049 min Scan# 768
Delta R.T. 0.010 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion: 56 Resp: 49
Ion Ratio Lower Upper
56 100
55 0.0 57.4 86.0#




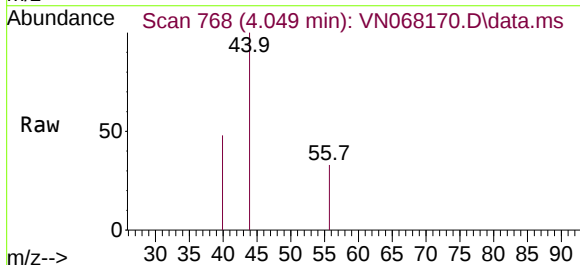




#16
Acetone
Concen: 1.939 ug/l
RT: 4.304 min Scan# 863
Delta R.T. 0.016 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion: 43 Resp: 2514
Ion Ratio Lower Upper
43 100
58 25.8 21.2 31.8

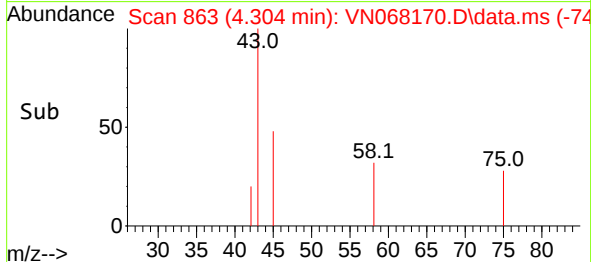

#18
Methyl Acetate
Concen: Below Cal
RT: 4.843 min Scan# 1064
Delta R.T. -0.011 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion: 43 Resp: 733
Ion Ratio Lower Upper
43 100
74 0.0 17.4 26.0#




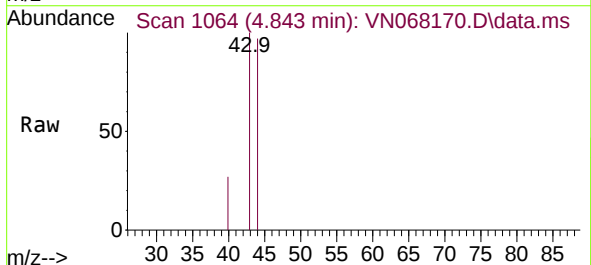


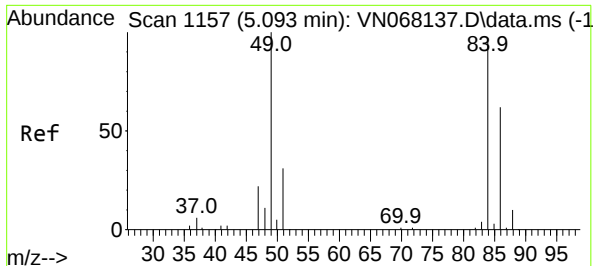

#20
Methylene Chloride
Concen: Below Cal
RT: 5.098 min Scan# 1159
Delta R.T. 0.005 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion:	84	Resp:	144
Ion	Ratio	Lower	Upper
84	100		
49	81.0	110.9	166.3#
51	0.0	32.6	49.0#
86	0.0	51.6	77.4#

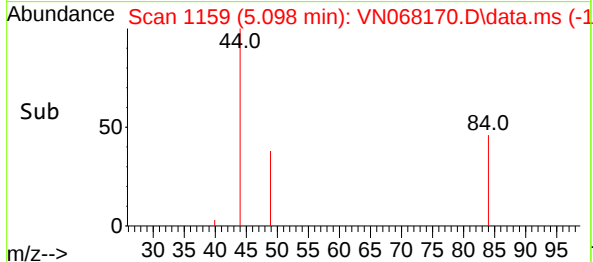

#24
1,1-Dichloroethane
Concen: 0.200 ug/l
RT: 6.377 min Scan# 1636
Delta R.T. -0.006 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion:	63	Resp:	1260
Ion	Ratio	Lower	Upper
63	100		
98	0.0	3.0	9.0#
100	0.0	1.9	5.7#

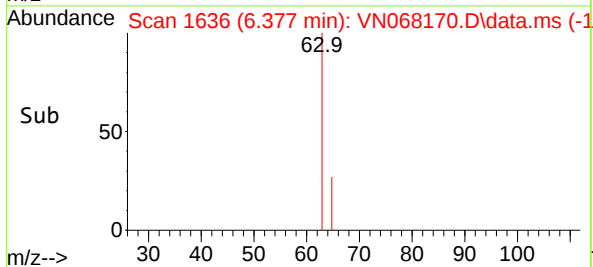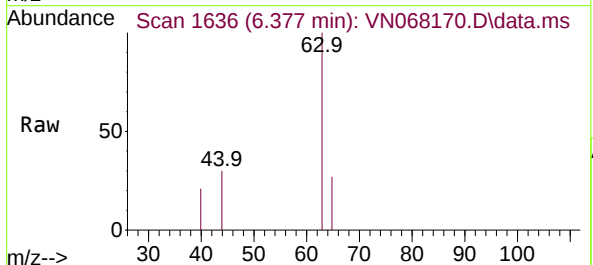







#27

cis-1,2-Dichloroethene
Concen: 1.100 ug/l
RT: 7.329 min Scan# 1991
Delta R.T. 0.005 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816




Tgt Ion: 96	Resp: 4970
Ion Ratio	Lower Upper
96 100	
61 115.2	0.0 338.8
98 28.7	0.0 129.8

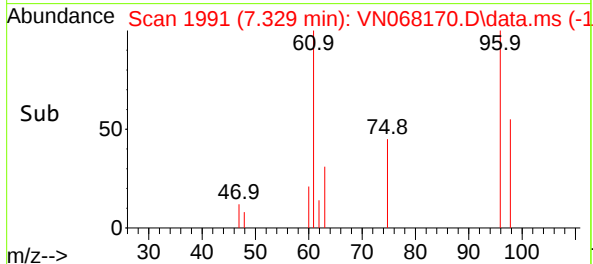


#28

Bromochloromethane
Concen: 0.260 ug/l
RT: 7.823 min Scan# 2175
Delta R.T. 0.164 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion: 49	Resp: 719
Ion Ratio	Lower Upper
49 100	
129 0.0	0.0 3.8
130 0.0	49.7 74.5#

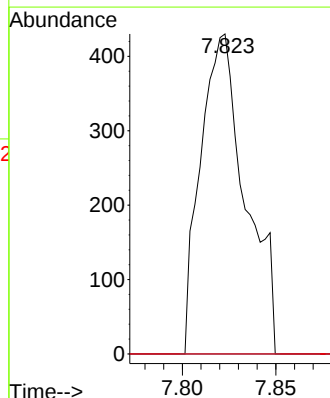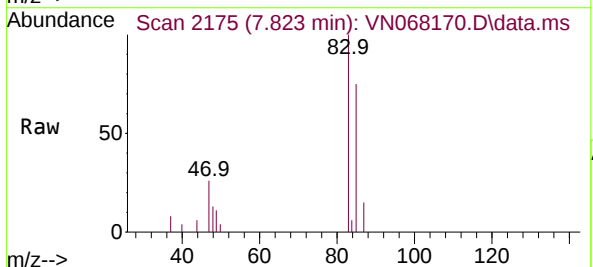

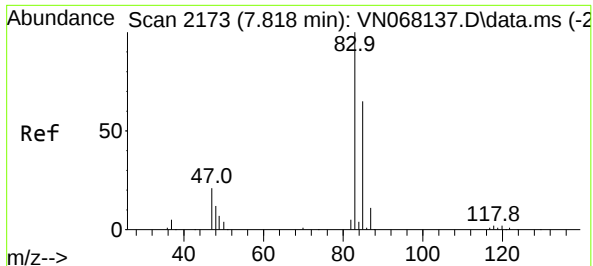

#30

Chloroform

Concen: 1.392 ug/l

RT: 7.817 min Scan# 2173

Delta R.T. -0.001 min

Lab File: VN068170.D

Acq: 18 Aug 2021 3:30

Tgt Ion: 83 Resp: 10429

Ion Ratio Lower Upper

83 100





85 65.1 51.5 77.3

Instrument :

MSVOA_N

ClientSampleId :

RW6B-GW-20210816

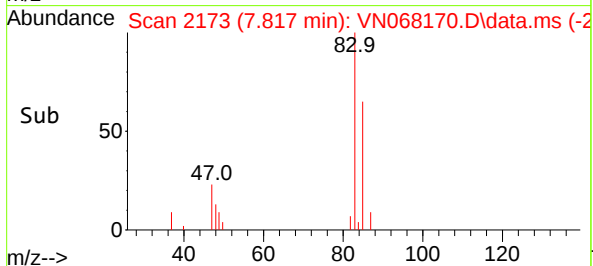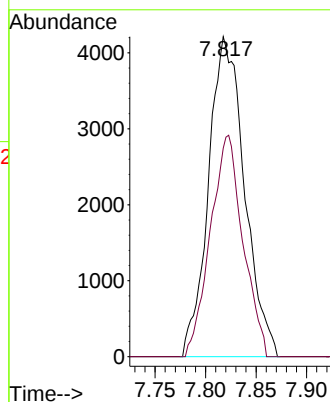

#31

Cyclohexane

Concen: 1.226 ug/l

RT: 8.091 min Scan# 2275

Delta R.T. -0.003 min

Lab File: VN068170.D

Acq: 18 Aug 2021 3:30




Tgt Ion: 56 Resp: 7170


Ion Ratio Lower Upper

56 100

69 143.1 27.3 40.9#

84 116.1 64.9 97.3#


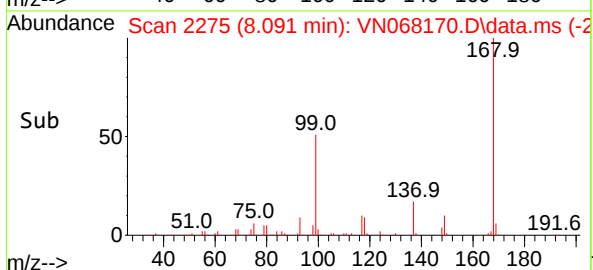

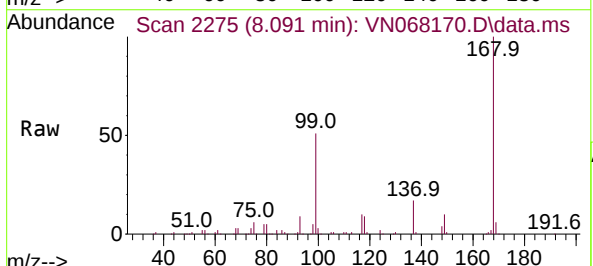




#33
 1,2-Dichloroethane-d4
 Concen: 53.465 ug/l
 RT: 8.440 min Scan# 2405
 Delta R.T. -0.000 min
 Lab File: VN068170.D
 Acq: 18 Aug 2021 3:30




Instrument :
 MSVOA_N
 ClientSampleId :
 RW6B-GW-20210816


Tgt Ion: 65 Resp: 237416
 Ion Ratio Lower Upper
 65 100
 67 52.4 0.0 98.6

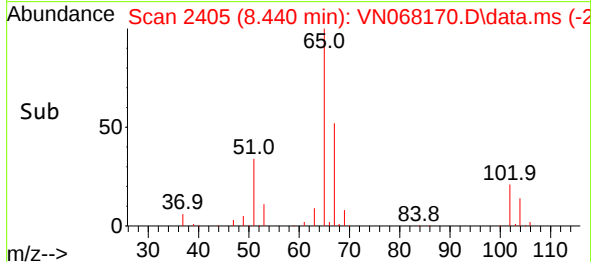

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.971 min Scan# 2603
 Delta R.T. 0.003 min
 Lab File: VN068170.D
 Acq: 18 Aug 2021 3:30

Tgt Ion: 114 Resp: 694776
 Ion Ratio Lower Upper
 114 100
 63 16.4 0.0 49.0
 88 14.1 0.0 36.6




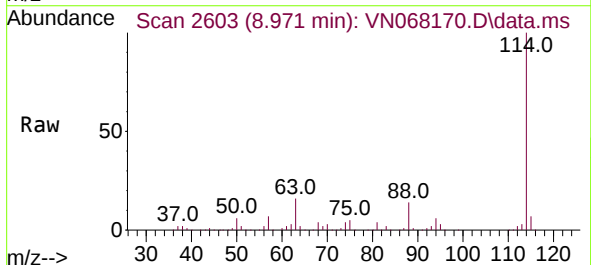




#35
Dibromofluoromethane
Concen: 49.173 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion:113 Resp: 214494
Ion Ratio Lower Upper
113 100
111 102.6 83.8 125.8
192 20.4 13.4 20.0#

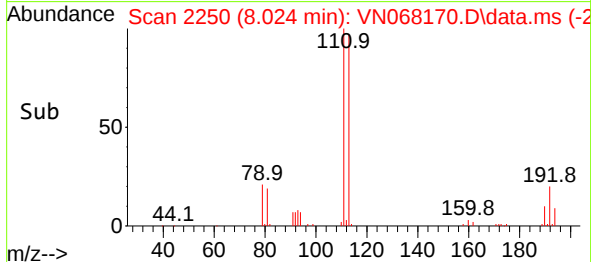

#36
1,1-Dichloropropene
Concen: 4.766 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.137 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion: 75 Resp: 27070
Ion Ratio Lower Upper
75 100
110 3.3 15.7 47.0#
77 0.0 24.6 37.0#




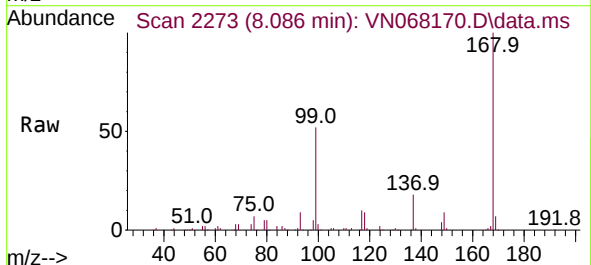




#38
Carbon Tetrachloride
Concen: 3.091 ug/l
RT: 8.209 min Scan# 2319
Delta R.T. 0.003 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion:117 Resp: 20245
Ion Ratio Lower Upper
117 100
119 97.2 75.4 113.2
121 32.0 23.5 35.3

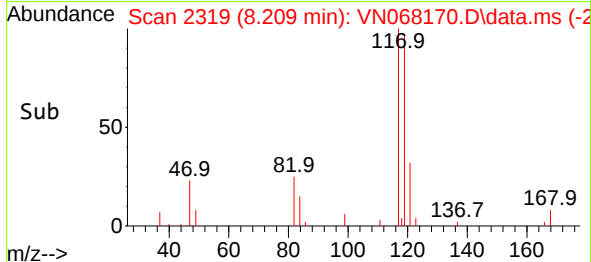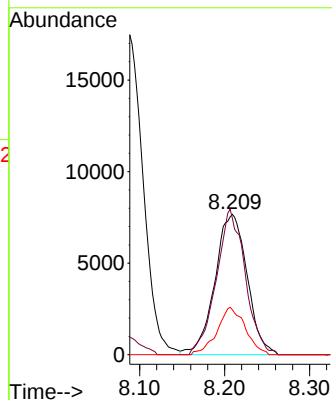

#39
Methylcyclohexane
Concen: 1.952 ug/l
RT: 9.215 min Scan# 2694
Delta R.T. -0.247 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion: 83 Resp: 12520
Ion Ratio Lower Upper
83 100
55 0.0 66.6 99.8#
98 200.6 35.3 52.9#



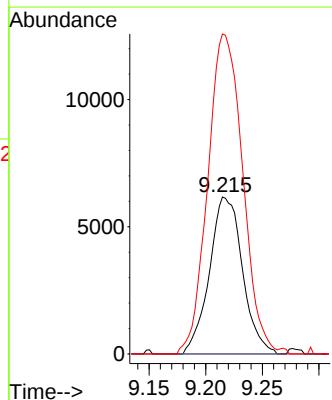
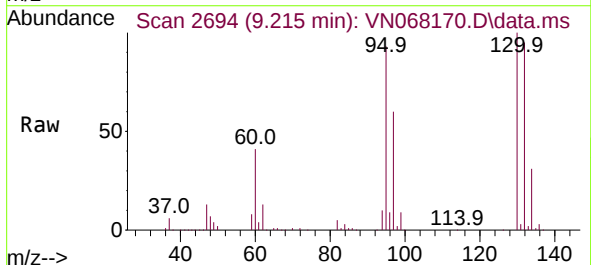


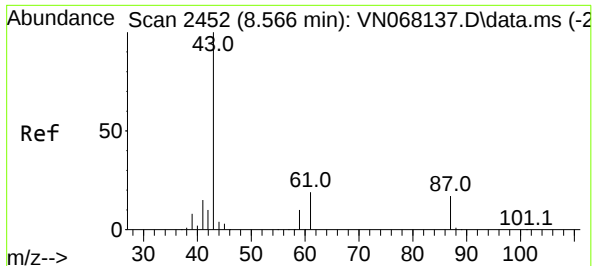

#43
Isopropyl Acetate
Concen: 0.526 ug/l
RT: 8.643 min Scan# 2481
Delta R.T. 0.077 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion: 43 Resp: 4080
Ion Ratio Lower Upper
43 100
61 0.0 19.0 28.4#
87 0.0 9.5 14.3#

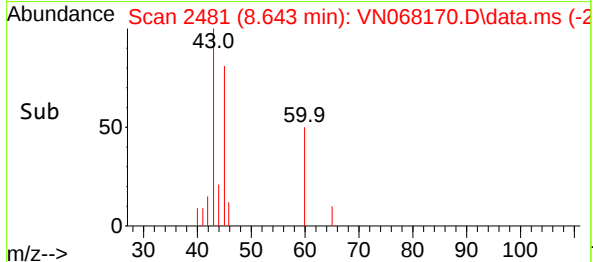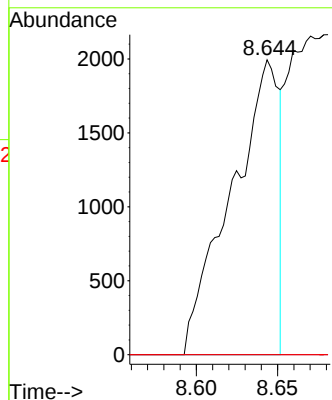

#44
Trichloroethene
Concen: 211.353 ug/l
RT: 9.217 min Scan# 2695
Delta R.T. -0.001 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion:130 Resp: 1101764
Ion Ratio Lower Upper
130 100
95 92.8 0.0 234.4


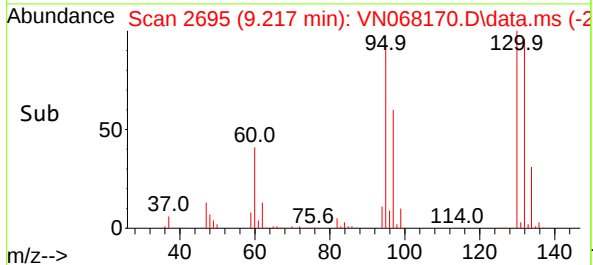
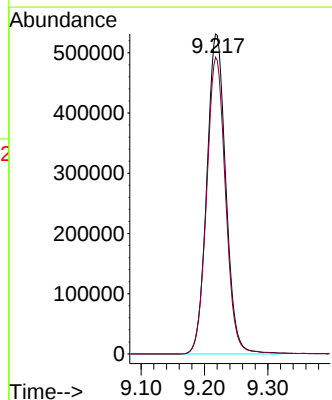
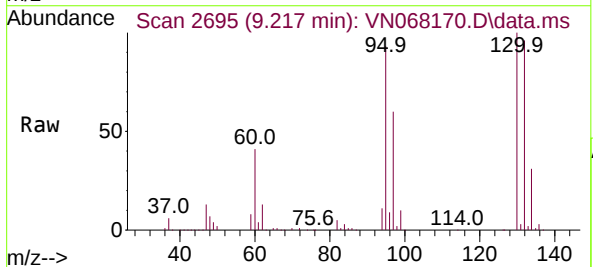




#45
1,2-Dichloropropane
Concen: 0.735 ug/l
RT: 9.217 min Scan# 2695
Delta R.T. -0.274 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion: 63 Resp: 2996
Ion Ratio Lower Upper
63 100
65 359.7 24.3 36.5#

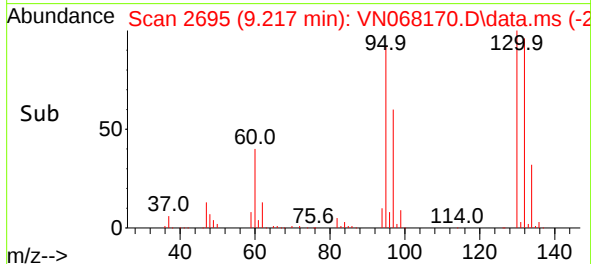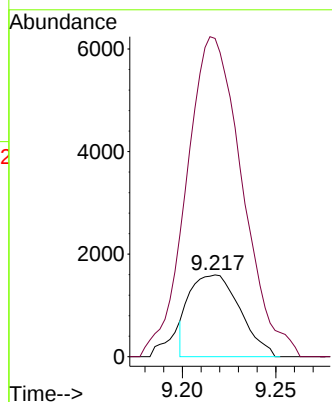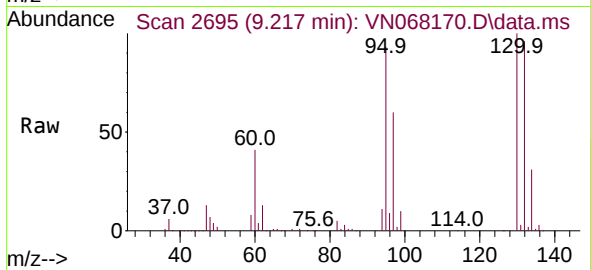

#49
1,4-Dioxane
Concen: 3.523 ug/l
RT: 9.571 min Scan# 2827
Delta R.T. -0.001 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion: 88 Resp: 275
Ion Ratio Lower Upper
88 100
43 72.4 28.8 43.2#
58 79.6 60.4 90.6


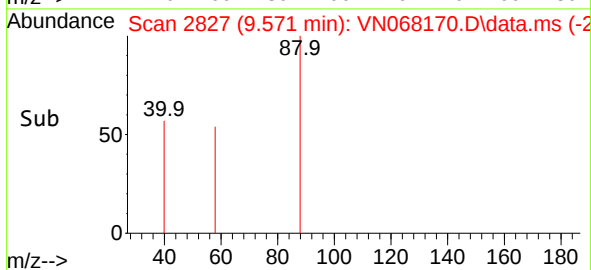
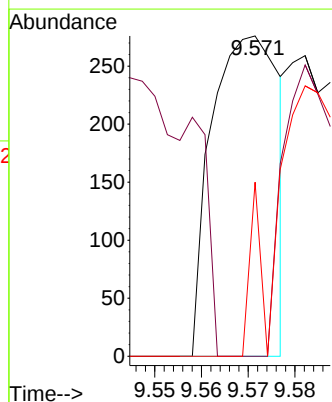





#50
Toluene-d8
Concen: 50.958 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion: 98 Resp: 846952
Ion Ratio Lower Upper
98 100
100 63.2 51.7 77.5

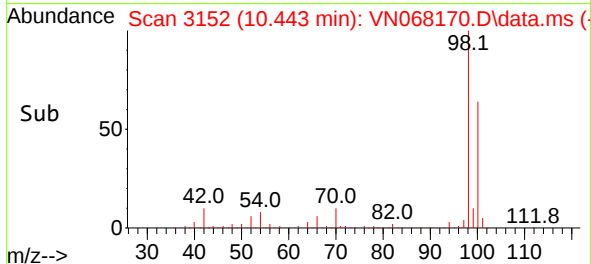

#55
1,1,2-Trichloroethane
Concen: 0.271 ug/l
RT: 10.904 min Scan# 3324
Delta R.T. 0.005 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion: 97 Resp: 1281
Ion Ratio Lower Upper
97 100
83 73.9 72.0 108.0
85 65.3 46.8 70.2
99 60.2 49.8 74.6


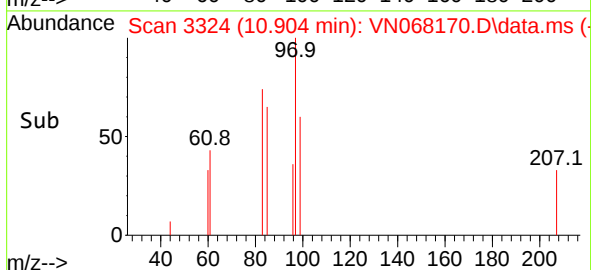
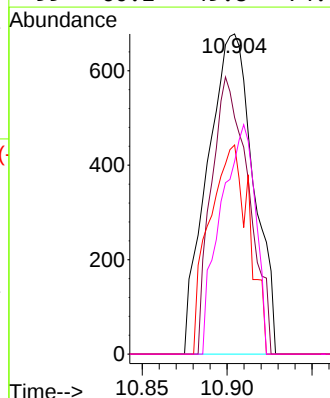
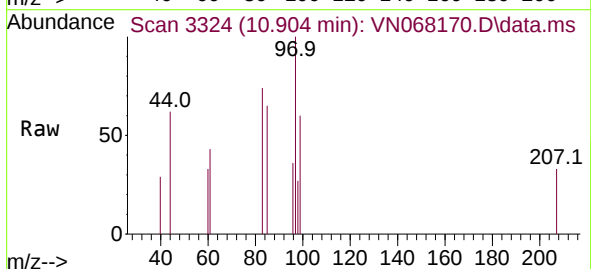




#60
Dibromochloromethane
Concen: 0.268 ug/l
RT: 10.982 min Scan# 3353
Delta R.T. -0.258 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion:129 Resp: 1428
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

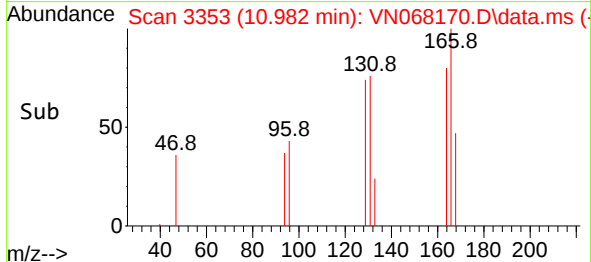

#62
4-Bromofluorobenzene
Concen: 49.444 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.002 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion: 95 Resp: 273574
Ion Ratio Lower Upper
95 100
174 91.3 0.0 122.0
176 87.8 0.0 117.6




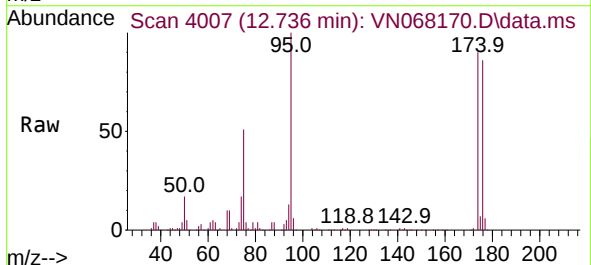




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. -0.000 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion:117 Resp: 690793
Ion Ratio Lower Upper
117 100
82 49.8 53.1 79.7#
119 32.3 25.5 38.3

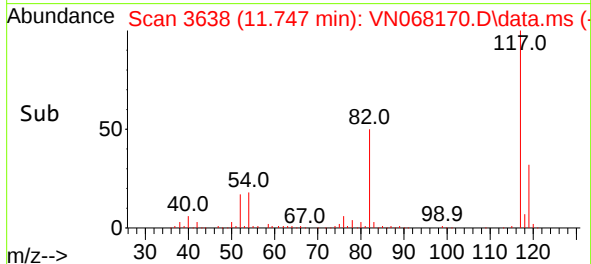

#64
Tetrachloroethene
Concen: 0.268 ug/l
RT: 10.977 min Scan# 3351
Delta R.T. -0.003 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion:164 Resp: 1432
Ion Ratio Lower Upper
164 100
166 102.9 102.1 153.1
129 78.5 86.9 130.3#
131 78.1 83.6 125.4#


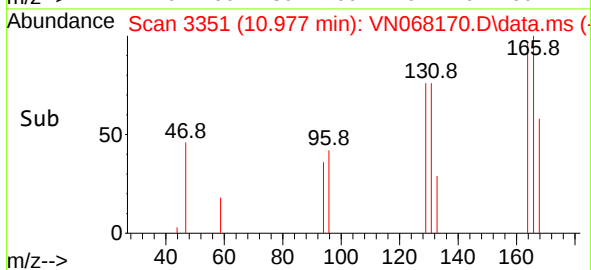




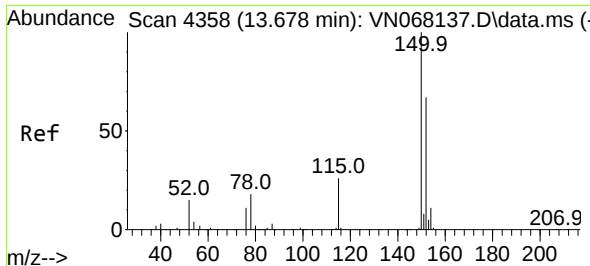

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.678 min Scan# 4358
 Delta R.T. -0.000 min
 Lab File: VN068170.D
 Acq: 18 Aug 2021 3:30




Instrument :
 MSVOA_N
 ClientSampleId :
 RW6B-GW-20210816


Tgt Ion:152 Resp: 260250
 Ion Ratio Lower Upper
 152 100
 115 54.7 36.1 108.5
 150 157.3 0.0 351.8

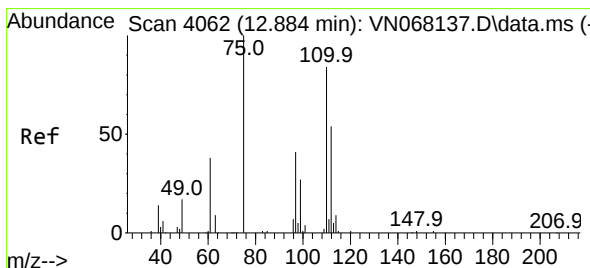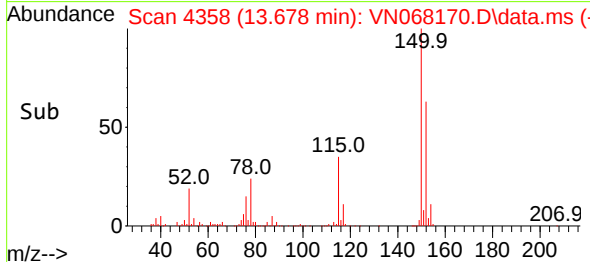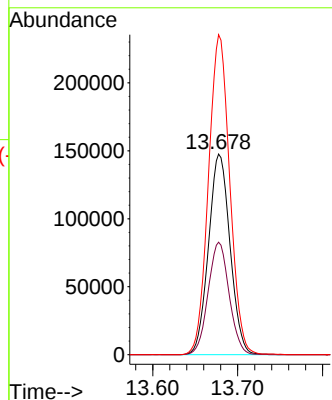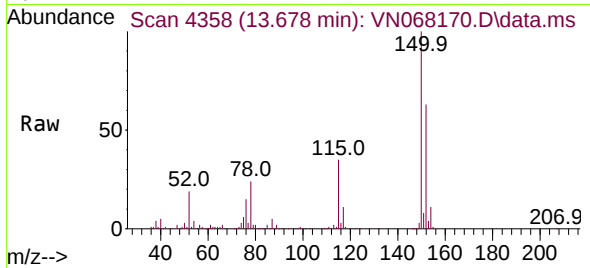

#76
 1,2,3-Trichloropropane
 Concen: 32.146 ug/l
 RT: 12.736 min Scan# 4007
 Delta R.T. -0.148 min
 Lab File: VN068170.D
 Acq: 18 Aug 2021 3:30

Tgt Ion: 75 Resp: 139050
 Ion Ratio Lower Upper
 75 100
 77 1.0 0.0 0.0#


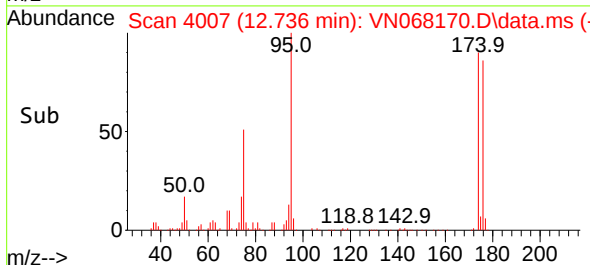
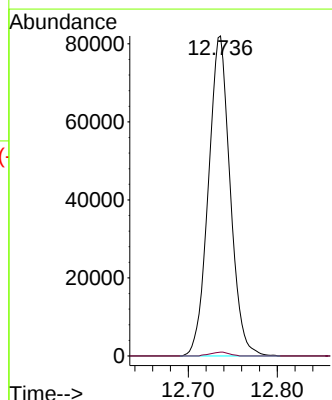
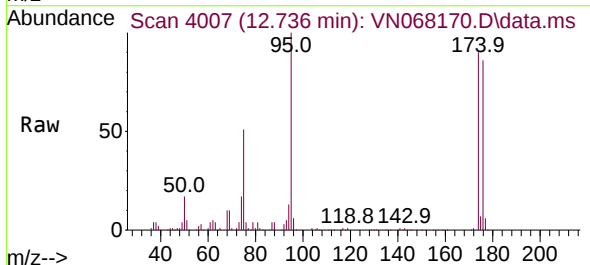




#81
trans-1,4-Dichloro-2-butene
Concen: 105.315 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.107 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30




Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816


Tgt Ion: 75 Resp: 139050
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

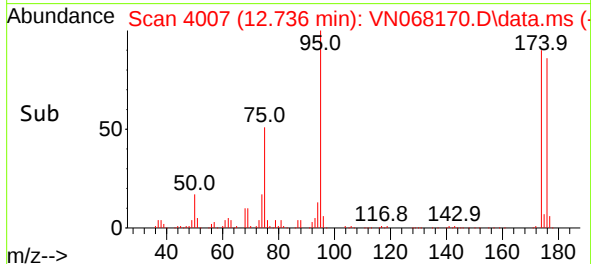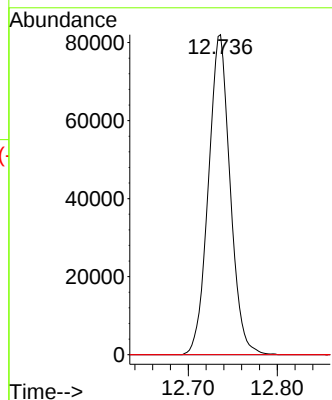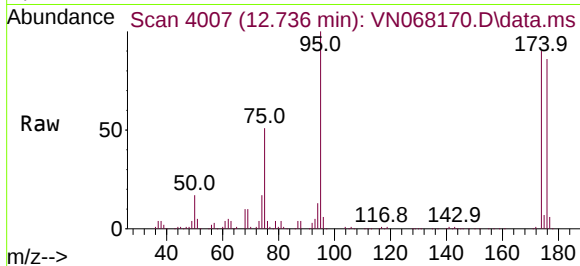

#93
1,2,4-Trichlorobenzene
Concen: 2.750 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion:180 Resp: 300
Ion Ratio Lower Upper
180 100
182 75.7 47.5 142.5
145 8.7 17.2 51.6#



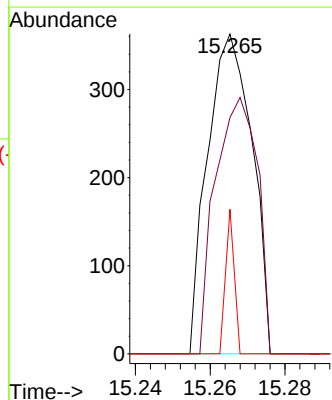
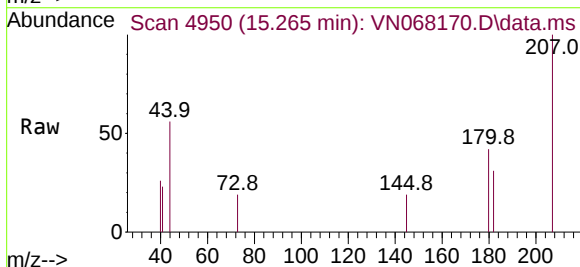




#95
Naphthalene
Concen: 3.486 ug/l
RT: 15.515 min Scan# 5043
Delta R.T. 0.008 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Instrument :
MSVOA_N
ClientSampleId :
RW6B-GW-20210816

Tgt Ion:128 Resp: 1553
Ion Ratio Lower Upper
128 100
127 0.0 10.6 15.8#
129 0.0 8.6 12.8#

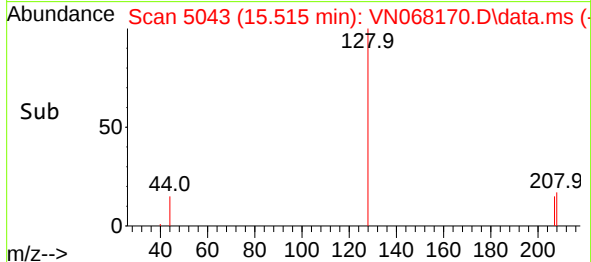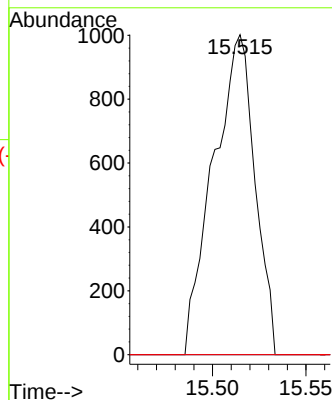

#96
1,2,3-Trichlorobenzene
Concen: 2.900 ug/l
RT: 15.702 min Scan# 5113
Delta R.T. -0.001 min
Lab File: VN068170.D
Acq: 18 Aug 2021 3:30

Tgt Ion:180 Resp: 298
Ion Ratio Lower Upper
180 100
182 65.1 47.8 143.3
145 0.0 18.2 54.6#

