

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081721\
 Data File : VN068168.D
 Acq On : 18 Aug 2021 2:41
 Operator : JC/MD
 Sample : M3446-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RW6B-TB-20210816

Quant Time: Aug 18 08:41:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 13:09:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	413668	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.971	114	700530	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	684024	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	270126	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	240508	54.452	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 108.900%	
35) Dibromofluoromethane	8.024	113	214927	48.868	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 97.740%	
50) Toluene-d8	10.446	98	837576	49.980	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 99.960%	
62) 4-Bromofluorobenzene	12.733	95	279353	50.074	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 100.140%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081721\
Data File : VN068168.D
Acq On : 18 Aug 2021 2:41
Operator : JC/MD
Sample : M3446-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RW6B-TB-20210816

Quant Time: Aug 18 08:41:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 13:09:49 2021
Response via : Initial Calibration




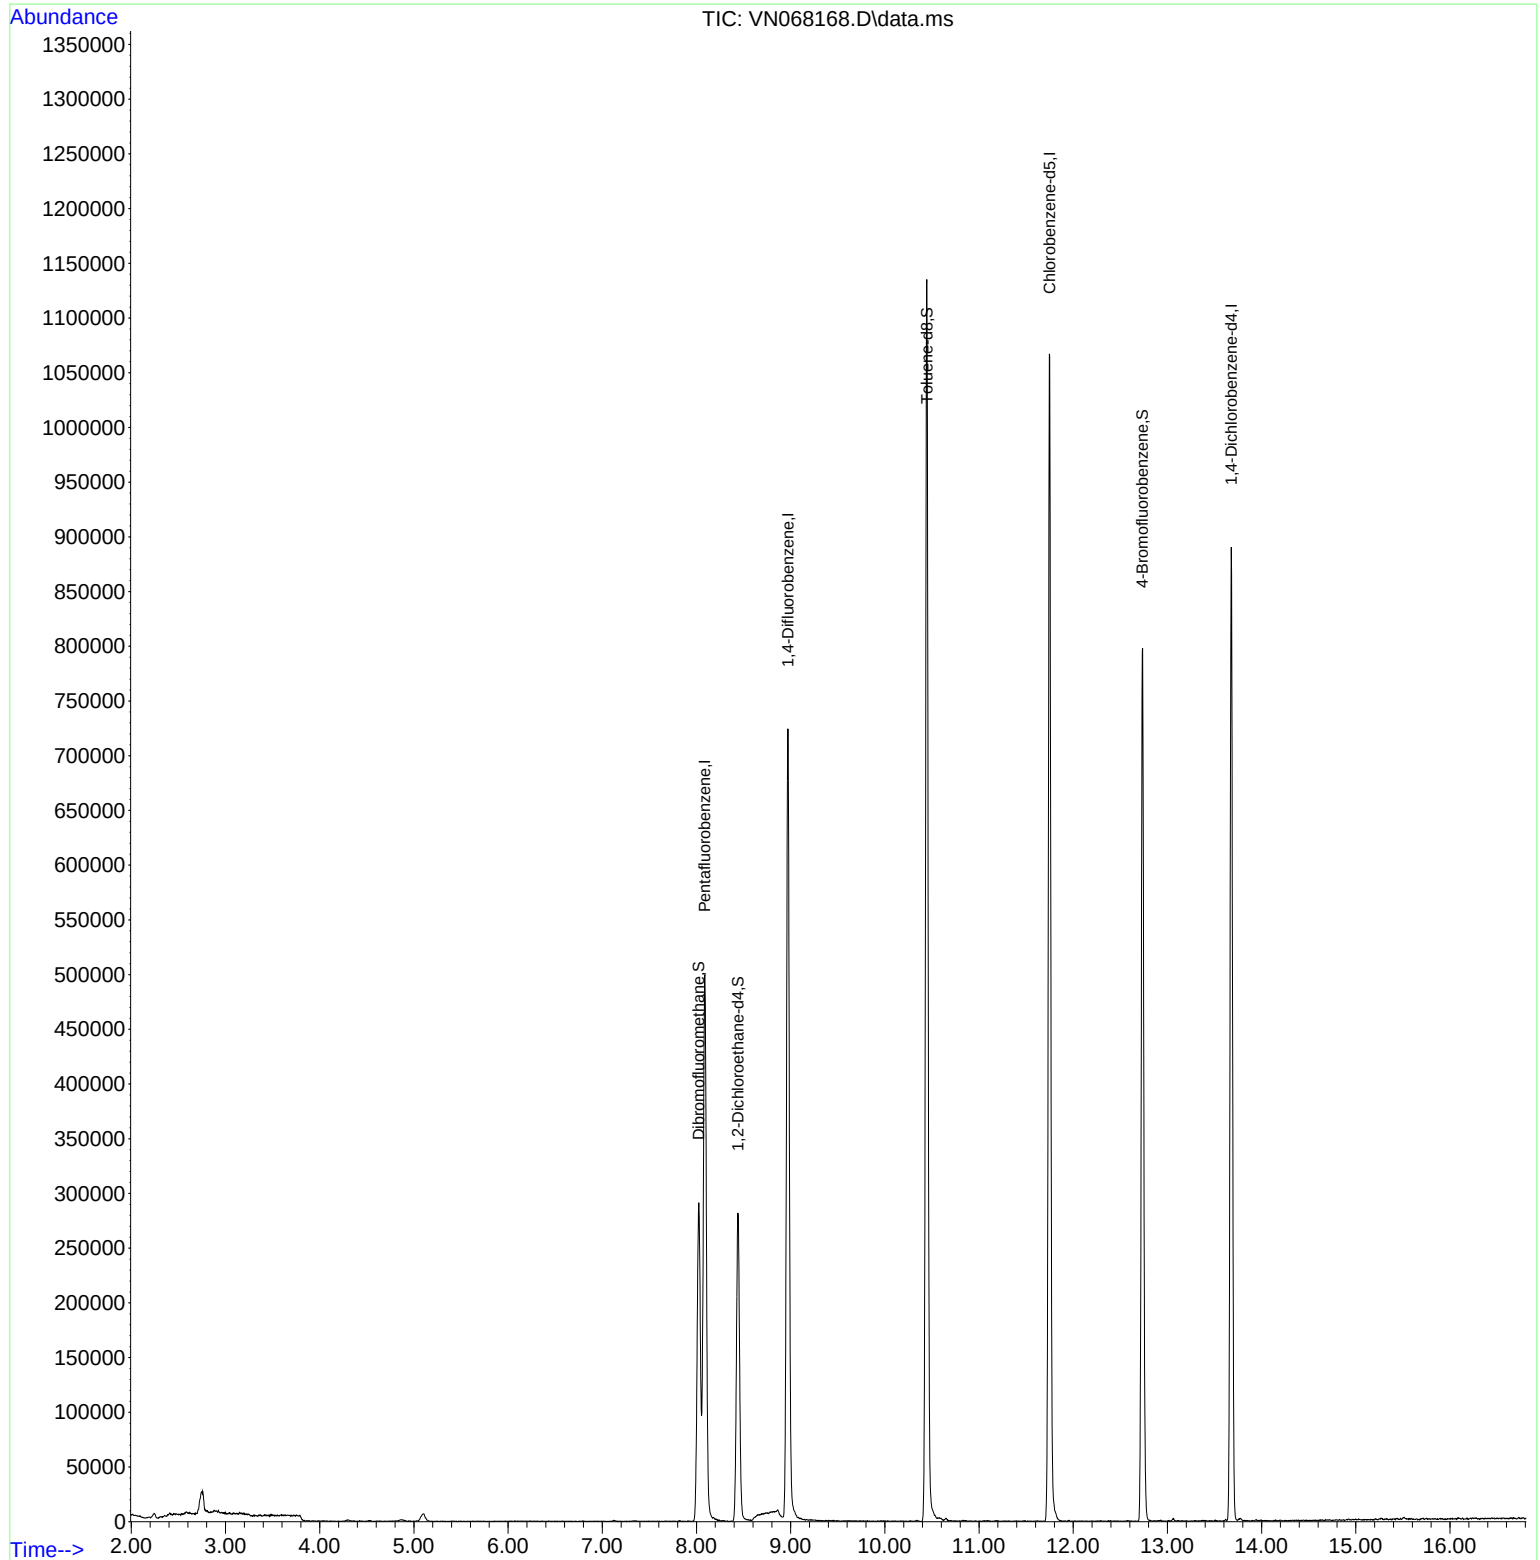


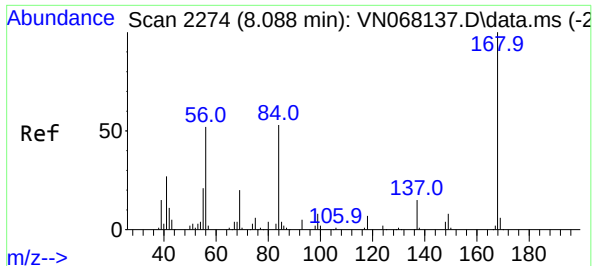

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.000 min
Lab File: VN068168.D
Acq: 18 Aug 2021 2:41




Instrument :
MSVOA_N
ClientSampleId :
RW6B-TB-20210816


Tgt Ion:168 Resp: 413668
Ion Ratio Lower Upper
168 100
99 52.0 62.9 94.3#

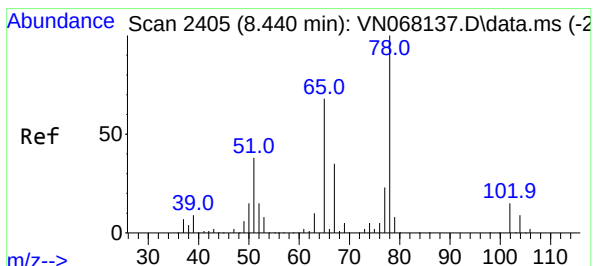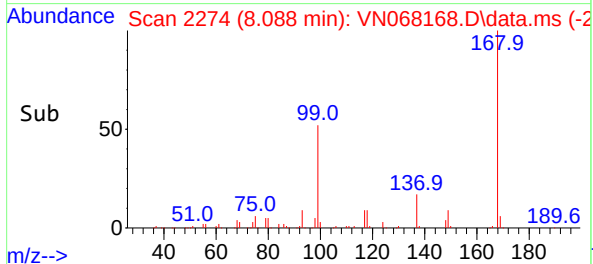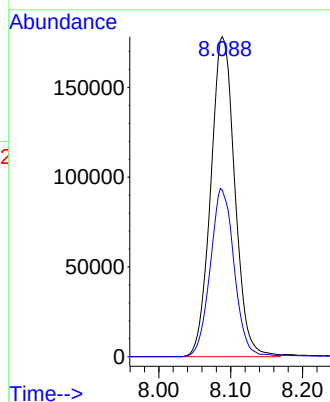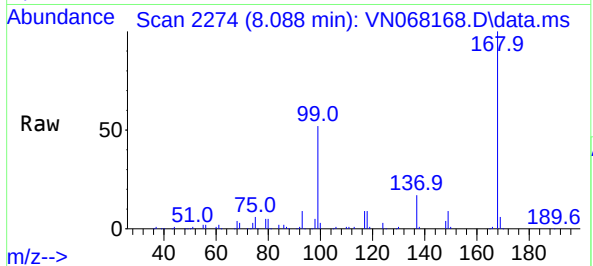

#33
1,2-Dichloroethane-d4
Concen: 54.452 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN068168.D
Acq: 18 Aug 2021 2:41

Tgt Ion: 65 Resp: 240508
Ion Ratio Lower Upper
65 100
67 50.9 0.0 98.6


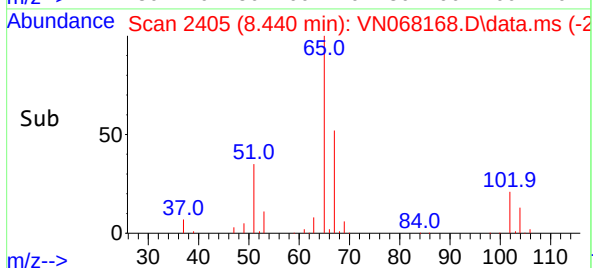
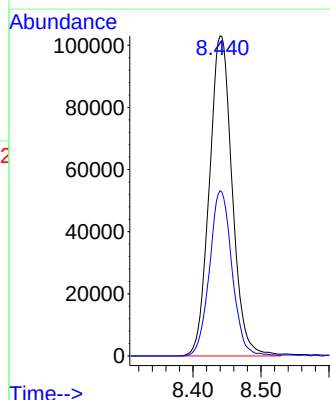
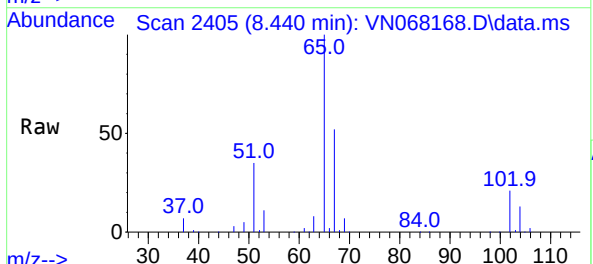


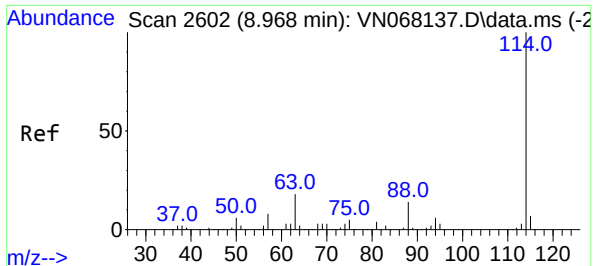

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN068168.D
Acq: 18 Aug 2021 2:41




Instrument :
MSVOA_N
ClientSampleId :
RW6B-TB-20210816


Tgt Ion:114 Resp: 700530
Ion Ratio Lower Upper
114 100
63 16.7 0.0 49.0
88 14.3 0.0 36.6

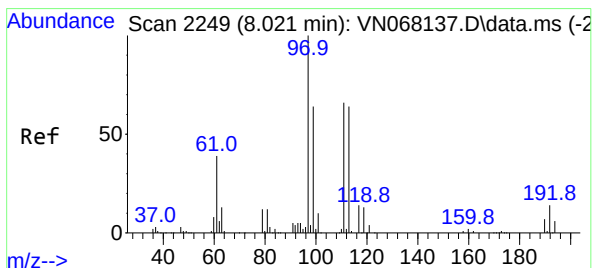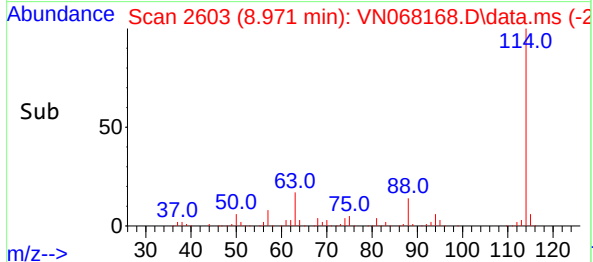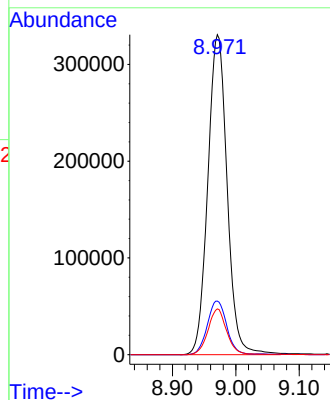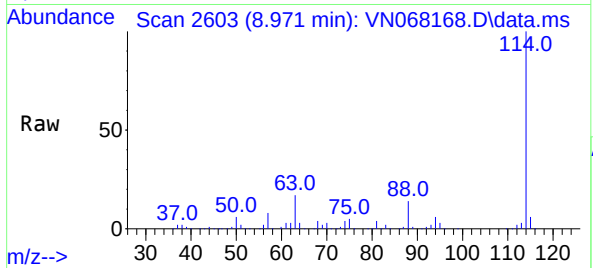

#35
Dibromofluoromethane
Concen: 48.868 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN068168.D
Acq: 18 Aug 2021 2:41

Tgt Ion:113 Resp: 214927
Ion Ratio Lower Upper
113 100
111 102.4 83.8 125.8
192 20.9 13.4 20.0#


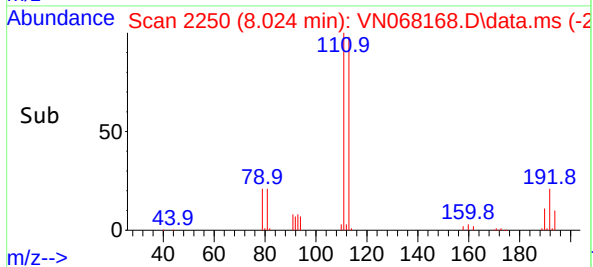
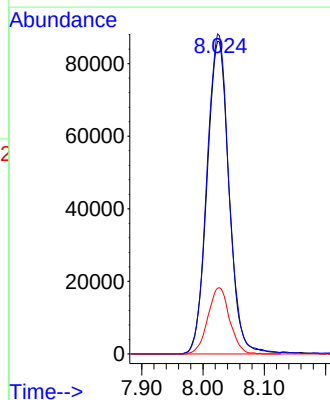
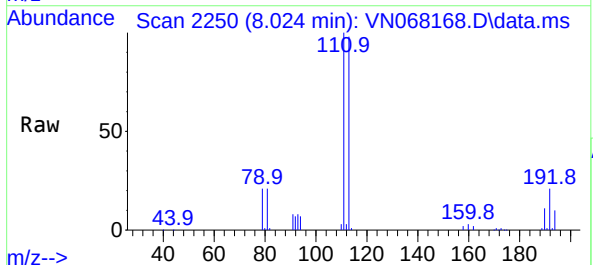


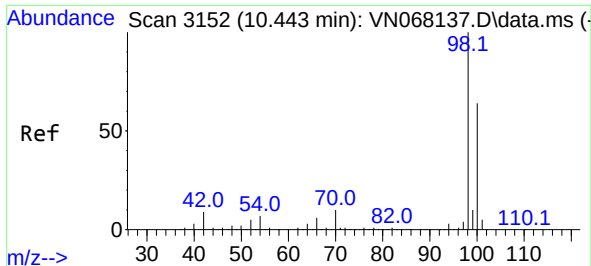

#50
Toluene-d8
Concen: 49.980 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN068168.D
Acq: 18 Aug 2021 2:41




Instrument :
MSVOA_N
ClientSampleId :
RW6B-TB-20210816


Tgt Ion: 98 Resp: 837576
Ion Ratio Lower Upper
98 100
100 63.6 51.7 77.5

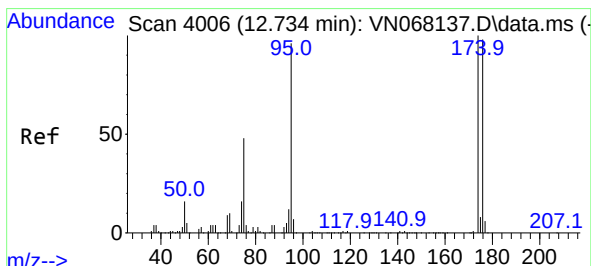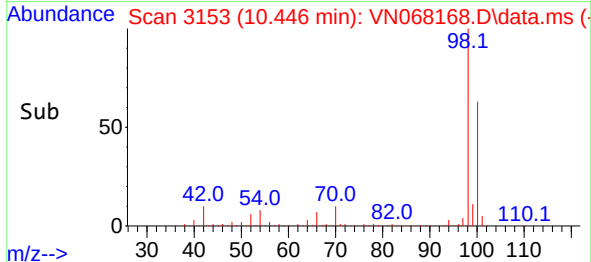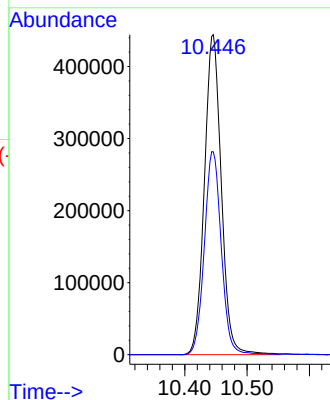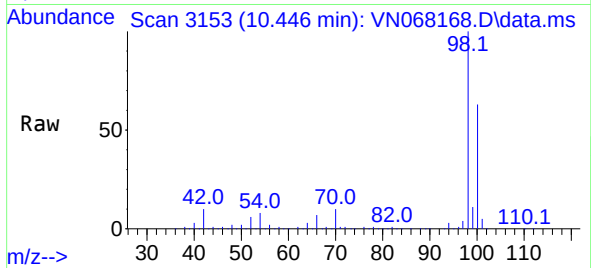

#62
4-Bromofluorobenzene
Concen: 50.074 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.001 min
Lab File: VN068168.D
Acq: 18 Aug 2021 2:41

Tgt Ion: 95 Resp: 279353
Ion Ratio Lower Upper
95 100
174 90.8 0.0 122.0
176 87.3 0.0 117.6


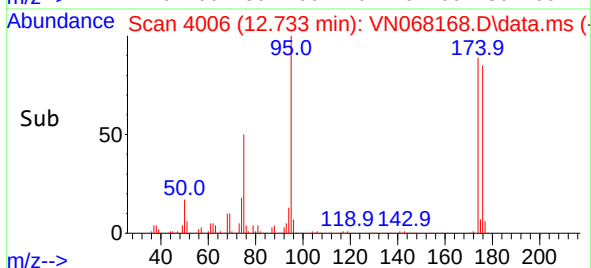
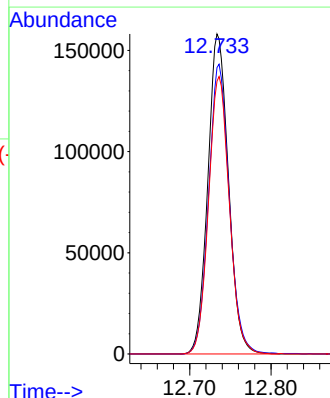
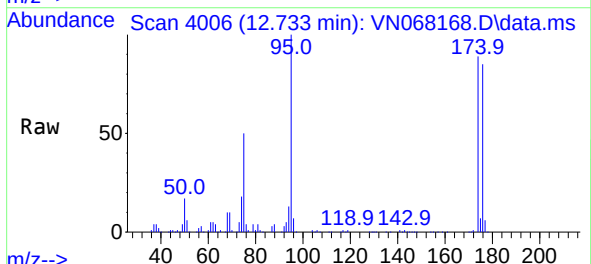


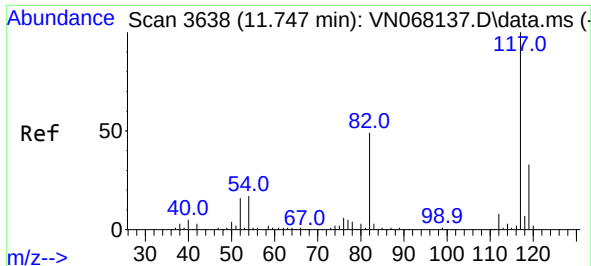

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.002 min
Lab File: VN068168.D
Acq: 18 Aug 2021 2:41

Instrument :
MSVOA_N
ClientSampleId :
RW6B-TB-20210816

Tgt Ion:117 Resp: 684024
Ion Ratio Lower Upper
117 100
82 50.6 53.1 79.7#
119 31.7 25.5 38.3

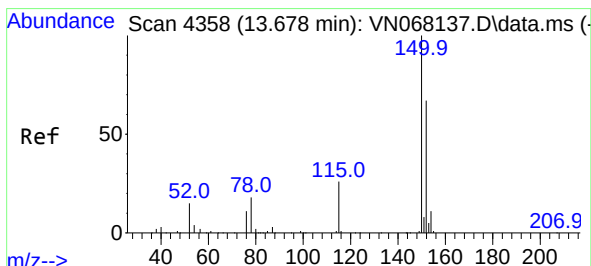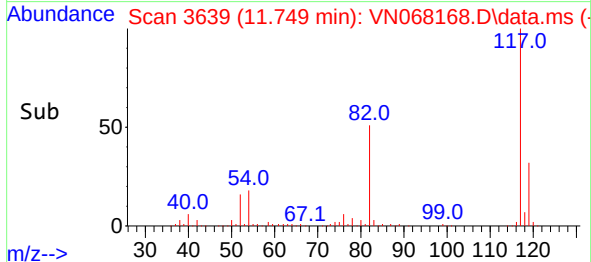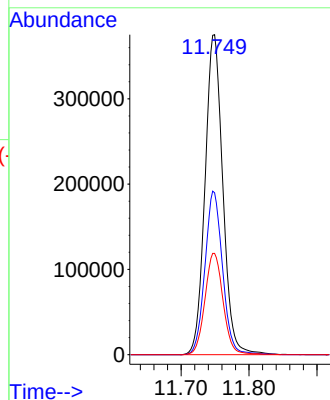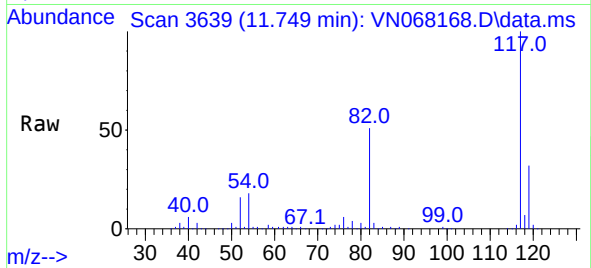

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. -0.000 min
Lab File: VN068168.D
Acq: 18 Aug 2021 2:41

Tgt Ion:152 Resp: 270126
Ion Ratio Lower Upper
152 100
115 54.9 36.1 108.5
150 155.8 0.0 351.8

