

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081721\
 Data File : VN068178.D
 Acq On : 18 Aug 2021 6:47
 Operator : JC/MD
 Sample : M3432-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: Aug 18 08:42:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081721W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 17 13:09:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	394560	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.971	114	661069	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	651569	50.000	ug/l	# 0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	248380	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	225291	53.477	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	106.960%
35) Dibromofluoromethane	8.024	113	203574	49.050	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	98.100%
50) Toluene-d8	10.446	98	790778	50.004	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	100.000%
62) 4-Bromofluorobenzene	12.736	95	257186	48.853	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	97.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081721\
Data File : VN068178.D
Acq On : 18 Aug 2021 6:47
Operator : JC/MD
Sample : M3432-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: Aug 18 08:42:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081721W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 17 13:09:49 2021
Response via : Initial Calibration




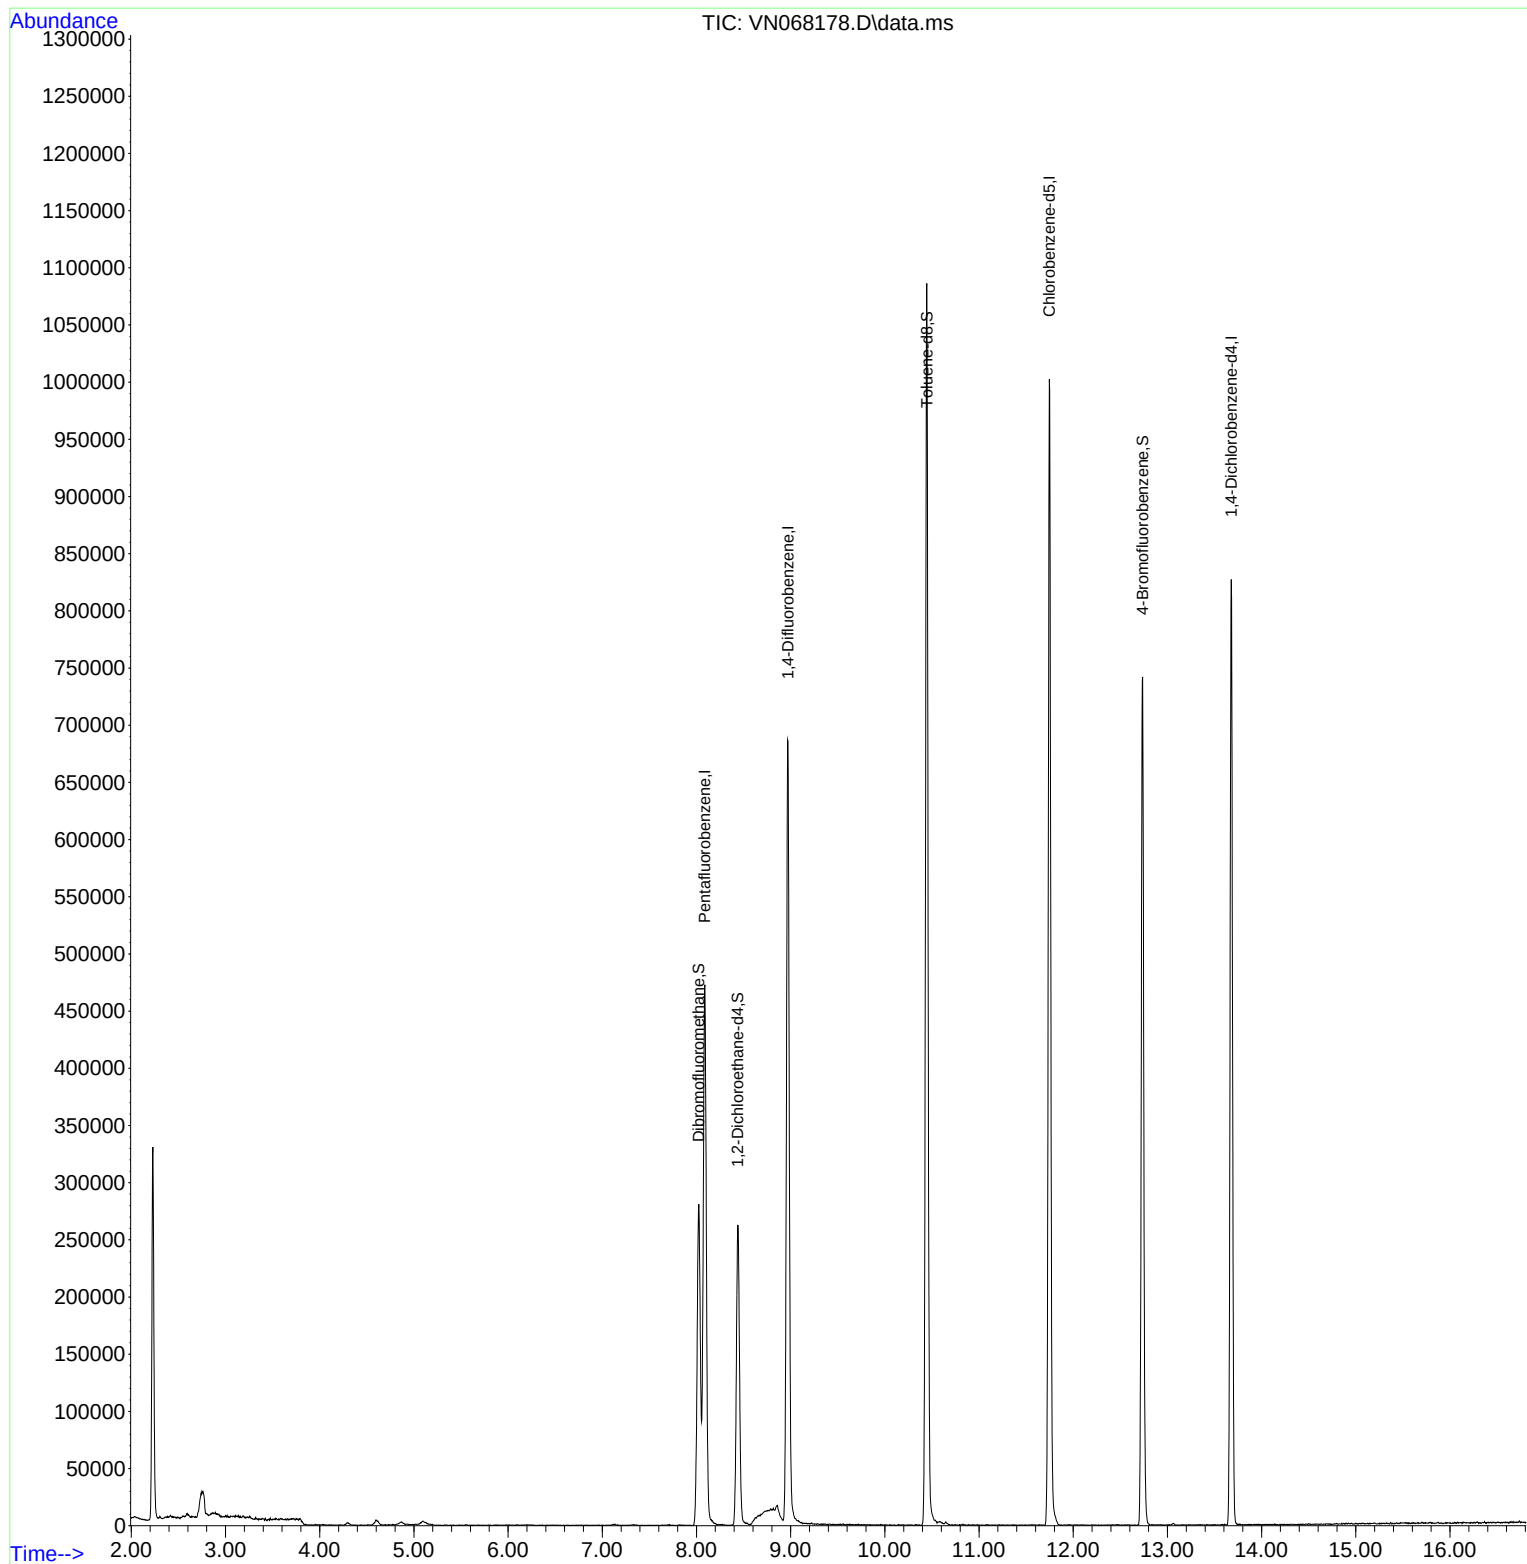


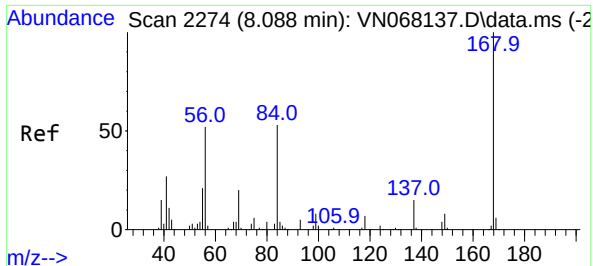

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.000 min
Lab File: VN068178.D
Acq: 18 Aug 2021 6:47




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:168 Resp: 394560
Ion Ratio Lower Upper
168 100
99 50.3 62.9 94.3#

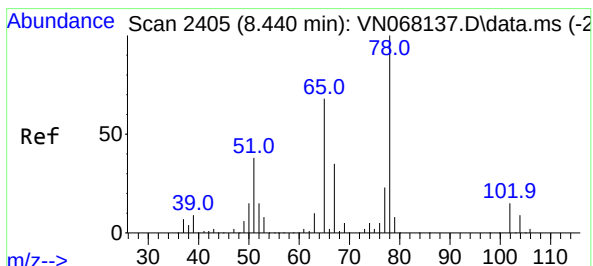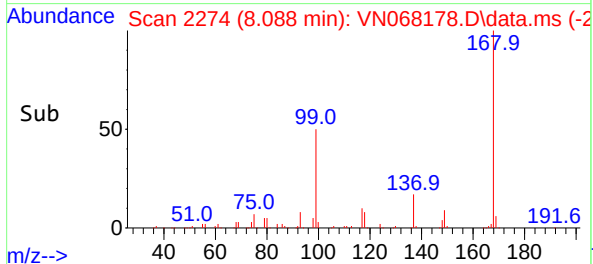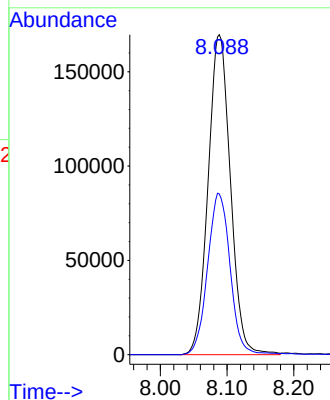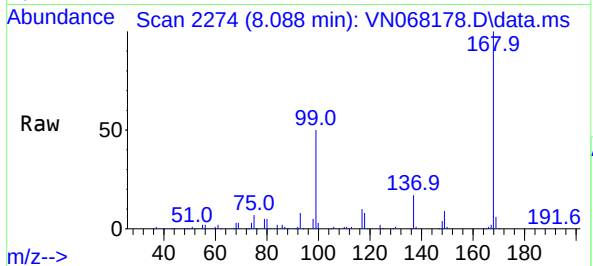

#33
1,2-Dichloroethane-d4
Concen: 53.477 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. -0.003 min
Lab File: VN068178.D
Acq: 18 Aug 2021 6:47

Tgt Ion: 65 Resp: 225291
Ion Ratio Lower Upper
65 100
67 50.3 0.0 98.6


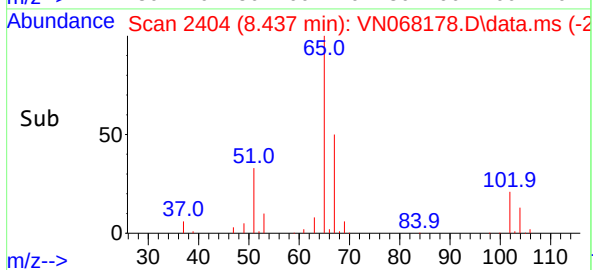
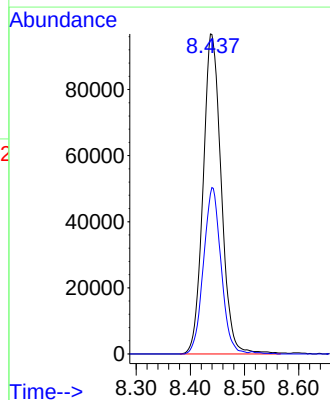
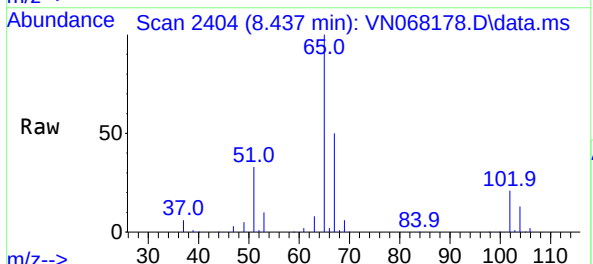


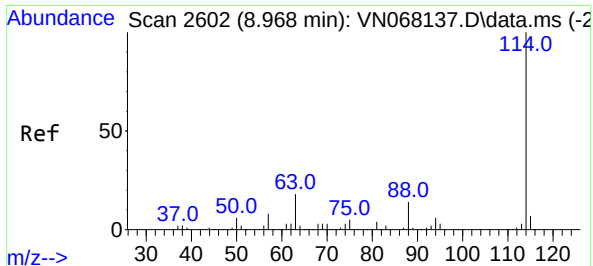

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN068178.D
Acq: 18 Aug 2021 6:47




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion:114 Resp: 661069
Ion Ratio Lower Upper
114 100
63 17.0 0.0 49.0
88 14.0 0.0 36.6

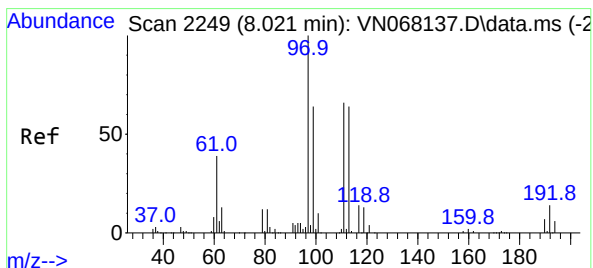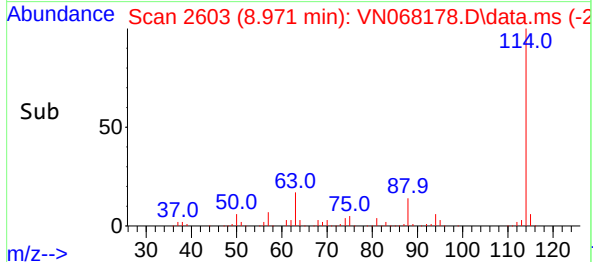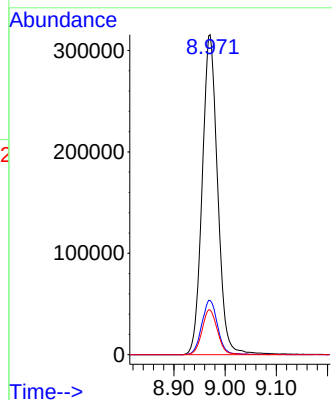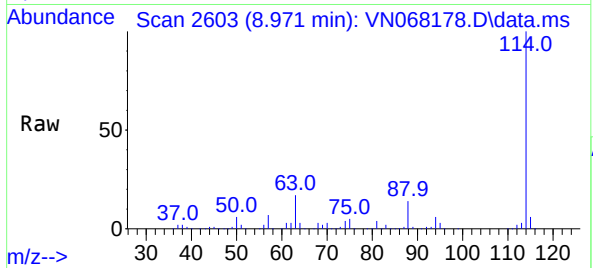

#35
Dibromofluoromethane
Concen: 49.050 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN068178.D
Acq: 18 Aug 2021 6:47

Tgt Ion:113 Resp: 203574
Ion Ratio Lower Upper
113 100
111 103.4 83.8 125.8
192 20.5 13.4 20.0#


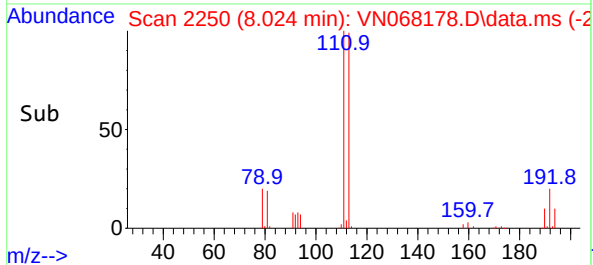
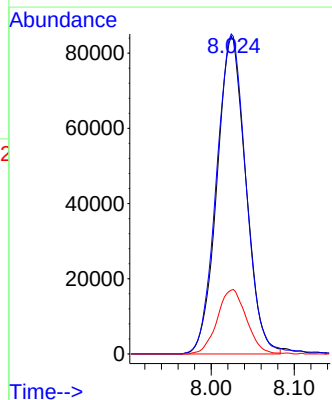
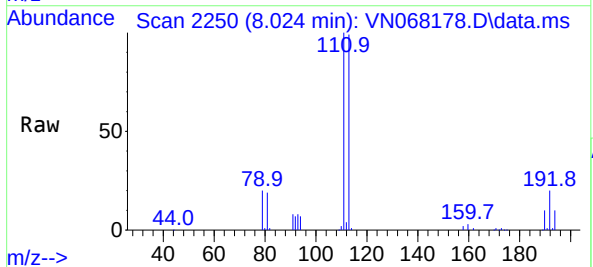


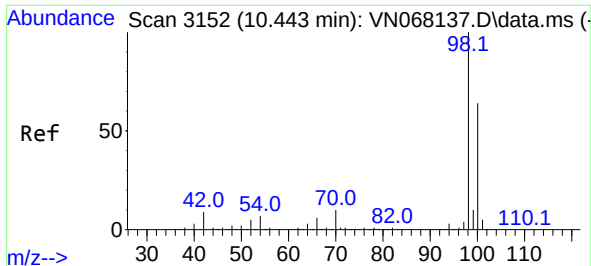

#50
Toluene-d8
Concen: 50.004 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN068178.D
Acq: 18 Aug 2021 6:47




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4


Tgt Ion: 98 Resp: 790778
Ion Ratio Lower Upper
98 100
100 63.5 51.7 77.5

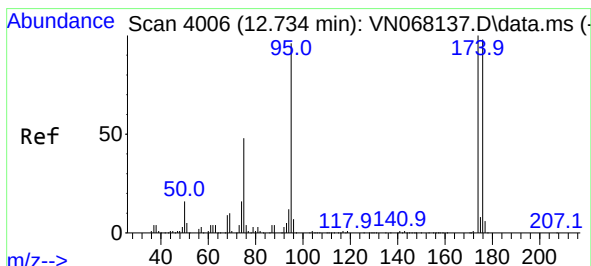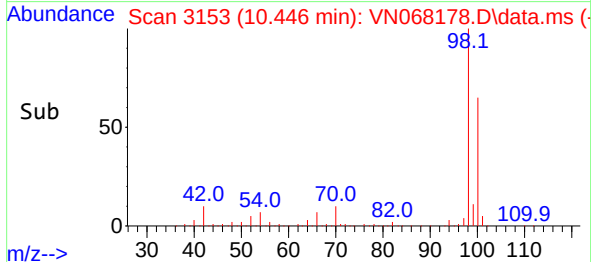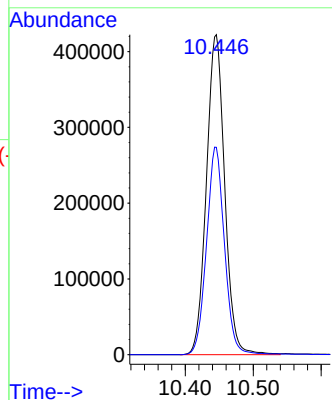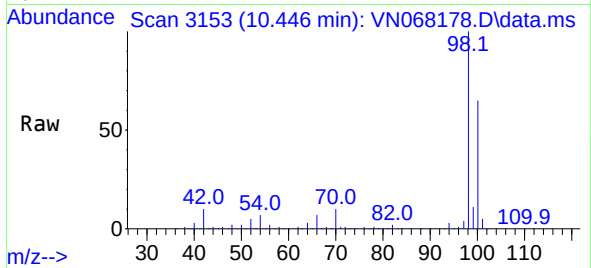

#62
4-Bromofluorobenzene
Concen: 48.853 ug/l
RT: 12.736 min Scan# 4007
Delta R.T. 0.002 min
Lab File: VN068178.D
Acq: 18 Aug 2021 6:47

Tgt Ion: 95 Resp: 257186
Ion Ratio Lower Upper
95 100
174 93.2 0.0 122.0
176 89.7 0.0 117.6


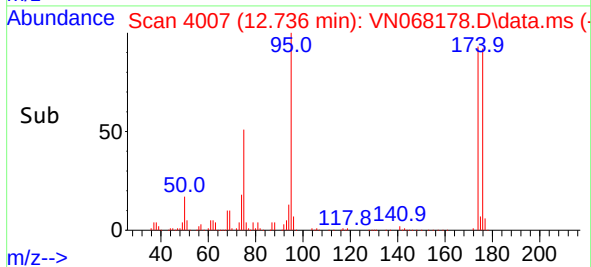
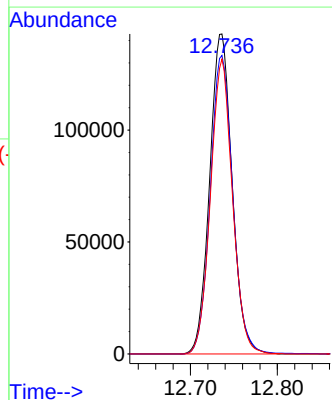
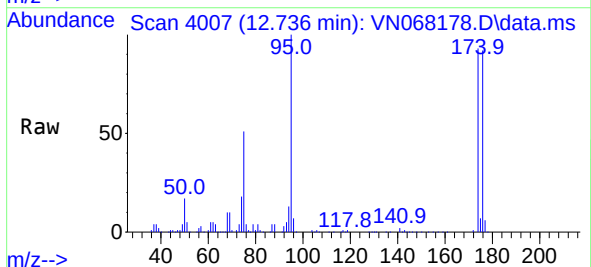


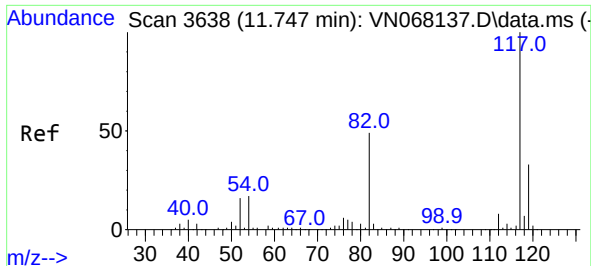

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.001 min
Lab File: VN068178.D
Acq: 18 Aug 2021 6:47

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tgt Ion:117 Resp: 651569
Ion Ratio Lower Upper
117 100
82 49.9 53.1 79.7#
119 32.2 25.5 38.3

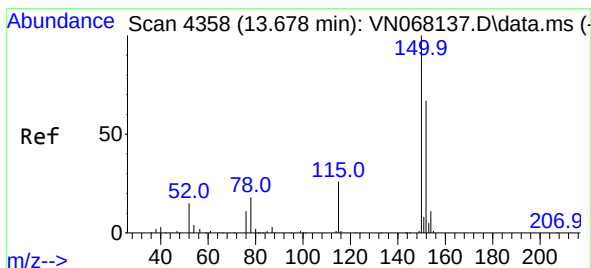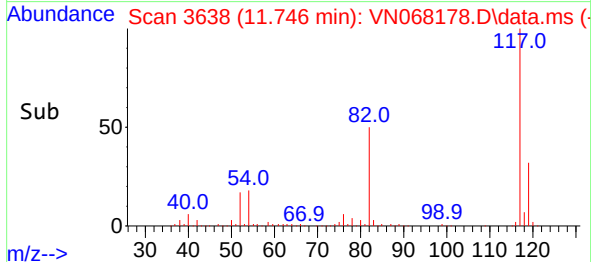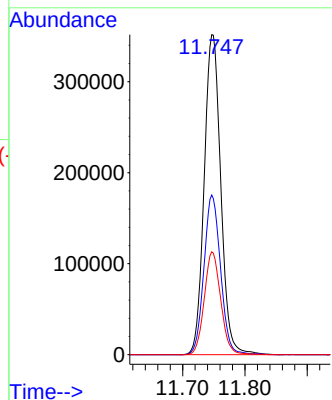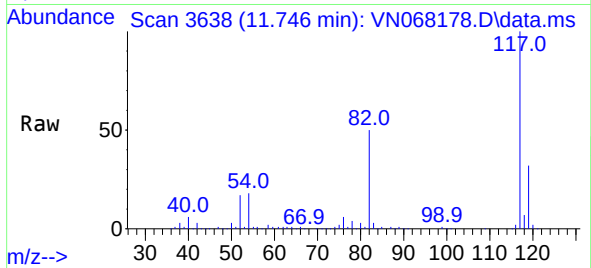

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. -0.000 min
Lab File: VN068178.D
Acq: 18 Aug 2021 6:47

Tgt Ion:152 Resp: 248380
Ion Ratio Lower Upper
152 100
115 55.9 36.1 108.5
150 157.0 0.0 351.8

