


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081721\
 Data File : VN068132.D
 Acq On : 17 Aug 2021 9:50
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081721W.M
 Title : SW846 8260
 Last Update : Tue Aug 17 13:09:49 2021

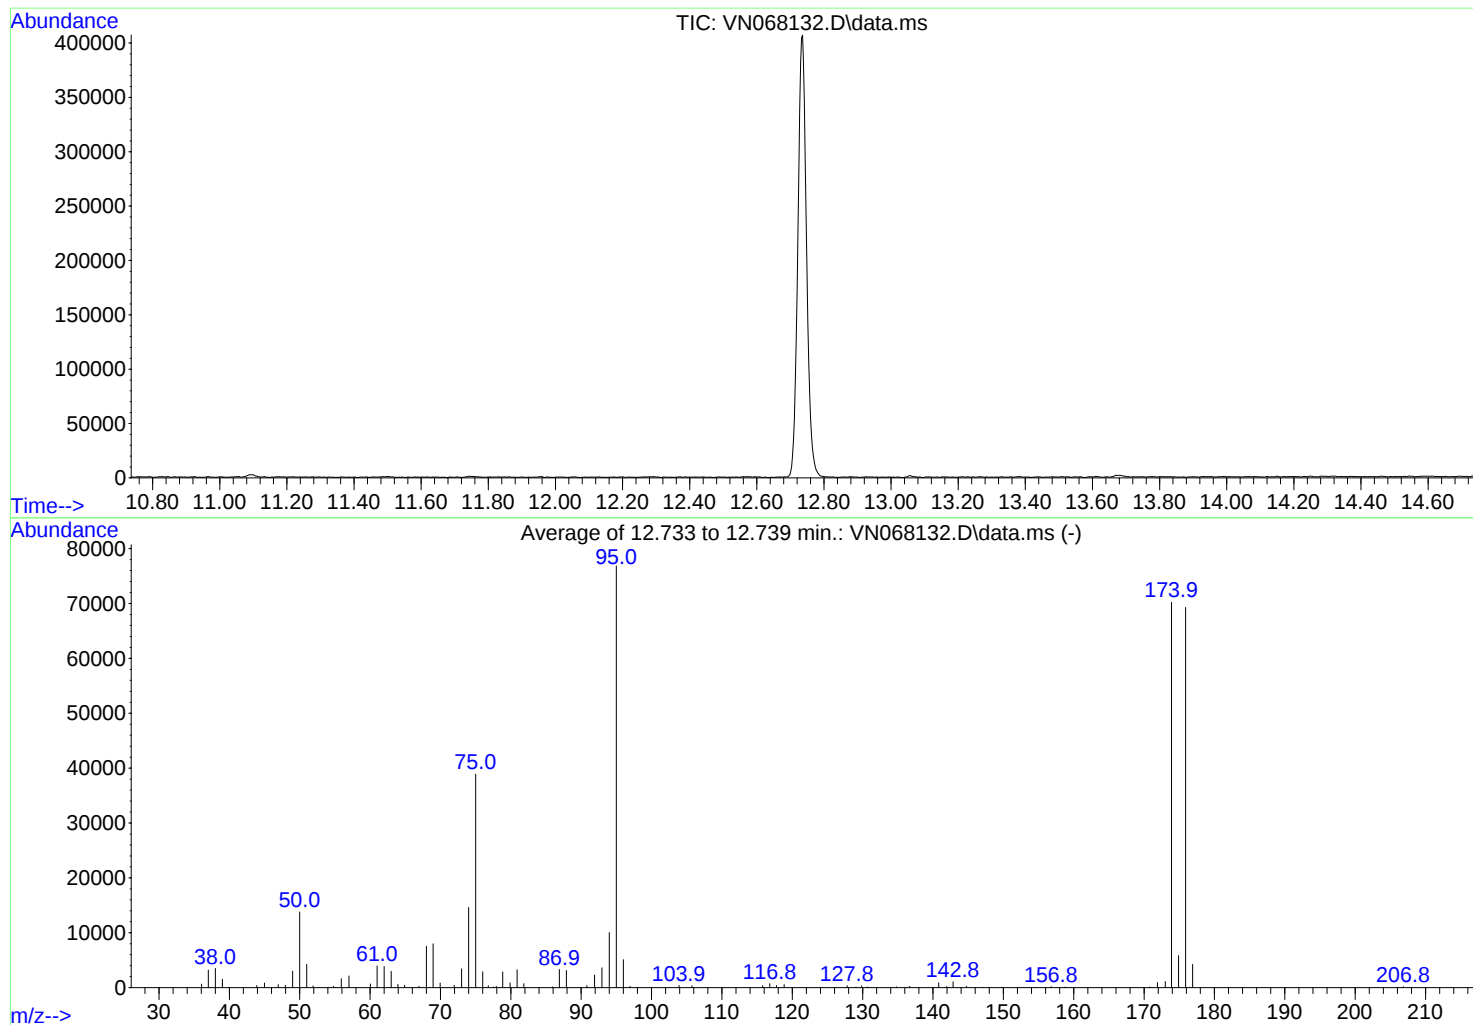

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3988

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	13796	PASS
75	95	30	60	50.6	38909	PASS
95	95	100	100	100.0	76861	PASS
96	95	5	9	6.6	5102	PASS
173	174	0.00	2	1.6	1120	PASS
174	95	50	100	91.3	70208	PASS
175	174	5	9	8.3	5837	PASS
176	174	95	101	98.7	69267	PASS
177	176	5	9	6.1	4221	PASS