


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081721\
Data File : VN068158.D
Acq On : 17 Aug 2021 21:47
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081721W.M
Title : SW846 8260
Last Update : Tue Aug 17 13:09:49 2021

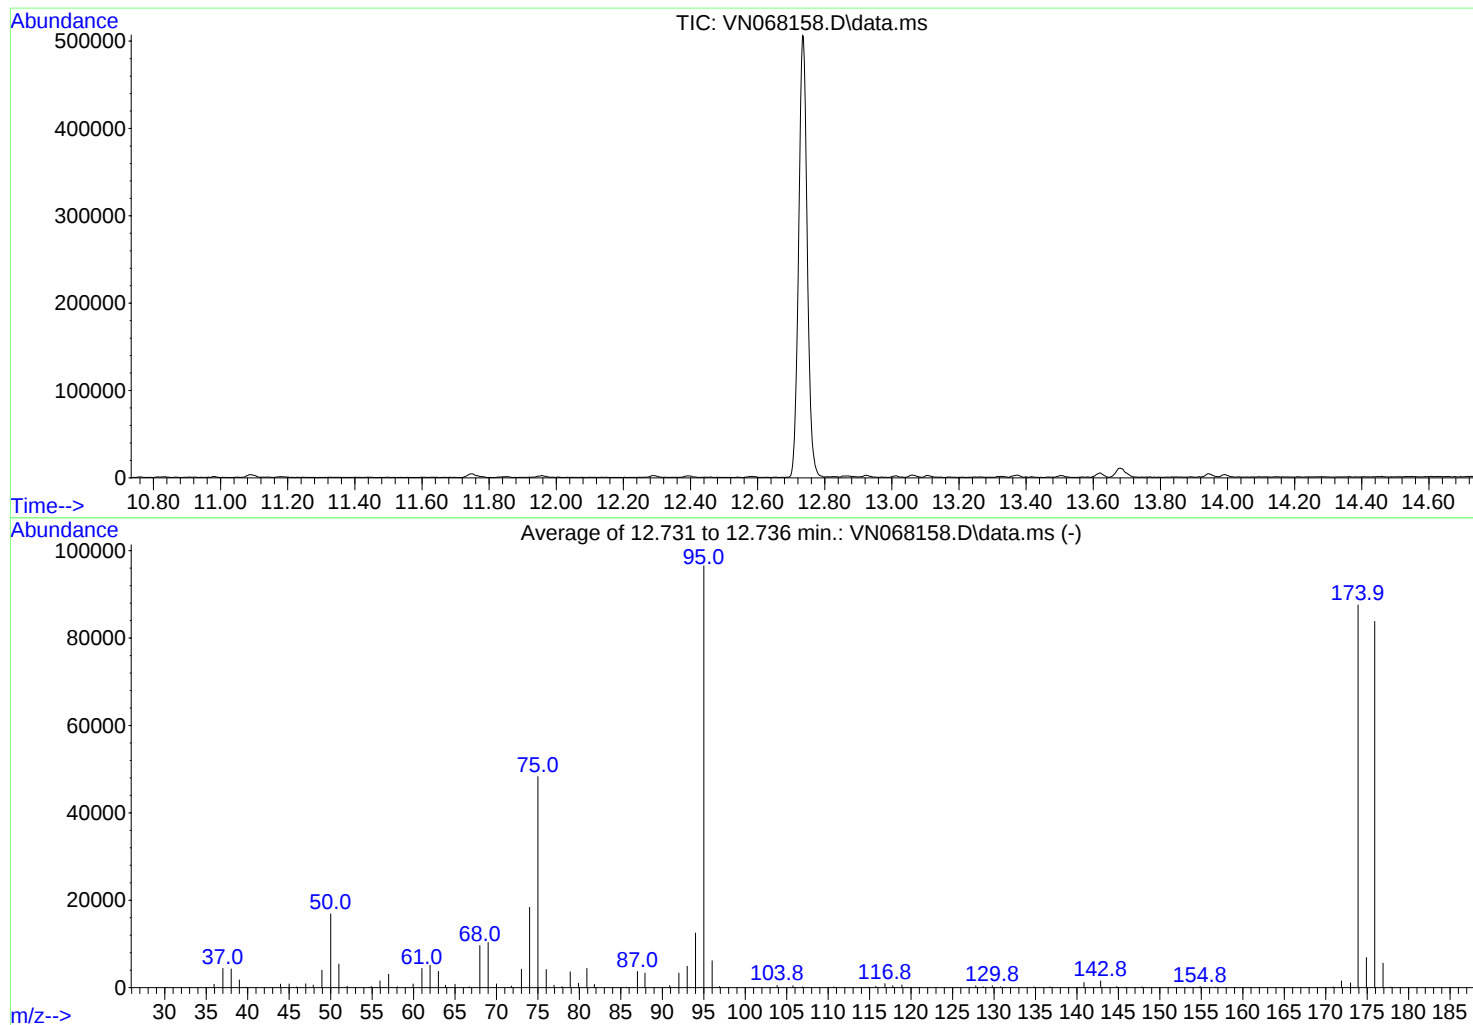

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	16880	PASS
75	95	30	60	50.0	48291	PASS
95	95	100	100	100.0	96533	PASS
96	95	5	9	6.4	6155	PASS
173	174	0.00	2	1.3	1110	PASS
174	95	50	100	90.7	87595	PASS
175	174	5	9	7.8	6872	PASS
176	174	95	101	95.7	83827	PASS
177	176	5	9	6.7	5588	PASS