


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081819\
Data File : VN057358.D
Acq On : 16 Aug 2019 16:17
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Title : SW846 8260
Last Update : Thu Aug 15 11:33:14 2019

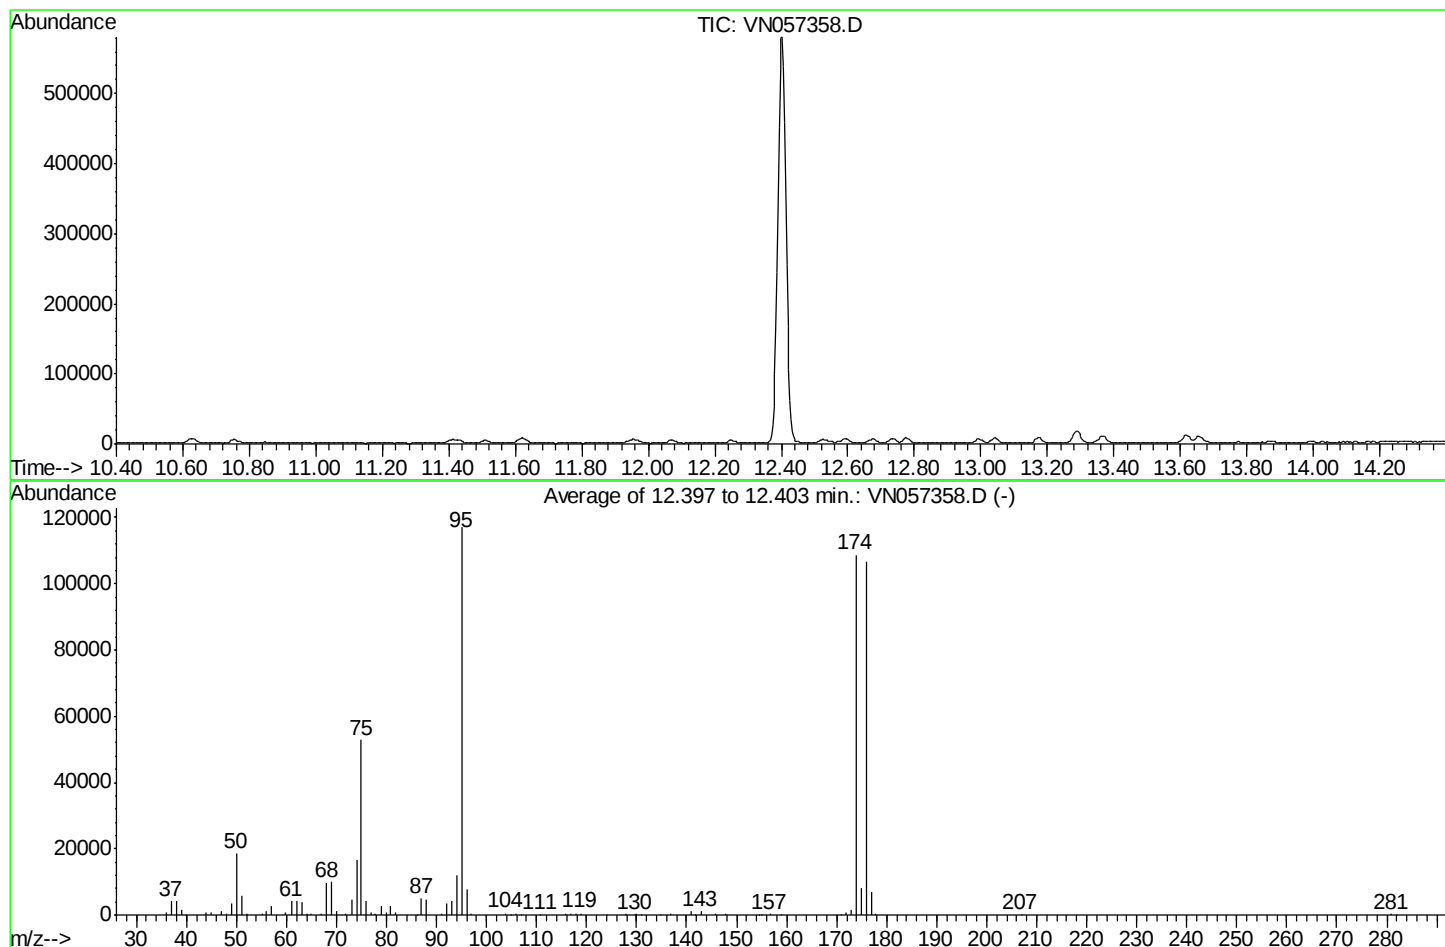

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	18453	PASS
75	95	30	60	45.2	52890	PASS
95	95	100	100	100.0	117021	PASS
96	95	5	9	6.5	7623	PASS
173	174	0.00	2	1.3	1461	PASS
174	95	50	100	92.8	108618	PASS
175	174	5	9	7.4	8015	PASS
176	174	95	101	98.1	106592	PASS
177	176	5	9	6.5	6918	PASS