



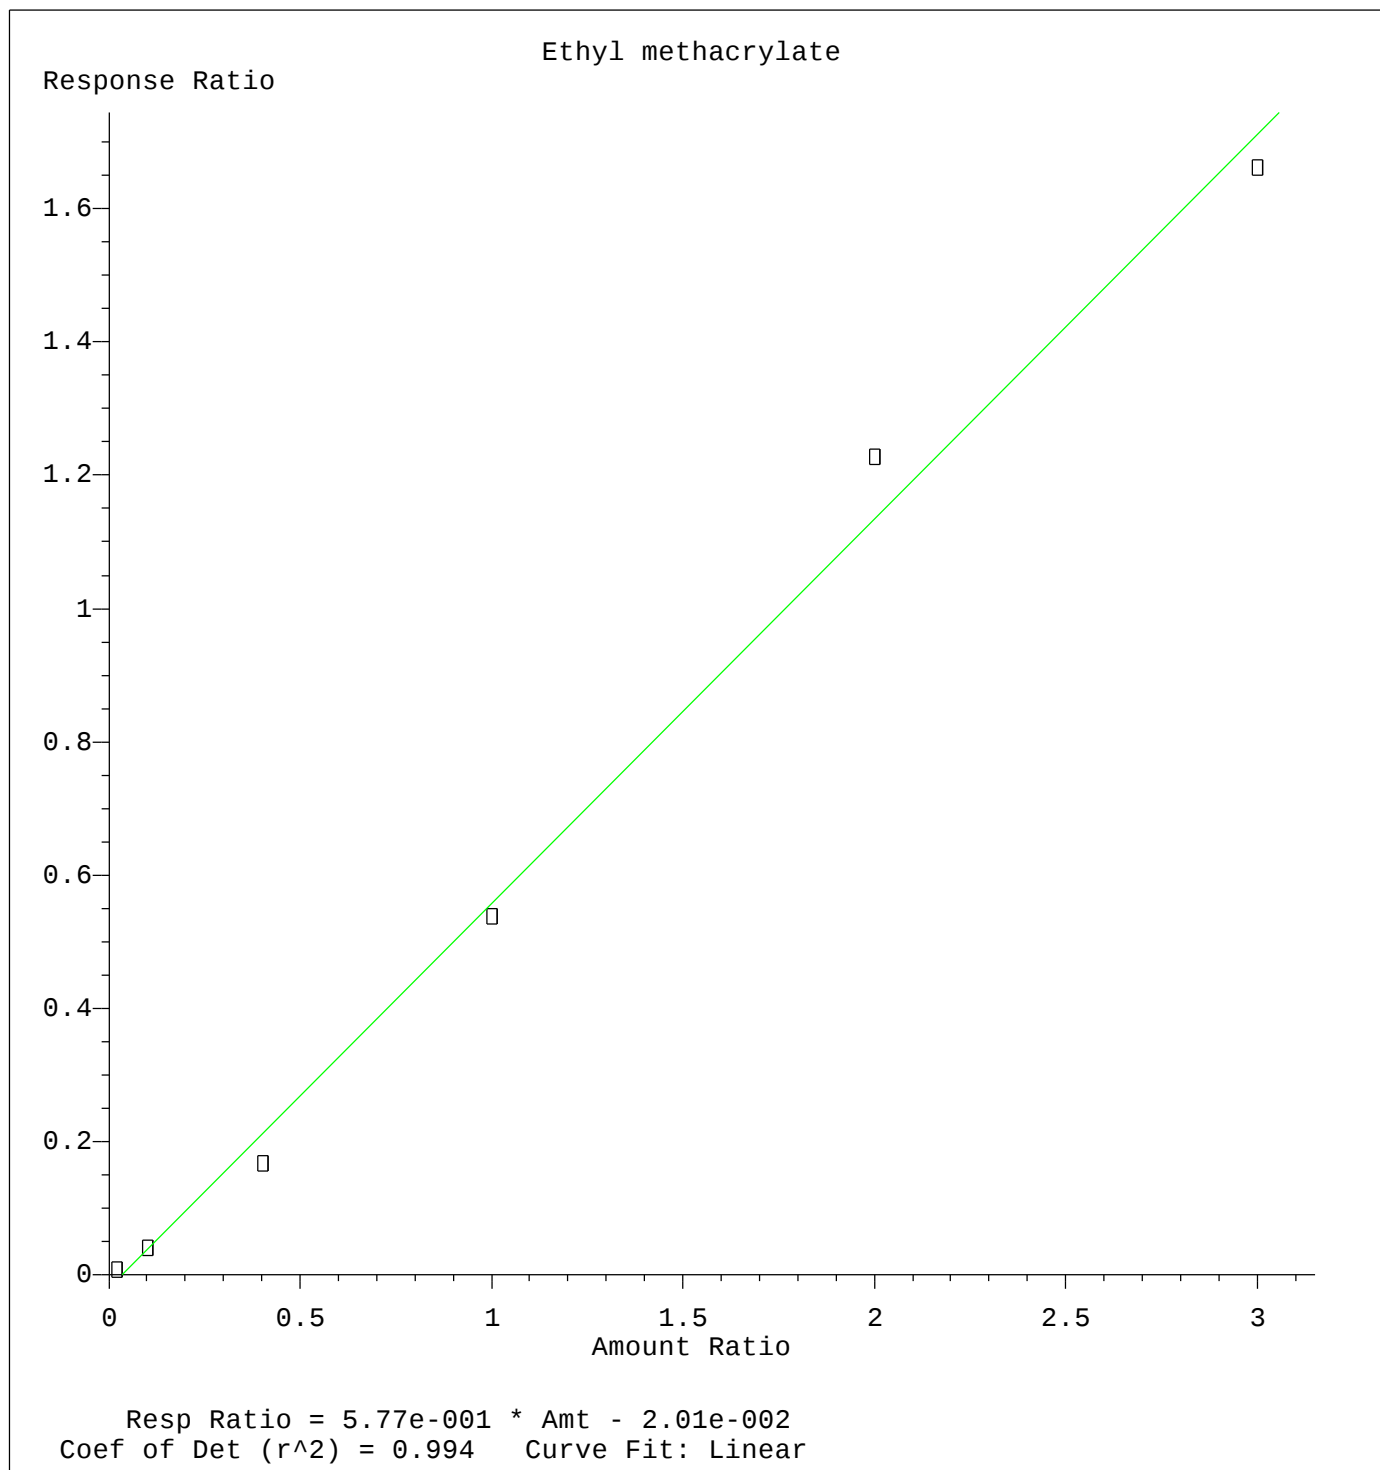

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020

2-Chloroethyl Vinyl ether

Response Ratio

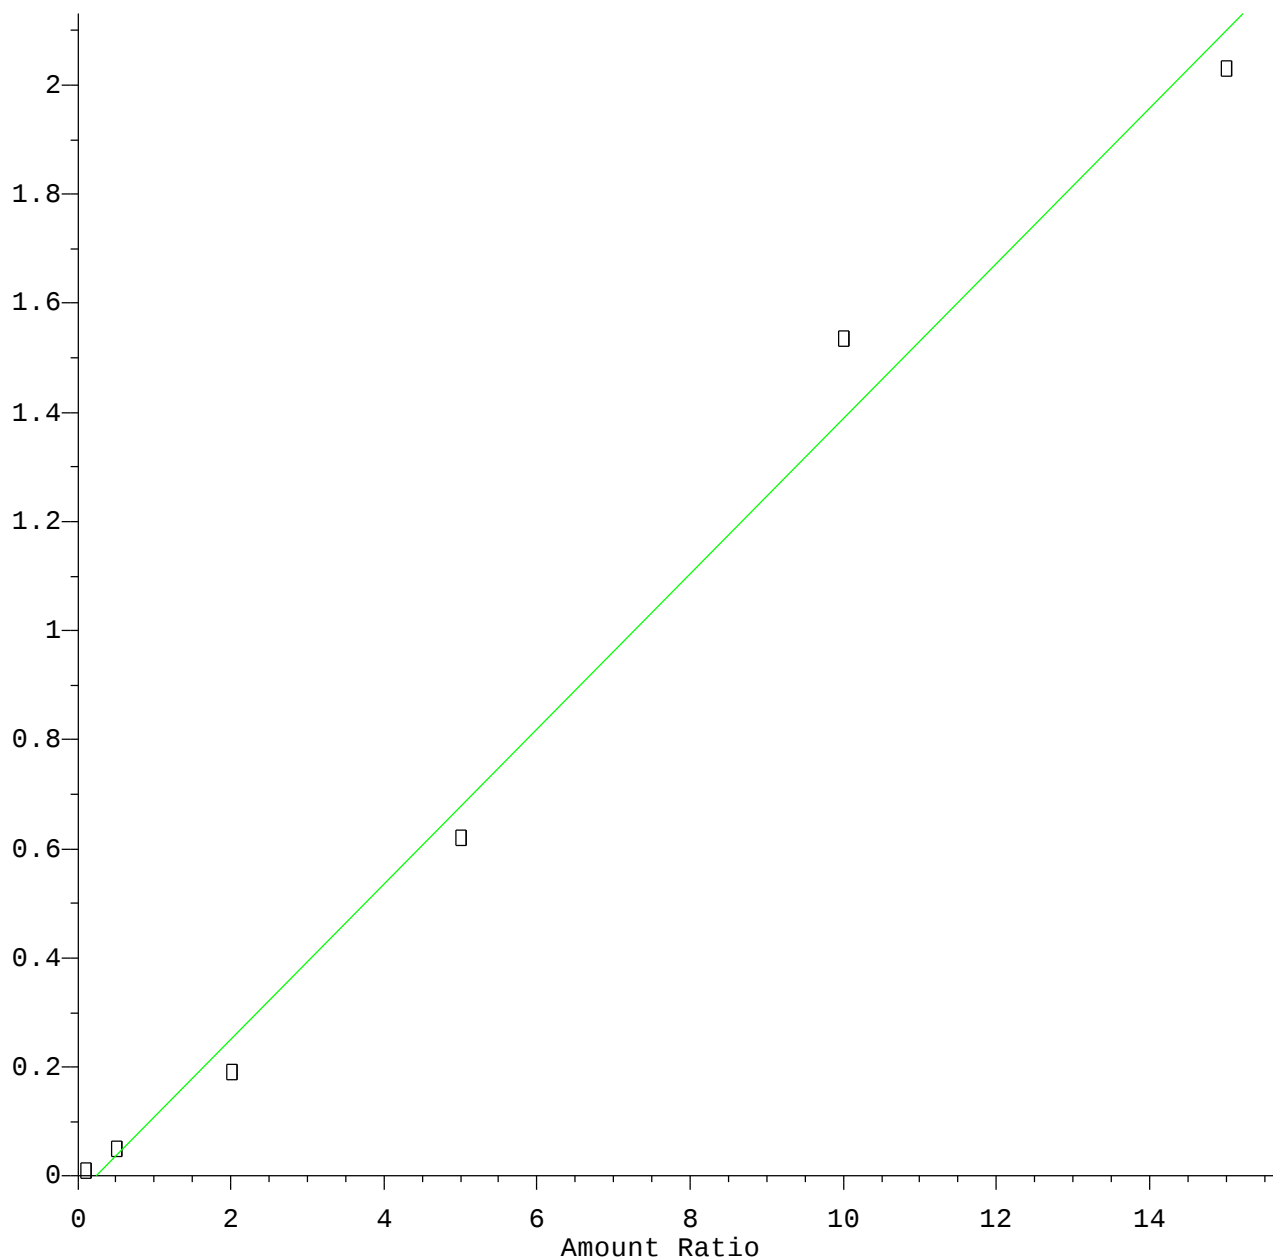


Resp Ratio = $1.42 \times 10^{-1} \times \text{Amt} - 3.47 \times 10^{-2}$
Coef of Det (r^2) = 0.991 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020

1,2,4-Trichlorobenzene

Response Ratio

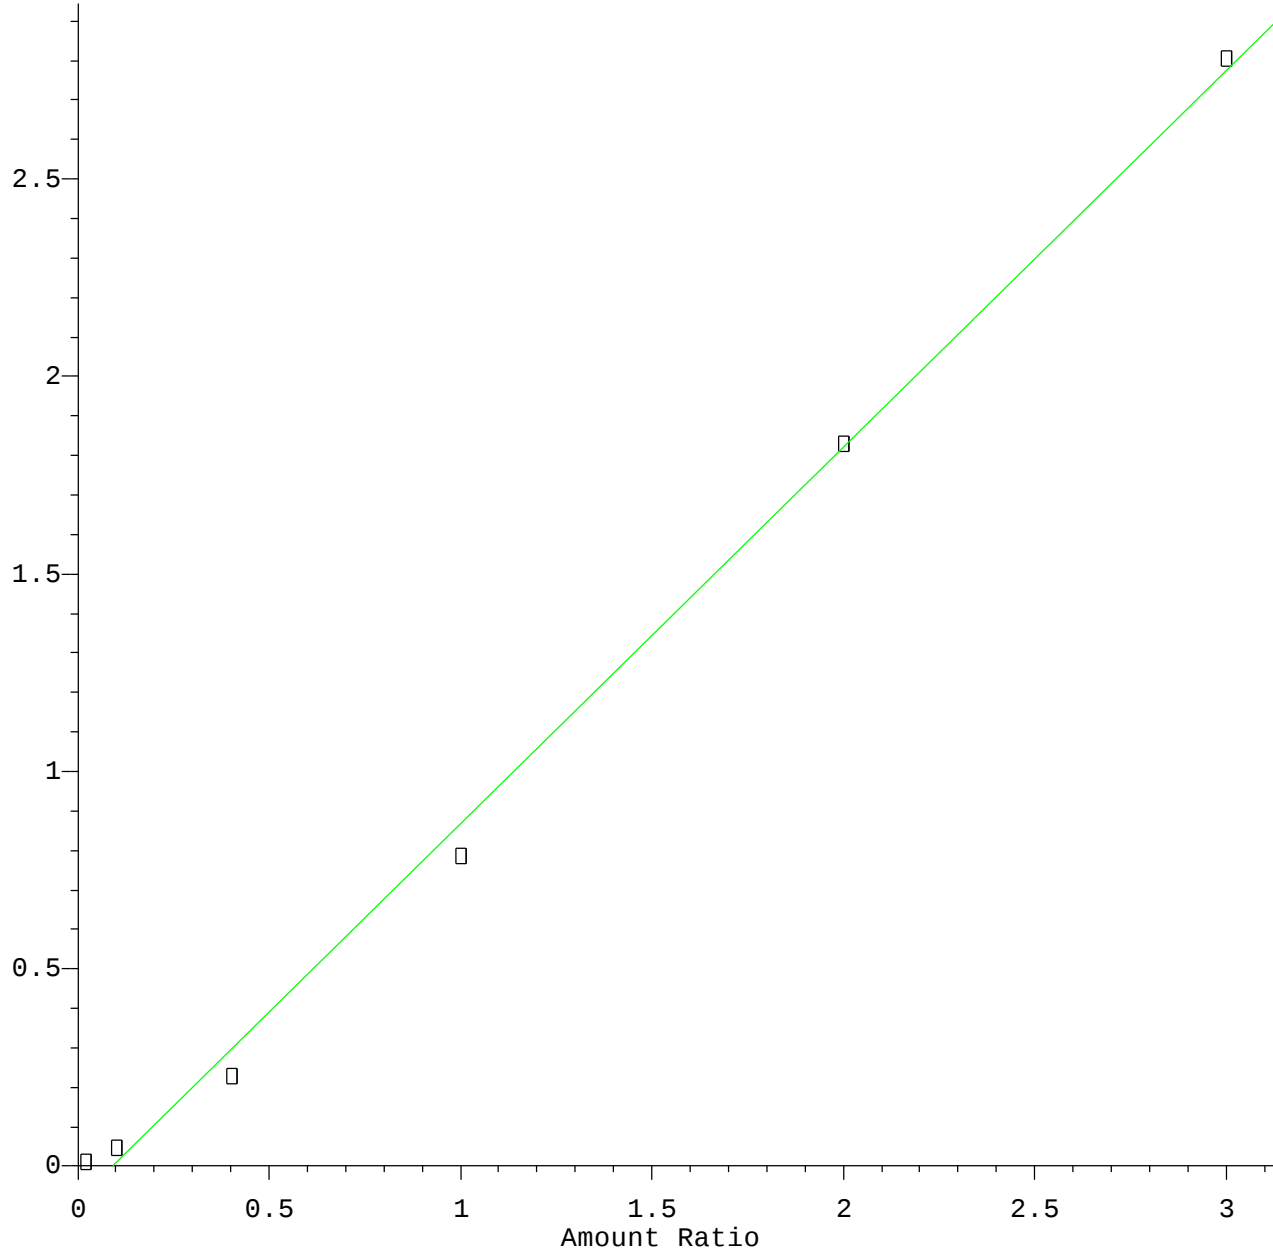


Resp Ratio = $9.53 \times 10^{-1} \times \text{Amt} - 8.66 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020

Naphthalene

Response Ratio

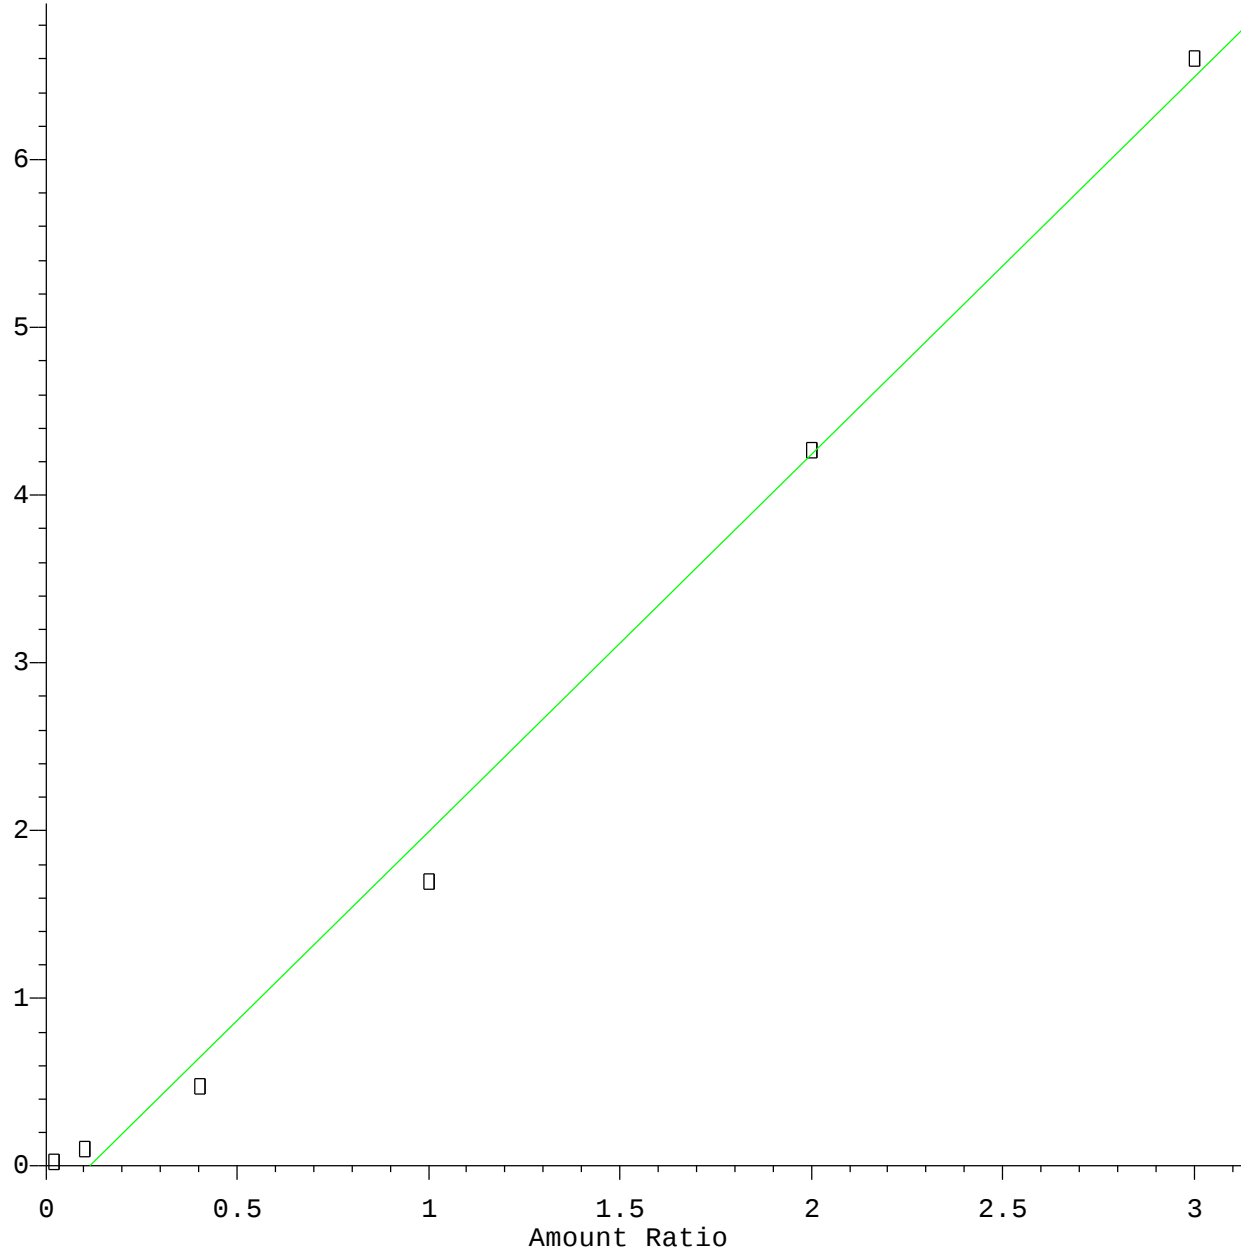


Resp Ratio = 2.25×10^0 * Amt - 2.54×10^{-1}
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020

1,2,3-Trichlorobenzene

Response Ratio

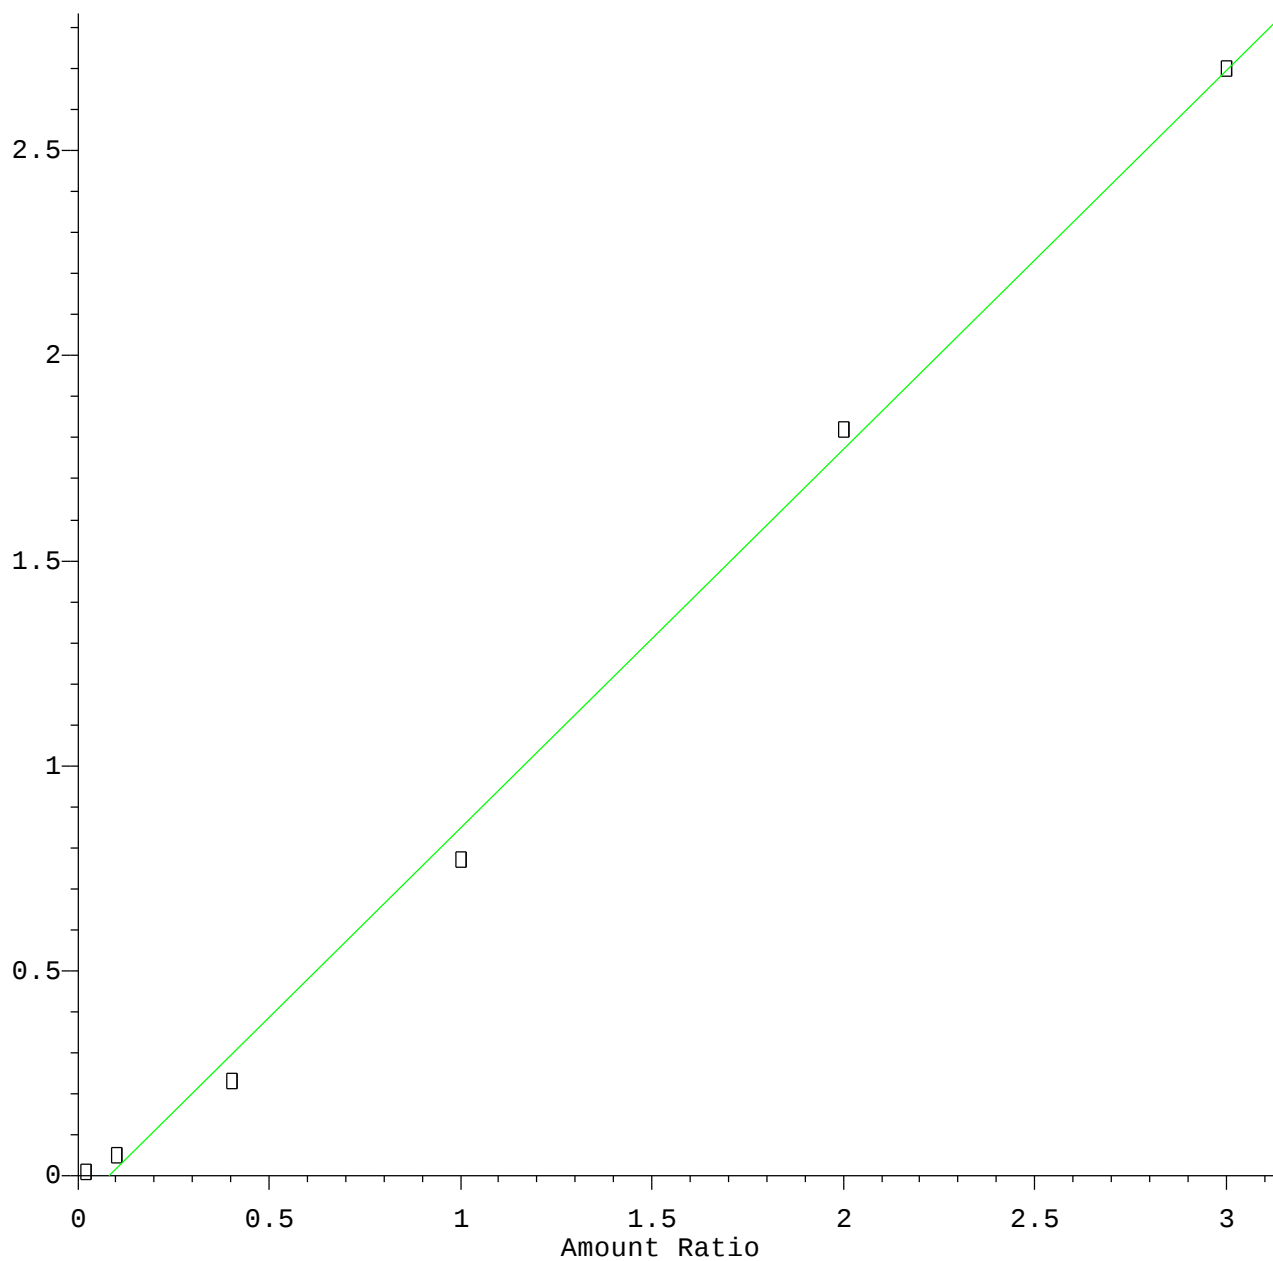


Resp Ratio = 9.23e-001 * Amt - 7.32e-002
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020


Dichlorodifluoromethane

Response Ratio

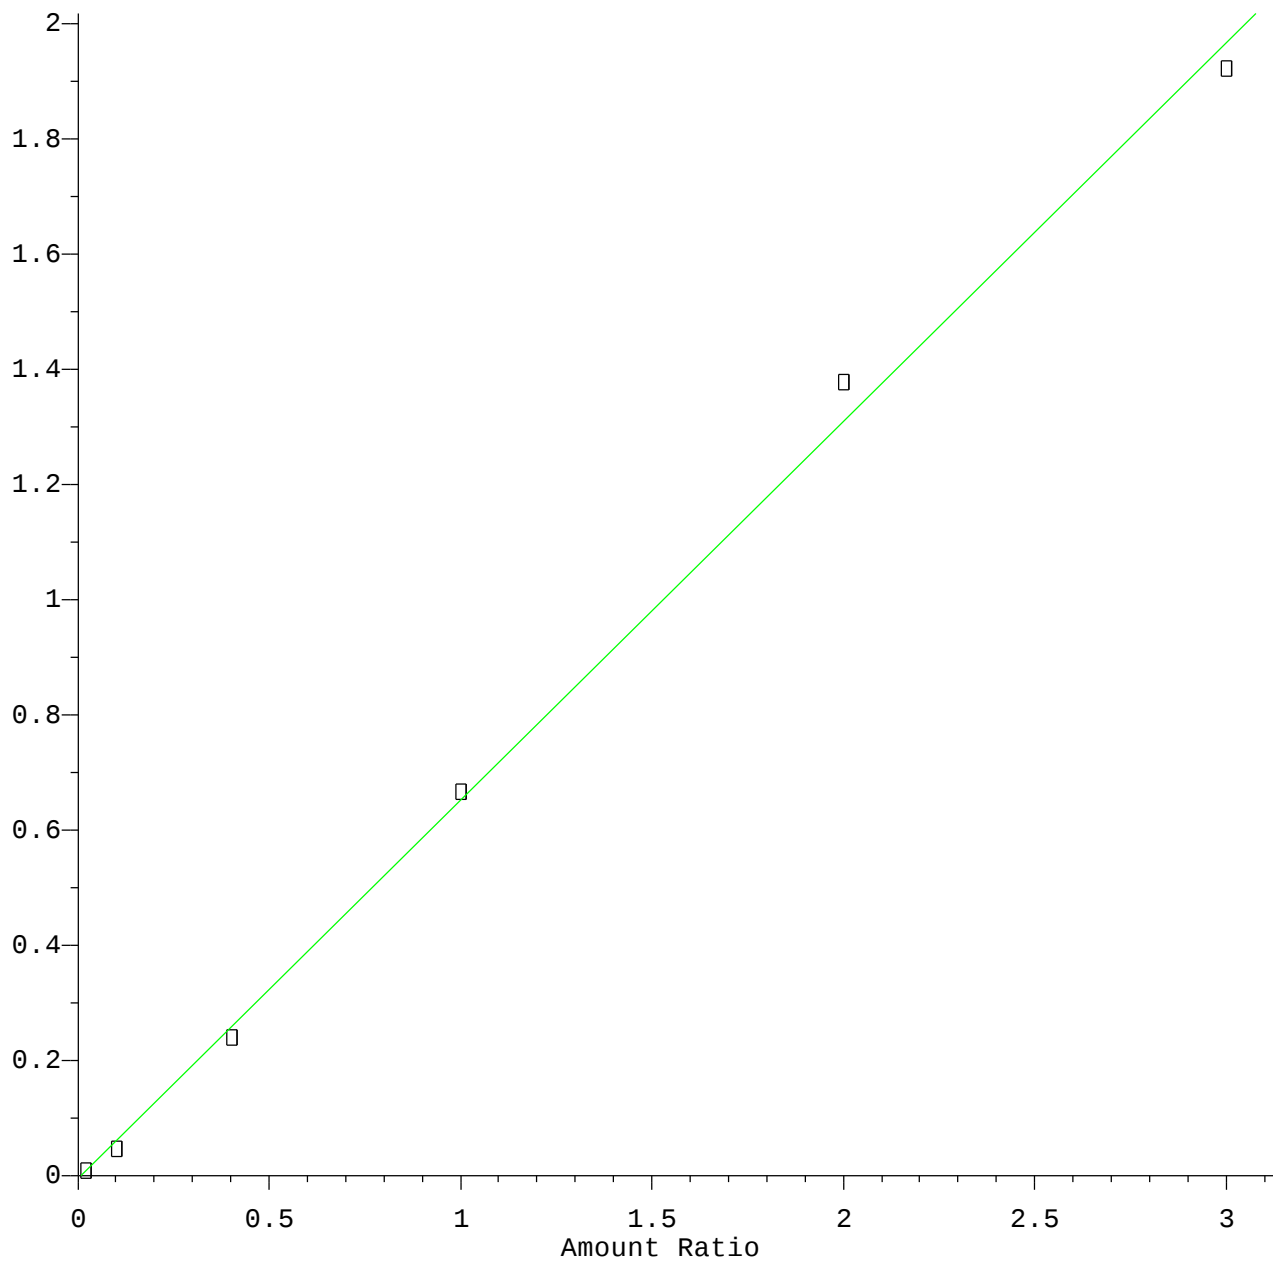

Resp Ratio = $6.57 \times 10^{-1} \times \text{Amt} - 3.63 \times 10^{-3}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020

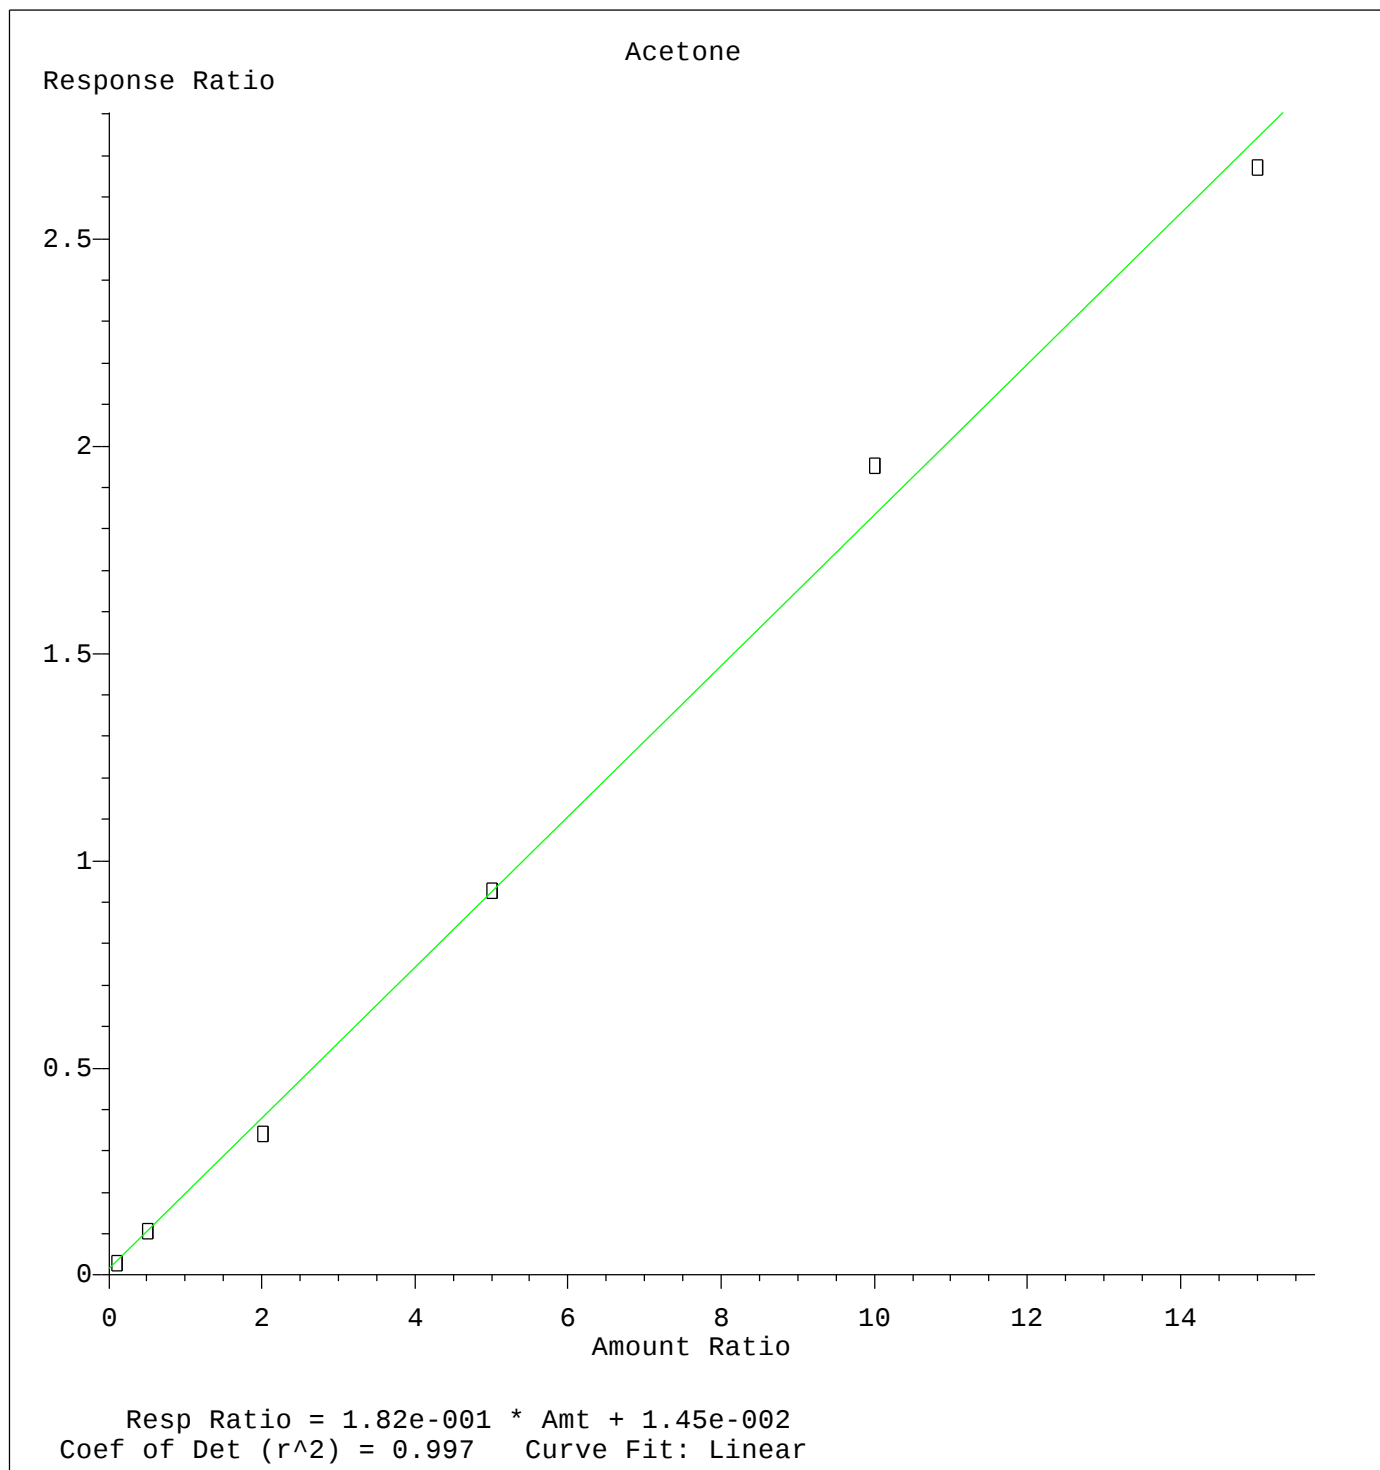

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020


Methylene Chloride

Response Ratio

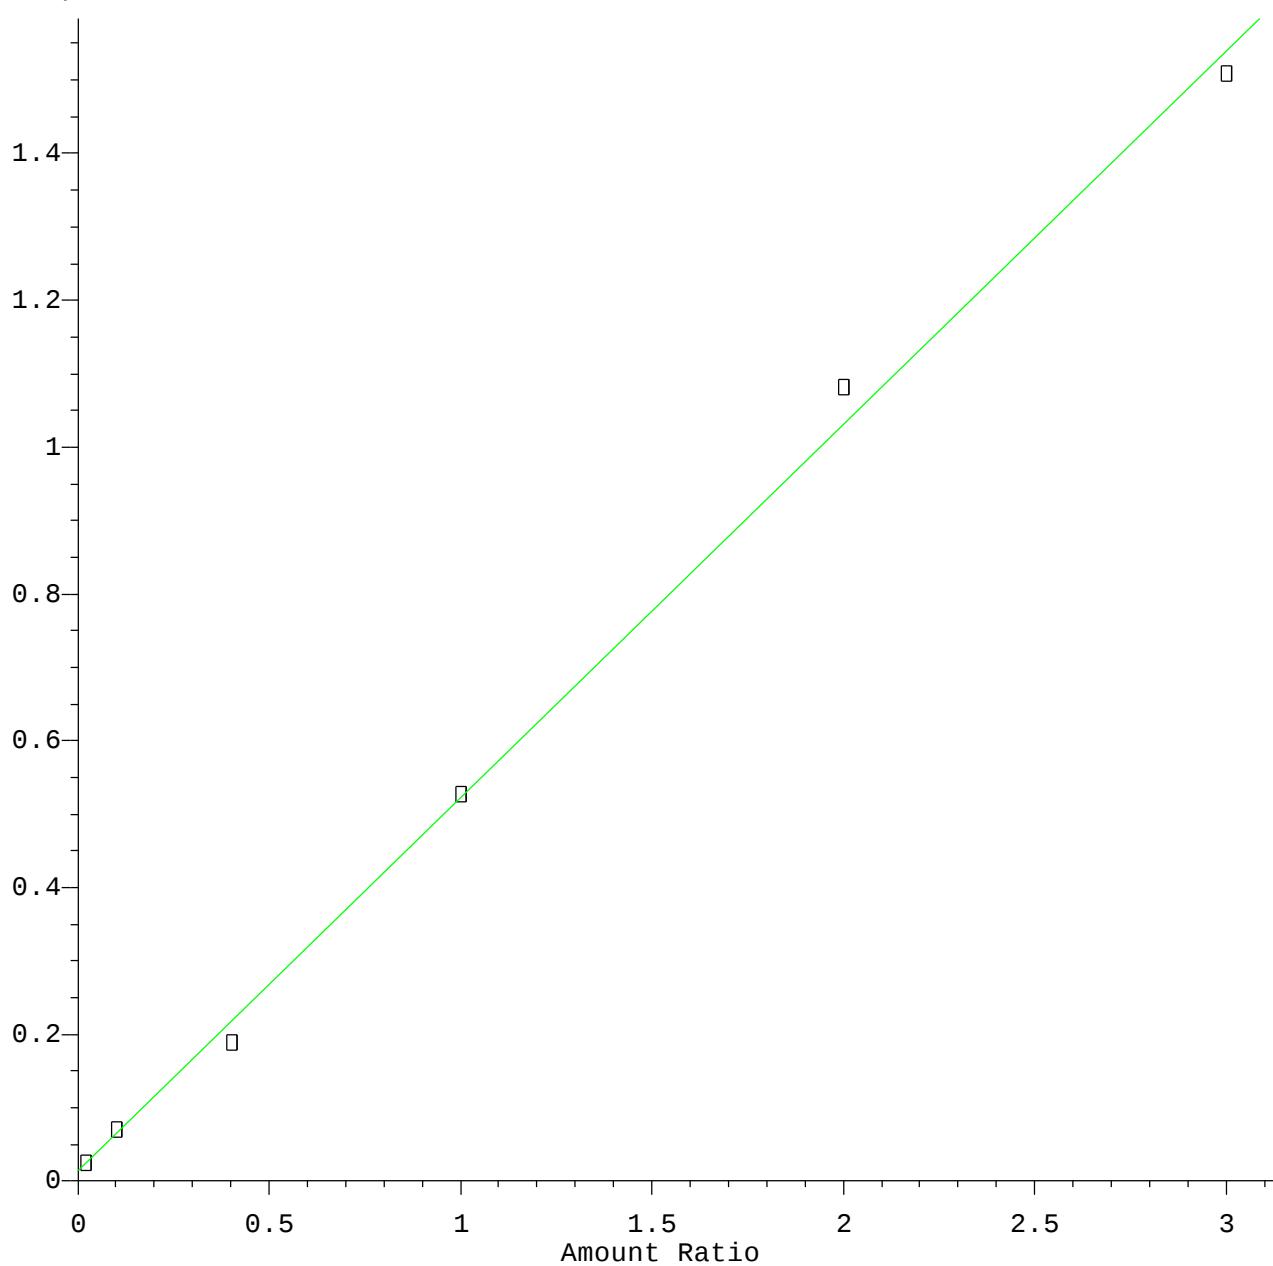

Resp Ratio = $5.09 \times 10^{-1} \times \text{Amt} + 1.40 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020

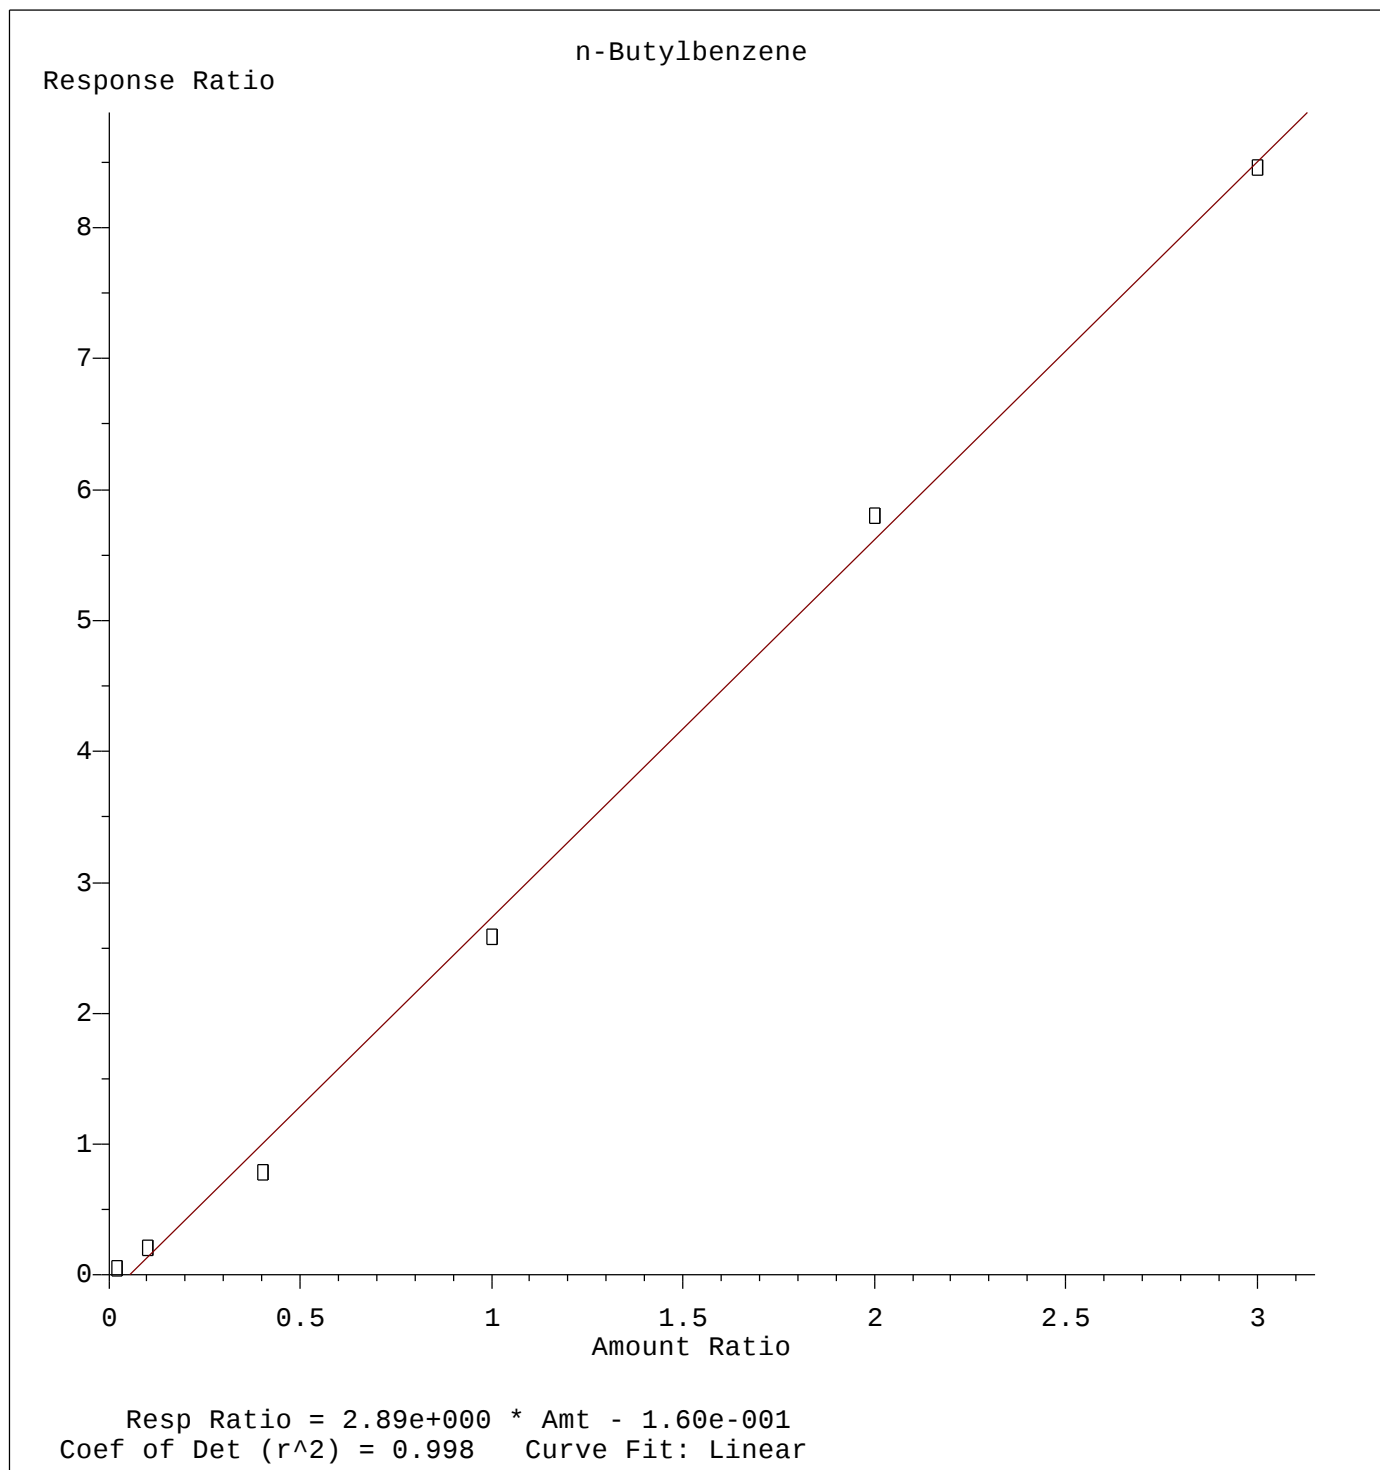

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020


1,1,2,2-Tetrachloroethane

Response Ratio

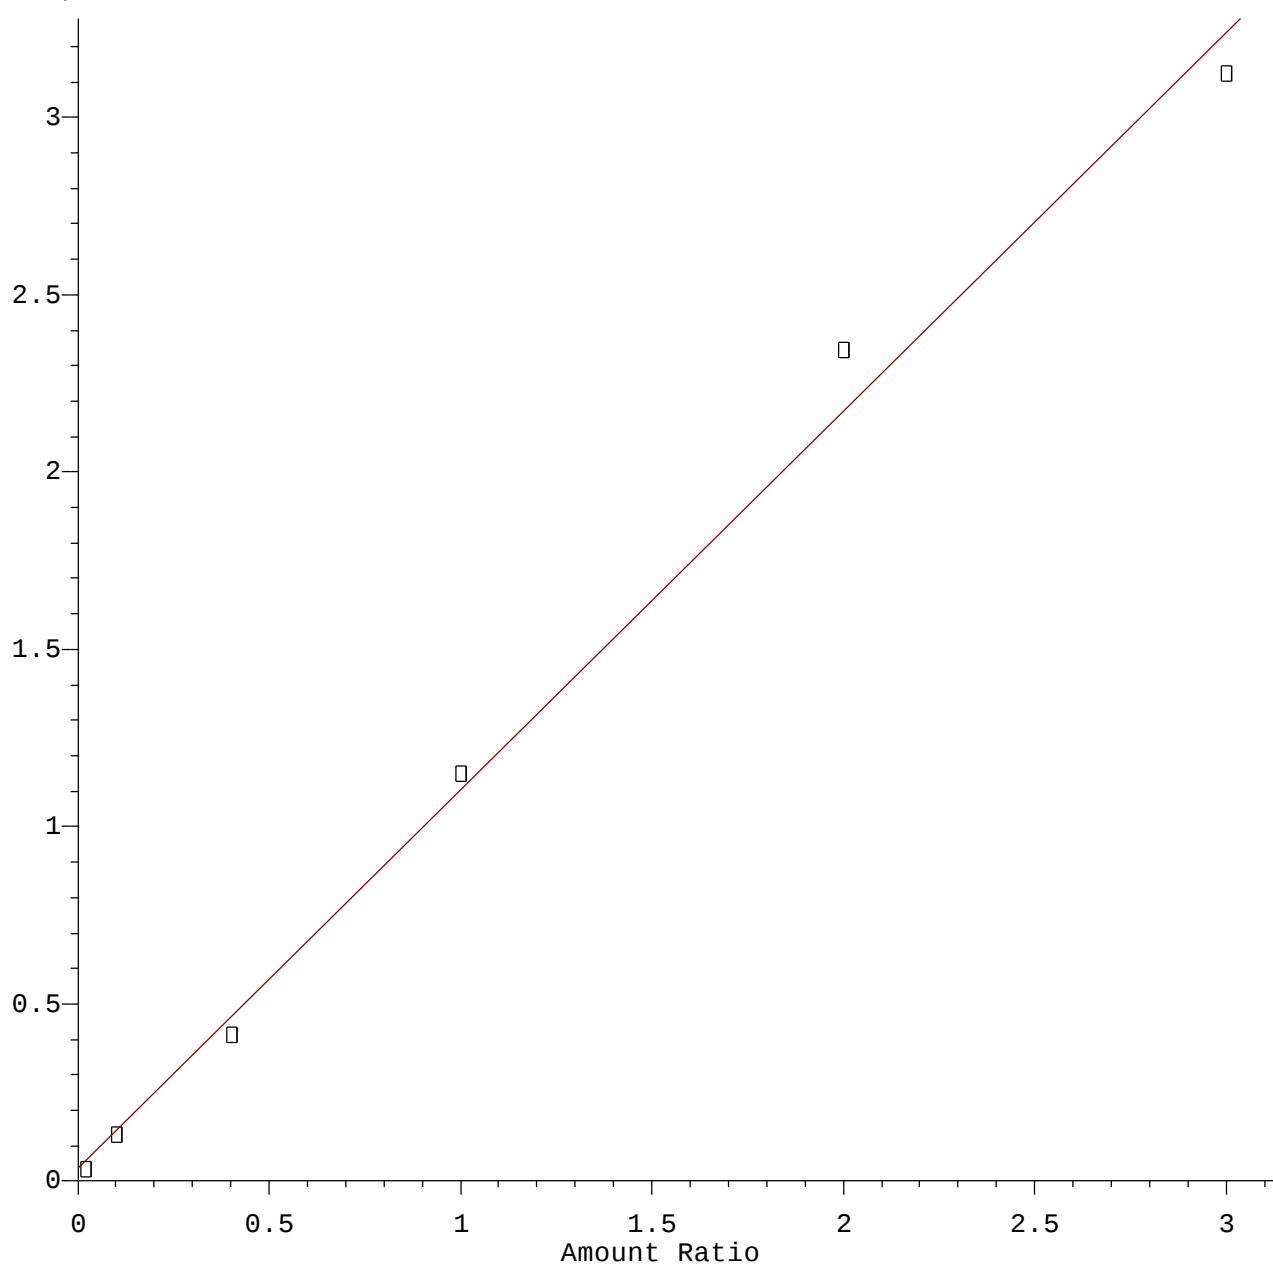


Resp Ratio = 1.07e+000 * Amt + 3.72e-002
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020

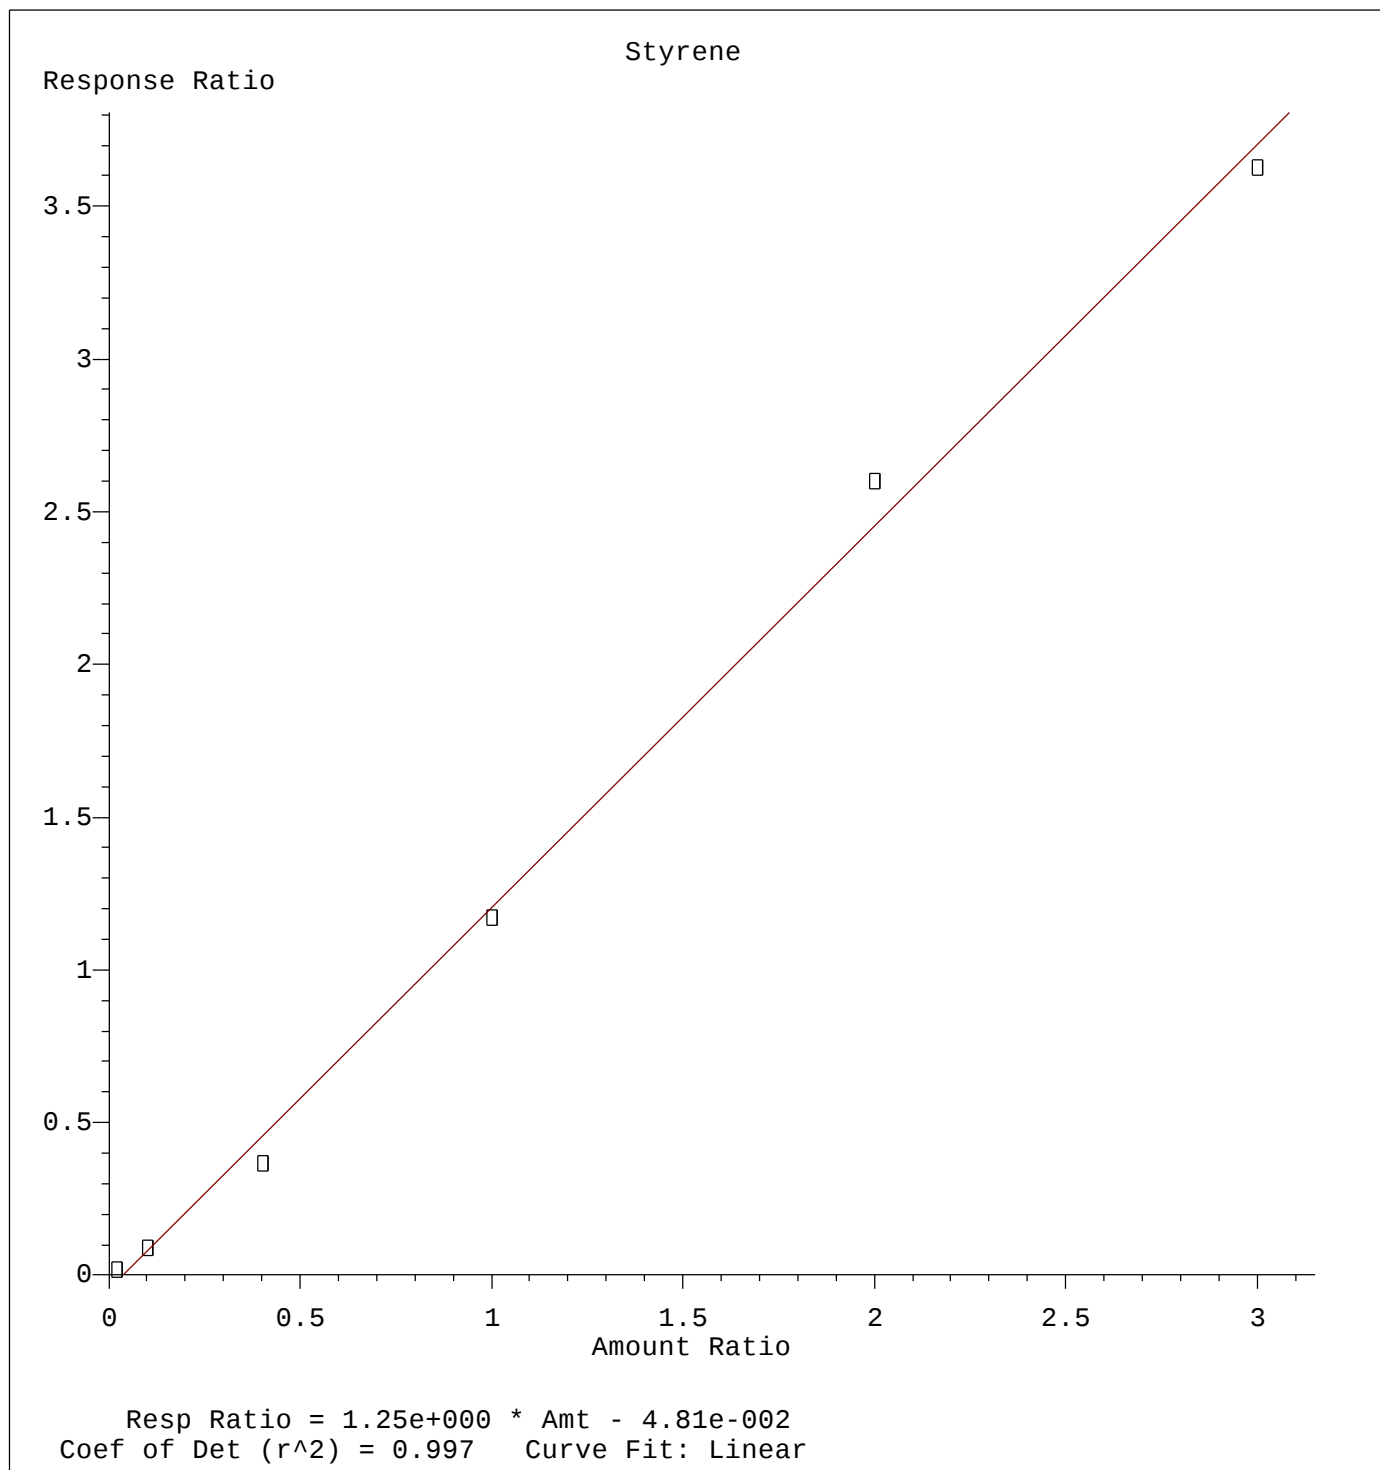


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020

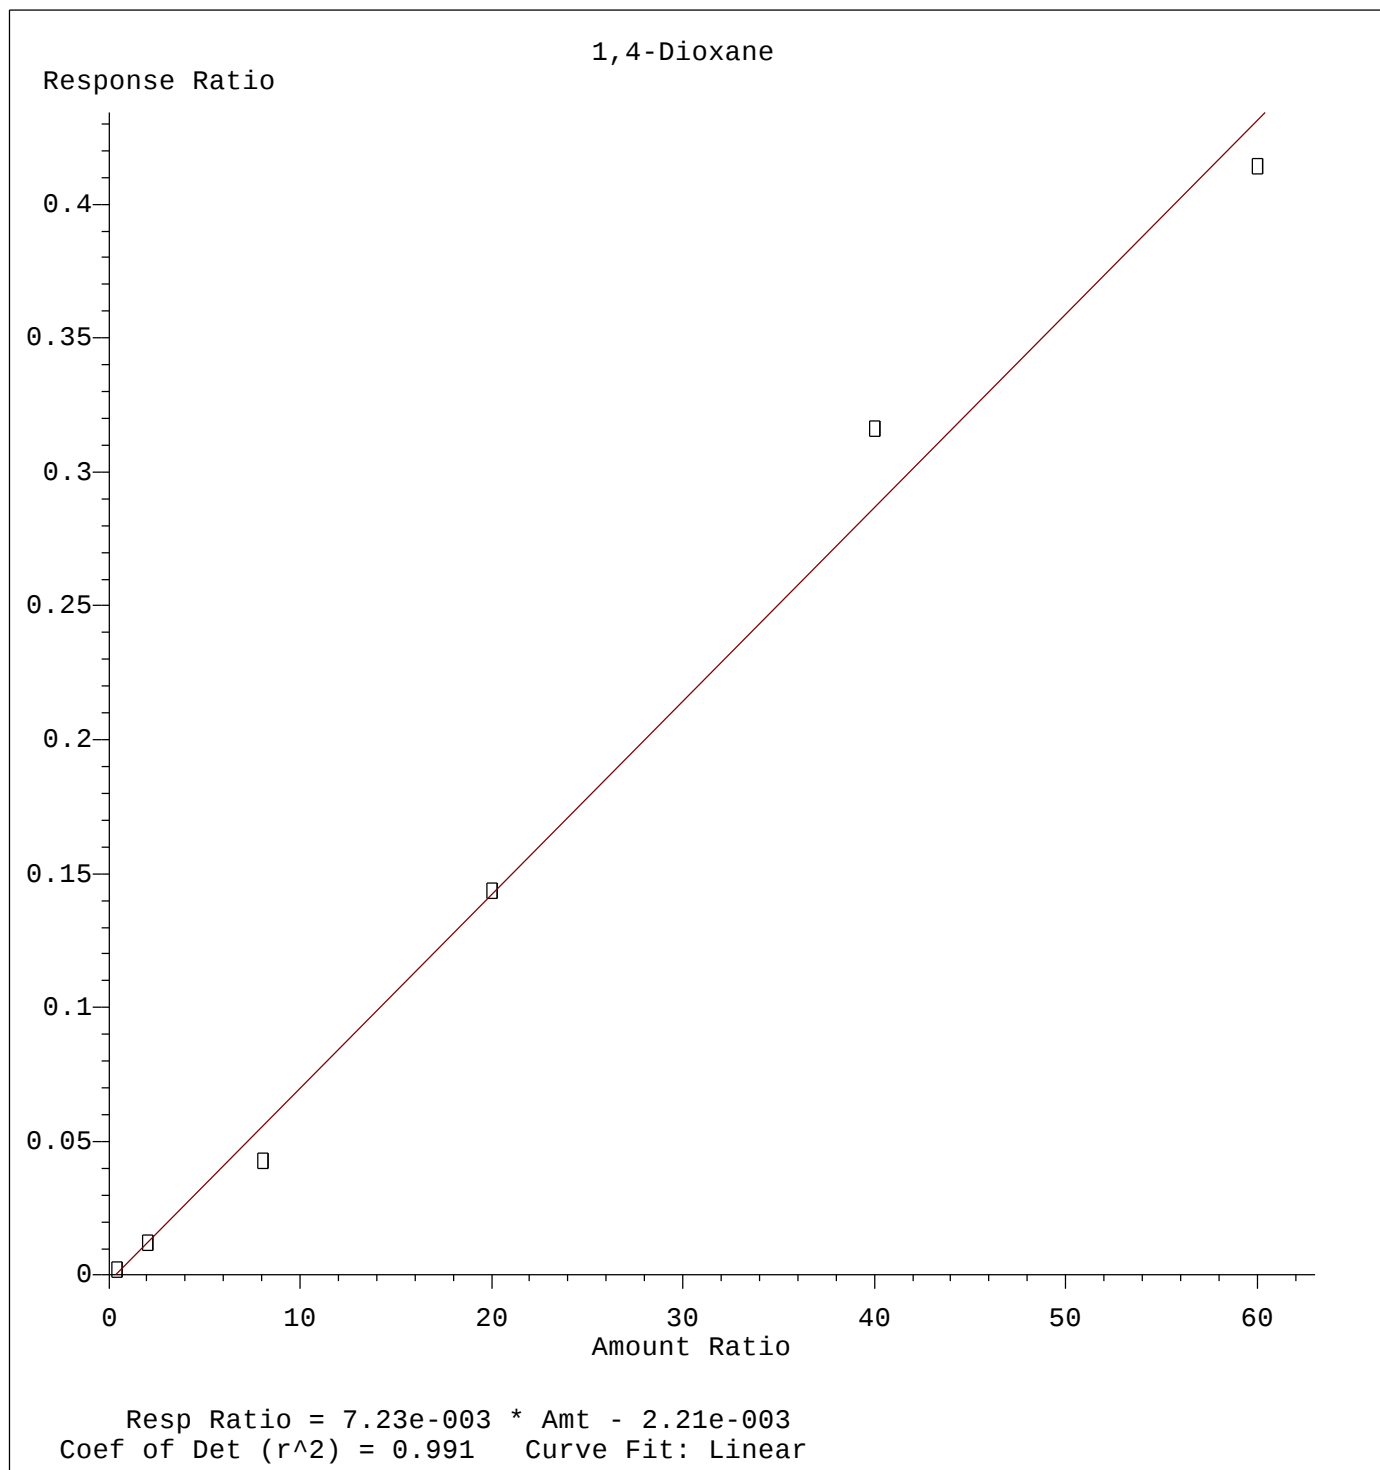

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020

Methylcyclohexane

Response Ratio

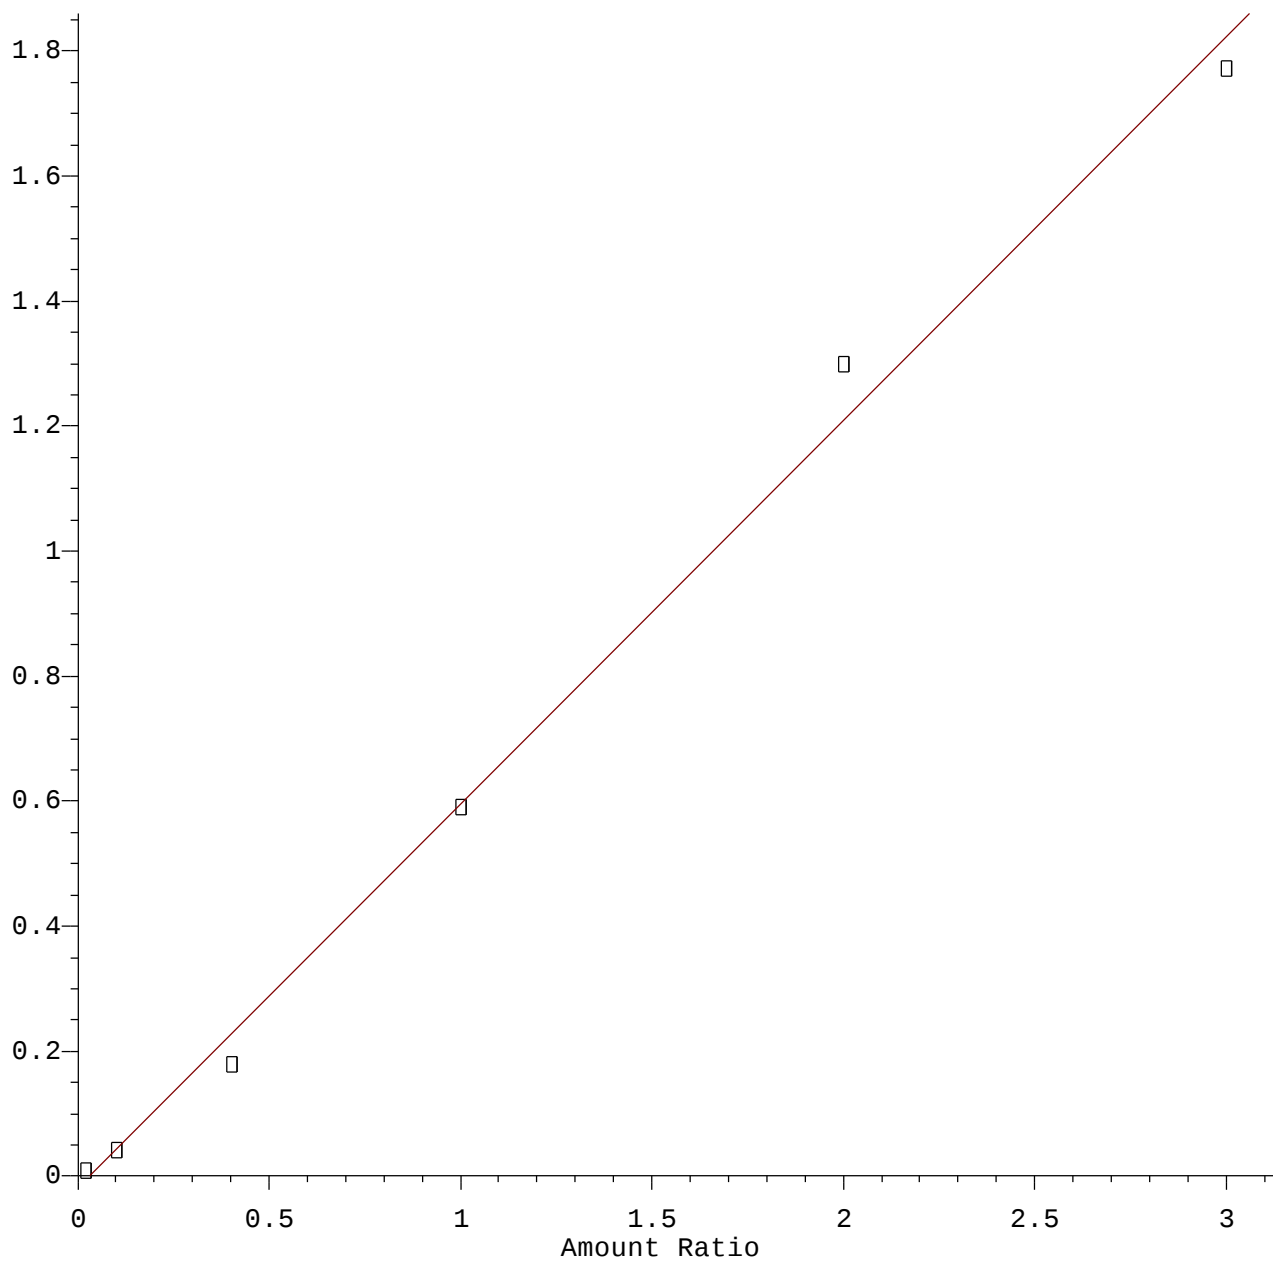

Resp Ratio = $6.14 \times 10^{-1} \times \text{Amt} - 1.92 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Calibration Table Last Updated: Wed Aug 19 06:09:27 2020