

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN081821\  
 Data File : VN068201.D  
 Acq On : 18 Aug 2021 18:29  
 Operator : JC/MD  
 Sample : M3449-14  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :

Quant Time: Aug 19 03:08:03 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N081721W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Aug 17 13:09:49 2021  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response | Conc       | Units  | Dev(Min) |
|-------------------------------|----------------|------|----------|------------|--------|----------|
| Internal Standards            |                |      |          |            |        |          |
| 1) Pentafluorobenzene         | 8.088          | 168  | 404192   | 50.000     | ug/l   | # 0.00   |
| 34) 1,4-Difluorobenzene       | 8.971          | 114  | 693127   | 50.000     | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.749         | 117  | 739389   | 50.000     | ug/l   | # 0.00   |
| 72) 1,4-Dichlorobenzene-d4    | 13.677         | 152  | 275447   | 50.000     | ug/l   | 0.00     |
| System Monitoring Compounds   |                |      |          |            |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.442          | 65   | 232249   | 53.815     | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 61 - 141 |      | Recovery | = 107.640% |        |          |
| 35) Dibromofluoromethane      | 8.024          | 113  | 211810   | 48.674     | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 69 - 133 |      | Recovery | = 97.340%  |        |          |
| 50) Toluene-d8                | 10.446         | 98   | 863775   | 52.093     | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 65 - 126 |      | Recovery | = 104.180% |        |          |
| 62) 4-Bromofluorobenzene      | 12.736         | 95   | 283383   | 51.339     | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 58 - 135 |      | Recovery | = 102.680% |        |          |
| Target Compounds              |                |      |          |            |        |          |
|                               |                |      |          |            | Qvalue |          |
| 5) Bromomethane               | 2.823          | 94   | 25       | Below Cal  | #      | 4        |
| 6) Chloroethane               | 3.019          | 64   | 380      | Below Cal  | #      | 44       |
| 11) Tert butyl alcohol        | 5.385          | 59   | 221      | 0.411      | ug/l # | 71       |
| 13) Acrolein                  | 4.036          | 56   | 121      | Below Cal  | #      | 71       |
| 16) Acetone                   | 4.296          | 43   | 11922    | 9.462      | ug/l # | 89       |
| 18) Methyl Acetate            | 4.848          | 43   | 768      | Below Cal  | #      | 54       |
| 20) Methylene Chloride        | 5.095          | 84   | 30790    | 7.004      | ug/l # | 81       |
| 25) 2-Butanone                | 7.351          | 43   | 5230     | 2.663      | ug/l # | 81       |
| 29) Tetrahydrofuran           | 7.694          | 42   | 523      | 0.416      | ug/l # | 39       |
| 31) Cyclohexane               | 8.085          | 56   | 6746     | 1.187      | ug/l # | 1        |
| 36) 1,1-Dichloropropene       | 8.088          | 75   | 26003    | 4.589      | ug/l # | 53       |
| 37) Ethyl Acetate             | 7.351          | 43   | 5230     | 1.083      | ug/l # | 69       |
| 38) Carbon Tetrachloride      | 8.088          | 117  | 37632    | 5.758      | ug/l # | 16       |
| 43) Isopropyl Acetate         | 8.566          | 43   | 37116    | 4.800      | ug/l # | 92       |
| 45) 1,2-Dichloropropane       | 9.628          | 63   | 2755     | 0.677      | ug/l # | 44       |
| 48) Methyl methacrylate       | 9.550          | 41   | 8431     | 2.617      | ug/l # | 12       |
| 49) 1,4-Dioxane               | 9.612          | 88   | 55       | 0.706      | ug/l # | 20       |
| 51) 4-Methyl-2-Pentanone      | 10.336         | 43   | 3902     | 0.822      | ug/l # | 30       |
| 54) cis-1,3-Dichloropropene   | 10.247         | 75   | 67307    | 10.257     | ug/l # | 56       |
| 57) 1,3-Dichloropropane       | 11.095         | 76   | 41855    | 5.768      | ug/l # | 43       |
| 59) 2-Hexanone                | 11.095         | 43   | 509969   | 154.630    | ug/l # | 58       |
| 76) 1,2,3-Trichloropropane    | 12.733         | 75   | 142517   | 31.129     | ug/l # | 100      |
| 81) trans-1,4-Dichloro-2-b... | 12.733         | 75   | 142517   | 101.985    | ug/l # | 6        |
| 93) 1,2,4-Trichlorobenzene    | 15.268         | 180  | 133      | 2.712      | ug/l # | 12       |
| 95) Naphthalene               | 15.507         | 128  | 609      | 3.397      | ug/l # | 69       |
| 96) 1,2,3-Trichlorobenzene    | 15.705         | 180  | 51       | 2.842      | ug/l # | 12       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN081821\  
Data File : VN068201.D  
Acq On : 18 Aug 2021 18:29  
Operator : JC/MD  
Sample : M3449-14  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :

Quant Time: Aug 19 03:08:03 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N081721W.M  
Quant Title : SW846 8260  
QLast Update : Tue Aug 17 13:09:49 2021  
Response via : Initial Calibration




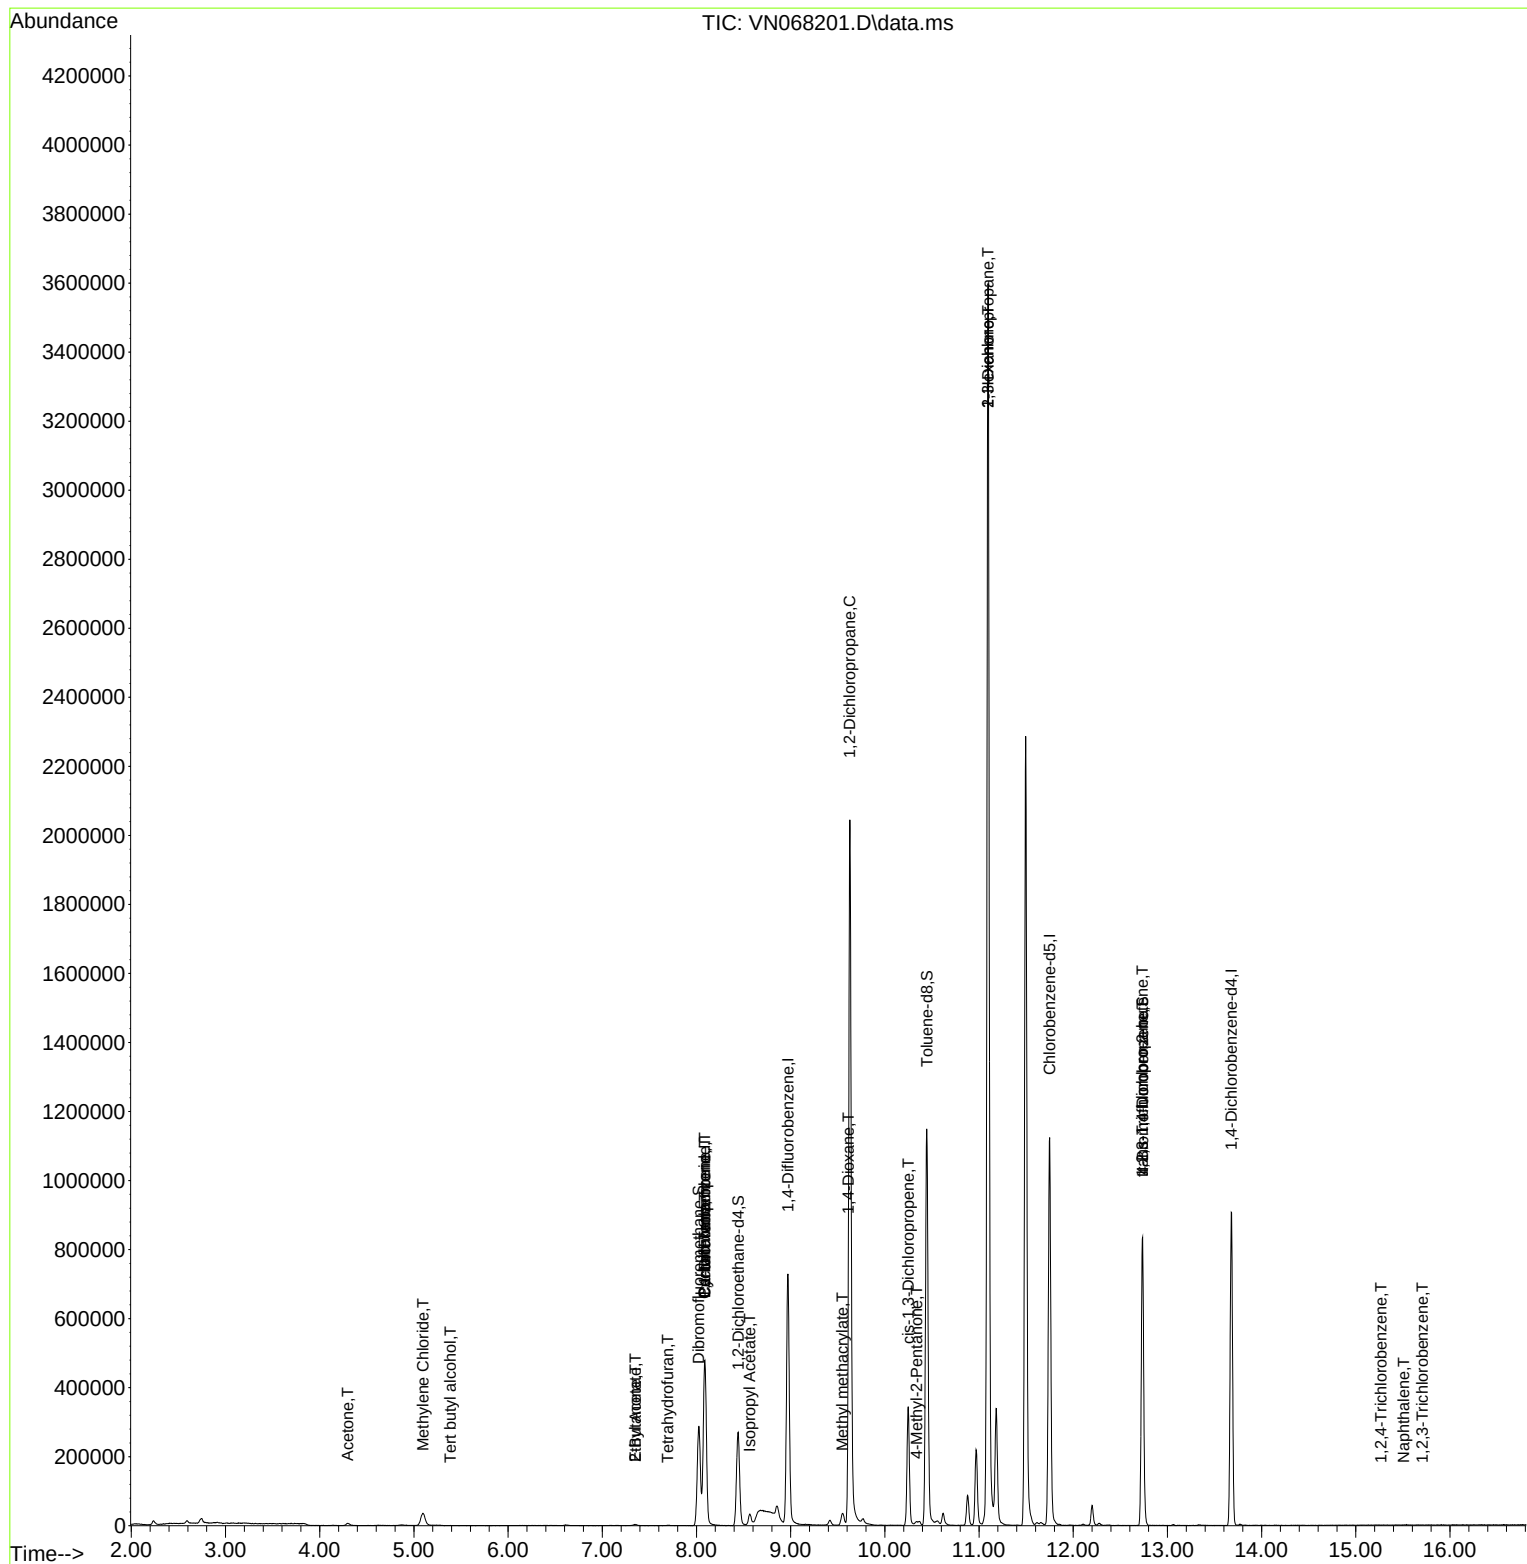




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.088 min Scan# 2274  
Delta R.T. 0.000 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion:168 Resp: 404192  
Ion Ratio Lower Upper  
168 100  
99 51.0 62.9 94.3#

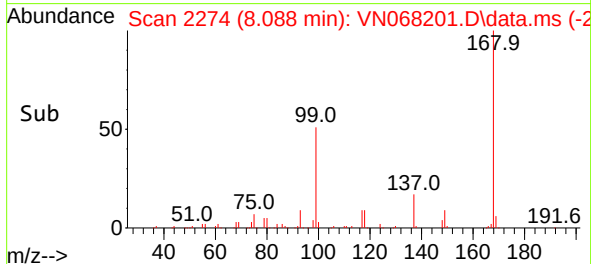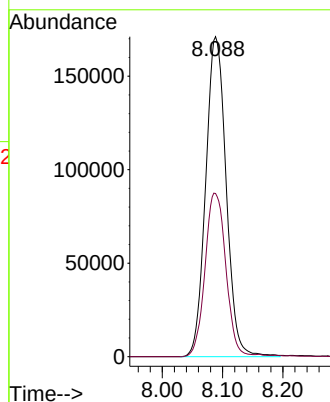

#5  
Bromomethane  
Concen: Below Cal  
RT: 2.823 min Scan# 311  
Delta R.T. -0.014 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Tgt Ion: 94 Resp: 25  
Ion Ratio Lower Upper  
94 100  
96 0.0 73.7 110.5#


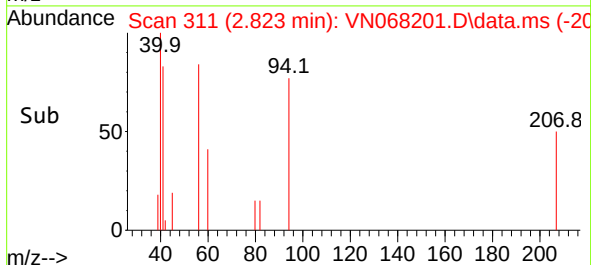
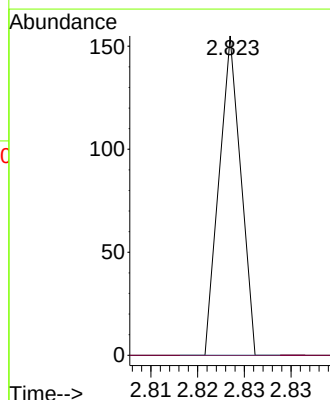
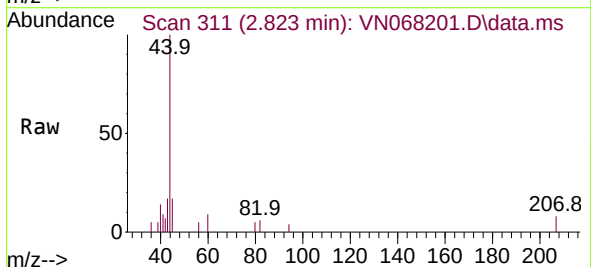




#6  
Chloroethane  
Concen: Below Cal  
RT: 3.019 min Scan# 384  
Delta R.T. 0.013 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 64 Resp: 380  
Ion Ratio Lower Upper  
64 100  
66 0.0 24.7 37.1#

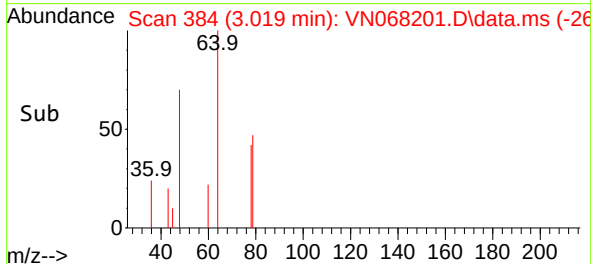

#11  
Tert butyl alcohol  
Concen: 0.411 ug/l  
RT: 5.385 min Scan# 1266  
Delta R.T. -0.005 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Tgt Ion: 59 Resp: 221  
Ion Ratio Lower Upper  
59 100  
57 0.0 8.7 13.1#


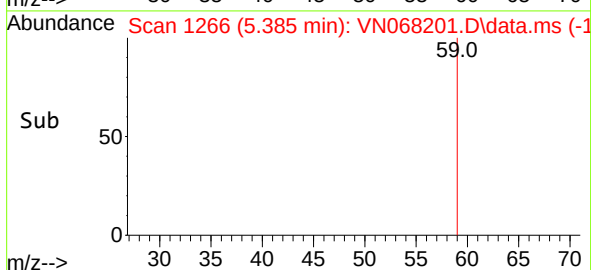






#13  
Acrolein  
Concen: Below Cal  
RT: 4.036 min Scan# 763  
Delta R.T. -0.003 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 56 Resp: 121  
Ion Ratio Lower Upper  
56 100  
55 47.9 57.4 86.0#

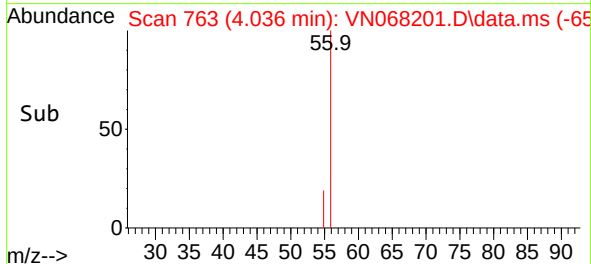

#16  
Acetone  
Concen: 9.462 ug/l  
RT: 4.296 min Scan# 860  
Delta R.T. 0.008 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Tgt Ion: 43 Resp: 11922  
Ion Ratio Lower Upper  
43 100  
58 32.1 21.2 31.8#




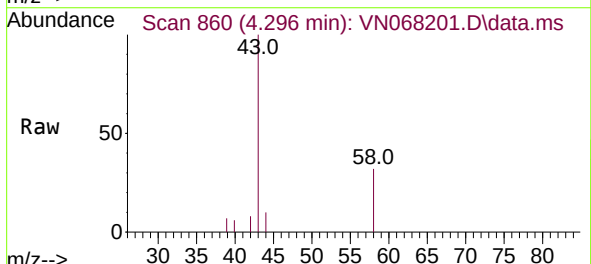


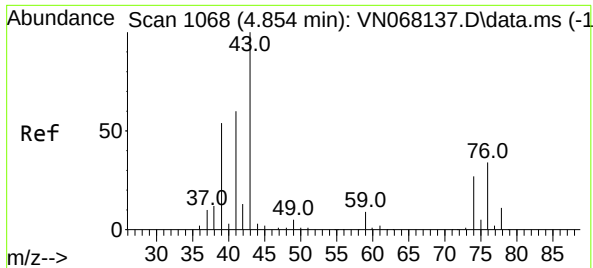

#18  
Methyl Acetate  
Concen: Below Cal  
RT: 4.848 min Scan# 1066  
Delta R.T. -0.006 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 43 Resp: 768  
Ion Ratio Lower Upper  
43 100  
74 0.0 17.4 26.0#

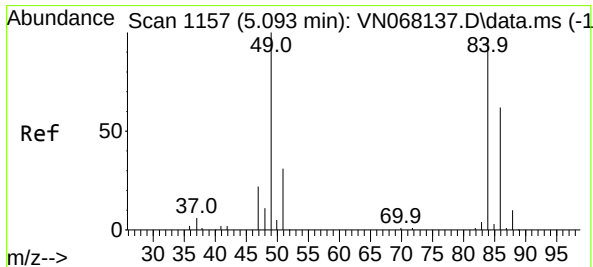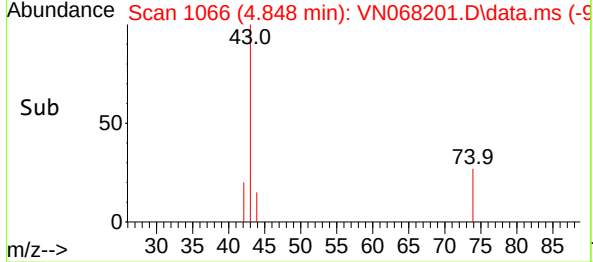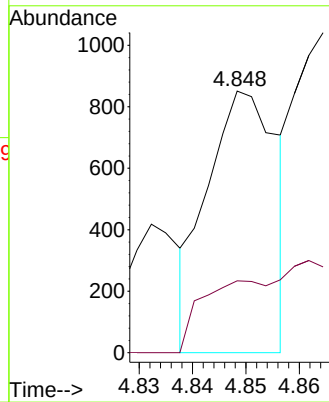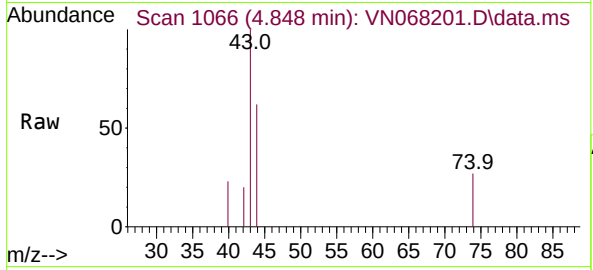

#20  
Methylene Chloride  
Concen: 7.004 ug/l  
RT: 5.095 min Scan# 1158  
Delta R.T. 0.002 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Tgt Ion: 84 Resp: 30790  
Ion Ratio Lower Upper  
84 100  
49 103.3 110.9 166.3#  
51 31.3 32.6 49.0#  
86 63.8 51.6 77.4


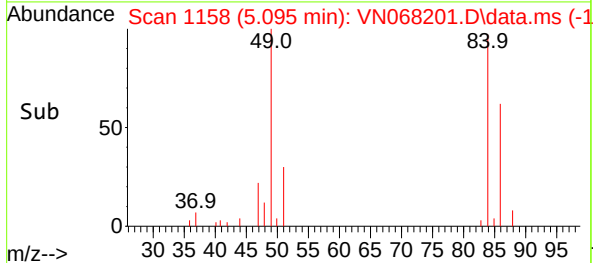
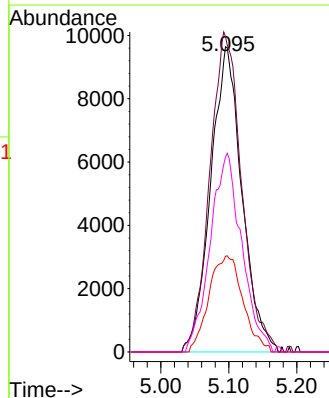
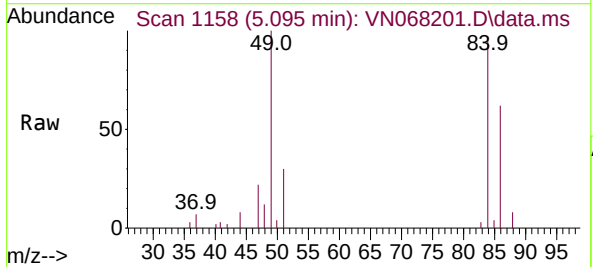


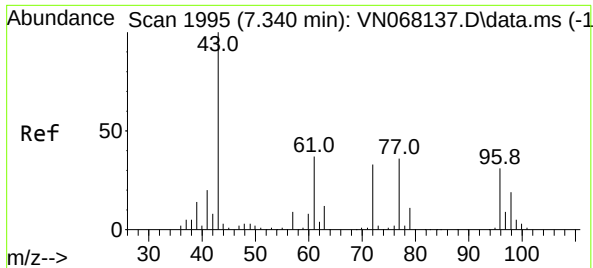

#25  
2-Butanone  
Concen: 2.663 ug/l  
RT: 7.351 min Scan# 1999  
Delta R.T. 0.011 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 43 Resp: 5230  
Ion Ratio Lower Upper  
43 100  
72 34.1 19.7 29.5#

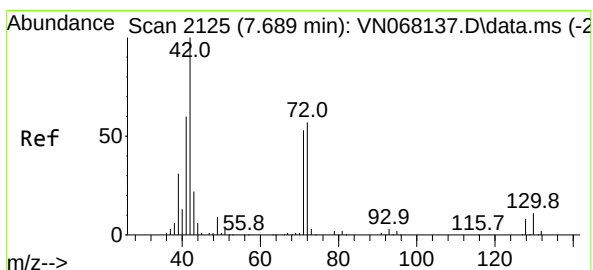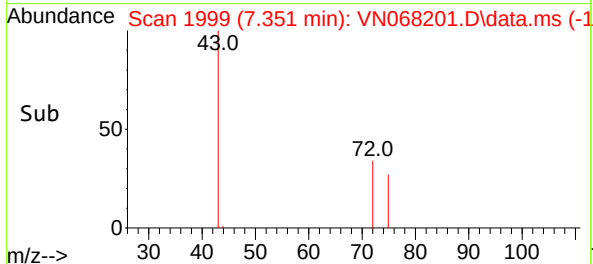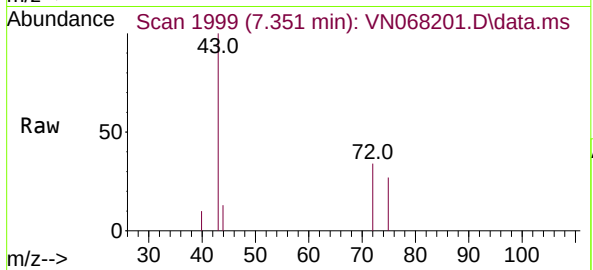

#29  
Tetrahydrofuran  
Concen: 0.416 ug/l  
RT: 7.694 min Scan# 2127  
Delta R.T. 0.005 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Tgt Ion: 42 Resp: 523  
Ion Ratio Lower Upper  
42 100  
72 0.0 32.8 49.2#  
71 4.8 31.2 46.8#

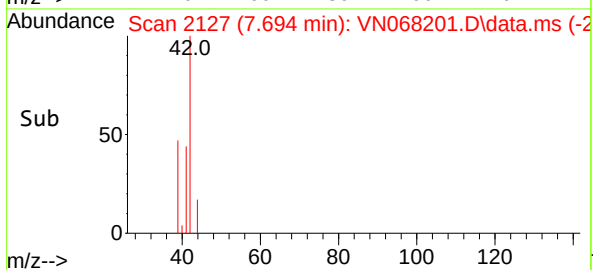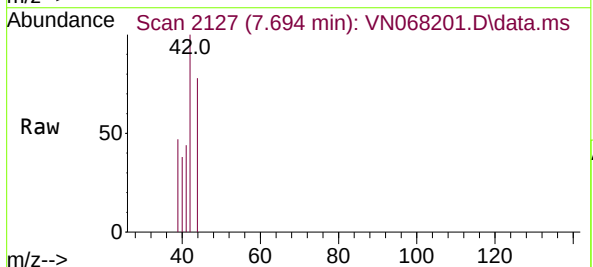



#31

Cyclohexane

Concen: 1.187 ug/l

RT: 8.085 min Scan# 2273

Delta R.T. -0.009 min

Lab File: VN068201.D

Acq: 18 Aug 2021 18:29

Tgt Ion: 56 Resp: 6746

Ion Ratio Lower Upper

56 100





69 178.3 27.3 40.9#

84 121.0 64.9 97.3#

Instrument :

MSVOA\_N

ClientSampled :

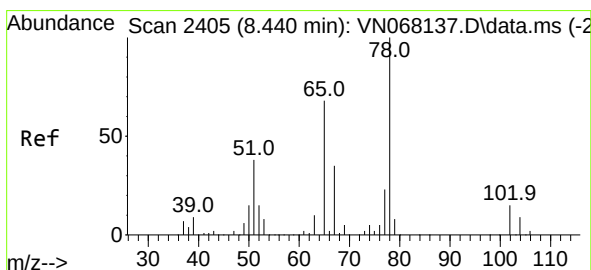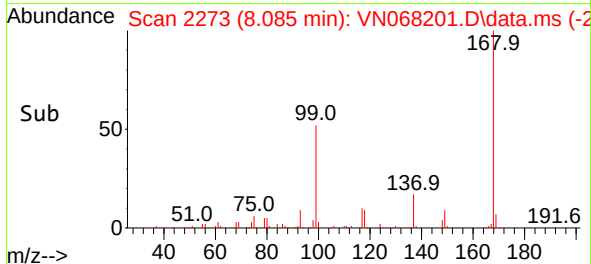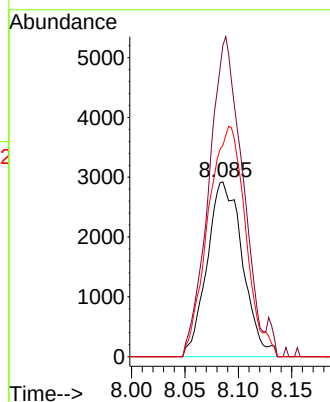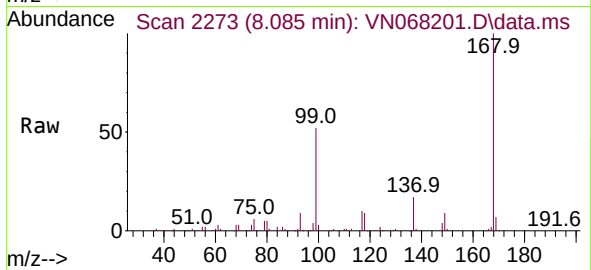

#33

1,2-Dichloroethane-d4

Concen: 53.815 ug/l

RT: 8.442 min Scan# 2406

Delta R.T. 0.002 min

Lab File: VN068201.D




Acq: 18 Aug 2021 18:29

Tgt Ion: 65 Resp: 232249


Ion Ratio Lower Upper

65 100

67 52.5 0.0 98.6

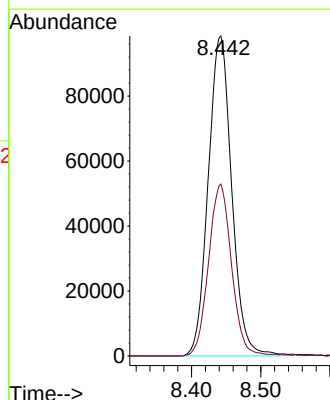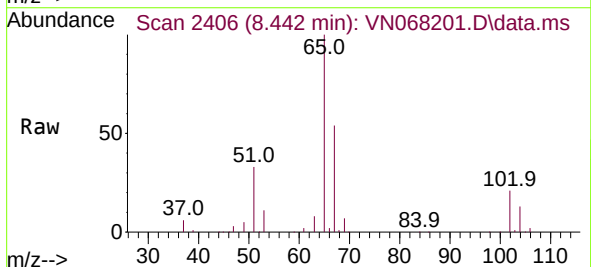









#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 8.971 min Scan# 2603  
Delta R.T. 0.003 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion:114 Resp: 693127  
Ion Ratio Lower Upper  
114 100  
63 17.5 0.0 49.0  
88 14.3 0.0 36.6

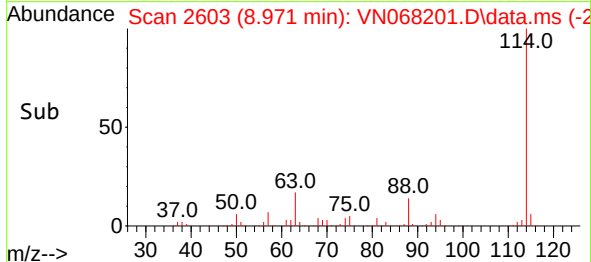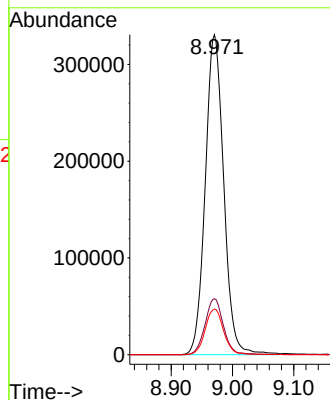

#35  
Dibromofluoromethane  
Concen: 48.674 ug/l  
RT: 8.024 min Scan# 2250  
Delta R.T. 0.003 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Tgt Ion:113 Resp: 211810  
Ion Ratio Lower Upper  
113 100  
111 102.6 83.8 125.8  
192 20.3 13.4 20.0#


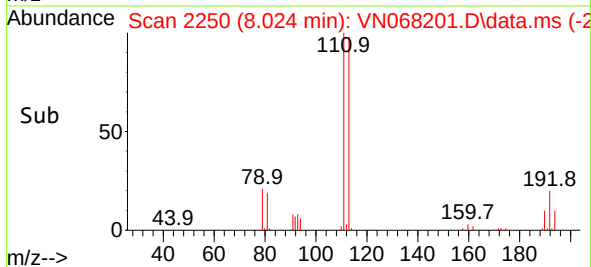
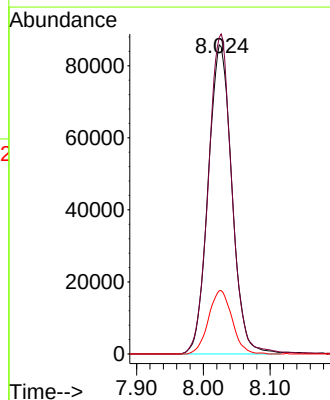
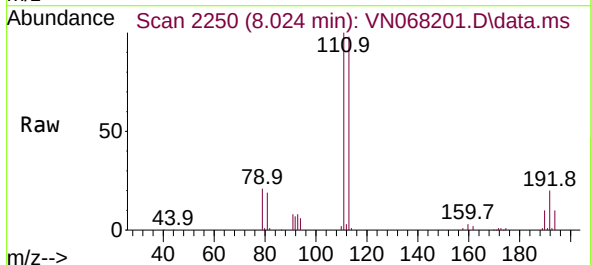


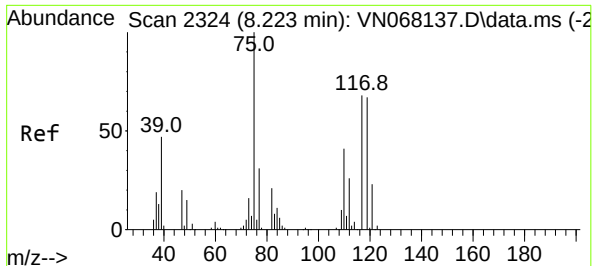

#36  
1,1-Dichloropropene  
Concen: 4.589 ug/l  
RT: 8.088 min Scan# 2274  
Delta R.T. -0.135 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 75 Resp: 26003  
Ion Ratio Lower Upper  
75 100  
110 10.1 15.7 47.0#  
77 0.0 24.6 37.0#

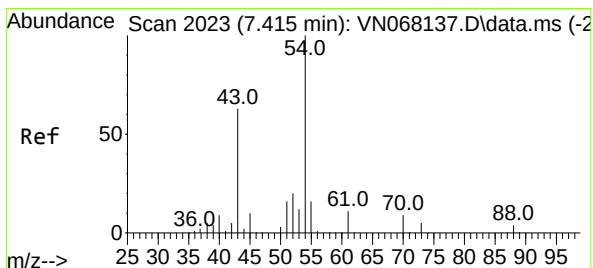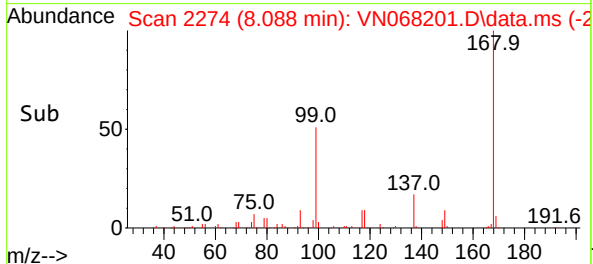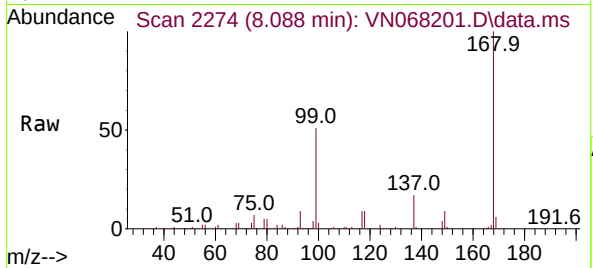

#37  
Ethyl Acetate  
Concen: 1.083 ug/l  
RT: 7.351 min Scan# 1999  
Delta R.T. -0.064 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29


Tgt Ion: 43 Resp: 5230  
Ion Ratio Lower Upper  
43 100  
61 0.0 10.6 16.0#  
70 0.0 8.1 12.1#

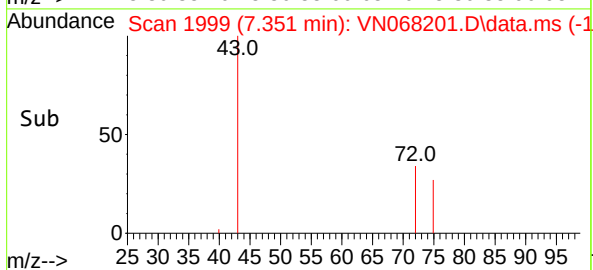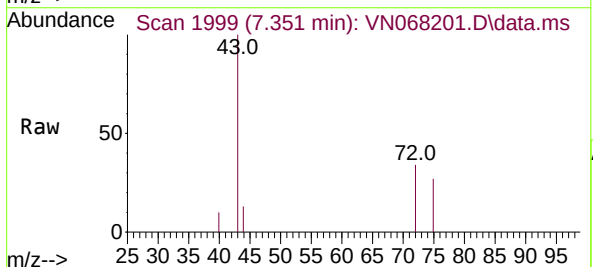






#38  
Carbon Tetrachloride  
Concen: 5.758 ug/l  
RT: 8.088 min Scan# 2274  
Delta R.T. -0.118 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29


Instrument :  
MSVOA\_N  
ClientSampled :

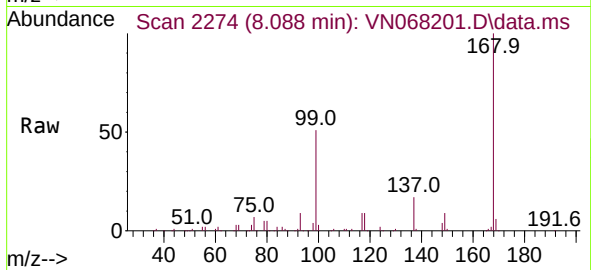



Tgt Ion:117 Resp: 37632  
Ion Ratio Lower Upper  
117 100  
119 4.5 75.4 113.2#  
121 0.0 23.5 35.3#

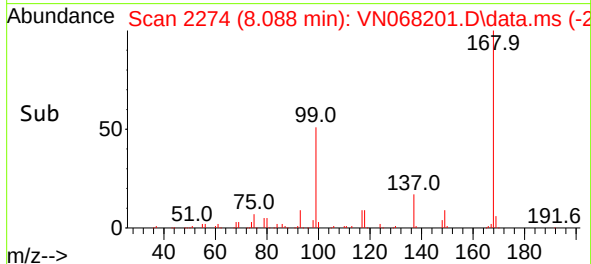


#43  
Isopropyl Acetate  
Concen: 4.800 ug/l  
RT: 8.566 min Scan# 2452  
Delta R.T. -0.000 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

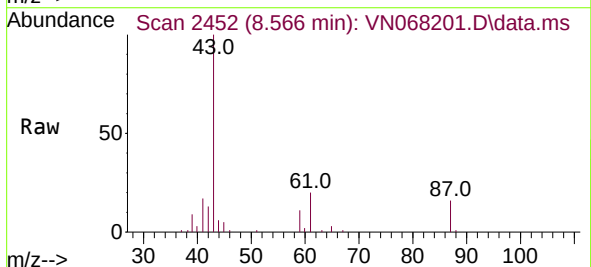

Tgt Ion: 43 Resp: 37116  
Ion Ratio Lower Upper  
43 100  
61 19.7 19.0 28.4  
87 15.0 9.5 14.3#



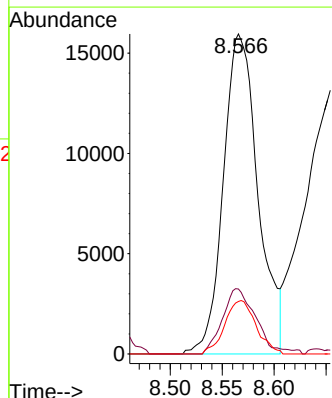



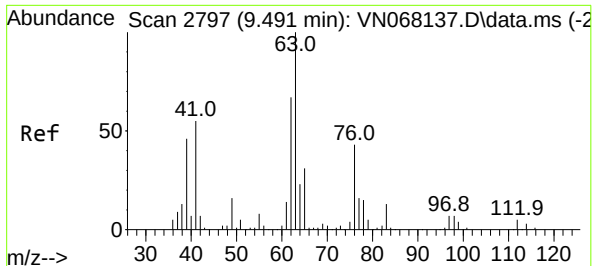

#45  
1,2-Dichloropropane  
Concen: 0.677 ug/l  
RT: 9.628 min Scan# 2848  
Delta R.T. 0.137 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 63 Resp: 2755  
Ion Ratio Lower Upper  
63 100  
65 0.0 24.3 36.5#

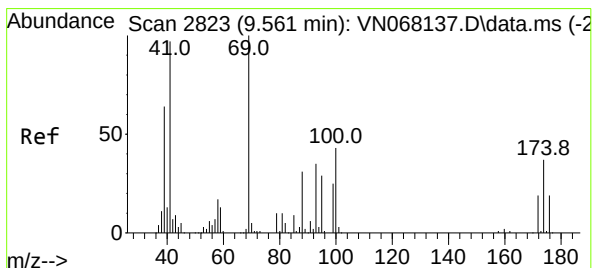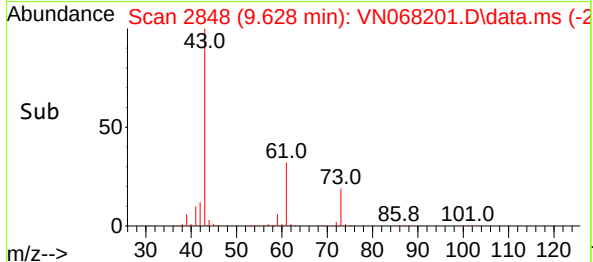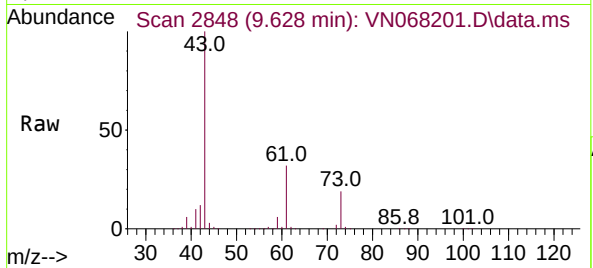

#48  
Methyl methacrylate  
Concen: 2.617 ug/l  
RT: 9.550 min Scan# 2819  
Delta R.T. -0.011 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Tgt Ion: 41 Resp: 8431  
Ion Ratio Lower Upper  
41 100  
69 0.0 64.6 96.8#  
39 0.0 53.3 79.9#


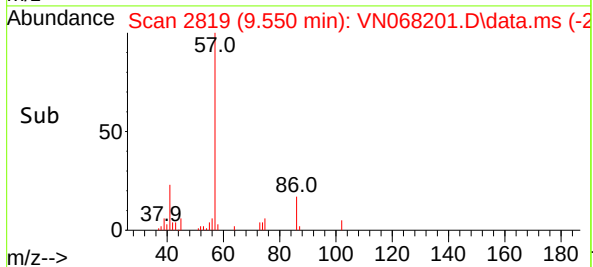

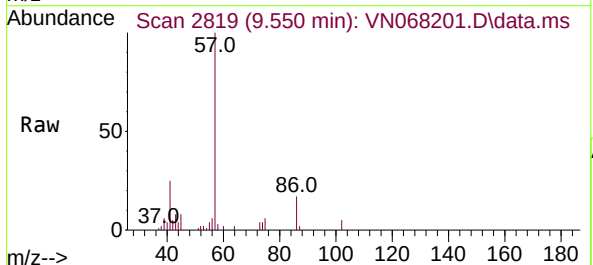


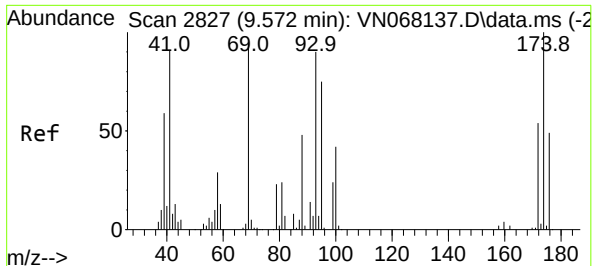

#49  
1,4-Dioxane  
Concen: 0.706 ug/l  
RT: 9.612 min Scan# 2842  
Delta R.T. 0.040 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampleId :


Tgt Ion: 88 Resp: 55  
Ion Ratio Lower Upper  
88 100  
43 0.0 28.8 43.2#  
58 0.0 60.4 90.6#

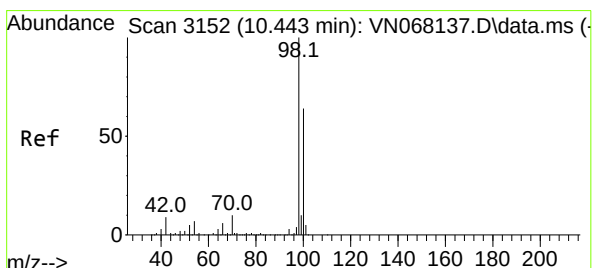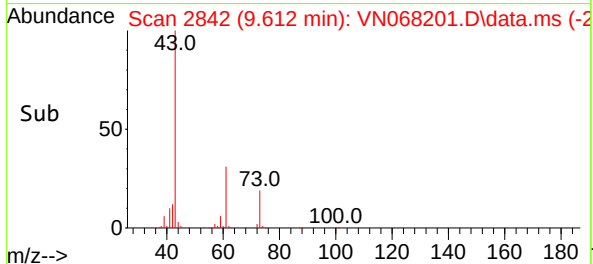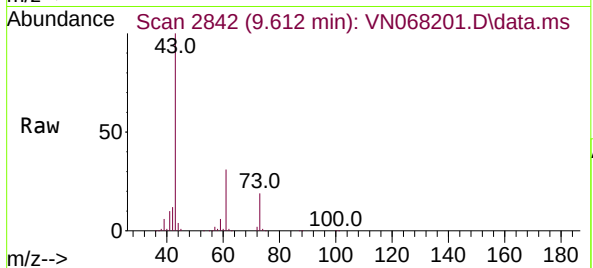

#50  
Toluene-d8  
Concen: 52.093 ug/l  
RT: 10.446 min Scan# 3153  
Delta R.T. 0.003 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Tgt Ion: 98 Resp: 863775  
Ion Ratio Lower Upper  
98 100  
100 63.9 51.7 77.5


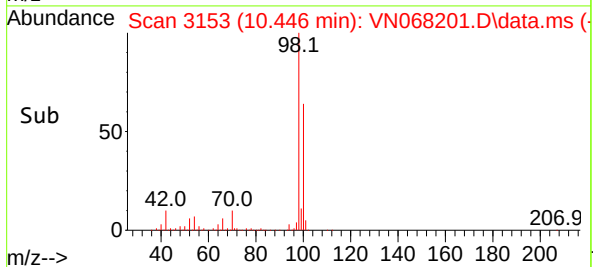

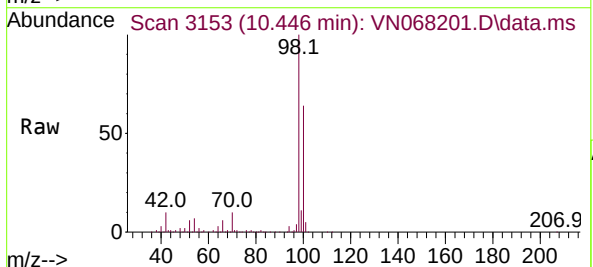




#51  
4-Methyl-2-Pentanone  
Concen: 0.822 ug/l  
RT: 10.336 min Scan# 3112  
Delta R.T. 0.003 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 43 Resp: 3902  
Ion Ratio Lower Upper  
43 100  
58 77.1 28.6 43.0#

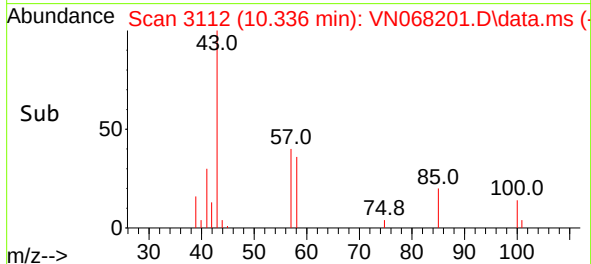

#54  
cis-1,3-Dichloropropene  
Concen: 10.257 ug/l  
RT: 10.247 min Scan# 3079  
Delta R.T. 0.056 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Tgt Ion: 75 Resp: 67307  
Ion Ratio Lower Upper  
75 100  
77 0.5 24.6 37.0#  
39 32.9 50.7 76.1#


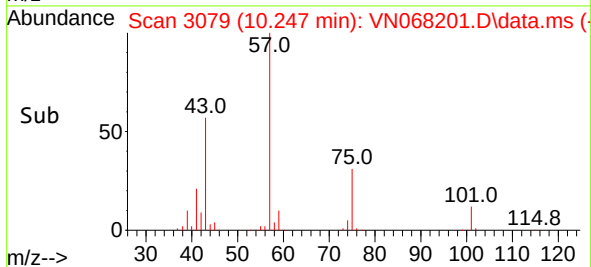

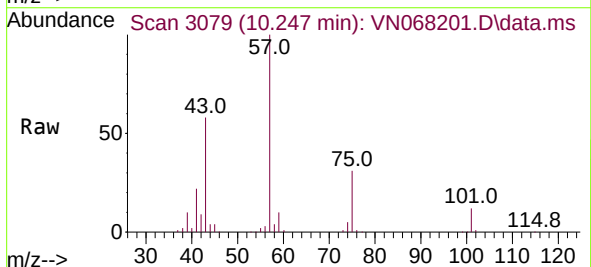


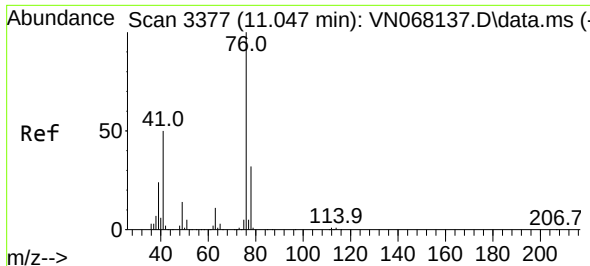

#57  
1,3-Dichloropropane  
Concen: 5.768 ug/l  
RT: 11.095 min Scan# 3395  
Delta R.T. 0.048 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampled :


Tgt Ion: 76 Resp: 41855  
Ion Ratio Lower Upper  
76 100  
78 0.2 25.7 38.5#

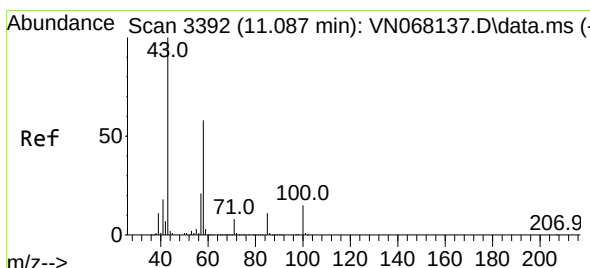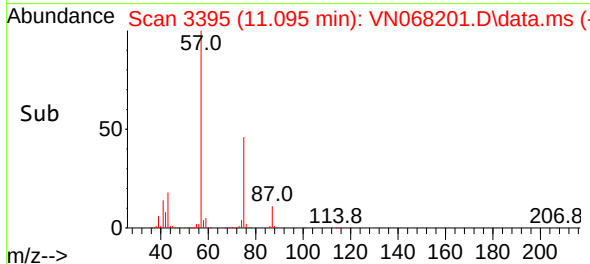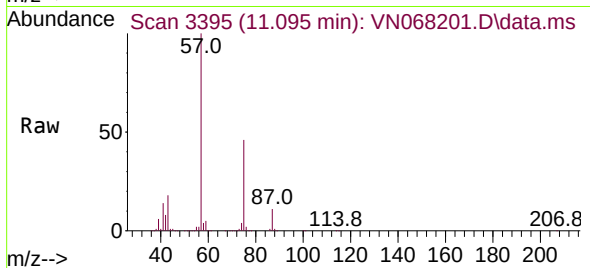

#59  
2-Hexanone  
Concen: 154.630 ug/l  
RT: 11.095 min Scan# 3395  
Delta R.T. 0.008 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Tgt Ion: 43 Resp: 509969  
Ion Ratio Lower Upper  
43 100  
58 20.6 24.7 74.1#


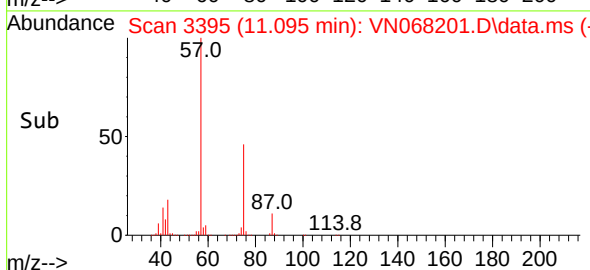

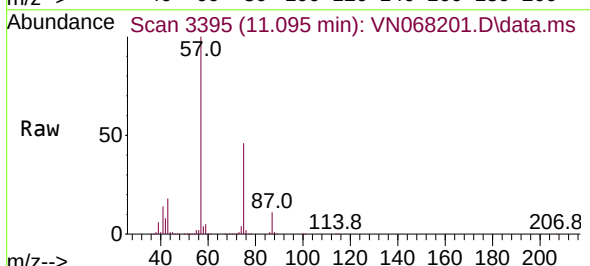


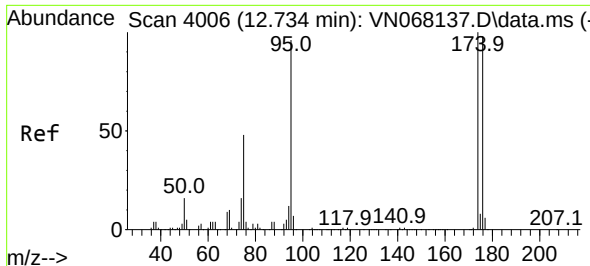

#62  
4-Bromofluorobenzene  
Concen: 51.339 ug/l  
RT: 12.736 min Scan# 4007  
Delta R.T. 0.002 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampleId :

Tgt Ion: 95 Resp: 283383  
Ion Ratio Lower Upper  
95 100  
174 93.6 0.0 122.0  
176 90.2 0.0 117.6

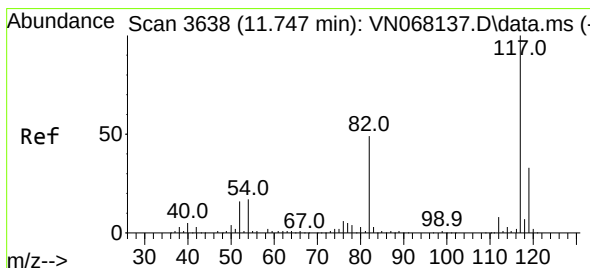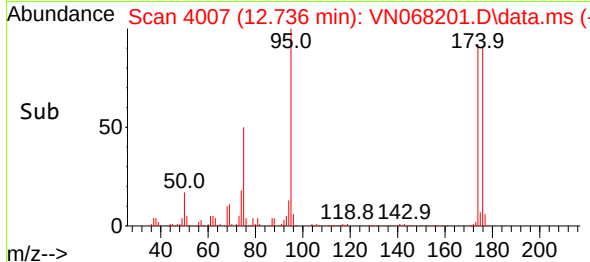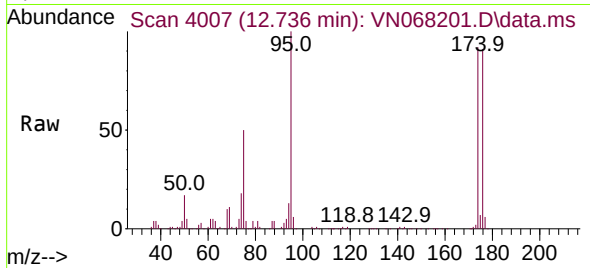


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.749 min Scan# 3639  
Delta R.T. 0.002 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Tgt Ion: 117 Resp: 739389  
Ion Ratio Lower Upper  
117 100  
82 49.5 53.1 79.7#  
119 32.4 25.5 38.3

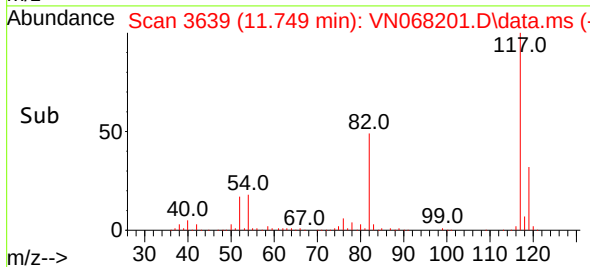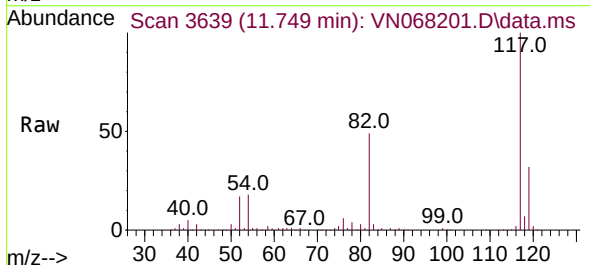







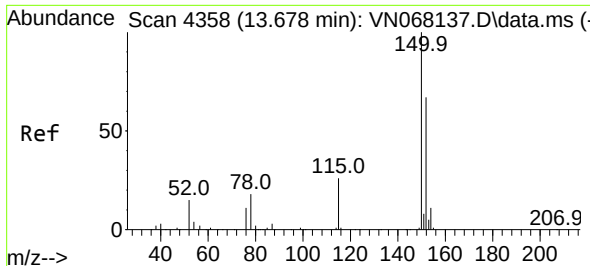

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.677 min Scan# 4358  
Delta R.T. -0.001 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29




Instrument :  
MSVOA\_N  
ClientSampled :


| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 152     | 100   |       |       |
| 115     | 55.6  | 36.1  | 108.5 |
| 150     | 159.1 | 0.0   | 351.8 |

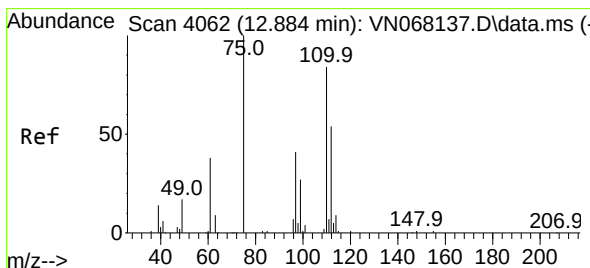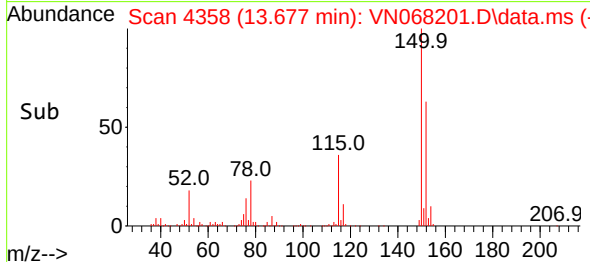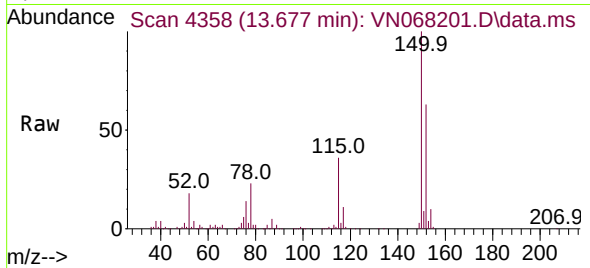

#76  
1,2,3-Trichloropropane  
Concen: 31.129 ug/l  
RT: 12.733 min Scan# 4006  
Delta R.T. -0.151 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 75      | 100   |       |       |
| 77      | 0.3   | 0.0   | 0.0#  |


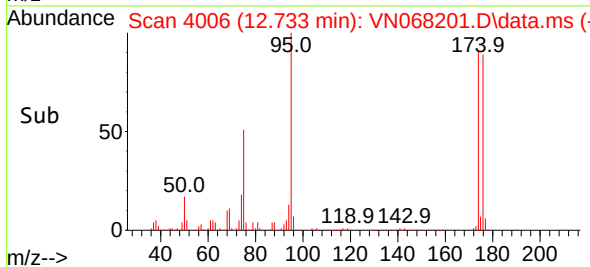

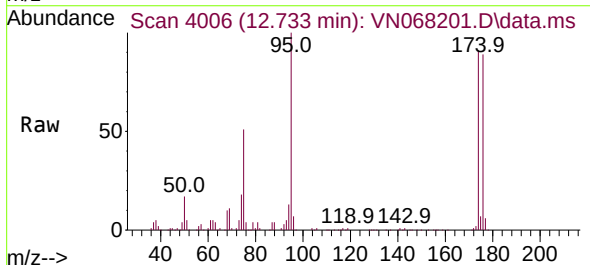




#81  
 trans-1,4-Dichloro-2-butene  
 Concen: 101.985 ug/l  
 RT: 12.733 min Scan# 4006  
 Delta R.T. 0.104 min  
 Lab File: VN068201.D  
 Acq: 18 Aug 2021 18:29




Instrument :  
 MSVOA\_N  
 ClientSampled :


Tgt Ion: 75 Resp: 142517  
 Ion Ratio Lower Upper  
 75 100  
 53 0.0 87.6 131.4#  
 89 0.0 37.8 56.8#

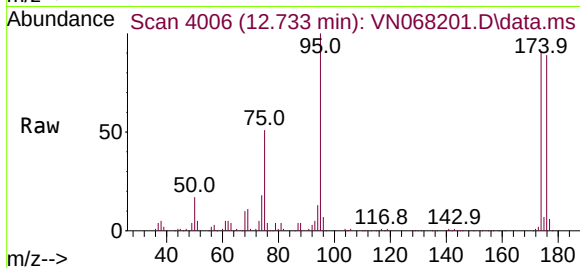

#93  
 1,2,4-Trichlorobenzene  
 Concen: 2.712 ug/l  
 RT: 15.268 min Scan# 4951  
 Delta R.T. 0.003 min  
 Lab File: VN068201.D  
 Acq: 18 Aug 2021 18:29

Tgt Ion:180 Resp: 133  
 Ion Ratio Lower Upper  
 180 100  
 182 0.0 47.5 142.5#  
 145 0.0 17.2 51.6#


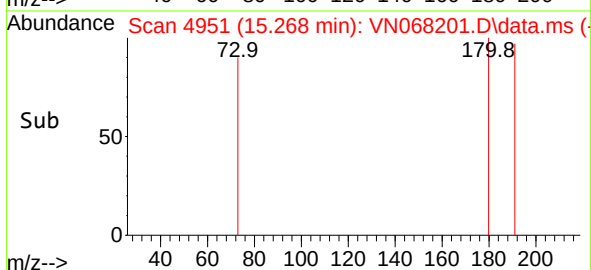

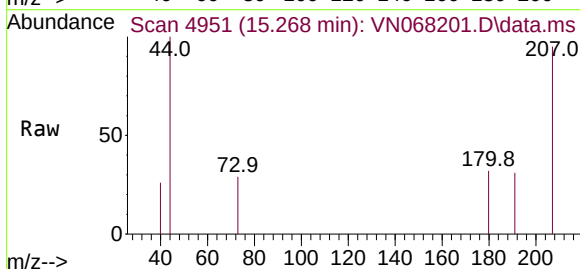




#95  
Naphthalene  
Concen: 3.397 ug/l  
RT: 15.507 min Scan# 5040  
Delta R.T. -0.000 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Instrument :  
MSVOA\_N  
ClientSampled :

Tgt Ion:128 Resp: 609  
Ion Ratio Lower Upper  
128 100  
127 0.0 10.6 15.8#  
129 0.0 8.6 12.8#

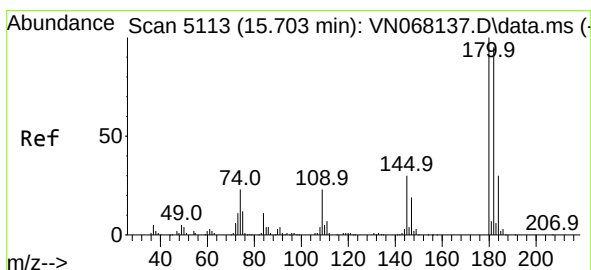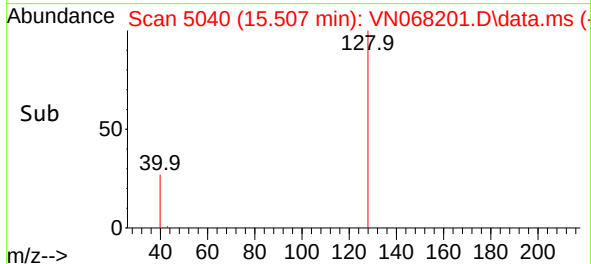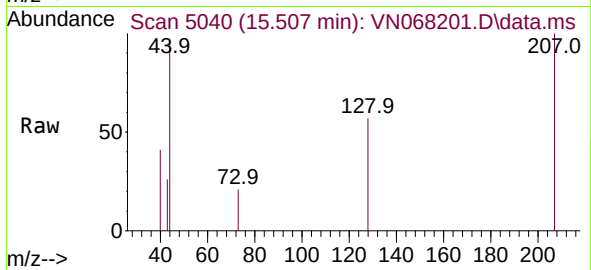

#96  
1,2,3-Trichlorobenzene  
Concen: 2.842 ug/l  
RT: 15.705 min Scan# 5114  
Delta R.T. 0.002 min  
Lab File: VN068201.D  
Acq: 18 Aug 2021 18:29

Tgt Ion:180 Resp: 51  
Ion Ratio Lower Upper  
180 100  
182 0.0 47.8 143.3#  
145 0.0 18.2 54.6#

