

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081822\
 Data File : VN073999.D
 Acq On : 18 Aug 2022 12:56
 Operator : JC\MD
 Sample : N4204-23DL 50X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-3DL2

Quant Time: Aug 18 21:49:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081522W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 16 00:45:21 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	668617	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	965455	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	906662	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.615	152	467078	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	315272	48.412	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	96.820%		
35) Dibromofluoromethane	7.951	113	307043	53.777	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	107.560%		
50) Toluene-d8	10.380	98	1025607	46.381	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	92.760%		
62) 4-Bromofluorobenzene	12.674	95	428068	58.329	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	116.660%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.269	50	1230	0.209	ug/l	100
11) Tert butyl alcohol	5.292	59	1049	0.720	ug/l #	72
13) Acrolein	3.998	56	353	0.346	ug/l #	16
16) Acetone	4.187	43	7936	2.583	ug/l #	42
18) Methyl Acetate	4.781	43	4325	Below Cal		98
19) Methyl tert-butyl Ether	5.540	73	4786	0.252	ug/l #	1
20) Methylene Chloride	5.004	84	3021	0.466	ug/l #	62
25) 2-Butanone	7.228	43	2218	0.455	ug/l #	45
26) 2,2-Dichloropropane	7.239	77	2273	0.235	ug/l #	53
31) Cyclohexane	8.016	56	26576	2.927	ug/l #	50
36) 1,1-Dichloropropene	8.016	75	41743	5.264	ug/l #	50
38) Carbon Tetrachloride	8.022	117	59395	6.552	ug/l #	16
39) Methylcyclohexane	9.398	83	8478	0.853	ug/l	96
40) Benzene	8.386	78	46349	1.852	ug/l	100
52) Toluene	10.445	92	71138	4.145	ug/l	98
67) Ethyl Benzene	11.786	91	908824	28.361	ug/l	97
68) m/p-Xylenes	11.898	106	92119	7.075	ug/l	97
69) o-Xylene	12.221	106	6883	0.527	ug/l	95
73) Isopropylbenzene	12.521	105	290398	8.538	ug/l	100
76) 1,2,3-Trichloropropane	12.668	75	210118	21.643	ug/l #	1
78) n-propylbenzene	12.863	91	329646	9.093	ug/l	98
79) 2-Chlorotoluene	12.863	91	329646	14.591	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.998	105	45018	1.627	ug/l	100
81) trans-1,4-Dichloro-2-b...	12.668	75	210118	61.558	ug/l #	10
82) 4-Chlorotoluene	12.863	91	329646	15.362	ug/l #	40
83) tert-Butylbenzene	13.310	119	11417	0.448	ug/l #	70
84) 1,2,4-Trimethylbenzene	13.310	105	78816	2.853	ug/l	98
85) sec-Butylbenzene	13.439	105	8743	0.265	ug/l #	70
89) n-Butylbenzene	13.886	91	7025	0.315	ug/l #	73
90) Hexachloroethane	14.151	117	5483	1.067	ug/l #	9
95) Naphthalene	15.433	128	195462	5.975	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Aug 18 21:49:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081522W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 16 00:45:21 2022
Response via : Initial Calibration







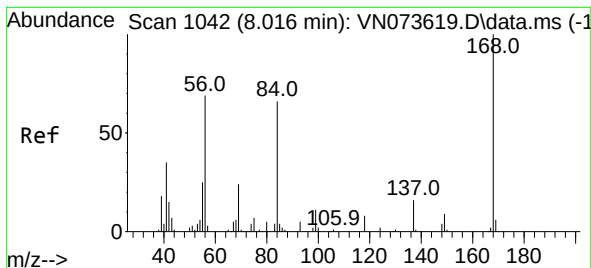

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56




Instrument :
MSVOA_N
ClientSampleId :
MW-3DL2


Tgt Ion:168 Resp: 668617
Ion Ratio Lower Upper
168 100
99 49.1 42.3 63.5

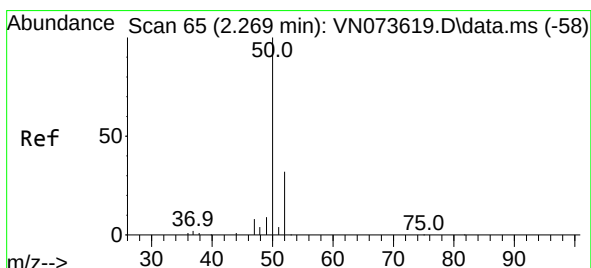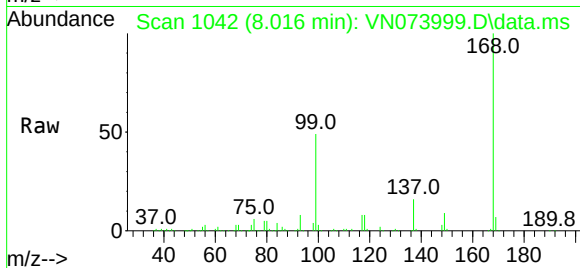

#3
Chloromethane
Concen: 0.209 ug/l
RT: 2.269 min Scan# 65
Delta R.T. 0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56

Tgt Ion: 50 Resp: 1230
Ion Ratio Lower Upper
50 100
52 32.0 25.7 38.5

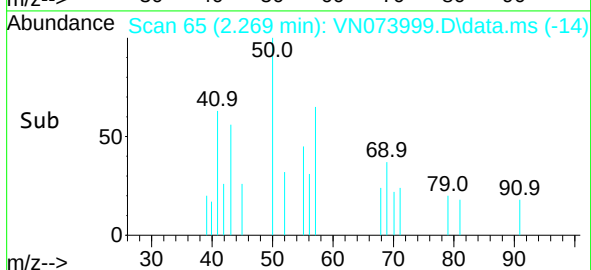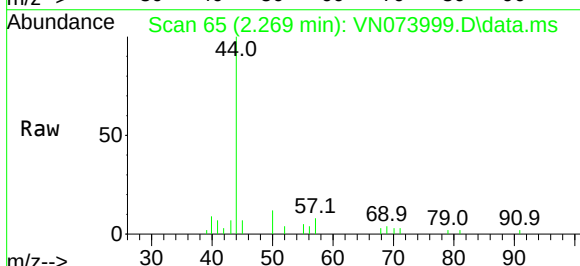



#11

Tert butyl alcohol

Concen: 0.720 ug/l

RT: 5.292 min Scan# 51

Delta R.T. 0.000 min

Lab File: VN073999.D

Acq: 18 Aug 2022 12:56

Instrument :

MSVOA_N

ClientSampleId :





MW-3DL2

Tgt Ion: 59 Resp: 1049

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#

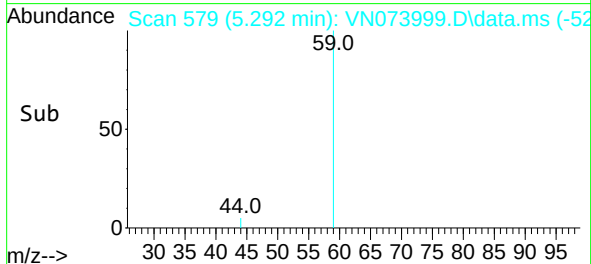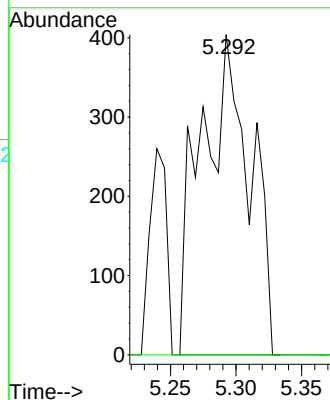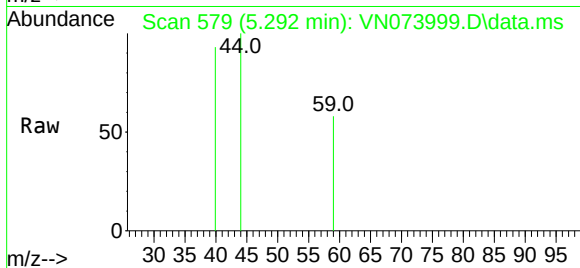

#13

Acrolein

Concen: 0.346 ug/l

RT: 3.998 min Scan# 359

Delta R.T. 0.017 min

Lab File: VN073999.D




Acq: 18 Aug 2022 12:56


Tgt Ion: 56 Resp: 353

Ion Ratio Lower Upper

56 100

55 0.0 54.8 82.2#

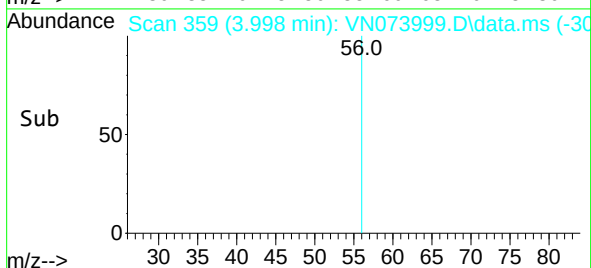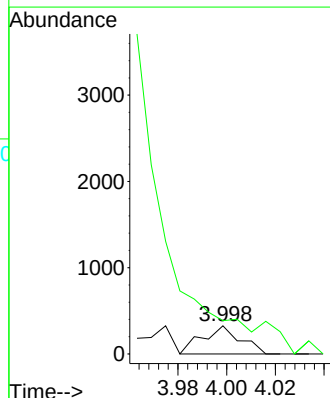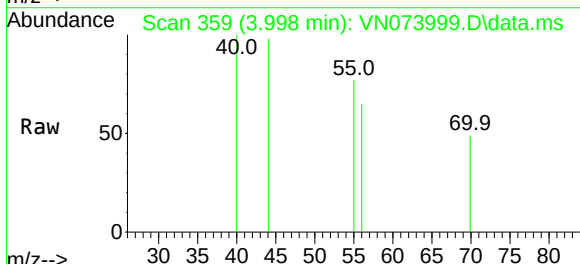

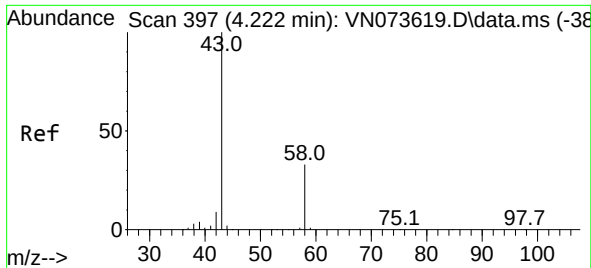

#16

Acetone

Concen: 2.583 ug/l

RT: 4.187 min Scan# 391

Delta R.T. -0.035 min

Lab File: VN073999.D

Acq: 18 Aug 2022 12:56

Instrument :

MSVOA_N

ClientSampleId :





MW-3DL2

Tgt Ion: 43 Resp: 7936

Ion Ratio Lower Upper

43 100

58 0.0 26.0 39.0#

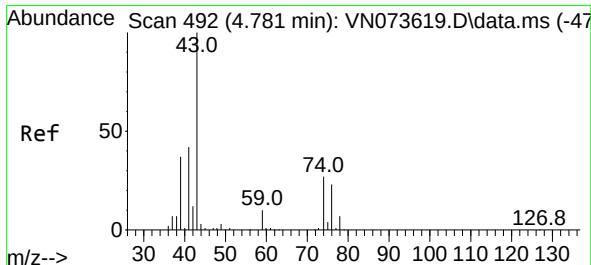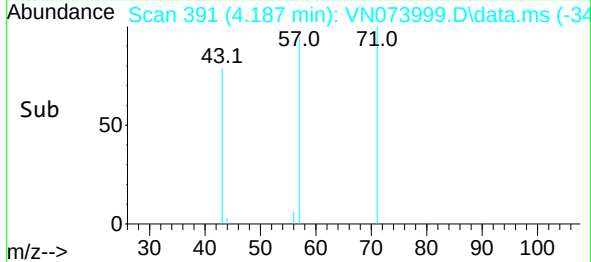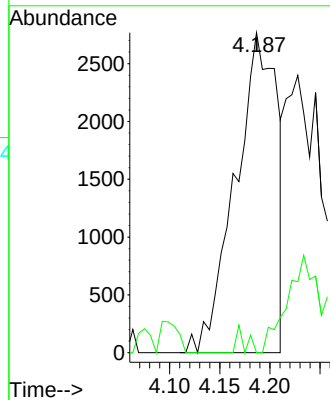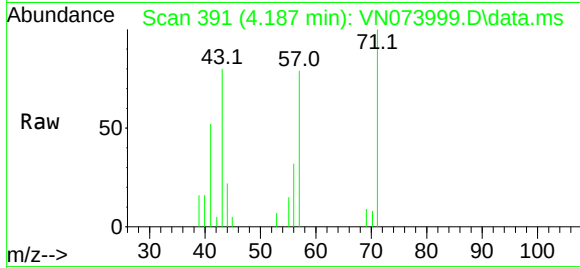

#18

Methyl Acetate

Concen: Below Cal

RT: 4.781 min Scan# 492

Delta R.T. -0.000 min

Lab File: VN073999.D




Acq: 18 Aug 2022 12:56


Tgt Ion: 43 Resp: 4325

Ion Ratio Lower Upper

43 100

74 25.8 21.6 32.4


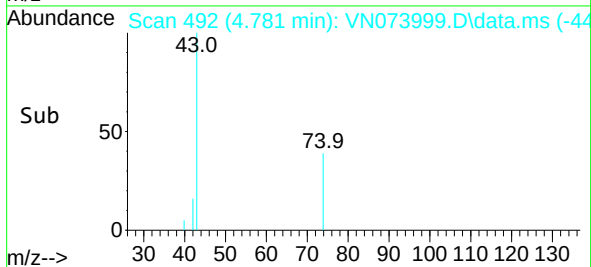
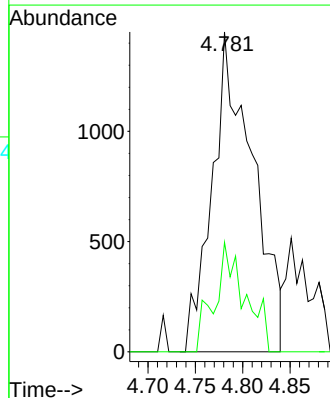
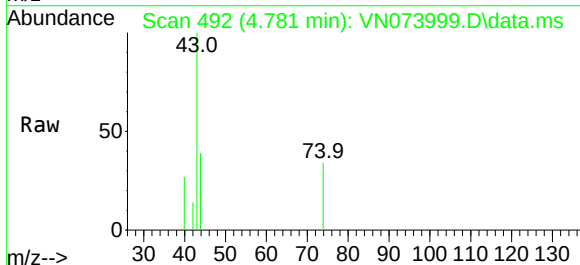


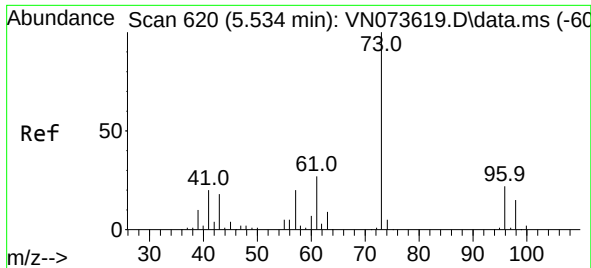

#19
Methyl tert-butyl Ether
Concen: 0.252 ug/l
RT: 5.540 min Scan# 61
Delta R.T. 0.006 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56




Instrument :
MSVOA_N
ClientSampleId :
MW-3DL2


Tgt Ion: 73 Resp: 4786
Ion Ratio Lower Upper
73 100
57 357.4 17.6 26.4#

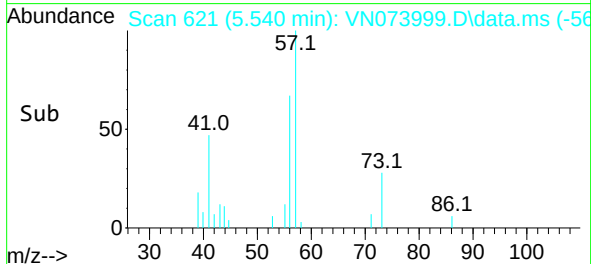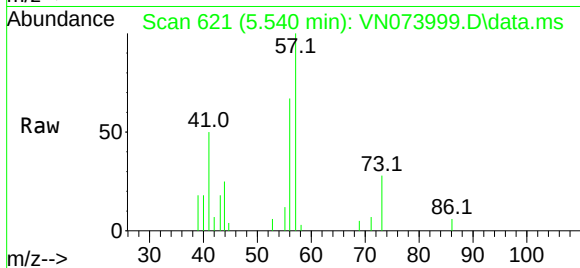

#20
Methylene Chloride
Concen: 0.466 ug/l
RT: 5.004 min Scan# 530
Delta R.T. -0.006 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56

Tgt Ion: 84 Resp: 3021
Ion Ratio Lower Upper
84 100
49 70.1 88.3 132.5#
51 30.1 28.2 42.2
86 20.1 50.6 76.0#

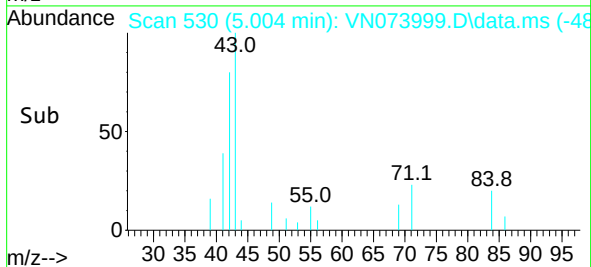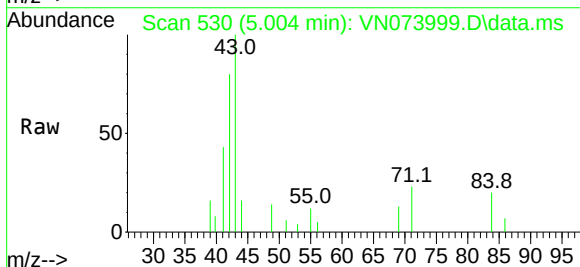

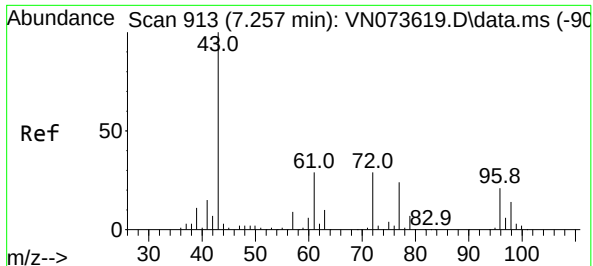

#25

2-Butanone

Concen: 0.455 ug/l

RT: 7.228 min Scan# 90

Delta R.T. -0.029 min

Lab File: VN073999.D

Acq: 18 Aug 2022 12:56

Instrument :

MSVOA_N

ClientSampleId :





MW-3DL2

Tgt Ion: 43 Resp: 2218

Ion Ratio Lower Upper

43 100

72 0.0 23.7 35.5#

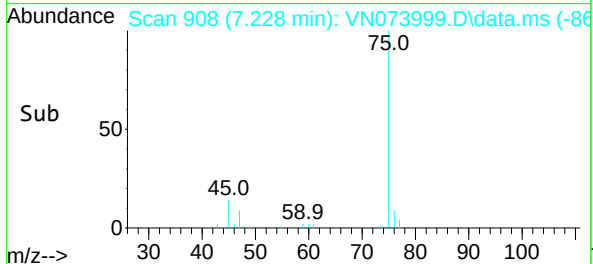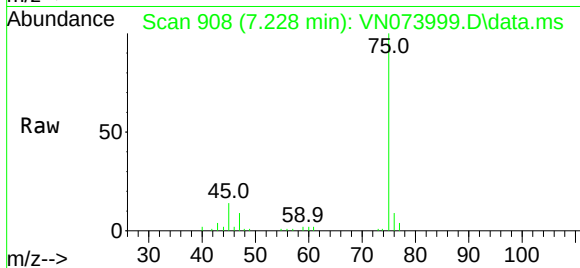

#26

2,2-Dichloropropane

Concen: 0.235 ug/l

RT: 7.239 min Scan# 910

Delta R.T. -0.012 min

Lab File: VN073999.D




Acq: 18 Aug 2022 12:56


Tgt Ion: 77 Resp: 2273

Ion Ratio Lower Upper

77 100

97 0.0 11.4 34.2#


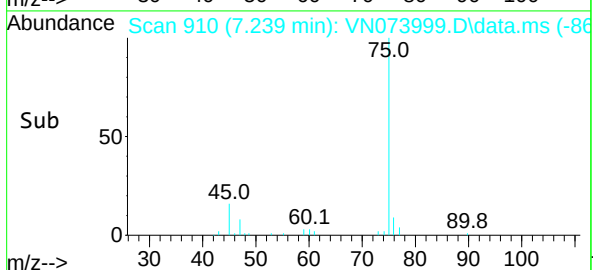

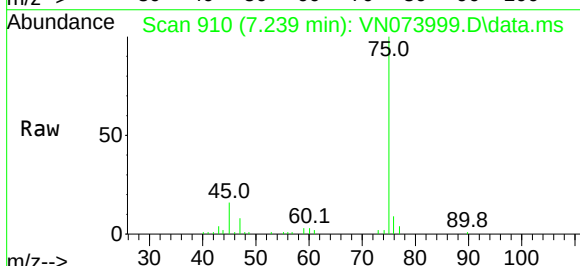




#31
Cyclohexane
Concen: 2.927 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.006 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56




Instrument :
MSVOA_N
ClientSampleId :
MW-3DL2


Tgt Ion: 56 Resp: 26576
Ion Ratio Lower Upper
56 100
69 97.6 27.8 41.8#
84 124.3 76.9 115.3#

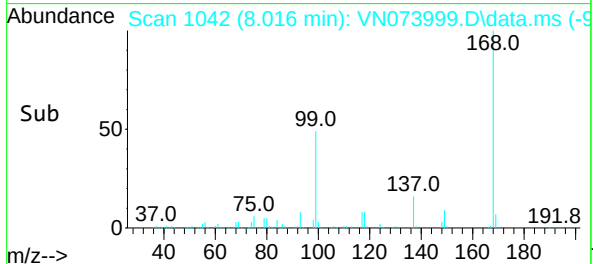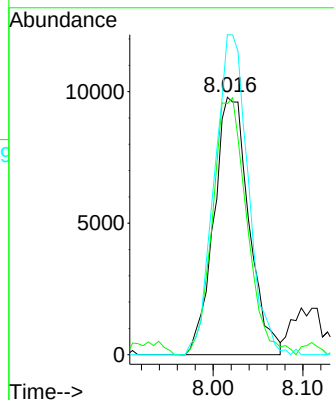

#33
1,2-Dichloroethane-d4
Concen: 48.412 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56

Tgt Ion: 65 Resp: 315272
Ion Ratio Lower Upper
65 100
67 52.4 0.0 104.8

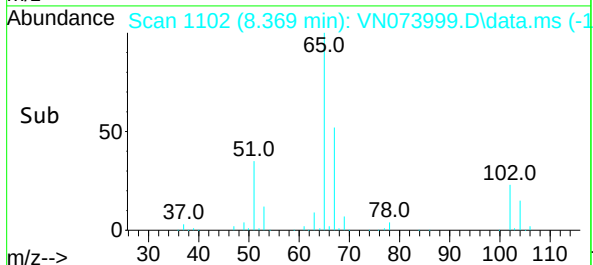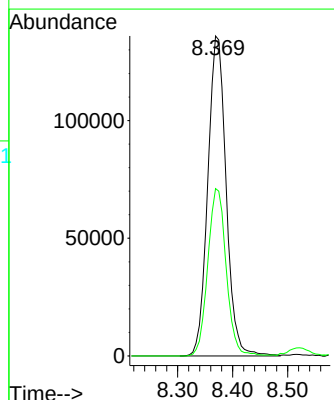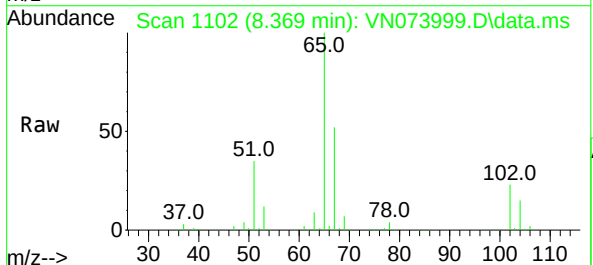

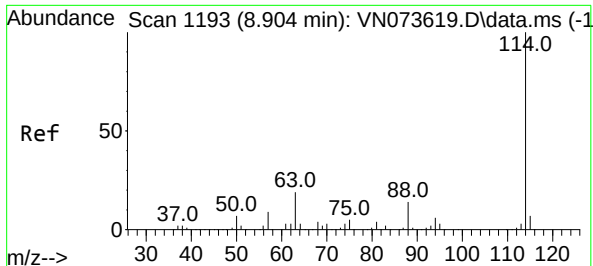

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. -0.000 min

Lab File: VN073999.D

Acq: 18 Aug 2022 12:56

Instrument :

MSVOA_N

ClientSampleId :

MW-3DL2





Tgt Ion:114 Resp: 965455

Ion Ratio Lower Upper

114 100

63 18.1 0.0 40.0

88 15.5 0.0 32.6

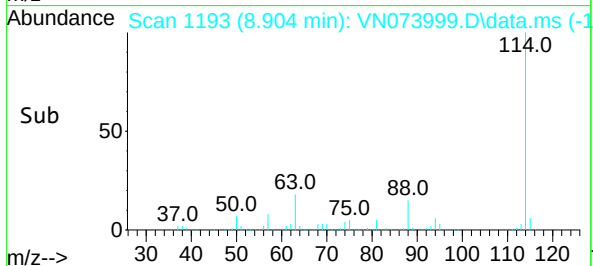

#35

Dibromofluoromethane

Concen: 53.777 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN073999.D

Acq: 18 Aug 2022 12:56




Tgt Ion:113 Resp: 307043


Ion Ratio Lower Upper

113 100

111 101.7 81.4 122.0

192 23.4 17.0 25.6

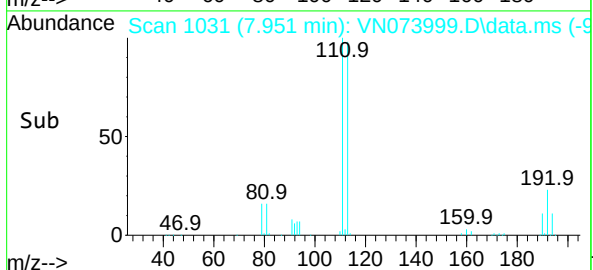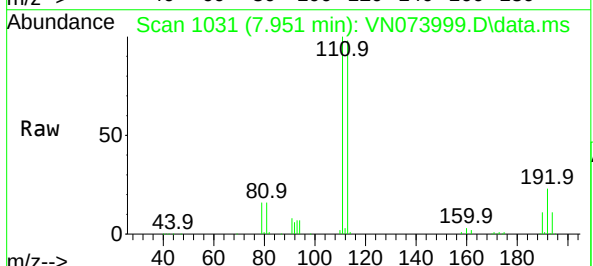



#36

1,1-Dichloropropene

Concen: 5.264 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.135 min

Lab File: VN073999.D

Acq: 18 Aug 2022 12:56

Instrument :

MSVOA_N

ClientSampleId :

MW-3DL2





Tgt Ion: 75 Resp: 41743

Ion Ratio Lower Upper

75 100

110 9.7 18.3 54.8#

77 0.8 25.1 37.7#

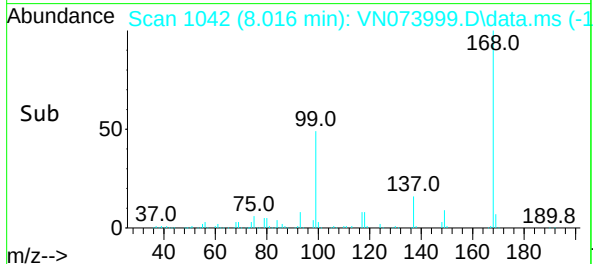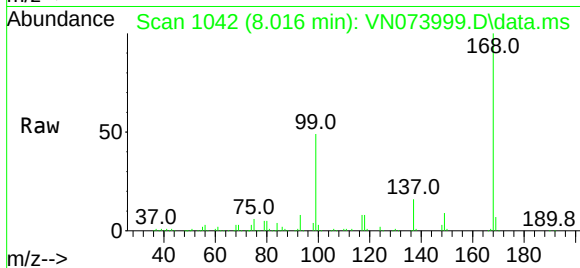

#38

Carbon Tetrachloride

Concen: 6.552 ug/l

RT: 8.022 min Scan# 1043

Delta R.T. -0.111 min

Lab File: VN073999.D

Acq: 18 Aug 2022 12:56




Tgt Ion: 117 Resp: 59395


Ion Ratio Lower Upper

117 100

119 4.6 75.8 113.8#

121 0.0 24.6 37.0#

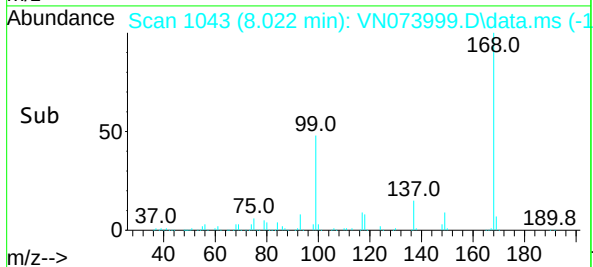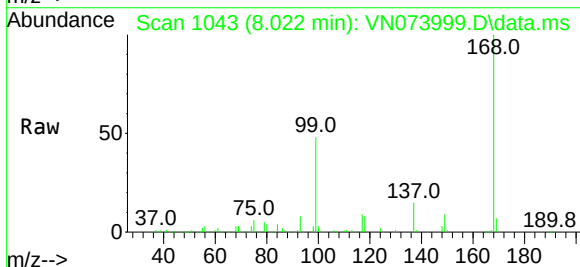



#39

Methylcyclohexane

Concen: 0.853 ug/l

RT: 9.398 min Scan# 1105

Delta R.T. 0.000 min

Lab File: VN073999.D

Acq: 18 Aug 2022 12:56

Instrument :

MSVOA_N

ClientSampleId :

MW-3DL2





Tgt Ion: 83 Resp: 8478

Ion Ratio Lower Upper

83 100

55 66.8 57.8 86.8

98 49.7 39.4 59.2

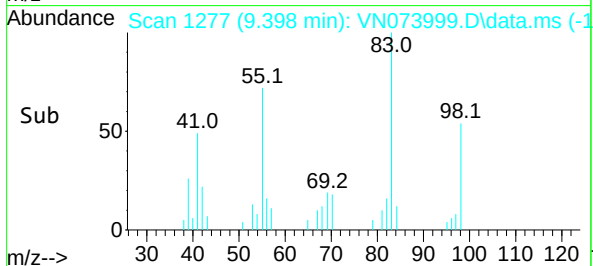

#40

Benzene

Concen: 1.852 ug/l

RT: 8.386 min Scan# 1105

Delta R.T. -0.006 min

Lab File: VN073999.D




Acq: 18 Aug 2022 12:56


Tgt Ion: 78 Resp: 46349

Ion Ratio Lower Upper

78 100

77 24.3 19.4 29.0


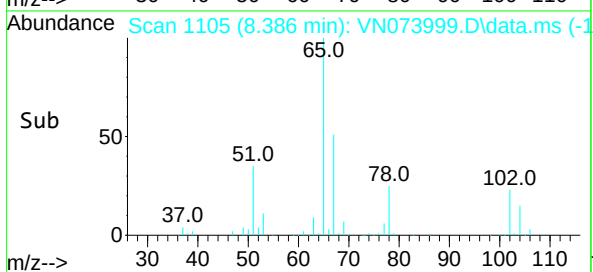

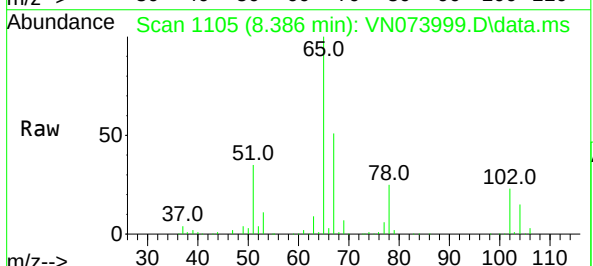


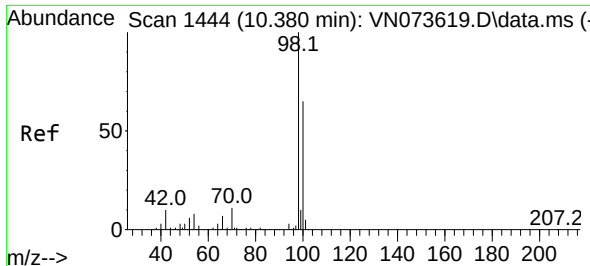

#50
Toluene-d8
Concen: 46.381 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56




Instrument :
MSVOA_N
ClientSampleId :
MW-3DL2


Tgt Ion: 98 Resp: 1025607
Ion Ratio Lower Upper
98 100
100 64.4 52.6 78.8

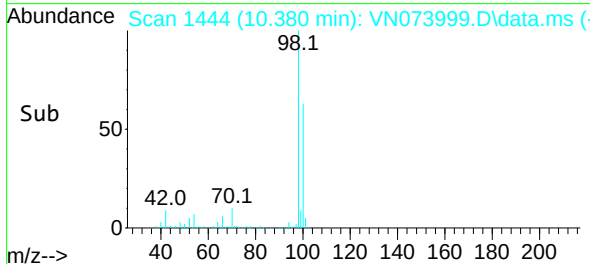

#52
Toluene
Concen: 4.145 ug/l
RT: 10.445 min Scan# 1455
Delta R.T. 0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56

Tgt Ion: 92 Resp: 71138
Ion Ratio Lower Upper
92 100
91 175.8 138.6 207.8




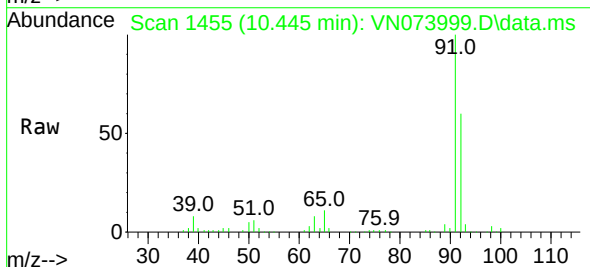




#62
4-Bromofluorobenzene
Concen: 58.329 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56




Instrument :
MSVOA_N
ClientSampleId :
MW-3DL2


Tgt Ion: 95 Resp: 428068
Ion Ratio Lower Upper
95 100
174 92.2 0.0 167.6
176 89.7 0.0 163.4

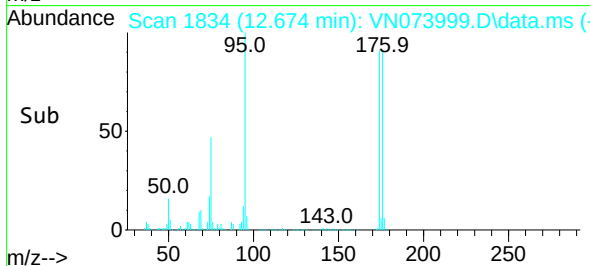

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. 0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56

Tgt Ion: 117 Resp: 906662
Ion Ratio Lower Upper
117 100
82 50.5 44.2 66.2
119 33.3 25.4 38.0


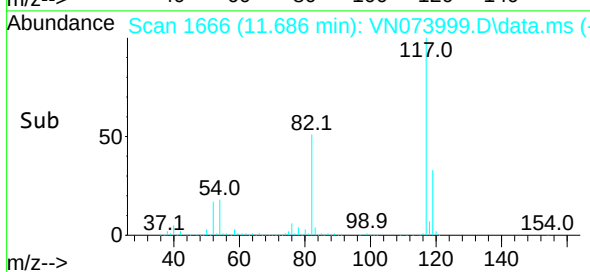

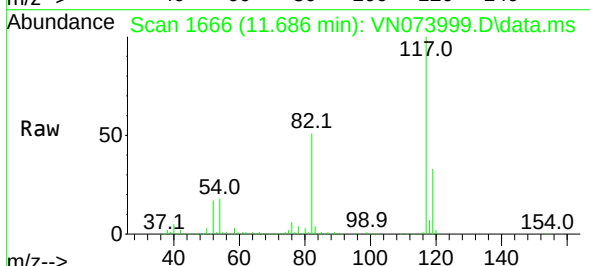




#67
Ethyl Benzene
Concen: 28.361 ug/l
RT: 11.786 min Scan# 1170
Delta R.T. 0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56




Instrument :
MSVOA_N
ClientSampleId :
MW-3DL2


Tgt Ion: 91 Resp: 908824
Ion Ratio Lower Upper
91 100
106 32.8 24.9 37.3

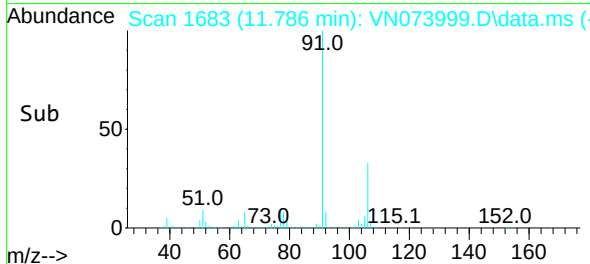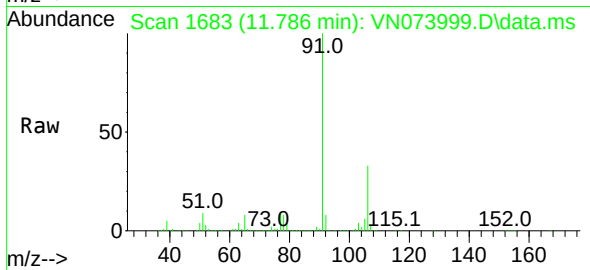

#68
m/p-Xylenes
Concen: 7.075 ug/l
RT: 11.898 min Scan# 1702
Delta R.T. -0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56

Tgt Ion: 106 Resp: 92119
Ion Ratio Lower Upper
106 100
91 194.4 158.9 238.3


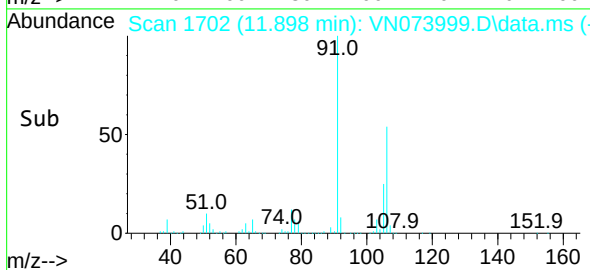

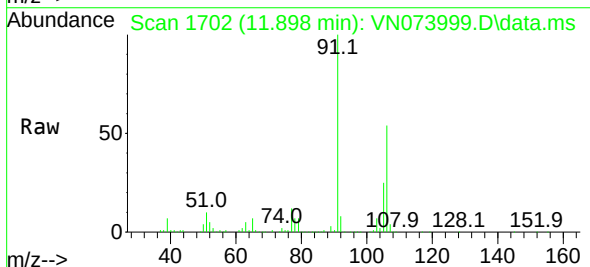




#69
o-Xylene
Concen: 0.527 ug/l
RT: 12.221 min Scan# 1757
Delta R.T. 0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56




Instrument :
MSVOA_N
ClientSampleId :
MW-3DL2


Tgt Ion:106 Resp: 6883
Ion Ratio Lower Upper
106 100
91 220.3 106.0 318.0

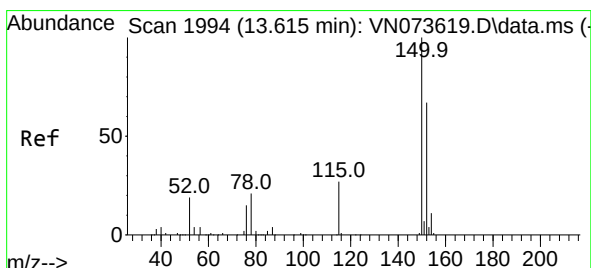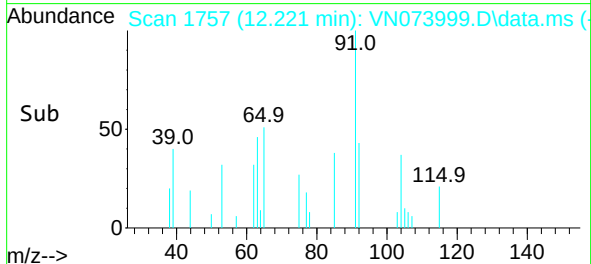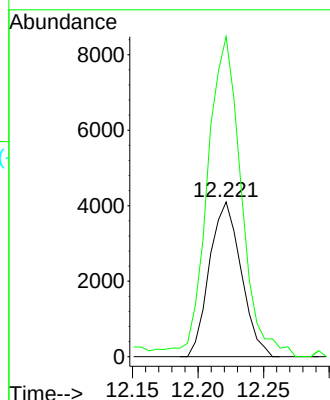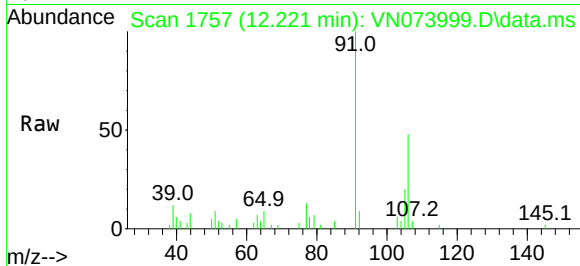

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.615 min Scan# 1994
Delta R.T. 0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56

Tgt Ion:152 Resp: 467078
Ion Ratio Lower Upper
152 100
115 55.6 28.9 86.7
150 156.6 0.0 356.2


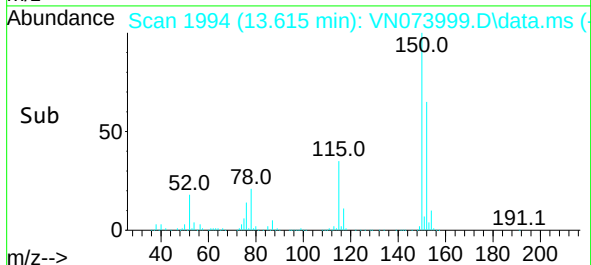
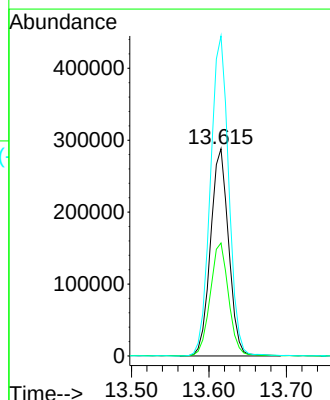
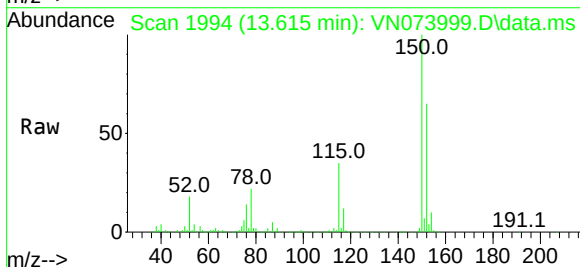




#73
Isopropylbenzene
Concen: 8.538 ug/l
RT: 12.521 min Scan# 1808
Delta R.T. 0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56




Instrument :
MSVOA_N
ClientSampleId :
MW-3DL2


Tgt Ion:105 Resp: 290398
Ion Ratio Lower Upper
105 100
120 27.0 13.5 40.4

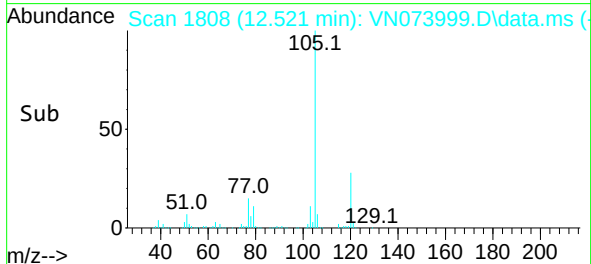

#76
1,2,3-Trichloropropane
Concen: 21.643 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. -0.153 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56

Tgt Ion: 75 Resp: 210118
Ion Ratio Lower Upper
75 100
77 1.4 98.5 295.5#

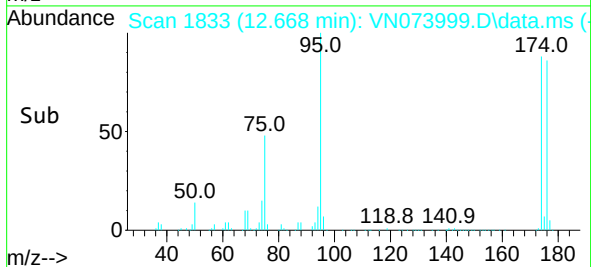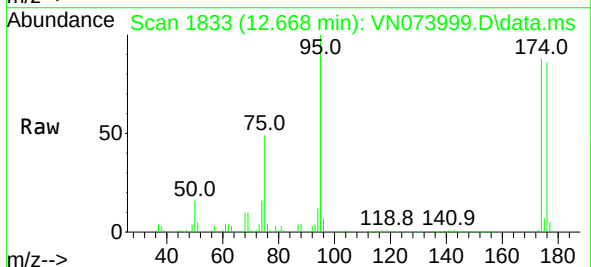



#78

n-propylbenzene

Concen: 9.093 ug/l

RT: 12.863 min Scan# 1866

Delta R.T. -0.000 min

Lab File: VN073999.D

Acq: 18 Aug 2022 12:56

Instrument :

MSVOA_N

ClientSampleId :





MW-3DL2

Tgt Ion: 91 Resp: 329646

Ion Ratio Lower Upper

91 100

120 24.7 11.9 35.5

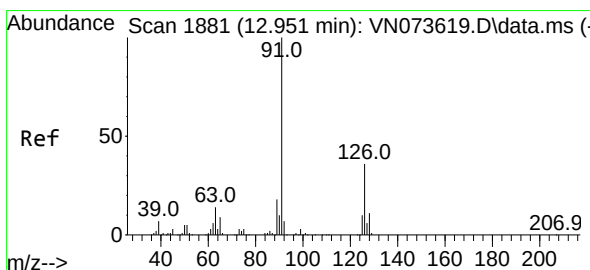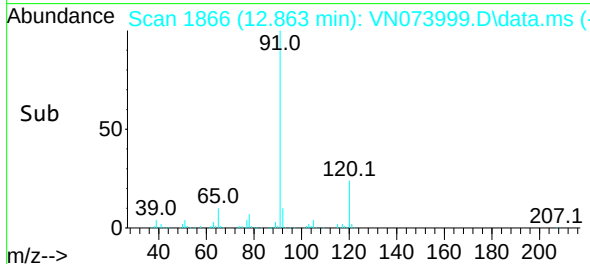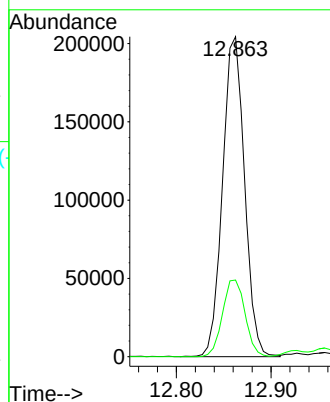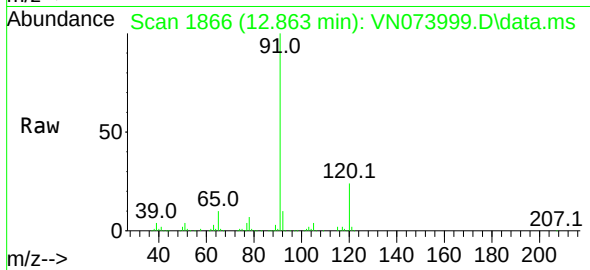

#79

2-Chlorotoluene

Concen: 14.591 ug/l

RT: 12.863 min Scan# 1866

Delta R.T. -0.088 min

Lab File: VN073999.D




Acq: 18 Aug 2022 12:56


Tgt Ion: 91 Resp: 329646

Ion Ratio Lower Upper

91 100

126 0.0 17.3 51.9#

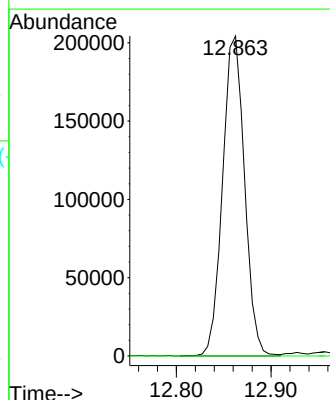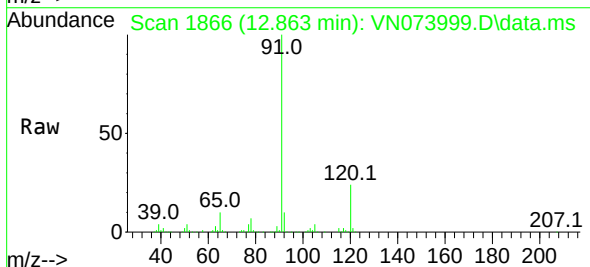

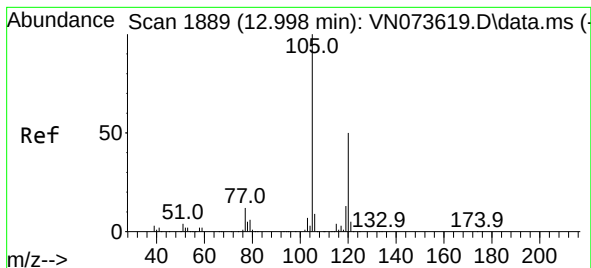

#80

1,3,5-Trimethylbenzene

Concen: 1.627 ug/l

RT: 12.998 min Scan# 1889

Delta R.T. -0.000 min

Lab File: VN073999.D

Acq: 18 Aug 2022 12:56

Instrument :

MSVOA_N

ClientSampleId :





MW-3DL2

Tgt Ion:105 Resp: 45018

Ion Ratio Lower Upper

105 100

120 49.8 24.9 74.7

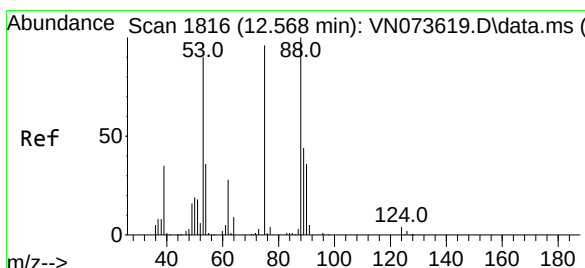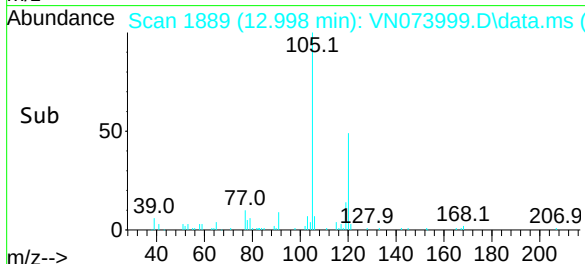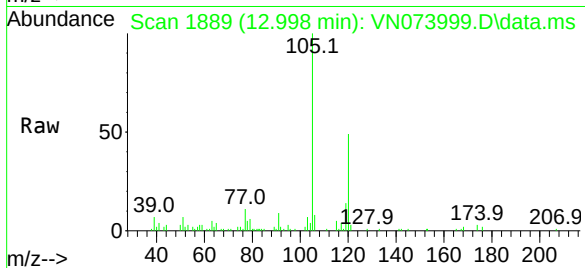

#81

trans-1,4-Dichloro-2-butene

Concen: 61.558 ug/l

RT: 12.668 min Scan# 1833

Delta R.T. 0.100 min

Lab File: VN073999.D

Acq: 18 Aug 2022 12:56




Tgt Ion: 75 Resp: 210118


Ion Ratio Lower Upper

75 100

53 0.0 78.0 117.0#

89 0.0 37.2 55.8#


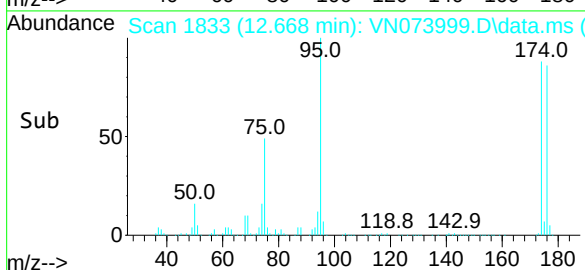

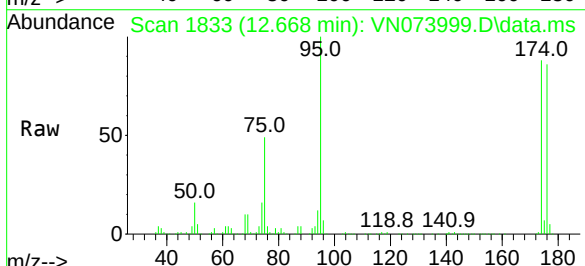




#82
4-Chlorotoluene
Concen: 15.362 ug/l
RT: 12.863 min Scan# 1897
Delta R.T. -0.182 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56




Instrument :
MSVOA_N
ClientSampleId :
MW-3DL2


Tgt Ion: 91 Resp: 329646
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#

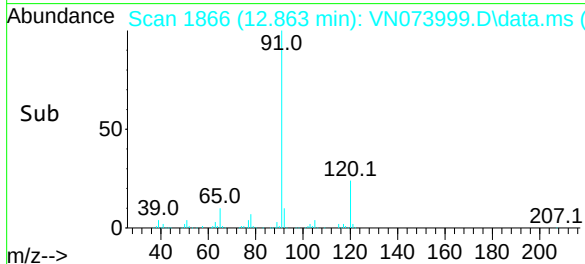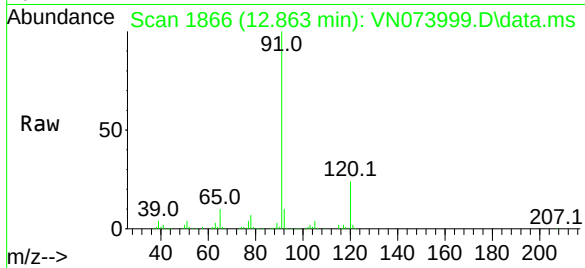

#83
tert-Butylbenzene
Concen: 0.448 ug/l
RT: 13.310 min Scan# 1942
Delta R.T. 0.047 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56

Tgt Ion: 119 Resp: 11417
Ion Ratio Lower Upper
119 100
91 79.2 31.6 94.8
134 0.0 13.7 41.1#


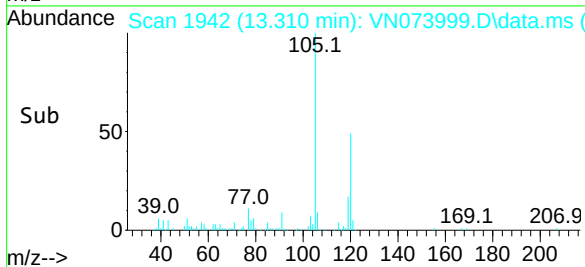

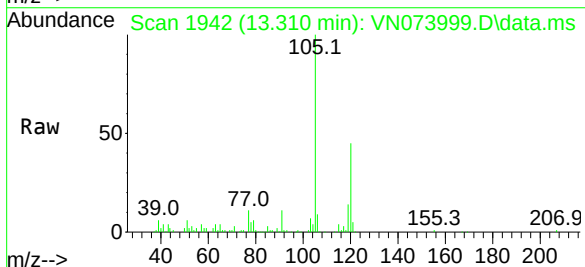




#84
1,2,4-Trimethylbenzene
Concen: 2.853 ug/l
RT: 13.310 min Scan# 1942
Delta R.T. -0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56




Instrument :
MSVOA_N
ClientSampleId :
MW-3DL2


Tgt Ion:105 Resp: 78816
Ion Ratio Lower Upper
105 100
120 45.1 23.3 69.8

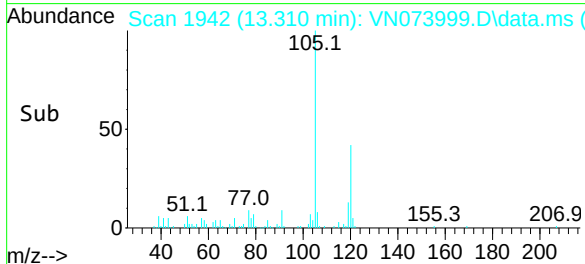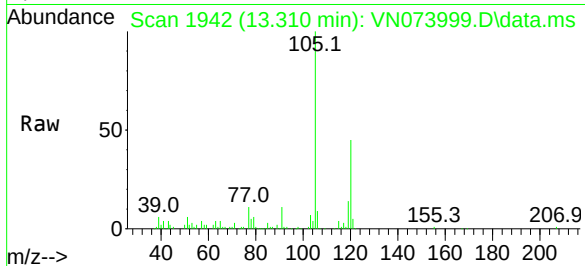

#85
sec-Butylbenzene
Concen: 0.265 ug/l
RT: 13.439 min Scan# 1964
Delta R.T. -0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56

Tgt Ion:105 Resp: 8743
Ion Ratio Lower Upper
105 100
134 34.4 10.4 31.1#

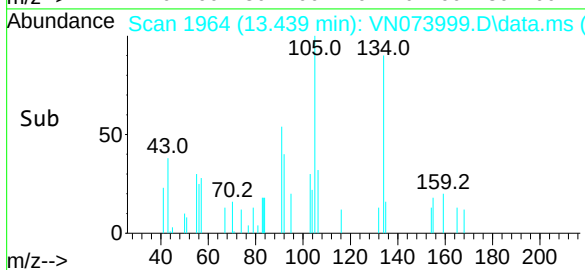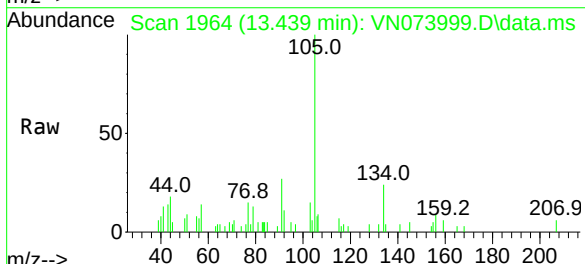



#89

n-Butylbenzene

Concen: 0.315 ug/l

RT: 13.886 min Scan# 2039

Delta R.T. 0.006 min

Lab File: VN073999.D

Acq: 18 Aug 2022 12:56

Instrument :

MSVOA_N

ClientSampleId :

MW-3DL2





Tgt Ion: 91 Resp: 7025

Ion Ratio Lower Upper

91 100

92 43.7 26.9 80.7

134 0.0 13.6 40.8#

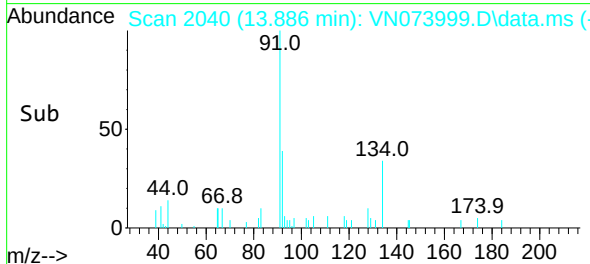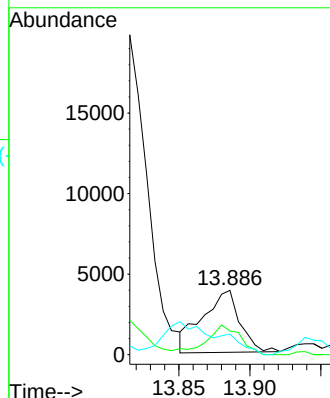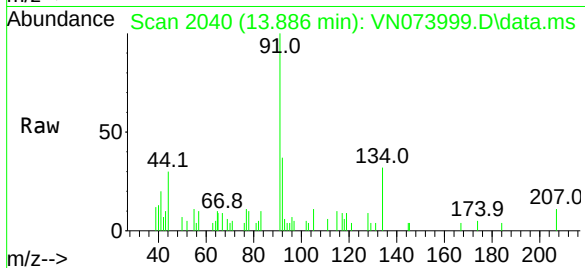

#90

Hexachloroethane

Concen: 1.067 ug/l

RT: 14.151 min Scan# 2085

Delta R.T. -0.000 min

Lab File: VN073999.D




Acq: 18 Aug 2022 12:56


Tgt Ion: 117 Resp: 5483

Ion Ratio Lower Upper

117 100


201 0.0 40.6 122.0#

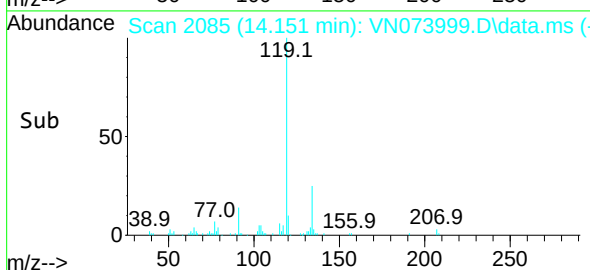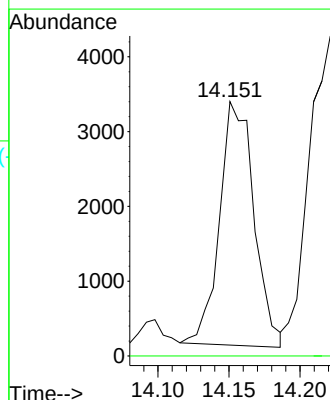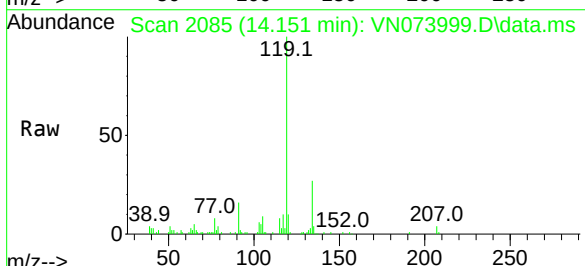

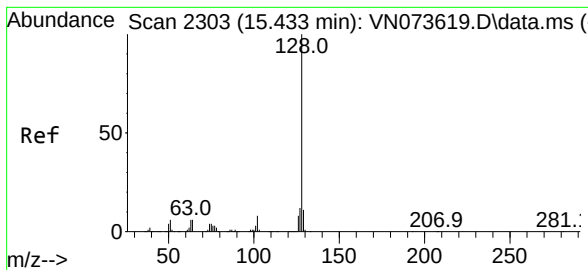

#95
Naphthalene
Concen: 5.975 ug/l
RT: 15.433 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN073999.D
Acq: 18 Aug 2022 12:56

Instrument :
MSVOA_N
ClientSampleId :
MW-3DL2

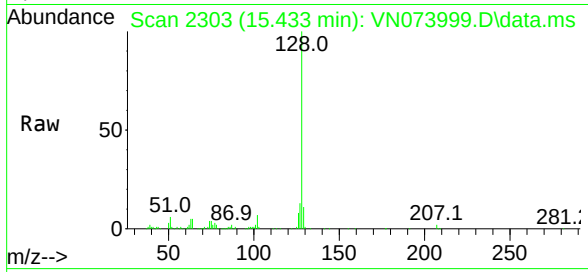

Tgt Ion:	128	Resp:	195462
Ion	Ratio	Lower	Upper
128	100		
127	13.5	10.3	15.5
129	11.4	8.6	13.0

