

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081823\
 Data File : VN078957.D
 Acq On : 18 Aug 2023 21:13
 Operator : JC\MD
 Sample : 04043-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Aug 18 23:50:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 16 02:42:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	202640	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	398097	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	377236	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	120436	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.589	65	162394	51.501	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 103.000%			
35) Dibromofluoromethane	8.171	113	132258	49.354	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 98.700%			
50) Toluene-d8	10.571	98	488294	49.074	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 98.140%			
62) 4-Bromofluorobenzene	12.853	95	145882	44.854	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 89.700%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.371	50	1150	0.293	ug/l #	87
6) Chloroethane	3.136	64	1311	0.545	ug/l #	43
11) Tert butyl alcohol	5.495	59	789	1.491	ug/l #	72
13) Acrolein	4.183	56	152	7.269	ug/l #	16
16) Acetone	4.436	43	37608	28.905	ug/l	88
17) Carbon Disulfide	4.706	76	1222	0.201	ug/l #	75
18) Methyl Acetate	5.036	43	6549	1.192	ug/l #	73
20) Methylene Chloride	5.277	84	8354	3.013	ug/l #	78
25) 2-Butanone	7.489	43	19434	9.316	ug/l #	69
29) Tetrahydrofuran	7.841	42	454	0.329	ug/l #	60
31) Cyclohexane	8.230	56	5693	Below Cal	#	15
36) 1,1-Dichloropropene	8.230	75	17492	4.339	ug/l #	44
37) Ethyl Acetate	7.571	43	4857	1.077	ug/l #	68
38) Carbon Tetrachloride	8.230	117	22137	5.481	ug/l #	14
42) 1,2-Dichloroethane	8.688	62	1163	0.261	ug/l #	73
43) Isopropyl Acetate	8.694	43	224634	28.179	ug/l #	71
45) 1,2-Dichloropropane	9.747	63	1813	0.572	ug/l #	45
48) Methyl methacrylate	9.659	41	5557	1.538	ug/l #	30
49) 1,4-Dioxane	9.747	88	101	1.641	ug/l #	1
51) 4-Methyl-2-Pentanone	10.447	43	66555	14.077	ug/l #	81
53) t-1,3-Dichloropropene	10.730	75	928	0.201	ug/l #	62
54) cis-1,3-Dichloropropene	10.365	75	50690	10.101	ug/l #	74
56) Ethyl methacrylate	10.982	69	2458	0.541	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	6650	1.268	ug/l #	42
59) 2-Hexanone	11.177	43	129539	37.827	ug/l #	19
71) Bromoform	12.853	173	1365	0.619	ug/l #	1
74) N-amyl acetate	12.488	43	2279	0.450	ug/l #	36
76) 1,2,3-Trichloropropane	12.853	75	82830	28.543	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.853	75	82830	72.915	ug/l #	15
95) Naphthalene	15.635	128	54	2.584	ug/l #	70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081823\
Data File : VN078957.D
Acq On : 18 Aug 2023 21:13
Operator : JC\MD
Sample : 04043-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Aug 18 23:50:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 16 02:42:02 2023
Response via : Initial Calibration




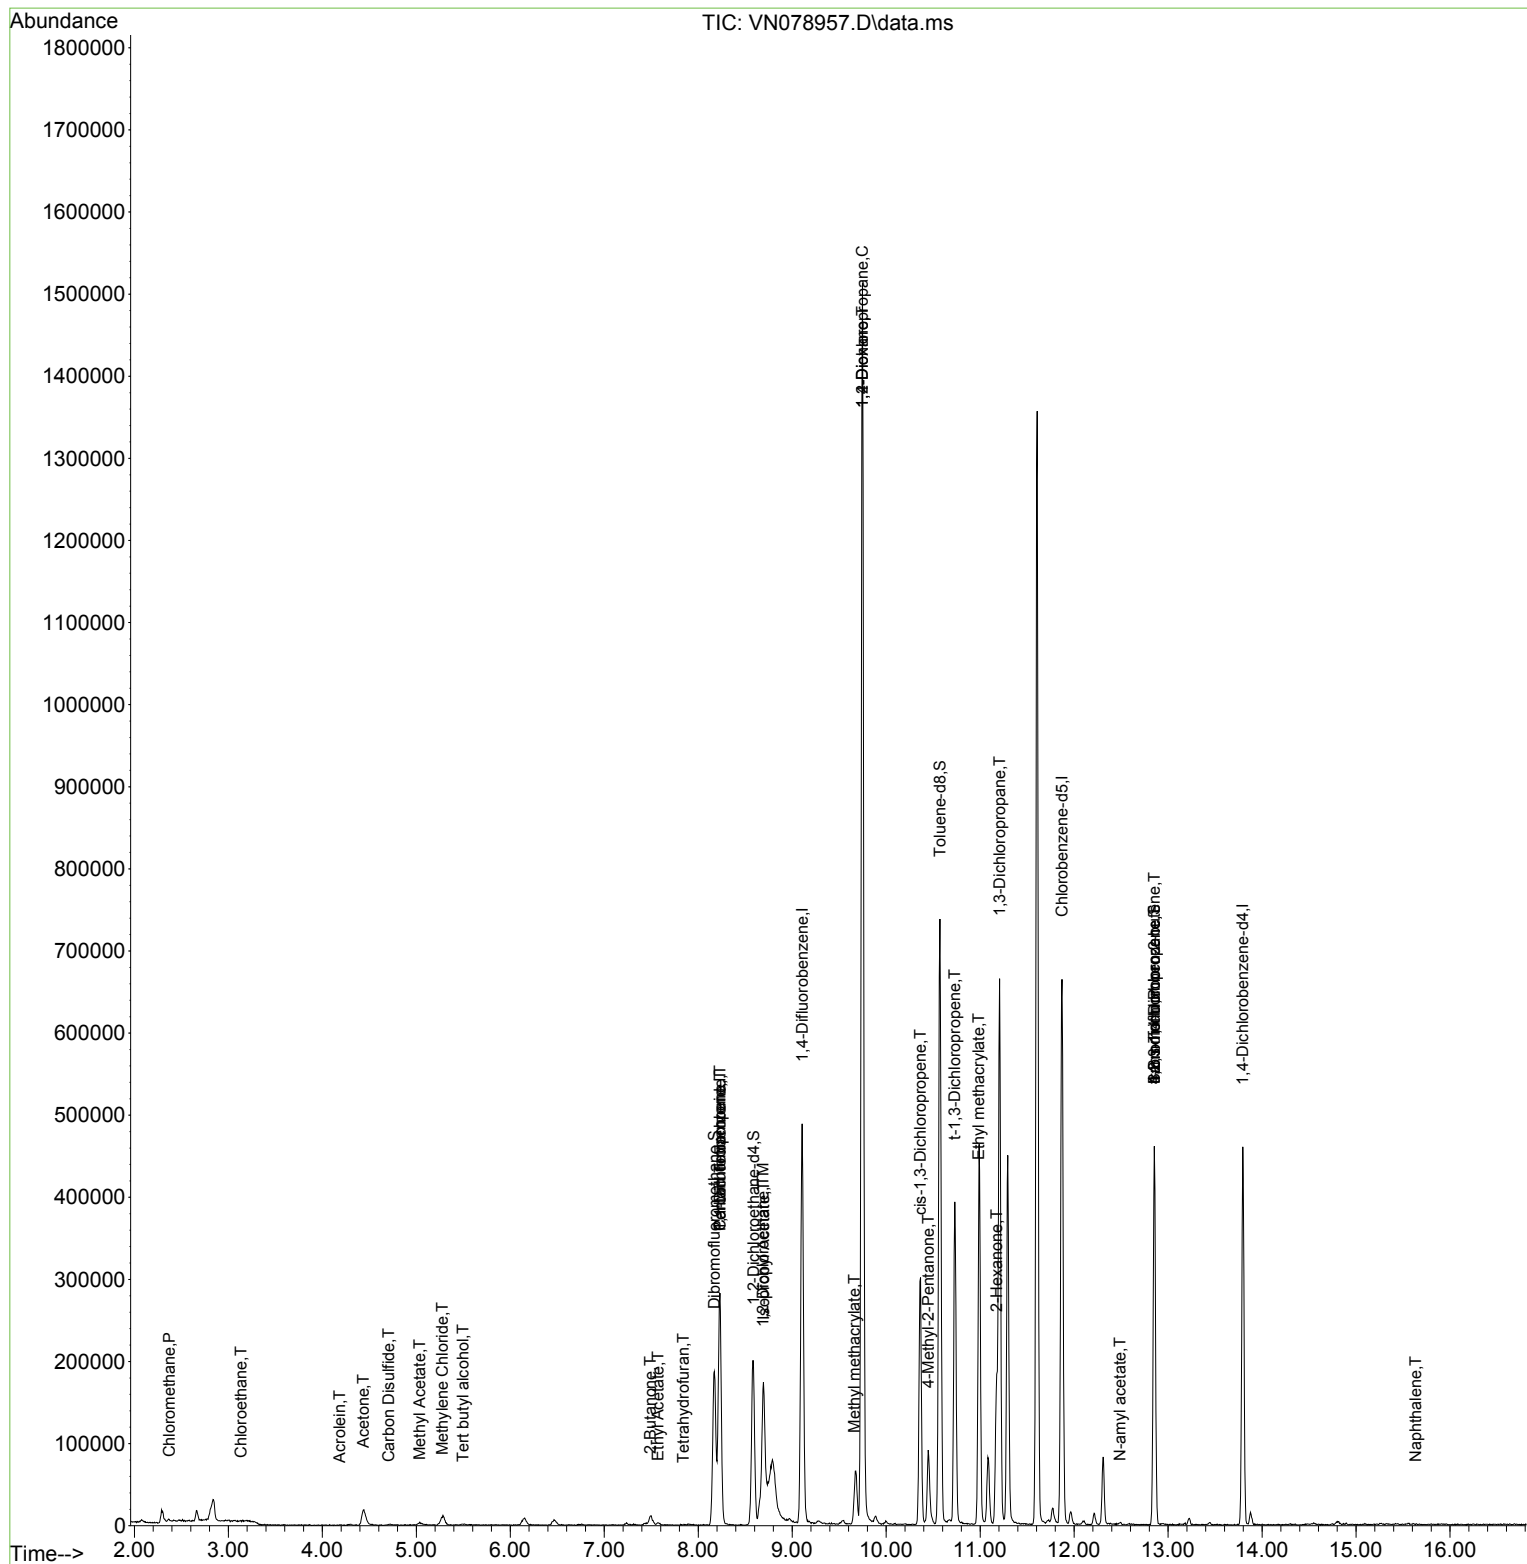


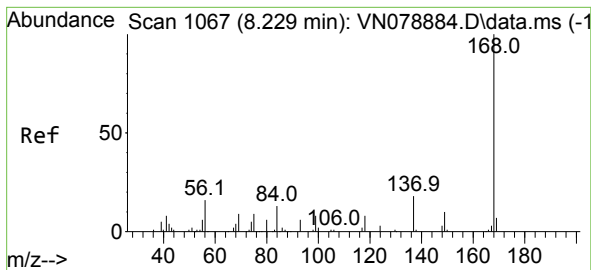

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 202640
Ion Ratio Lower Upper
168 100
99 60.1 53.0 79.6

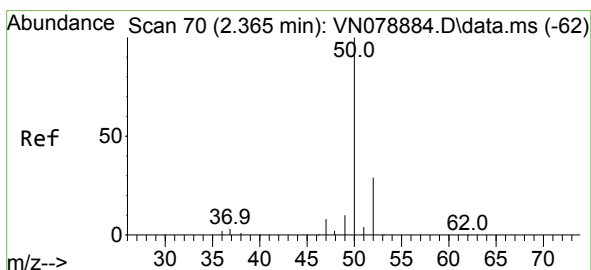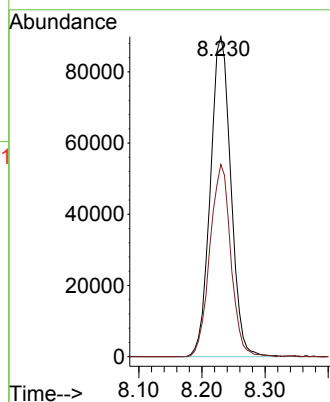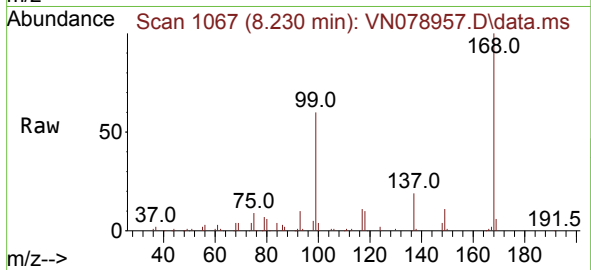

#3
Chloromethane
Concen: 0.293 ug/l
RT: 2.371 min Scan# 71
Delta R.T. 0.000 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13

Tgt Ion: 50 Resp: 1150
Ion Ratio Lower Upper
50 100
52 25.8 26.5 39.7#



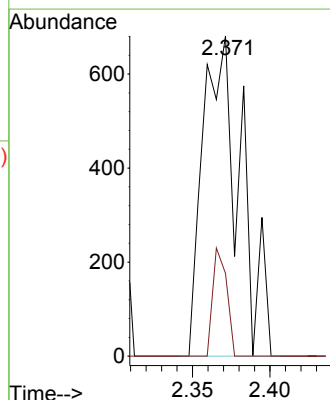
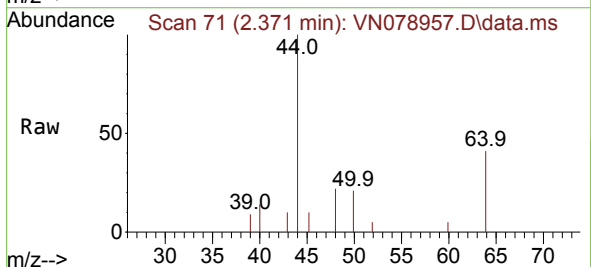




#6
Chloroethane
Concen: 0.545 ug/l
RT: 3.136 min Scan# 201
Delta R.T. 0.018 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 64 Resp: 1311
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#

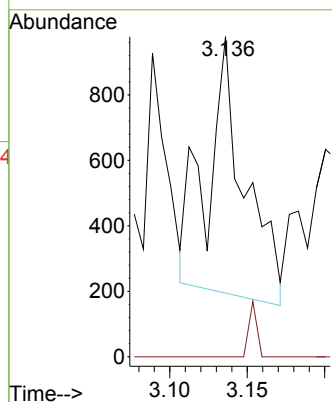

#11
Tert butyl alcohol
Concen: 1.491 ug/l
RT: 5.495 min Scan# 602
Delta R.T. -0.047 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13


Tgt Ion: 59 Resp: 789
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

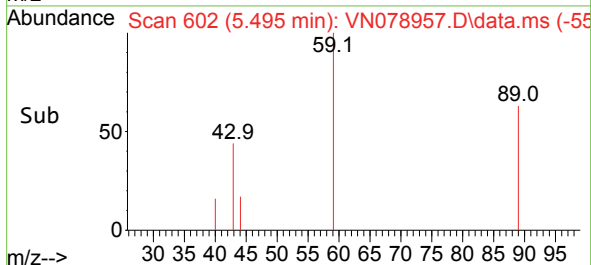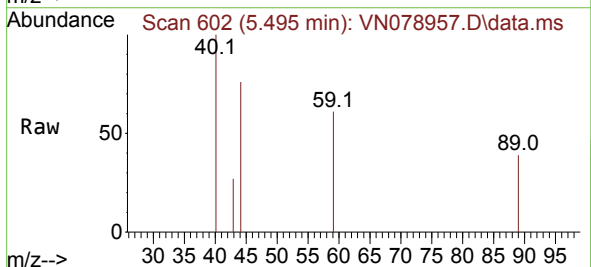






#13
Acrolein
Concen: 7.269 ug/l
RT: 4.183 min Scan# 379
Delta R.T. -0.012 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 152
Ion Ratio Lower Upper
56 100
55 0.0 54.5 81.7#



#16
Acetone
Concen: 28.905 ug/l
RT: 4.436 min Scan# 422
Delta R.T. -0.006 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13


Tgt Ion: 43 Resp: 37608
Ion Ratio Lower Upper
43 100
58 28.0 28.0 42.0

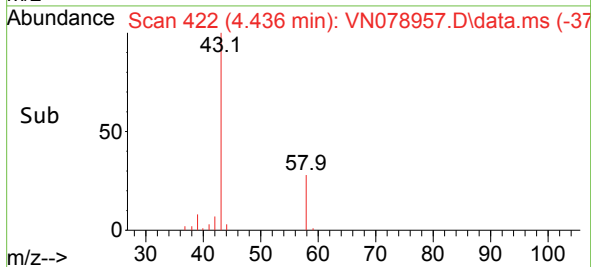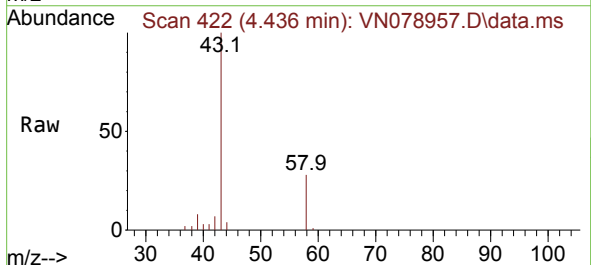






#17
Carbon Disulfide
Concen: 0.201 ug/l
RT: 4.706 min Scan# 417
Delta R.T. -0.018 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 76 Resp: 1222
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#

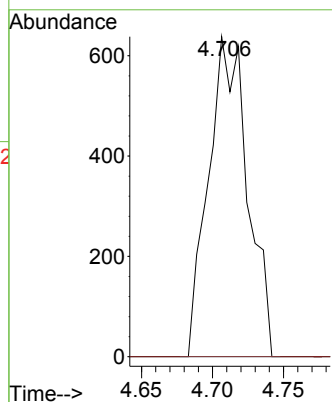

#18
Methyl Acetate
Concen: 1.192 ug/l
RT: 5.036 min Scan# 524
Delta R.T. -0.006 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13


Tgt Ion: 43 Resp: 6549
Ion Ratio Lower Upper
43 100
74 17.6 26.2 39.4#

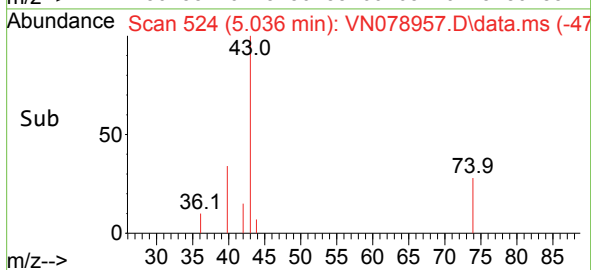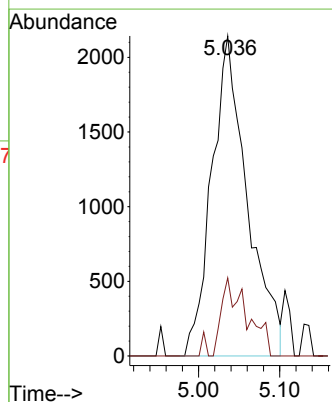






#20
Methylene Chloride
Concen: 3.013 ug/l
RT: 5.277 min Scan# 51
Delta R.T. -0.006 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:	84	Resp:	8354
Ion	Ratio	Lower	Upper
84	100		
49	117.6	79.7	119.5
51	27.1	25.2	37.8
86	39.0	53.3	79.9#



#25
2-Butanone
Concen: 9.316 ug/l
RT: 7.489 min Scan# 941
Delta R.T. -0.005 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13

Tgt Ion:	43	Resp:	19434
Ion	Ratio	Lower	Upper
43	100		
72	19.1	30.2	45.2#

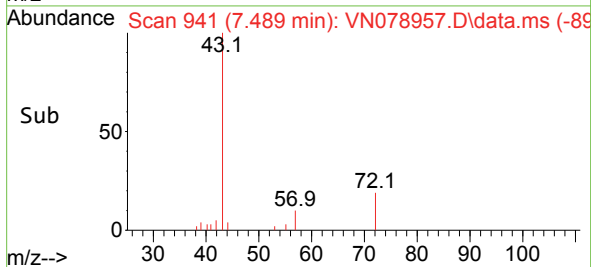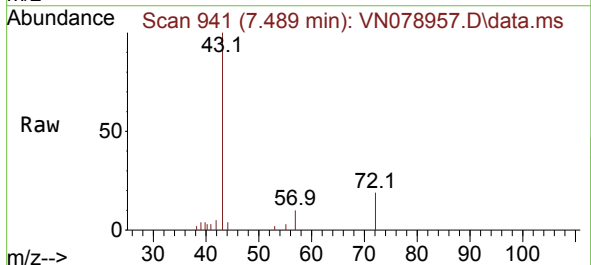



#29

Tetrahydrofuran

Concen: 0.329 ug/l

RT: 7.841 min Scan# 1002

Delta R.T. -0.006 min

Lab File: VN078957.D

Acq: 18 Aug 2023 21:13

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 42 Resp: 454

Ion Ratio Lower Upper

42 100

72 43.2 49.8 74.6#

71 17.6 47.4 71.2#

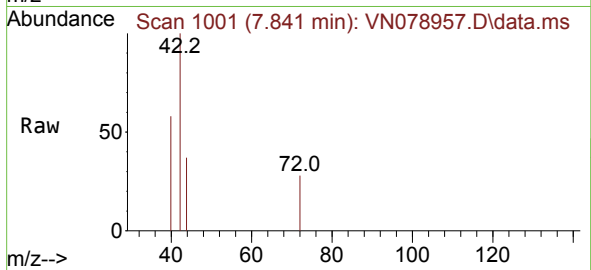

#31

Cyclohexane

Concen: Below Cal

RT: 8.230 min Scan# 1067

Delta R.T. -0.035 min

Lab File: VN078957.D

Acq: 18 Aug 2023 21:13




Tgt Ion: 56 Resp: 5693


Ion Ratio Lower Upper

56 100

69 160.9 26.8 40.2#

84 142.8 81.8 122.6#

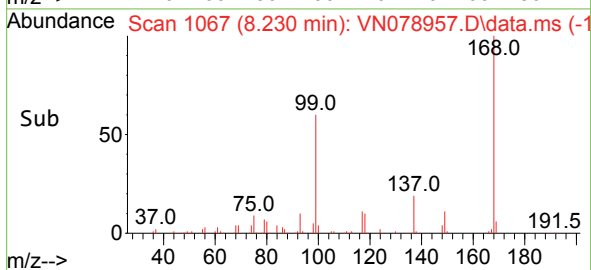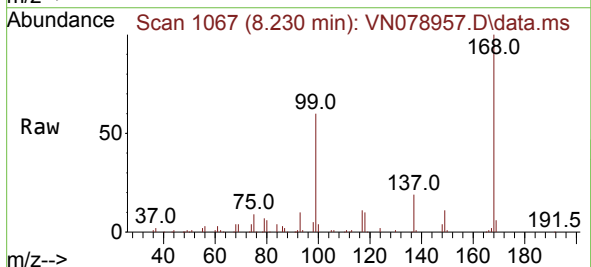



#33

1,2-Dichloroethane-d4

Concen: 51.501 ug/l

RT: 8.589 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VN078957.D

Acq: 18 Aug 2023 21:13

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 65 Resp: 162394

Ion Ratio Lower Upper

65 100

67 51.8 0.0 106.6

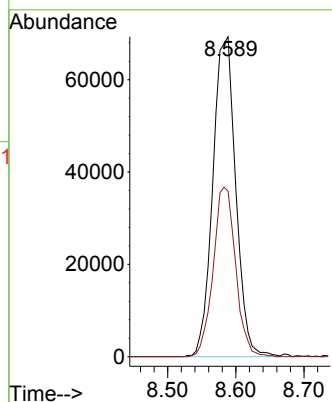

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. -0.006 min

Lab File: VN078957.D

Acq: 18 Aug 2023 21:13




Tgt Ion: 114 Resp: 398097


Ion Ratio Lower Upper

114 100

63 21.7 0.0 36.4


88 15.3 0.0 30.6

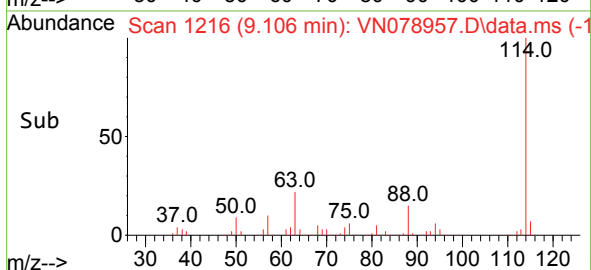






#35
Dibromofluoromethane
Concen: 49.354 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.000 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:113 Resp: 132258
Ion Ratio Lower Upper
113 100
111 104.4 82.6 123.8
192 18.3 12.7 19.1



#36
1,1-Dichloropropene
Concen: 4.339 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13


Tgt Ion: 75 Resp: 17492
Ion Ratio Lower Upper
75 100
110 4.1 19.1 57.3#
77 0.0 25.0 37.4#

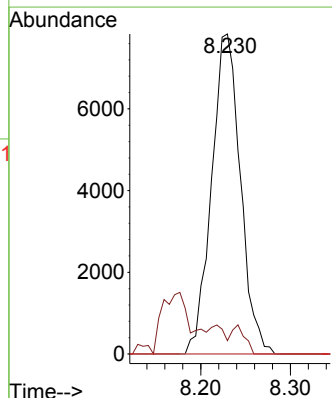






#37
Ethyl Acetate
Concen: 1.077 ug/l
RT: 7.571 min Scan# 91
Delta R.T. -0.000 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 4857
Ion Ratio Lower Upper
43 100
61 2.3 13.2 19.8#
70 1.3 11.3 16.9#

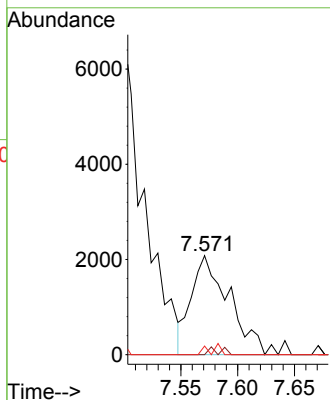

#38
Carbon Tetrachloride
Concen: 5.481 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.141 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13

Tgt Ion: 117 Resp: 22137
Ion Ratio Lower Upper
117 100
119 3.2 77.3 115.9#
121 0.0 23.3 34.9#

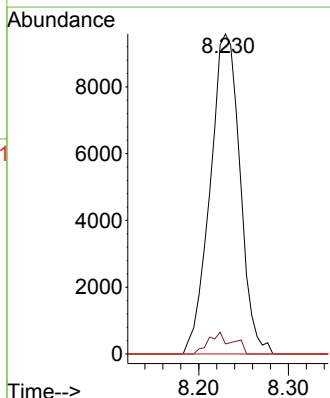



#42

1,2-Dichloroethane

Concen: 0.261 ug/l

RT: 8.688 min Scan# 1145

Delta R.T. 0.011 min

Lab File: VN078957.D

Acq: 18 Aug 2023 21:13

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 62 Resp: 1163

Ion Ratio Lower Upper

62 100

98 0.0 0.0 19.8

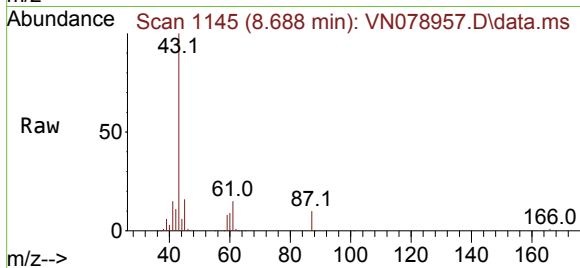

#43

Isopropyl Acetate

Concen: 28.179 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. 0.000 min

Lab File: VN078957.D

Acq: 18 Aug 2023 21:13




Tgt Ion: 43 Resp: 224634


Ion Ratio Lower Upper

43 100

61 12.9 24.7 37.1#

87 7.6 14.6 21.8#


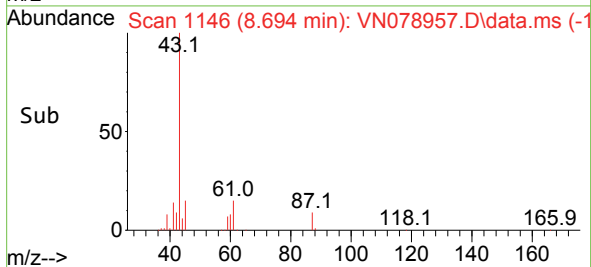

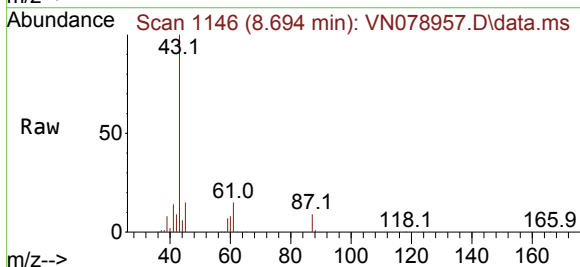




#45
1,2-Dichloropropane
Concen: 0.572 ug/l
RT: 9.747 min Scan# 11
Delta R.T. 0.123 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 63 Resp: 1813
Ion Ratio Lower Upper
63 100
65 0.0 23.9 35.9#

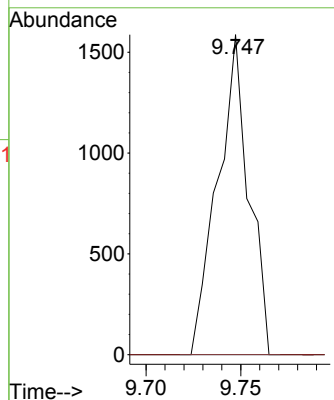

#48
Methyl methacrylate
Concen: 1.538 ug/l
RT: 9.659 min Scan# 1310
Delta R.T. -0.029 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13

Tgt Ion: 41 Resp: 5557
Ion Ratio Lower Upper
41 100
69 0.0 90.4 135.6#
39 58.6 54.6 81.8

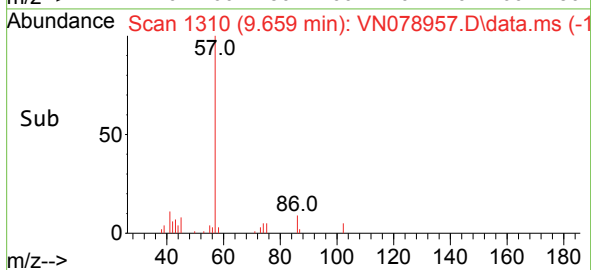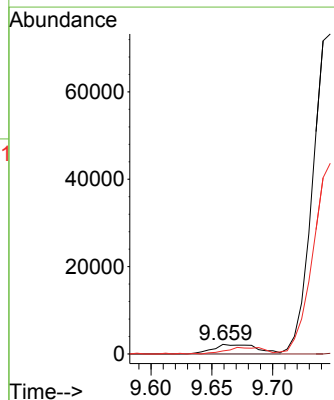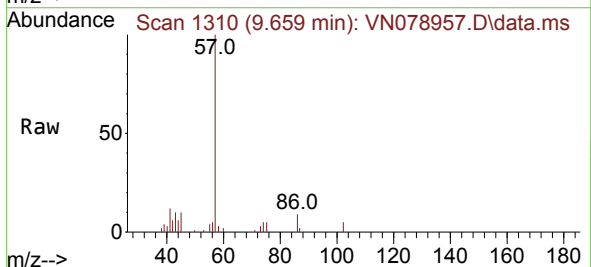



#49

1,4-Dioxane

Concen: 1.641 ug/l

RT: 9.747 min Scan# 11

Delta R.T. 0.047 min


Lab File: VN078957.D

Acq: 18 Aug 2023 21:13

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 88 Resp: 101

Ion Ratio Lower Upper

88 100

43 1440508.9 17.0 25.6#

58 7263.4 47.0 70.4#



#50

Toluene-d8

Concen: 49.074 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. -0.000 min

Lab File: VN078957.D




Acq: 18 Aug 2023 21:13


Tgt Ion: 98 Resp: 488294

Ion Ratio Lower Upper

98 100

100 65.3 52.0 78.0


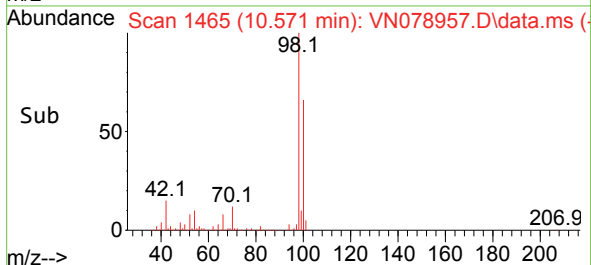
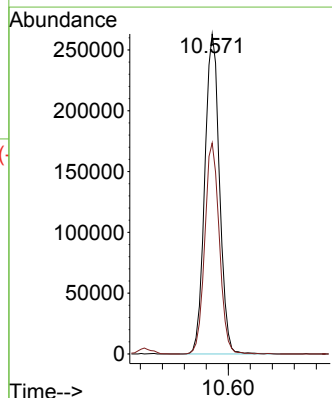
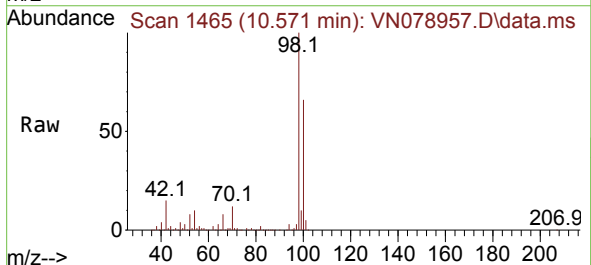


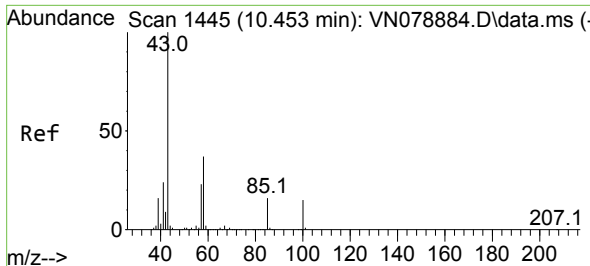

#51
4-Methyl-2-Pentanone
Concen: 14.077 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. -0.006 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 66555
Ion Ratio Lower Upper
43 100
58 33.5 36.6 54.8#

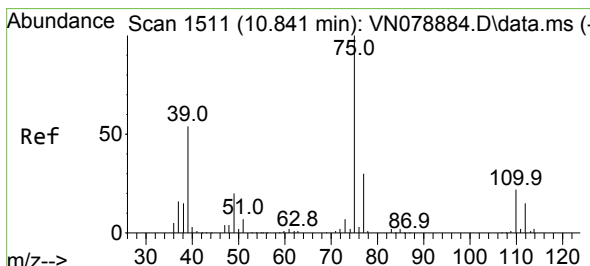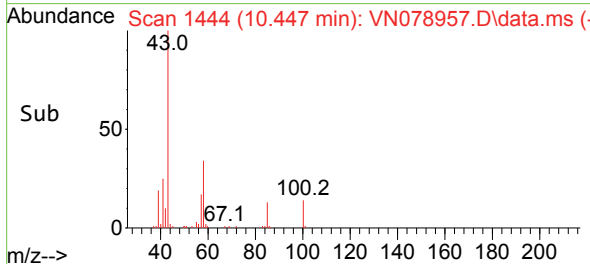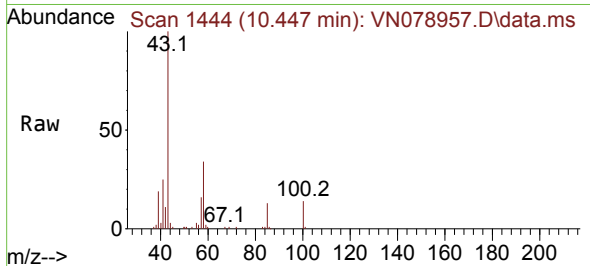

#53
t-1,3-Dichloropropene
Concen: 0.201 ug/l
RT: 10.730 min Scan# 1492
Delta R.T. -0.111 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13


Tgt Ion: 75 Resp: 928
Ion Ratio Lower Upper
75 100
77 53.0 25.4 38.0#

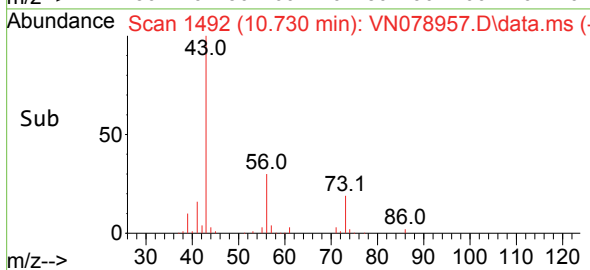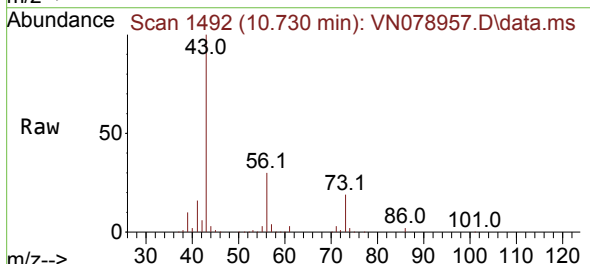



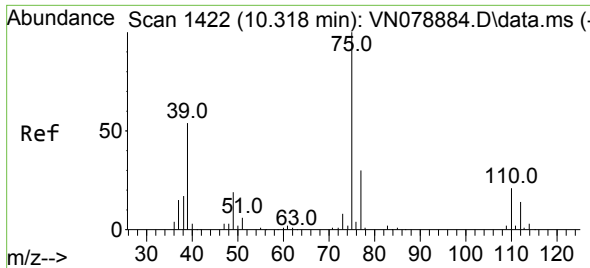


#54
 cis-1,3-Dichloropropene
 Concen: 10.101 ug/l
 RT: 10.365 min Scan# 1422
 Delta R.T. 0.047 min
 Lab File: VN078957.D
 Acq: 18 Aug 2023 21:13

Instrument :
 MSVOA_N
 ClientSampleId :



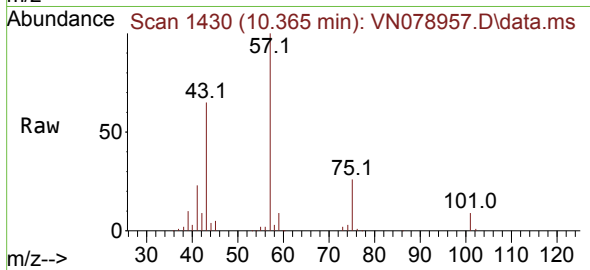



Tgt Ion: 75 Resp: 50690
 Ion Ratio Lower Upper
 75 100
 77 0.9 26.1 39.1#
 39 39.5 31.6 47.4

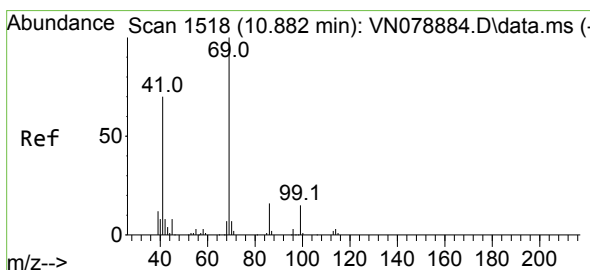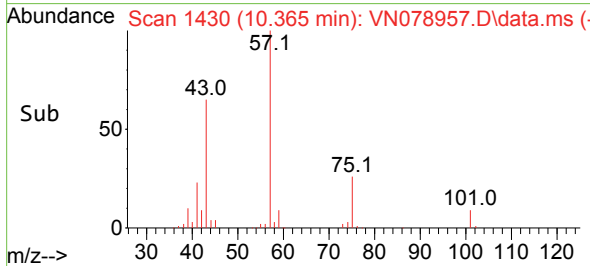

#56
 Ethyl methacrylate
 Concen: 0.541 ug/l
 RT: 10.982 min Scan# 1535
 Delta R.T. 0.105 min
 Lab File: VN078957.D
 Acq: 18 Aug 2023 21:13

Tgt Ion: 69 Resp: 2458
 Ion Ratio Lower Upper
 69 100
 41 3781.0 39.6 59.4#
 39 1775.1 28.6 43.0#

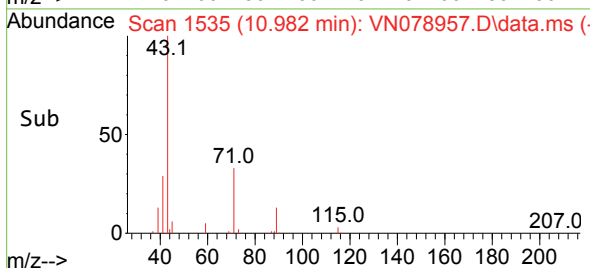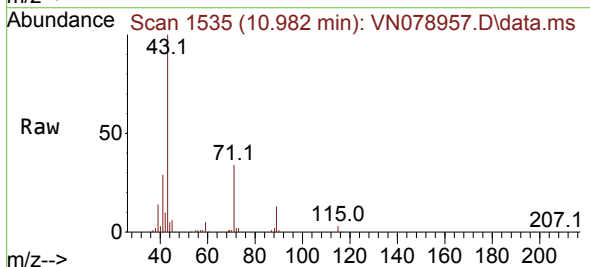

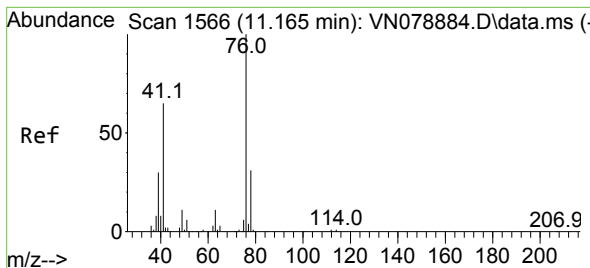

#57

1,3-Dichloropropane

Concen: 1.268 ug/l

RT: 11.206 min Scan# 11

Delta R.T. 0.041 min

Lab File: VN078957.D

Acq: 18 Aug 2023 21:13

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 76 Resp: 6650

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#

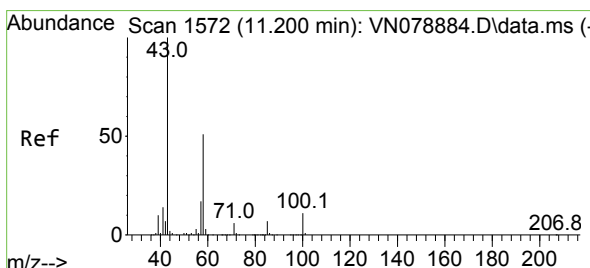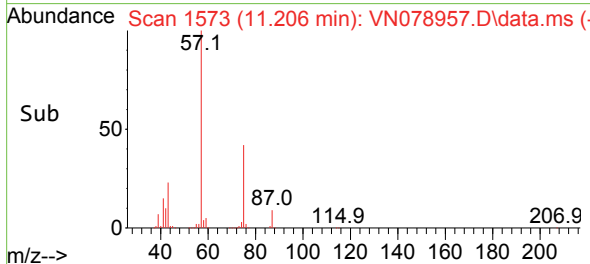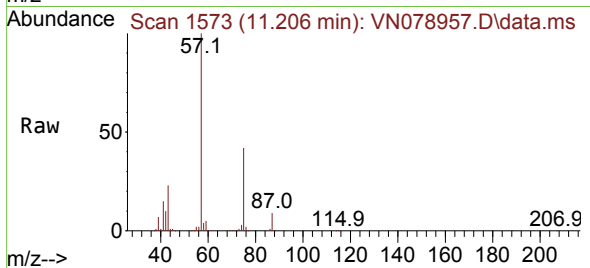

#59

2-Hexanone

Concen: 37.827 ug/l

RT: 11.177 min Scan# 1568

Delta R.T. -0.023 min

Lab File: VN078957.D




Acq: 18 Aug 2023 21:13


Tgt Ion: 43 Resp: 129539

Ion Ratio Lower Upper

43 100

58 0.0 31.7 95.1#


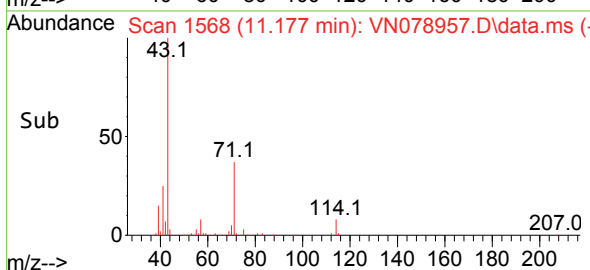

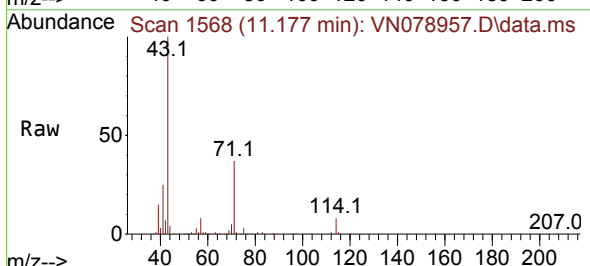


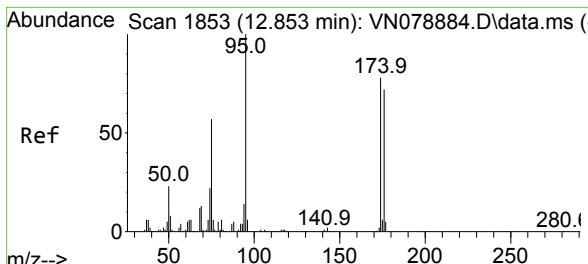

#62
 4-Bromofluorobenzene
 Concen: 44.854 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. -0.000 min
 Lab File: VN078957.D
 Acq: 18 Aug 2023 21:13




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:	95	Resp:	145882
Ion	Ratio	Lower	Upper
95	100		
174	82.3	0.0	143.8
176	78.8	0.0	135.8

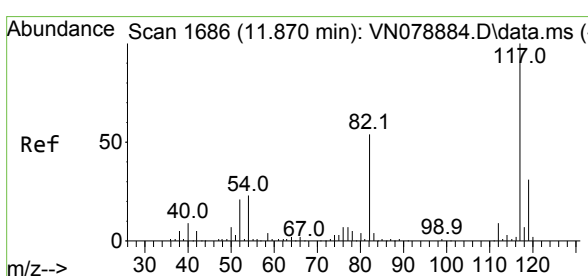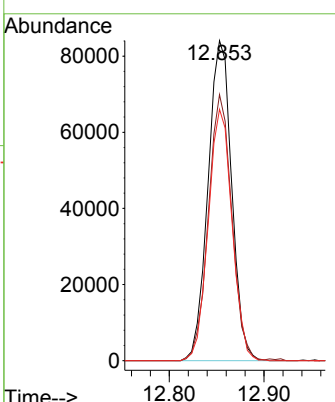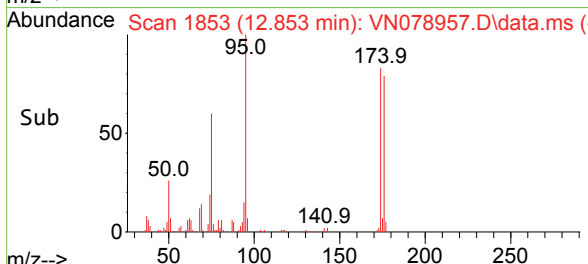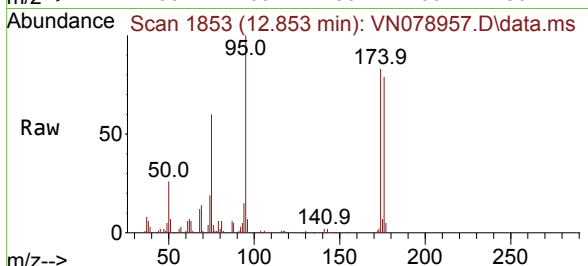

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 11.871 min Scan# 1686
 Delta R.T. -0.000 min
 Lab File: VN078957.D
 Acq: 18 Aug 2023 21:13

Tgt Ion:	117	Resp:	377236
Ion	Ratio	Lower	Upper
117	100		
82	55.8	44.0	66.0
119	32.6	25.6	38.4

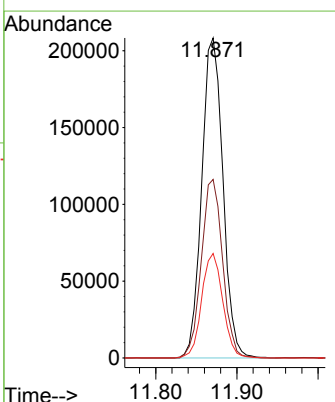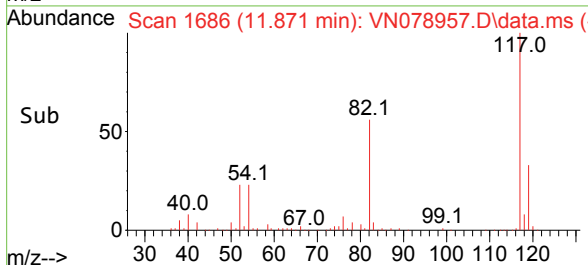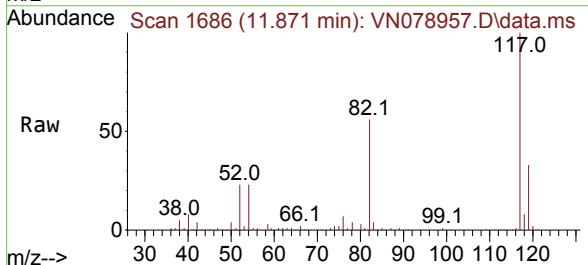



#71

Bromoform

Concen: 0.619 ug/l

RT: 12.853 min Scan# 1807

Delta R.T. 0.271 min


Lab File: VN078957.D

Acq: 18 Aug 2023 21:13




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	173	Resp:	1365
Ion Ratio	Lower	Upper	
173	100		
175	540.5	24.3	73.0#
254	0.0	0.0	0.0

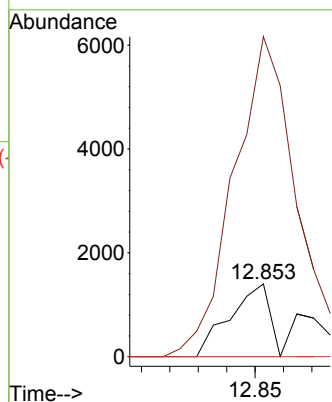

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l




RT: 13.794 min Scan# 2013


Delta R.T. 0.000 min

Lab File: VN078957.D

Acq: 18 Aug 2023 21:13


Tgt Ion:	152	Resp:	120436
Ion Ratio	Lower	Upper	
152	100		
115	58.8	32.3	96.8
150	153.3	0.0	355.8

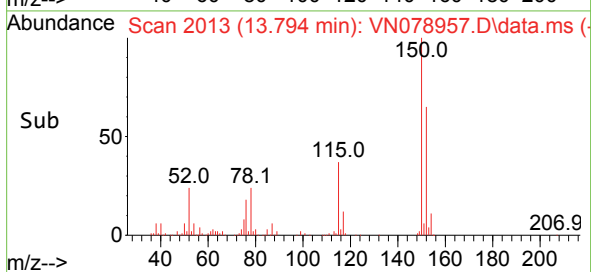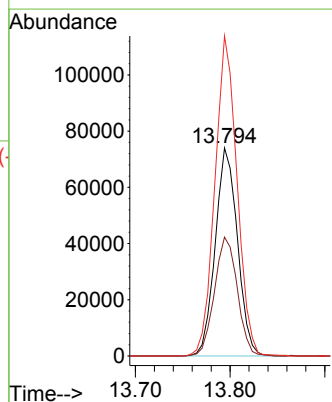






#74
N-amy1 acetate
Concen: 0.450 ug/l
RT: 12.488 min Scan# 1791
Delta R.T. -0.012 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13

Instrument :
MSVOA_N
ClientSampleId :



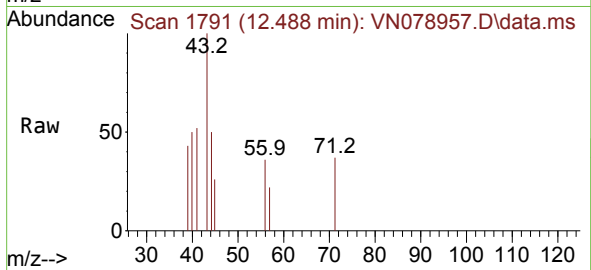



Tgt Ion:	43	Resp:	2279
Ion	Ratio	Lower	Upper
43	100		
70	0.0	43.4	65.2#
55	0.0	21.4	32.0#
61	0.0	22.8	34.2#

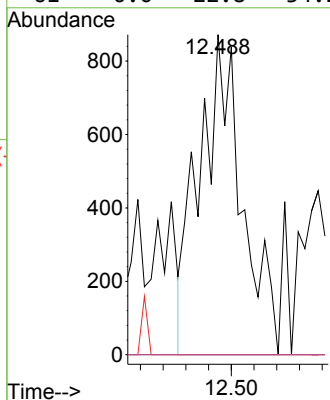

#76
1,2,3-Trichloropropane
Concen: 28.543 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN078957.D
Acq: 18 Aug 2023 21:13

Tgt Ion:	75	Resp:	82830
Ion	Ratio	Lower	Upper
75	100		
77	1.2	84.5	253.5#


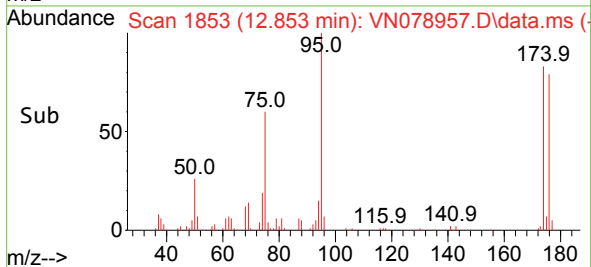
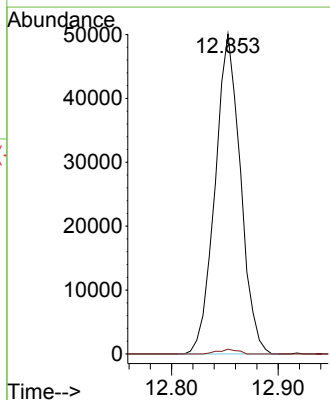
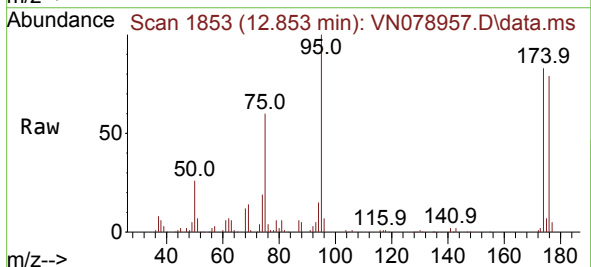




#81
 trans-1,4-Dichloro-2-butene
 Concen: 72.915 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. 0.112 min
 Lab File: VN078957.D
 Acq: 18 Aug 2023 21:13

Instrument :
 MSVOA_N
 ClientSampleId :

Tgt Ion: 75 Resp: 82830
 Ion Ratio Lower Upper
 75 100
 53 0.3 67.4 101.2#
 89 0.0 38.8 58.2#

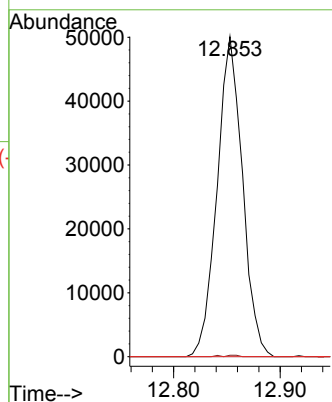

#95
 Naphthalene
 Concen: 2.584 ug/l
 RT: 15.635 min Scan# 2326
 Delta R.T. -0.012 min
 Lab File: VN078957.D
 Acq: 18 Aug 2023 21:13

Tgt Ion:128 Resp: 54
 Ion Ratio Lower Upper
 128 100
 127 0.0 10.0 15.0#
 129 0.0 8.7 13.1#

