
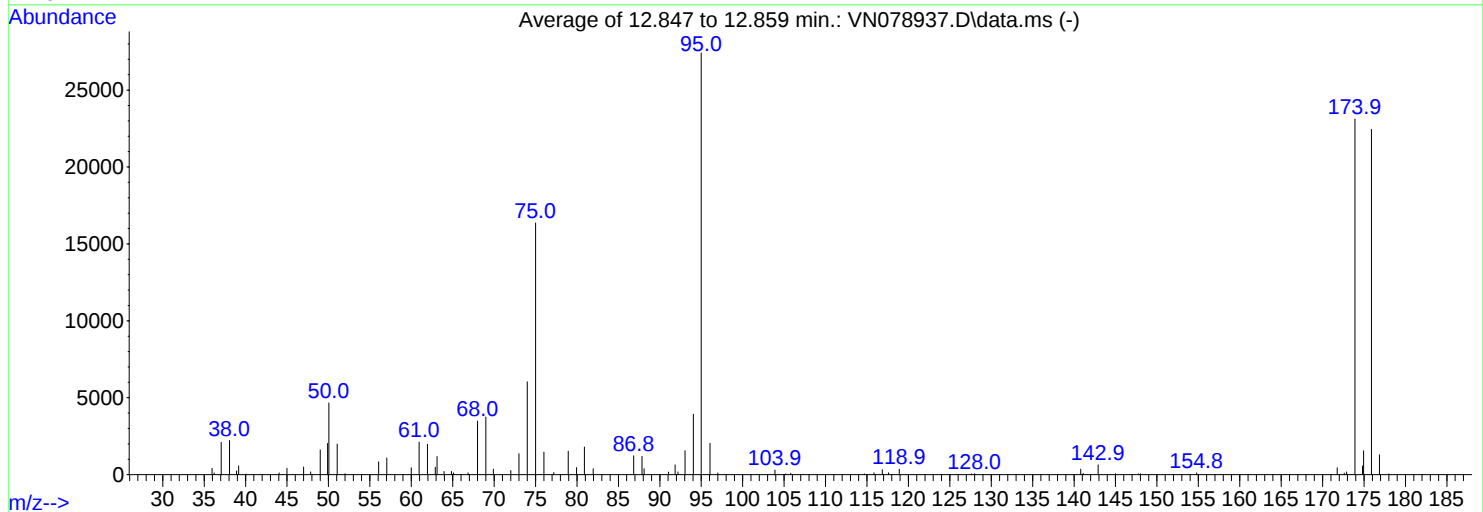


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081823\
 Data File : VN078937.D
 Acq On : 18 Aug 2023 12:39
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081523W.M
 Title : SW846 8260
 Last Update : Wed Aug 16 02:42:02 2023

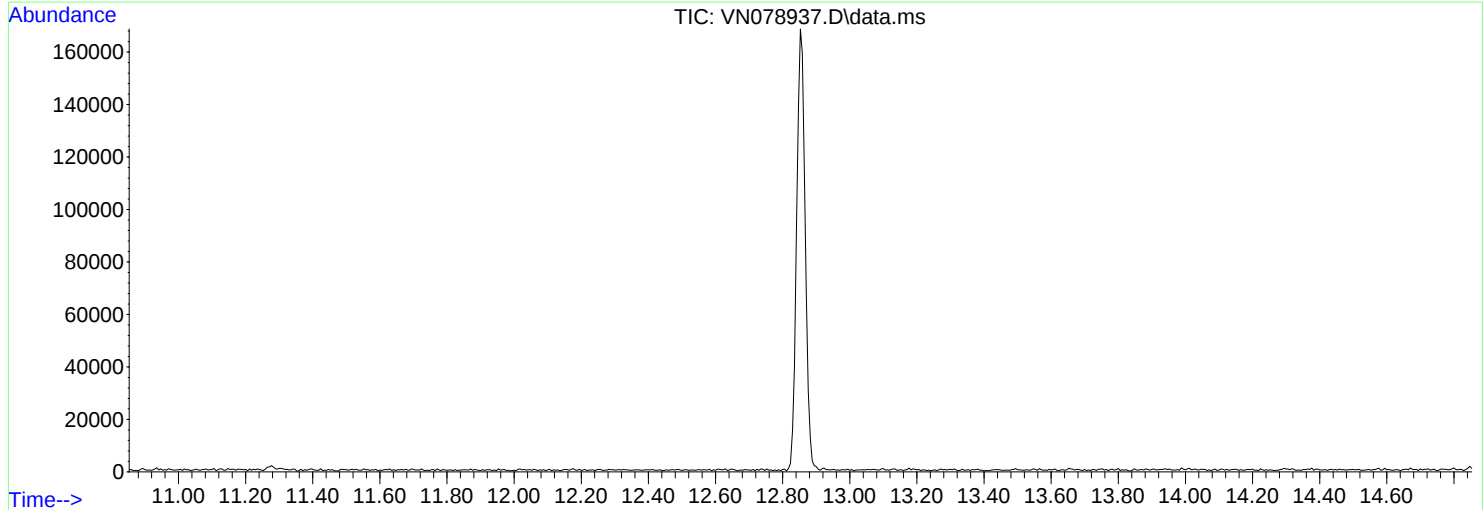

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	4663	PASS
75	95	30	60	59.7	16361	PASS
95	95	100	100	100.0	27421	PASS
96	95	5	9	7.4	2041	PASS
173	174	0.00	2	0.8	178	PASS
174	95	50	100	84.3	23123	PASS
175	174	5	9	6.7	1550	PASS
176	174	95	101	97.1	22448	PASS
177	176	5	9	5.8	1291	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	408	49.00	1614	63.10	1176	75.00	1636
36.20	116	49.90	2026	63.95	204	76.00	146
37.05	2101	50.05	4663	64.85	213	77.20	13
38.05	2212	51.05	1991	65.10	117	78.95	151
38.90	240	52.00	58	66.85	112	79.95	453
39.15	571	56.05	828	68.00	3489	80.90	1805
40.05	37	57.05	1081	69.00	3750	81.95	382
44.05	116	60.00	452	69.90	355	86.85	1224
45.00	417	60.95	2115	72.00	266	87.85	1190
47.00	498	61.95	1972	73.00	1364	88.10	389
47.85	173	62.90	479	74.00	6037	91.05	162

Average of 12.847 to 12.859 min.: VN078937.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.85	630	115.85	123	148.00	62		
92.20	173	116.85	325	154.80	119		
93.05	1559	117.60	120	171.75	446		
94.05	3932	118.90	352	172.60	103		
95.00	27421	127.60	57	172.90	178		
96.05	2041	128.00	62	173.90	23123		
97.00	116	140.80	356	174.80	559		
103.90	305	141.10	83	174.95	1550		
105.20	53	142.90	633	175.90	22448		
105.80	95	145.00	62	176.85	1291		
114.70	50	147.80	57	178.00	54		

Instrument :

MSVOA_N

ClientSampleId :

BFB