


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081825\
Data File : VN087594.D
Acq On : 18 Aug 2025 08:56
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080525W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Aug 06 02:01:21 2025

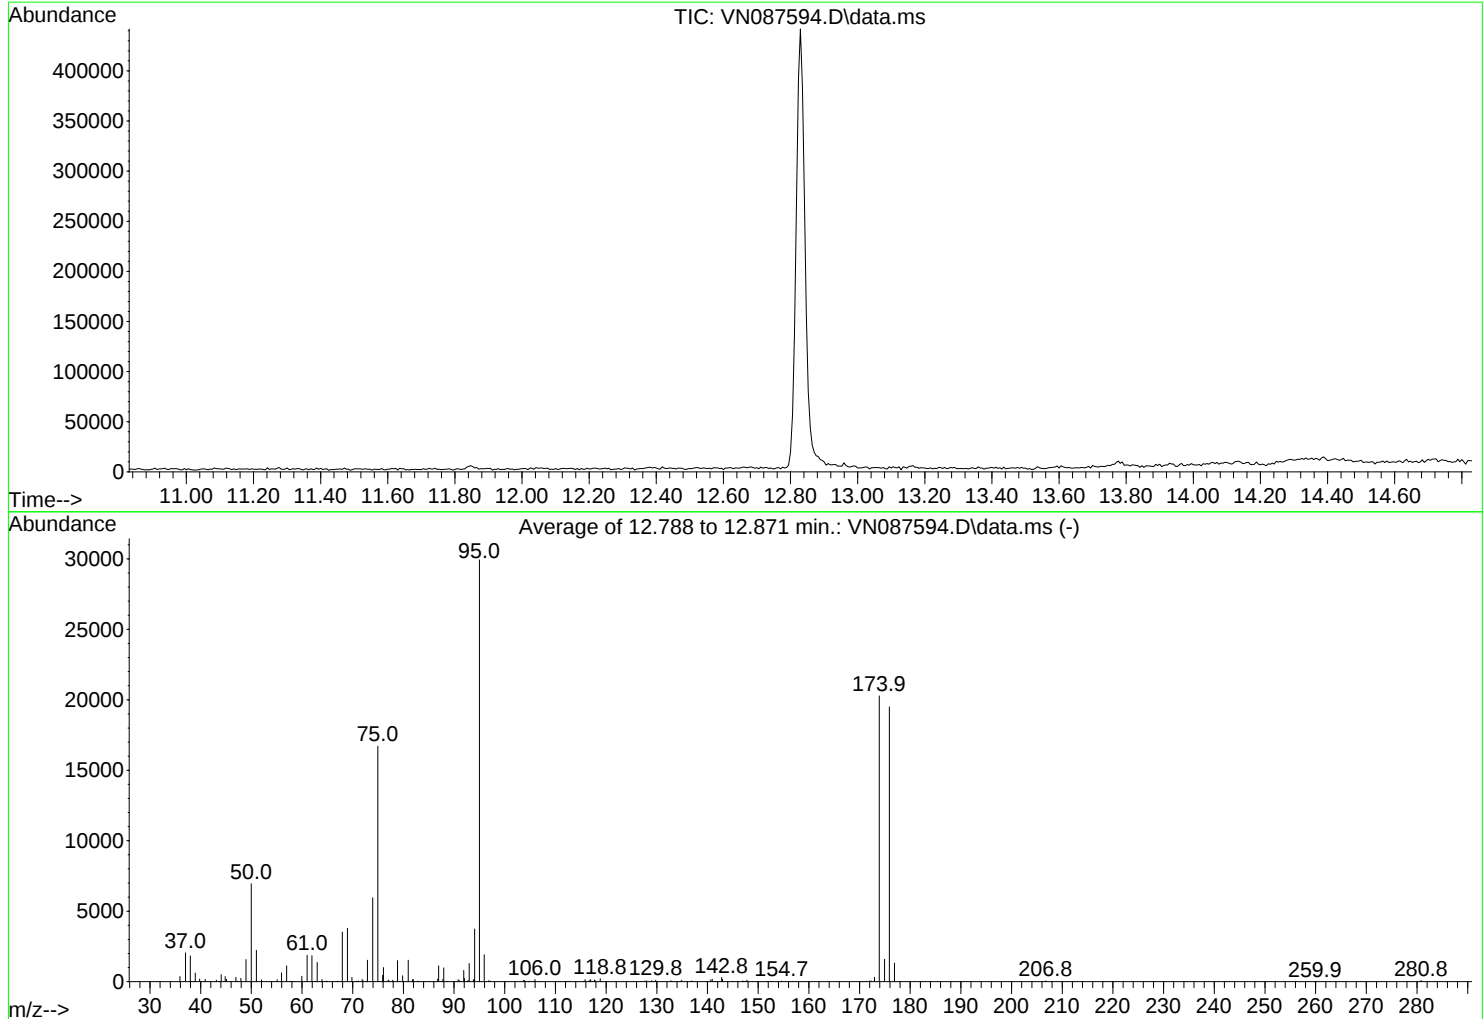

AutoFind: Averaged scan 1842 to 1856; Bkg corrected with scan 1841

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.2	6944	PASS
75	95	30	60	55.8	16710	PASS
95	95	100	100	100.0	29931	PASS
96	95	5	9	6.4	1905	PASS
173	174	0.00	2	1.5	304	PASS
174	95	50	100	67.8	20279	PASS
175	174	5	9	7.8	1591	PASS
176	174	95	101	96.1	19497	PASS
177	176	5	9	6.8	1320	PASS