

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN081919\
 Data File : VN057434.D
 Acq On : 20 Aug 2019 6:04
 Operator : JC/SP
 Sample : K4386-39
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 T6-A4-(2)

Quant Time: Aug 20 08:54:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 15 11:33:14 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.66	168	1016176	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.58	114	1417972	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1206469	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	332991	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.02	65	482469	43.67	ug/l	0.00
Spiked Amount	50.000		Recovery	=	87.34%	
35) Dibromofluoromethane	7.58	113	435194	46.82	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.64%	
50) Toluene-d8	10.08	98	1646215	48.42	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.84%	
62) 4-Bromofluorobenzene	12.40	95	445740	37.10	ug/l	0.00
Spiked Amount	50.000		Recovery	=	74.20%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.72	59	4190	2.668	ug/l #	73
16) Acetone	3.81	43	12214	3.187	ug/l	95
20) Methylene Chloride	4.54	84	8495	0.792	ug/l #	78
25) 2-Butanone	6.82	43	1271	0.229	ug/l #	48
31) Cyclohexane	7.65	56	14036	0.932	ug/l #	1
36) 1,1-Dichloropropene	7.65	75	59714	4.770	ug/l #	48
38) Carbon Tetrachloride	7.66	117	85244	6.553	ug/l #	16
43) Isopropyl Acetate	8.16	43	159817	7.565	ug/l #	86
44) Trichloroethene	8.83	130	3524	0.327	ug/l	86
45) 1,2-Dichloropropane	9.26	63	2607	0.264	ug/l #	44
48) Methyl methacrylate	9.17	41	6615	0.783	ug/l #	11
51) 4-Methyl-2-Pentanone	9.98	43	7538	0.713	ug/l	99
54) cis-1,3-Dichloropropene	9.90	75	61413	3.946	ug/l #	60
57) 1,3-Dichloropropane	10.76	76	9412	0.601	ug/l #	43
59) 2-Hexanone	10.76	43	117541	15.455	ug/l #	49
71) Bromoform	12.40	173	2813	0.378	ug/l #	1
73) Isopropylbenzene	12.25	105	29	Below Cal	#	49
74) N-amyl acetate	12.03	43	4129	0.427	ug/l #	42
75) 1,1,2,2-Tetrachloroethane	12.40	83	63	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.40	75	204823	30.512	ug/l #	100
77) Bromobenzene	12.40	156	102	Below Cal	#	1
79) 2-Chlorotoluene	12.59	91	129	Below Cal	#	39
80) 1,3,5-Trimethylbenzene	12.74	105	1187	Below Cal	#	87
81) trans-1,4-Dichloro-2-buten	12.40	75	204823	75.004	ug/l #	15
85) sec-Butylbenzene	13.04	105	206	Below Cal	#	55
95) Naphthalene	15.14	128	566	Below Cal	#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN081919\
Data File : VN057434.D
Acq On : 20 Aug 2019 6:04
Operator : JC/SP
Sample : K4386-39
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
T6-A4-(2)

Quant Time: Aug 20 08:54:03 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 15 11:33:14 2019
Response via : Initial Calibration

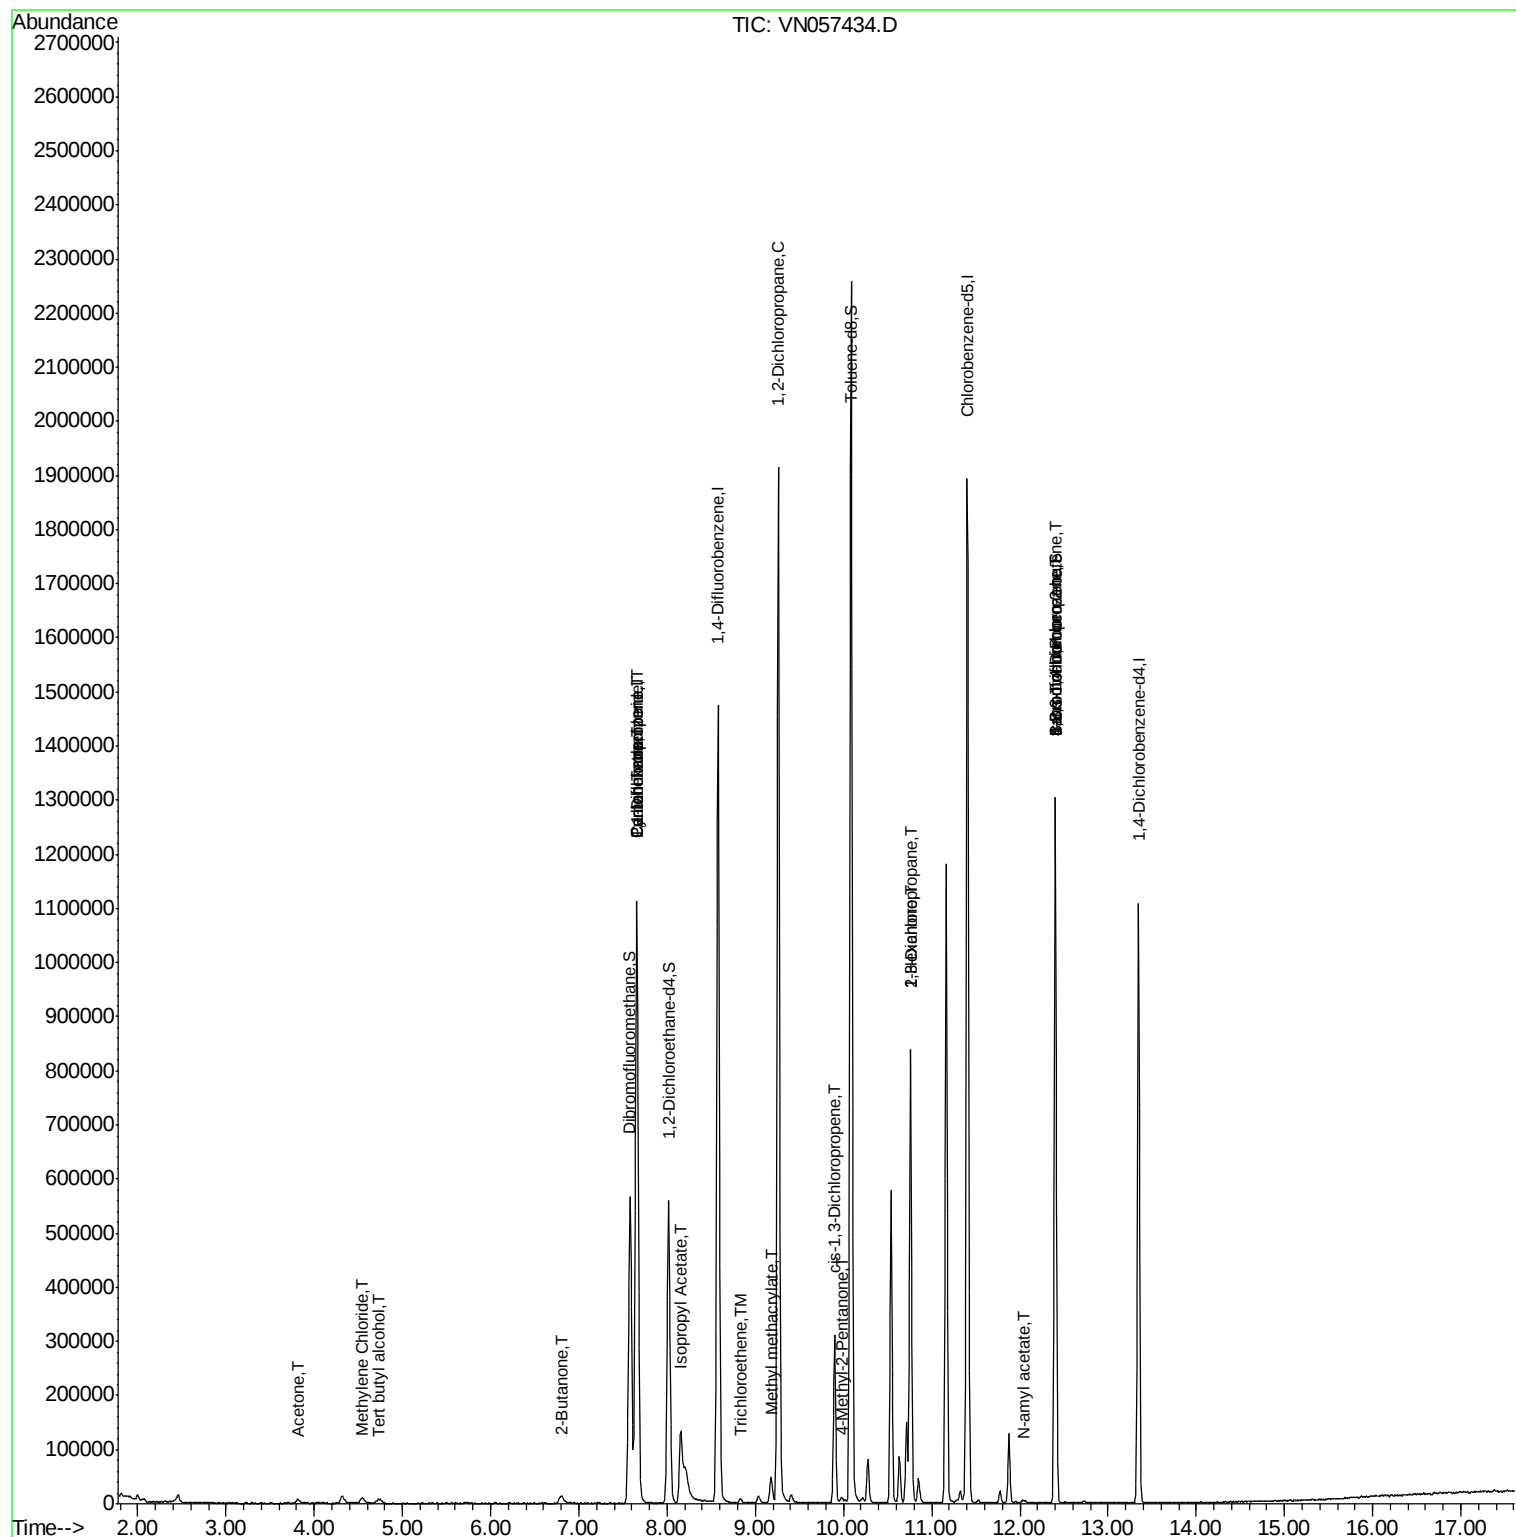



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.66 min Scan# 1830

Delta R.T. 0.00 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Instrument :

MSVOA_N

ClientSampleId :


T6-A4-(2)

Tgt Ion:168 Resp: 1016176

Ion Ratio Lower Upper

168 100

99 47.3 39.4 59.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

7.66

400000



300000

200000

100000

0

Time-->

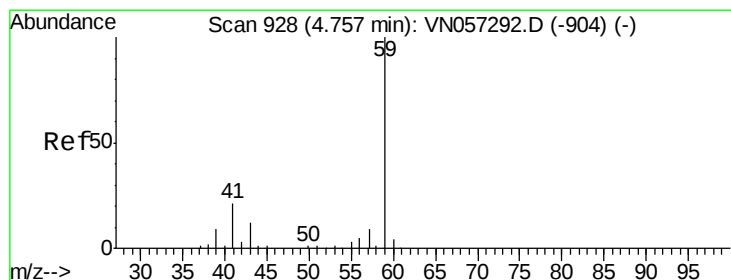

#11

Tert butyl alcohol

Concen: 2.668 ug/l

RT: 4.72 min Scan# 918

Delta R.T. -0.03 min

Lab File: VN057434.D


Acq: 20 Aug 2019 6:04

Tgt Ion: 59 Resp: 4190

Ion Ratio Lower Upper

59 100

57 0.0 8.2 12.2#

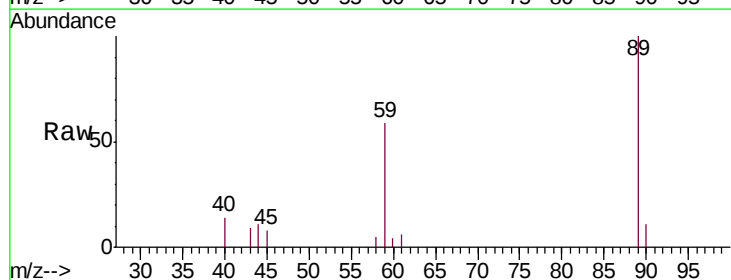

Abundance Ion 59.00 (58.70 to 59.70): VN

Ion 57.00 (56.70 to 57.70): VN

4.72

2500

2000


1500


1000

500

0

Time-->





#16

Acetone

Concen: 3.187 ug/l

RT: 3.81 min Scan# 634

Delta R.T. 0.01 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Instrument :

MSVOA_N

ClientSampleId :





T6-A4-(2)

Tgt Ion: 43 Resp: 12214

Ion Ratio Lower Upper

43 100

58 30.9 27.0 40.6

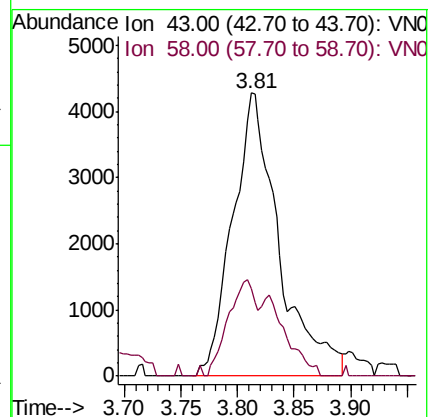

#20

Methylene Chloride

Concen: 0.792 ug/l

RT: 4.54 min Scan# 860

Delta R.T. -0.00 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Tgt Ion: 84 Resp: 8495




Ion Ratio Lower Upper


84 100

49 79.8 92.0 138.0#

51 40.5 27.1 40.7

86 58.0 52.2 78.2

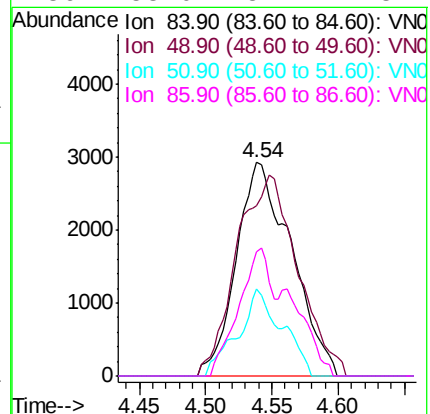



#25

2-Butanone

Concen: 0.229 ug/l

RT: 6.82 min Scan# 1569

Delta R.T. -0.00 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Instrument :

MSVOA_N

ClientSampled :


T6-A4-(2)

Tgt Ion: 43 Resp: 1271

Ion Ratio Lower Upper

43 100

72 0.0 21.5 32.3#

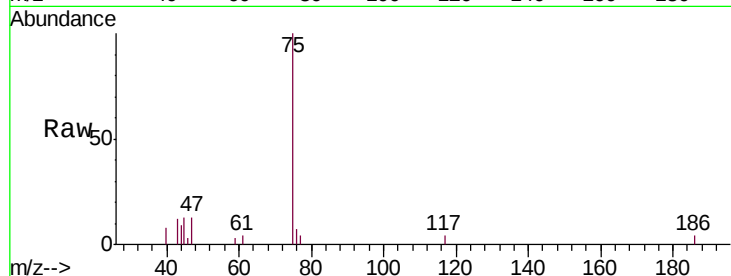

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82

6.82



6.82

6.82

6.82

6.82

6.82



#31

Cyclohexane

Concen: 0.932 ug/l

RT: 7.65 min Scan# 1828

Delta R.T. 0.00 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04


Tgt Ion: 56 Resp: 14036

Ion Ratio Lower Upper

56 100

69 188.6 27.3 40.9#

84 153.6 71.0 106.6#



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65

7.65


7.65

7.65


7.65

7.65

7.65



Time-->



#33

1,2-Dichloroethane-d4

Concen: 43.674 ug/l

RT: 8.02 min Scan# 1942

Delta R.T. 0.00 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Instrument :

MSVOA_N

ClientSampleId :





T6-A4-(2)

Tgt Ion: 65 Resp: 482469

Ion Ratio Lower Upper

65 100

67 51.9 0.0 107.4

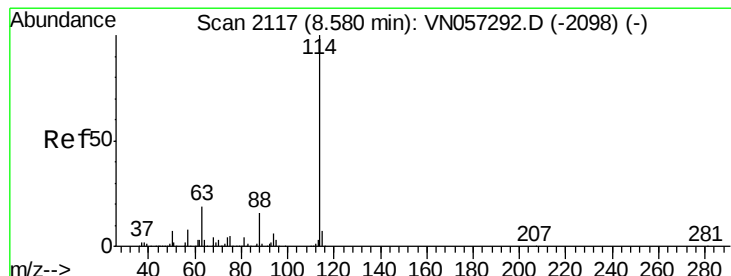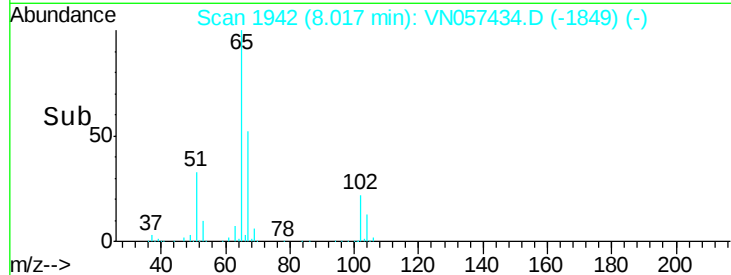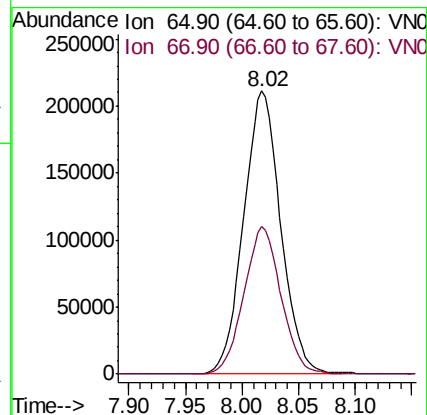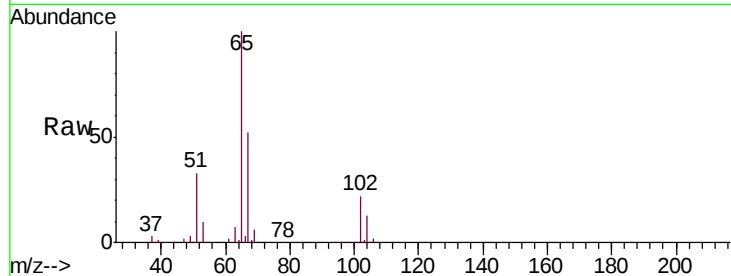

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.58 min Scan# 2116

Delta R.T. -0.00 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04




Tgt Ion: 114 Resp: 1417972


Ion Ratio Lower Upper

114 100

63 17.9 0.0 38.8

88 15.5 0.0 31.4



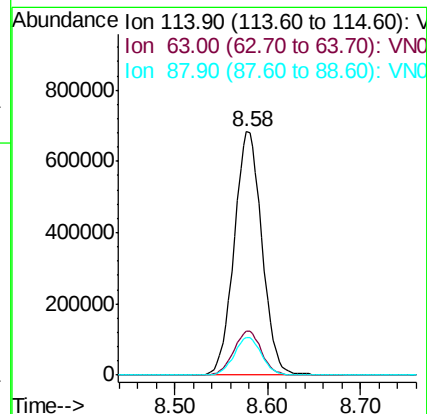
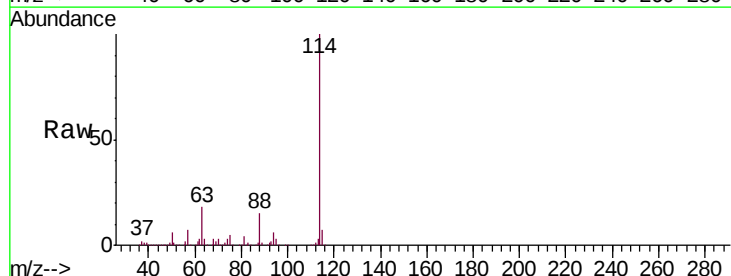




#35
 Dibromofluoromethane
 Concen: 46.820 ug/l
 RT: 7.58 min Scan# 1807
 Delta R.T. 0.00 min
 Lab File: VN057434.D
 Acq: 20 Aug 2019 6:04




Instrument :
 MSVOA_N
 ClientSampleId :
 T6-A4-(2)


Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.1	82.1	123.1
192	23.8	19.3	28.9

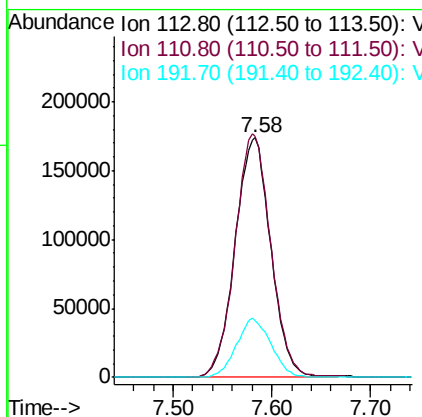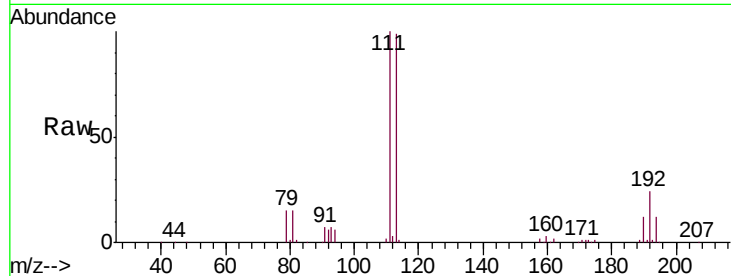

#36
 1,1-Dichloropropene
 Concen: 4.770 ug/l
 RT: 7.65 min Scan# 1829
 Delta R.T. -0.13 min
 Lab File: VN057434.D
 Acq: 20 Aug 2019 6:04

Tgt Ion	Ratio	Lower	Upper
75	100		
110	9.7	19.5	58.5#
77	0.0	25.0	37.6#

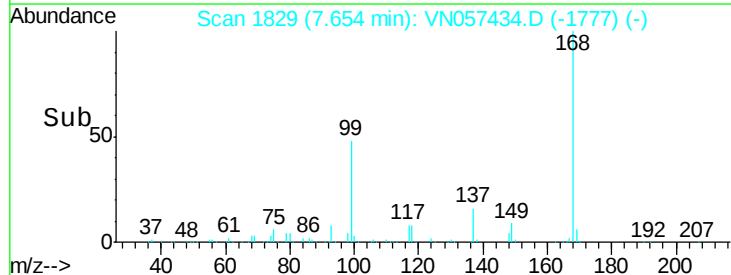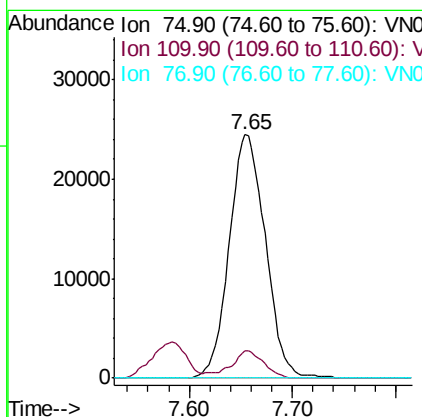







#38
Carbon Tetrachloride
Concen: 6.553 ug/l
RT: 7.66 min Scan# 1830
Delta R.T. -0.11 min
Lab File: VN057434.D
Acq: 20 Aug 2019 6:04

Instrument :
MSVOA_N
ClientSampled :
T6-A4-(2)

Tgt Ion: 117 Resp: 85244
Ion Ratio Lower Upper
117 100
119 5.5 76.8 115.2#
121 0.0 25.0 37.4#




Abundance Ion 116.80 (116.50 to 117.50): V
Ion 118.80 (118.50 to 119.50): V
Ion 120.80 (120.50 to 121.50): V

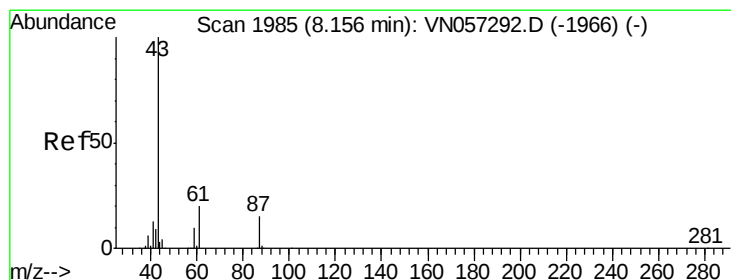
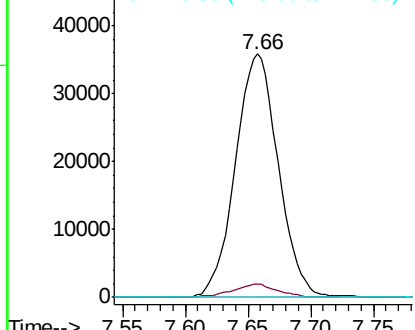



#43
Isopropyl Acetate
Concen: 7.565 ug/l
RT: 8.16 min Scan# 1985
Delta R.T. 0.00 min
Lab File: VN057434.D
Acq: 20 Aug 2019 6:04

Tgt Ion: 43 Resp: 159817
Ion Ratio Lower Upper
43 100
61 17.1 21.6 32.4#
87 12.1 11.4 17.0

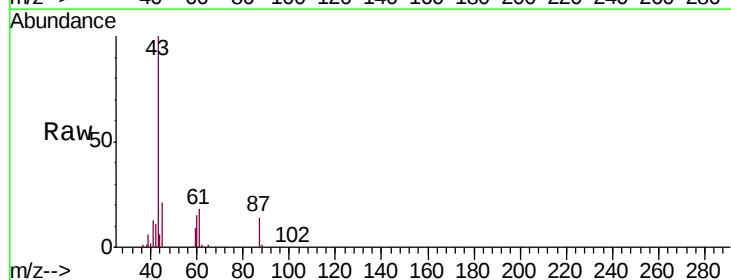

Abundance Ion 43.00 (42.70 to 43.70): V
Ion 61.00 (60.70 to 61.70): V
Ion 87.00 (86.70 to 87.70): V

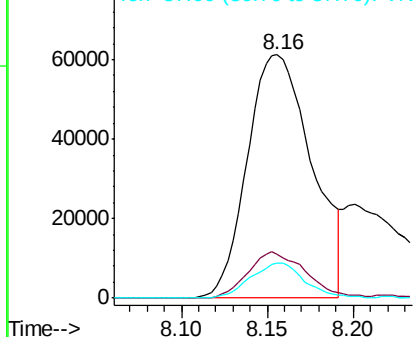

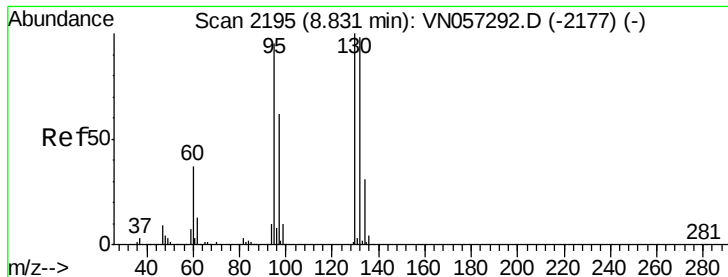

#44

Trichloroethene

Concen: 0.327 ug/l

RT: 8.83 min Scan# 2194

Delta R.T. -0.00 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Instrument :

MSVOA_N

ClientSampled :


T6-A4-(2)

Tgt Ion:130 Resp: 3524

Ion Ratio Lower Upper

130 100

95 80.8 0.0 189.2

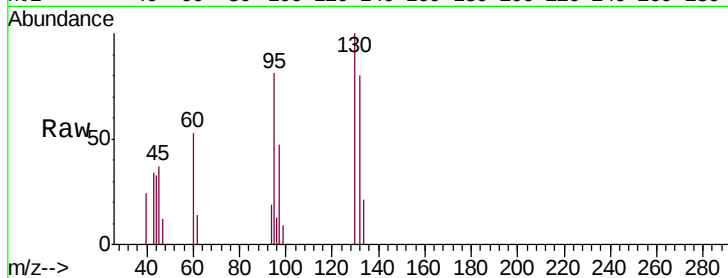

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VN0

8.83

1500



1000

500

0

8.80 8.85

Time-->

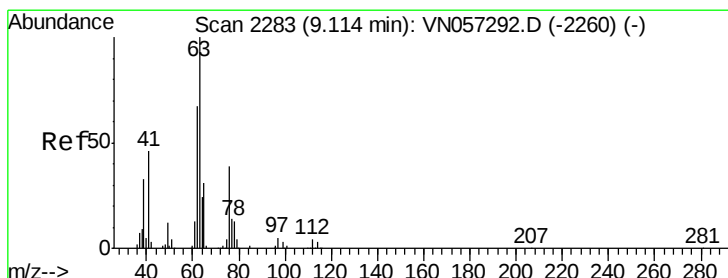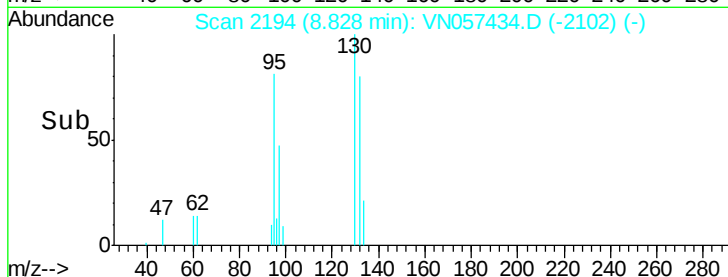

#45

1,2-Dichloropropane

Concen: 0.264 ug/l

RT: 9.26 min Scan# 2328

Delta R.T. 0.14 min

Lab File: VN057434.D


Acq: 20 Aug 2019 6:04

Tgt Ion: 63 Resp: 2607

Ion Ratio Lower Upper

63 100

65 0.0 24.8 37.2#

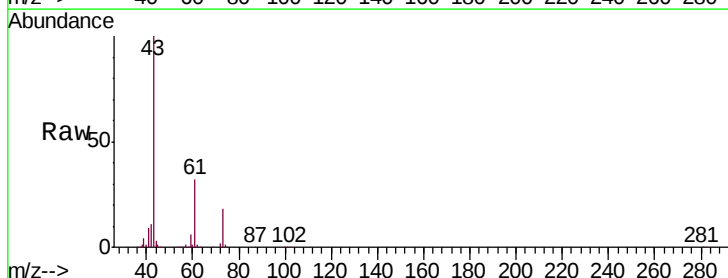

Abundance Ion 62.90 (62.60 to 63.60): VN0

Ion 64.90 (64.60 to 65.60): VN0

9.26

1500


1000


500

0

9.20 9.25 9.30

Time-->

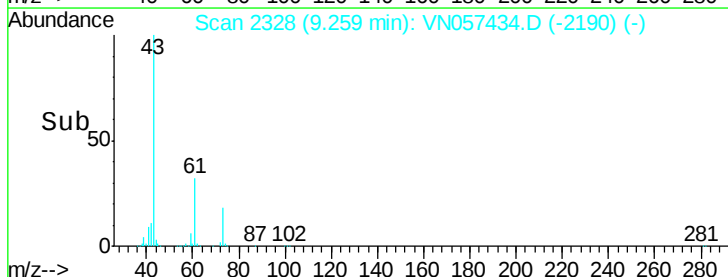







#48
Methyl methacrylate
Concen: 0.783 ug/l
RT: 9.17 min Scan# 2301
Delta R.T. -0.02 min
Lab File: VN057434.D
Acq: 20 Aug 2019 6:04

Instrument :
MSVOA_N
ClientSampleId :
T6-A4-(2)

Tgt Ion: 41 Resp: 6615
Ion Ratio Lower Upper
41 100
69 0.0 75.9 113.9#
39 0.0 42.3 63.5#




Abundance Ion 41.00 (40.70 to 41.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 39.00 (38.70 to 39.70): VN0


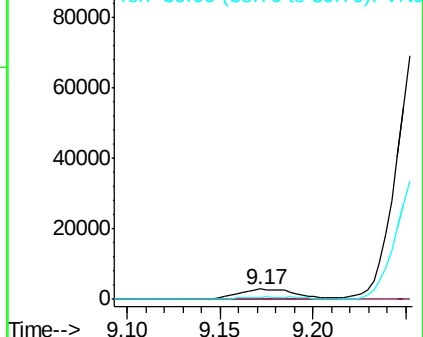



#50
Toluene-d8
Concen: 48.422 ug/l
RT: 10.08 min Scan# 2585
Delta R.T. -0.00 min
Lab File: VN057434.D
Acq: 20 Aug 2019 6:04

Tgt Ion: 98 Resp: 1646215
Ion Ratio Lower Upper
98 100
100 65.1 51.9 77.9



Abundance Ion 98.00 (97.70 to 98.70): VN0
Ion 100.00 (99.70 to 100.70): VN0




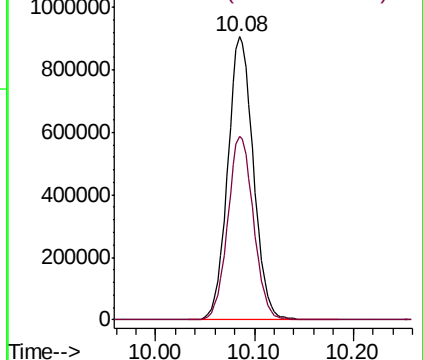




#51
 4-Methyl-2-Pentanone
 Concen: 0.713 ug/l
 RT: 9.98 min Scan# 2551
 Delta R.T. -0.00 min
 Lab File: VN057434.D
 Acq: 20 Aug 2019 6:04




Instrument :
 MSVOA_N
 ClientSampled :
 T6-A4-(2)


Tgt Ion: 43 Resp: 7538
 Ion Ratio Lower Upper
 43 100
 58 42.1 33.2 49.8

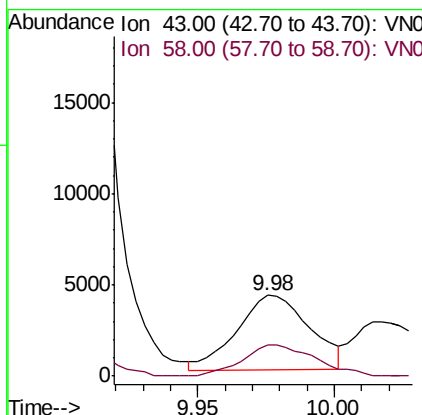

#54
 cis-1,3-Dichloropropene
 Concen: 3.946 ug/l
 RT: 9.90 min Scan# 2527
 Delta R.T. 0.06 min
 Lab File: VN057434.D
 Acq: 20 Aug 2019 6:04

Tgt Ion: 75 Resp: 61413
 Ion Ratio Lower Upper
 75 100
 77 0.7 24.9 37.3#
 39 22.9 32.7 49.1#



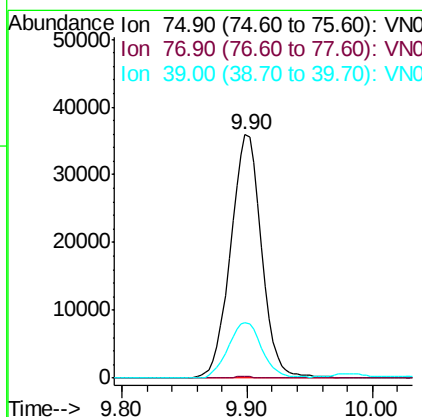



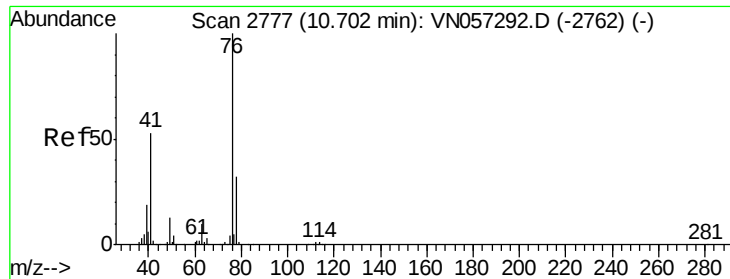

#57
 1,3-Dichloropropane
 Concen: 0.601 ug/l
 RT: 10.76 min Scan# 2794
 Delta R.T. 0.05 min
 Lab File: VN057434.D
 Acq: 20 Aug 2019 6:04




Instrument :
 MSVOA_N
 ClientSampleId :
 T6-A4-(2)


Tgt Ion: 76 Resp: 9412
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.6 38.4#

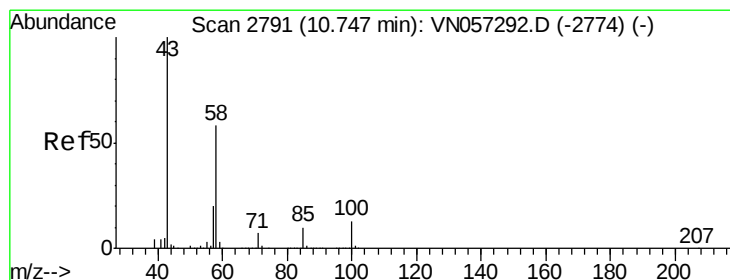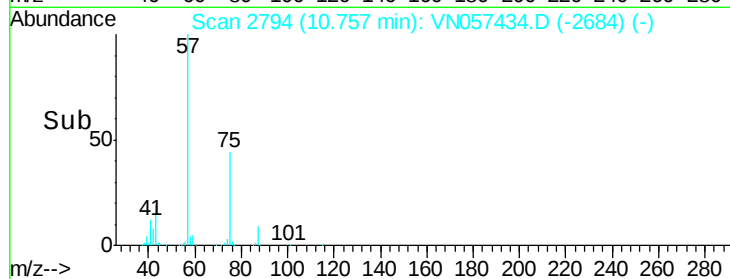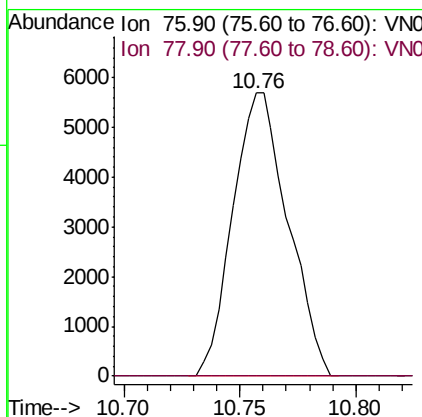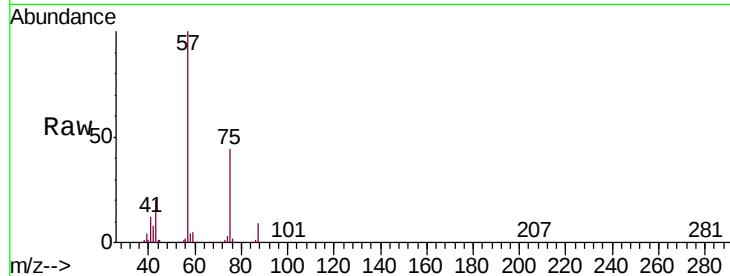

#59
 2-Hexanone
 Concen: 15.455 ug/l
 RT: 10.76 min Scan# 2795
 Delta R.T. 0.01 min
 Lab File: VN057434.D
 Acq: 20 Aug 2019 6:04

Tgt Ion: 43 Resp: 117541
 Ion Ratio Lower Upper
 43 100
 58 19.9 28.6 85.9#

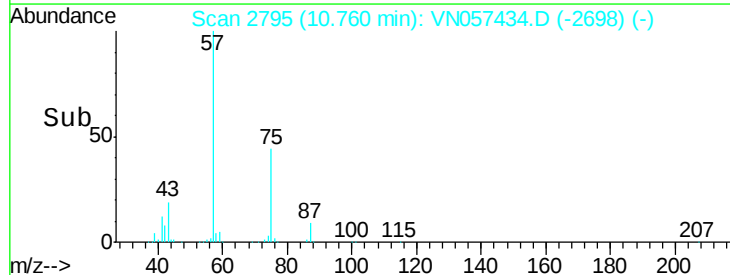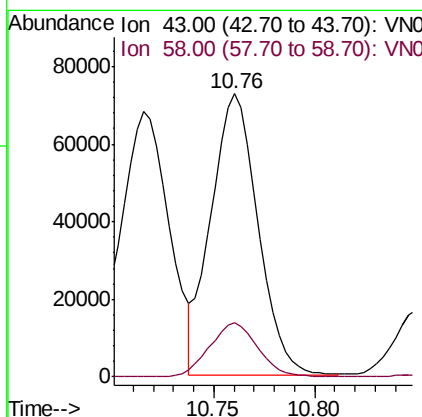



#62

4-Bromofluorobenzene

Concen: 37.101 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.00 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Instrument :

MSVOA_N

ClientSampleId :

T6-A4-(2)


Tgt Ion: 95 Resp: 445740

Ion Ratio Lower Upper

95 100

174 96.7 0.0 185.0




176 92.9 0.0 181.0

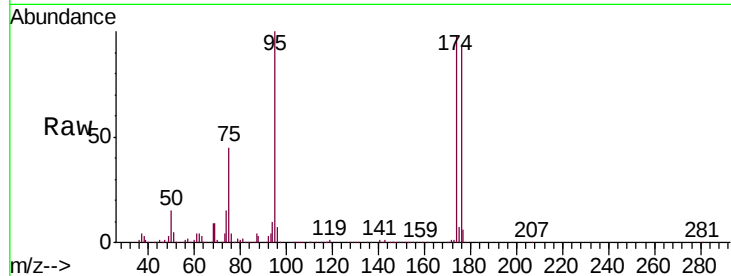

Abundance Ion 94.90 (94.60 to 95.60): VN057292.D (-3290) (-)

Ion 173.80 (173.50 to 174.50): VN057292.D (-3290) (-)

Ion 175.80 (175.50 to 176.50): VN057292.D (-3290) (-)

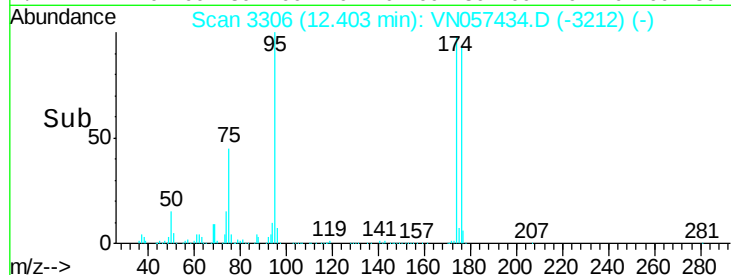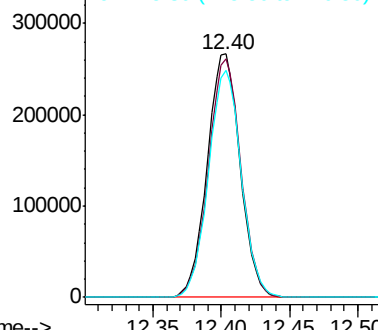

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. 0.00 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04


Tgt Ion: 117 Resp: 1206469

Ion Ratio Lower Upper

117 100

82 50.8 41.2 61.8



119 32.1 25.8 38.8




Abundance Ion 116.90 (116.60 to 117.60): VN057292.D (-2979) (-)

Ion 82.00 (81.70 to 82.70): VN057292.D (-2979) (-)

Ion 118.90 (118.60 to 119.60): VN057292.D (-2979) (-)

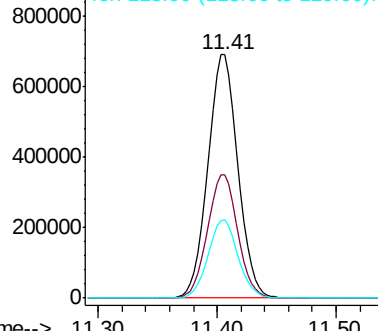



#71

Bromoform

Concen: 0.378 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.27 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Instrument :

MSVOA_N

ClientSampled :

T6-A4-(2)


Tgt Ion:173 Resp: 2813

Ion Ratio Lower Upper

173 100

175 1022.7 24.2 72.6#




254 0.0 0.2 0.2#

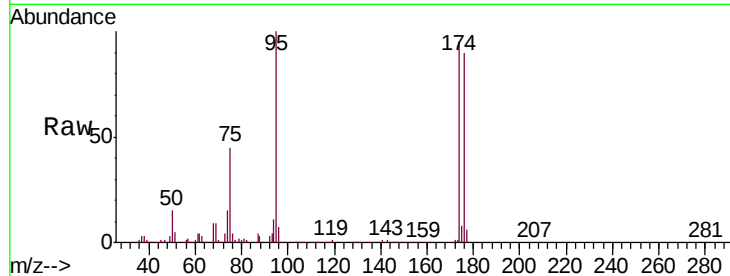

Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

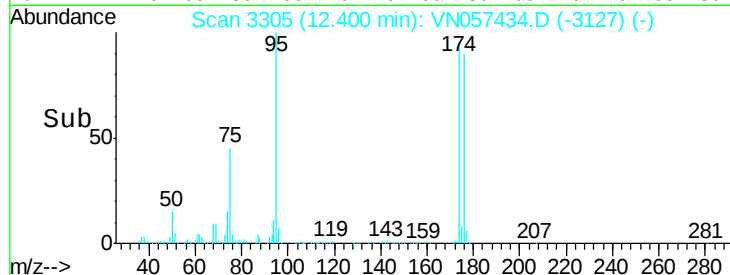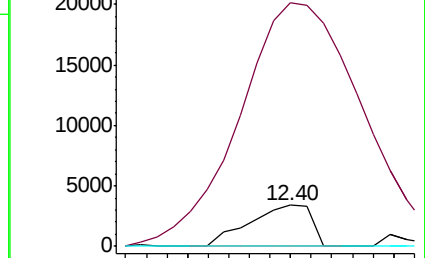

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.35 min Scan# 3599

Delta R.T. 0.00 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04


Tgt Ion:152 Resp: 332991

Ion Ratio Lower Upper

152 100

115 54.7 27.3 81.9



150 155.6 0.0 344.4




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

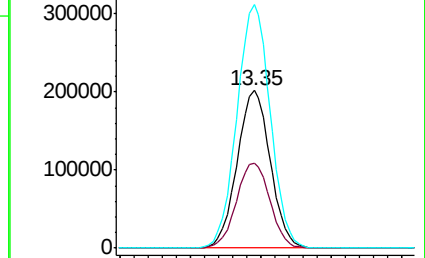



#73

Isopropylbenzene

Concen: Below Cal

RT: 12.25 min Scan# 3258

Delta R.T. 0.00 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Instrument :

MSVOA_N

ClientSampleId :





T6-A4-(2)

Tgt Ion: 105 Resp: 29

Ion Ratio Lower Upper

105 100

120 0.0 13.2 39.6#

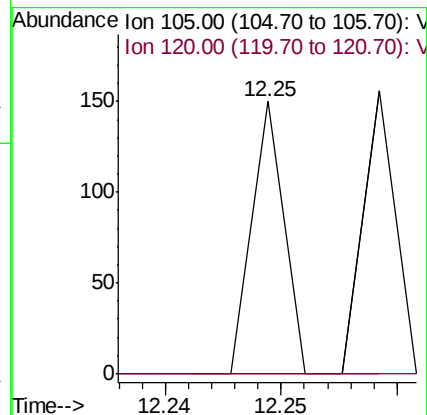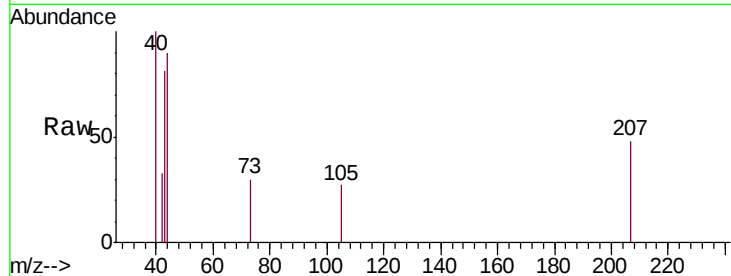

#74

N-ethyl acetate

Concen: 0.427 ug/l

RT: 12.03 min Scan# 3189

Delta R.T. -0.04 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Tgt Ion: 43 Resp: 4129




Ion Ratio Lower Upper


43 100

70 0.0 36.2 54.2#

55 1.9 20.1 30.1#

61 0.0 20.9 31.3#

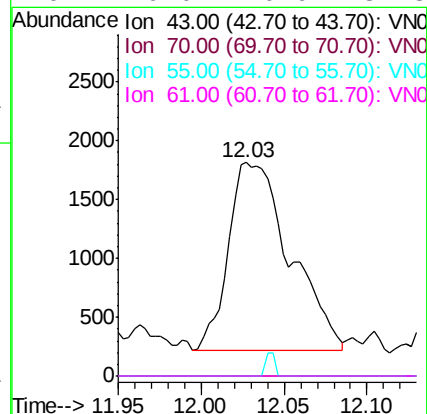



#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.40 min Scan# 3306

Delta R.T. -0.10 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Instrument :

MSVOA_N

ClientSampled :

T6-A4-(2)





Tgt Ion: 83 Resp: 63

Ion Ratio Lower Upper

83 100

131 911.1 5.4 16.2#

85 0.0 32.3 96.9#

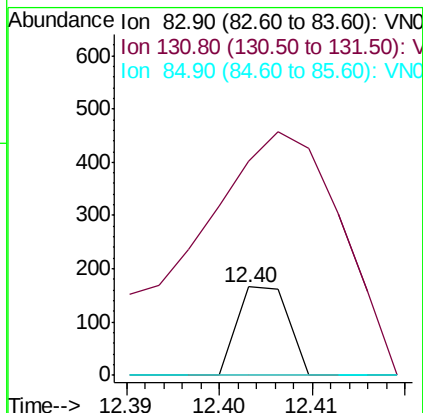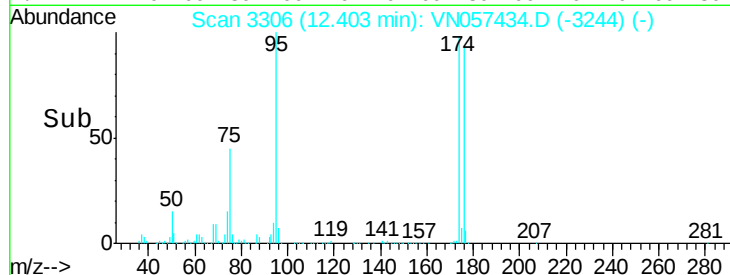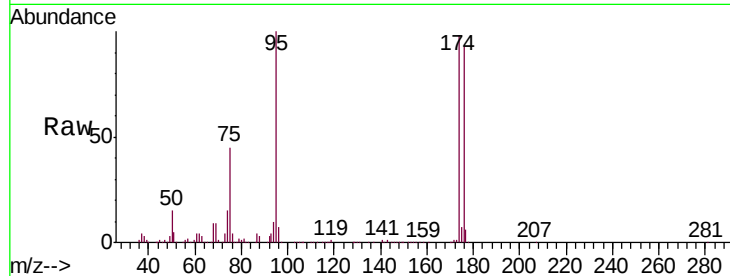

#76

1,2,3-Trichloropropane

Concen: 30.512 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. -0.15 min

Lab File: VN057434.D




Acq: 20 Aug 2019 6:04


Tgt Ion: 75 Resp: 204823

Ion Ratio Lower Upper

75 100

77 1.3 0.0 0.0#

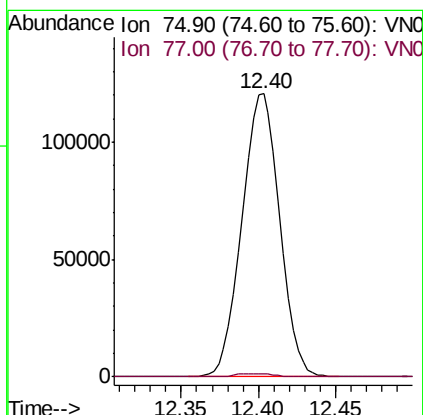



#77

Bromobenzene

Concen: Below Cal

RT: 12.40 min Scan# 3304

Delta R.T. -0.13 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Instrument :

MSVOA_N

ClientSampleId :

T6-A4-(2)


Tgt Ion: 156 Resp: 102

Ion Ratio Lower Upper

156 100

77 2519.6 89.8 269.6#




158 0.0 49.3 147.8#



Abundance Ion 155.80 (155.50 to 156.50): V

Ion 77.00 (76.70 to 77.70): VN0

Ion 157.80 (157.50 to 158.50): V

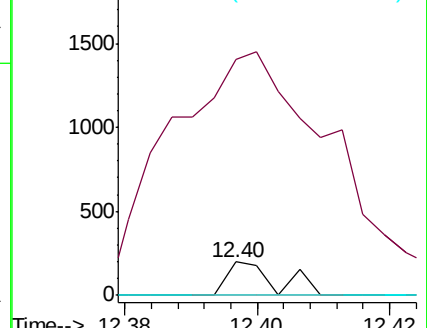

#79

2-Chlorotoluene

Concen: Below Cal

RT: 12.59 min Scan# 3364

Delta R.T. -0.08 min

Lab File: VN057434.D


Acq: 20 Aug 2019 6:04

Tgt Ion: 91 Resp: 129

Ion Ratio Lower Upper



91 100


126 0.0 18.1 54.1#



Abundance Ion 91.00 (90.70 to 91.70): VN0

Ion 125.90 (125.60 to 126.60): V

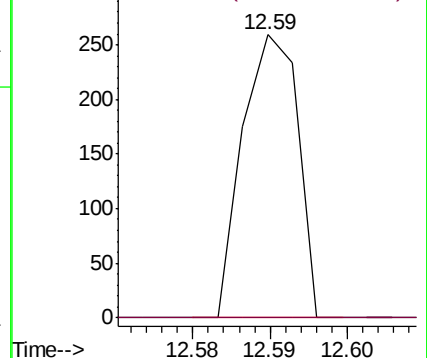



#80

1,3,5-Trimethylbenzene

Concen: Below Cal

RT: 12.74 min Scan# 3410

Delta R.T. 0.00 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04

Instrument :

MSVOA_N

ClientSampled :





T6-A4-(2)

Tgt Ion: 105 Resp: 1187

Ion Ratio Lower Upper

105 100

120 40.2 24.3 73.0

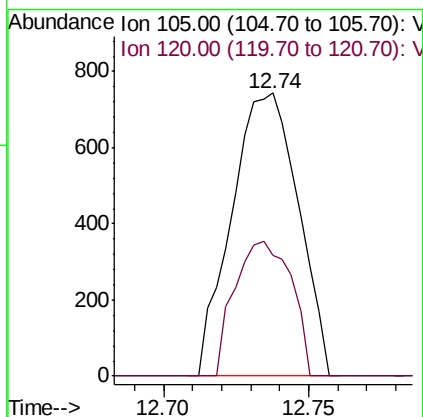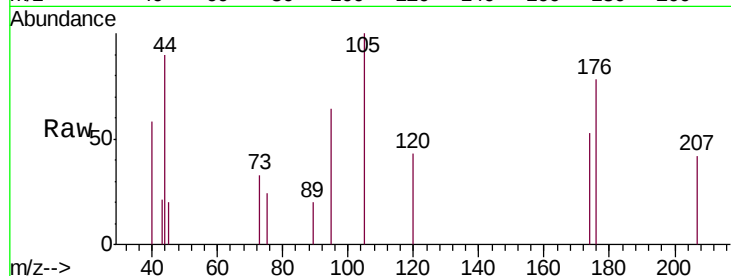

#81

trans-1,4-Dichloro-2-butene

Concen: 75.004 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.10 min

Lab File: VN057434.D

Acq: 20 Aug 2019 6:04




Tgt Ion: 75 Resp: 204823


Ion Ratio Lower Upper

75 100

53 0.0 67.9 101.9#

89 0.0 36.2 54.4#



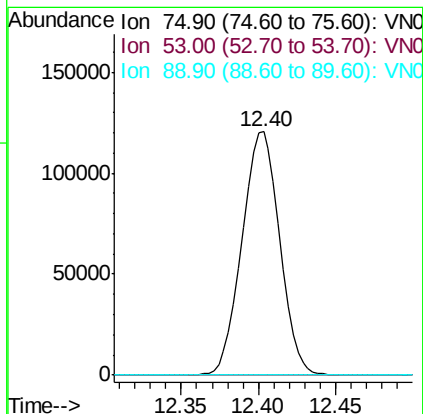





#85
 sec-Butylbenzene
 Concen: Below Cal
 RT: 13.04 min Scan# 3505
 Delta R.T. -0.13 min
 Lab File: VN057434.D
 Acq: 20 Aug 2019 6:04

Instrument :
 MSVOA_N
 ClientSampled :
 T6-A4-(2)

Tgt Ion:105 Resp: 206
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.4 31.2#

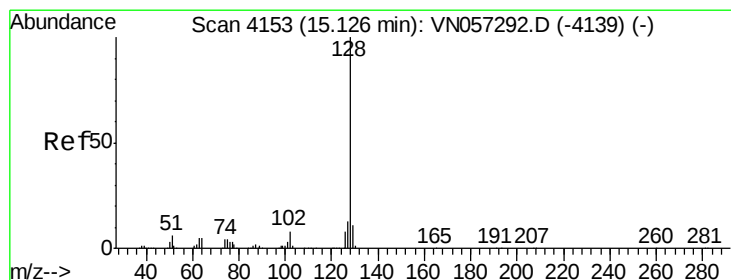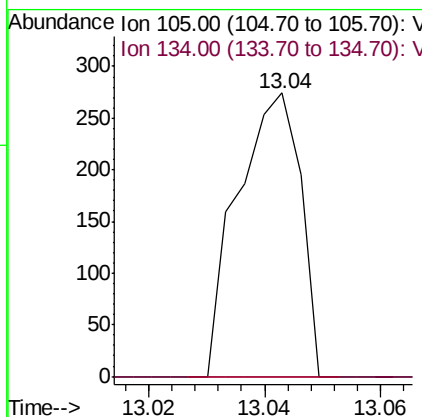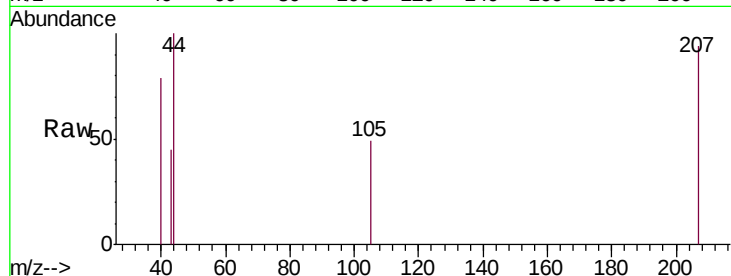

#95
 Naphthalene
 Concen: Below Cal
 RT: 15.14 min Scan# 4157
 Delta R.T. 0.01 min
 Lab File: VN057434.D
 Acq: 20 Aug 2019 6:04

Tgt Ion:128 Resp: 566
 Ion Ratio Lower Upper
 128 100
 127 0.0 10.5 15.7#
 129 0.0 8.8 13.2#

