

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN081919\
 Data File : VN057429.D
 Acq On : 20 Aug 2019 4:03
 Operator : JC/SP
 Sample : K4386-34
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 T6-A3-(0)

Quant Time: Aug 20 09:33:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 15 11:33:14 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.66	168	1045919	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.58	114	1450860	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1226342	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	325299	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.02	65	481811	42.37	ug/l	0.00
Spiked Amount 50.000			Recovery	=	84.74%	
35) Dibromofluoromethane	7.58	113	437510	46.00	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.00%	
50) Toluene-d8	10.08	98	1678137	48.24	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.48%	
62) 4-Bromofluorobenzene	12.40	95	453902	36.92	ug/l	0.00
Spiked Amount 50.000			Recovery	=	73.84%	
Target Compounds						
16) Acetone	3.82	43	9804	2.486	ug/l	93
43) Isopropyl Acetate	8.16	43	296714	14.667	ug/l #	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN081919\
Data File : VN057429.D
Acq On : 20 Aug 2019 4:03
Operator : JC/SP
Sample : K4386-34
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
T6-A3-(0)

Quant Time: Aug 20 09:33:28 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 15 11:33:14 2019
Response via : Initial Calibration

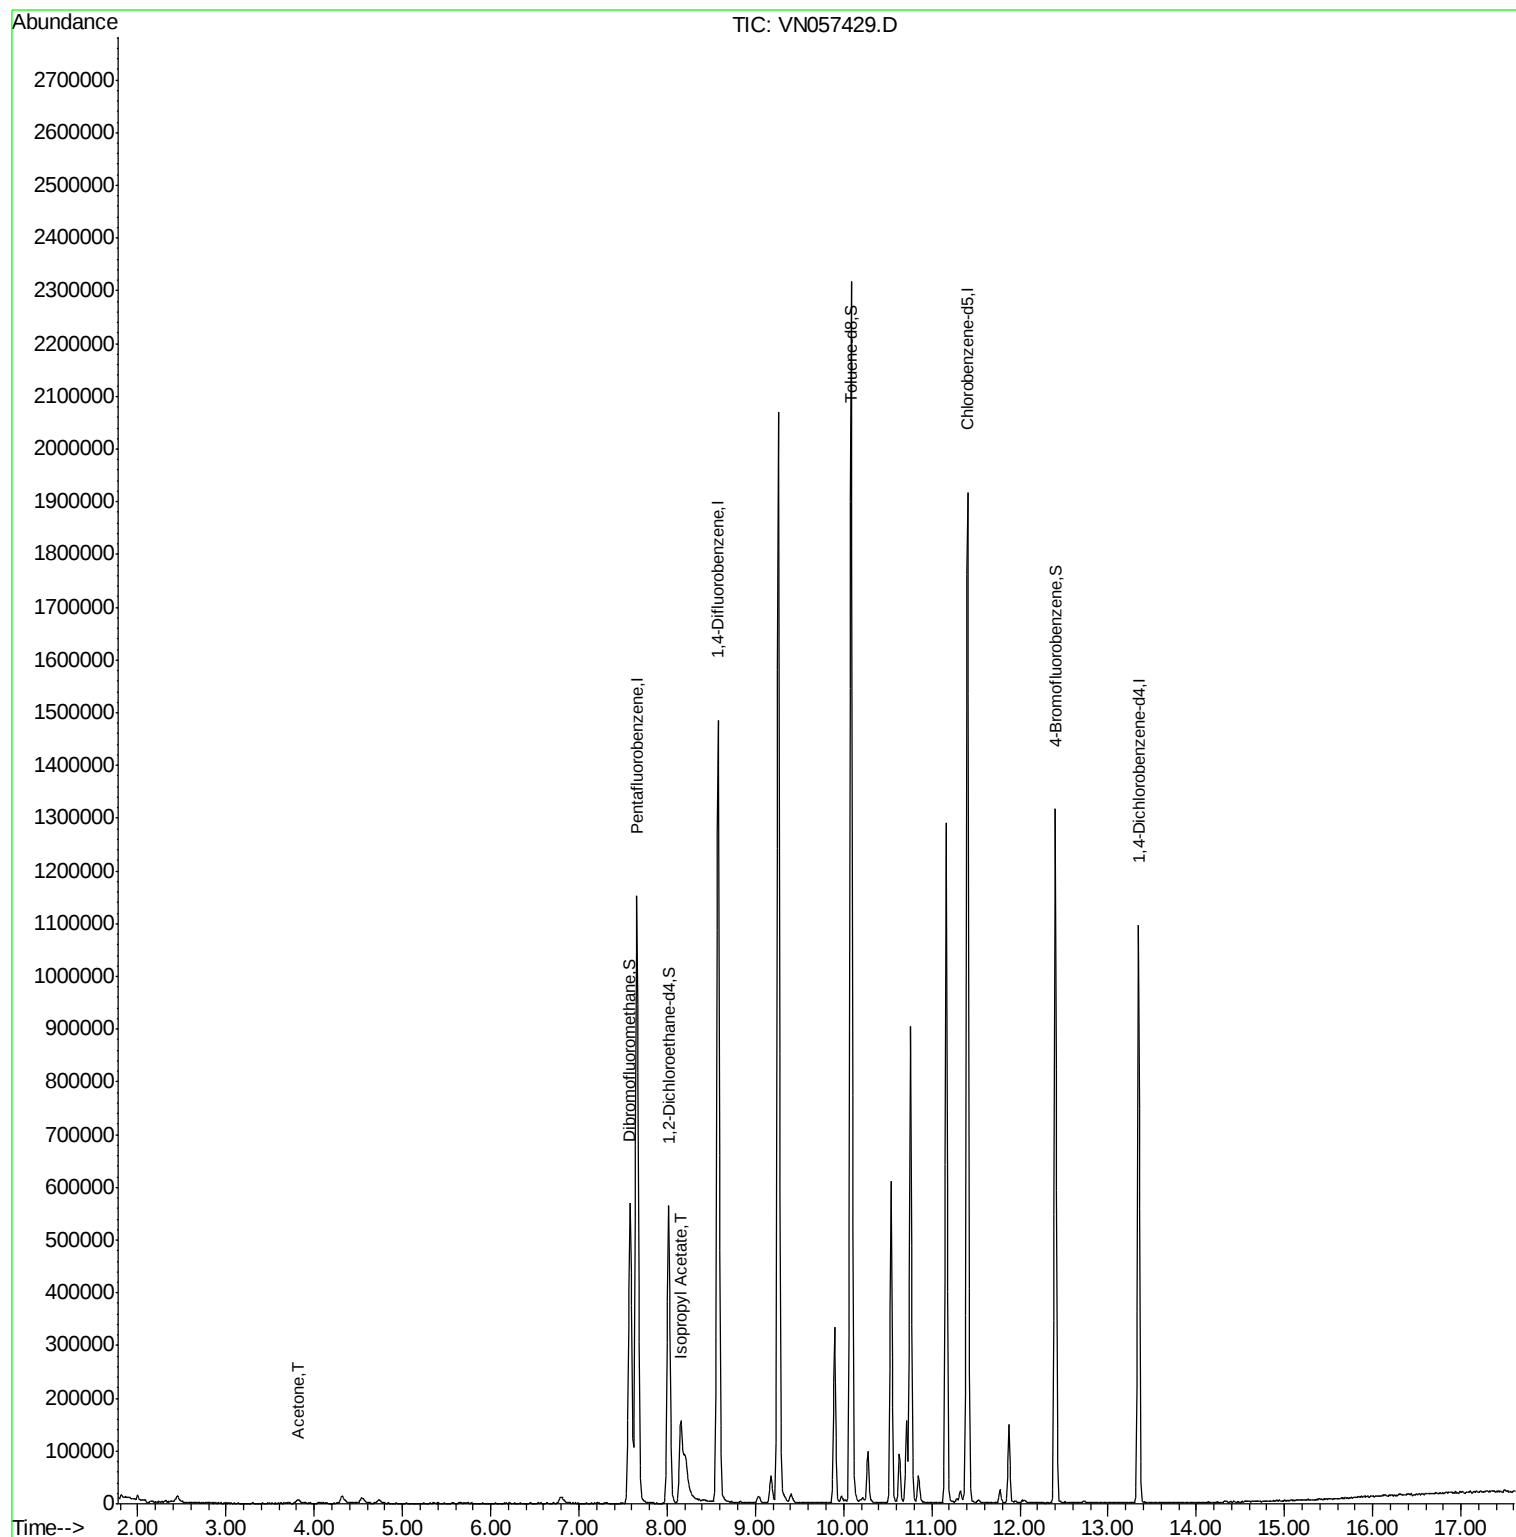

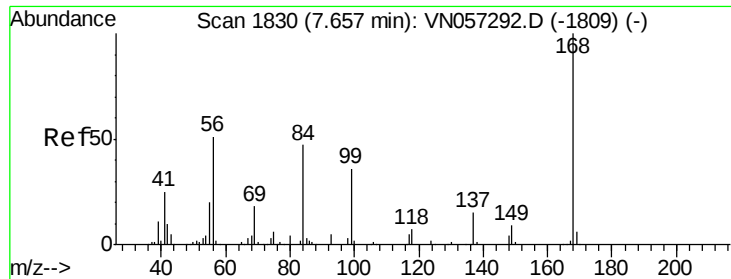

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.66 min Scan# 1830

Delta R.T. -0.00 min

Lab File: VN057429.D

Acq: 20 Aug 2019 4:03

Instrument :

MSVOA_N

ClientSampled :


T6-A3-(0)

Tot Ion:168 Resp: 1045919

Ion Ratio Lower Upper

168 100

99 47.7 39.4 59.2

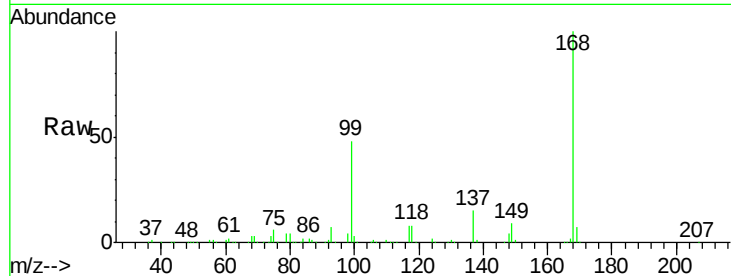

Abundance Ion 167.90 (167.60 to 168.60): VN057429.D (-1737) (-)

Ion 98.90 (98.60 to 99.60): VN057429.D (-1737) (-)

7.66

400000

300000



200000

100000

0

7.60 7.70

Time-->

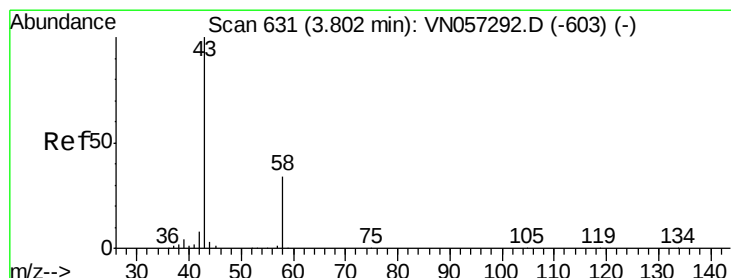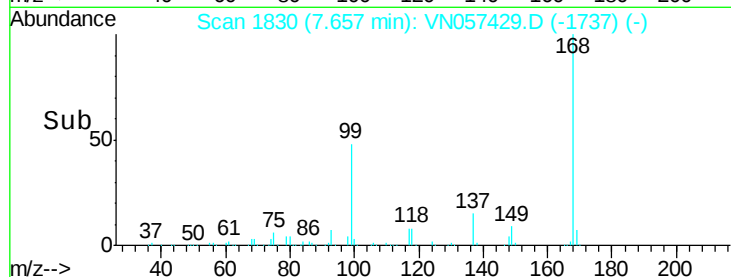

#16

Acetone

Concen: 2.486 ug/l

RT: 3.82 min Scan# 636

Delta R.T. 0.02 min

Lab File: VN057429.D


Acq: 20 Aug 2019 4:03

Tgt Ion: 43 Resp: 9804

Ion Ratio Lower Upper

43 100

58 29.6 27.0 40.6

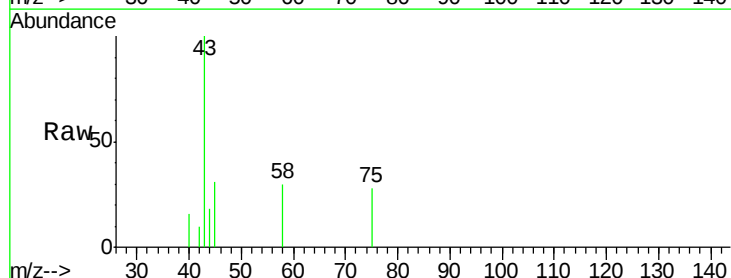

Abundance Ion 43.00 (42.70 to 43.70): VN057429.D (-538) (-)

Ion 58.00 (57.70 to 58.70): VN057429.D (-538) (-)

3.82

3000


2000


1000

0

3.75 3.80 3.85 3.90

Time-->




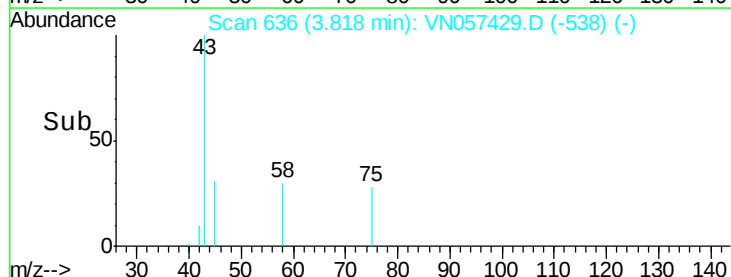


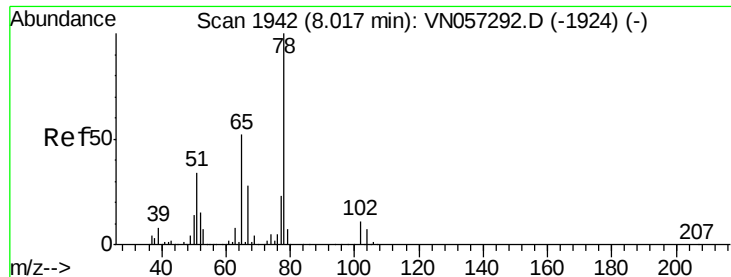

#33
 1,2-Dichloroethane-d4
 Concen: 42.375 ug/l
 RT: 8.02 min Scan# 1942
 Delta R.T. -0.00 min
 Lab File: VN057429.D
 Acq: 20 Aug 2019 4:03




Instrument :
 MSVOA_N
 ClientSampleId :
 T6-A3-(0)


Tot Ion: 65 Resp: 481811
 Ion Ratio Lower Upper
 65 100
 67 53.2 0.0 107.4

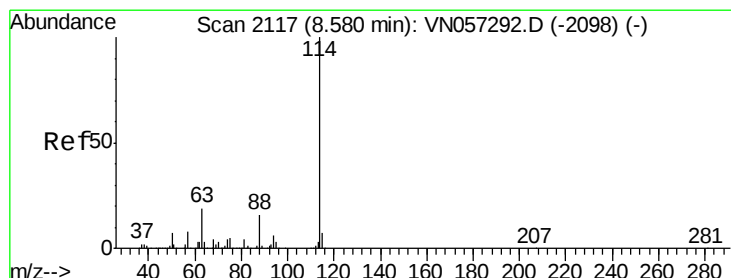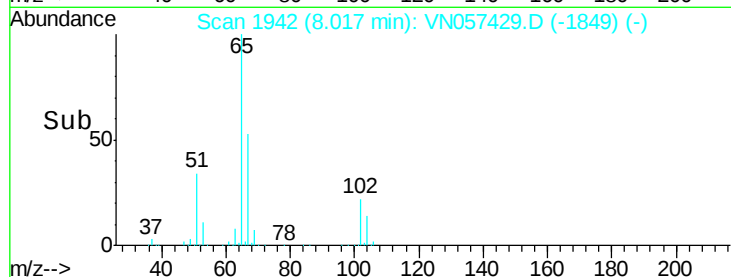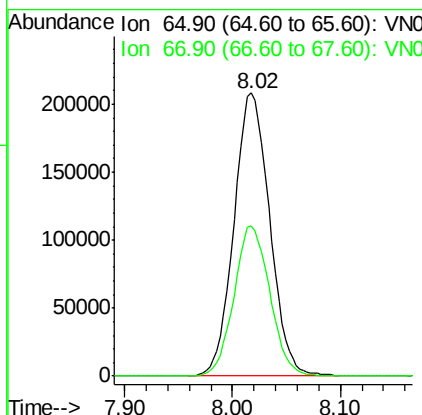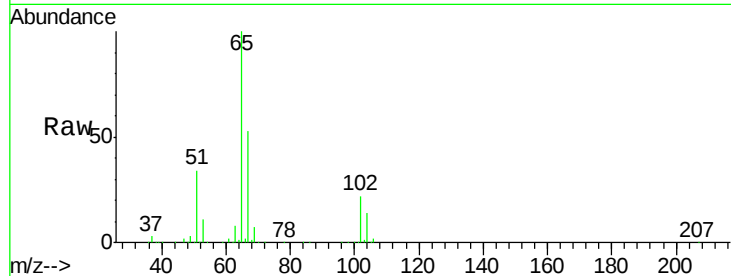

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.58 min Scan# 2117
 Delta R.T. -0.00 min
 Lab File: VN057429.D
 Acq: 20 Aug 2019 4:03

Tgt Ion: 114 Resp: 1450860
 Ion Ratio Lower Upper
 114 100
 63 17.8 0.0 38.8
 88 15.1 0.0 31.4


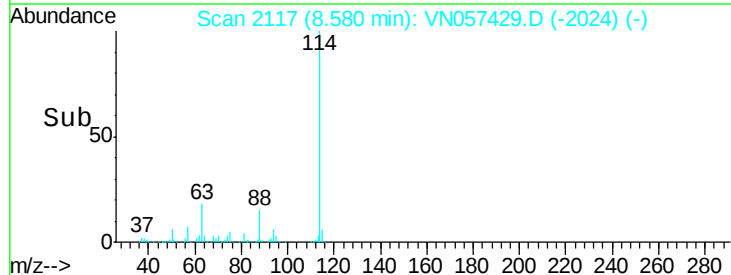
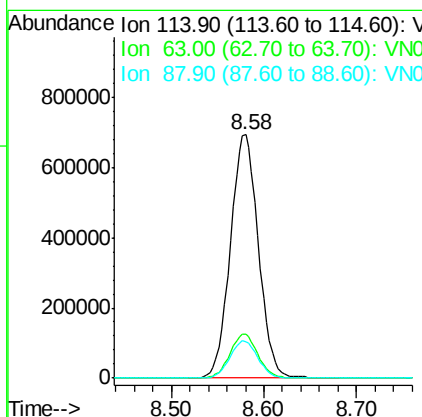
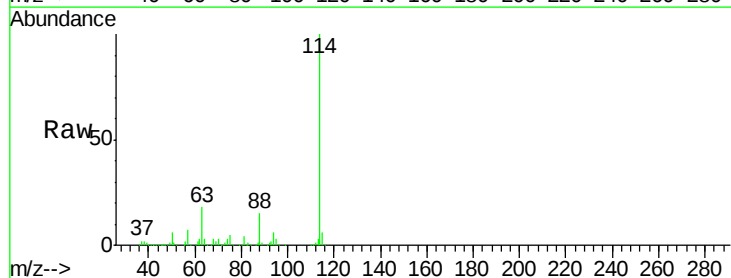


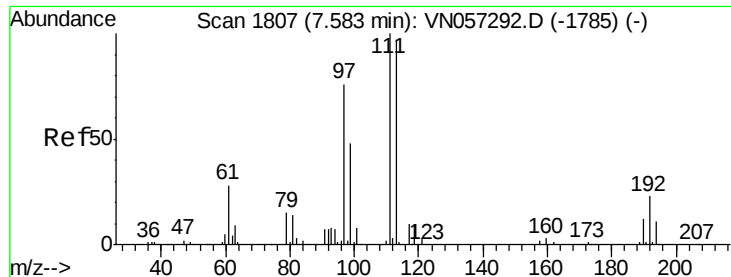

#35
 Dibromofluoromethane
 Concen: 46.002 ug/l
 RT: 7.58 min Scan# 1807
 Delta R.T. -0.00 min
 Lab File: VN057429.D
 Acq: 20 Aug 2019 4:03




Instrument :
 MSVOA_N
 ClientSampleId :
 T6-A3-(0)


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.2	82.1	123.1
192	24.5	19.3	28.9

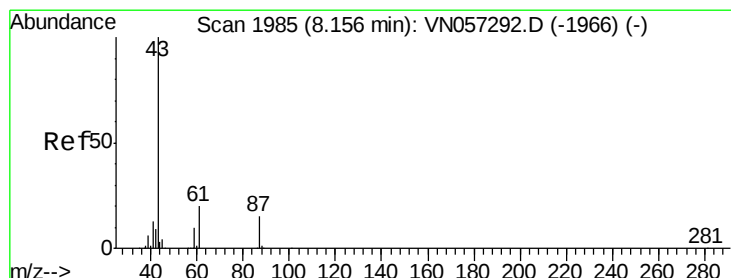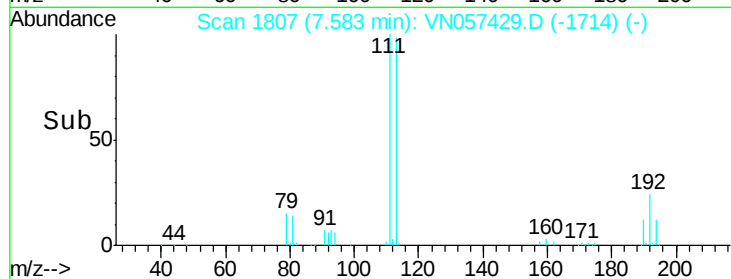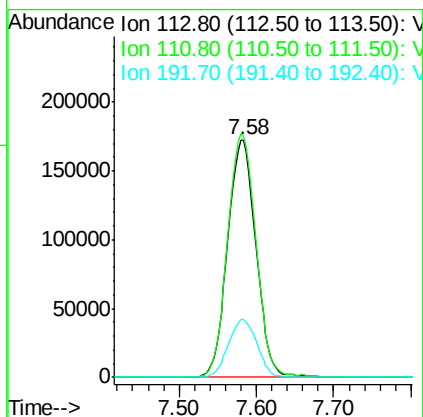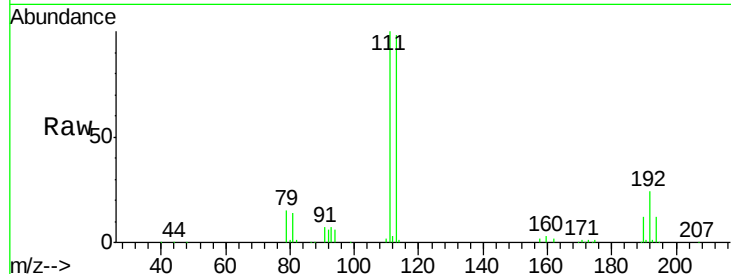

#43
 Isopropyl Acetate
 Concen: 14.667 ug/l
 RT: 8.16 min Scan# 1985
 Delta R.T. 0.00 min
 Lab File: VN057429.D
 Acq: 20 Aug 2019 4:03

Tgt Ion	Ratio	Lower	Upper
43	100		
61	9.7	21.6	32.4#
87	6.8	11.4	17.0#

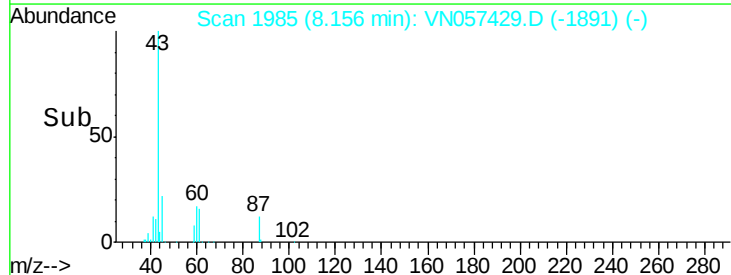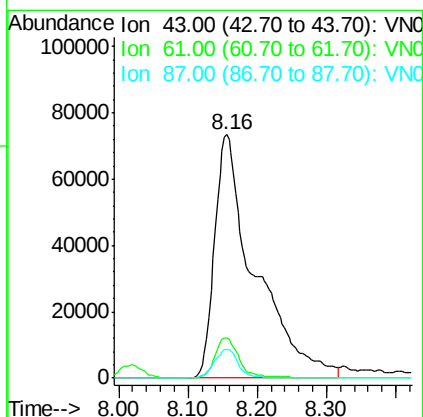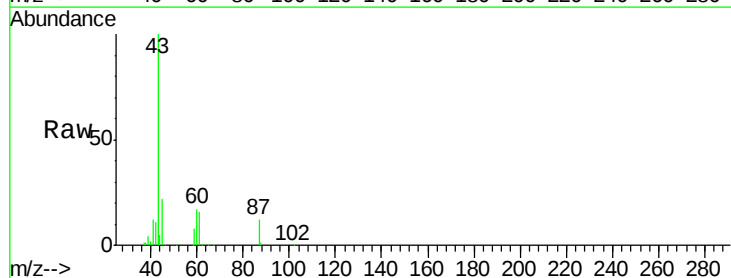

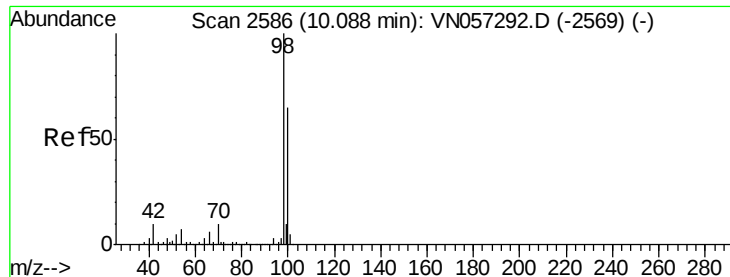

#50

Toluene-d8

Concen: 48.242 ug/l

RT: 10.08 min Scan# 2585

Delta R.T. -0.00 min

Lab File: VN057429.D

Acq: 20 Aug 2019 4:03

Instrument :

MSVOA_N

ClientSampled :





T6-A3-(0)

Tot Ion: 98 Resp: 1678137

Ion Ratio Lower Upper

98 100

100 65.7 51.9 77.9

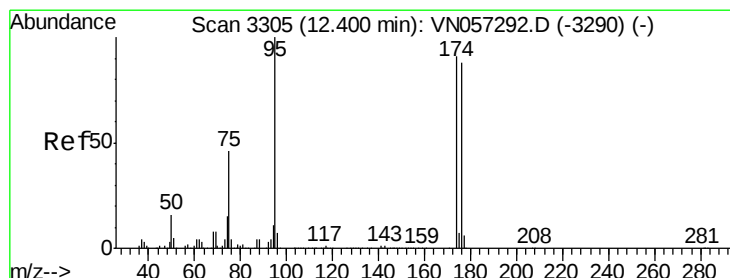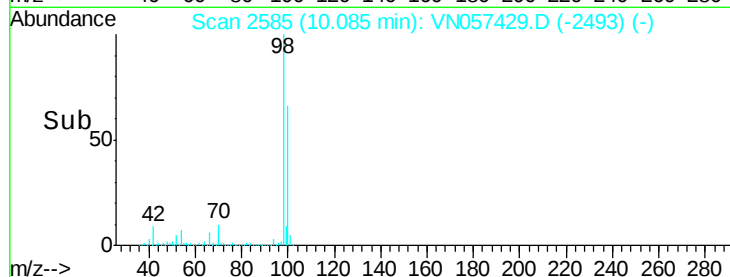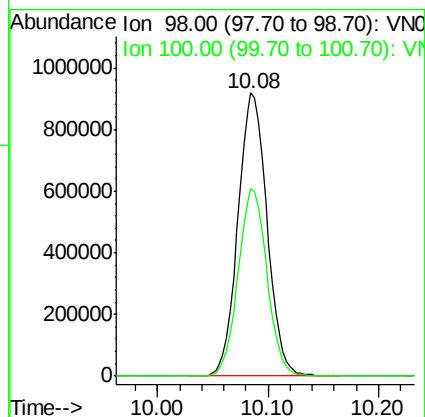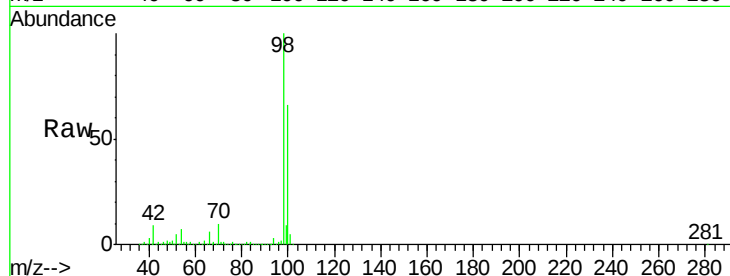

#62

4-Bromofluorobenzene

Concen: 36.924 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN057429.D

Acq: 20 Aug 2019 4:03




Tgt Ion: 95 Resp: 453902


Ion Ratio Lower Upper

95 100

174 96.6 0.0 185.0

176 94.5 0.0 181.0

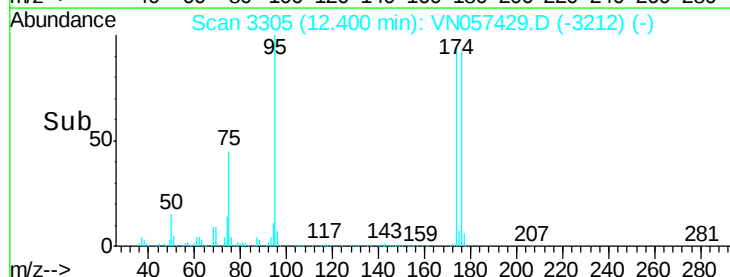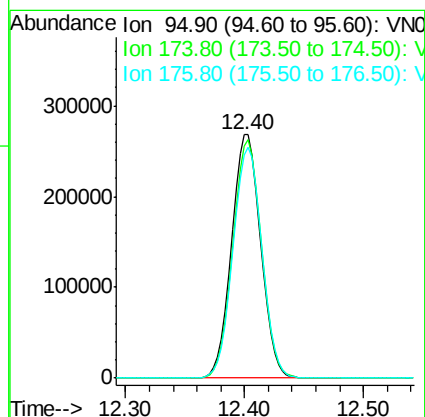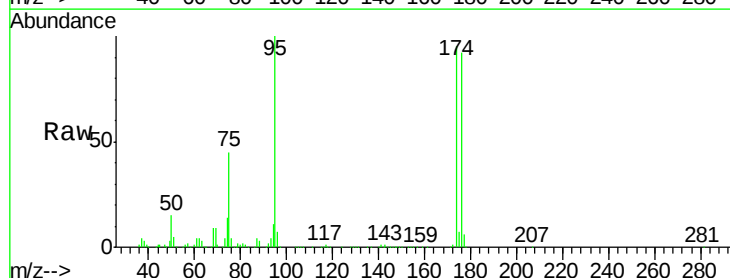


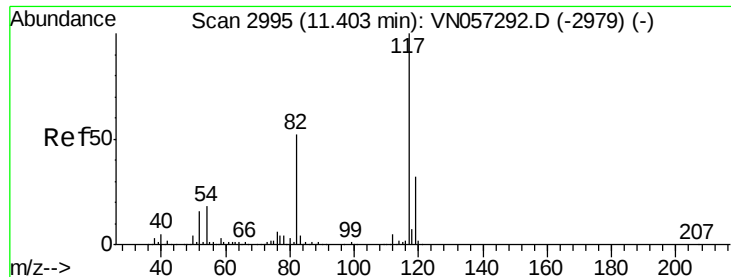




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN057429.D
Acq: 20 Aug 2019 4:03

Instrument :
MSVOA_N
ClientSampleId :
T6-A3-(0)

Tot Ion:117 Resp: 1226342
Ion Ratio Lower Upper
117 100
82 51.8 41.2 61.8
119 33.1 25.8 38.8

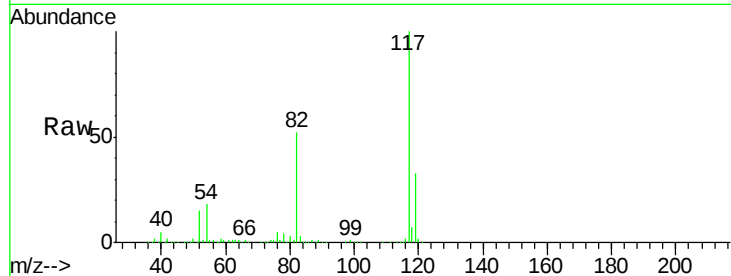


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

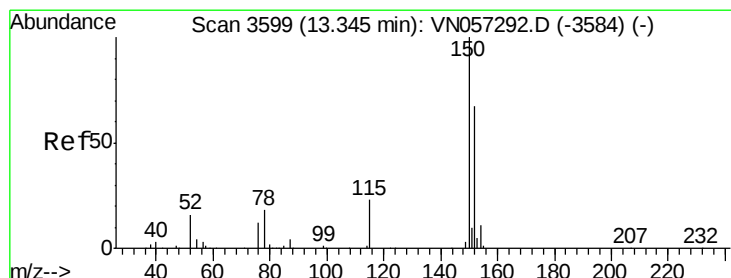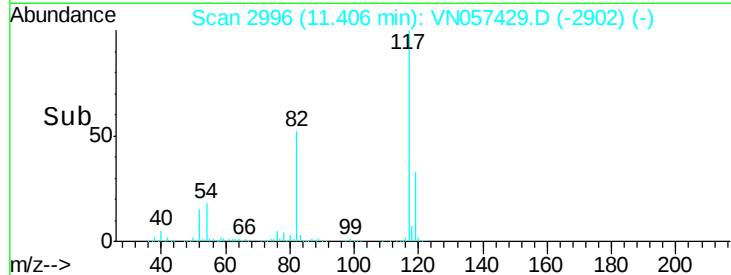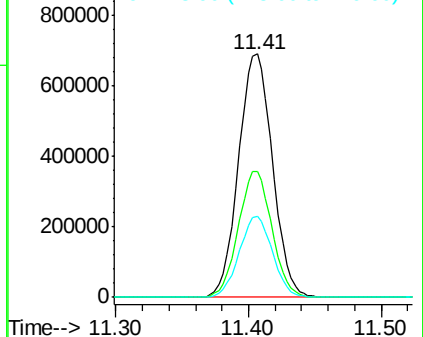

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.35 min Scan# 3599
Delta R.T. -0.00 min
Lab File: VN057429.D
Acq: 20 Aug 2019 4:03

Tgt Ion:152 Resp: 325299
Ion Ratio Lower Upper
152 100
115 55.0 27.3 81.9
150 157.9 0.0 344.4

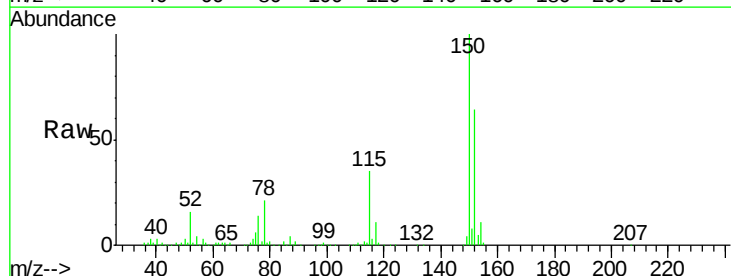

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

