


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081919\
Data File : VN057384.D
Acq On : 19 Aug 2019 8:20
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081519W.M
Title : SW846 8260
Last Update : Thu Aug 15 11:33:14 2019

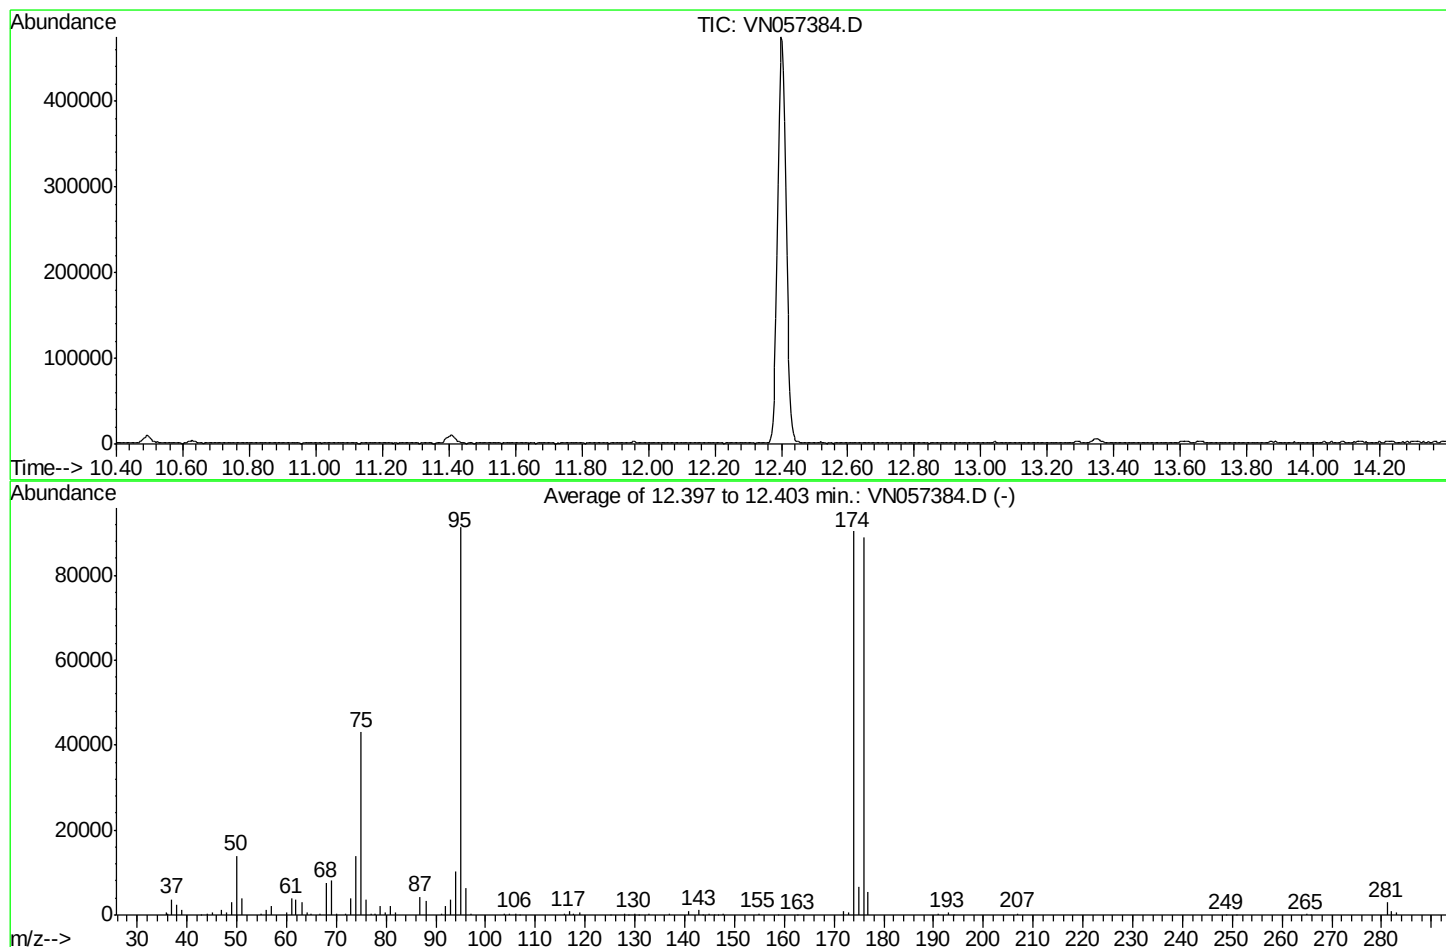

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	13932	PASS
75	95	30	60	47.1	42965	PASS
95	95	100	100	100.0	91269	PASS
96	95	5	9	6.9	6292	PASS
173	174	0.00	2	0.7	667	PASS
174	95	50	100	99.2	90496	PASS
175	174	5	9	7.5	6756	PASS
176	174	95	101	98.1	88802	PASS
177	176	5	9	6.1	5378	PASS