


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081919\  
 Data File : VN057413.D  
 Acq On : 19 Aug 2019 20:23  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 30 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N081519W.M  
 Title : SW846 8260  
 Last Update : Thu Aug 15 11:33:14 2019

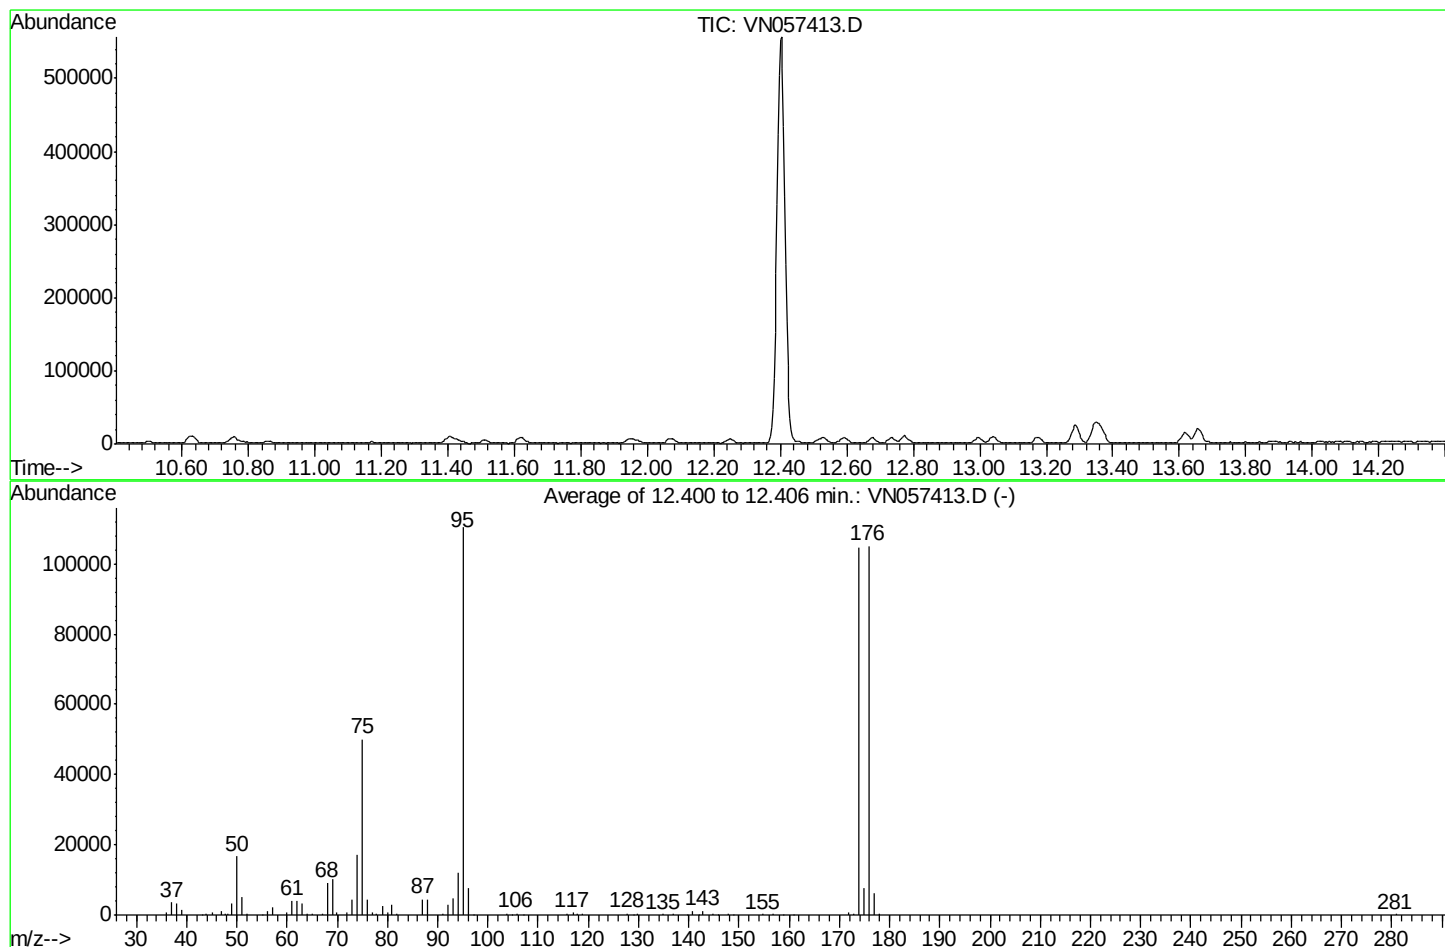

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 15.2      | 16758   | PASS             |
| 75          | 95           | 30           | 60           | 45.4      | 50104   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 110424  | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 7527    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.4       | 434     | PASS             |
| 174         | 95           | 50           | 100          | 94.8      | 104701  | PASS             |
| 175         | 174          | 5            | 9            | 7.3       | 7667    | PASS             |
| 176         | 174          | 95           | 101          | 100.5     | 105197  | PASS             |
| 177         | 176          | 5            | 9            | 5.9       | 6172    | PASS             |