


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN081920\
 Data File : VN063000.D
 Acq On : 19 Aug 2020 8:48
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
 Title : SW846 8260
 Last Update : Wed Aug 19 06:09:27 2020

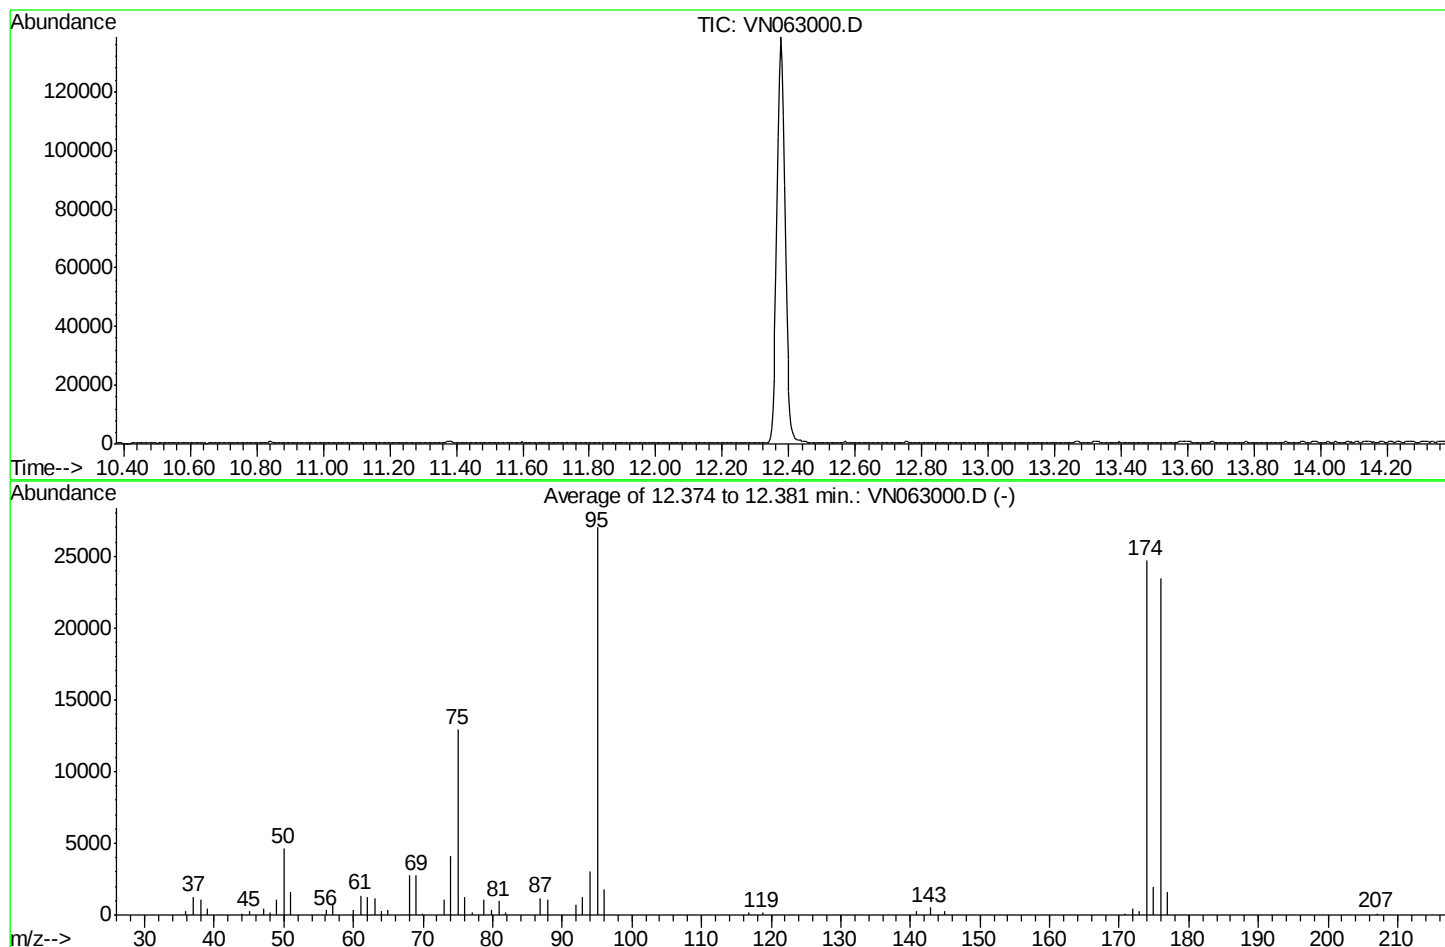

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3284

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	4615	PASS
75	95	30	60	47.8	12905	PASS
95	95	100	100	100.0	27018	PASS
96	95	5	9	6.5	1746	PASS
173	174	0.00	2	1.2	304	PASS
174	95	50	100	91.4	24688	PASS
175	174	5	9	8.1	1996	PASS
176	174	95	101	95.1	23477	PASS
177	176	5	9	6.9	1620	PASS