
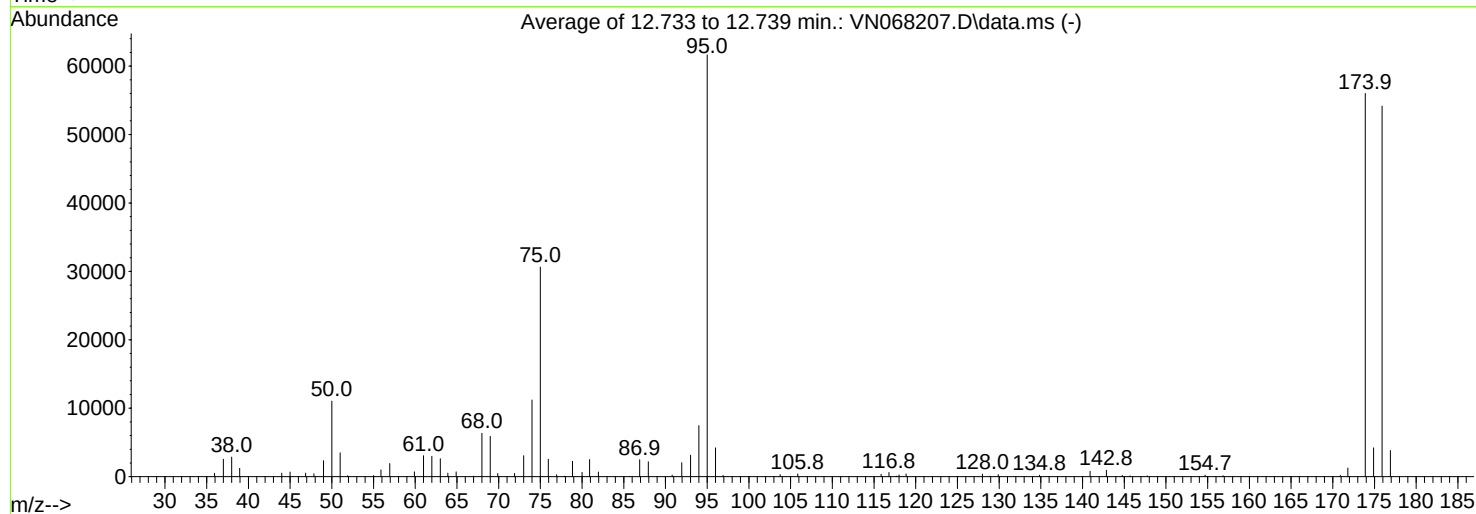


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081921\
Data File : VN068207.D
Acq On : 19 Aug 2021 10:47
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081721W.M
Title : SW846 8260
Last Update : Tue Aug 17 13:09:49 2021

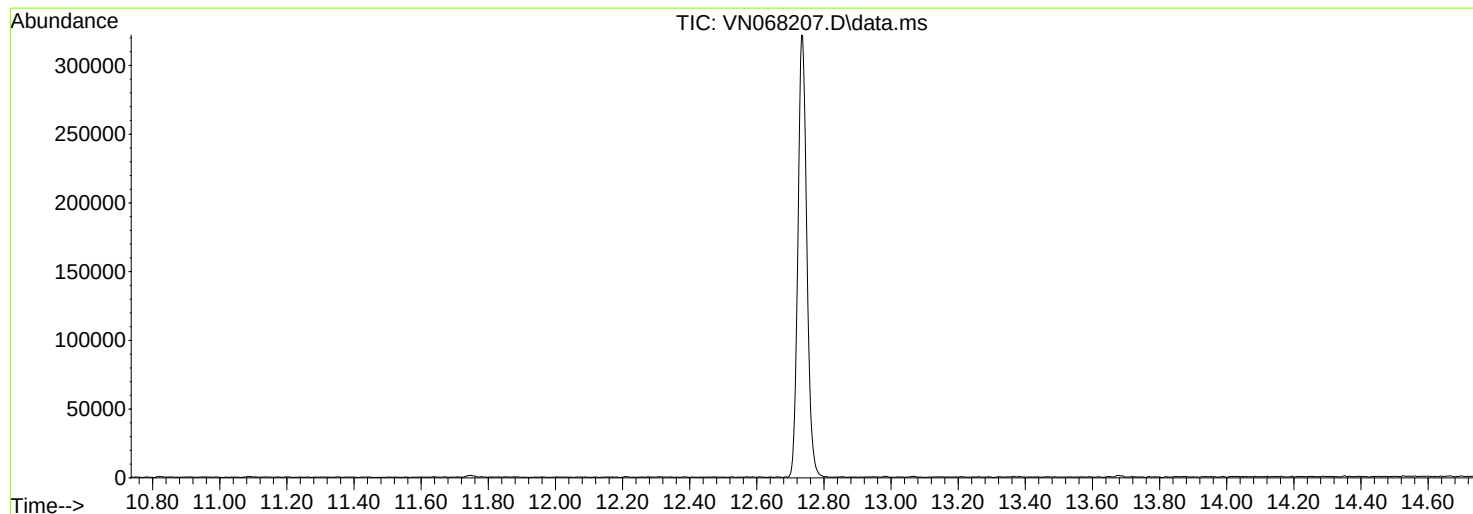

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3989

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.9	11043	PASS
75	95	30	60	49.7	30640	PASS
95	95	100	100	100.0	61648	PASS
96	95	5	9	6.8	4215	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.8	56005	PASS
175	174	5	9	7.5	4200	PASS
176	174	95	101	96.7	54157	PASS
177	176	5	9	7.0	3818	PASS