

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081922\
 Data File : VN074041.D
 Acq On : 19 Aug 2022 21:10
 Operator : JC\MD
 Sample : N4247-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-4

Quant Time: Aug 20 03:09:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081522W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 16 00:45:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	515674	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	821462	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	845121	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.615	152	505065	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.375	65	279309	55.610	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 111.220%			
35) Dibromofluoromethane	7.957	113	263660	54.273	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 108.540%			
50) Toluene-d8	10.380	98	906301	48.170	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 96.340%			
62) 4-Bromofluorobenzene	12.674	95	406664	65.126	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 130.260%#			
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	5.292	59	1972	1.755	ug/l #	80
13) Acrolein	3.993	56	393	0.500	ug/l	87
16) Acetone	4.228	43	62916	26.551	ug/l	98
18) Methyl Acetate	4.787	43	5343	Below Cal		97
20) Methylene Chloride	5.010	84	34321	6.864	ug/l	91
25) 2-Butanone	7.275	43	13110	3.489	ug/l #	87
29) Tetrahydrofuran	7.634	42	1703	0.707	ug/l #	67
31) Cyclohexane	8.016	56	8727	1.246	ug/l #	8
36) 1,1-Dichloropropene	8.022	75	35738	5.296	ug/l #	49
37) Ethyl Acetate	7.345	43	79952	9.780	ug/l	99
38) Carbon Tetrachloride	8.016	117	46291	6.002	ug/l #	16
40) Benzene	8.392	78	14094	0.662	ug/l	95
42) 1,2-Dichloroethane	8.504	62	2347	0.321	ug/l #	74
43) Isopropyl Acetate	8.498	43	339410	29.145	ug/l #	90
45) 1,2-Dichloropropane	9.569	63	4557	0.893	ug/l #	44
48) Methyl methacrylate	9.480	41	12294	2.467	ug/l #	37
49) 1,4-Dioxane	9.510	88	56	0.378	ug/l #	25
51) 4-Methyl-2-Pentanone	10.275	43	25483	3.237	ug/l #	78
52) Toluene	10.445	92	16628	1.139	ug/l	94
53) t-1,3-Dichloropropene	10.557	75	2495	0.321	ug/l #	82
54) cis-1,3-Dichloropropene	10.186	75	116180	13.642	ug/l #	61
57) 1,3-Dichloropropane	11.033	76	16785	1.817	ug/l #	42
59) 2-Hexanone	11.033	43	200904	33.155	ug/l #	50
68) m/p-Xylenes	11.886	106	7893	0.650	ug/l	97
69) o-Xylene	12.221	106	5011	0.412	ug/l	98
71) Bromoform	12.668	173	1925	0.317	ug/l #	28
74) N-amyl acetate	12.298	43	3863	0.278	ug/l #	40
76) 1,2,3-Trichloropropane	12.674	75	198233	18.883	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.674	75	198233	53.708	ug/l #	11
84) 1,2,4-Trimethylbenzene	13.321	105	13314	0.446	ug/l #	53
95) Naphthalene	15.433	128	62549	1.768	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081922\
Data File : VN074041.D
Acq On : 19 Aug 2022 21:10
Operator : JC\MD
Sample : N4247-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SB-4

Quant Time: Aug 20 03:09:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081522W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 16 00:45:21 2022
Response via : Initial Calibration




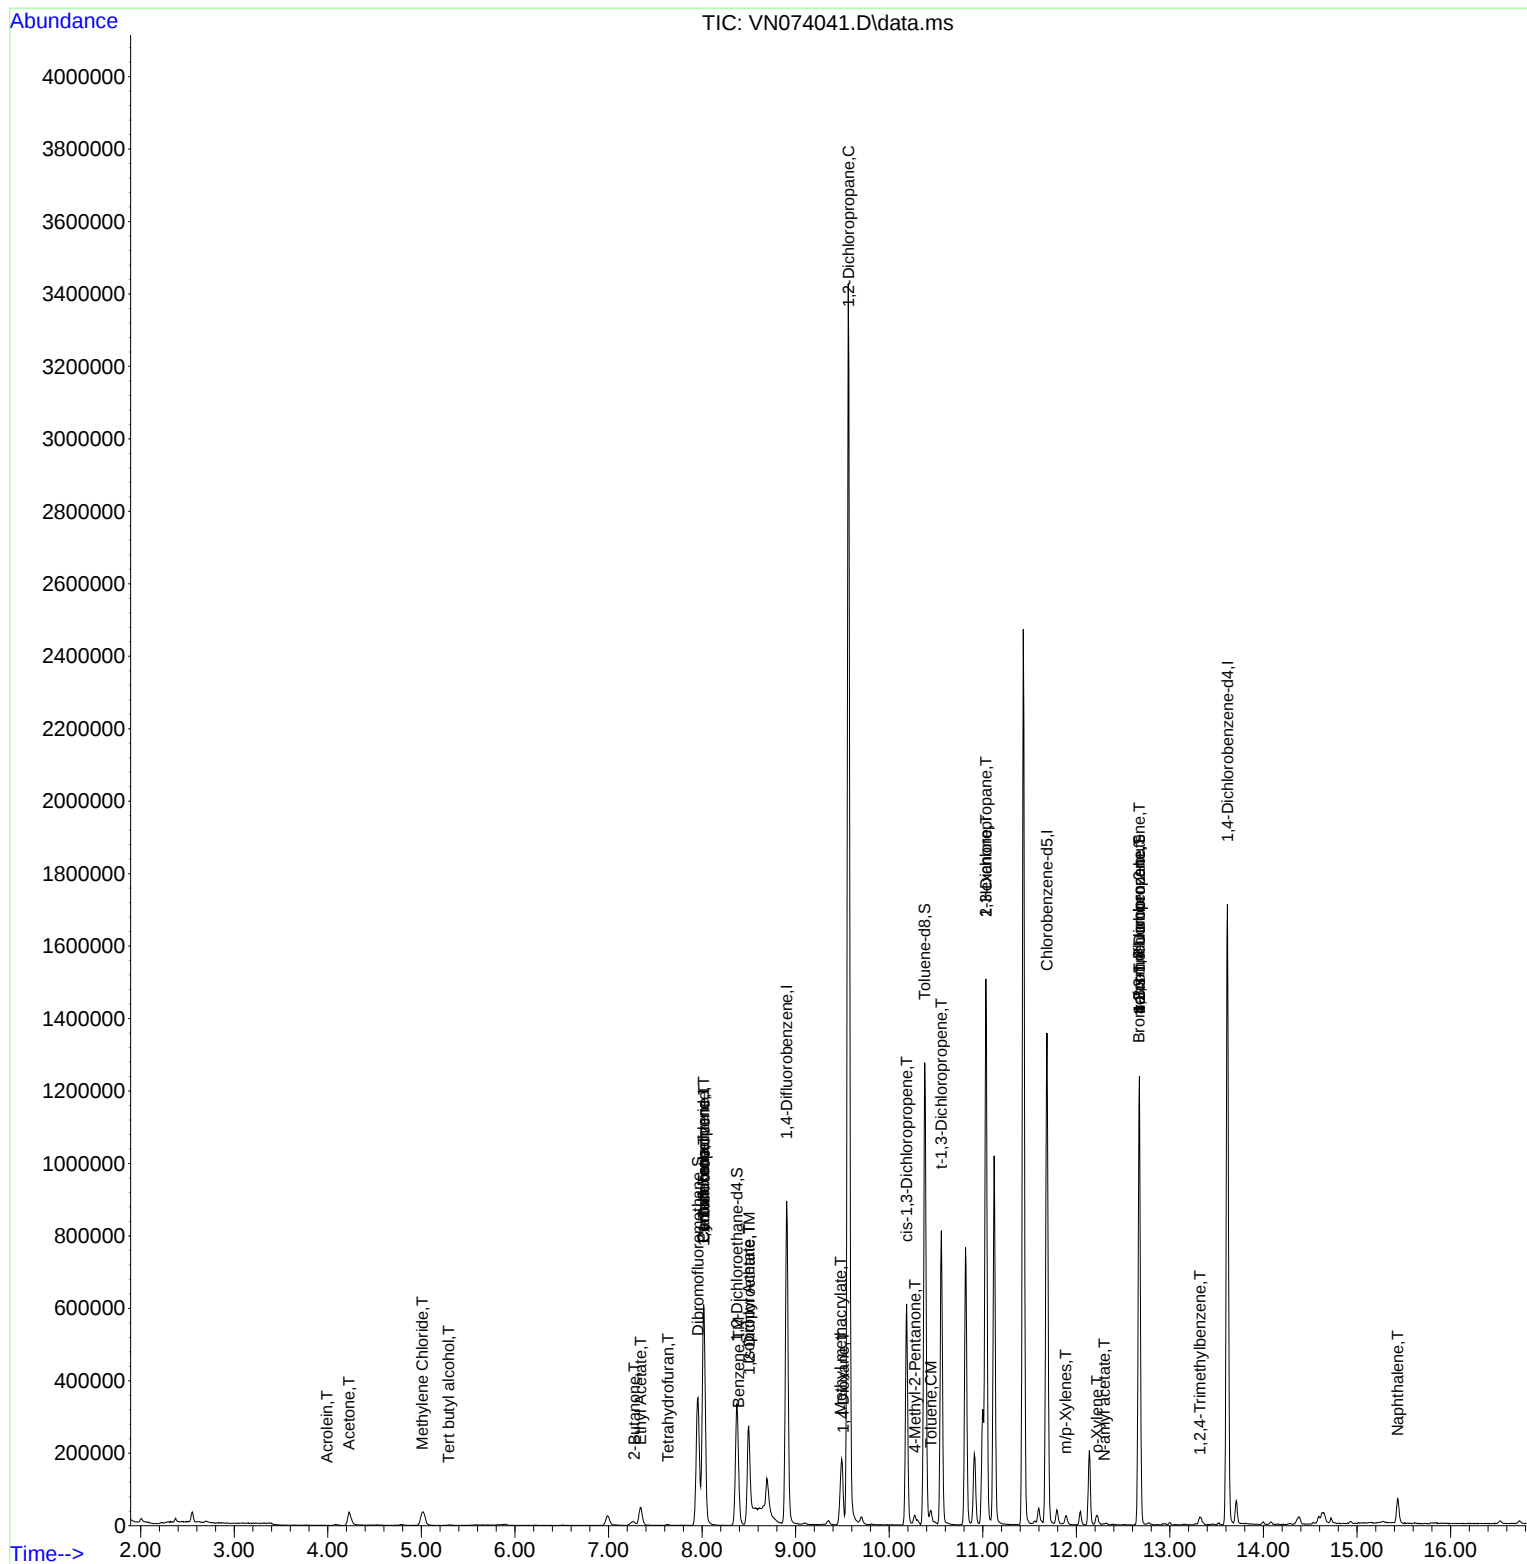




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion:168 Resp: 515674
Ion Ratio Lower Upper
168 100
99 50.8 42.3 63.5

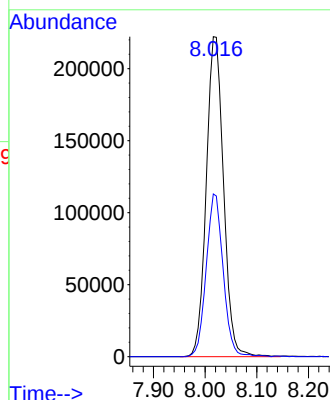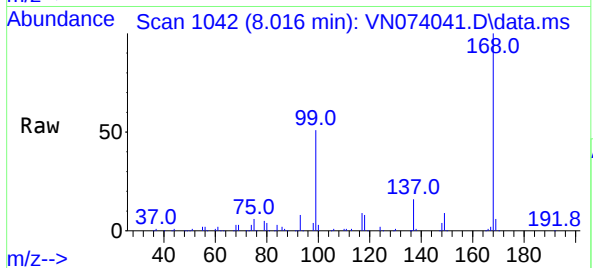

#11
Tert butyl alcohol
Concen: 1.755 ug/l
RT: 5.292 min Scan# 579
Delta R.T. 0.000 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion: 59 Resp: 1972
Ion Ratio Lower Upper
59 100
57 2.8 8.3 12.5#

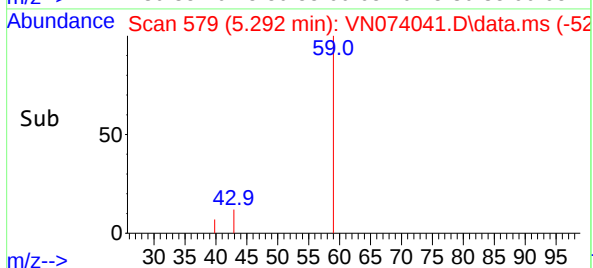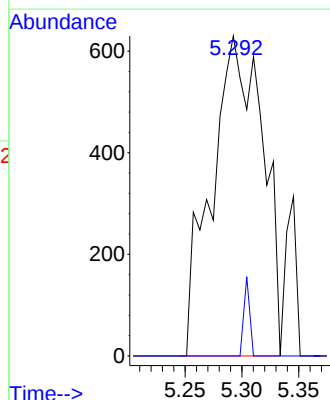



#13

Acrolein

Concen: 0.500 ug/l

RT: 3.993 min Scan# 3

Delta R.T. 0.012 min

Lab File: VN074041.D

Acq: 19 Aug 2022 21:10

Instrument :

MSVOA_N

ClientSampleId :





SB-4

Tgt Ion: 56 Resp: 393

Ion Ratio Lower Upper

56 100

55 78.9 54.8 82.2

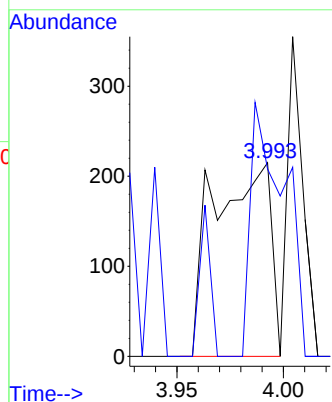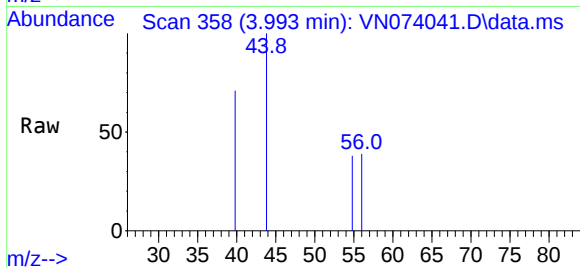

#16

Acetone

Concen: 26.551 ug/l

RT: 4.228 min Scan# 398

Delta R.T. 0.006 min

Lab File: VN074041.D




Acq: 19 Aug 2022 21:10


Tgt Ion: 43 Resp: 62916

Ion Ratio Lower Upper

43 100

58 33.8 26.0 39.0




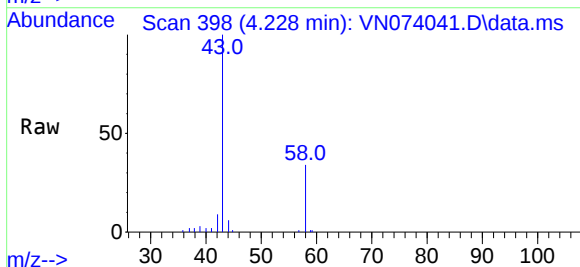




#18
Methyl Acetate
Concen: Below Cal
RT: 4.787 min Scan# 493
Delta R.T. 0.006 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 43 Resp: 5343
Ion Ratio Lower Upper
43 100
74 25.3 21.6 32.4

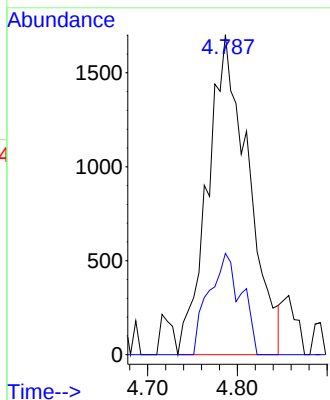

#20
Methylene Chloride
Concen: 6.864 ug/l
RT: 5.010 min Scan# 531
Delta R.T. 0.000 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion: 84 Resp: 34321
Ion Ratio Lower Upper
84 100
49 96.0 88.3 132.5
51 31.3 28.2 42.2
86 62.3 50.6 76.0



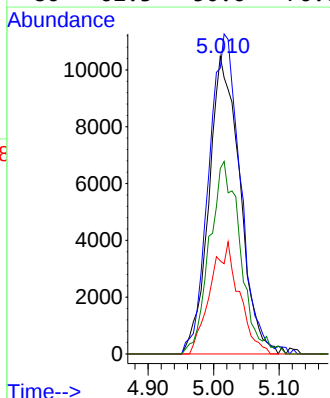





#25
2-Butanone
Concen: 3.489 ug/l
RT: 7.275 min Scan# 913
Delta R.T. 0.018 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 43 Resp: 13110
Ion Ratio Lower Upper
43 100
72 22.9 23.7 35.5#

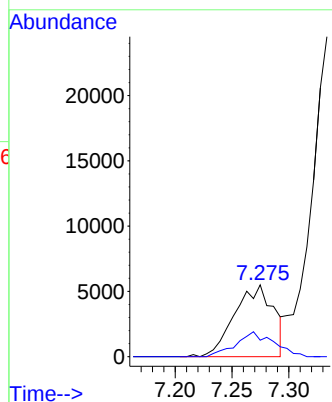

#29
Tetrahydrofuran
Concen: 0.707 ug/l
RT: 7.634 min Scan# 977
Delta R.T. 0.024 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion: 42 Resp: 1703
Ion Ratio Lower Upper
42 100
72 28.5 39.7 59.5#
71 22.1 36.6 55.0#


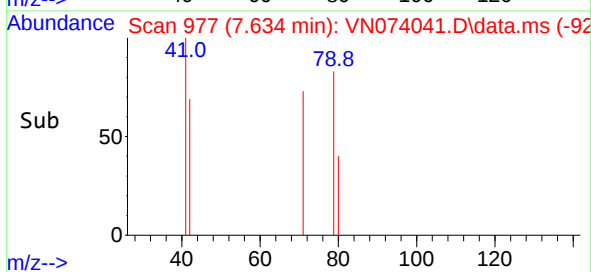






#31
Cyclohexane
Concen: 1.246 ug/l
RT: 8.016 min Scan# 1103
Delta R.T. -0.006 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 56 Resp: 8727
Ion Ratio Lower Upper
56 100
69 155.5 27.8 41.8#
84 144.4 76.9 115.3#

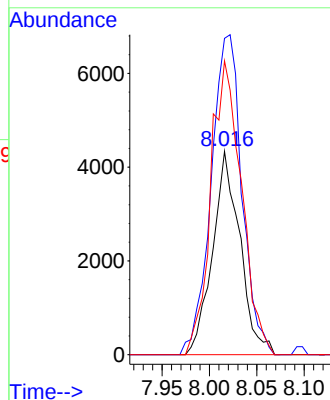

#33
1,2-Dichloroethane-d4
Concen: 55.610 ug/l
RT: 8.375 min Scan# 1103
Delta R.T. 0.006 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion: 65 Resp: 279309
Ion Ratio Lower Upper
65 100
67 52.1 0.0 104.8


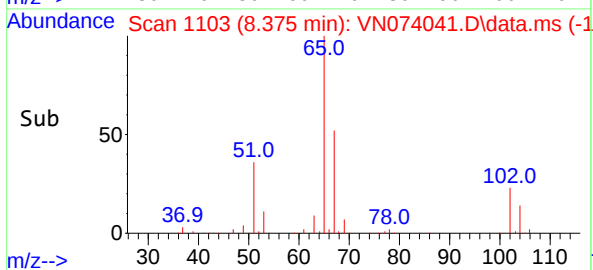
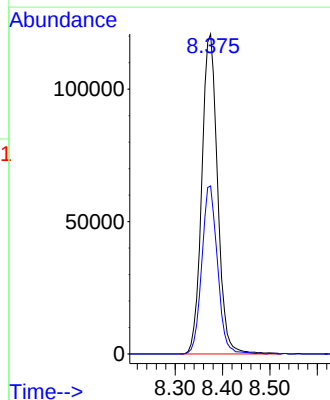



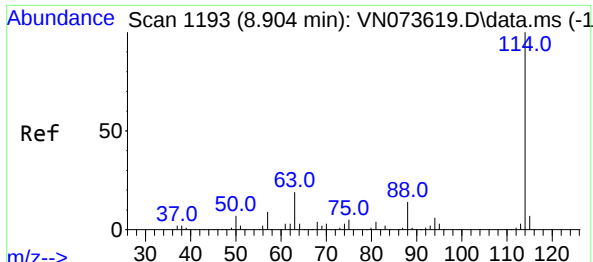

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.904 min Scan# 1193
Delta R.T. 0.000 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion:114 Resp: 821462
Ion Ratio Lower Upper
114 100
63 19.0 0.0 40.0
88 15.6 0.0 32.6

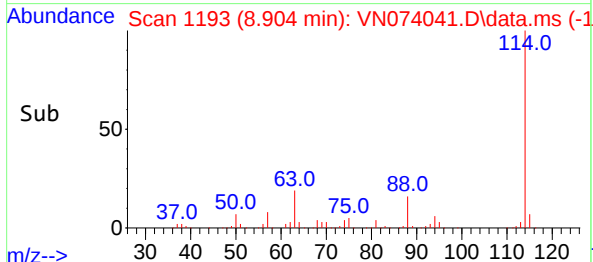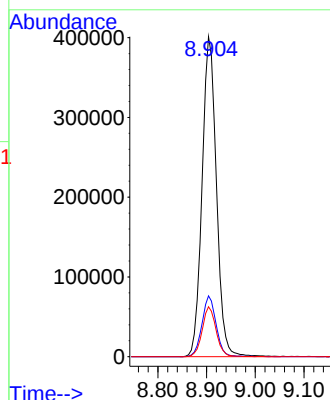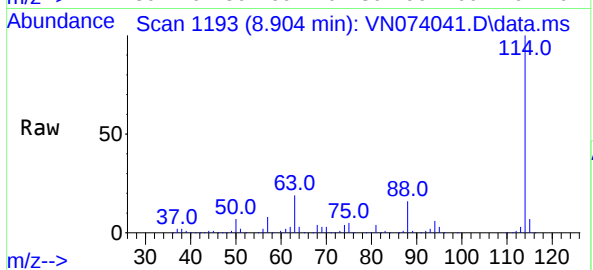

#35
Dibromofluoromethane
Concen: 54.273 ug/l
RT: 7.957 min Scan# 1032
Delta R.T. 0.006 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion:113 Resp: 263660
Ion Ratio Lower Upper
113 100
111 103.6 81.4 122.0
192 22.8 17.0 25.6


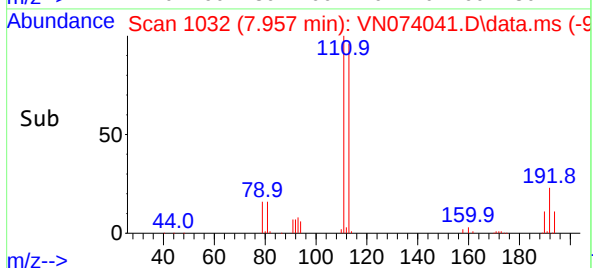
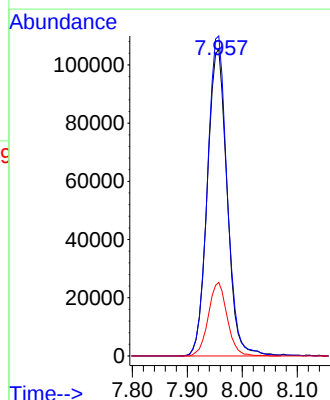





#36
1,1-Dichloropropene
Concen: 5.296 ug/l
RT: 8.022 min Scan# 1043
Delta R.T. -0.129 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 75 Resp: 35738
Ion Ratio Lower Upper
75 100
110 8.8 18.3 54.8#
77 0.0 25.1 37.7#



#37
Ethyl Acetate
Concen: 9.780 ug/l
RT: 7.345 min Scan# 928
Delta R.T. 0.006 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion: 43 Resp: 79952
Ion Ratio Lower Upper
43 100
61 15.2 11.8 17.6
70 11.7 9.3 13.9


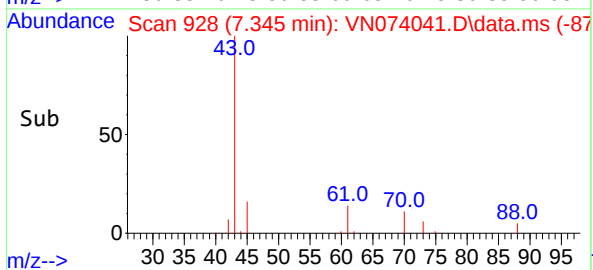






#38
Carbon Tetrachloride
Concen: 6.002 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.117 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion:117 Resp: 46291
Ion Ratio Lower Upper
117 100
119 4.4 75.8 113.8#
121 0.0 24.6 37.0#

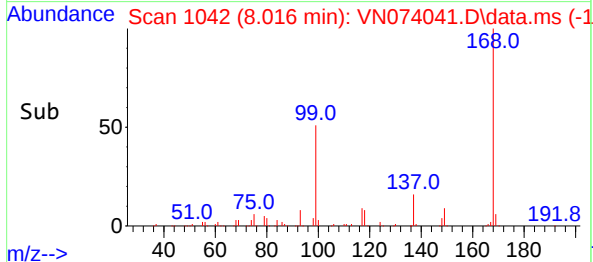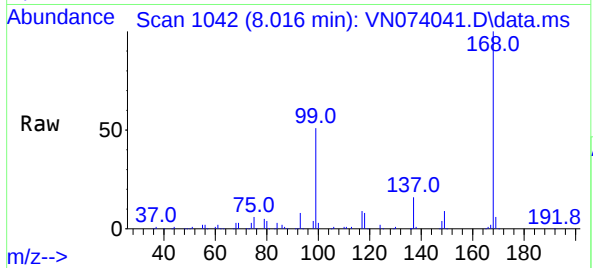

#40
Benzene
Concen: 0.662 ug/l
RT: 8.392 min Scan# 1106
Delta R.T. 0.000 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion: 78 Resp: 14094
Ion Ratio Lower Upper
78 100
77 21.9 19.4 29.0

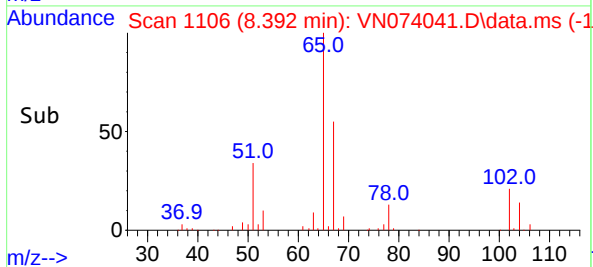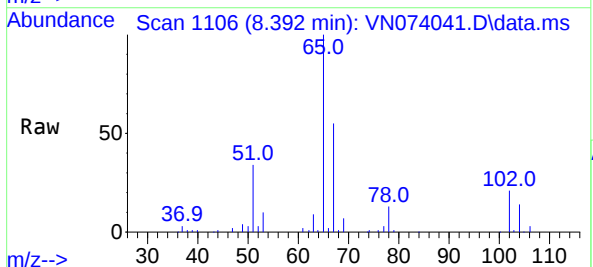



#42

1,2-Dichloroethane

Concen: 0.321 ug/l

RT: 8.504 min Scan# 1118

Delta R.T. 0.041 min

Lab File: VN074041.D

Acq: 19 Aug 2022 21:10

Instrument :

MSVOA_N

ClientSampleId :





SB-4

Tgt Ion: 62 Resp: 2347

Ion Ratio Lower Upper

62 100

98 0.0 0.0 19.4

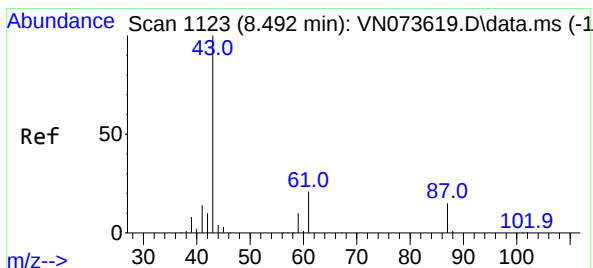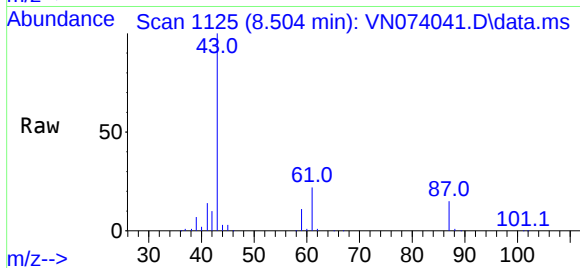

#43

Isopropyl Acetate

Concen: 29.145 ug/l

RT: 8.498 min Scan# 1124

Delta R.T. 0.006 min

Lab File: VN074041.D

Acq: 19 Aug 2022 21:10




Tgt Ion: 43 Resp: 339410


Ion Ratio Lower Upper

43 100

61 19.9 21.9 32.9#

87 13.9 12.0 18.0


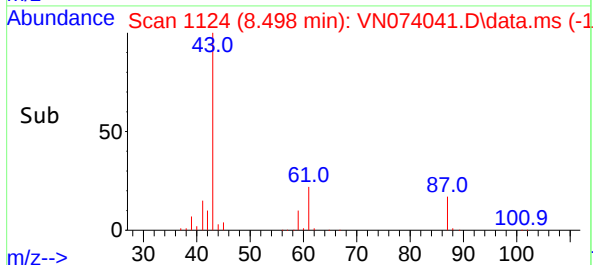
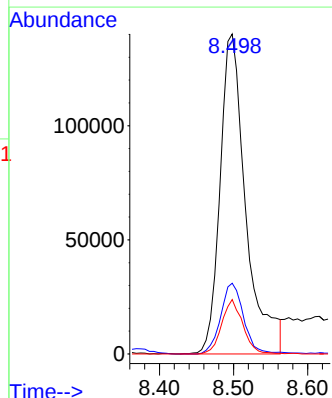
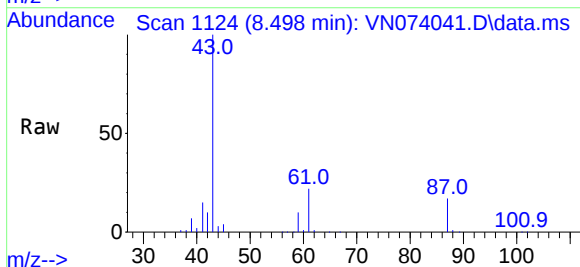




#45
1,2-Dichloropropane
Concen: 0.893 ug/l
RT: 9.569 min Scan# 11
Delta R.T. 0.141 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 63 Resp: 4557
Ion Ratio Lower Upper
63 100
65 0.0 24.9 37.3#

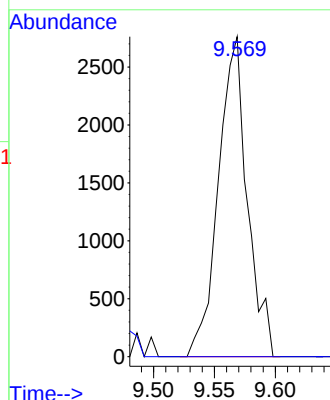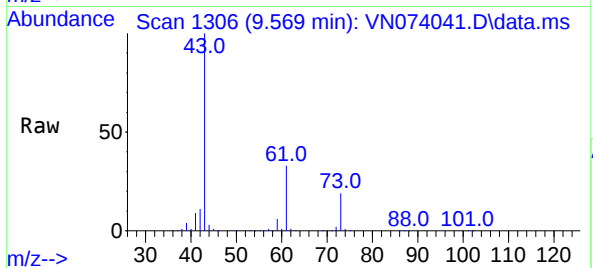

#48
Methyl methacrylate
Concen: 2.467 ug/l
RT: 9.480 min Scan# 1291
Delta R.T. -0.018 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion: 41 Resp: 12294
Ion Ratio Lower Upper
41 100
69 0.0 74.7 112.1#
39 51.2 45.6 68.4


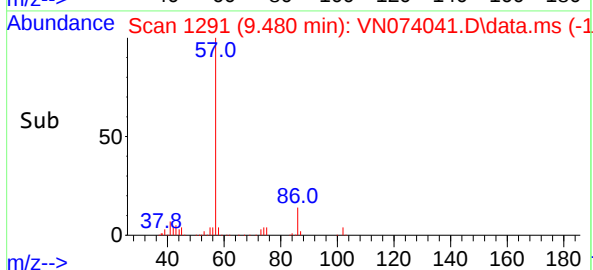
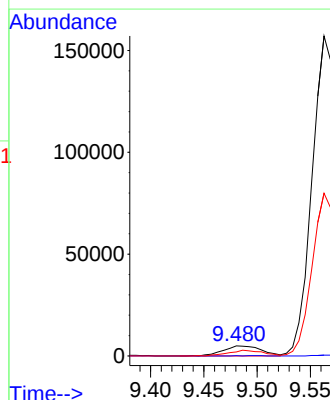





#49
1,4-Dioxane
Concen: 0.378 ug/l
RT: 9.510 min Scan# 1295
Delta R.T. 0.006 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 88 Resp: 56
Ion Ratio Lower Upper
88 100
43 0.0 20.2 30.4#
58 0.0 54.2 81.4#

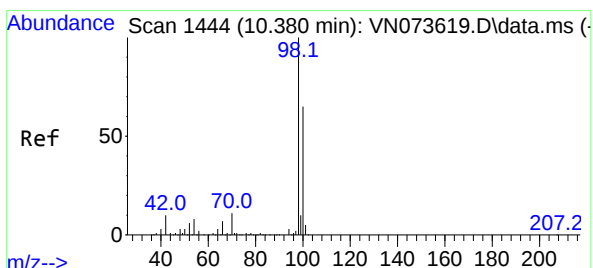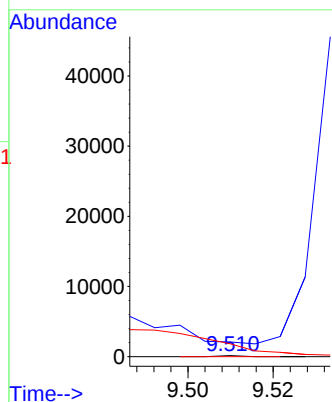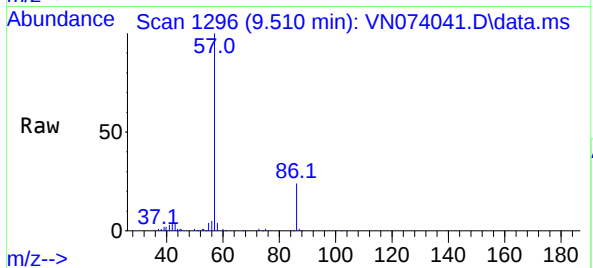

#50
Toluene-d8
Concen: 48.170 ug/l
RT: 10.380 min Scan# 1444
Delta R.T. 0.000 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion: 98 Resp: 906301
Ion Ratio Lower Upper
98 100
100 64.6 52.6 78.8

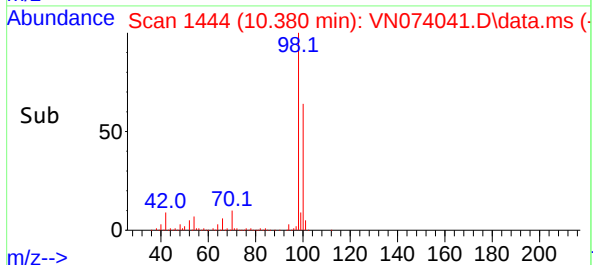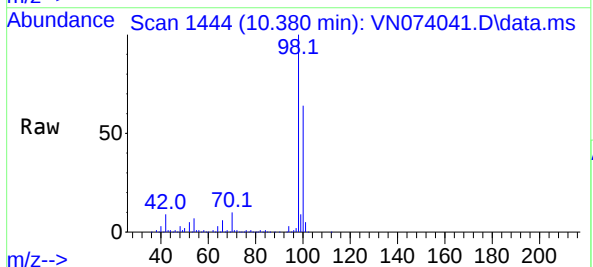



#51

4-Methyl-2-Pentanone

Concen: 3.237 ug/l

RT: 10.275 min Scan# 1426

Delta R.T. -0.000 min

Lab File: VN074041.D

Acq: 19 Aug 2022 21:10

Instrument :

MSVOA_N

ClientSampleId :





SB-4

Tgt Ion: 43 Resp: 25483

Ion Ratio Lower Upper

43 100

58 28.4 34.1 51.1#

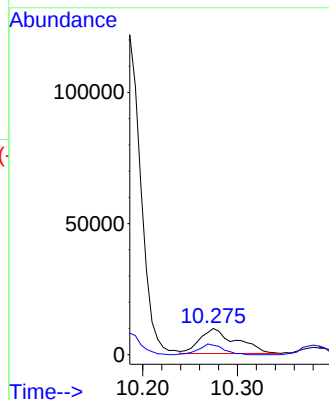

#52

Toluene

Concen: 1.139 ug/l

RT: 10.445 min Scan# 1455

Delta R.T. 0.000 min

Lab File: VN074041.D




Acq: 19 Aug 2022 21:10


Tgt Ion: 92 Resp: 16628

Ion Ratio Lower Upper

92 100

91 165.3 138.6 207.8


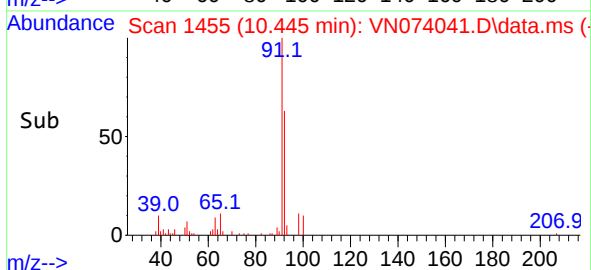
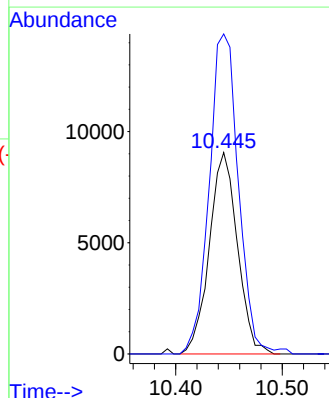





#53
t-1,3-Dichloropropene
Concen: 0.321 ug/l
RT: 10.557 min Scan# 1410
Delta R.T. -0.106 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 75 Resp: 2495
Ion Ratio Lower Upper
75 100
77 42.1 25.6 38.4#

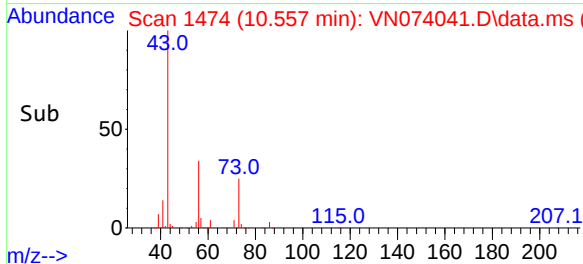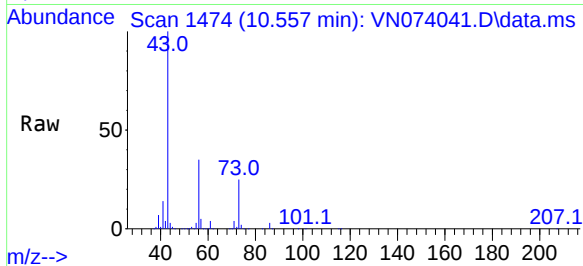

#54
cis-1,3-Dichloropropene
Concen: 13.642 ug/l
RT: 10.186 min Scan# 1411
Delta R.T. 0.059 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion: 75 Resp: 116180
Ion Ratio Lower Upper
75 100
77 0.5 25.2 37.8#
39 27.3 35.7 53.5#

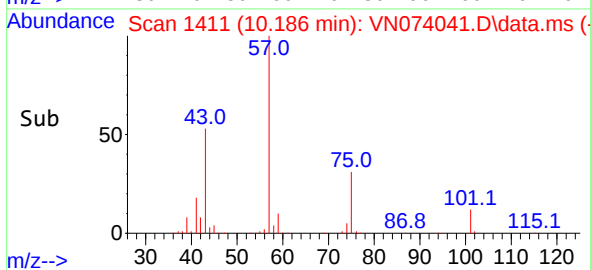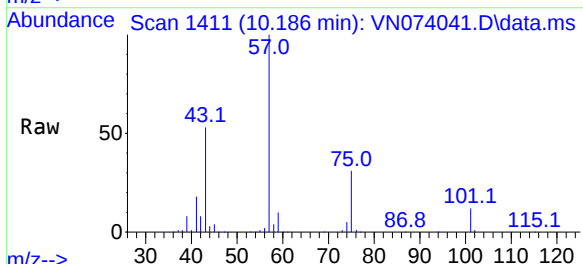

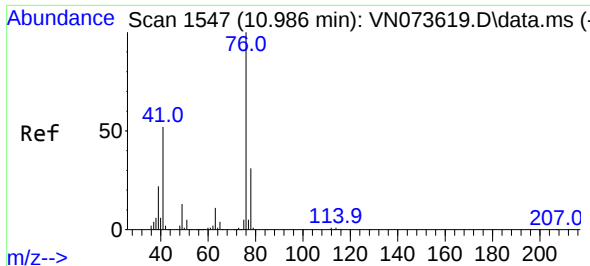

#57

1,3-Dichloropropane

Concen: 1.817 ug/l

RT: 11.033 min Scan# 1555

Delta R.T. 0.047 min

Lab File: VN074041.D

Acq: 19 Aug 2022 21:10

Instrument :

MSVOA_N

ClientSampleId :





SB-4

Tgt Ion: 76 Resp: 16785

Ion Ratio Lower Upper

76 100

78 0.0 26.2 39.2#

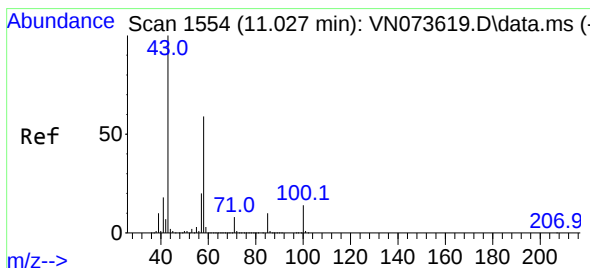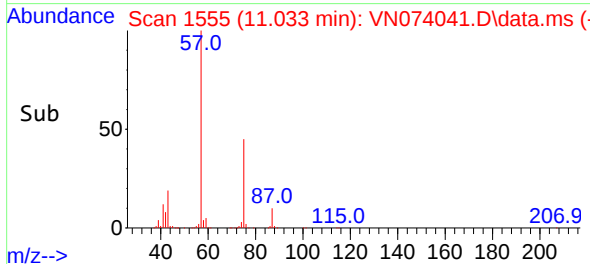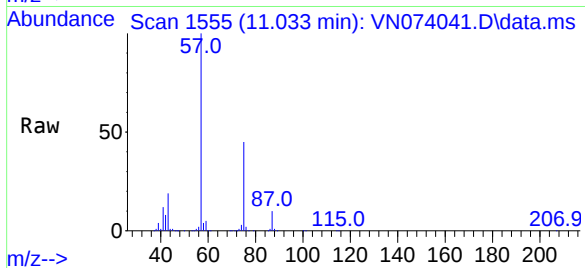

#59

2-Hexanone

Concen: 33.155 ug/l

RT: 11.033 min Scan# 1555

Delta R.T. 0.006 min

Lab File: VN074041.D




Acq: 19 Aug 2022 21:10


Tgt Ion: 43 Resp: 200904

Ion Ratio Lower Upper

43 100

58 21.7 29.7 89.1#


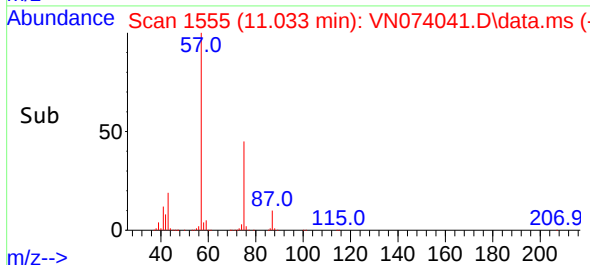
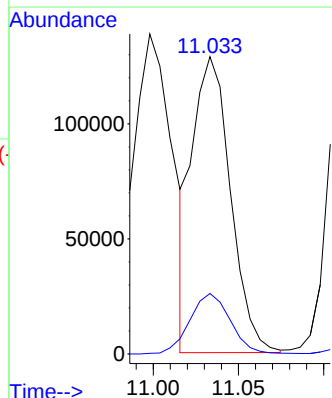
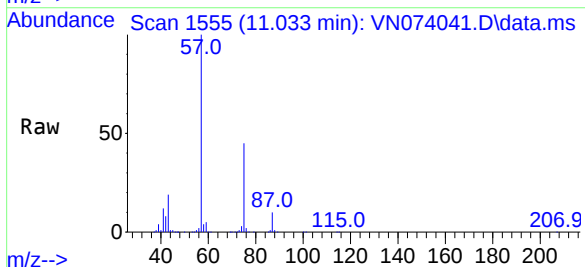




#62
4-Bromofluorobenzene
Concen: 65.126 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.000 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 95 Resp: 406664
Ion Ratio Lower Upper
95 100
174 90.5 0.0 167.6
176 87.0 0.0 163.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. 0.000 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion: 117 Resp: 845121
Ion Ratio Lower Upper
117 100
82 53.0 44.2 66.2
119 31.8 25.4 38.0


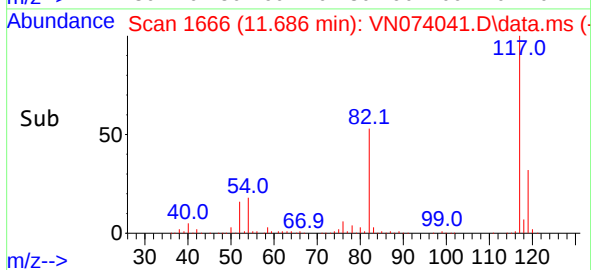






#68
m/p-Xylenes
Concen: 0.650 ug/l
RT: 11.886 min Scan# 11
Delta R.T. -0.012 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion:106 Resp: 7893
Ion Ratio Lower Upper
106 100
91 203.6 158.9 238.3

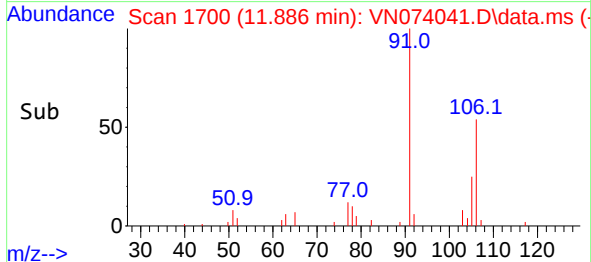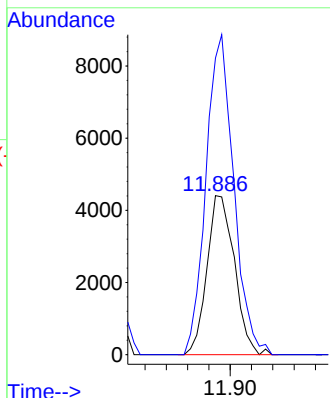

#69
o-Xylene
Concen: 0.412 ug/l
RT: 12.221 min Scan# 1757
Delta R.T. 0.000 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion:106 Resp: 5011
Ion Ratio Lower Upper
106 100
91 215.7 106.0 318.0



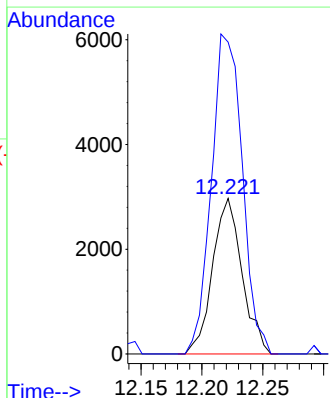





#71
Bromoform
Concen: 0.317 ug/l
RT: 12.668 min Scan# 1833
Delta R.T. 0.270 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion:173 Resp: 1925
Ion Ratio Lower Upper
173 100
175 0.0 24.6 73.6#
254 0.0 0.1 0.1#

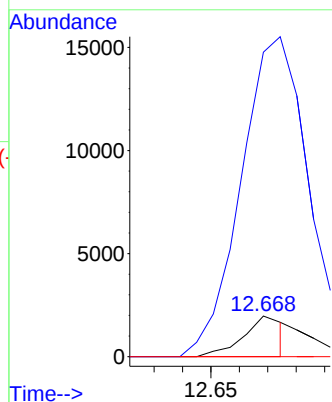

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.615 min Scan# 1994
Delta R.T. 0.000 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion:152 Resp: 505065
Ion Ratio Lower Upper
152 100
115 55.1 28.9 86.7
150 155.0 0.0 356.2


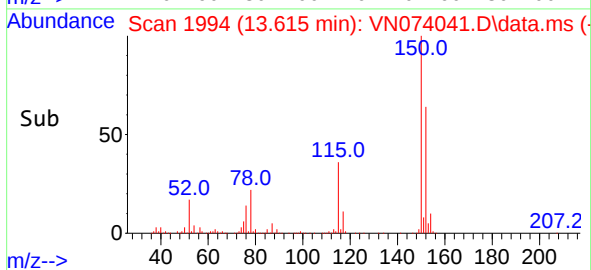






#74
N-amy1 acetate
Concen: 0.278 ug/l
RT: 12.298 min Scan# 11
Delta R.T. -0.029 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 43 Resp: 3863
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.4#
55 2.8 21.1 31.7#
61 0.0 21.1 31.7#

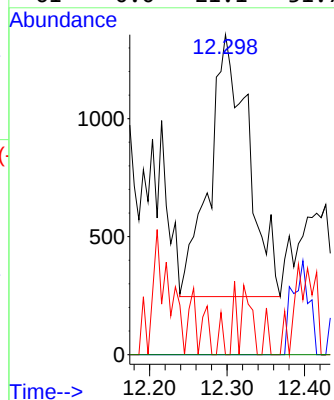

#76
1,2,3-Trichloropropane
Concen: 18.883 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. -0.147 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion: 75 Resp: 198233
Ion Ratio Lower Upper
75 100
77 1.3 98.5 295.5#


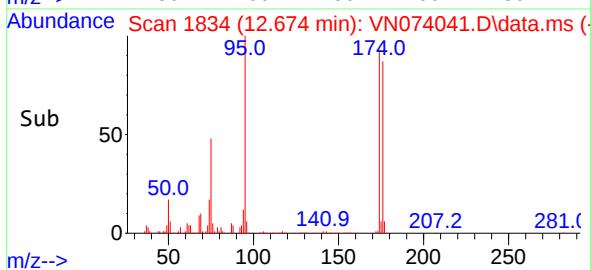
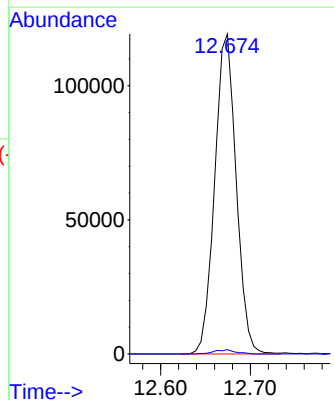





#81
trans-1,4-Dichloro-2-butene
Concen: 53.708 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.106 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10




Instrument :
MSVOA_N
ClientSampleId :
SB-4


Tgt Ion: 75 Resp: 198233
Ion Ratio Lower Upper
75 100
53 0.2 78.0 117.0#
89 0.0 37.2 55.8#



#84
1,2,4-Trimethylbenzene
Concen: 0.446 ug/l
RT: 13.321 min Scan# 1944
Delta R.T. 0.011 min
Lab File: VN074041.D
Acq: 19 Aug 2022 21:10

Tgt Ion: 105 Resp: 13314
Ion Ratio Lower Upper
105 100
120 15.5 23.3 69.8#

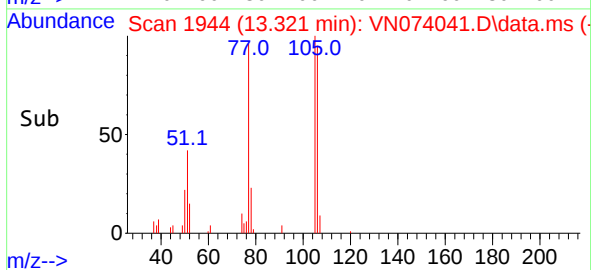



#95

Naphthalene

Concen: 1.768 ug/l

RT: 15.433 min Scan# 21

Delta R.T. 0.000 min

Lab File: VN074041.D


Acq: 19 Aug 2022 21:10

Instrument :

MSVOA_N

ClientSampleId :

SB-4



Tgt Ion:128 Resp: 62549

Ion Ratio Lower Upper

128 100

127 13.0 10.3 15.5

129 11.1 8.6 13.0

