

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN082018\
 Data File : VN050777.D
 Acq On : 20 Aug 2018 16:24
 Operator : MD\SY
 Sample : PB112183ZHE#04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB112183ZHE#04

Quant Time: Aug 21 03:31:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 14 08:07:08 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	648551	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1073947	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	886697	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	270795	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	8.03	65	435796	53.31	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.62%	
35) Dibromofluoromethane	7.59	113	407532	47.53	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.06%	
50) Toluene-d8	10.09	98	1468331	45.50	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.00%	
62) 4-Bromofluorobenzene	12.40	95	371325	34.83	ug/l	0.00
Spiked Amount	50.000		Recovery	=	69.66%	

Target Compounds


						Qvalue
3) Chloromethane	2.06	50	2625	Below Cal		93
5) Bromomethane	2.57	94	2886	Below Cal		91
6) Chloroethane	2.70	64	97	Below Cal	#	43
10) Methyl Iodide	3.97	142	260	6.99	ug/l #	88
16) Acetone	3.83	43	17944	7.38	ug/l	99
18) Methyl Acetate	4.33	43	15278	1.70	ug/l #	79
20) Methylene Chloride	4.55	84	38026	3.72	ug/l	97
25) 2-Butanone	6.85	43	3213	0.96	ug/l	98
29) Tetrahydrofuran	7.22	42	739	0.42	ug/l #	49
31) Cyclohexane	7.66	56	11524	0.59	ug/l #	1
36) 1,1-Dichloropropene	7.67	75	44650	3.73	ug/l #	48
38) Carbon Tetrachloride	7.67	117	57870	4.67	ug/l #	17
43) Isopropyl Acetate	8.17	43	300511	24.40	ug/l	95
48) Methyl methacrylate	9.18	41	6918	1.12	ug/l #	22
51) 4-Methyl-2-Pentanone	9.99	43	1979	0.24	ug/l	95
56) Ethyl methacrylate	10.23	69	2352	2.12	ug/l #	65
59) 2-Hexanone	10.77	43	18168	3.38	ug/l #	57
70) Styrene	11.97	104	268	0.95	ug/l #	51
71) Bromoform	12.41	173	1878	0.34	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	12.40	83	213	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.40	75	175402	39.88	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.73	105	4211	0.25	ug/l	94
81) trans-1,4-Dichloro-2-buten	12.40	75	175402	144.00	ug/l #	13
95) Naphthalene	15.13	128	233	3.88	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN082018\
Data File : VN050777.D
Acq On : 20 Aug 2018 16:24
Operator : MD\SY
Sample : PB112183ZHE#04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB112183ZHE#04

Quant Time: Aug 21 03:31:48 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
Quant Title : SW846 8260
QLast Update : Tue Aug 14 08:07:08 2018
Response via : Initial Calibration





#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1891

Delta R.T. 0.00 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24

Instrument :

MSVOA_N

ClientSampleId :


PB112183ZHE#04

Tot Ion:168 Resp: 648551

Ion Ratio Lower Upper

168 100

99 50.3 40.8 61.2



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.67

250000

200000



150000

100000

50000

0

Time-->



#3

Chloromethane

Concen: Below Cal

RT: 2.06 min Scan# 146

Delta R.T. 0.00 min

Lab File: VN050777.D


Acq: 20 Aug 2018 16:24

Tgt Ion: 50 Resp: 2625

Ion Ratio Lower Upper

50 100

52 36.7 26.0 39.0



Abundance Ion 49.90 (49.60 to 50.60): VNO

Ion 51.90 (51.60 to 52.60): VNO

2000


1500


1000

500

0

Time-->





#5

Bromomethane

Concen: Below Cal

RT: 2.57 min Scan# 305

Delta R.T. 0.01 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24

Instrument :

MSVOA_N

ClientSampleId :


PB112183ZHE#04

Tot Ion: 94 Resp: 2886

Ion Ratio Lower Upper




94 100

96 101.5 74.0 111.0



Abundance Ion 93.90 (93.60 to 94.60): VN0

Ion 95.90 (95.60 to 96.60): VN0



#6

Chloroethane

Concen: Below Cal

RT: 2.70 min Scan# 344

Delta R.T. -0.00 min

Lab File: VN050777.D


Acq: 20 Aug 2018 16:24

Tgt Ion: 64 Resp: 97

Ion Ratio Lower Upper



64 100


66 0.0 25.7 38.5#



Abundance Ion 63.90 (63.60 to 64.60): VN0

Ion 65.90 (65.60 to 66.60): VN0









#10
Methvl Iodide
Concen: 6.99 ug/l
RT: 3.97 min Scan# 741
Delta R.T. 0.02 min
Lab File: VN050777.D
Acq: 20 Aug 2018 16:24




Instrument :
MSVOA_N
ClientSampleId :
PB112183ZHE#04


Tot Ion:142 Resp: 260
Ion Ratio Lower Upper
142 100
127 38.1 32.6 49.0
141 0.0 11.5 17.3#



#16
Acetone
Concen: 7.38 ug/l
RT: 3.83 min Scan# 696
Delta R.T. 0.01 min
Lab File: VN050777.D
Acq: 20 Aug 2018 16:24

Tgt Ion: 43 Resp: 17944
Ion Ratio Lower Upper
43 100
58 33.1 27.1 40.7









#18
Methyl Acetate
Concen: 1.70 ug/l
RT: 4.33 min Scan# 853
Delta R.T. 0.01 min
Lab File: VN050777.D
Acq: 20 Aug 2018 16:24




Instrument :
MSVOA_N
ClientSampleId :
PB112183ZHE#04


Tot Ion: 43 Resp: 15278
Ion Ratio Lower Upper
43 100
74 14.1 19.7 29.5#



#20
Methylene Chloride
Concen: 3.72 ug/l
RT: 4.55 min Scan# 921
Delta R.T. 0.00 min
Lab File: VN050777.D
Acq: 20 Aug 2018 16:24

Tgt Ion: 84 Resp: 38026
Ion Ratio Lower Upper
84 100
49 118.8 92.6 138.8
51 35.1 28.6 43.0
86 61.2 52.2 78.2









#25
2-Butanone
Concen: 0.96 ug/l
RT: 6.85 min Scan# 1636
Delta R.T. 0.01 min
Lab File: VN050777.D
Acq: 20 Aug 2018 16:24




Instrument :
MSVOA_N
ClientSampleId :
PB112183ZHE#04


Tot Ion: 43 Resp: 3213
Ion Ratio Lower Upper
43 100
72 26.2 21.8 32.6



#29
Tetrahydrofuran
Concen: 0.42 ug/l
RT: 7.22 min Scan# 1751
Delta R.T. 0.01 min
Lab File: VN050777.D
Acq: 20 Aug 2018 16:24

Tgt Ion: 42 Resp: 739
Ion Ratio Lower Upper
42 100
72 8.3 35.8 53.6#
71 12.7 33.4 50.0#









#31
Cyclohexane
Concen: 0.59 ug/l
RT: 7.66 min Scan# 1889
Delta R.T. 0.01 min
Lab File: VN050777.D
Acq: 20 Aug 2018 16:24

Instrument :
MSVOA_N
ClientSampleId :
PB112183ZHE#04

Tot Ion: 56 Resp: 11524
Ion Ratio Lower Upper
56 100
69 203.6 25.8 38.6#
84 144.9 67.8 101.6#




Abundance Ion 56.00 (55.70 to 56.70): VNC
Ion 69.00 (68.70 to 69.70): VNC
Ion 84.00 (83.70 to 84.70): VNC






#33
1,2-Dichloroethane-d4
Concen: 53.31 ug/l
RT: 8.03 min Scan# 2003
Delta R.T. 0.00 min
Lab File: VN050777.D
Acq: 20 Aug 2018 16:24

Tgt Ion: 65 Resp: 435796
Ion Ratio Lower Upper
65 100
67 54.1 0.0 109.8



Abundance Ion 64.90 (64.60 to 65.60): VNC
Ion 66.90 (66.60 to 67.60): VNC









#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2176
 Delta R.T. -0.00 min
 Lab File: VN050777.D
 Acq: 20 Aug 2018 16:24

Instrument :
 MSVOA_N
 ClientSampleId :
 PB112183ZHE#04

Tot Ion:114 Resp: 1073947
 Ion Ratio Lower Upper
 114 100
 63 19.8 0.0 40.0
 88 15.3 0.0 30.8




Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN






#35
 Dibromofluoromethane
 Concen: 47.53 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. -0.00 min
 Lab File: VN050777.D
 Acq: 20 Aug 2018 16:24

Tgt Ion:113 Resp: 407532
 Ion Ratio Lower Upper
 113 100
 111 102.6 81.0 121.6
 192 22.5 17.6 26.4



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V







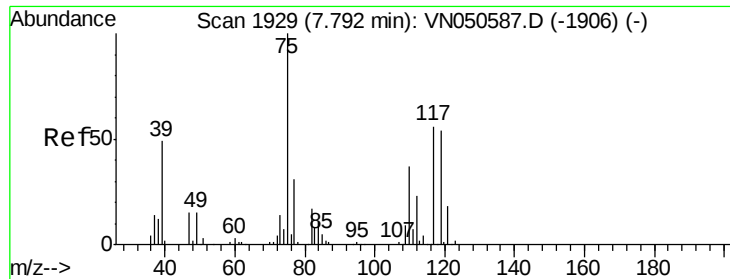

#36
 1,1-Dichloropropene
 Concen: 3.73 ug/l
 RT: 7.67 min Scan# 1891
 Delta R.T. -0.12 min
 Lab File: VN050777.D
 Acq: 20 Aug 2018 16:24




Instrument :
 MSVOA_N
 ClientSampleId :
 PB112183ZHE#04


Tot Ion	Ratio	Lower	Upper
75	100		
110	8.1	18.3	54.9#
77	0.0	25.0	37.4#



#38
 Carbon Tetrachloride
 Concen: 4.67 ug/l
 RT: 7.67 min Scan# 1890
 Delta R.T. -0.11 min
 Lab File: VN050777.D
 Acq: 20 Aug 2018 16:24

Tgt Ion	Ratio	Lower	Upper
117	100		
119	6.4	76.6	115.0#
121	0.0	25.0	37.6#





#43

Isopropyl Acetate

Concen: 24.40 ug/l

RT: 8.17 min Scan# 2046

Delta R.T. 0.00 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24

Instrument :

MSVOA_N

ClientSampleId :

PB112183ZHE#04


Tot Ion: 43 Resp: 300511

Ion Ratio Lower Upper




43 100

61 18.3 16.2 24.2

87 11.4 10.9 16.3



Abundance Ion 43.00 (42.70 to 43.70): VNC
Ion 61.00 (60.70 to 61.70): VNC
Ion 87.00 (86.70 to 87.70): VNC



#48

Methyl methacrylate

Concen: 1.12 ug/l

RT: 9.18 min Scan# 2361

Delta R.T. -0.02 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24


Tgt Ion: 41 Resp: 6918

Ion Ratio Lower Upper



41 100


69 0.0 73.4 110.0#

39 19.5 43.0 64.6#



Abundance Ion 41.00 (40.70 to 41.70): VNC
Ion 69.00 (68.70 to 69.70): VNC
Ion 39.00 (38.70 to 39.70): VNC





#50

Toluene-d8

Concen: 45.50 ug/l

RT: 10.09 min Scan# 2644

Delta R.T. -0.00 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24

Instrument :

MSVOA_N

ClientSampleId :


PB112183ZHE#04

Tot Ion: 98 Resp: 1468331




Ion Ratio Lower Upper

98 100

100 63.5 51.8 77.8



Abundance Ion 98.00 (97.70 to 98.70): VN050587.D (-2627) (-)



#51

4-Methyl-2-Pentanone

Concen: 0.24 ug/l

RT: 9.99 min Scan# 2613

Delta R.T. 0.01 min

Lab File: VN050777.D


Acq: 20 Aug 2018 16:24

Tgt Ion: 43 Resp: 1979



Ion Ratio Lower Upper


43 100

58 44.0 32.5 48.7



Abundance Ion 43.00 (42.70 to 43.70): VN050587.D (-2591) (-)





#56

Ethyl methacrylate

Concen: 2.12 ug/l

RT: 10.23 min Scan# 2687

Delta R.T. -0.20 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24

Instrument :

MSVOA_N

ClientSampleId :

PB112183ZHE#04


Tot Ion: 69 Resp: 2352

Ion Ratio Lower Upper

69 100

41 29.8 49.7 74.5#




39 41.9 24.2 36.2#



Abundance Ion 69.00 (68.70 to 69.70): VN0

Ion 41.00 (40.70 to 41.70): VN0

Ion 39.00 (38.70 to 39.70): VN0



#59

2-Hexanone

Concen: 3.38 ug/l

RT: 10.77 min Scan# 2854

Delta R.T. 0.01 min

Lab File: VN050777.D


Acq: 20 Aug 2018 16:24

Tgt Ion: 43 Resp: 18168

Ion Ratio Lower Upper



43 100


58 24.3 28.0 84.0#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0





#62

4-Bromofluorobenzene

Concen: 34.83 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.00 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24

Instrument :

MSVOA_N

ClientSampleId :

PB112183ZHE#04


Tot Ion: 95 Resp: 371325

Ion Ratio Lower Upper

95 100

174 91.7 0.0 177.8




176 87.3 0.0 175.0



Abundance Ion 94.90 (94.60 to 95.60): VN050777.D (-3269) (-)

Ion 173.80 (173.50 to 174.50): VN050777.D (-3269) (-)

Ion 175.80 (175.50 to 176.50): VN050777.D (-3269) (-)



#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 11.41 min Scan# 3054

Delta R.T. -0.00 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24


Tgt Ion: 117 Resp: 886697

Ion Ratio Lower Upper

117 100

82 53.4 42.4 63.6



119 32.5 25.8 38.8




Abundance Ion 116.90 (116.60 to 117.60): VN050777.D (-2961) (-)

Ion 82.00 (81.70 to 82.70): VN050777.D (-2961) (-)

Ion 118.90 (118.60 to 119.60): VN050777.D (-2961) (-)





#70

Stvrene

Concen: 0.95 ug/l

RT: 11.97 min Scan# 3227

Delta R.T. 0.00 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24

Instrument :

MSVOA_N

ClientSampleId :

PB112183ZHE#04


Tot Ion:104 Resp: 268

Ion Ratio Lower Upper

104 100

78 0.0 39.1 58.7#




103 34.7 44.9 67.3#



Abundance Ion 104.00 (103.70 to 104.70): V

Ion 78.00 (77.70 to 78.70): VN

Ion 103.00 (102.70 to 103.70): V



#71

Bromoform

Concen: 0.34 ug/l

RT: 12.41 min Scan# 3364

Delta R.T. 0.28 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24


Tgt Ion:173 Resp: 1878

Ion Ratio Lower Upper

173 100

175 1096.6 24.4 73.2#



254 0.0 0.0 0.0




Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V



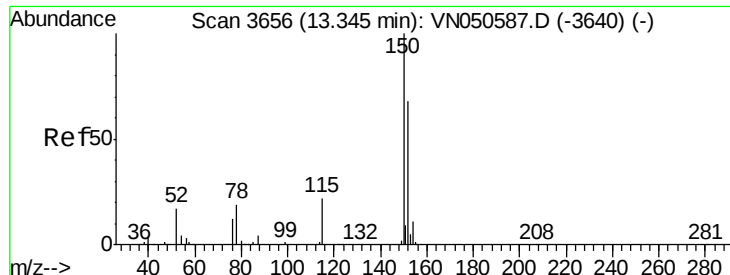

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.35 min Scan# 3656

Delta R.T. -0.00 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24

Instrument :

MSVOA_N

ClientSampleId :

PB112183ZHE#04


Tot Ion:152 Resp: 270795

Ion Ratio Lower Upper

152 100

115 56.4 28.1 84.2




150 156.3 0.0 347.8



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V



#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.40 min Scan# 3363

Delta R.T. -0.10 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24


Tgt Ion: 83 Resp: 213

Ion Ratio Lower Upper

83 100

131 139.4 5.3 15.9#



85 0.0 32.1 96.5#




Abundance Ion 82.90 (82.60 to 83.60): V

Ion 130.80 (130.50 to 131.50): V

Ion 84.90 (84.60 to 85.60): V





#76

1,2,3-Trichloropropane

Concen: 39.88 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. -0.15 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24

Instrument :

MSVOA_N

ClientSampleId :


PB112183ZHE#04

Tot Ion: 75 Resp: 175402

Ion Ratio Lower Upper




75 100

77 1.2 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN050777.D (-3317) (-)

Ion 77.00 (76.70 to 77.70): VN050777.D (-3317) (-)



#80

1,3,5-Trimethylbenzene

Concen: 0.25 ug/l

RT: 12.73 min Scan# 3466

Delta R.T. -0.00 min

Lab File: VN050777.D


Acq: 20 Aug 2018 16:24

Tgt Ion: 105 Resp: 4211

Ion Ratio Lower Upper



105 100


120 53.7 24.7 74.1



Abundance Ion 105.00 (104.70 to 105.70): VN050777.D (-3373) (-)

Ion 120.00 (119.70 to 120.70): VN050777.D (-3373) (-)





#81

trans-1,4-Dichloro-2-butene

Concen: 144.00 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.10 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24

Instrument :

MSVOA_N

ClientSampleId :

PB112183ZHE#04


Tot Ion: 75 Resp: 175402

Ion Ratio Lower Upper

75 100

53 0.2 72.2 108.2#




89 0.0 36.3 54.5#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 53.00 (52.70 to 53.70): VN0

Ion 88.90 (88.60 to 89.60): VN0



#95

Naphthalene

Concen: 3.88 ug/l

RT: 15.13 min Scan# 4212

Delta R.T. 0.00 min

Lab File: VN050777.D

Acq: 20 Aug 2018 16:24


Tgt Ion: 128 Resp: 233

Ion Ratio Lower Upper

128 100

127 0.0 10.3 15.5#

129 0.0 8.5 12.7#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

