


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082018\
Data File : VN050762.D
Acq On : 20 Aug 2018 9:39
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081418W.M
Title : SW846 8260
Last Update : Tue Aug 14 08:07:08 2018

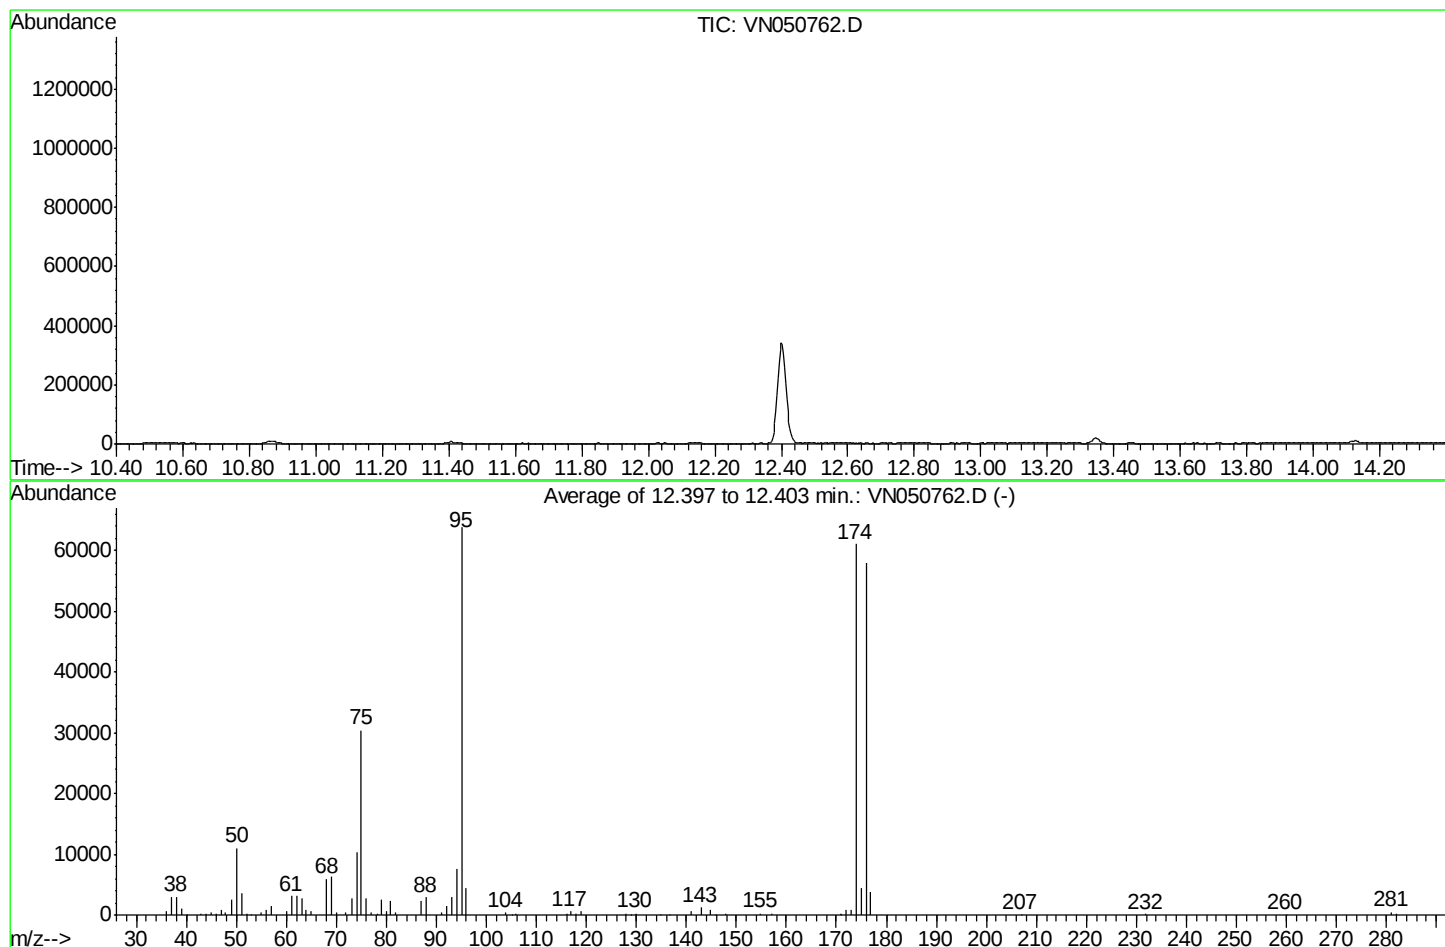

AutoFind: Scans 3361, 3362, 3363; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	11075	PASS
75	95	30	60	47.6	30392	PASS
95	95	100	100	100.0	63850	PASS
96	95	5	9	7.0	4438	PASS
173	174	0.00	2	1.4	874	PASS
174	95	50	100	95.6	61072	PASS
175	174	5	9	7.4	4521	PASS
176	174	95	101	94.9	57968	PASS
177	176	5	9	6.6	3805	PASS