

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN082020\
 Data File : VN063047.D
 Acq On : 20 Aug 2020 20:50
 Operator : JC/MD
 Sample : VN0820WBL02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0820WBL02

Quant Time: Aug 21 06:49:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
 Quant Title : SW846 8260
 QLast Update : Wed Aug 19 06:09:27 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	142978	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	238750	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	242888	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	89555	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.99	65	96455	56.92	ug/l	0.00
Spiked Amount	50.000		Recovery	=	113.84%	
35) Dibromofluoromethane	7.55	113	82548	53.06	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.12%	
50) Toluene-d8	10.06	98	305798	51.18	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.36%	
62) 4-Bromofluorobenzene	12.38	95	101072	47.93	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.86%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN082020\
Data File : VN063047.D
Acq On : 20 Aug 2020 20:50
Operator : JC/MD
Sample : VN0820WBL02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0820WBL02

Quant Time: Aug 21 06:49:23 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
Quant Title : SW846 8260
QLast Update : Wed Aug 19 06:09:27 2020
Response via : Initial Calibration

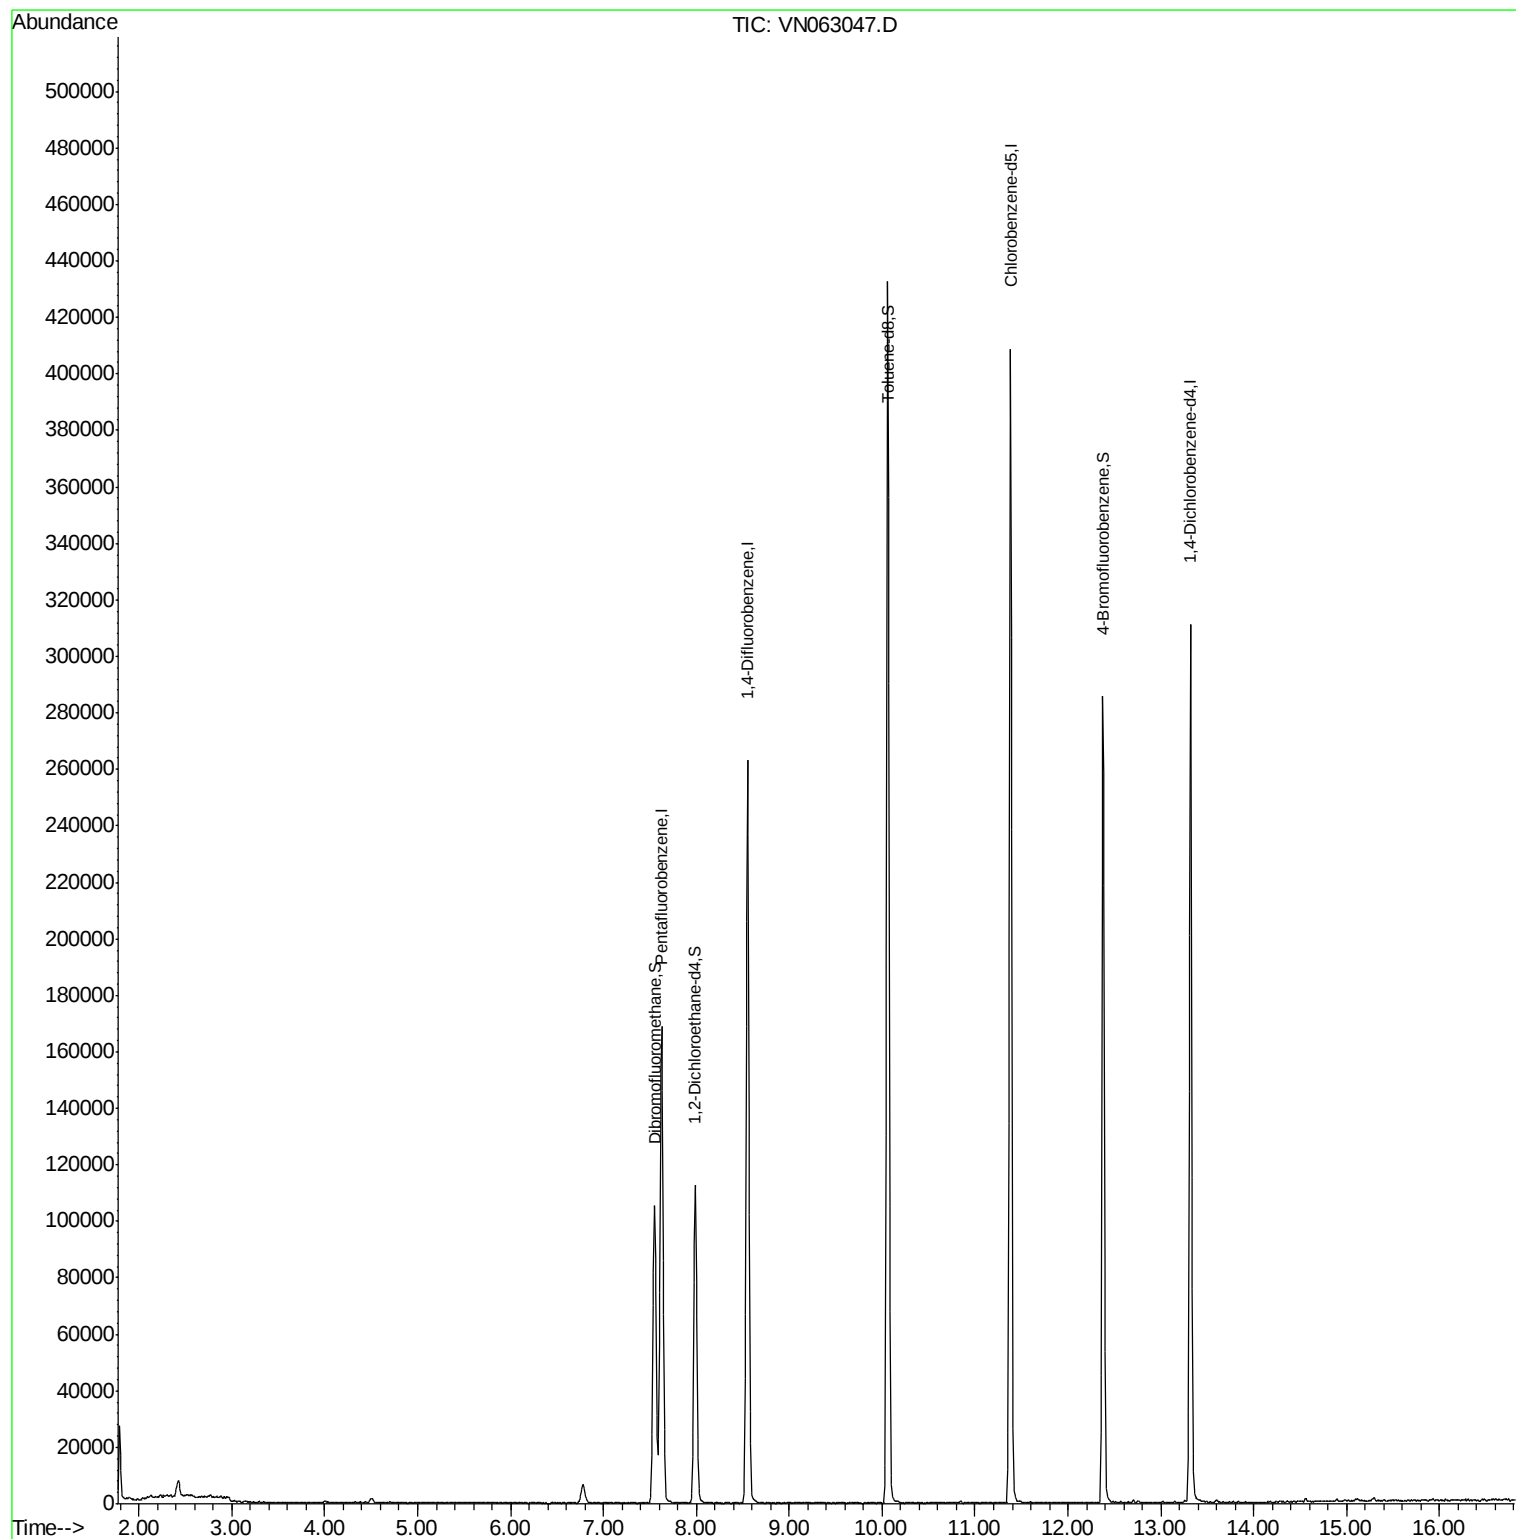

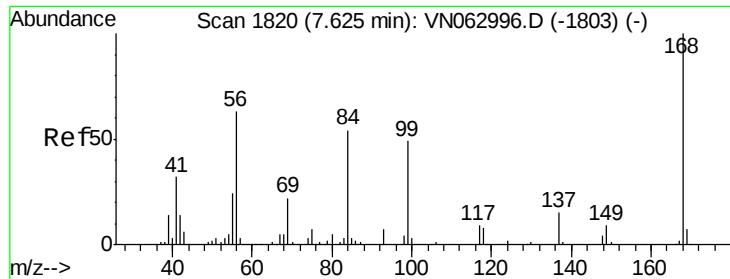

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1821

Delta R.T. 0.00 min

Lab File: VN063047.D

Acq: 20 Aug 2020 20:50

Instrument :

MSVOA_N

ClientSampleId :


VN0820WBL02

Tot Ion:168 Resp: 142978

Ion Ratio Lower Upper




168 100

99 52.9 42.0 63.0

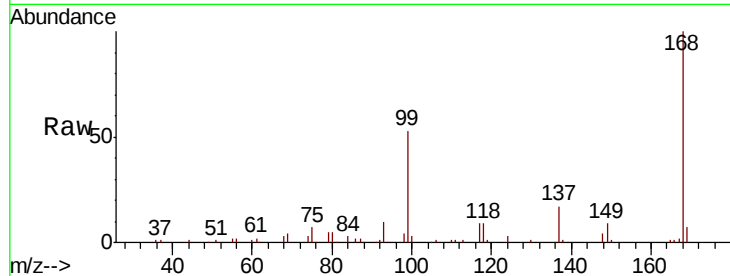

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

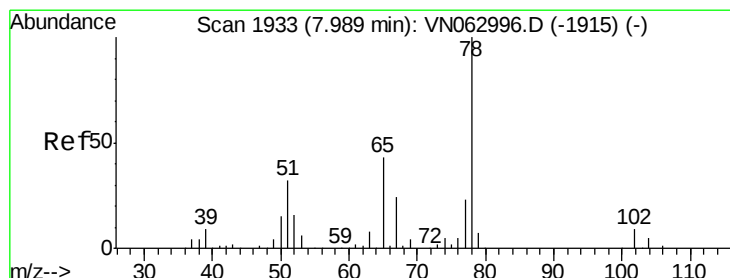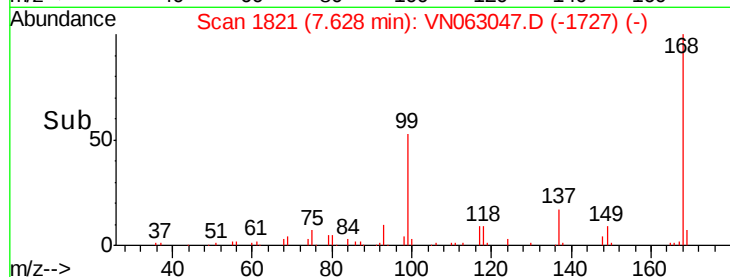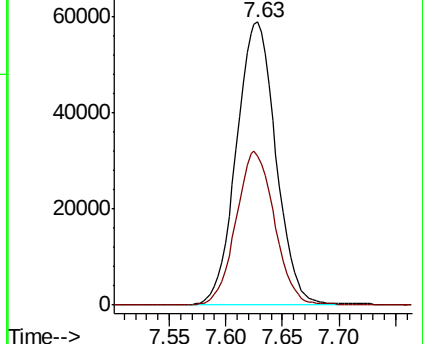

#33

1,2-Dichloroethane-d4

Concen: 56.921 ug/l

RT: 7.99 min Scan# 1933

Delta R.T. -0.00 min

Lab File: VN063047.D


Acq: 20 Aug 2020 20:50

Tgt Ion: 65 Resp: 96455

Ion Ratio Lower Upper



65 100


67 54.1 0.0 112.0

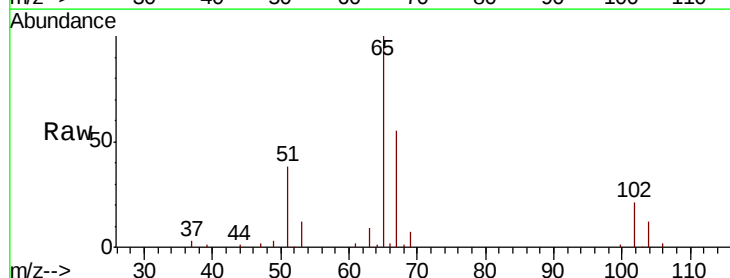

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

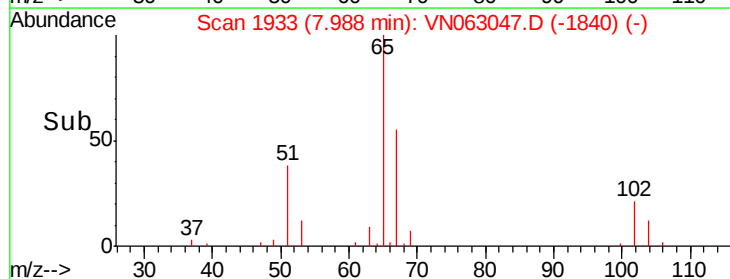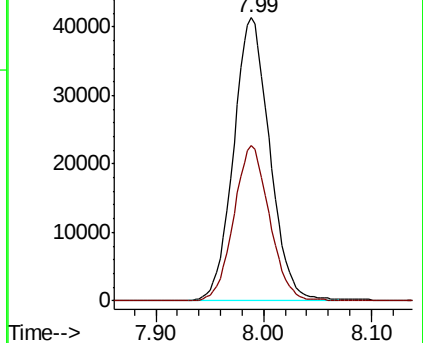


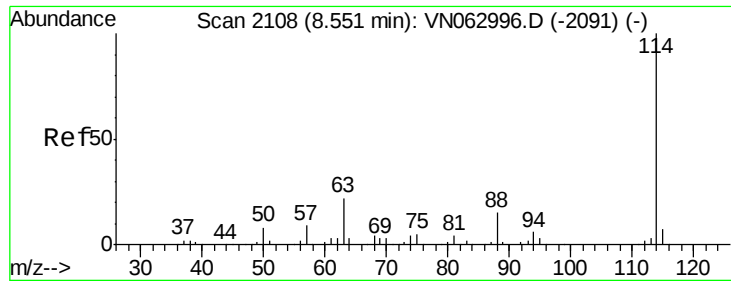




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.55 min Scan# 2108
Delta R.T. -0.00 min
Lab File: VN063047.D
Acq: 20 Aug 2020 20:50

Instrument :
MSVOA_N
ClientSampleId :
VN0820WBL02

Tot Ion:114 Resp: 238750
Ion Ratio Lower Upper
114 100
63 21.1 0.0 43.2
88 15.6 0.0 30.6

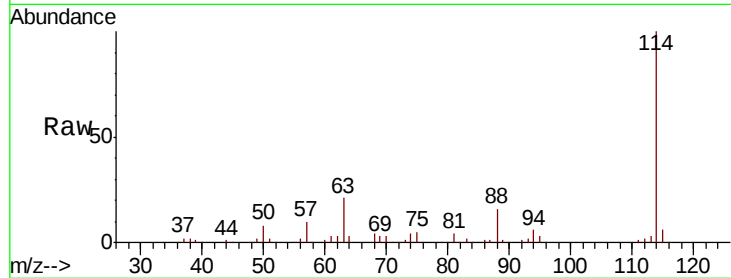


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): V
Ion 87.90 (87.60 to 88.60): V

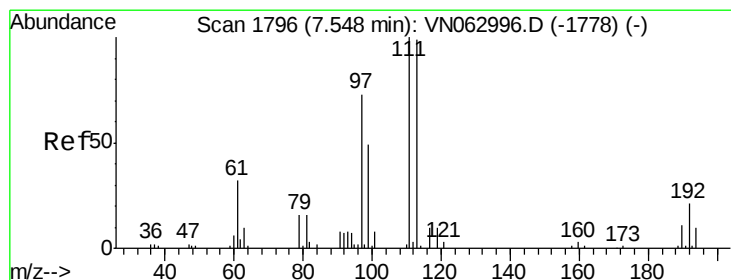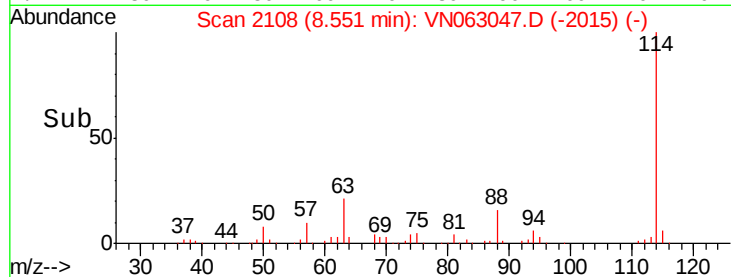
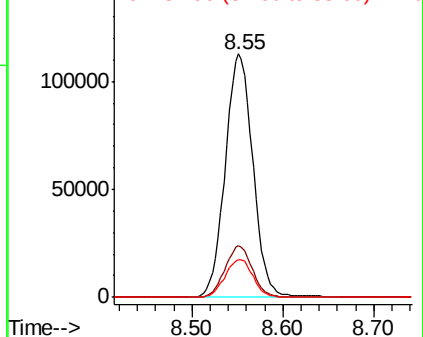



#35
Dibromofluoromethane
Concen: 53.062 ug/l
RT: 7.55 min Scan# 1797
Delta R.T. 0.00 min
Lab File: VN063047.D
Acq: 20 Aug 2020 20:50

Tgt Ion:113 Resp: 82548
Ion Ratio Lower Upper
113 100
111 102.3 81.7 122.5
192 21.4 17.5 26.3

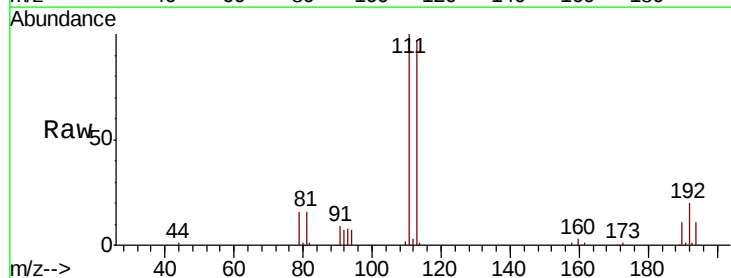

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

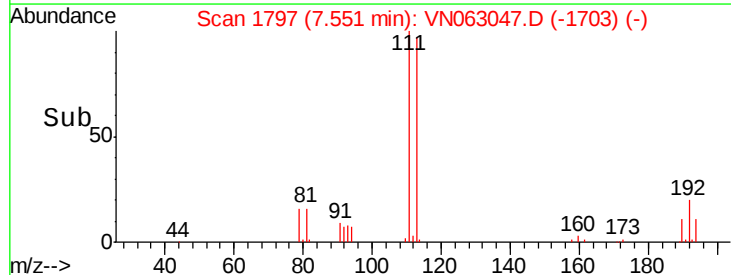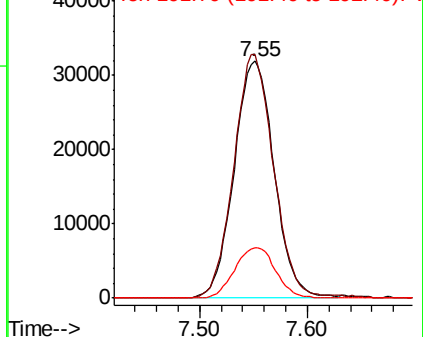

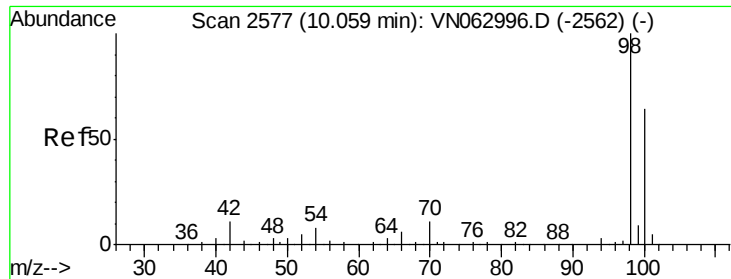

#50

Toluene-d8

Concen: 51.176 ug/l

RT: 10.06 min Scan# 2578

Delta R.T. 0.00 min

Lab File: VN063047.D

Acq: 20 Aug 2020 20:50

Instrument :

MSVOA_N

ClientSampleId :


VN0820WBL02

Tot Ion: 98 Resp: 305798

Ion Ratio Lower Upper

98 100

100 63.3 51.2 76.8

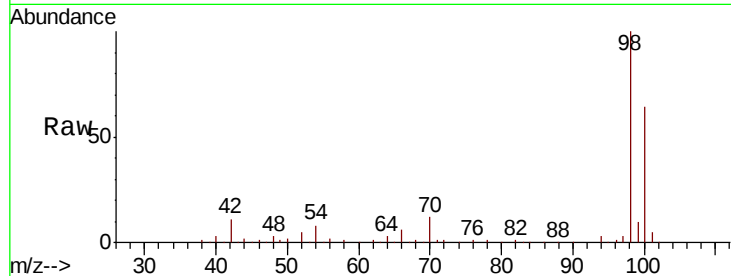

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN

200000

150000



100000

50000

0

10.00 10.10 10.20

Time-->

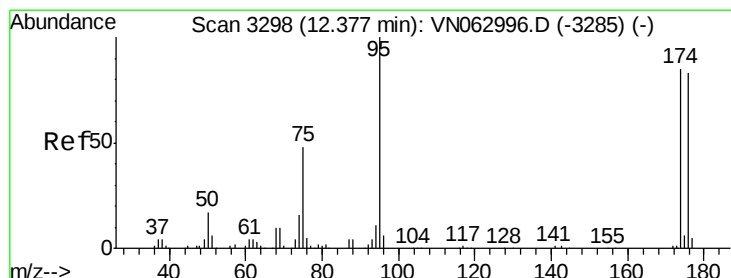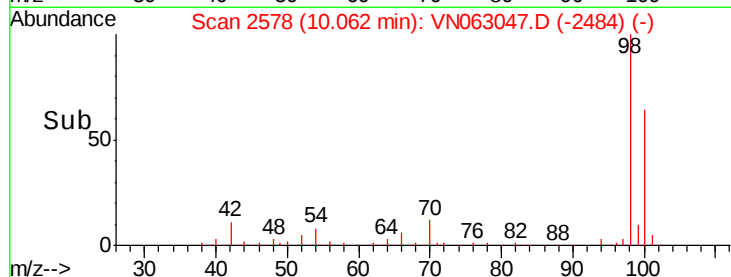

#62

4-Bromofluorobenzene

Concen: 47.932 ug/l

RT: 12.38 min Scan# 3298

Delta R.T. -0.00 min

Lab File: VN063047.D

Acq: 20 Aug 2020 20:50


Tgt Ion: 95 Resp: 101072

Ion Ratio Lower Upper

95 100

174 86.9 0.0 170.8

176 82.7 0.0 164.8

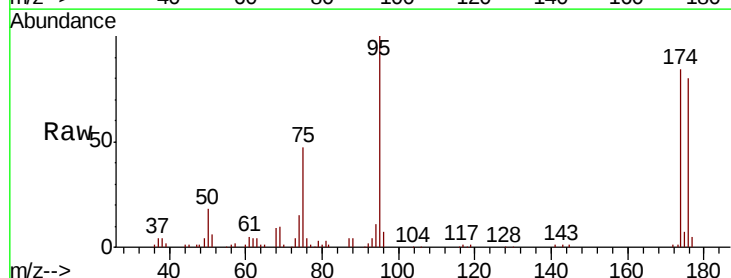

Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

80000

60000


40000


20000

0

12.30 12.40 12.50

Time-->

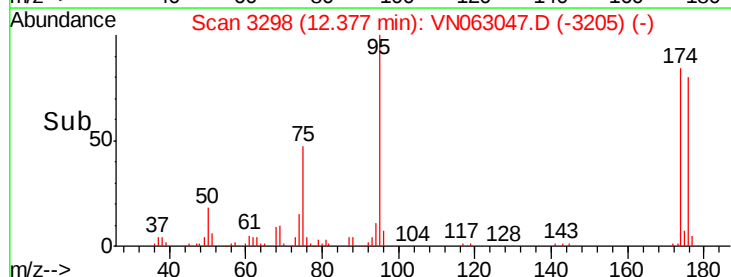

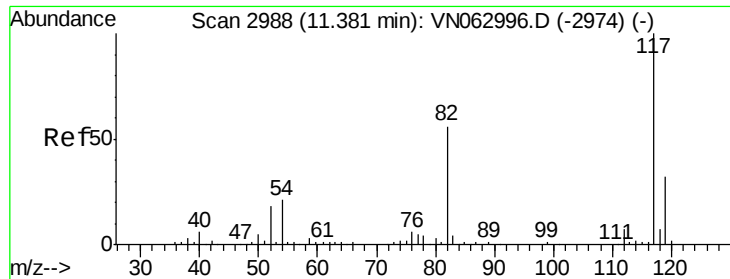

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 2988

Delta R.T. -0.00 min

Lab File: VN063047.D

Acq: 20 Aug 2020 20:50

Instrument :

MSVOA_N

ClientSampleId :

VN0820WBL02


Tot Ion:117 Resp: 242888

Ion Ratio Lower Upper

117 100

82 56.1 44.5 66.7




119 31.9 25.5 38.3

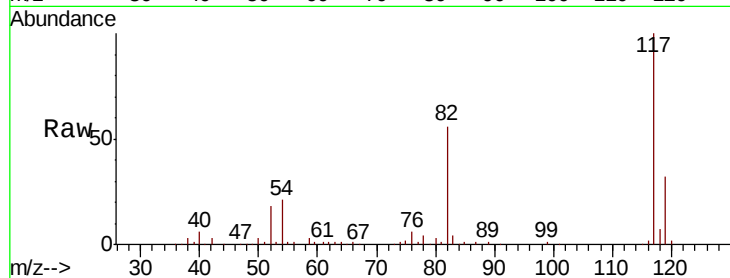

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VN

Ion 118.90 (118.60 to 119.60): V

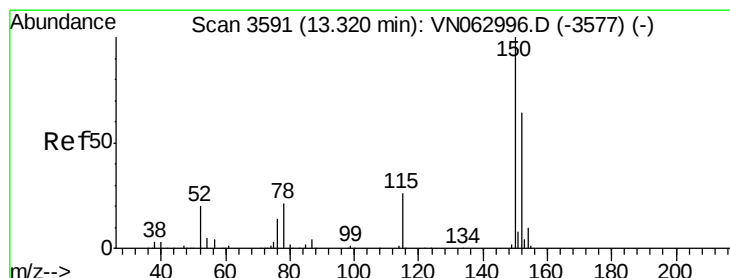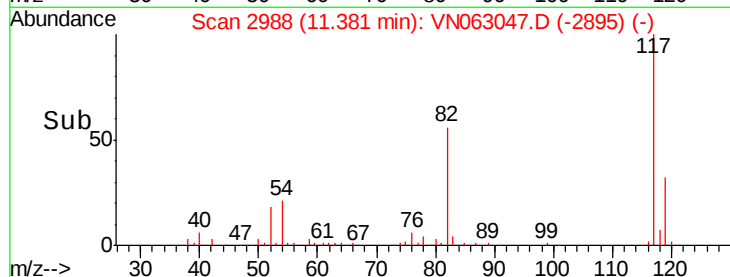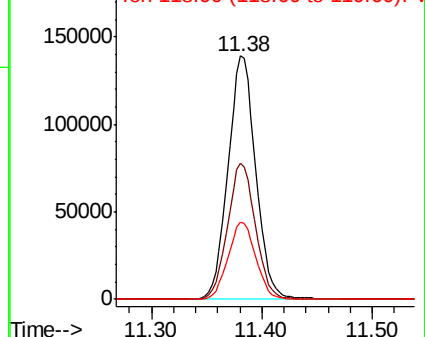

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3591

Delta R.T. -0.00 min

Lab File: VN063047.D

Acq: 20 Aug 2020 20:50


Tgt Ion:152 Resp: 89555

Ion Ratio Lower Upper

152 100

115 55.1 28.7 86.3

150 155.2 0.0 348.8

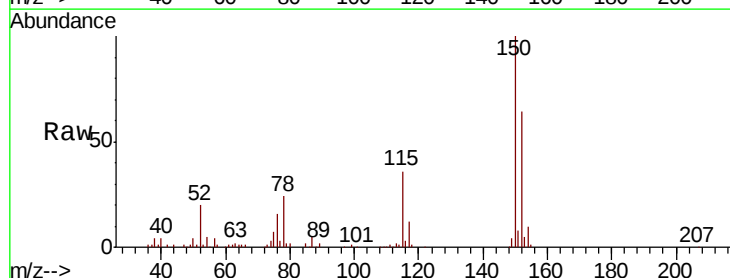

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

