


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082020\
 Data File : VN063025.D
 Acq On : 20 Aug 2020 8:51
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N082020W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Aug 20 14:01:17 2020

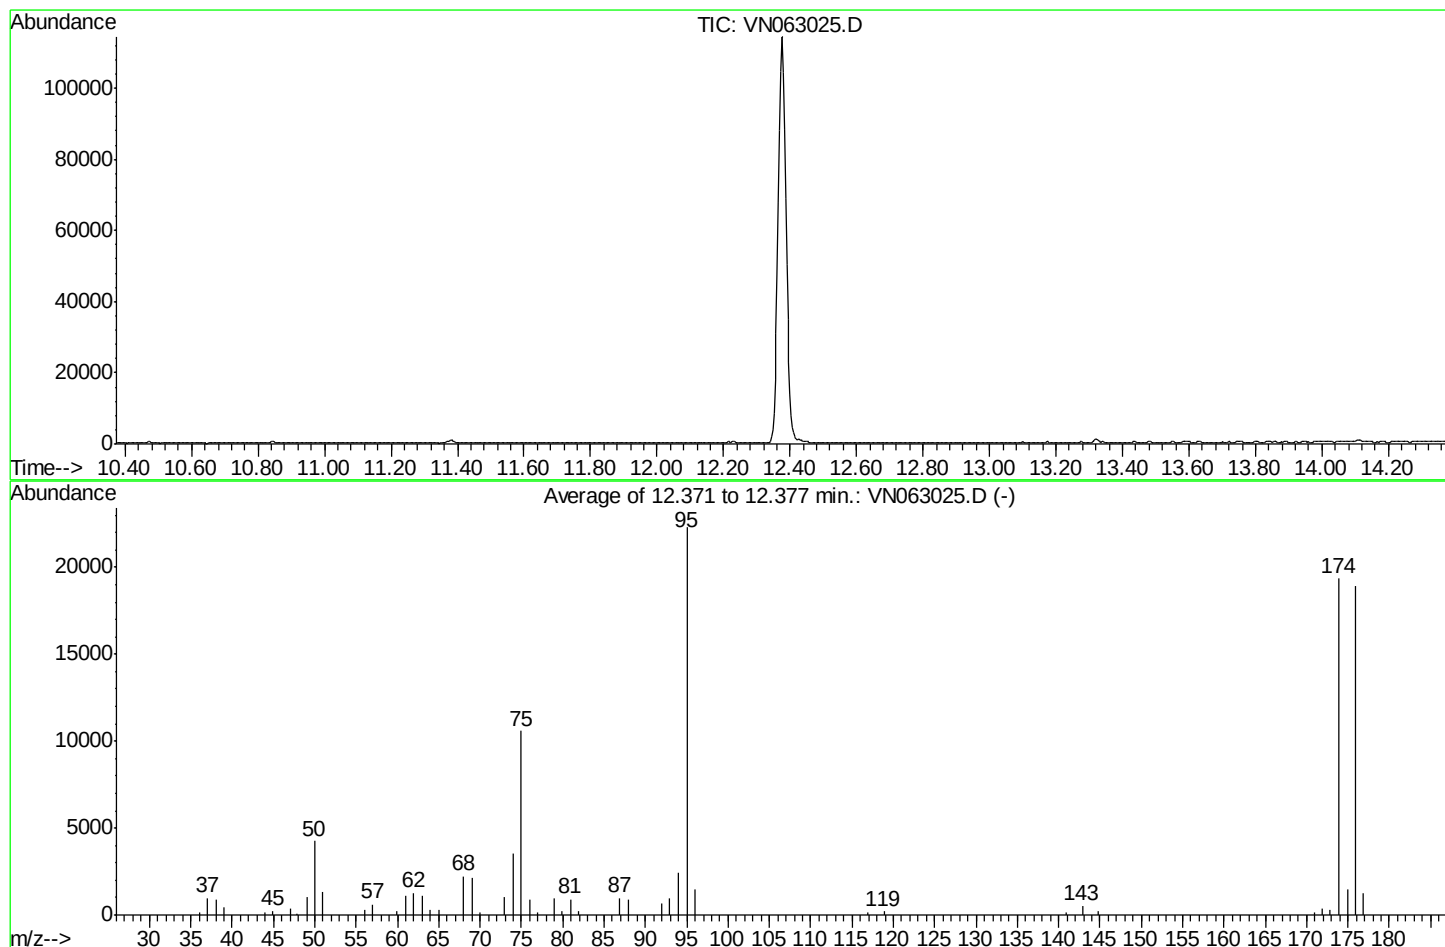

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3285

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	4258	PASS
75	95	30	60	47.4	10574	PASS
95	95	100	100	100.0	22298	PASS
96	95	5	9	6.5	1460	PASS
173	174	0.00	2	1.7	329	PASS
174	95	50	100	86.8	19354	PASS
175	174	5	9	7.8	1508	PASS
176	174	95	101	97.7	18904	PASS
177	176	5	9	6.5	1236	PASS