


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN082020\
 Data File : VN063045.D
 Acq On : 20 Aug 2020 19:13
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N081820W.M
 Title : SW846 8260
 Last Update : Wed Aug 19 06:09:27 2020

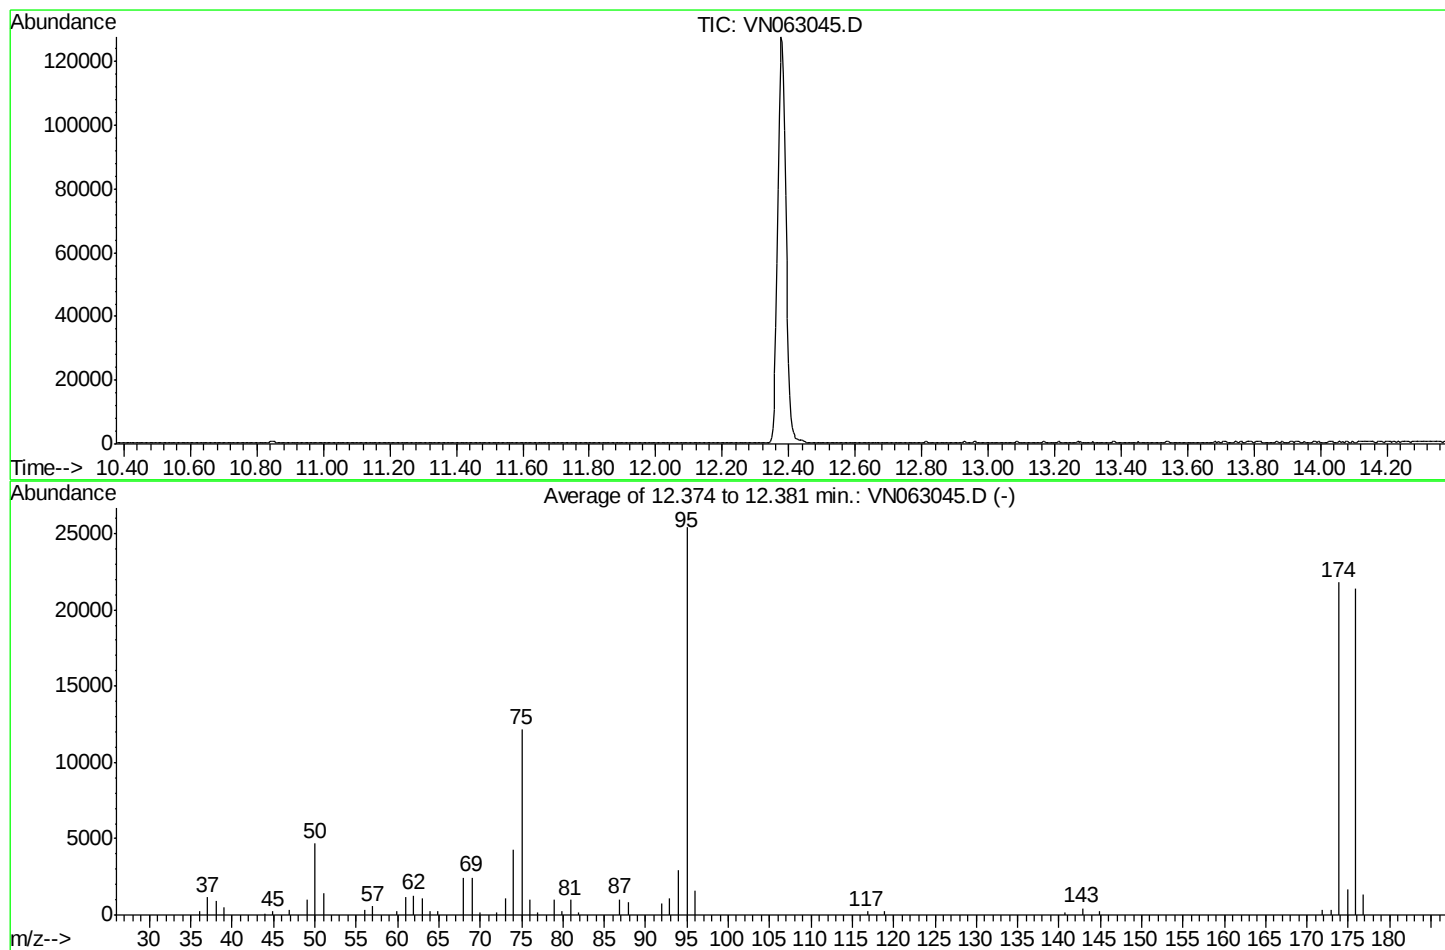

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3285

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	4669	PASS
75	95	30	60	47.8	12147	PASS
95	95	100	100	100.0	25410	PASS
96	95	5	9	6.3	1612	PASS
173	174	0.00	2	1.7	360	PASS
174	95	50	100	85.8	21810	PASS
175	174	5	9	7.7	1689	PASS
176	174	95	101	98.1	21405	PASS
177	176	5	9	6.1	1308	PASS