


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082021\
 Data File : VN068234.D
 Acq On : 20 Aug 2021 9:34
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N081721W.M
 Title : SW846 8260
 Last Update : Tue Aug 17 13:09:49 2021

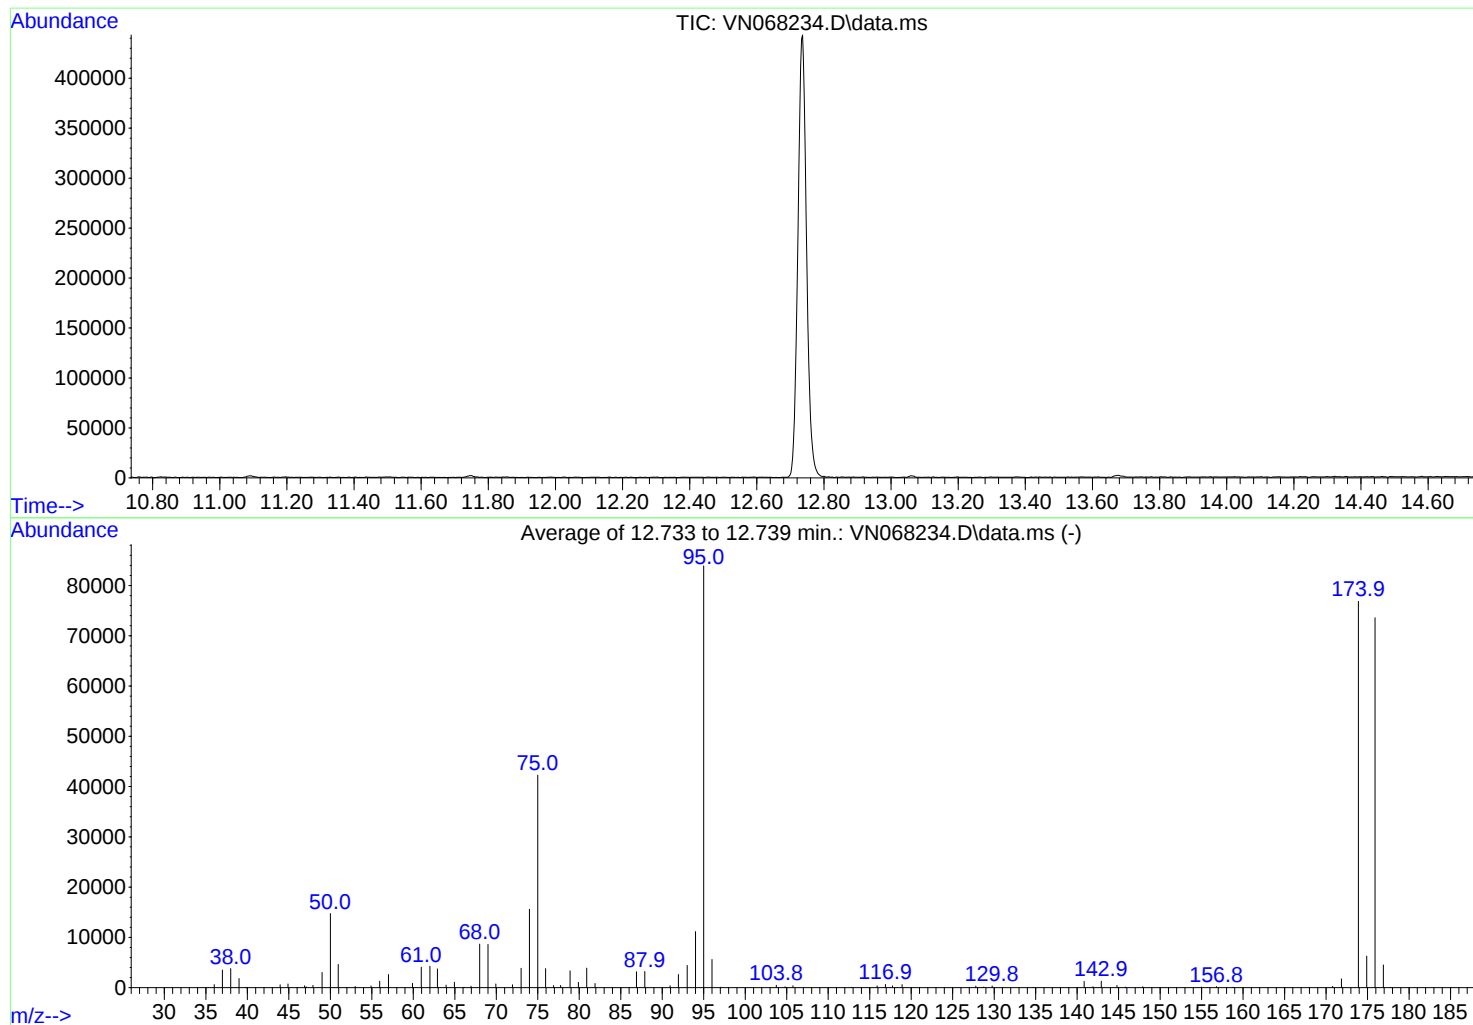

AutoFind: Scans 4006, 4007, 4008; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	14734	PASS
75	95	30	60	50.4	42275	PASS
95	95	100	100	100.0	83915	PASS
96	95	5	9	6.7	5618	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.6	76851	PASS
175	174	5	9	8.2	6268	PASS
176	174	95	101	95.8	73592	PASS
177	176	5	9	6.1	4518	PASS