

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082024\
 Data File : VN083403.D
 Acq On : 20 Aug 2024 16:27
 Operator : JC\MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Aug 21 02:26:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 08 06:30:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	103537	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	211773	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	228461	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	109127	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.576	65	97723	66.310	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 132.620%#	
35) Dibromofluoromethane	8.165	113	76759	58.070	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 116.140%	
50) Toluene-d8	10.565	98	275894	55.953	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 111.900%	
62) 4-Bromofluorobenzene	12.847	95	122513	63.732	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 127.460%#	


Target Compounds				Qvalue		
3) Chloromethane	2.359	50	413	0.344	ug/l #	43
5) Bromomethane	2.906	94	409	0.537	ug/l #	80
11) Tert butyl alcohol	5.494	59	1589	5.188	ug/l #	71
16) Acetone	4.441	43	649	1.125	ug/l #	48
17) Carbon Disulfide	4.706	76	1829	0.545	ug/l #	75
18) Methyl Acetate	5.024	43	5142	2.993	ug/l #	88
20) Methylene Chloride	5.271	84	287	0.216	ug/l #	7
29) Tetrahydrofuran	7.841	42	120	0.210	ug/l #	38
31) Cyclohexane	8.212	56	2914	1.334	ug/l #	42
36) 1,1-Dichloropropene	8.218	75	9764	4.883	ug/l #	53
38) Carbon Tetrachloride	8.218	117	11184	4.966	ug/l #	17
43) Isopropyl Acetate	8.647	43	6083	Below Cal	#	60
44) Trichloroethene	9.359	130	290	0.205	ug/l	76
53) t-1,3-Dichloropropene	10.841	75	515	0.221	ug/l #	50
59) 2-Hexanone	11.200	43	675	0.412	ug/l #	28
65) Chlorobenzene	11.894	112	1171	0.232	ug/l #	63
68) m/p-Xylenes	12.076	106	1203	0.347	ug/l	99
70) Styrene	12.406	104	1574	0.274	ug/l	91
76) 1,2,3-Trichloropropane	12.847	75	67820	28.317	ug/l #	1
77) Bromobenzene	12.982	156	644	0.318	ug/l	97
78) n-propylbenzene	13.041	91	2675	0.255	ug/l	90
79) 2-Chlorotoluene	13.123	91	1512	0.227	ug/l	90
81) trans-1,4-Dichloro-2-b...	12.847	75	67820	61.595	ug/l #	6
82) 4-Chlorotoluene	13.223	91	2714	0.406	ug/l	92
87) 1,3-Dichlorobenzene	13.723	146	1977	0.518	ug/l	96
88) 1,4-Dichlorobenzene	13.723	146	1977	0.514	ug/l	96
89) n-Butylbenzene	14.053	91	2477	0.375	ug/l	90
91) 1,2-Dichlorobenzene	14.106	146	1442	0.391	ug/l	97
93) 1,2,4-Trichlorobenzene	15.388	180	1476	0.714	ug/l	96
94) Hexachlorobutadiene	15.500	225	352	0.383	ug/l	85
95) Naphthalene	15.641	128	4478	0.611	ug/l #	85
96) 1,2,3-Trichlorobenzene	15.835	180	1350	0.660	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082024\
Data File : VN083403.D
Acq On : 20 Aug 2024 16:27
Operator : JC\MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :


Quant Time: Aug 21 02:26:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 08 06:30:41 2024
Response via : Initial Calibration

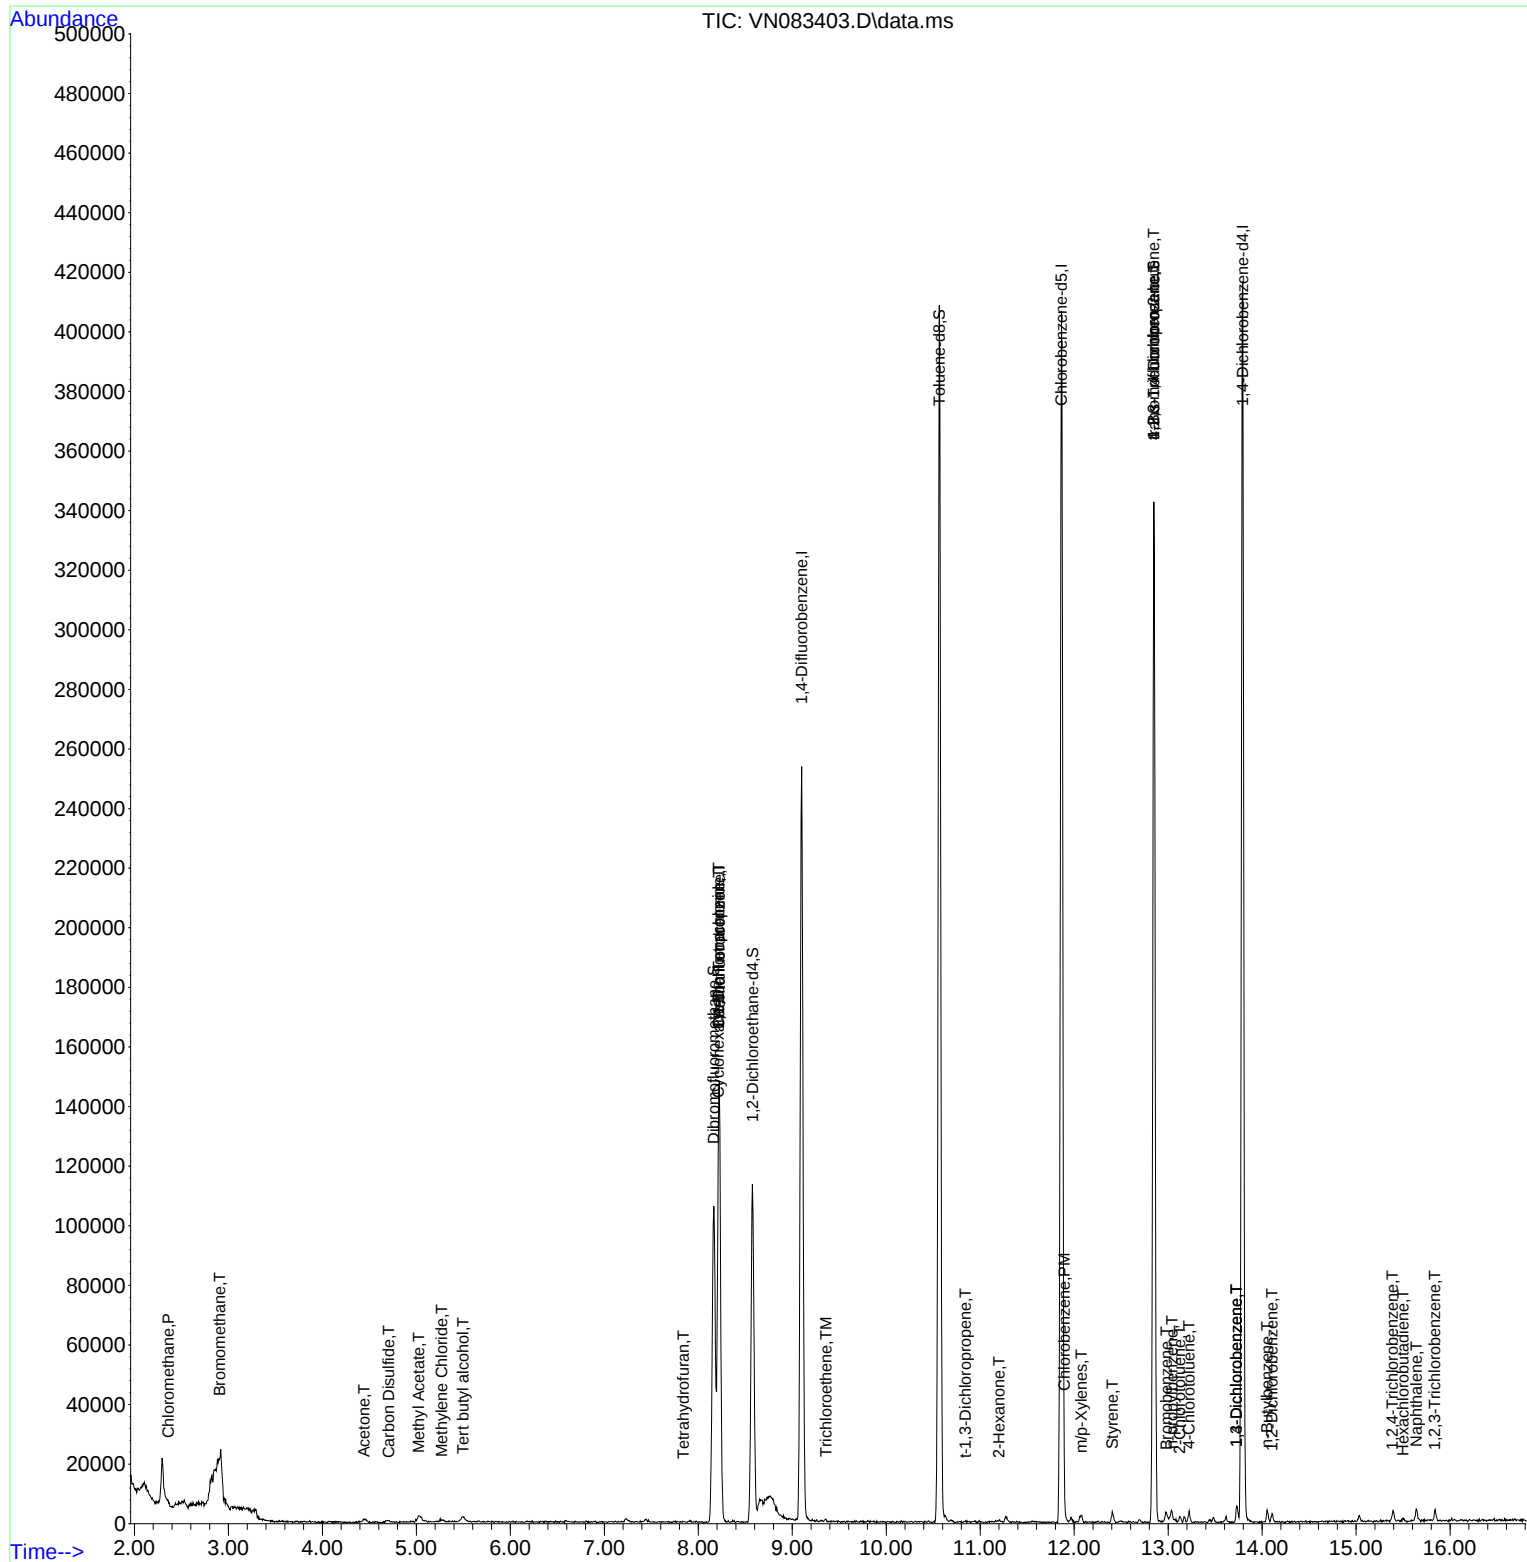





#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:168 Resp: 103537
Ion Ratio Lower Upper
168 100
99 66.8 48.2 72.4



#3
Chloromethane
Concen: 0.344 ug/l
RT: 2.359 min Scan# 69
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27


Tgt Ion: 50 Resp: 413
Ion Ratio Lower Upper
50 100
52 0.0 25.0 37.4#

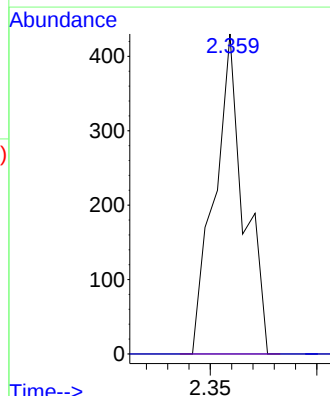






#5
Bromomethane
Concen: 0.537 ug/l
RT: 2.906 min Scan# 11
Delta R.T. -0.041 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 94 Resp: 409
Ion Ratio Lower Upper
94 100
96 77.8 78.0 117.0#

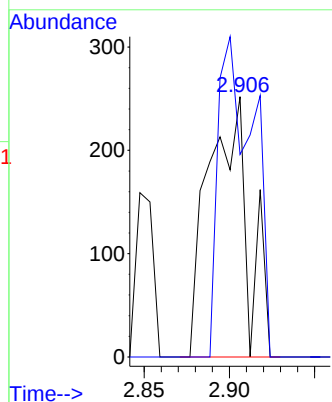

#11
Tert butyl alcohol
Concen: 5.188 ug/l
RT: 5.494 min Scan# 602
Delta R.T. -0.035 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27


Tgt Ion: 59 Resp: 1589
Ion Ratio Lower Upper
59 100
57 0.0 8.9 13.3#

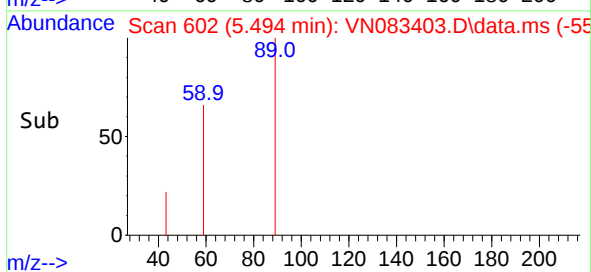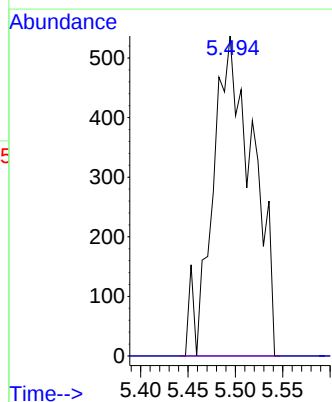






#16
Acetone
Concen: 1.125 ug/l
RT: 4.441 min Scan# 41
Delta R.T. 0.012 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 649
Ion Ratio Lower Upper
43 100
58 0.0 21.8 32.6#

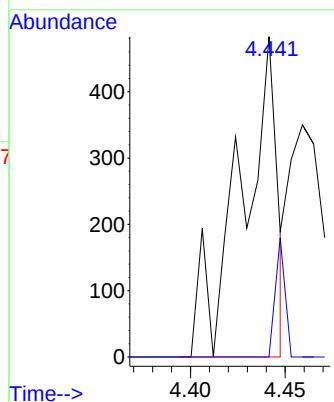

#17
Carbon Disulfide
Concen: 0.545 ug/l
RT: 4.706 min Scan# 468
Delta R.T. -0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Tgt Ion: 76 Resp: 1829
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

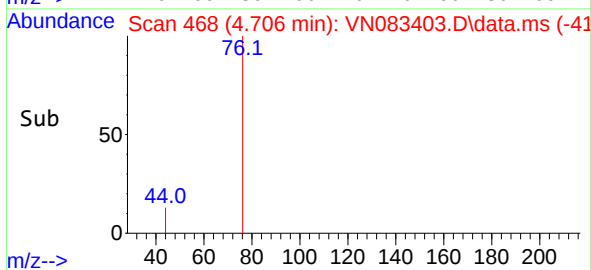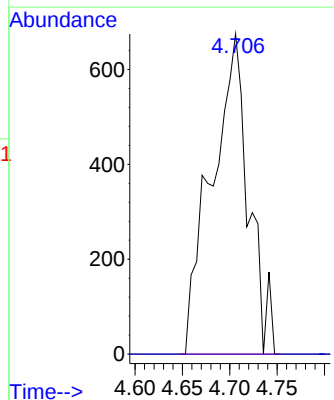



#18

Methyl Acetate

Concen: 2.993 ug/l

RT: 5.024 min Scan# 51

Delta R.T. -0.000 min


Lab File: VN083403.D

Acq: 20 Aug 2024 16:27

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 43 Resp: 5142

Ion Ratio Lower Upper

43 100

74 14.8 16.3 24.5#

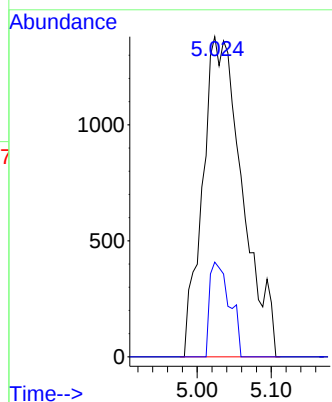

#20

Methylene Chloride

Concen: 0.216 ug/l

RT: 5.271 min Scan# 564

Delta R.T. -0.006 min

Lab File: VN083403.D

Acq: 20 Aug 2024 16:27

Tgt Ion: 84 Resp: 287




Ion Ratio Lower Upper


84 100

49 17.1 119.6 179.4#

51 0.0 34.8 52.2#

86 0.0 52.9 79.3#


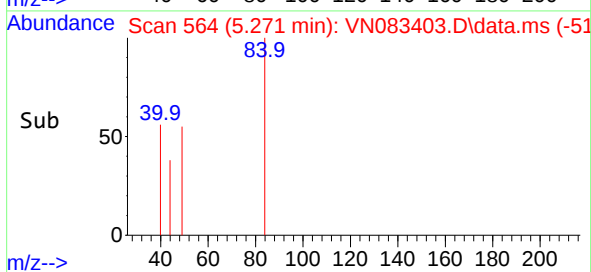

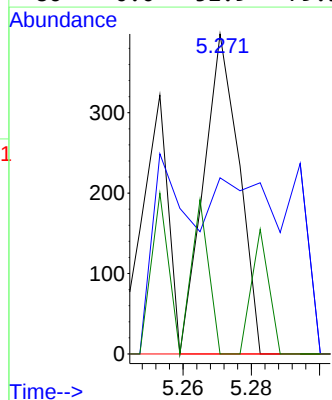




#29
Tetrahydrofuran
Concen: 0.210 ug/l
RT: 7.841 min Scan# 1064
Delta R.T. 0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 42	Resp:	120
Ion	Ratio	Lower Upper
42	100	
72	0.0	30.0 45.0#
71	0.0	28.3 42.5#

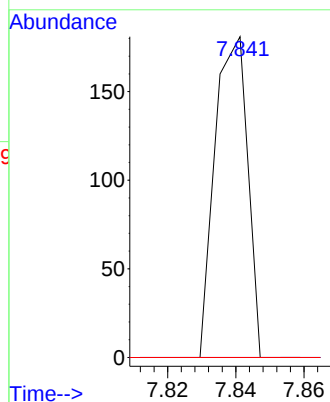

#31
Cyclohexane
Concen: 1.334 ug/l
RT: 8.212 min Scan# 1064
Delta R.T. -0.047 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Tgt Ion: 56	Resp:	2914
Ion	Ratio	Lower Upper
56	100	
69	126.1	24.5 36.7#
84	95.2	66.0 99.0


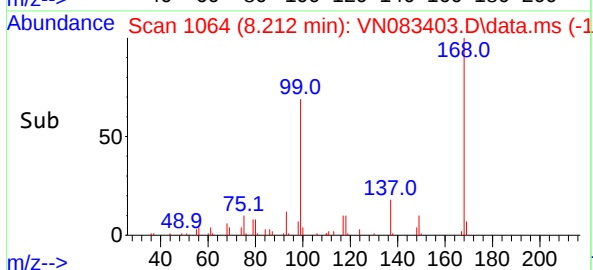






#33
1,2-Dichloroethane-d4
Concen: 66.310 ug/l
RT: 8.576 min Scan# 1127
Delta R.T. -0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 65 Resp: 97723
Ion Ratio Lower Upper
65 100
67 49.8 0.0 104.4

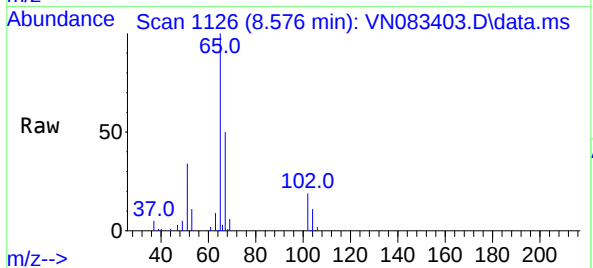

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 1215
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27


Tgt Ion: 114 Resp: 211773
Ion Ratio Lower Upper
114 100
63 23.4 0.0 44.6
88 16.9 0.0 31.4

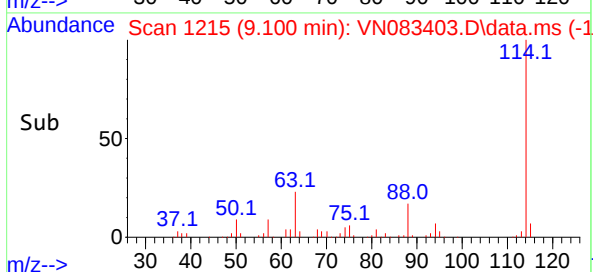






#35
Dibromofluoromethane
Concen: 58.070 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Instrument :
MSVOA_N
ClientSampleId :



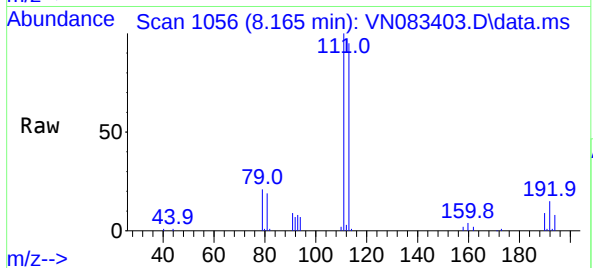



Tgt Ion:113 Resp: 76759
Ion Ratio Lower Upper
113 100
111 105.5 82.4 123.6
192 16.6 14.9 22.3

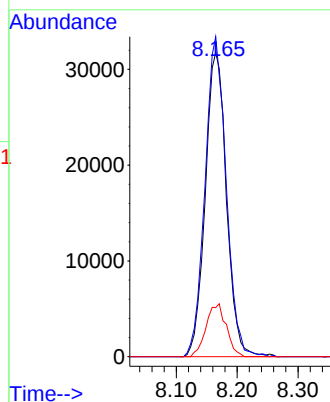

#36
1,1-Dichloropropene
Concen: 4.883 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.153 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27


Tgt Ion: 75 Resp: 9764
Ion Ratio Lower Upper
75 100
110 11.3 16.3 48.9#
77 0.0 24.6 37.0#

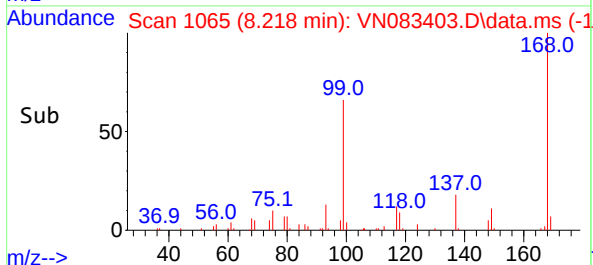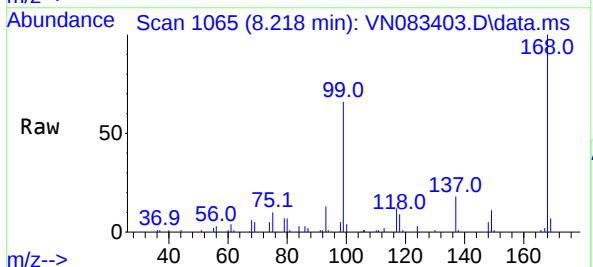






#38
Carbon Tetrachloride
Concen: 4.966 ug/l
RT: 8.218 min Scan# 11184
Delta R.T. -0.141 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Instrument :
MSVOA_N
ClientSampleId :



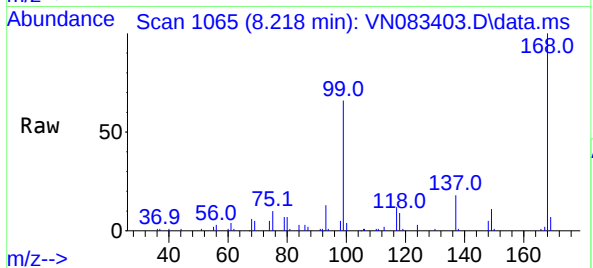



Tgt Ion:117 Resp: 11184
Ion Ratio Lower Upper
117 100
119 5.6 74.9 112.3#
121 0.0 24.3 36.5#

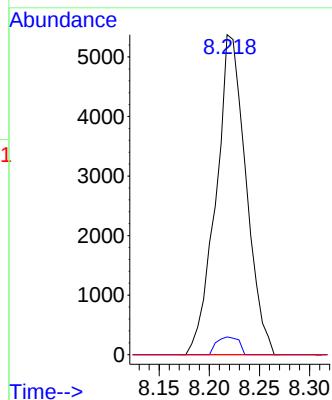

#43
Isopropyl Acetate
Concen: Below Cal
RT: 8.647 min Scan# 1138
Delta R.T. -0.041 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27


Tgt Ion: 43 Resp: 6083
Ion Ratio Lower Upper
43 100
61 0.0 17.8 26.6#
87 0.0 8.2 12.2#

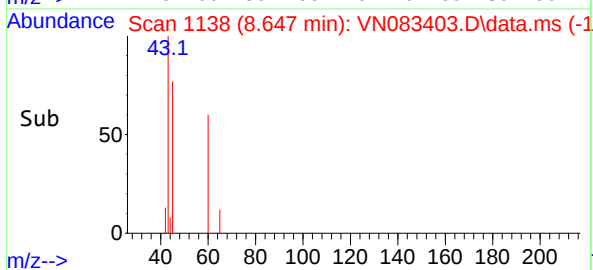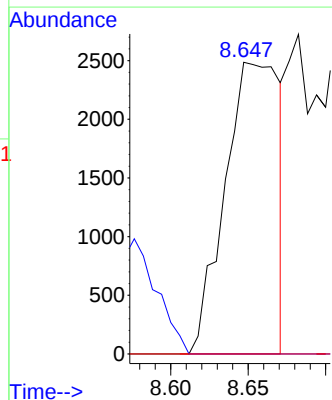






#44
Trichloroethene
Concen: 0.205 ug/l
RT: 9.359 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:130 Resp: 290
Ion Ratio Lower Upper
130 100
95 122.3 0.0 197.8



#50
Toluene-d8
Concen: 55.953 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27


Tgt Ion: 98 Resp: 275894
Ion Ratio Lower Upper
98 100
100 65.3 51.5 77.3

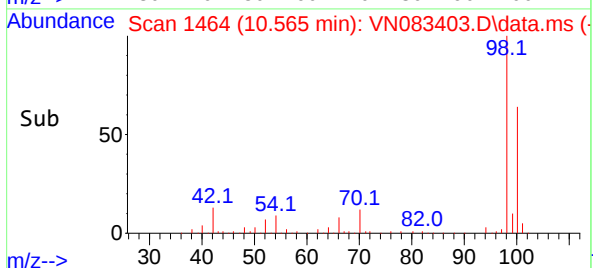






#53
t-1,3-Dichloropropene
Concen: 0.221 ug/l
RT: 10.841 min Scan# 1511
Delta R.T. 0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 75 Resp: 515
Ion Ratio Lower Upper
75 100
77 59.9 25.7 38.5#

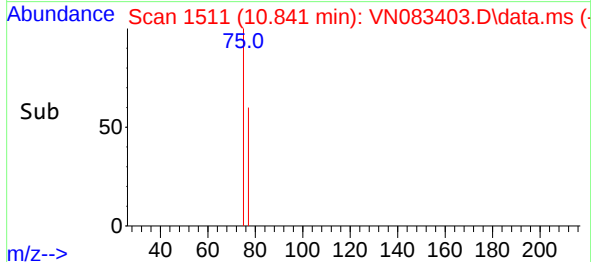

#59
2-Hexanone
Concen: 0.412 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. 0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Tgt Ion: 43 Resp: 675
Ion Ratio Lower Upper
43 100
58 0.0 24.6 73.8#


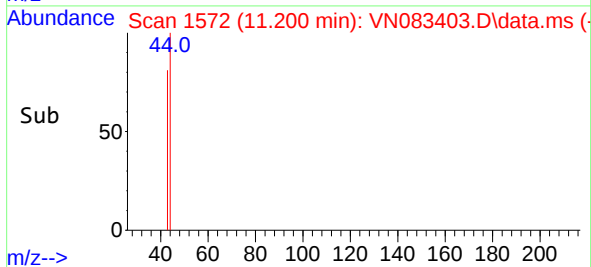

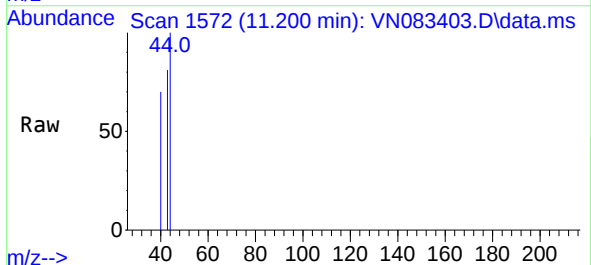




#62
4-Bromofluorobenzene
Concen: 63.732 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 122513
Ion Ratio Lower Upper
95 100
174 69.5 0.0 159.2
176 66.4 0.0 147.6

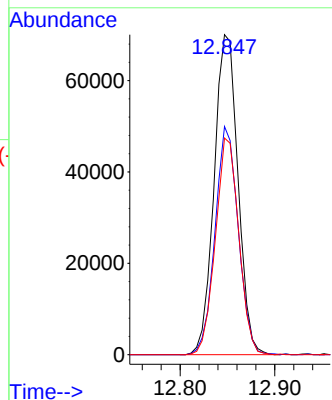

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27


Tgt Ion: 117 Resp: 228461
Ion Ratio Lower Upper
117 100
82 59.3 47.5 71.3
119 30.2 25.6 38.4

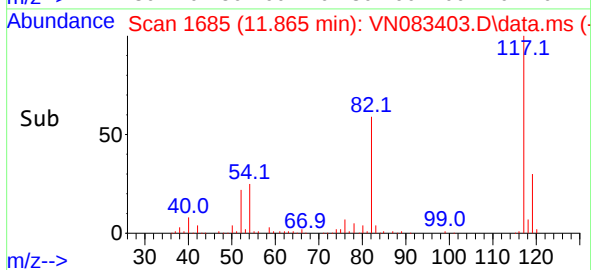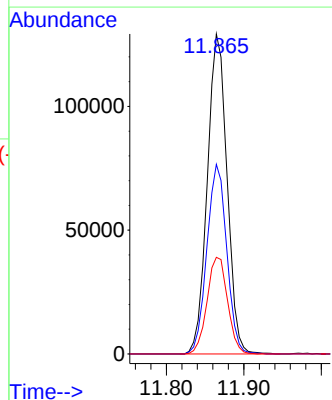






#65
Chlorobenzene
Concen: 0.232 ug/l
RT: 11.894 min Scan# 1171
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:112 Resp: 1171
Ion Ratio Lower Upper
112 100
114 53.5 26.2 39.2#

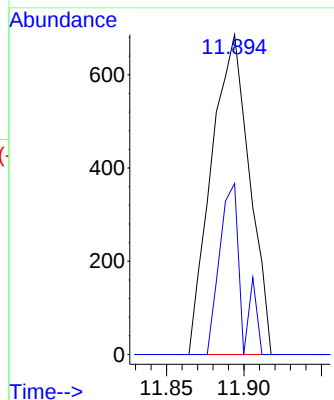


#68
m/p-Xylenes
Concen: 0.347 ug/l
RT: 12.076 min Scan# 1721
Delta R.T. 0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27



Tgt Ion:106 Resp: 1203
Ion Ratio Lower Upper
106 100
91 209.4 166.1 249.1



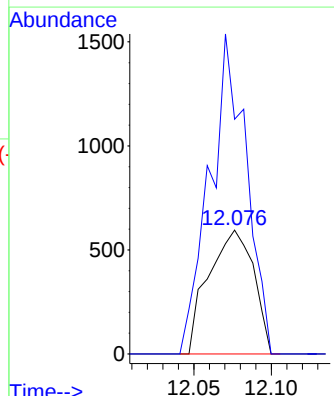





#70
Styrene
Concen: 0.274 ug/l
RT: 12.406 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:104 Resp: 1574
Ion Ratio Lower Upper
104 100
78 45.3 41.6 62.4
103 48.2 44.0 66.0



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Tgt Ion:152 Resp: 109127
Ion Ratio Lower Upper
152 100
115 63.4 30.6 91.6
150 159.0 0.0 348.6


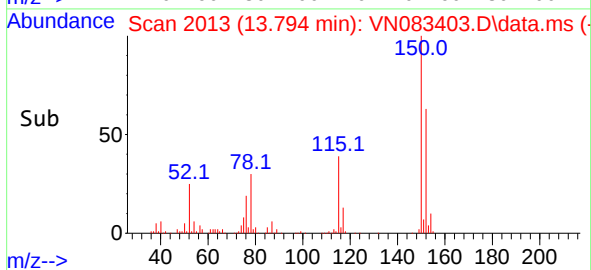






#76
1,2,3-Trichloropropane
Concen: 28.317 ug/l
RT: 12.847 min Scan# 11
Delta R.T. -0.147 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 67820
Ion Ratio Lower Upper
75 100
77 0.9 110.9 332.6#

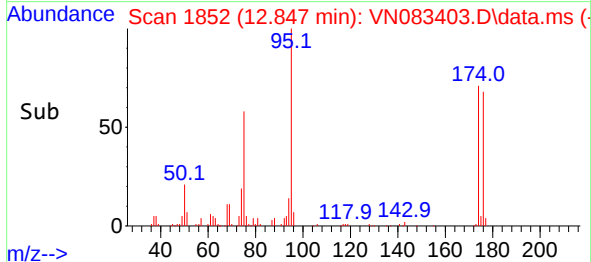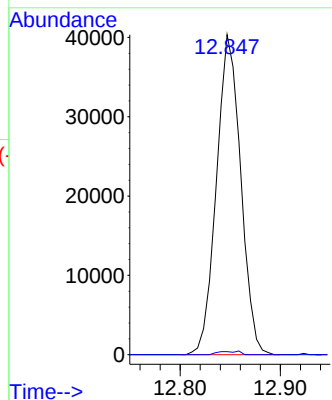

#77
Bromobenzene
Concen: 0.318 ug/l
RT: 12.982 min Scan# 1875
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Tgt Ion:156 Resp: 644
Ion Ratio Lower Upper
156 100
77 223.0 111.3 333.8
158 104.3 48.3 144.9


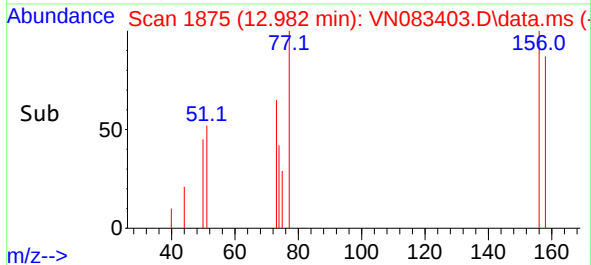
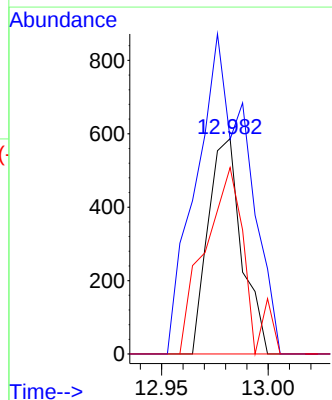
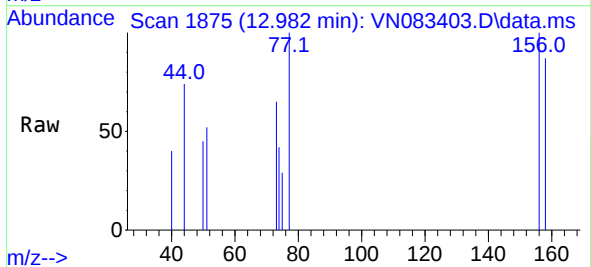




#78
n-propylbenzene
Concen: 0.255 ug/l
RT: 13.041 min Scan# 1885
Delta R.T. 0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 91 Resp: 2675
Ion Ratio Lower Upper
91 100
120 17.0 10.9 32.9



#79
2-Chlorotoluene
Concen: 0.227 ug/l
RT: 13.123 min Scan# 1899
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27


Tgt Ion: 91 Resp: 1512
Ion Ratio Lower Upper
91 100
126 27.0 16.2 48.6

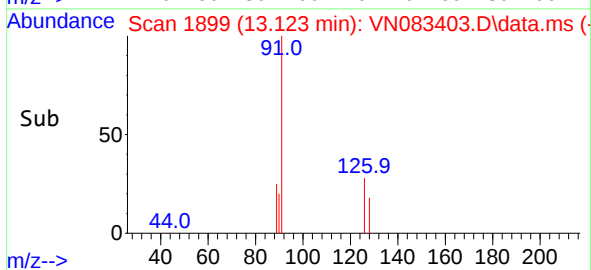



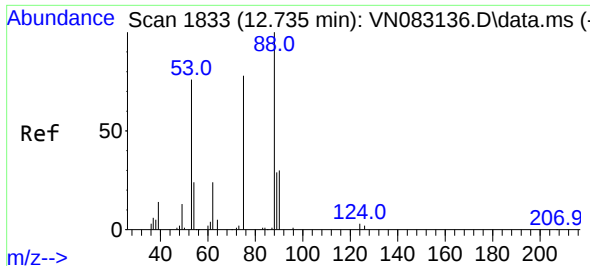


#81
trans-1,4-Dichloro-2-butene
Concen: 61.595 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.112 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Instrument :
MSVOA_N
ClientSampleId :



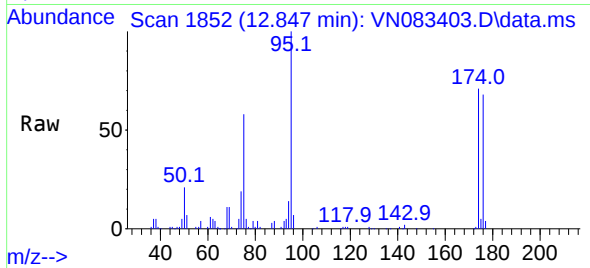



Tgt Ion: 75 Resp: 67820
Ion Ratio Lower Upper
75 100
53 0.0 88.4 132.6#
89 0.0 36.3 54.5#

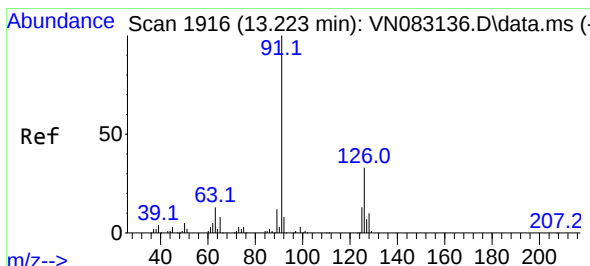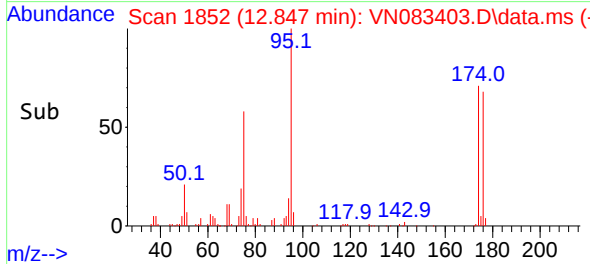

#82
4-Chlorotoluene
Concen: 0.406 ug/l
RT: 13.223 min Scan# 1916
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Tgt Ion: 91 Resp: 2714
Ion Ratio Lower Upper
91 100
126 37.1 16.2 48.6

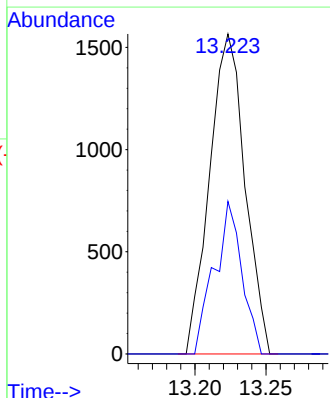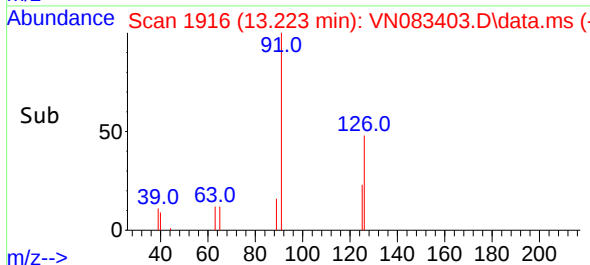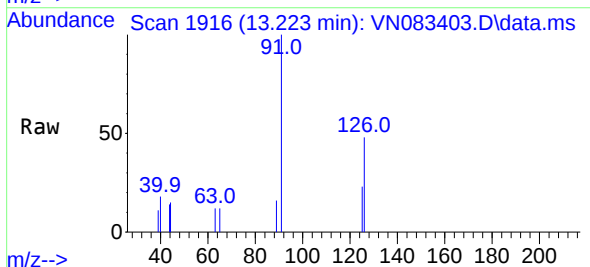



#87

1,3-Dichlorobenzene

Concen: 0.518 ug/l

RT: 13.723 min Scan# 2001

Delta R.T. -0.012 min


Lab File: VN083403.D

Acq: 20 Aug 2024 16:27

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion:146 Resp: 1977

Ion Ratio Lower Upper

146 100

111 41.5 20.6 61.9

148 68.4 31.8 95.3

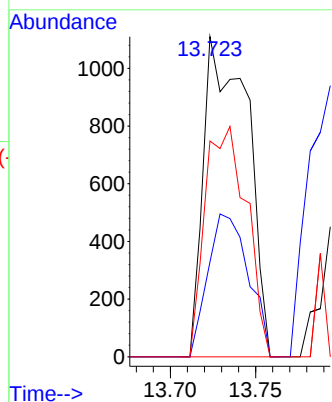

#88

1,4-Dichlorobenzene

Concen: 0.514 ug/l

RT: 13.723 min Scan# 2001

Delta R.T. -0.088 min

Lab File: VN083403.D

Acq: 20 Aug 2024 16:27




Tgt Ion:146 Resp: 1977


Ion Ratio Lower Upper

146 100

111 41.5 20.1 60.3


148 68.4 32.2 96.6

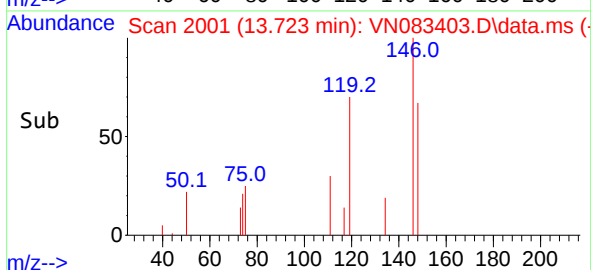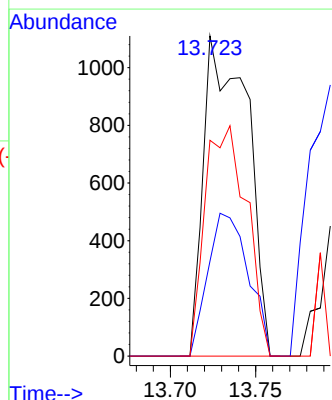






#89
n-Butylbenzene
Concen: 0.375 ug/l
RT: 14.053 min Scan# 2057
Delta R.T. -0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 91 Resp: 2477
Ion Ratio Lower Upper
91 100
92 60.4 26.1 78.3
134 21.0 12.1 36.3

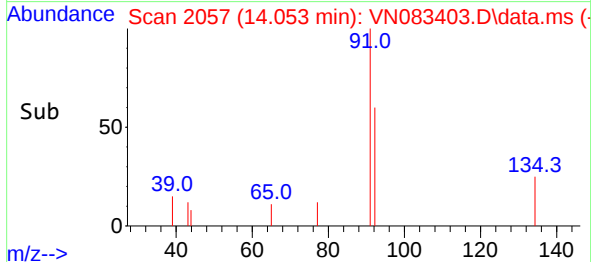

#91
1,2-Dichlorobenzene
Concen: 0.391 ug/l
RT: 14.106 min Scan# 2066
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27


Tgt Ion: 146 Resp: 1442
Ion Ratio Lower Upper
146 100
111 39.7 21.4 64.2
148 63.4 32.1 96.5

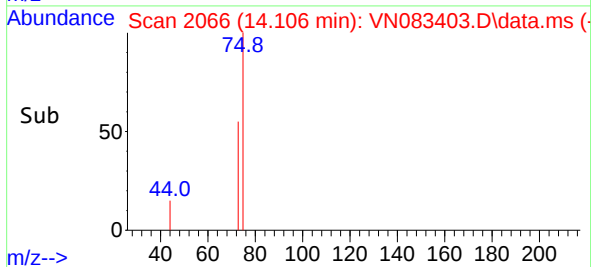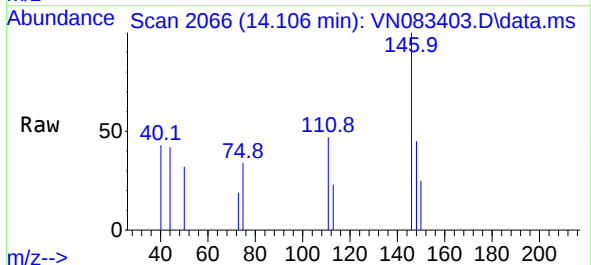






#93
1,2,4-Trichlorobenzene
Concen: 0.714 ug/l
RT: 15.388 min Scan# 21
Delta R.T. -0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:180 Resp: 1476
Ion Ratio Lower Upper
180 100
182 99.1 47.3 141.8
145 31.6 15.7 47.1




#94
Hexachlorobutadiene
Concen: 0.383 ug/l
RT: 15.500 min Scan# 2303
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

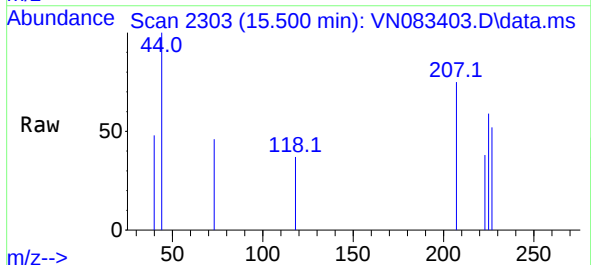


Tgt Ion:225 Resp: 352
Ion Ratio Lower Upper
225 100
223 44.3 31.9 95.7
227 61.6 32.5 97.5

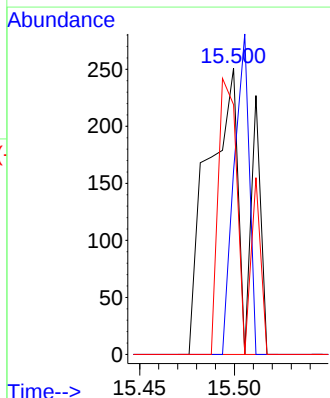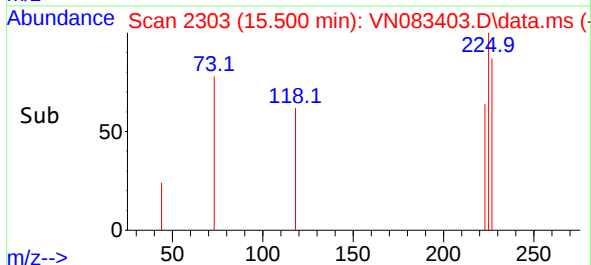






#95
Naphthalene
Concen: 0.611 ug/l
RT: 15.641 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27


Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion:128 Resp: 4478
Ion Ratio Lower Upper
128 100
127 5.3 10.6 16.0#
129 7.5 8.6 12.8#

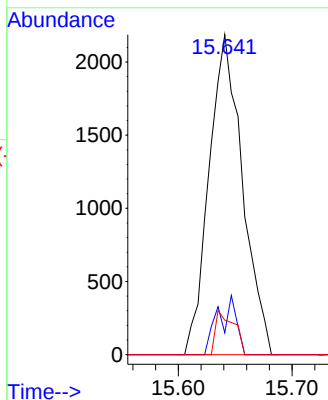

#96
1,2,3-Trichlorobenzene
Concen: 0.660 ug/l
RT: 15.835 min Scan# 2360
Delta R.T. -0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

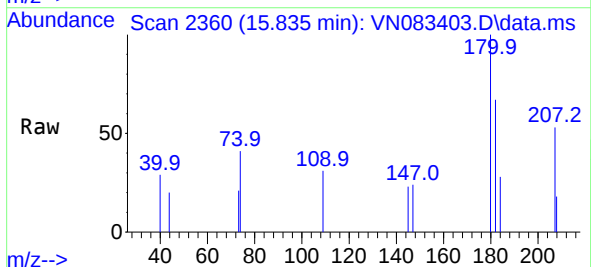

Tgt Ion:180 Resp: 1350
Ion Ratio Lower Upper
180 100
182 96.6 48.9 146.8
145 21.9 16.8 50.4

