

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082024\
 Data File : VN083403.D
 Acq On : 20 Aug 2024 16:27
 Operator : JC\MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VIBLK

Quant Time: Aug 21 02:26:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 08 06:30:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	103537	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	211773	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	228461	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	109127	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.576	65	97723	66.310	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	132.620%#
35) Dibromofluoromethane	8.165	113	76759	58.070	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	116.140%
50) Toluene-d8	10.565	98	275894	55.953	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	111.900%
62) 4-Bromofluorobenzene	12.847	95	122513	63.732	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	127.460%#


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082024\
Data File : VN083403.D
Acq On : 20 Aug 2024 16:27
Operator : JC\MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VIBLK

Quant Time: Aug 21 02:26:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 08 06:30:41 2024
Response via : Initial Calibration




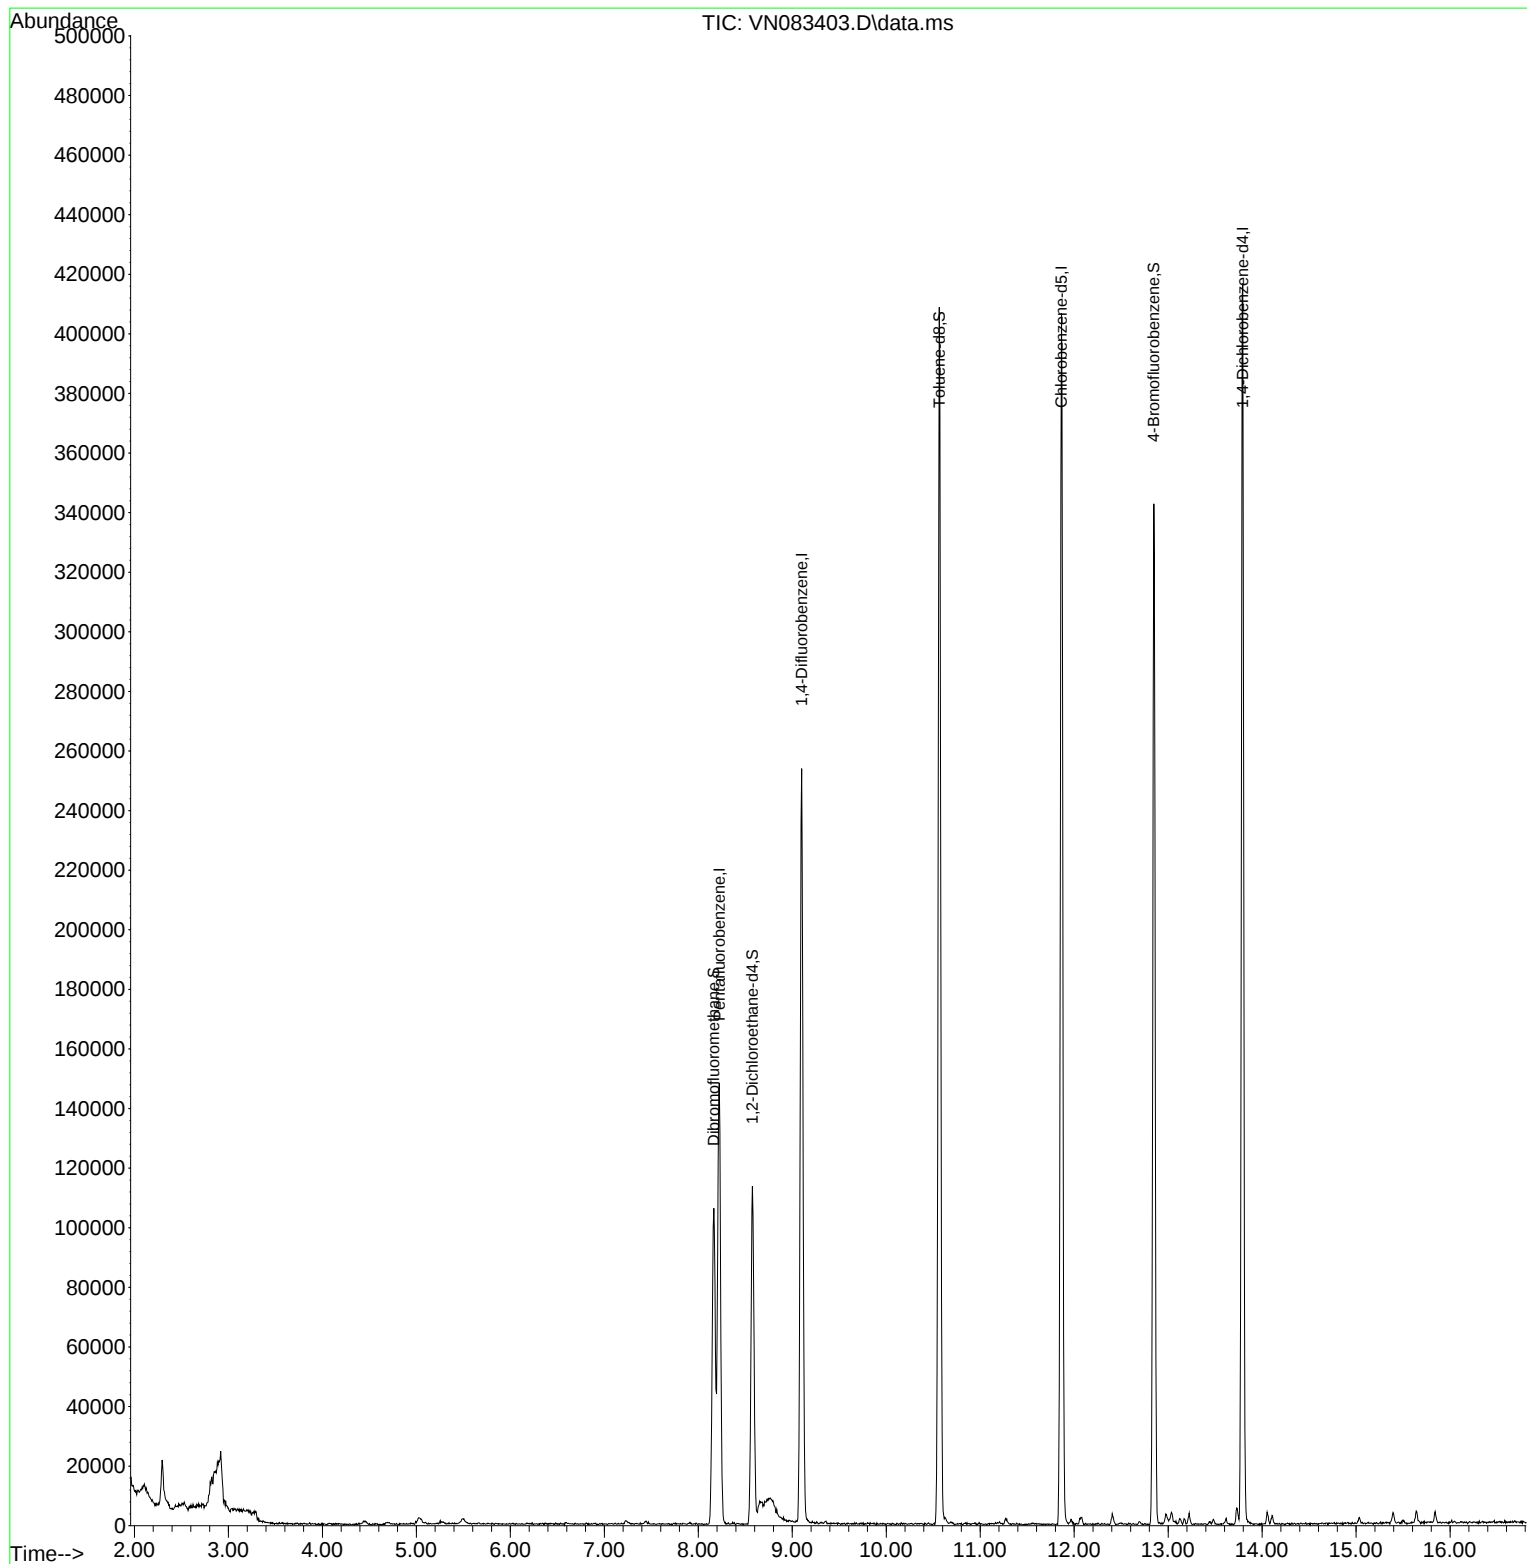




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27




Instrument :
MSVOA_N
ClientSampleId :
VIBLK

Tgt Ion:168 Resp: 103537
Ion Ratio Lower Upper
168 100
99 66.8 48.2 72.4

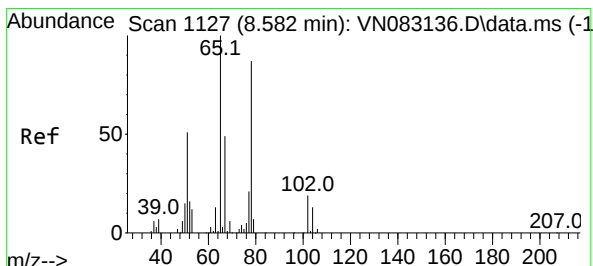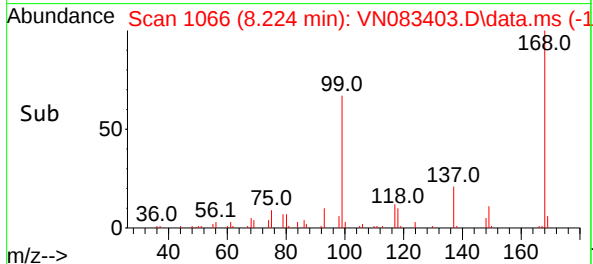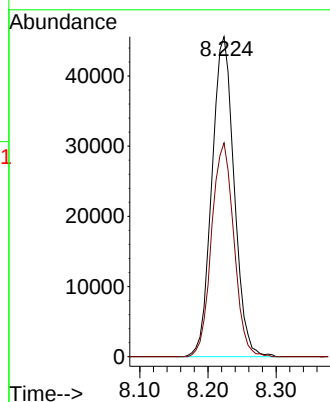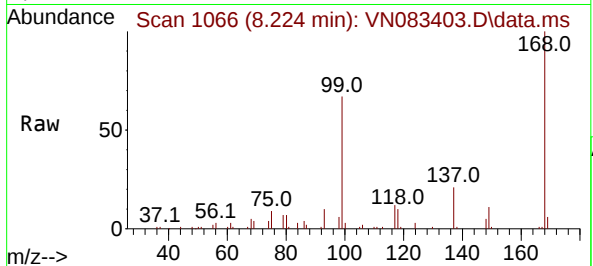

#33
1,2-Dichloroethane-d4
Concen: 66.310 ug/l
RT: 8.576 min Scan# 1126
Delta R.T. -0.006 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Tgt Ion: 65 Resp: 97723
Ion Ratio Lower Upper
65 100
67 49.8 0.0 104.4

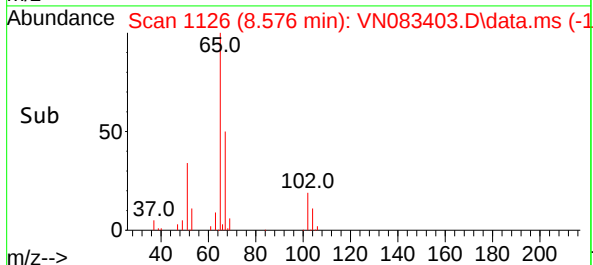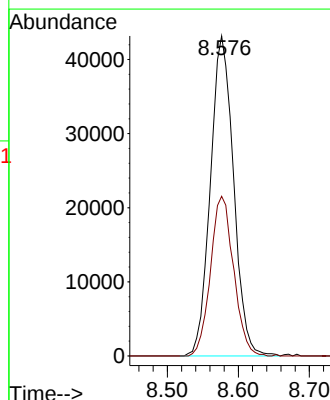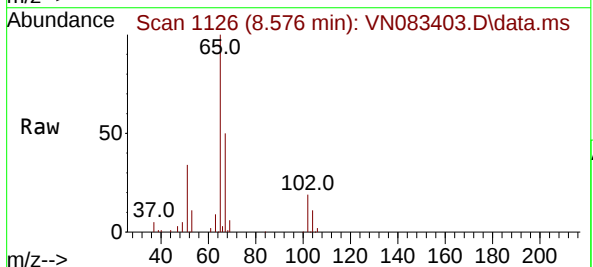



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN083403.D

Acq: 20 Aug 2024 16:27

Instrument :

MSVOA_N

ClientSampleId :

VIBLK





Tgt Ion:114 Resp: 211773

Ion Ratio Lower Upper

114 100

63 23.4 0.0 44.6

88 16.9 0.0 31.4

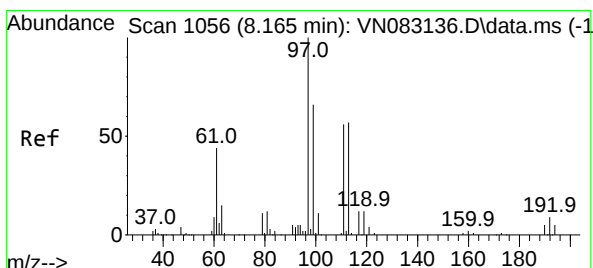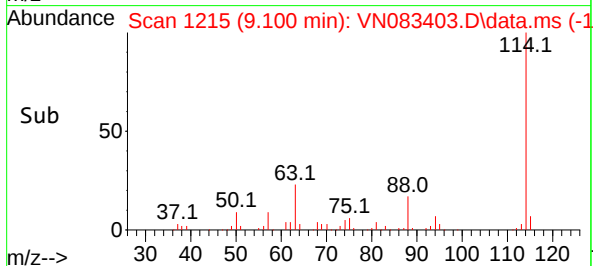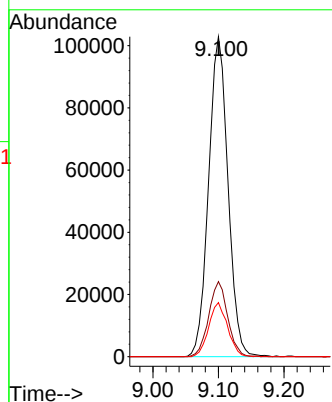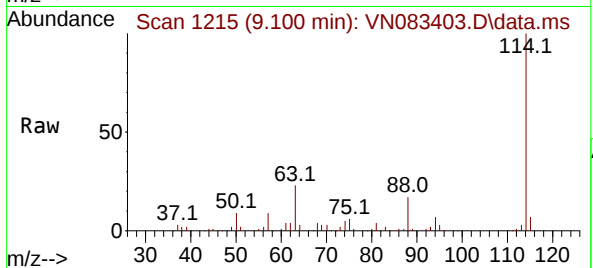

#35

Dibromofluoromethane

Concen: 58.070 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN083403.D

Acq: 20 Aug 2024 16:27




Tgt Ion:113 Resp: 76759

Ion Ratio Lower Upper

113 100

111 105.5 82.4 123.6

192 16.6 14.9 22.3


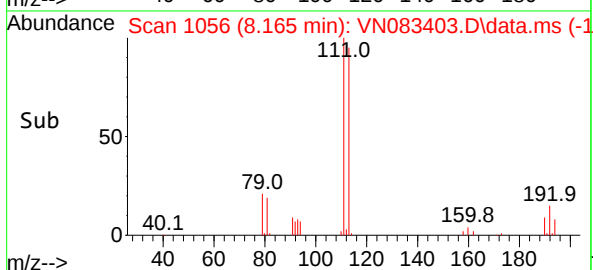
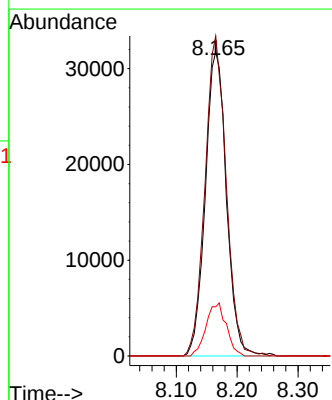
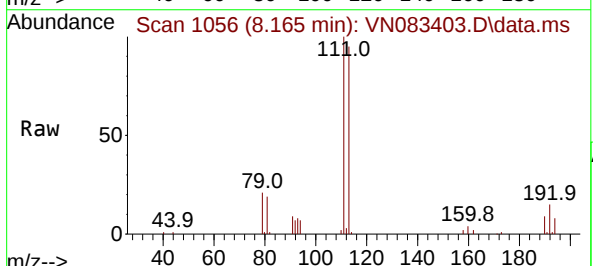




#50
Toluene-d8
Concen: 55.953 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27




Instrument :
MSVOA_N
ClientSampleId :
VIBLK


Tgt Ion: 98 Resp: 275894
Ion Ratio Lower Upper
98 100
100 65.3 51.5 77.3

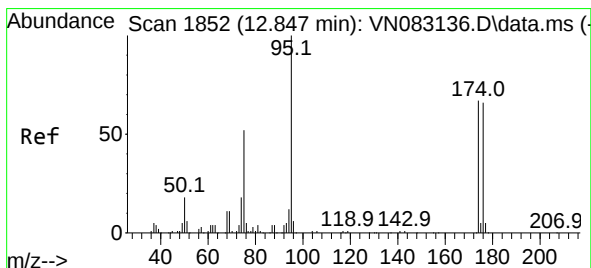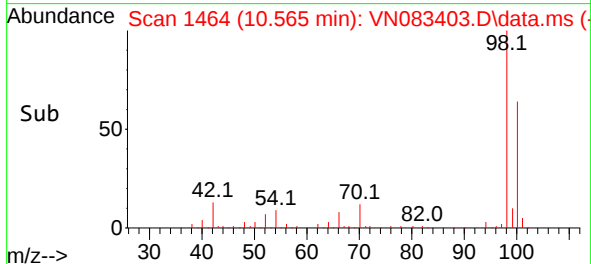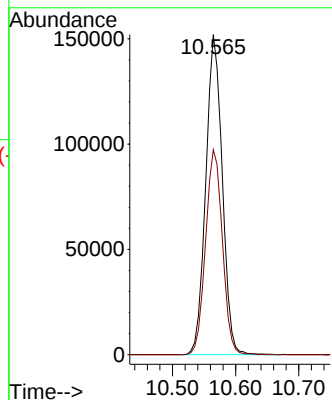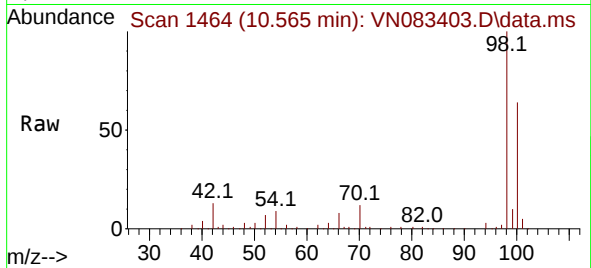

#62
4-Bromofluorobenzene
Concen: 63.732 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Tgt Ion: 95 Resp: 122513
Ion Ratio Lower Upper
95 100
174 69.5 0.0 159.2
176 66.4 0.0 147.6


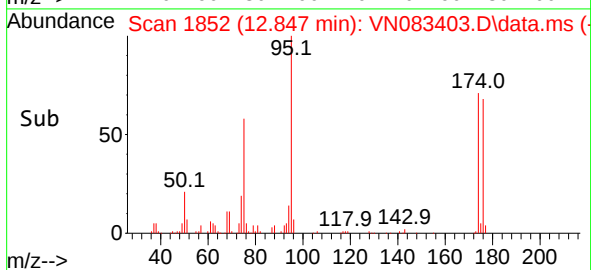
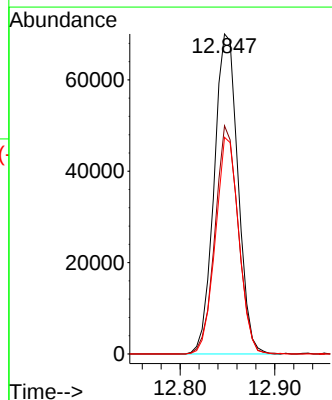
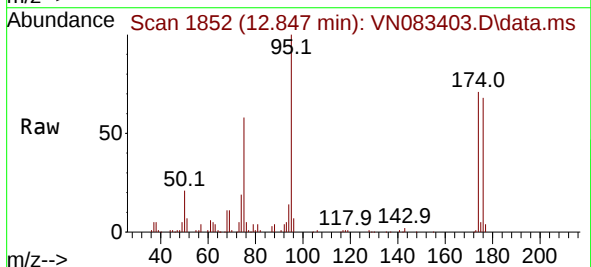


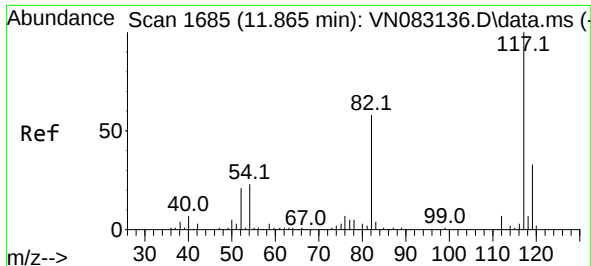

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Instrument :
MSVOA_N
ClientSampleId :
VIBLK

Tgt Ion:117 Resp: 228461
Ion Ratio Lower Upper
117 100
82 59.3 47.5 71.3
119 30.2 25.6 38.4

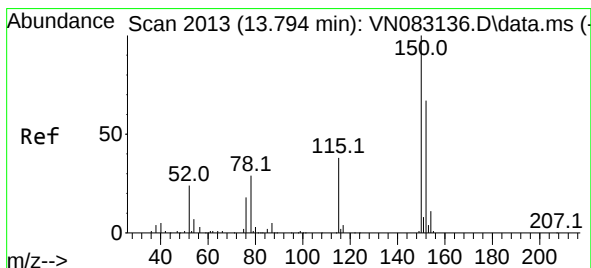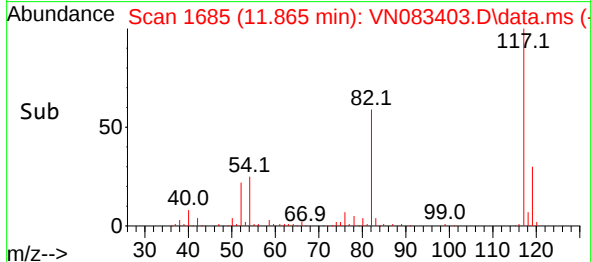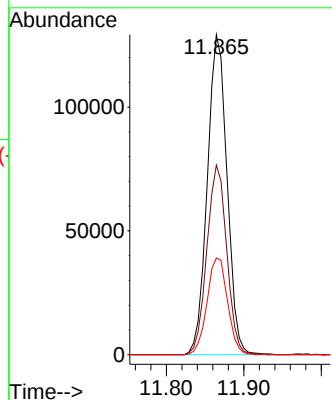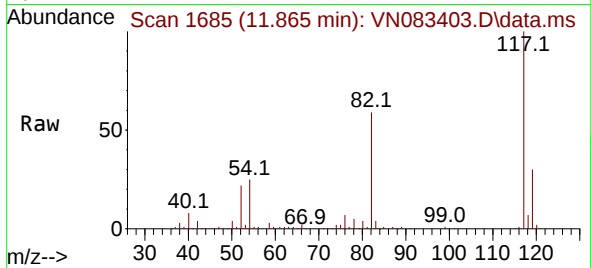

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN083403.D
Acq: 20 Aug 2024 16:27

Tgt Ion:152 Resp: 109127
Ion Ratio Lower Upper
152 100
115 63.4 30.6 91.6
150 159.0 0.0 348.6

