
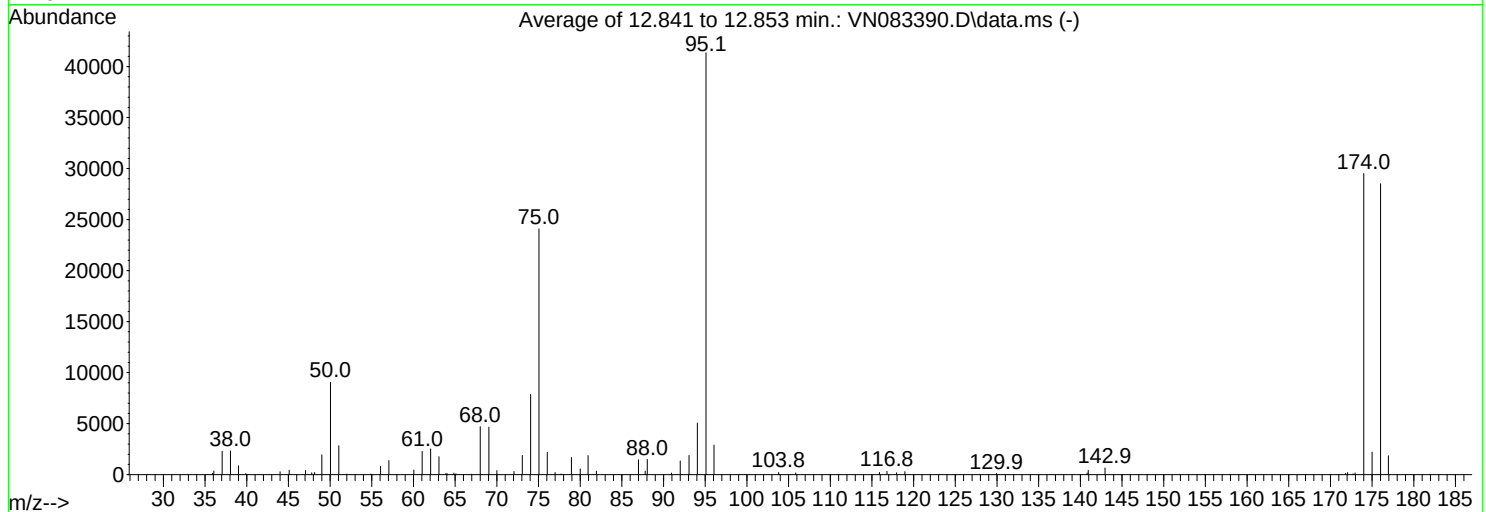


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN082024\
Data File : VN083390.D
Acq On : 20 Aug 2024 08:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N080724W.M
Title : SW846 8260
Last Update : Thu Aug 08 06:30:41 2024

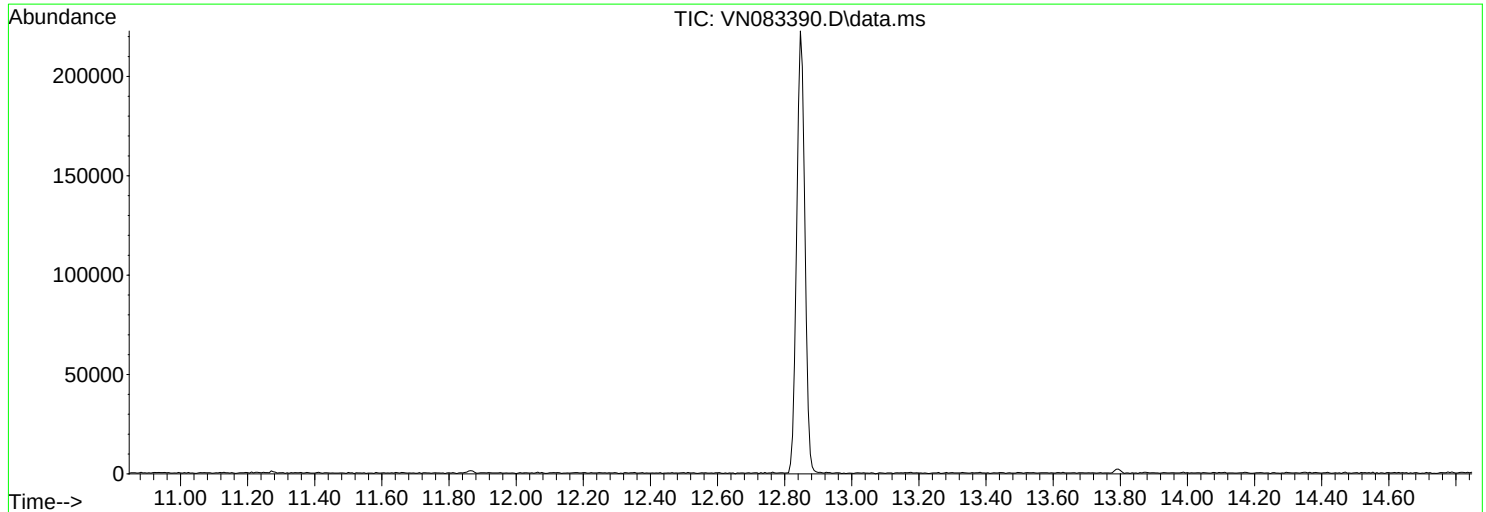

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	9059	PASS
75	95	30	60	58.3	24091	PASS
95	95	100	100	100.0	41347	PASS
96	95	5	9	7.0	2902	PASS
173	174	0.00	2	0.6	173	PASS
174	95	50	100	71.4	29523	PASS
175	174	5	9	7.5	2219	PASS
176	174	95	101	96.6	28523	PASS
177	176	5	9	6.5	1849	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	138	49.00	1944	63.90	136	75.05	2409
36.05	355	50.05	9059	64.10	85	76.05	2181
37.05	2290	51.05	2842	64.85	153	77.00	2211
38.05	2322	52.00	59	65.10	102	77.70	60
39.00	857	54.90	65	67.00	55	78.95	1675
39.90	111	56.05	806	68.00	4700	80.00	560
44.00	282	57.05	1384	69.05	4661	80.95	1860
45.10	438	60.05	448	70.00	392	81.95	345
47.05	404	61.05	2279	72.05	320	87.00	1448
47.80	188	62.05	2527	73.05	1890	87.80	353
48.15	226	63.05	1764	74.05	7855	88.05	1486

Average of 12.841 to 12.853 min.: VN083390.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.95	162	118.95	302	176.00	28523		
92.00	1357	129.95	110	176.95	1849		
93.05	1884	140.80	159				
94.05	5068	140.95	419				
95.10	41347	142.95	661				
96.05	2902	171.80	122				
103.80	221	172.05	208				
105.85	167	172.70	83				
115.90	216	172.95	173				
116.80	333	174.00	29523				
117.95	189	175.00	2219				

Instrument :

MSVOA_N

ClientSampleId :

BFB