



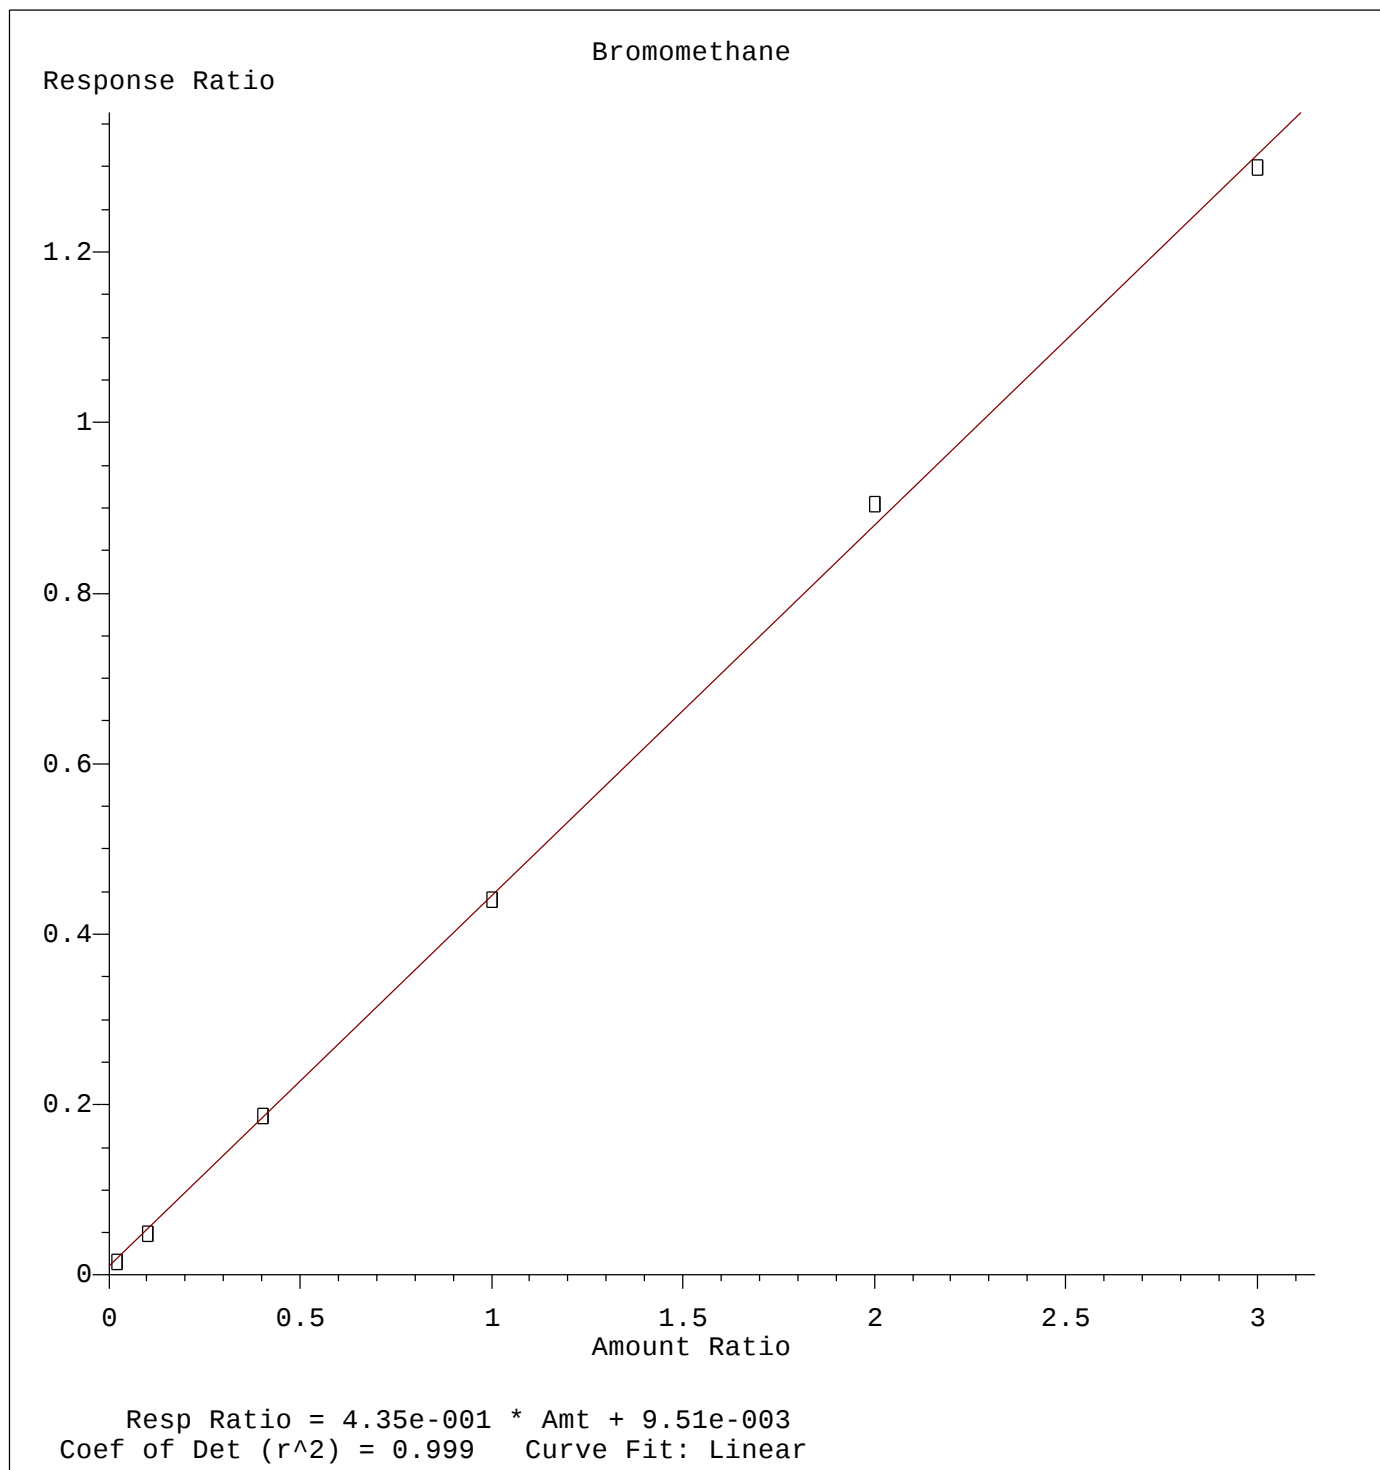

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018


1,2,3-Trichlorobenzene

Response Ratio

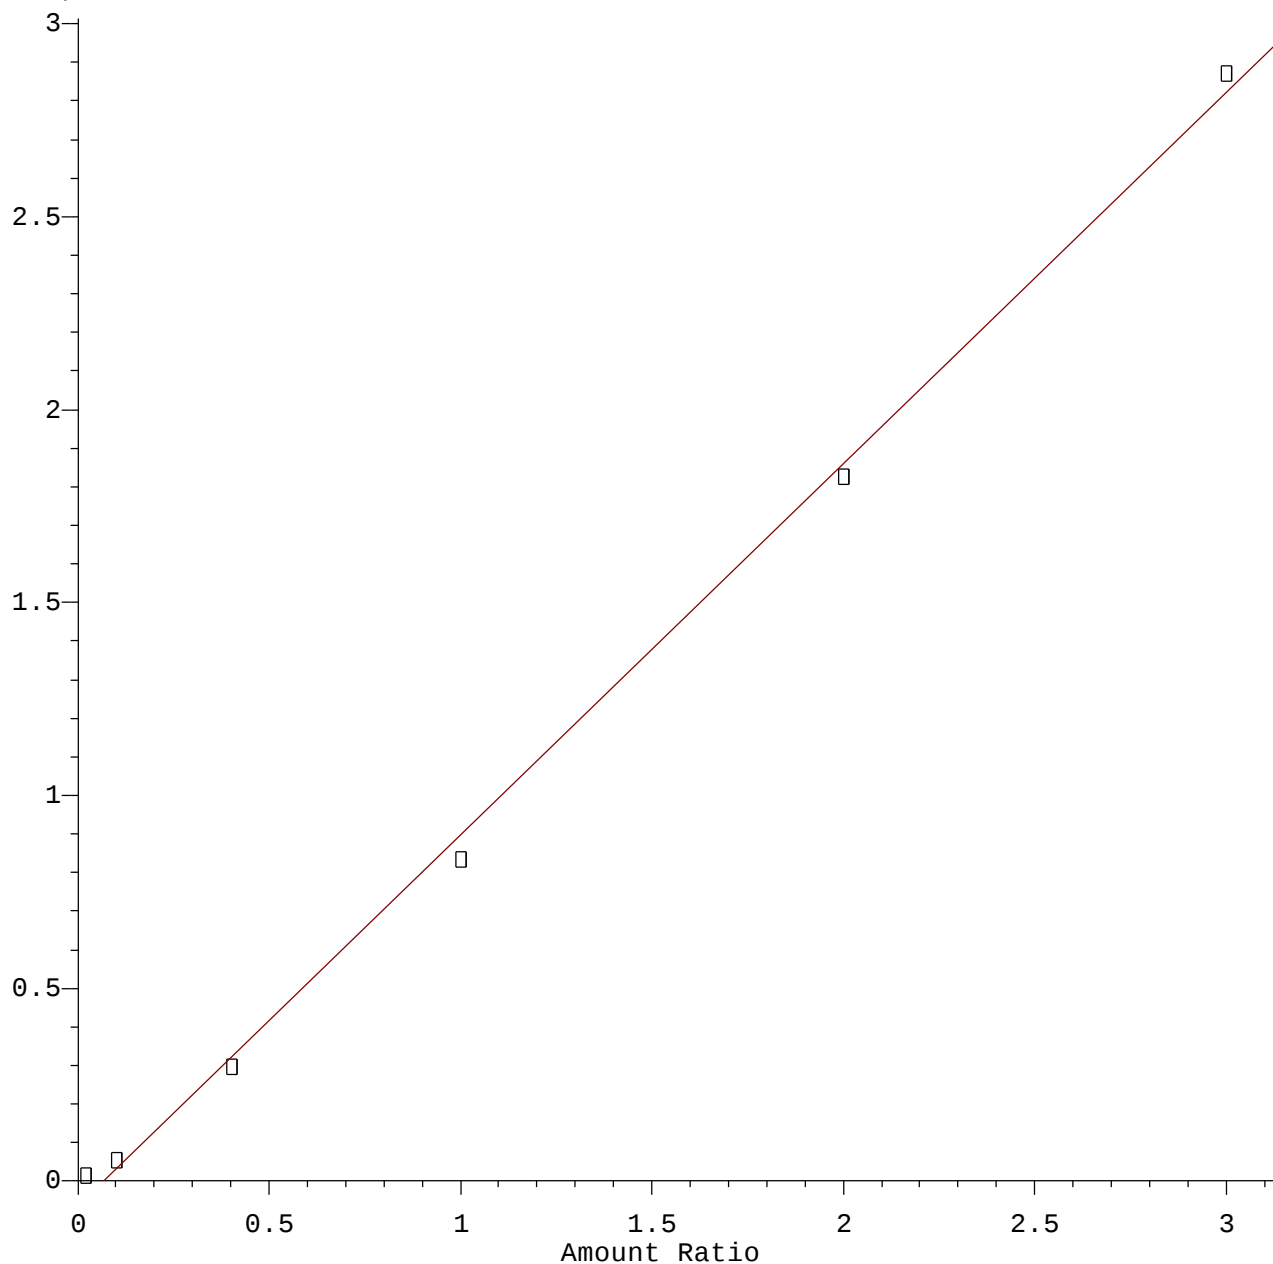


Resp Ratio = $9.62 \times 10^{-1} \times \text{Amt} - 6.34 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018

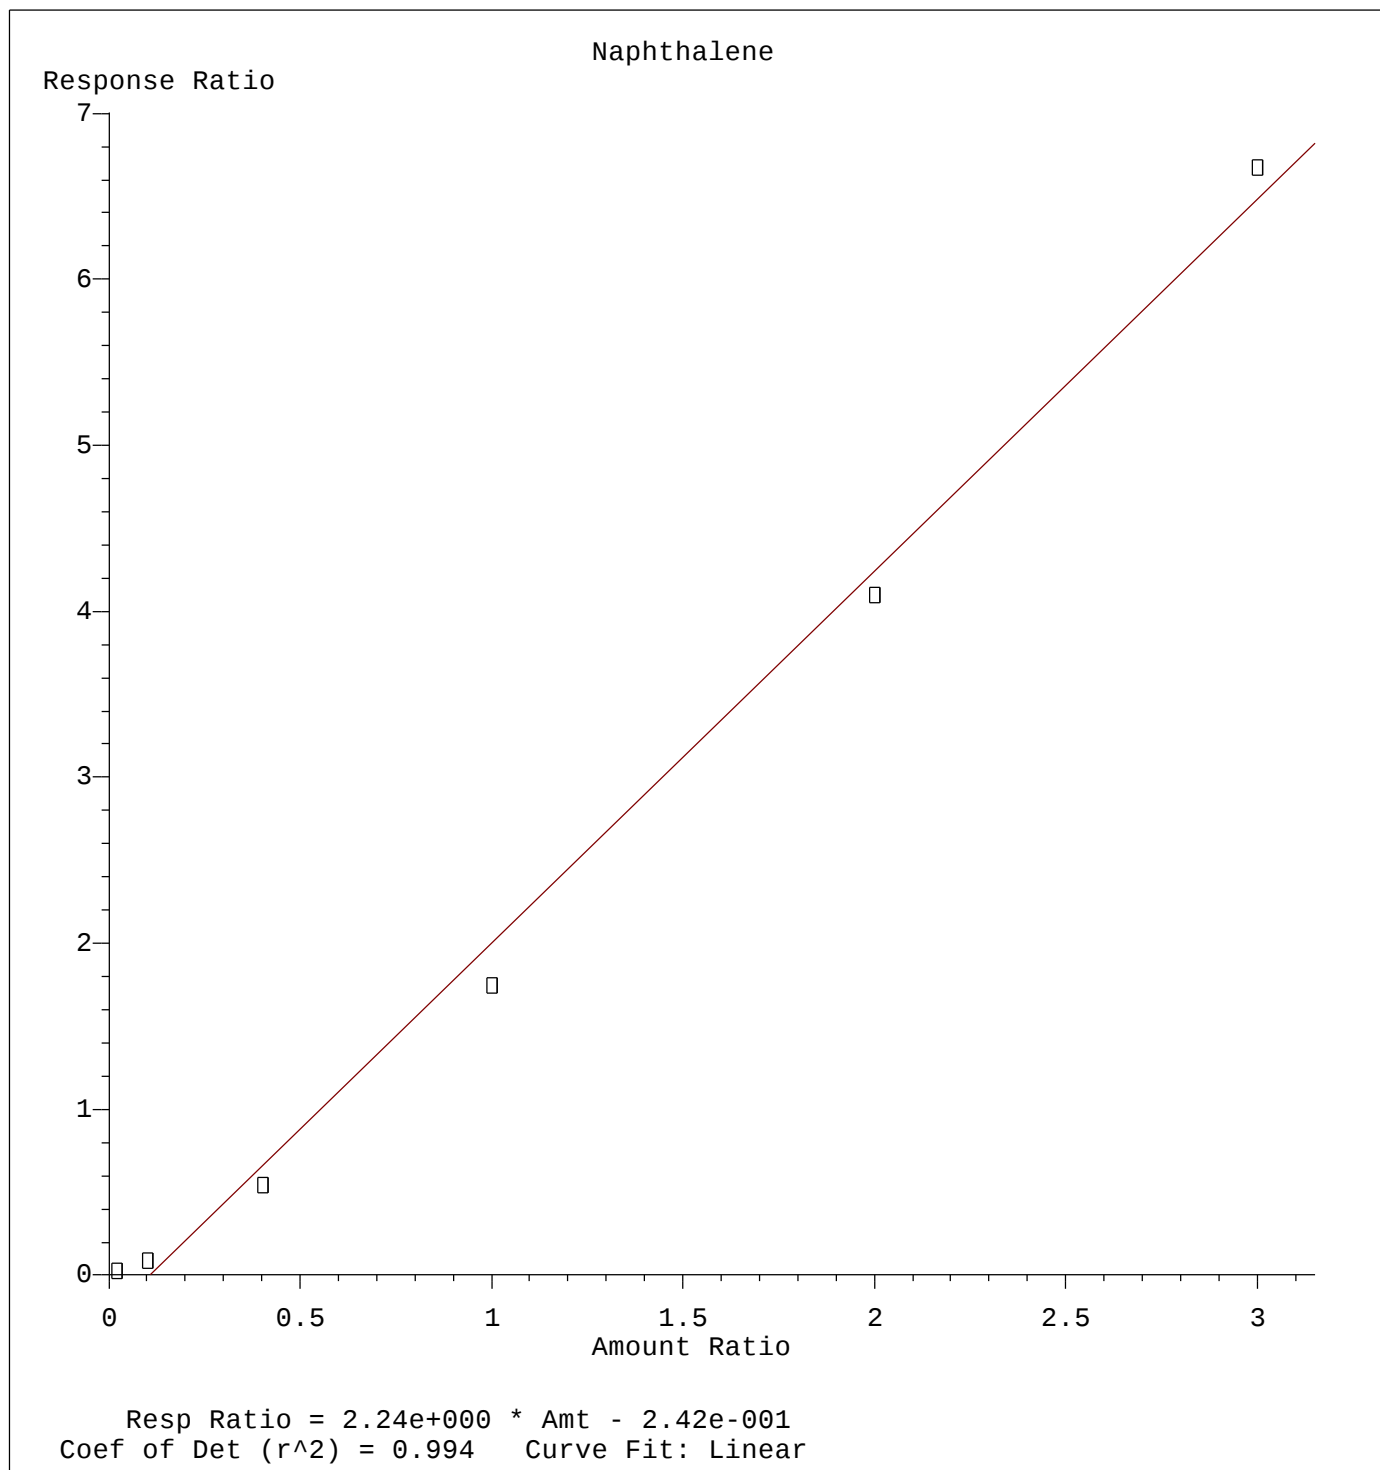


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018

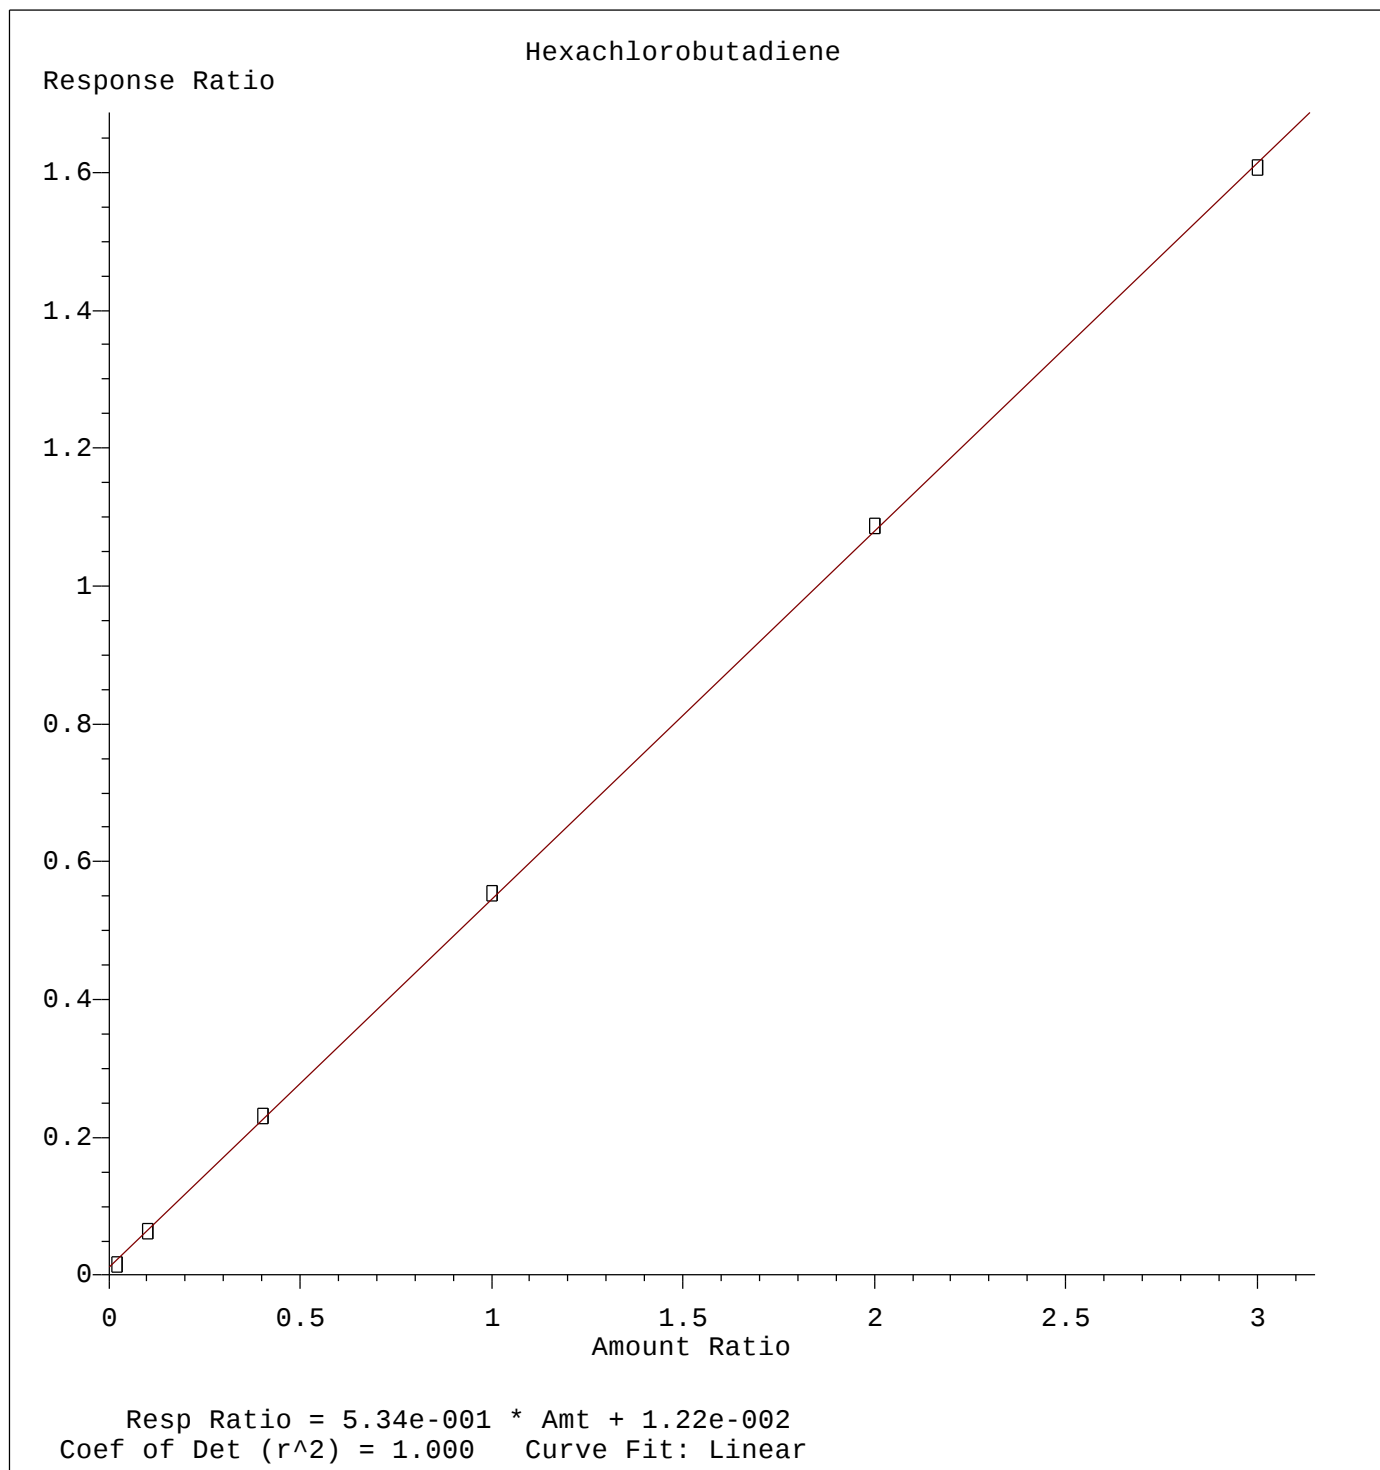

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018


1,2,4-Trichlorobenzene

Response Ratio

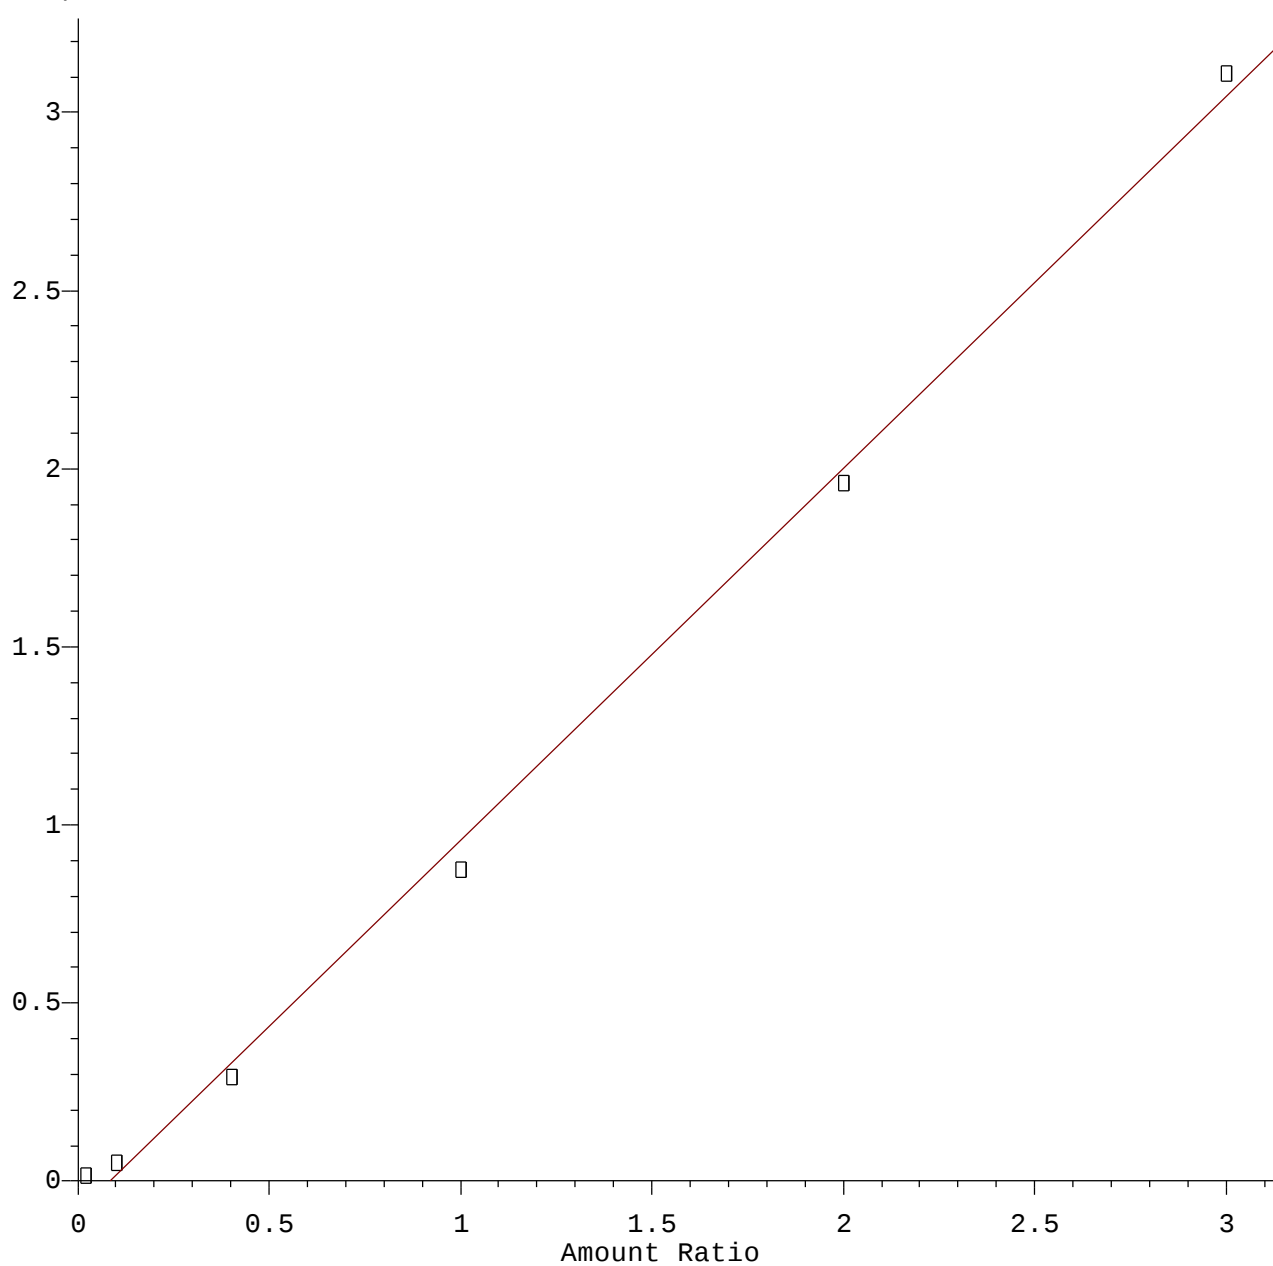

Resp Ratio = 1.04e+000 * Amt - 8.52e-002
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018

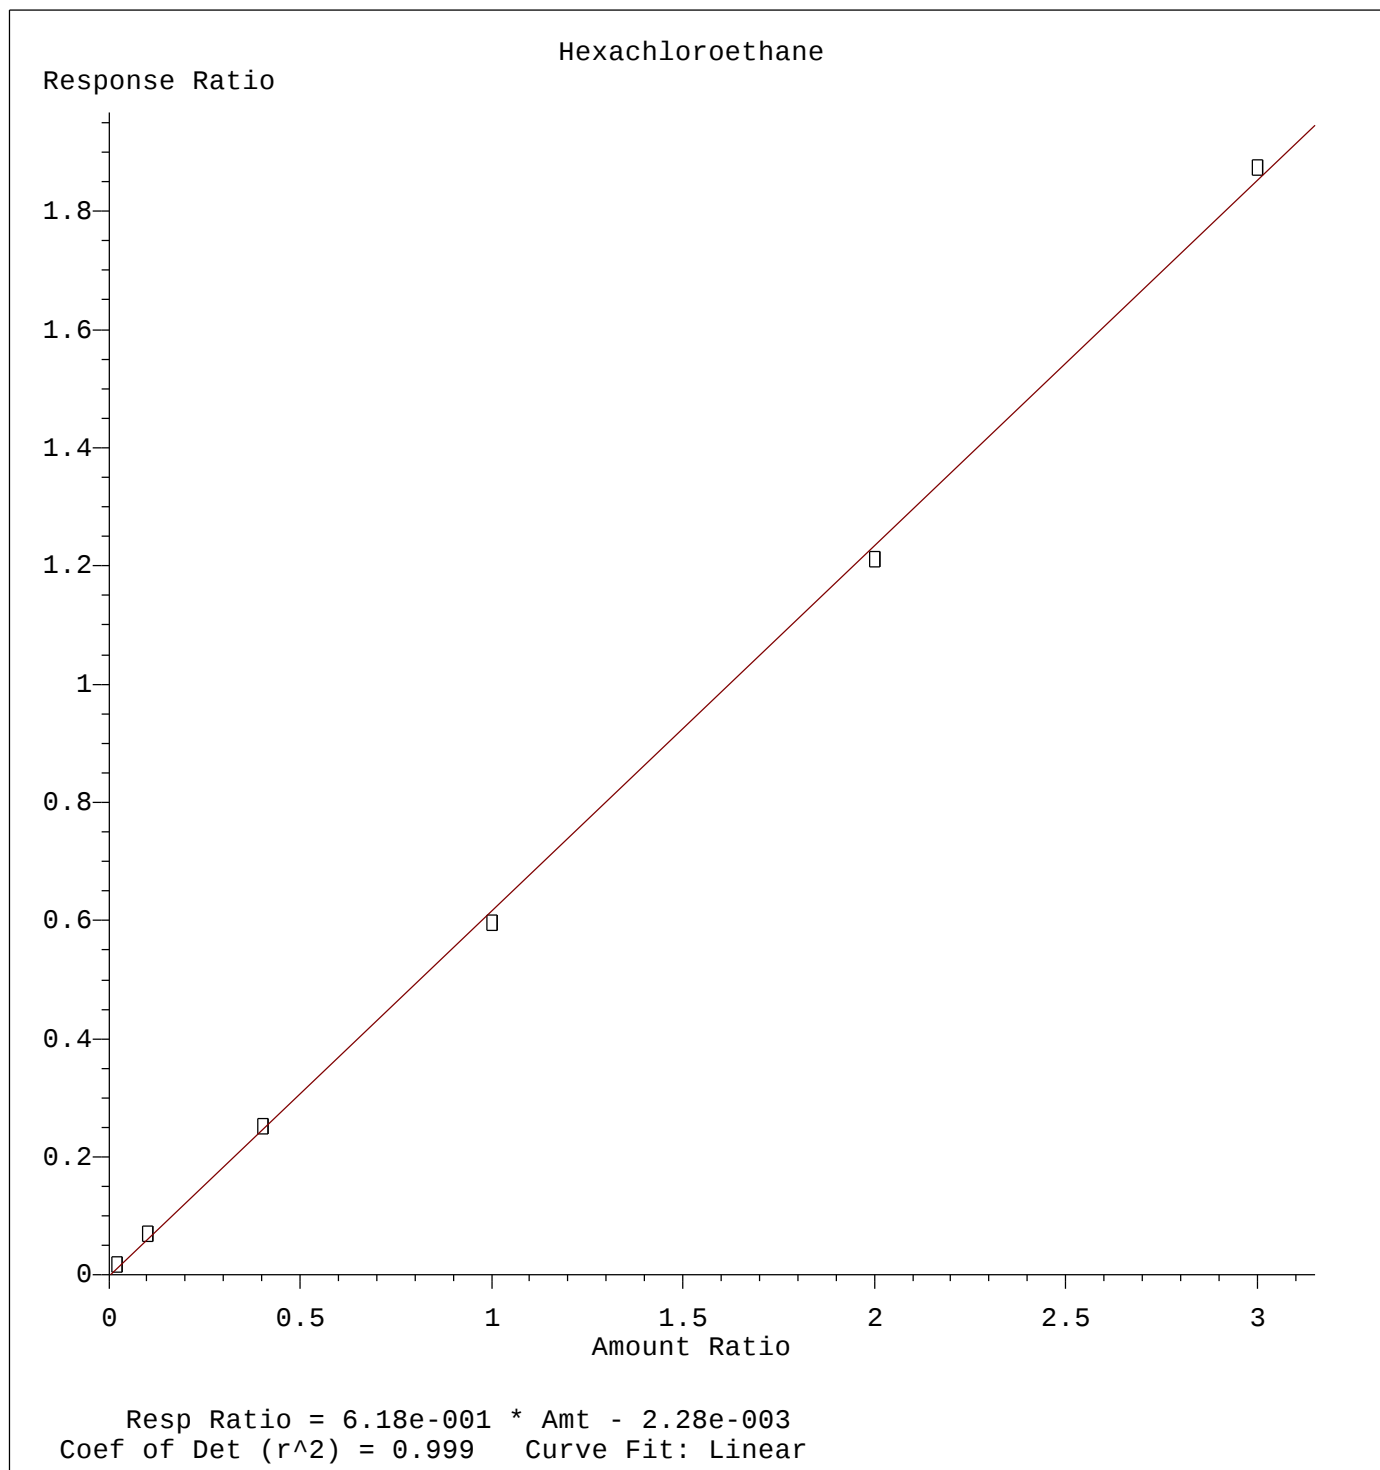

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018


1,1,2,2-Tetrachloroethane

Response Ratio

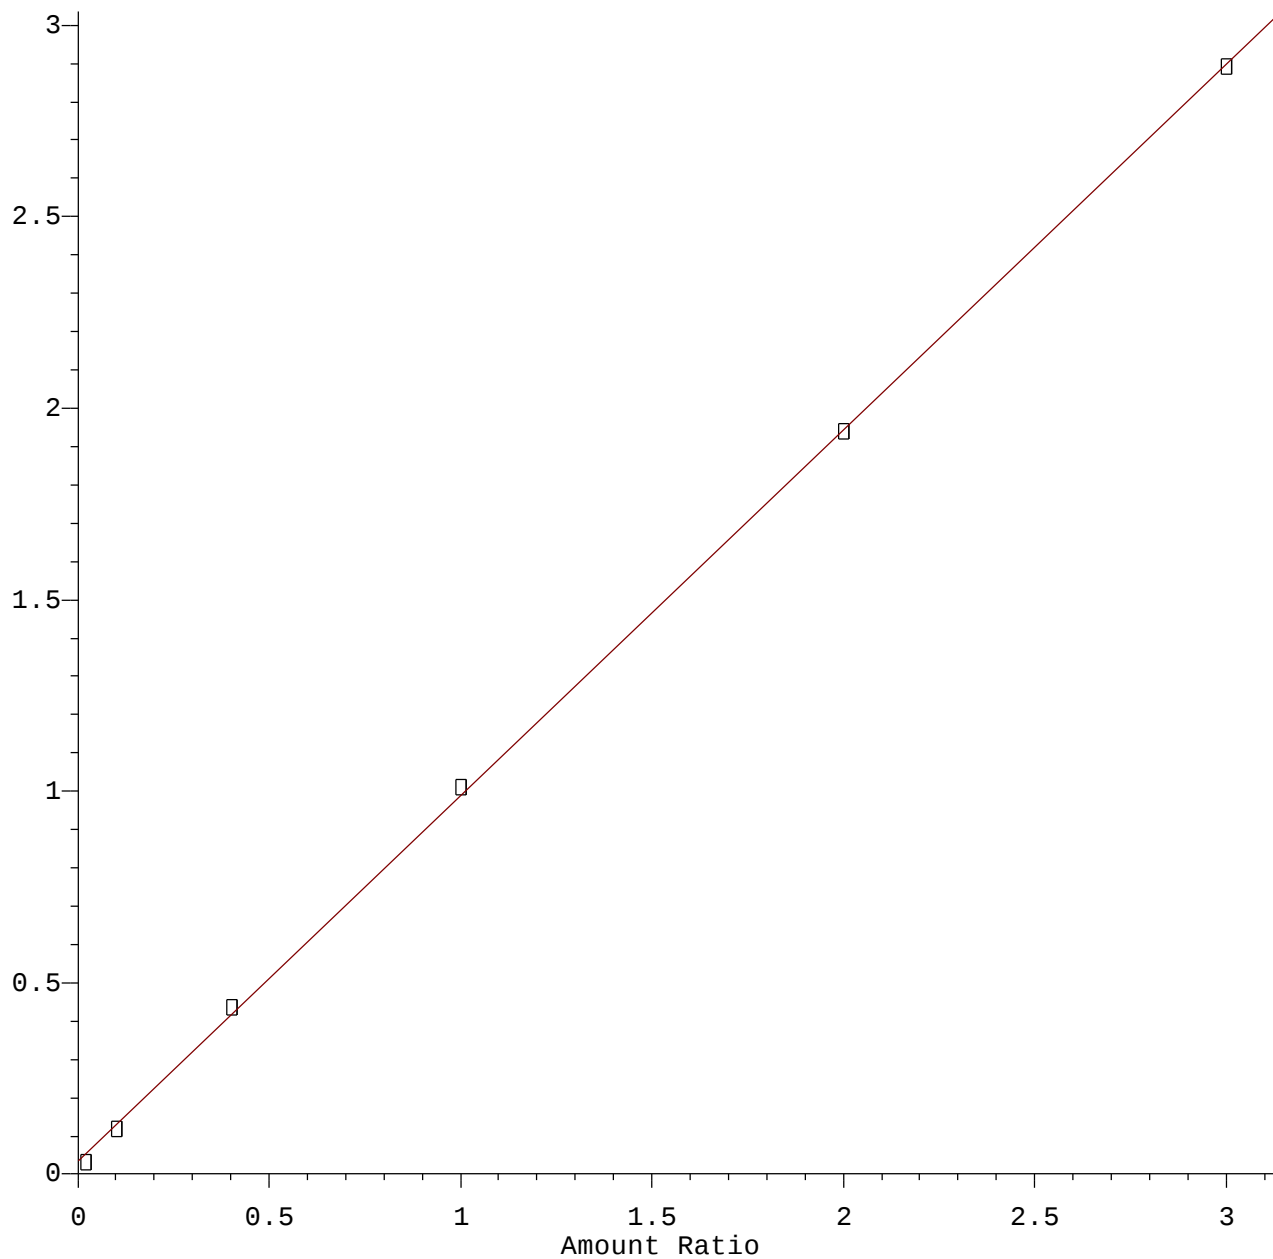

Resp Ratio = 9.55e-001 * Amt + 3.23e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018

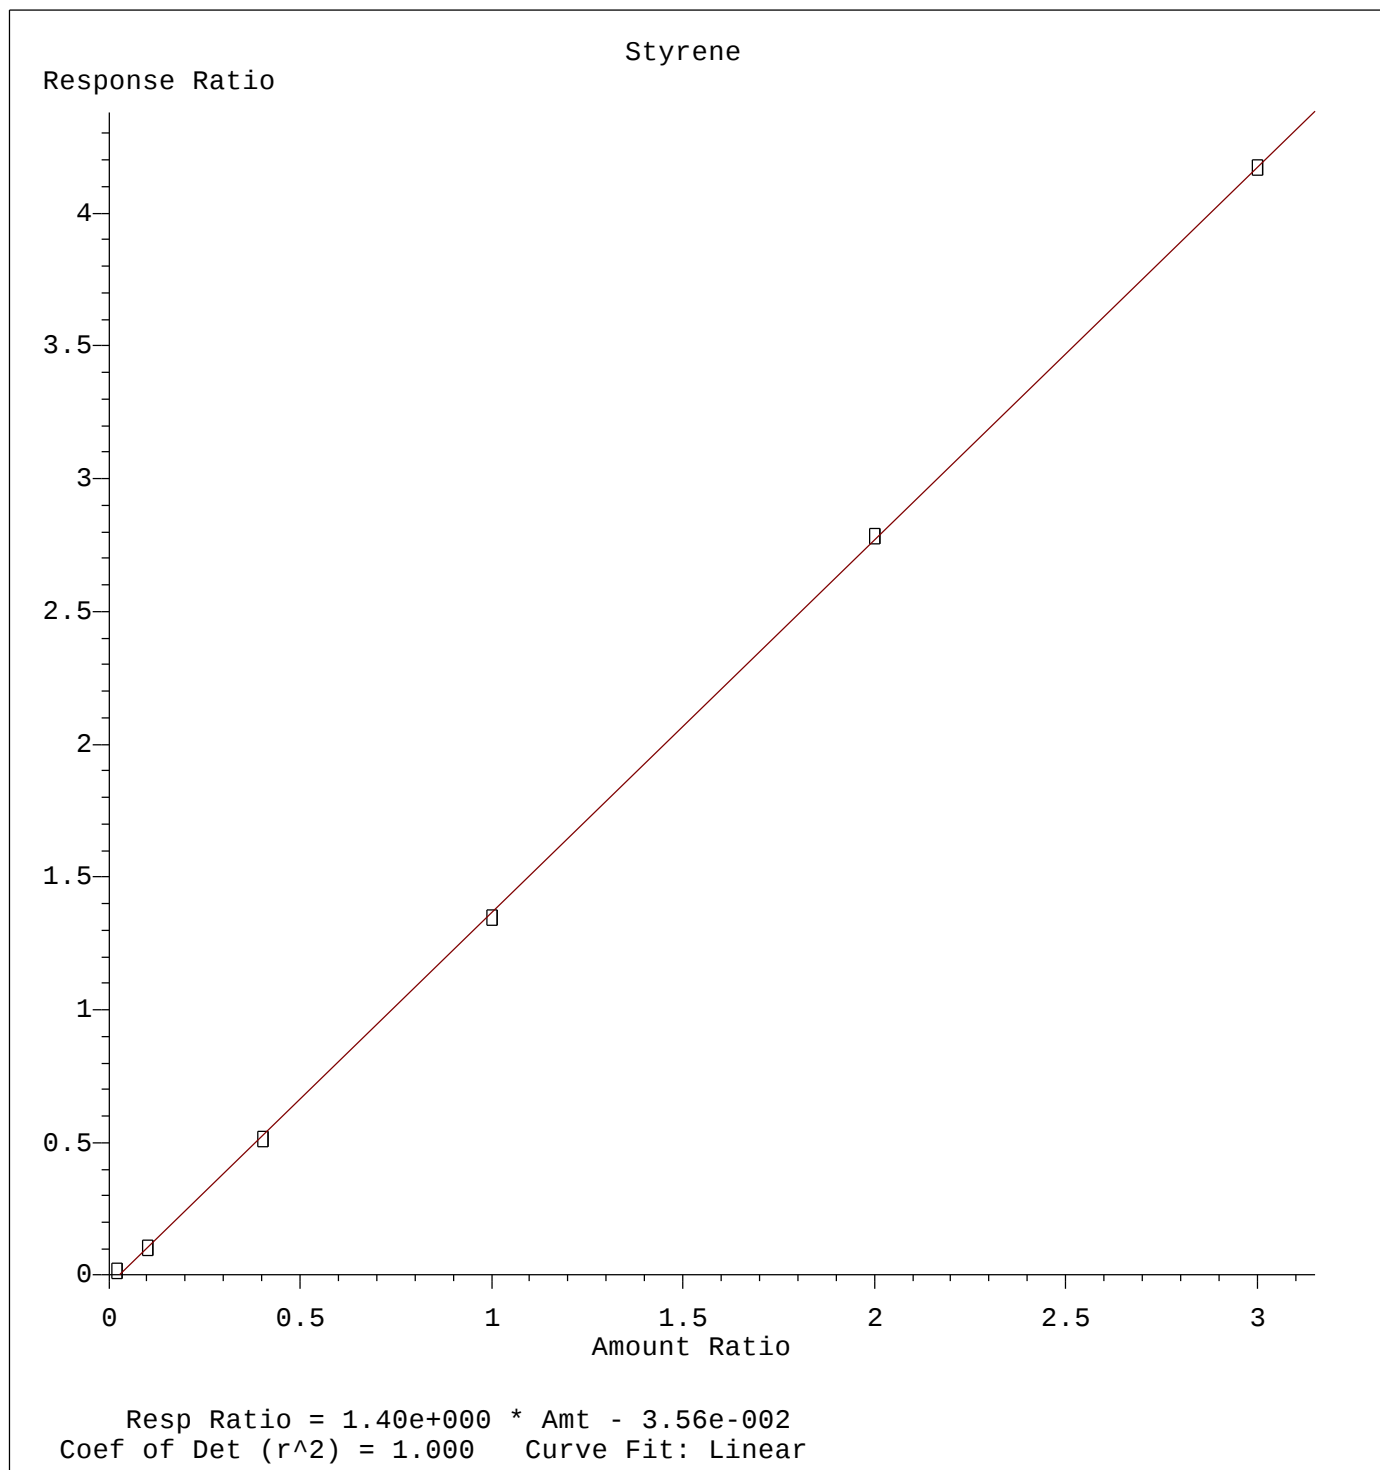

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018

2-Chloroethyl Vinyl ether

Response Ratio

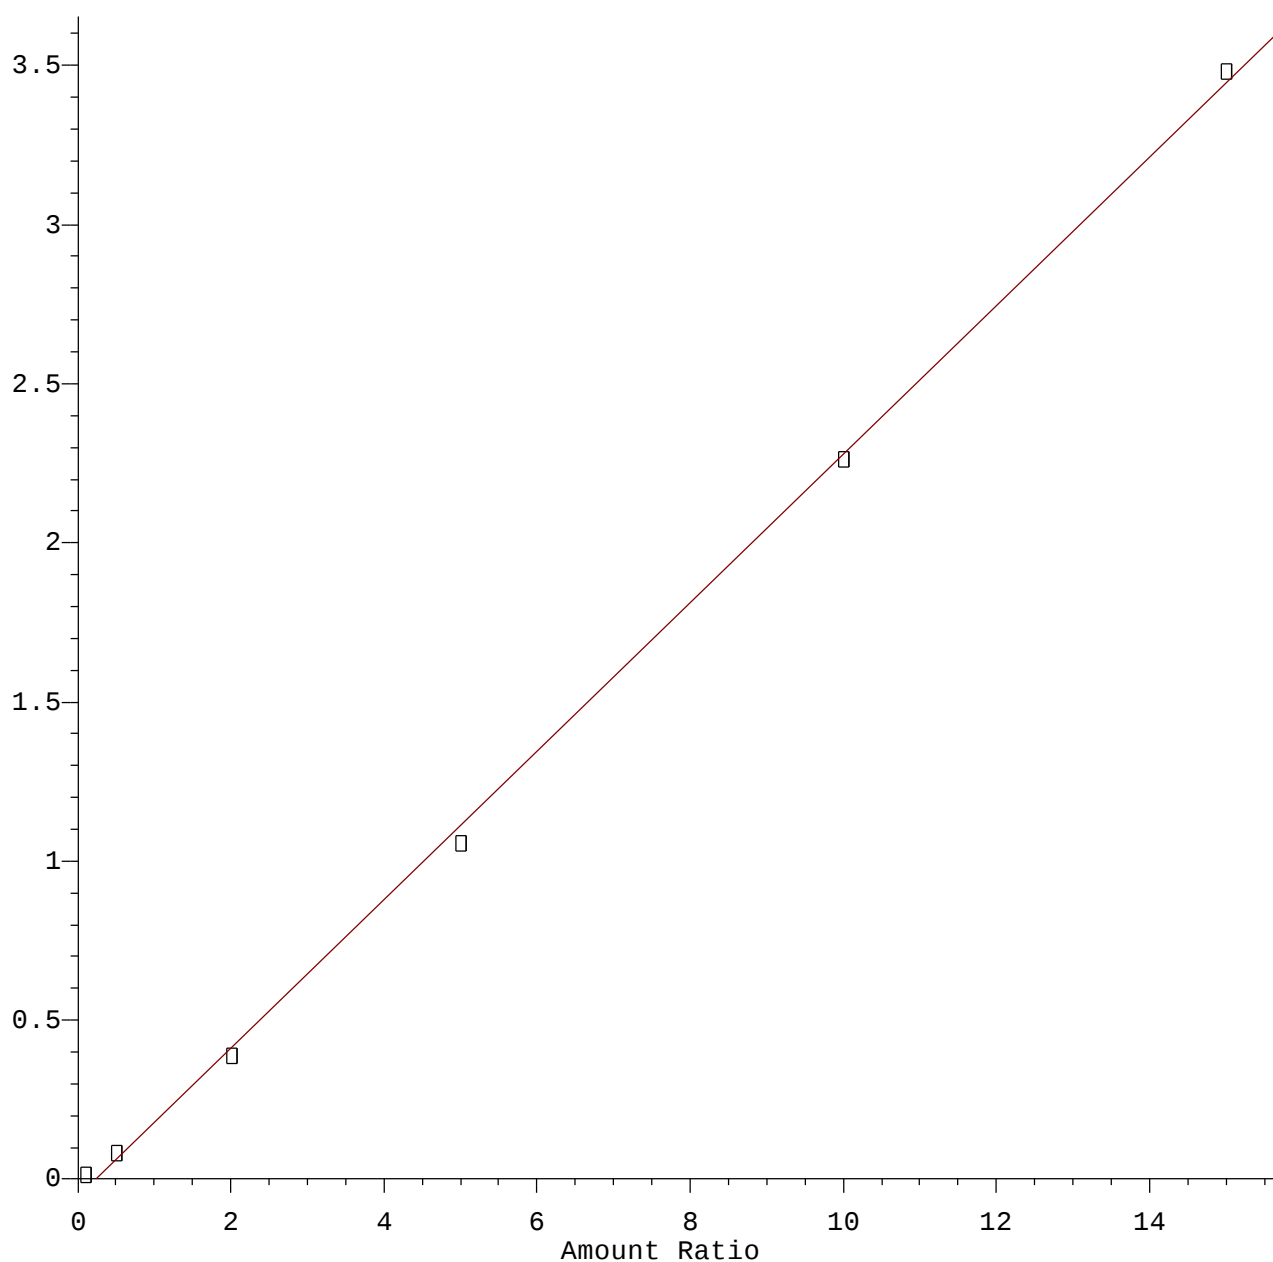


Resp Ratio = $2.33 \times 10^{-1} \times \text{Amt} - 5.71 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018


Ethyl methacrylate

Response Ratio

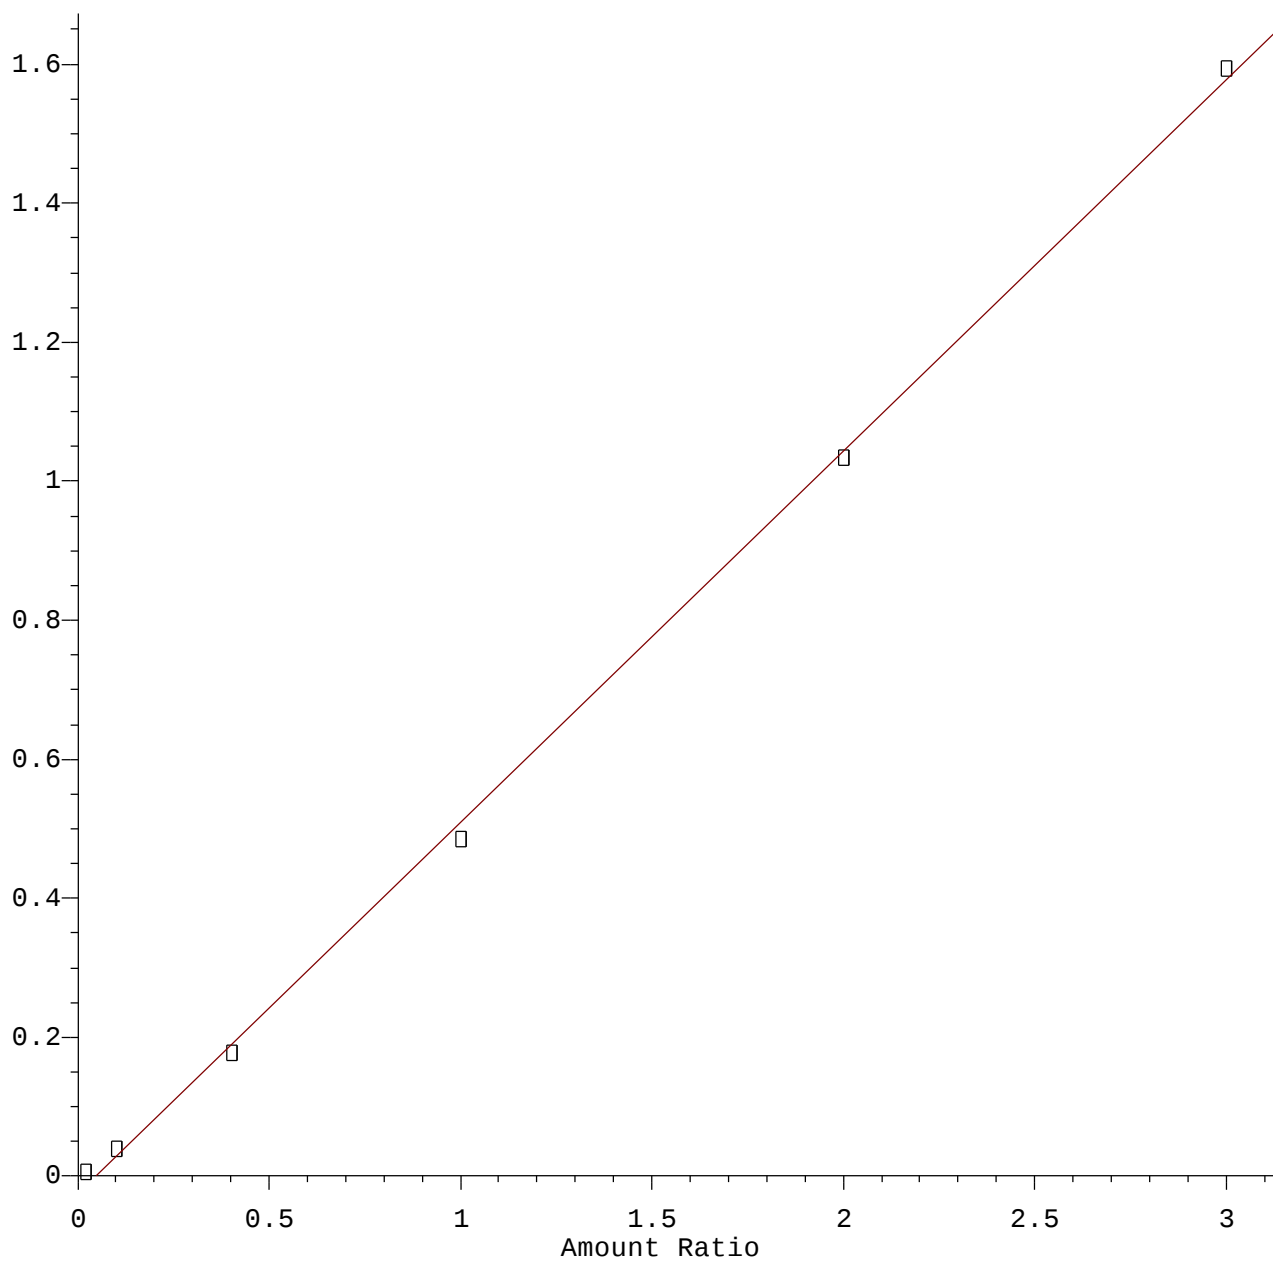


Resp Ratio = 5.34e-001 * Amt - 2.51e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018

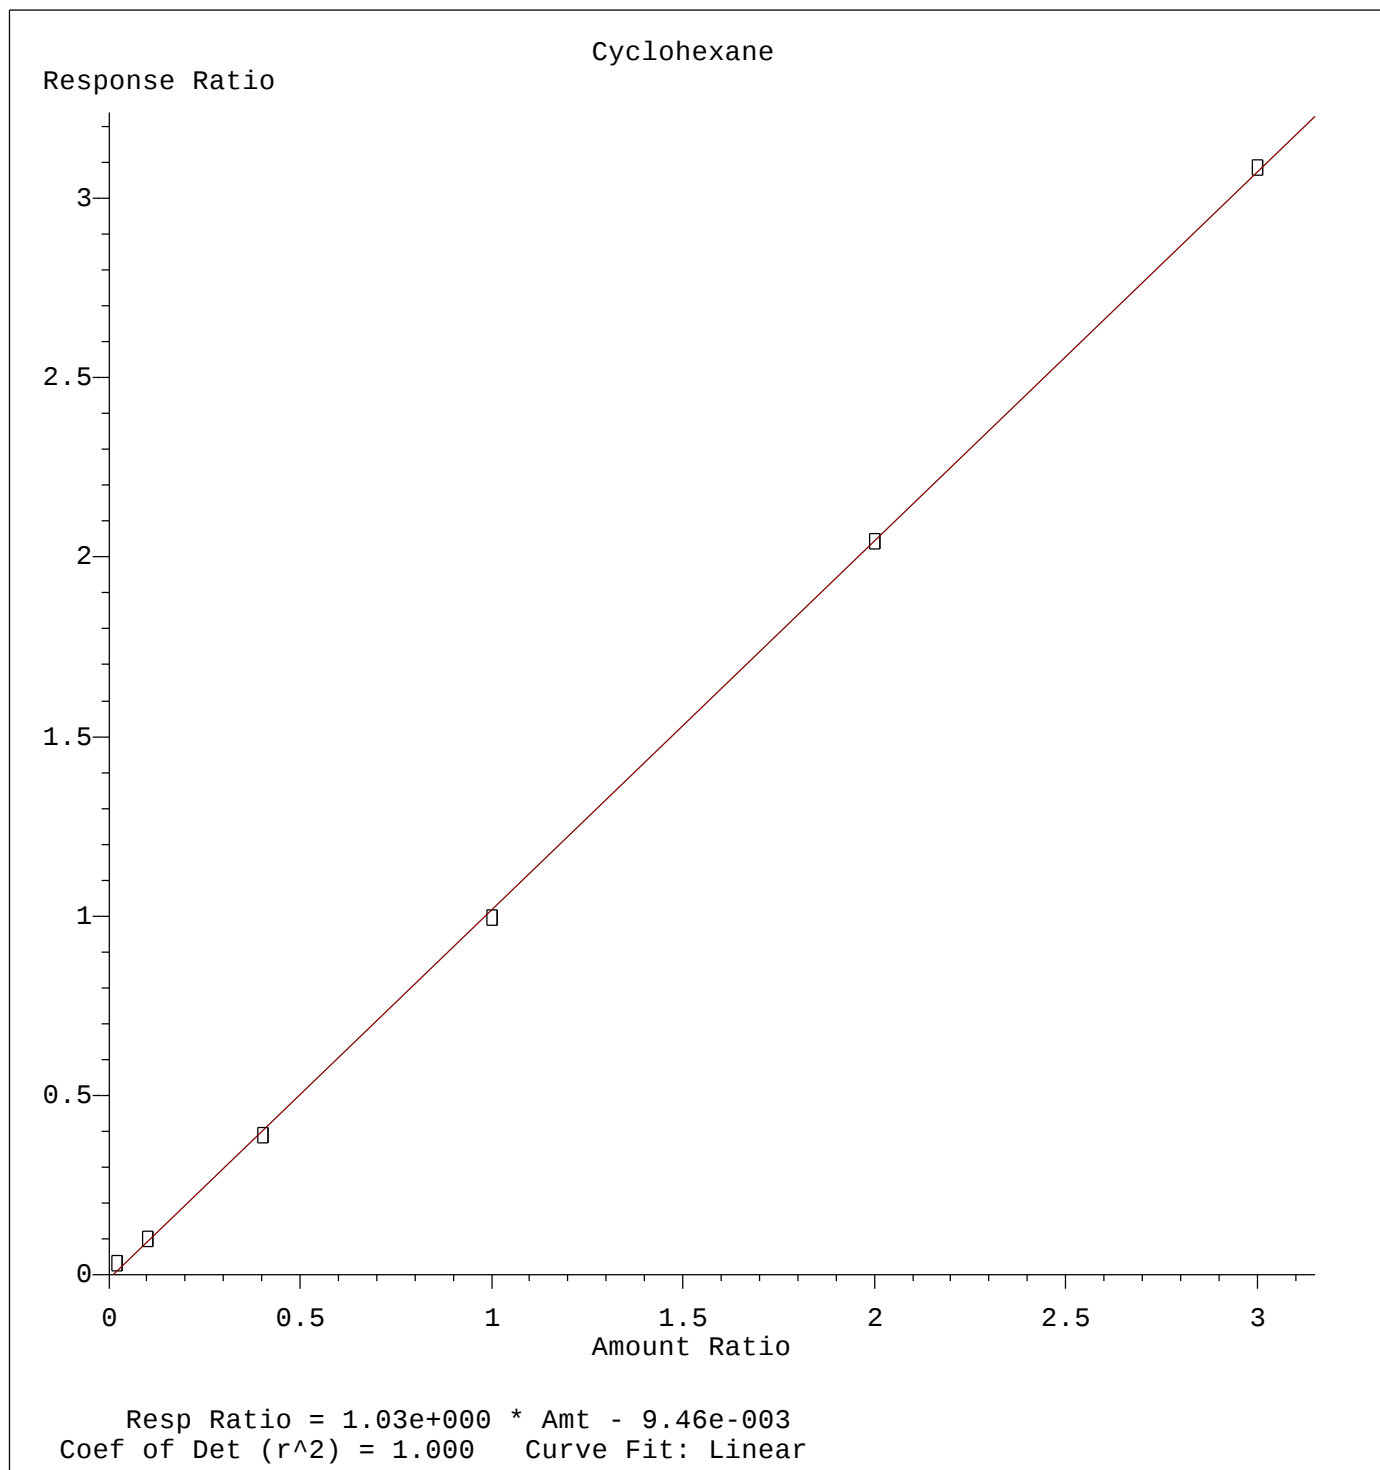


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018

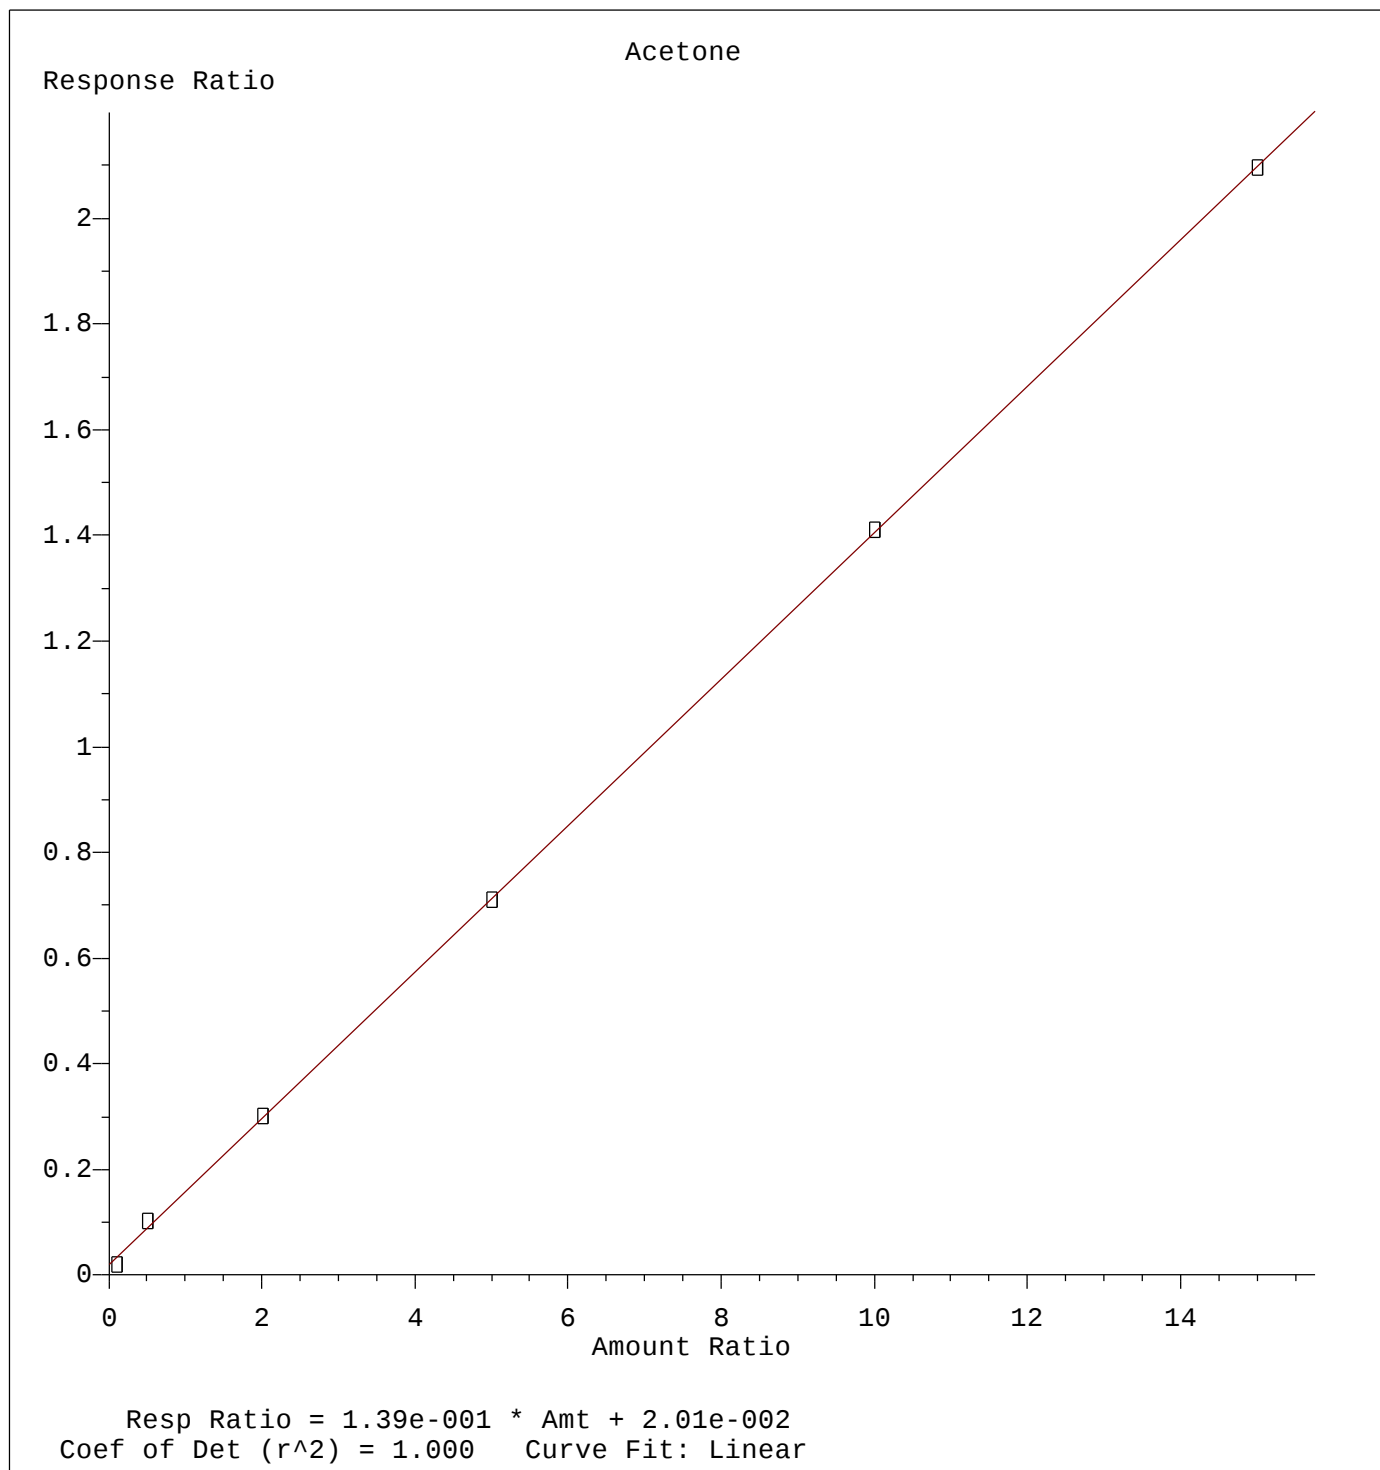

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018

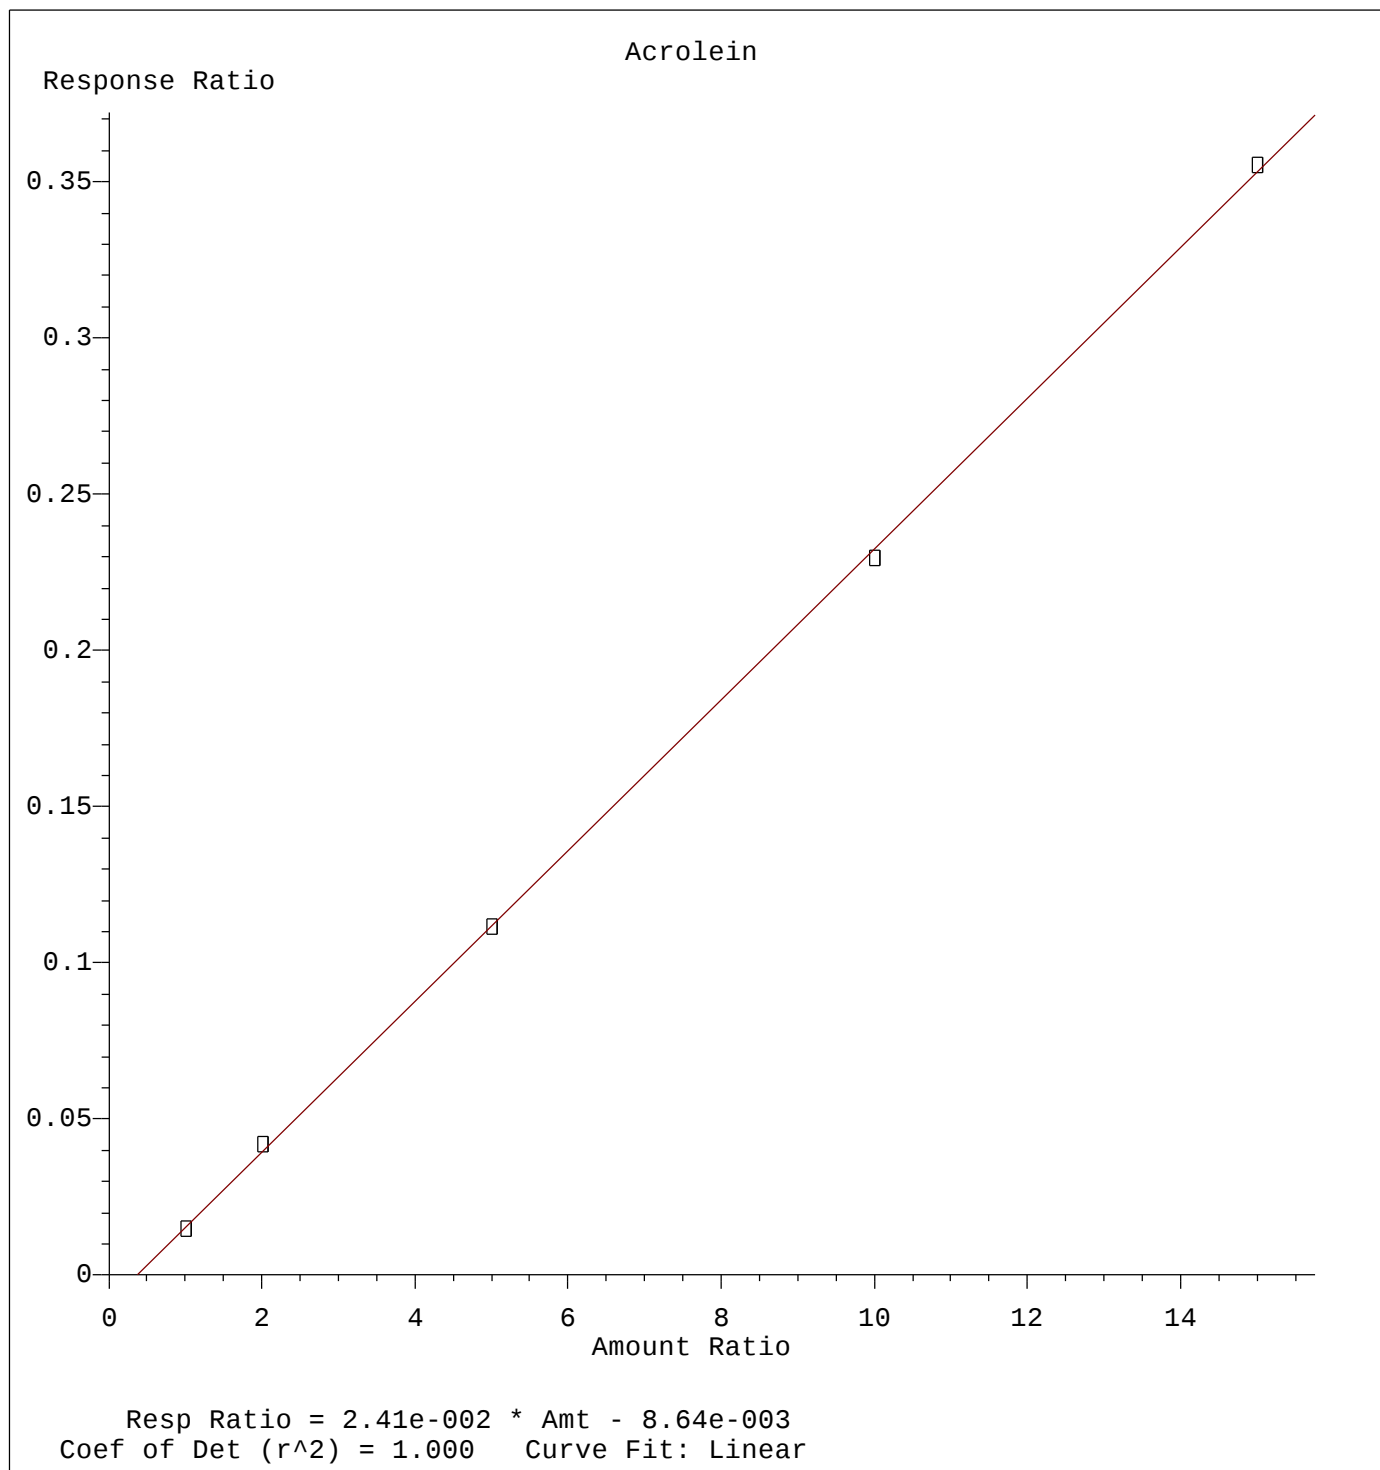

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018

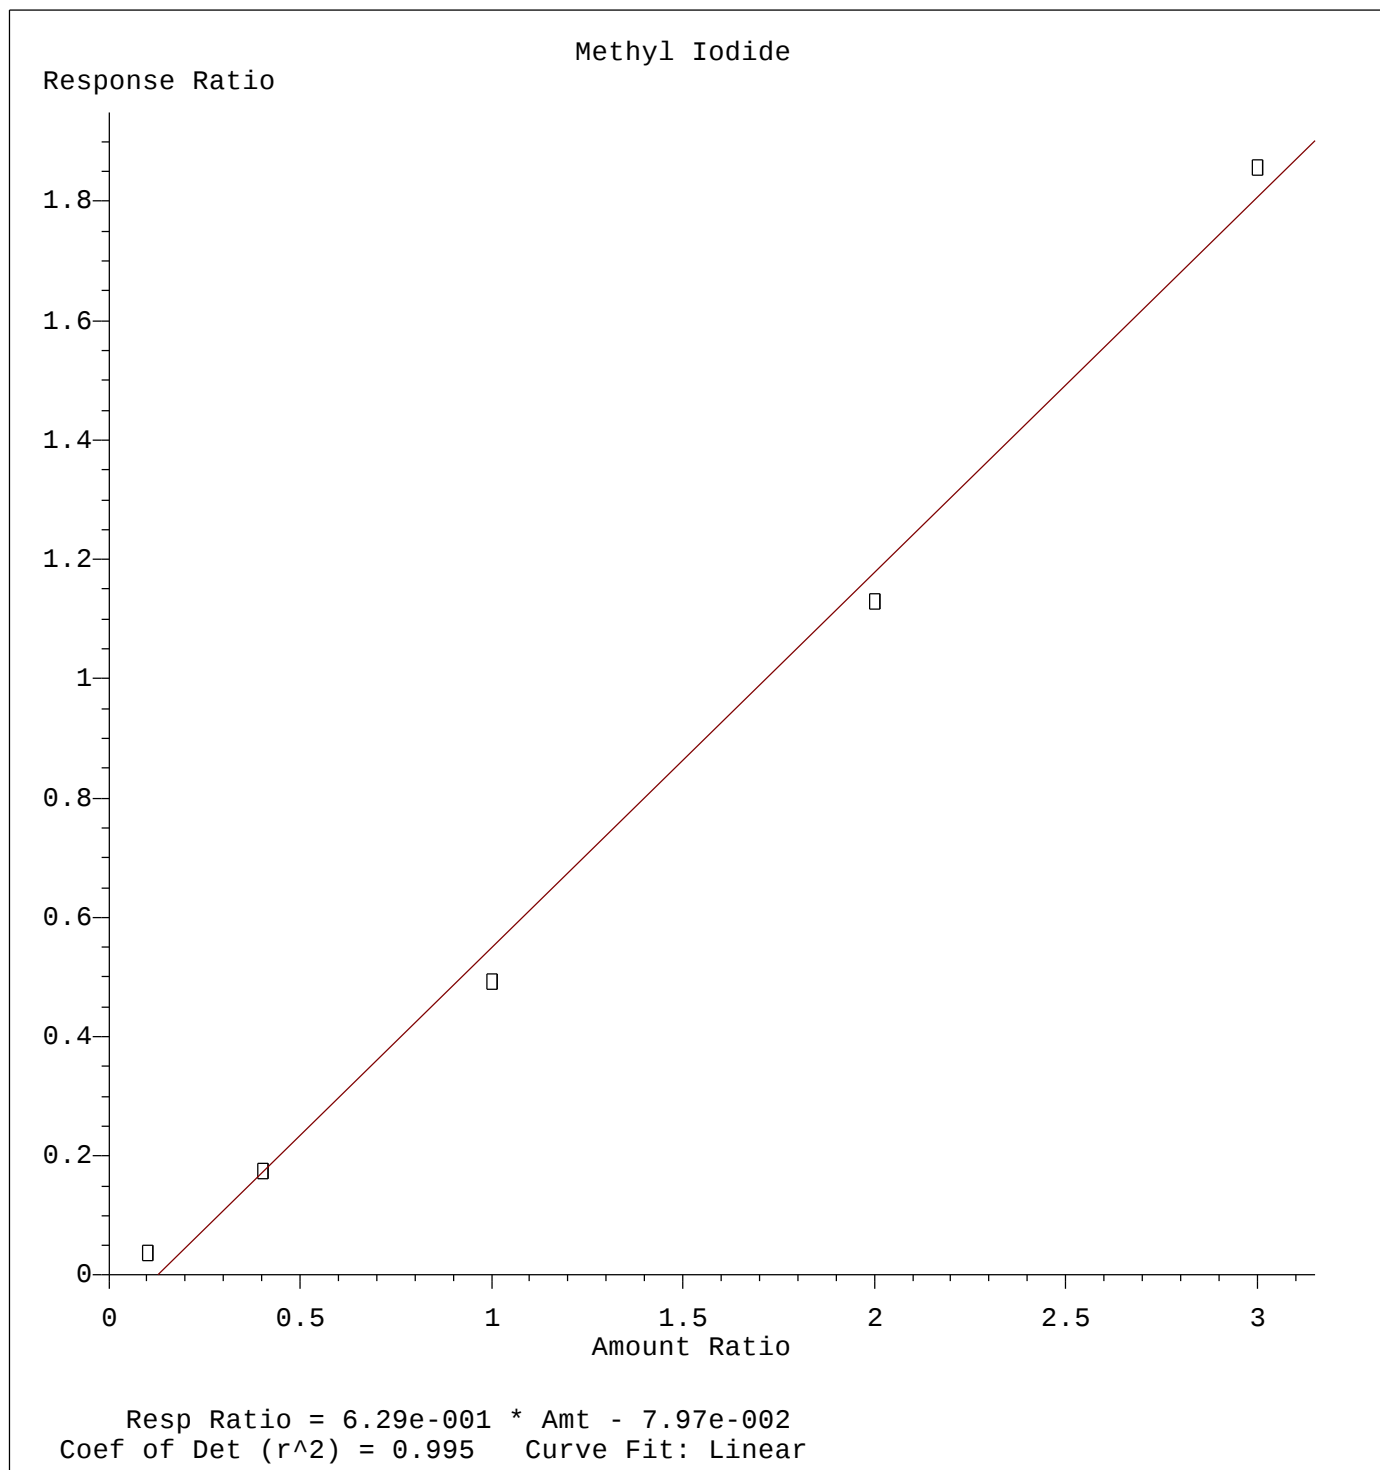

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
Calibration Table Last Updated: Thu Aug 23 11:57:39 2018