


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN082118\
 Data File : VN050778.D
 Acq On : 21 Aug 2018 9:05
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N082118W.M
 Title : SW846 8260
 Last Update : Wed Aug 22 05:38:12 2018

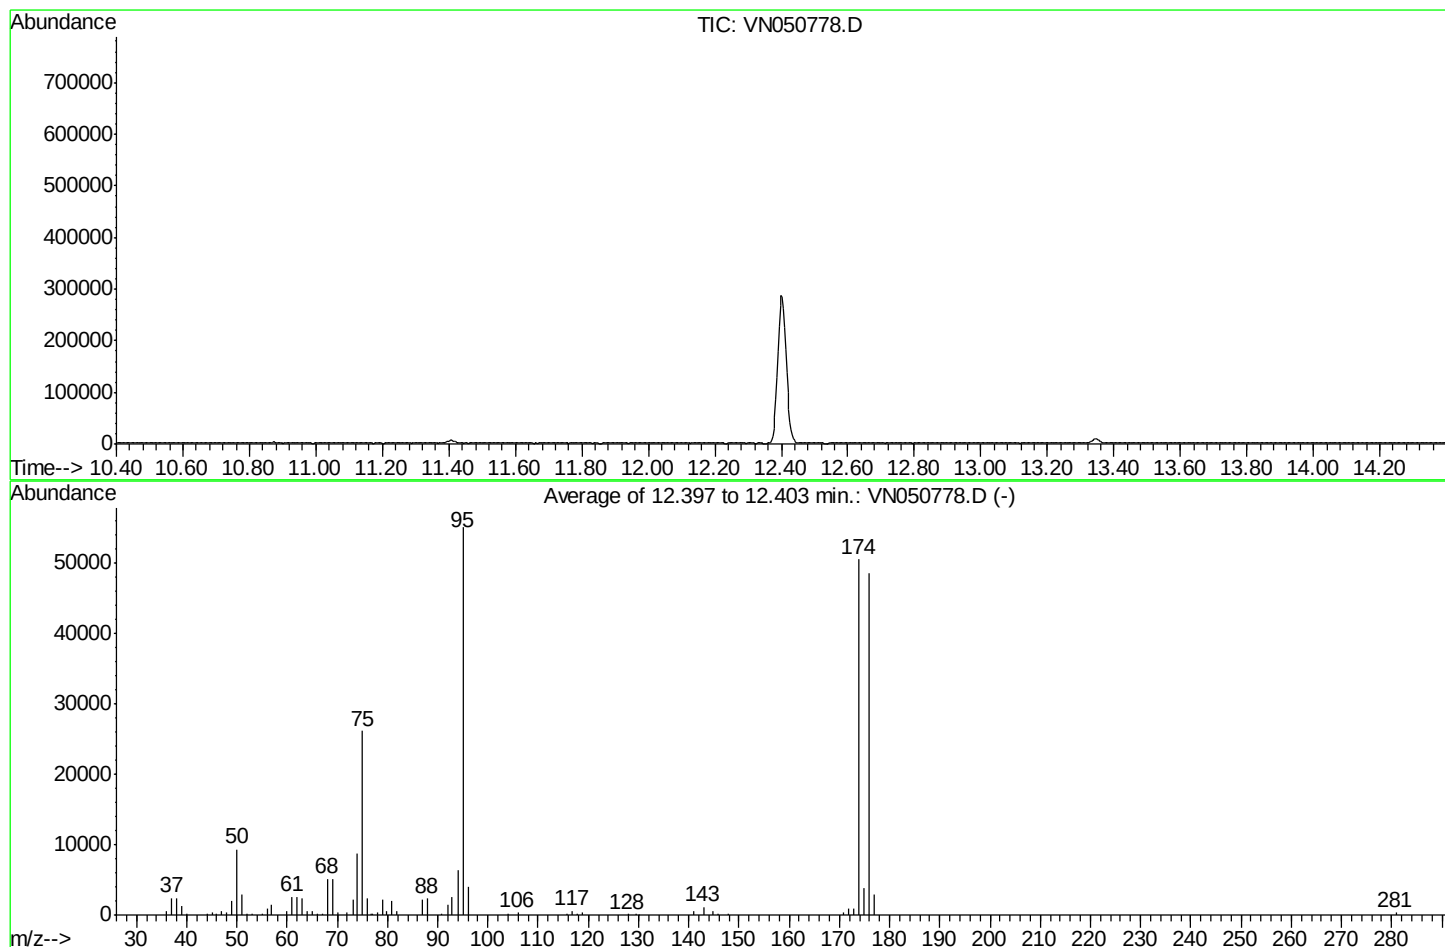

AutoFind: Scans 3361, 3362, 3363; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	9300	PASS
75	95	30	60	47.5	26181	PASS
95	95	100	100	100.0	55149	PASS
96	95	5	9	7.1	3943	PASS
173	174	0.00	2	1.9	950	PASS
174	95	50	100	91.8	50608	PASS
175	174	5	9	7.7	3883	PASS
176	174	95	101	96.2	48669	PASS
177	176	5	9	6.1	2958	PASS